

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035217.D
 Acq On : 20 Apr 2023 15:49
 Operator : JC/MD
 Sample : 02378-15DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	33	rBV3	2397	2617	0.09%	0.016%
2	1.368	42	46	59	rBV	144488	158392	5.23%	0.965%
3	1.672	92	96	108	rBV	120909	156185	5.16%	0.952%
4	2.307	194	200	211	rBV	297914	458822	15.16%	2.795%
5	2.654	255	257	260	rVB	486	531	0.02%	0.003%
6	2.691	260	263	265	rBV2	354	379	0.01%	0.002%
7	2.709	265	266	268	rVV	425	281	0.01%	0.002%
8	2.727	268	269	274	rVV2	314	343	0.01%	0.002%
9	2.794	274	280	289	rVV3	3387	6382	0.21%	0.039%
10	3.020	313	317	319	rBV2	316	406	0.01%	0.002%
11	3.160	338	340	345	rBV2	225	336	0.01%	0.002%
12	3.386	374	377	378	rBV	170	195	0.01%	0.001%
13	3.404	378	380	384	rVB3	236	317	0.01%	0.002%
14	3.636	417	418	421	rBV	331	275	0.01%	0.002%
15	4.020	479	481	483	rVV	321	200	0.01%	0.001%
16	4.288	524	525	526	rBV	364	217	0.01%	0.001%
17	4.465	545	554	574	rBV	109134	349803	11.55%	2.131%
18	4.745	598	600	602	rVV2	292	246	0.01%	0.001%
19	4.806	609	610	612	rVB2	419	250	0.01%	0.002%
20	4.965	634	636	638	rBV2	248	265	0.01%	0.002%
21	5.056	638	651	670	rVV2	195205	603956	19.95%	3.679%
22	5.208	674	676	681	rVB5	331	409	0.01%	0.002%
23	5.373	700	703	704	rBV2	852	1115	0.04%	0.007%
24	5.495	721	723	725	rVB3	313	306	0.01%	0.002%
25	5.550	725	732	741	rBV2	3123	9009	0.30%	0.055%
26	5.678	747	753	754	rBV3	590	807	0.03%	0.005%
27	5.812	774	775	778	rVB2	256	226	0.01%	0.001%
28	5.971	787	801	808	rBV2	514060	1559430	51.51%	9.500%
29	6.281	850	852	856	rVB	304	253	0.01%	0.002%
30	6.342	856	862	864	rBV2	253	423	0.01%	0.003%
31	6.537	893	894	896	rBV2	276	199	0.01%	0.001%
32	6.617	905	907	909	rBV	253	200	0.01%	0.001%
33	6.635	909	910	913	rVB2	251	249	0.01%	0.002%
34	6.666	913	915	919	rBV2	188	261	0.01%	0.002%
35	6.763	921	931	949	rBV	456596	1110413	36.68%	6.765%
36	6.983	965	967	969	rBV2	287	266	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035217.D
 Acq On : 20 Apr 2023 15:49
 Operator : JC/MD
 Sample : 02378-15DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	7.117	983	989	996	rBV4	4128	9196	0.30%	0.056%
38	7.172	996	998	1001	rVB2	443	369	0.01%	0.002%
39	7.306	1011	1020	1036	rBV	326385	711615	23.50%	4.335%
40	7.495	1045	1051	1054	rBV3	924	1705	0.06%	0.010%
41	7.757	1092	1094	1097	rVB2	279	229	0.01%	0.001%
42	7.946	1119	1125	1132	rBV3	1580	3746	0.12%	0.023%
43	8.275	1175	1179	1181	rBV	247	447	0.01%	0.003%
44	8.324	1181	1187	1202	rVV	184319	309964	10.24%	1.888%
45	8.494	1211	1215	1219	rBV4	1234	2175	0.07%	0.013%
46	8.647	1234	1240	1255	rBV	764619	1197988	39.57%	7.298%
47	8.952	1284	1290	1305	rBV	128317	194732	6.43%	1.186%
48	9.122	1316	1318	1323	rVB2	289	325	0.01%	0.002%
49	9.189	1327	1329	1331	rVB	371	283	0.01%	0.002%
50	9.220	1331	1334	1335	rBV	196	214	0.01%	0.001%
51	9.299	1346	1347	1351	rBV3	320	221	0.01%	0.001%
52	9.385	1356	1361	1384	rVV	520737	754041	24.91%	4.594%
53	9.665	1406	1407	1410	rVB	409	192	0.01%	0.001%
54	9.720	1413	1416	1417	rVV2	295	284	0.01%	0.002%
55	9.884	1441	1443	1447	rBV2	281	367	0.01%	0.002%
56	10.055	1465	1471	1473	rBV	959880	1455942	48.09%	8.870%
57	10.390	1524	1526	1529	rVV2	294	335	0.01%	0.002%
58	10.433	1532	1533	1536	rVV	323	203	0.01%	0.001%
59	10.531	1547	1549	1552	rBV2	190	248	0.01%	0.002%
60	10.829	1596	1598	1600	rBV2	242	238	0.01%	0.001%
61	11.000	1623	1626	1628	rVB2	268	249	0.01%	0.002%
62	11.024	1628	1630	1632	rBV	232	258	0.01%	0.002%
63	11.189	1652	1657	1673	rVV	558479	743564	24.56%	4.530%
64	11.299	1673	1675	1677	rVB3	375	266	0.01%	0.002%
65	11.323	1677	1679	1680	rBV2	279	232	0.01%	0.001%
66	11.439	1696	1698	1701	rBV3	281	334	0.01%	0.002%
67	11.500	1704	1708	1709	rBV2	287	223	0.01%	0.001%
68	11.610	1724	1726	1728	rBV	341	228	0.01%	0.001%
69	11.707	1739	1742	1745	rBV3	568	783	0.03%	0.005%
70	11.732	1745	1746	1748	rVB2	610	364	0.01%	0.002%
71	11.756	1748	1750	1752	rBV2	229	275	0.01%	0.002%
72	11.890	1769	1772	1774	rVB2	230	266	0.01%	0.002%
73	11.969	1780	1785	1789	rBV	89223	111716	3.69%	0.681%
74	12.036	1789	1796	1810	rVB2	1359920	2877659	95.05%	17.532%
75	12.329	1837	1844	1861	rBV2	1719733	3027518	100.00%	18.445%
76	12.542	1877	1879	1881	rVB2	237	228	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035217.D
 Acq On : 20 Apr 2023 15:49
 Operator : JC/MD
 Sample : 02378-15DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.725	1904	1909	1910	rBV3	317	511	0.02%	0.003%
78	12.756	1912	1914	1915	rVV2	581	432	0.01%	0.003%
79	12.927	1939	1942	1947	rBV3	1395	1949	0.06%	0.012%
80	13.012	1953	1956	1957	rVB	265	203	0.01%	0.001%
81	13.030	1957	1959	1962	rBV2	288	357	0.01%	0.002%
82	13.201	1984	1987	1991	rBV4	677	833	0.03%	0.005%
83	13.378	2014	2016	2019	rBV	287	201	0.01%	0.001%
84	13.475	2028	2032	2034	rVB2	306	415	0.01%	0.003%
85	13.500	2034	2036	2042	rBV2	314	709	0.02%	0.004%
86	13.585	2045	2050	2061	rBV	359636	465791	15.39%	2.838%
87	13.835	2089	2091	2092	rBV	250	198	0.01%	0.001%
88	13.872	2096	2097	2100	rVB2	302	198	0.01%	0.001%
89	13.908	2100	2103	2106	rVB2	278	336	0.01%	0.002%
90	13.963	2107	2112	2120	rVV	63345	83168	2.75%	0.507%
91	14.128	2136	2139	2145	rVB3	962	1199	0.04%	0.007%
92	14.274	2161	2163	2166	rVB3	314	286	0.01%	0.002%
93	14.335	2172	2173	2177	rBV3	327	404	0.01%	0.002%
94	14.554	2207	2209	2210	rVB2	554	258	0.01%	0.002%
95	14.725	2236	2237	2239	rBV2	489	355	0.01%	0.002%
96	14.786	2243	2247	2251	rVB4	4218	5584	0.18%	0.034%
97	14.908	2265	2267	2269	rBV2	730	541	0.02%	0.003%
98	14.987	2279	2280	2281	rBV	575	324	0.01%	0.002%
99	15.249	2319	2323	2329	rVB2	11629	16265	0.54%	0.099%
100	15.963	2439	2440	2442	rBV	726	489	0.02%	0.003%




Sum of corrected areas: 16414192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035217.D
Acq On : 20 Apr 2023 15:49
Operator : JC/MD
Sample : 02378-15DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMK8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

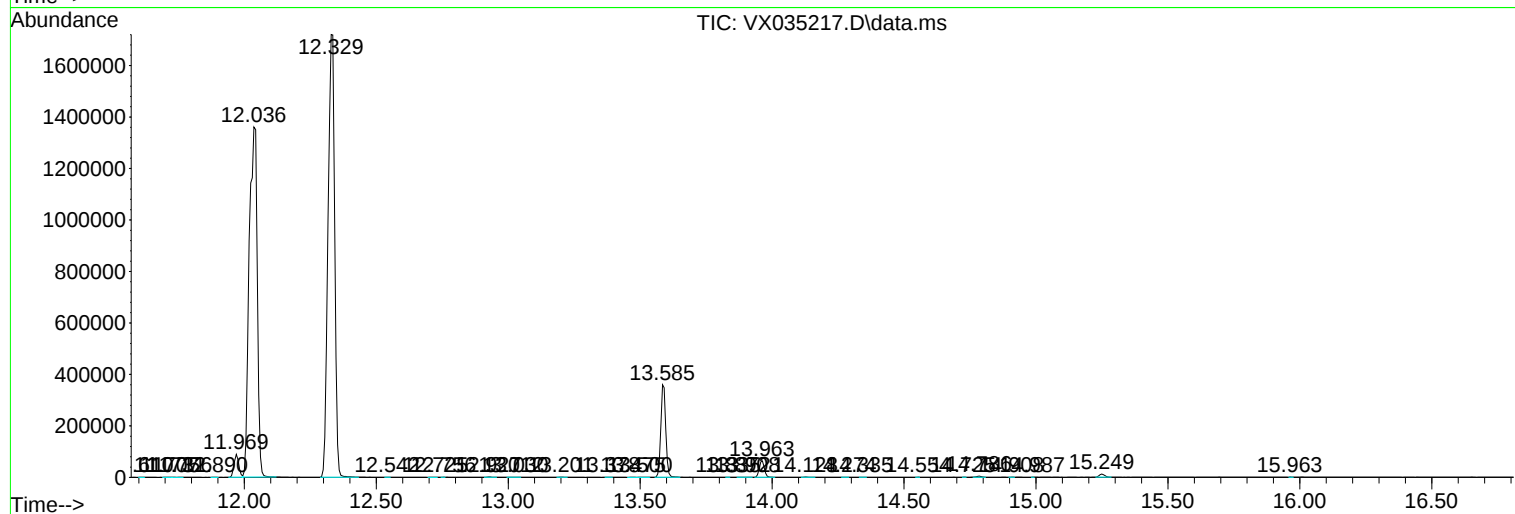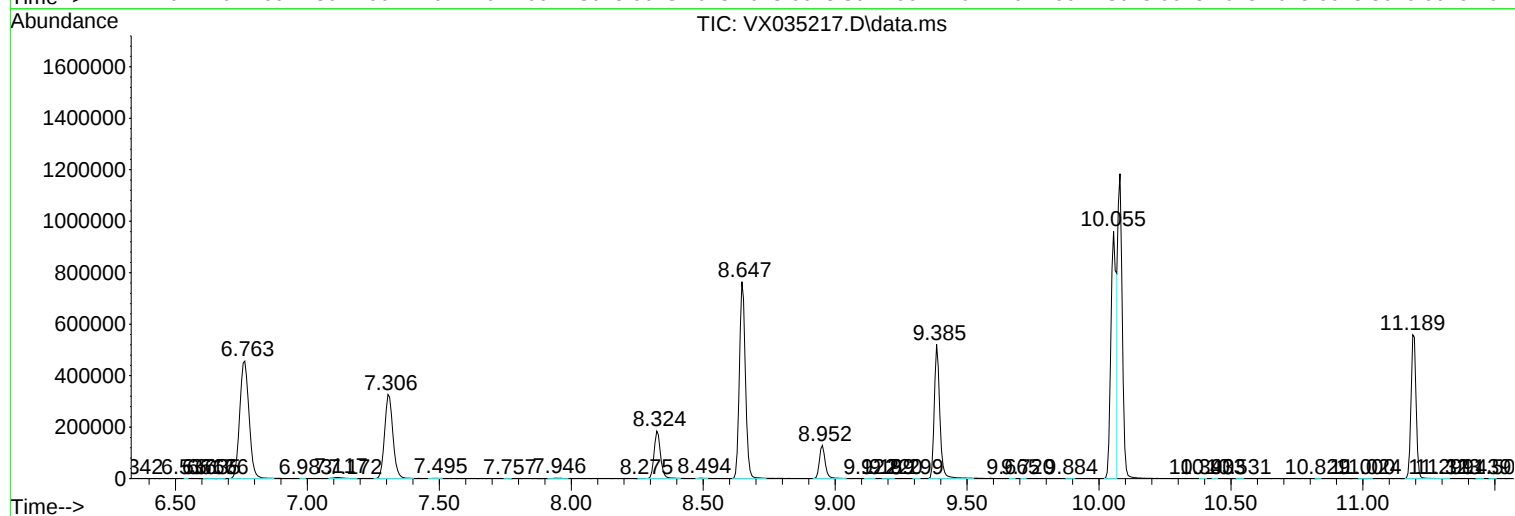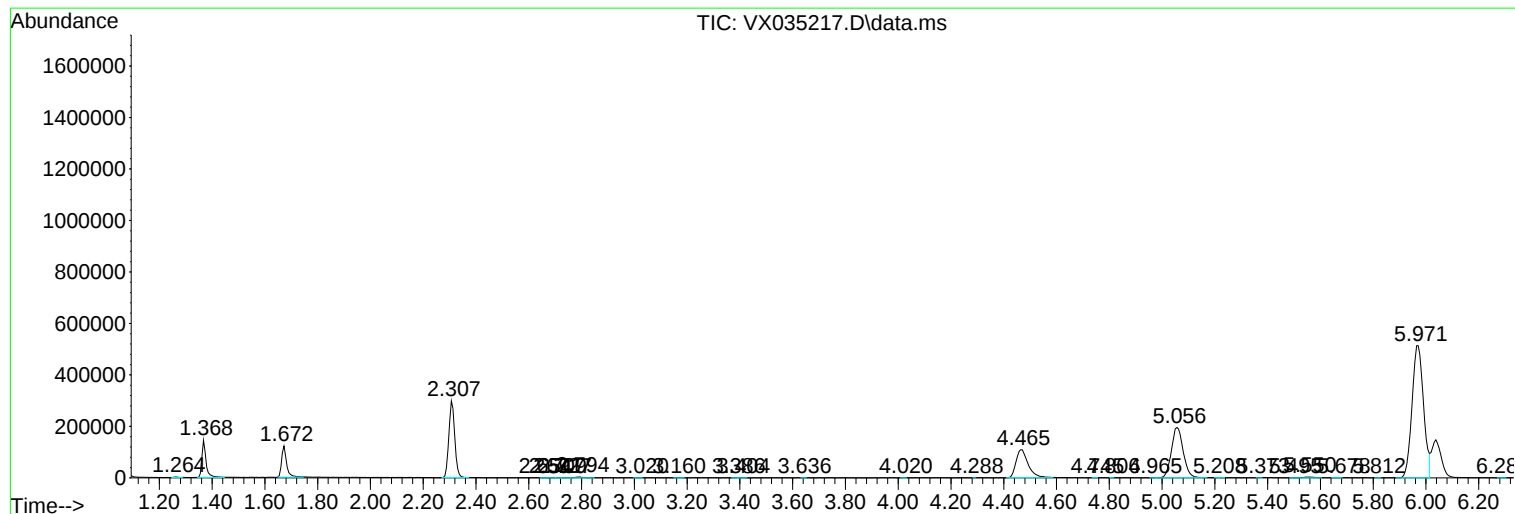

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035217.D
Acq On : 20 Apr 2023 15:49
Operator : JC/MD
Sample : 02378-15DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035217.D
Acq On : 20 Apr 2023 15:49
Operator : JC/MD
Sample : 02378-15DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------