

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035218.D
 Acq On : 20 Apr 2023 16:12
 Operator : JC/MD
 Sample : 02378-14DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2358	1969	0.04%	0.009%
2	1.368	42	46	60	rBV	146856	163732	3.01%	0.755%
3	1.672	91	96	106	rBV	127786	167991	3.09%	0.775%
4	2.306	194	200	211	rBV	301671	473602	8.72%	2.185%
5	2.514	231	234	237	rBV2	526	597	0.01%	0.003%
6	2.623	247	252	255	rBV3	439	575	0.01%	0.003%
7	2.739	269	271	273	rVV2	345	297	0.01%	0.001%
8	2.788	275	279	286	rVB2	2963	5555	0.10%	0.026%
9	2.940	303	304	308	rVB3	396	411	0.01%	0.002%
10	3.014	314	316	318	rVB	319	226	0.00%	0.001%
11	3.038	318	320	325	rBV2	187	198	0.00%	0.001%
12	3.075	325	326	329	rVB	263	210	0.00%	0.001%
13	3.135	334	336	339	rVB2	301	231	0.00%	0.001%
14	3.239	350	353	354	rBV2	271	212	0.00%	0.001%
15	3.556	403	405	408	rBV2	267	307	0.01%	0.001%
16	3.648	416	420	421	rBV2	241	326	0.01%	0.002%
17	3.727	429	433	435	rBV	258	261	0.00%	0.001%
18	3.824	446	449	451	rBV2	187	199	0.00%	0.001%
19	3.910	459	463	466	rBV2	237	277	0.01%	0.001%
20	3.971	470	473	476	rBV2	188	293	0.01%	0.001%
21	4.038	481	484	485	rBV	309	208	0.00%	0.001%
22	4.056	485	487	491	rBV	211	316	0.01%	0.001%
23	4.294	523	526	527	rBV3	425	436	0.01%	0.002%
24	4.379	539	540	545	rBV2	281	339	0.01%	0.002%
25	4.471	545	555	575	rBV2	107742	362511	6.67%	1.673%
26	4.733	597	598	601	rBV	393	339	0.01%	0.002%
27	4.763	601	603	606	rBV2	318	288	0.01%	0.001%
28	4.867	618	620	626	rBV3	302	489	0.01%	0.002%
29	5.062	640	652	670	rVV	204744	637482	11.73%	2.941%
30	5.330	694	696	698	rVB2	269	206	0.00%	0.001%
31	5.355	698	700	701	rVB2	495	257	0.00%	0.001%
32	5.379	701	704	705	rBV	443	509	0.01%	0.002%
33	5.556	727	733	739	rBV3	1804	4043	0.07%	0.019%
34	5.678	745	753	761	rVB5	2050	5594	0.10%	0.026%
35	5.739	761	763	768	rVB	376	480	0.01%	0.002%
36	5.787	768	771	773	rBV2	202	226	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035218.D
 Acq On : 20 Apr 2023 16:12
 Operator : JC/MD
 Sample : 02378-14DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	5.970	789	801	807	rBV2	537707	1589297	29.25%	7.333%
38	6.342	860	862	867	rVB2	387	536	0.01%	0.002%
39	6.385	867	869	870	rBV2	282	227	0.00%	0.001%
40	6.470	881	883	887	rVB2	414	472	0.01%	0.002%
41	6.507	887	889	891	rBV	296	239	0.00%	0.001%
42	6.550	893	896	897	rVV2	318	306	0.01%	0.001%
43	6.598	902	904	907	rBV	166	254	0.00%	0.001%
44	6.763	921	931	951	rBV	438896	1064706	19.60%	4.913%
45	6.946	960	961	965	rBV2	399	249	0.00%	0.001%
46	7.123	980	990	1002	rVB4	3985	10912	0.20%	0.050%
47	7.305	1011	1020	1038	rBV	331023	737109	13.57%	3.401%
48	7.641	1073	1075	1079	rVB	330	368	0.01%	0.002%
49	7.940	1118	1124	1133	rVV4	1555	3738	0.07%	0.017%
50	8.074	1144	1146	1147	rBV	310	186	0.00%	0.001%
51	8.086	1147	1148	1150	rBV	235	187	0.00%	0.001%
52	8.214	1166	1169	1170	rBV2	241	221	0.00%	0.001%
53	8.226	1170	1171	1174	rVB2	225	238	0.00%	0.001%
54	8.324	1181	1187	1202	rBV	197619	322351	5.93%	1.487%
55	8.567	1225	1227	1230	rBV3	382	409	0.01%	0.002%
56	8.647	1234	1240	1257	rVV	774751	1235676	22.74%	5.701%
57	8.952	1284	1290	1301	rBV	139712	207440	3.82%	0.957%
58	9.281	1340	1344	1346	rBV3	529	582	0.01%	0.003%
59	9.384	1356	1361	1382	rBV	549024	785116	14.45%	3.623%
60	9.701	1410	1413	1416	rBV	379	520	0.01%	0.002%
61	9.738	1416	1419	1420	rBV	382	299	0.01%	0.001%
62	9.909	1446	1447	1450	rVB2	324	293	0.01%	0.001%
63	10.079	1465	1475	1491	rBV2	3187685	5433261	100.00%	25.069%
64	10.366	1520	1522	1524	rVB2	464	272	0.01%	0.001%
65	10.598	1558	1560	1565	rVB3	388	339	0.01%	0.002%
66	10.793	1589	1592	1593	rBV	275	213	0.00%	0.001%
67	10.890	1607	1608	1612	rVB3	337	406	0.01%	0.002%
68	10.921	1612	1613	1615	rBV	259	250	0.00%	0.001%
69	11.085	1638	1640	1646	rBV2	413	493	0.01%	0.002%
70	11.189	1652	1657	1666	rBV	577688	774030	14.25%	3.571%
71	11.421	1692	1695	1698	rVV2	222	231	0.00%	0.001%
72	11.451	1698	1700	1703	rVB3	242	265	0.00%	0.001%
73	11.671	1734	1736	1741	rVB2	287	246	0.00%	0.001%
74	11.707	1741	1742	1745	rBV2	558	505	0.01%	0.002%
75	11.811	1757	1759	1760	rBV	386	183	0.00%	0.001%
76	11.969	1780	1785	1789	rBV	198345	249722	4.60%	1.152%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035218.D
 Acq On : 20 Apr 2023 16:12
 Operator : JC/MD
 Sample : 02378-14DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0MK7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.036	1789	1796	1810	rVB2	1773239	3349099	61.64%	15.453%
78	12.256	1831	1832	1835	rBV2	349	285	0.01%	0.001%
79	12.329	1837	1844	1865	rVB2	1878265	3337960	61.44%	15.401%
80	12.756	1911	1914	1916	rBV2	583	707	0.01%	0.003%
81	12.926	1938	1942	1946	rVB2	3121	4081	0.08%	0.019%
82	13.061	1961	1964	1969	rVB4	1152	1983	0.04%	0.009%
83	13.122	1969	1974	1975	rBV2	539	677	0.01%	0.003%
84	13.201	1984	1987	1991	rVB2	1687	1883	0.03%	0.009%
85	13.371	2012	2015	2017	rBV2	221	265	0.00%	0.001%
86	13.585	2045	2050	2060	rBV	442751	547470	10.08%	2.526%
87	13.731	2072	2074	2078	rBV2	271	347	0.01%	0.002%
88	13.774	2080	2081	2086	rBV2	436	571	0.01%	0.003%
89	13.963	2106	2112	2120	rBV	120527	155041	2.85%	0.715%
90	14.060	2126	2128	2129	rBV2	328	185	0.00%	0.001%
91	14.127	2137	2139	2145	rVB3	887	1447	0.03%	0.007%
92	14.176	2145	2147	2150	rVB	263	303	0.01%	0.001%
93	14.213	2150	2153	2155	rBV2	414	433	0.01%	0.002%
94	14.700	2231	2233	2235	rBV2	378	336	0.01%	0.002%
95	14.725	2235	2237	2239	rBV	355	373	0.01%	0.002%
96	14.780	2244	2246	2251	rVB4	2382	2927	0.05%	0.014%
97	14.865	2258	2260	2263	rBV3	447	437	0.01%	0.002%
98	15.249	2319	2323	2328	rBV4	8460	11595	0.21%	0.053%
99	16.072	2456	2458	2459	rBV2	711	440	0.01%	0.002%
100	16.328	2498	2500	2504	rBV3	756	822	0.02%	0.004%




Sum of corrected areas: 21673206

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035218.D
Acq On : 20 Apr 2023 16:12
Operator : JC/MD
Sample : 02378-14DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMK7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

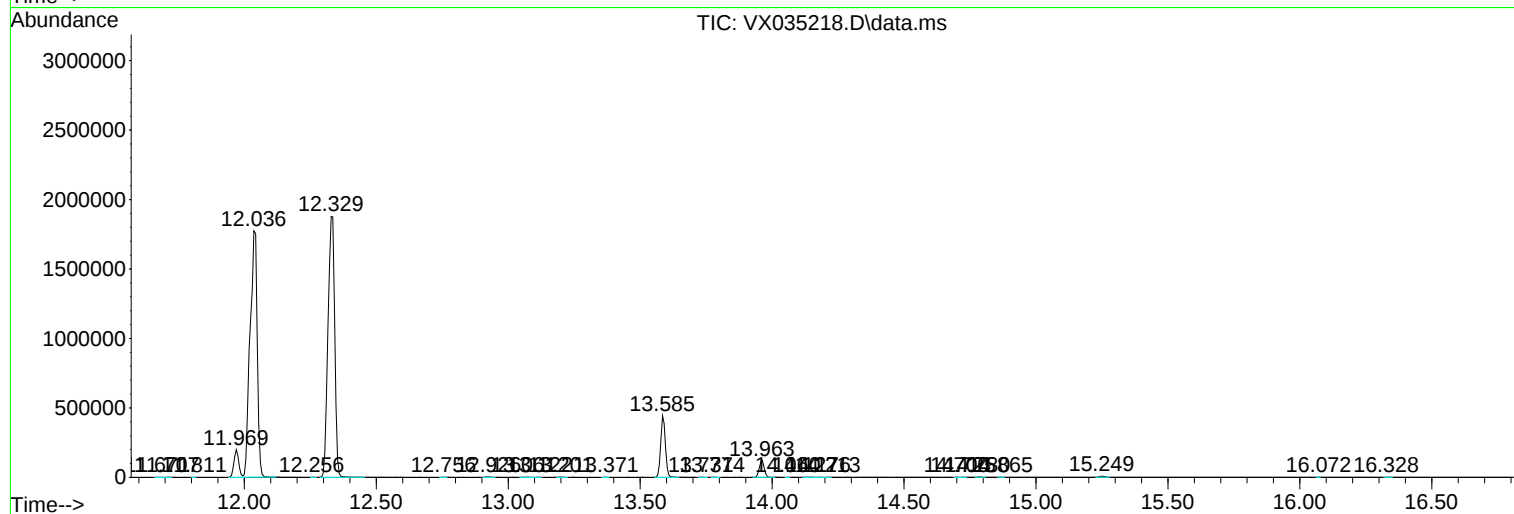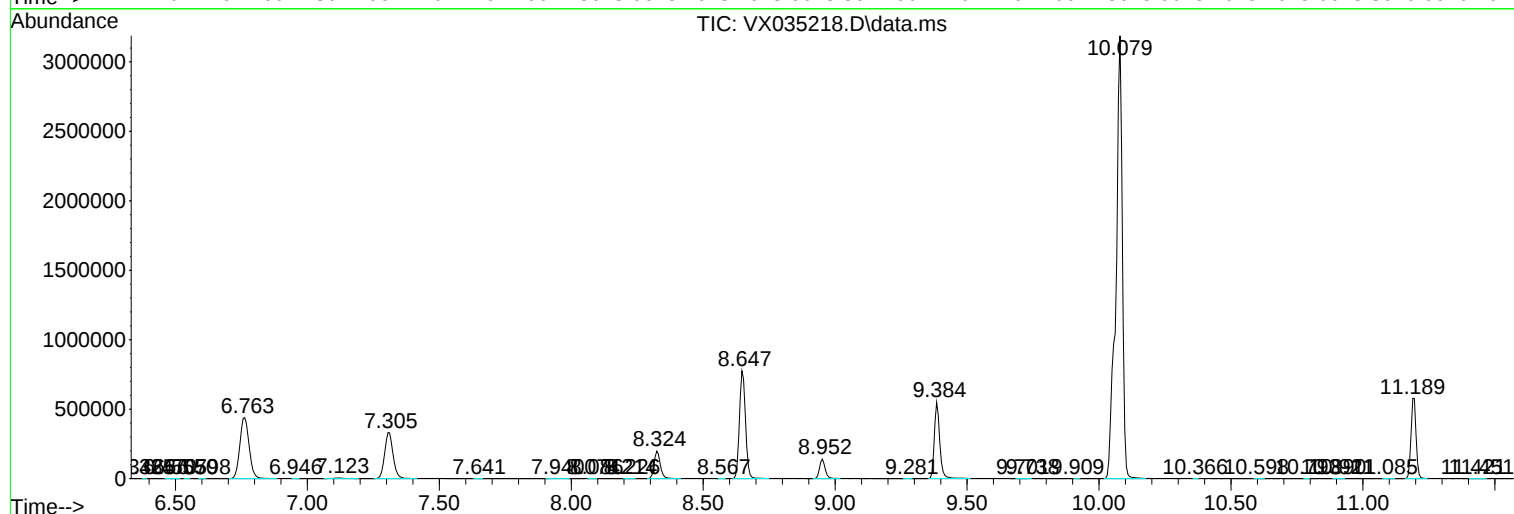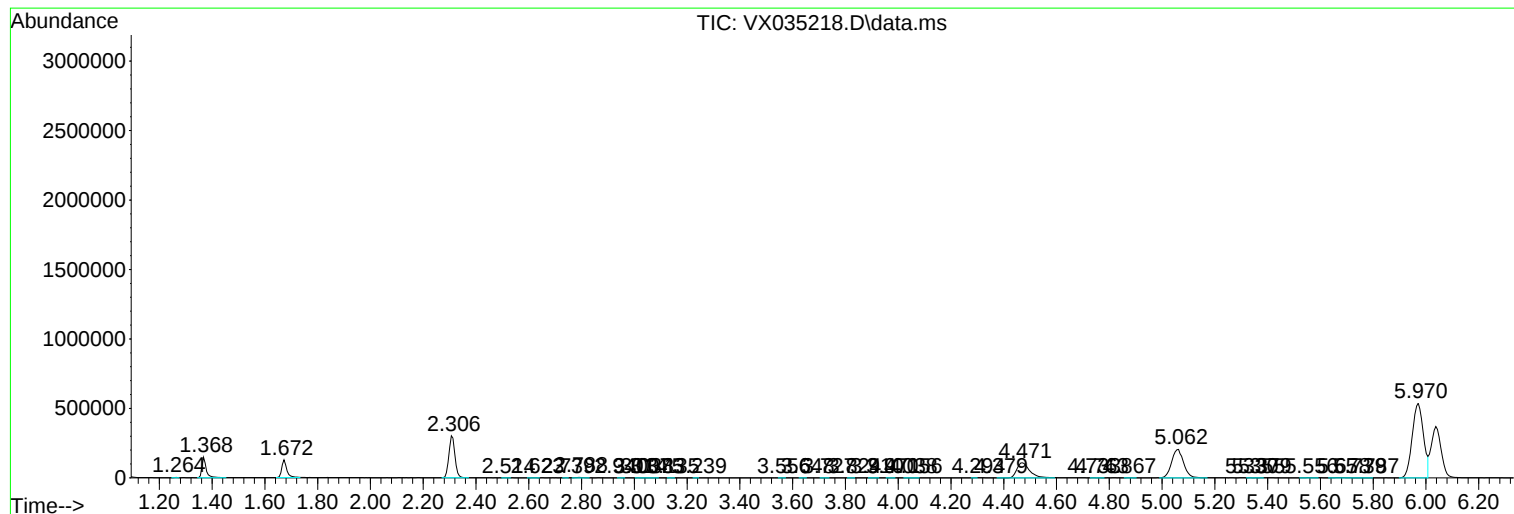

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035218.D
Acq On : 20 Apr 2023 16:12
Operator : JC/MD
Sample : 02378-14DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035218.D
Acq On : 20 Apr 2023 16:12
Operator : JC/MD
Sample : 02378-14DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------