

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035219.D
 Acq On : 20 Apr 2023 16:35
 Operator : JC/MD
 Sample : 02378-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	35	rBV3	2815	3274	0.04%	0.016%
2	1.368	42	46	57	rBV	141933	158392	2.00%	0.780%
3	1.673	91	96	104	rBV	119227	155872	1.97%	0.767%
4	2.307	193	200	211	rBV	289038	453453	5.72%	2.232%
5	2.782	276	278	279	rBV2	967	824	0.01%	0.004%
6	2.855	287	290	291	rBV2	306	265	0.00%	0.001%
7	2.941	296	304	315	rBV2	14151	32105	0.40%	0.158%
8	3.105	328	331	335	rBV2	605	1091	0.01%	0.005%
9	3.233	350	352	353	rVB2	453	307	0.00%	0.002%
10	3.447	383	387	389	rVV3	245	275	0.00%	0.001%
11	3.544	402	403	406	rBV2	209	212	0.00%	0.001%
12	3.593	409	411	413	rBV	208	214	0.00%	0.001%
13	3.636	413	418	421	rVB2	227	342	0.00%	0.002%
14	3.678	421	425	428	rBV2	273	256	0.00%	0.001%
15	3.739	433	435	439	rVB2	257	235	0.00%	0.001%
16	3.782	439	442	445	rBV2	273	331	0.00%	0.002%
17	3.831	449	450	453	rVB2	216	199	0.00%	0.001%
18	4.001	476	478	481	rBV2	269	350	0.00%	0.002%
19	4.099	492	494	497	rVB3	240	237	0.00%	0.001%
20	4.160	501	504	505	rBV2	308	236	0.00%	0.001%
21	4.257	516	520	523	rVB2	214	225	0.00%	0.001%
22	4.294	523	526	527	rBV	335	311	0.00%	0.002%
23	4.465	545	554	566	rBV	111485	339504	4.28%	1.671%
24	4.904	624	626	628	rBV	509	499	0.01%	0.002%
25	5.056	640	651	669	rBV	193164	605855	7.64%	2.982%
26	5.312	688	693	695	rBV3	376	575	0.01%	0.003%
27	5.361	698	701	702	rBV	312	328	0.00%	0.002%
28	5.379	702	704	705	rBV	408	337	0.00%	0.002%
29	5.452	715	716	718	rBV	206	203	0.00%	0.001%
30	5.507	724	725	727	rVB	332	214	0.00%	0.001%
31	5.550	727	732	734	rBV4	2192	3773	0.05%	0.019%
32	5.678	750	753	755	rVB2	266	298	0.00%	0.001%
33	5.733	760	762	764	rBV2	243	214	0.00%	0.001%
34	5.971	789	801	820	rBV2	517078	1551083	19.56%	7.635%
35	6.141	827	829	831	rVB3	395	278	0.00%	0.001%
36	6.233	842	844	846	rVB2	315	259	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035219.D
 Acq On : 20 Apr 2023 16:35
 Operator : JC/MD
 Sample : 02378-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.428	873	876	878	rBV	212	286	0.00%	0.001%
38	6.483	883	885	887	rVB	238	210	0.00%	0.001%
39	6.531	891	893	894	rBV2	323	241	0.00%	0.001%
40	6.556	894	897	898	rBV2	250	283	0.00%	0.001%
41	6.672	914	916	919	rBV2	209	230	0.00%	0.001%
42	6.763	921	931	944	rBV	422599	1010605	12.74%	4.975%
43	6.964	962	964	967	rVB	297	202	0.00%	0.001%
44	7.019	970	973	974	rBV2	350	308	0.00%	0.002%
45	7.117	981	989	1002	rBV4	4222	10148	0.13%	0.050%
46	7.306	1011	1020	1035	rBV	320257	715497	9.02%	3.522%
47	7.629	1070	1073	1074	rBV2	306	244	0.00%	0.001%
48	7.720	1086	1088	1090	rBV2	302	342	0.00%	0.002%
49	7.940	1119	1124	1130	rBV3	1704	3319	0.04%	0.016%
50	8.068	1141	1145	1148	rBV2	358	614	0.01%	0.003%
51	8.226	1169	1171	1176	rVB2	247	290	0.00%	0.001%
52	8.324	1181	1187	1205	rBV	191092	315466	3.98%	1.553%
53	8.482	1211	1213	1214	rBV	719	520	0.01%	0.003%
54	8.647	1234	1240	1260	rVV	748030	1193815	15.05%	5.877%
55	8.952	1284	1290	1305	rBV	136680	203554	2.57%	1.002%
56	9.110	1315	1316	1320	rVB2	406	368	0.00%	0.002%
57	9.214	1331	1333	1335	rBV2	402	280	0.00%	0.001%
58	9.275	1339	1343	1350	rBV2	1693	3109	0.04%	0.015%
59	9.385	1356	1361	1377	rBV	527851	752659	9.49%	3.705%
60	9.647	1402	1404	1407	rVB3	373	324	0.00%	0.002%
61	9.933	1448	1451	1452	rBV2	195	199	0.00%	0.001%
62	10.080	1465	1475	1499	rBV2	5108865	7930775	100.00%	39.040%
63	10.592	1557	1559	1561	rVB	307	236	0.00%	0.001%
64	10.622	1561	1564	1568	rBV2	320	449	0.01%	0.002%
65	10.927	1612	1614	1615	rVB	341	214	0.00%	0.001%
66	10.964	1615	1620	1622	rBV	416	478	0.01%	0.002%
67	11.018	1626	1629	1632	rBV2	305	449	0.01%	0.002%
68	11.085	1635	1640	1643	rBV3	340	496	0.01%	0.002%
69	11.189	1652	1657	1666	rBV	569255	751386	9.47%	3.699%
70	11.311	1674	1677	1682	rVV	2208	2888	0.04%	0.014%
71	11.366	1684	1686	1691	rVB2	774	1082	0.01%	0.005%
72	11.451	1697	1700	1703	rBV4	238	409	0.01%	0.002%
73	11.713	1741	1743	1745	rVB2	500	334	0.00%	0.002%
74	11.744	1745	1748	1750	rBV2	312	356	0.00%	0.002%
75	11.841	1762	1764	1767	rVB2	316	198	0.00%	0.001%
76	11.927	1777	1778	1780	rBV	330	253	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035219.D
 Acq On : 20 Apr 2023 16:35
 Operator : JC/MD
 Sample : 02378-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	11.969	1780	1785	1789	rBV	71119	89798	1.13%	0.442%
78	12.024	1789	1794	1811	rVB2	890982	1811462	22.84%	8.917%
79	12.225	1822	1827	1837	rBV3	2574	4451	0.06%	0.022%
80	12.323	1837	1843	1864	rVB2	1146453	2117330	26.70%	10.423%
81	12.512	1871	1874	1877	rVB2	375	419	0.01%	0.002%
82	12.536	1877	1878	1882	rBV2	311	205	0.00%	0.001%
83	12.713	1905	1907	1909	rVB2	266	226	0.00%	0.001%
84	12.768	1913	1916	1920	rVB2	730	739	0.01%	0.004%
85	12.866	1929	1932	1935	rVB2	212	286	0.00%	0.001%
86	12.945	1942	1945	1947	rVB2	200	217	0.00%	0.001%
87	13.158	1978	1980	1982	rBV2	268	243	0.00%	0.001%
88	13.244	1991	1994	1997	rBV	294	347	0.00%	0.002%
89	13.298	1999	2003	2004	rBV2	319	296	0.00%	0.001%
90	13.506	2035	2037	2039	rBV2	281	314	0.00%	0.002%
91	13.585	2046	2050	2059	rVV	40793	56593	0.71%	0.279%
92	13.786	2079	2083	2084	rBV	292	330	0.00%	0.002%
93	13.847	2092	2093	2095	rBV2	240	235	0.00%	0.001%
94	13.963	2108	2112	2117	rVB	7545	9586	0.12%	0.047%
95	14.128	2134	2139	2144	rVV3	1058	1821	0.02%	0.009%
96	14.640	2221	2223	2225	rBV2	393	246	0.00%	0.001%
97	15.066	2291	2293	2296	rBV3	420	364	0.00%	0.002%
98	15.255	2320	2324	2329	rVB3	2069	2756	0.03%	0.014%
99	15.914	2430	2432	2433	rBV2	590	255	0.00%	0.001%
100	16.152	2470	2471	2473	rBV	547	415	0.01%	0.002%


Sum of corrected areas: 20314476

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035219.D
Acq On : 20 Apr 2023 16:35
Operator : JC/MD
Sample : 02378-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

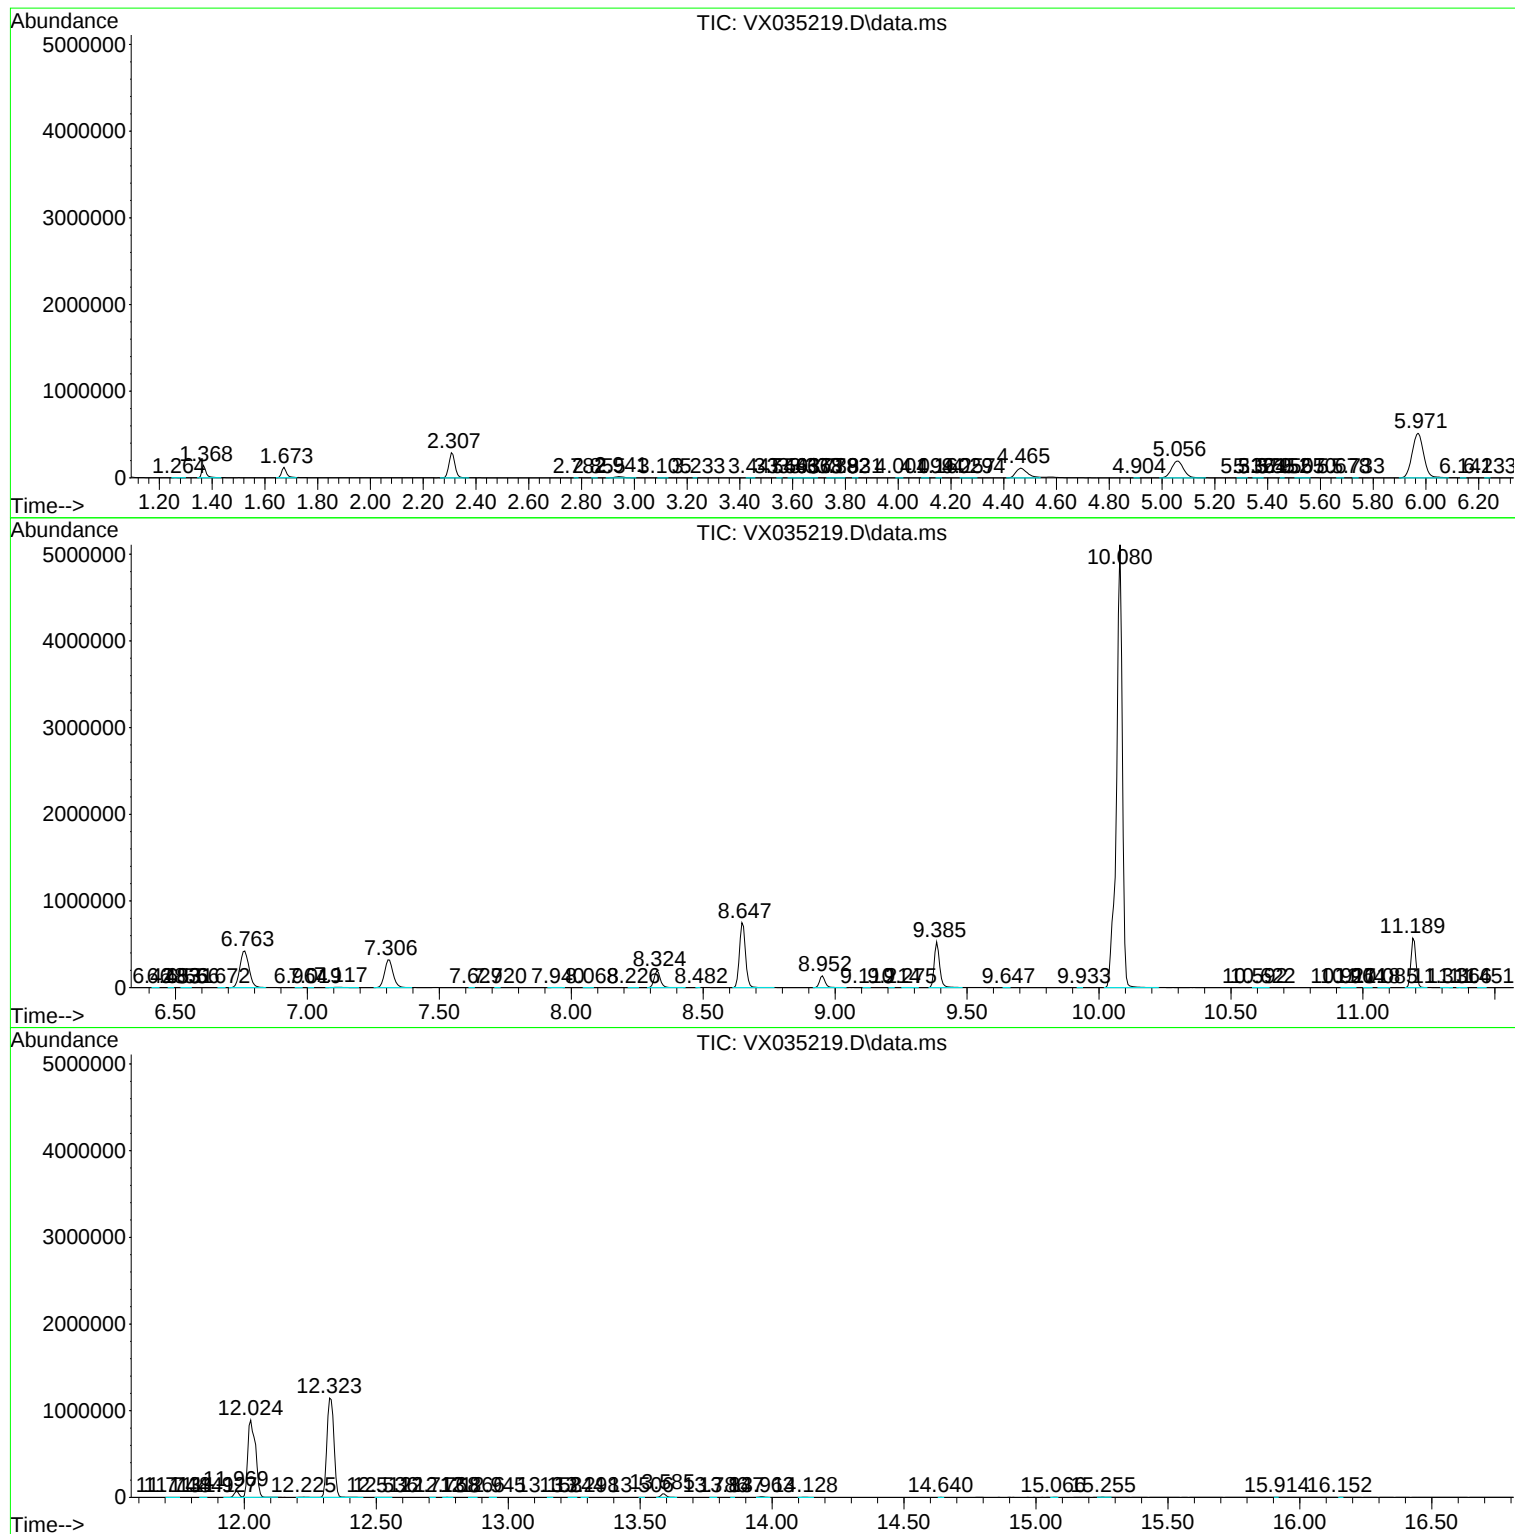

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035219.D
Acq On : 20 Apr 2023 16:35
Operator : JC/MD
Sample : 02378-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035219.D
Acq On : 20 Apr 2023 16:35
Operator : JC/MD
Sample : 02378-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------