

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035221.D
 Acq On : 20 Apr 2023 17:22
 Operator : JC/MD
 Sample : 02378-10DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2037	2002	0.13%	0.017%
2	1.368	42	46	58	rBV	156318	173581	11.67%	1.506%
3	1.672	92	96	107	rBV	123688	159089	10.69%	1.380%
4	2.307	194	200	212	rVV	317936	499004	33.54%	4.328%
5	2.404	214	216	221	rVB2	957	1020	0.07%	0.009%
6	2.654	255	257	258	rBV	270	219	0.01%	0.002%
7	2.788	272	279	289	rBV2	12425	23744	1.60%	0.206%
8	2.947	299	305	312	rVB2	3314	7719	0.52%	0.067%
9	3.099	328	330	331	rBV2	292	226	0.02%	0.002%
10	3.349	368	371	373	rVB3	289	372	0.03%	0.003%
11	3.380	373	376	381	rBV3	356	548	0.04%	0.005%
12	3.483	388	393	394	rBV3	346	408	0.03%	0.004%
13	3.593	408	411	413	rBV	221	247	0.02%	0.002%
14	3.636	414	418	421	rVB	262	253	0.02%	0.002%
15	3.678	421	425	427	rBV2	164	183	0.01%	0.002%
16	3.727	430	433	436	rVB2	349	431	0.03%	0.004%
17	3.922	463	465	466	rVB	382	179	0.01%	0.002%
18	3.940	466	468	470	rBV2	234	244	0.02%	0.002%
19	4.014	478	480	482	rVV2	238	207	0.01%	0.002%
20	4.349	534	535	539	rVB	295	247	0.02%	0.002%
21	4.471	546	555	574	rBV	97482	319869	21.50%	2.775%
22	4.769	603	604	607	rVB2	393	255	0.02%	0.002%
23	4.940	631	632	635	rBV3	314	218	0.01%	0.002%
24	5.056	638	651	669	rBV	191691	579663	38.96%	5.028%
25	5.373	701	703	705	rBV3	682	824	0.06%	0.007%
26	5.471	717	719	721	rBV	239	291	0.02%	0.003%
27	5.562	725	734	738	rBV3	2405	5642	0.38%	0.049%
28	5.690	753	755	757	rVV2	226	234	0.02%	0.002%
29	5.714	757	759	761	rVV2	214	182	0.01%	0.002%
30	5.806	773	774	776	rBV	383	194	0.01%	0.002%
31	5.867	782	784	785	rBV	257	196	0.01%	0.002%
32	5.971	788	801	818	rBV2	500613	1487927	100.00%	12.906%
33	6.324	856	859	860	rBV2	229	204	0.01%	0.002%
34	6.373	865	867	869	rVB2	243	167	0.01%	0.001%
35	6.409	870	873	876	rVB	210	181	0.01%	0.002%
36	6.458	879	881	886	rVB3	436	664	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035221.D
 Acq On : 20 Apr 2023 17:22
 Operator : JC/MD
 Sample : 02378-10DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.763	921	931	947	rVV	382758	924657	62.14%	8.020%
38	7.117	982	989	999	rVB4	3965	9794	0.66%	0.085%
39	7.190	999	1001	1002	rBV2	304	171	0.01%	0.001%
40	7.208	1002	1004	1006	rVB	429	313	0.02%	0.003%
41	7.306	1011	1020	1037	rBV	305612	679415	45.66%	5.893%
42	7.470	1043	1047	1048	rBV3	487	611	0.04%	0.005%
43	7.690	1081	1083	1086	rVB2	264	290	0.02%	0.003%
44	7.946	1121	1125	1130	rBV4	1145	2391	0.16%	0.021%
45	8.159	1159	1160	1163	rBV	223	245	0.02%	0.002%
46	8.196	1163	1166	1170	rVB3	323	463	0.03%	0.004%
47	8.226	1170	1171	1173	rBV2	195	211	0.01%	0.002%
48	8.324	1181	1187	1203	rBV	177881	294780	19.81%	2.557%
49	8.501	1212	1216	1226	rVB7	762	2308	0.16%	0.020%
50	8.647	1234	1240	1260	rBV	763175	1200200	80.66%	10.411%
51	8.872	1275	1277	1279	rVB2	716	520	0.03%	0.005%
52	8.897	1279	1281	1283	rBV2	293	321	0.02%	0.003%
53	8.952	1284	1290	1306	rVV	124712	185960	12.50%	1.613%
54	9.220	1332	1334	1336	rBV	341	242	0.02%	0.002%
55	9.281	1339	1344	1347	rBV3	1105	1538	0.10%	0.013%
56	9.385	1356	1361	1376	rBV	465997	677328	45.52%	5.875%
57	9.641	1401	1403	1404	rBV2	481	462	0.03%	0.004%
58	9.702	1411	1413	1415	rBV	231	169	0.01%	0.001%
59	10.055	1465	1471	1473	rBV	791761	1205389	81.01%	10.456%
60	10.305	1510	1512	1518	rVB3	691	1138	0.08%	0.010%
61	10.457	1535	1537	1538	rBV	221	204	0.01%	0.002%
62	10.537	1549	1550	1552	rBV	304	220	0.01%	0.002%
63	10.640	1564	1567	1569	rBV2	460	489	0.03%	0.004%
64	10.701	1575	1577	1580	rVB2	300	246	0.02%	0.002%
65	11.092	1639	1641	1645	rVB3	838	977	0.07%	0.008%
66	11.189	1652	1657	1671	rBV	518152	684356	45.99%	5.936%
67	11.555	1715	1717	1720	rBV2	272	326	0.02%	0.003%
68	11.622	1726	1728	1731	rBV2	329	237	0.02%	0.002%
69	11.701	1739	1741	1744	rVB3	452	401	0.03%	0.003%
70	11.762	1748	1751	1754	rVB3	546	731	0.05%	0.006%
71	11.902	1773	1774	1777	rBV3	261	262	0.02%	0.002%
72	11.969	1780	1785	1789	rBV	14449	18780	1.26%	0.163%
73	12.024	1789	1794	1807	rVB2	773074	1122148	75.42%	9.734%
74	12.165	1815	1817	1819	rBV2	355	294	0.02%	0.003%
75	12.225	1824	1827	1834	rVB6	1224	2038	0.14%	0.018%
76	12.317	1837	1842	1854	rBV2	799876	1215520	81.69%	10.543%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035221.D
 Acq On : 20 Apr 2023 17:22
 Operator : JC/MD
 Sample : 02378-10DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMK3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

77	12.555	1879	1881	1887	rVB2	262	304	0.02%	0.003%
78	12.768	1910	1916	1918	rVB2	545	994	0.07%	0.009%
79	12.890	1935	1936	1940	rVB2	480	288	0.02%	0.002%
80	12.927	1940	1942	1945	rVB2	288	282	0.02%	0.002%
81	13.036	1957	1960	1963	rBV	216	273	0.02%	0.002%
82	13.274	1998	1999	2002	rBV2	228	167	0.01%	0.001%
83	13.347	2006	2011	2013	rBV2	306	392	0.03%	0.003%
84	13.451	2026	2028	2030	rBV2	273	208	0.01%	0.002%
85	13.591	2046	2051	2056	rBV	11762	15040	1.01%	0.130%
86	13.731	2072	2074	2078	rBV2	202	359	0.02%	0.003%
87	13.768	2078	2080	2082	rVV2	448	530	0.04%	0.005%
88	13.811	2086	2087	2089	rVB2	509	275	0.02%	0.002%
89	13.865	2094	2096	2097	rBV	281	172	0.01%	0.001%
90	13.969	2109	2113	2120	rVB3	1739	2521	0.17%	0.022%
91	14.024	2120	2122	2124	rBV	355	283	0.02%	0.002%
92	14.109	2133	2136	2137	rBV2	359	317	0.02%	0.003%
93	14.134	2137	2140	2143	rVV2	1176	1489	0.10%	0.013%
94	14.189	2146	2149	2152	rBV2	416	498	0.03%	0.004%
95	14.280	2163	2164	2166	rBV	358	221	0.01%	0.002%
96	14.323	2170	2171	2173	rBV2	293	215	0.01%	0.002%
97	14.371	2177	2179	2182	rVB	293	202	0.01%	0.002%
98	14.512	2200	2202	2203	rVB	364	229	0.02%	0.002%
99	14.530	2203	2205	2206	rBV	343	275	0.02%	0.002%
100	14.884	2261	2263	2264	rBV	469	373	0.03%	0.003%




Sum of corrected areas: 11528686

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035221.D
Acq On : 20 Apr 2023 17:22
Operator : JC/MD
Sample : 02378-10DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

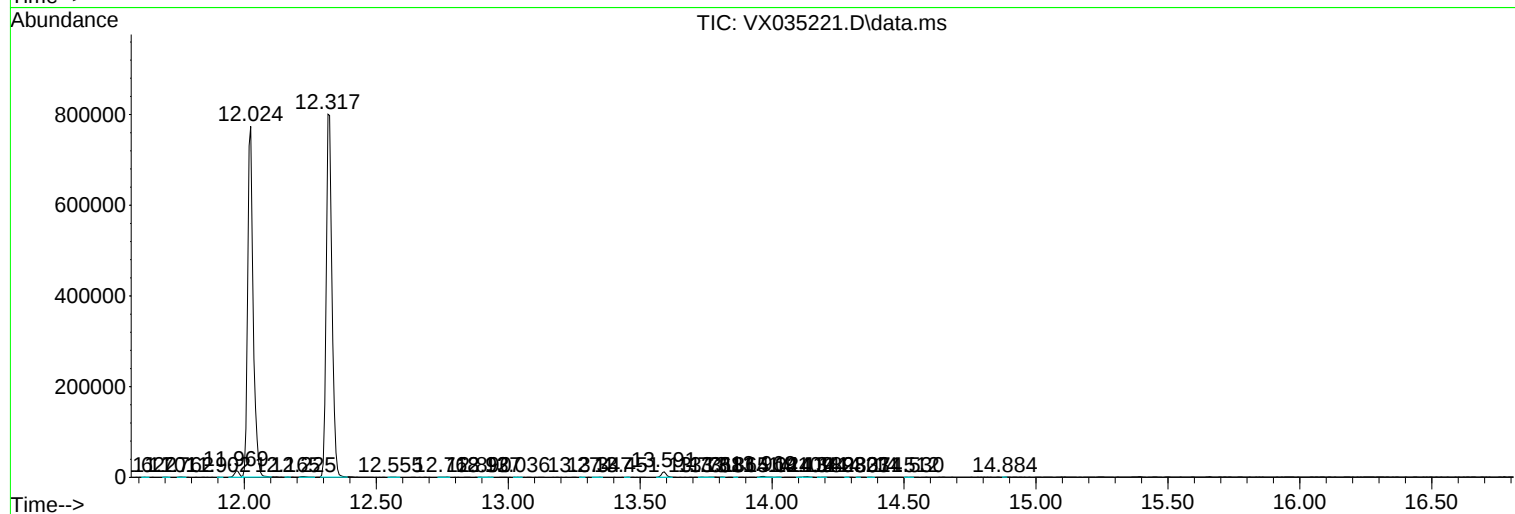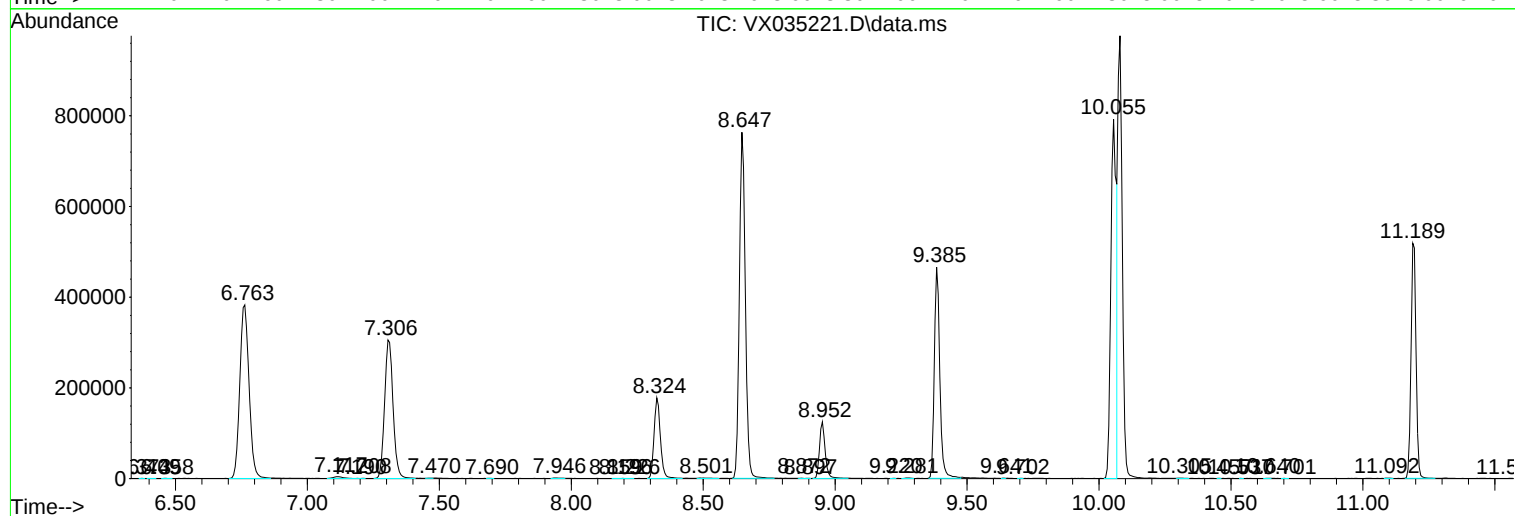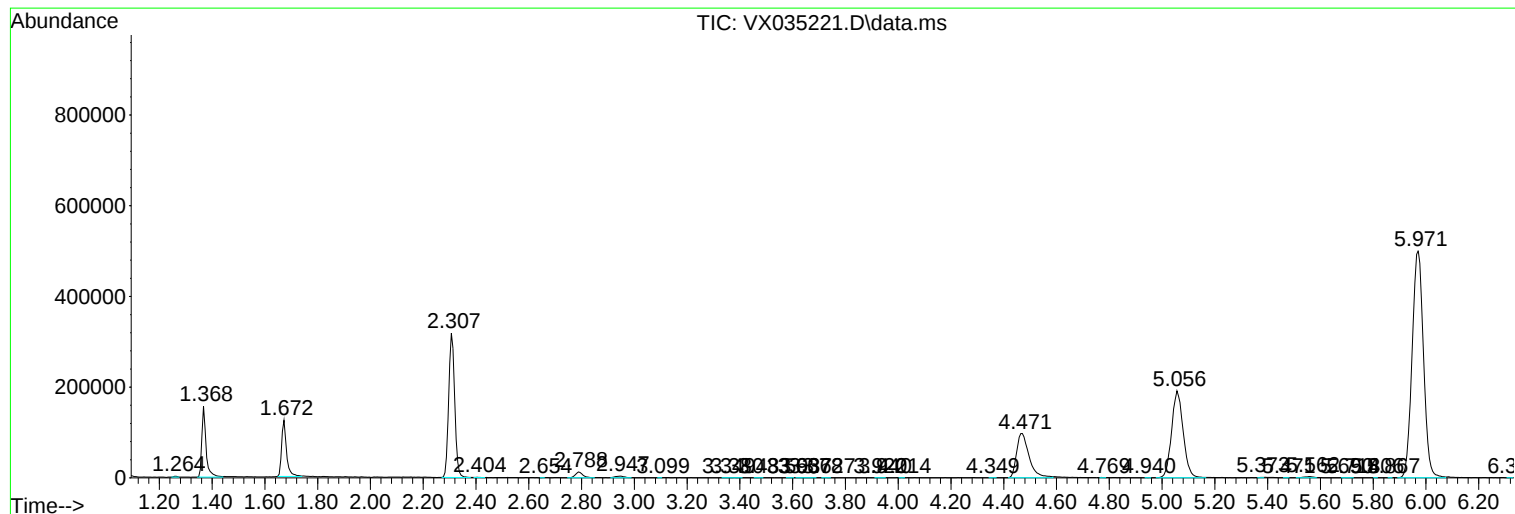

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035221.D
Acq On : 20 Apr 2023 17:22
Operator : JC/MD
Sample : 02378-10DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035221.D
Acq On : 20 Apr 2023 17:22
Operator : JC/MD
Sample : 02378-10DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0MK3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------