

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035222.D
 Acq On : 20 Apr 2023 17:45
 Operator : JC/MD
 Sample : 02378-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M

Title : VOC Analysis

Signal : TIC: VX035222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2061	2173	0.15%	0.020%
2	1.368	42	46	59	rBV	148458	164567	11.34%	1.520%
3	1.673	92	96	106	rBV	118100	152720	10.52%	1.411%
4	2.307	194	200	211	rBV	302001	467607	32.22%	4.319%
5	2.593	244	247	251	rBV2	304	447	0.03%	0.004%
6	2.654	255	257	258	rBV	236	204	0.01%	0.002%
7	2.788	274	279	285	rBV2	3422	5883	0.41%	0.054%
8	3.044	318	321	322	rBV2	300	274	0.02%	0.003%
9	3.123	332	334	335	rBV2	253	170	0.01%	0.002%
10	3.142	335	337	339	rBV	182	163	0.01%	0.002%
11	3.227	350	351	353	rVV2	216	151	0.01%	0.001%
12	3.252	353	355	356	rVB2	245	161	0.01%	0.001%
13	3.276	356	359	362	rBV2	270	263	0.02%	0.002%
14	3.447	385	387	391	rVV	215	221	0.02%	0.002%
15	3.520	397	399	400	rVB	378	246	0.02%	0.002%
16	3.544	400	403	404	rBV2	253	298	0.02%	0.003%
17	3.666	422	423	424	rBV	389	218	0.02%	0.002%
18	3.715	429	431	434	rVV2	186	226	0.02%	0.002%
19	3.751	435	437	438	rVV	233	129	0.01%	0.001%
20	3.800	443	445	446	rVV	230	188	0.01%	0.002%
21	3.843	450	452	454	rBV2	213	227	0.02%	0.002%
22	3.934	465	467	470	rVB2	174	167	0.01%	0.002%
23	3.977	473	474	477	rVV	210	191	0.01%	0.002%
24	4.190	507	509	511	rBV	278	275	0.02%	0.003%
25	4.337	531	533	535	rBV	174	163	0.01%	0.002%
26	4.373	537	539	542	rVB2	315	367	0.03%	0.003%
27	4.410	542	545	546	rBV	387	401	0.03%	0.004%
28	4.471	546	555	574	rBV	91443	309220	21.31%	2.856%
29	5.056	639	651	669	rBV	187414	564231	38.88%	5.211%
30	5.288	687	689	692	rVB	156	116	0.01%	0.001%
31	5.312	692	693	694	rBV	185	103	0.01%	0.001%
32	5.385	700	705	706	rBV	610	855	0.06%	0.008%
33	5.556	724	733	744	rBV5	2416	6089	0.42%	0.056%
34	5.727	759	761	762	rBV	231	167	0.01%	0.002%
35	5.971	789	801	820	rBV2	478839	1451242	100.00%	13.403%
36	6.397	869	871	873	rVV2	363	305	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035222.D
 Acq On : 20 Apr 2023 17:45
 Operator : JC/MD
 Sample : 02378-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.440	877	878	879	rVB	365	133	0.01%	0.001%
38	6.684	915	918	919	rVB	435	260	0.02%	0.002%
39	6.696	919	920	921	rBV	332	224	0.02%	0.002%
40	6.763	921	931	946	rVV	396223	941207	64.86%	8.693%
41	6.958	961	963	966	rBV3	330	389	0.03%	0.004%
42	7.117	982	989	1000	rVB3	4101	10416	0.72%	0.096%
43	7.306	1011	1020	1039	rBV	299044	665650	45.87%	6.148%
44	7.598	1067	1068	1069	rBV	168	100	0.01%	0.001%
45	7.678	1079	1081	1082	rBV	218	158	0.01%	0.001%
46	7.720	1087	1088	1089	rBV	191	127	0.01%	0.001%
47	7.769	1093	1096	1098	rVB2	193	189	0.01%	0.002%
48	7.812	1101	1103	1105	rBV2	262	343	0.02%	0.003%
49	7.946	1120	1125	1133	rBV3	1232	2460	0.17%	0.023%
50	8.037	1139	1140	1142	rBV	233	121	0.01%	0.001%
51	8.086	1146	1148	1149	rBV	176	102	0.01%	0.001%
52	8.159	1157	1160	1161	rBV2	188	182	0.01%	0.002%
53	8.214	1166	1169	1170	rBV2	284	228	0.02%	0.002%
54	8.324	1181	1187	1203	rVV	171256	287436	19.81%	2.655%
55	8.494	1213	1215	1220	rBV3	598	811	0.06%	0.007%
56	8.647	1234	1240	1259	rBV	744273	1158530	79.83%	10.700%
57	8.952	1284	1290	1305	rBV	120039	182585	12.58%	1.686%
58	9.220	1333	1334	1335	rVB	399	146	0.01%	0.001%
59	9.281	1341	1344	1347	rVB	695	829	0.06%	0.008%
60	9.311	1347	1349	1351	rBV	419	395	0.03%	0.004%
61	9.385	1356	1361	1373	rBV	464103	658704	45.39%	6.084%
62	9.872	1439	1441	1444	rBV2	432	428	0.03%	0.004%
63	10.055	1465	1471	1484	rBV	750934	1071358	73.82%	9.895%
64	10.305	1509	1512	1515	rBV4	516	570	0.04%	0.005%
65	10.330	1515	1516	1518	rBV	214	143	0.01%	0.001%
66	10.604	1559	1561	1563	rBV2	167	148	0.01%	0.001%
67	10.634	1565	1566	1567	rBV	395	186	0.01%	0.002%
68	10.653	1567	1569	1570	rVV2	281	176	0.01%	0.002%
69	10.896	1608	1609	1612	rVB2	280	274	0.02%	0.003%
70	10.964	1617	1620	1624	rVV3	351	469	0.03%	0.004%
71	11.049	1632	1634	1635	rVB2	225	131	0.01%	0.001%
72	11.085	1638	1640	1644	rVV3	269	386	0.03%	0.004%
73	11.153	1649	1651	1652	rVV2	220	116	0.01%	0.001%
74	11.189	1652	1657	1671	rVV	525414	678618	46.76%	6.268%
75	11.317	1676	1678	1680	rVB	514	410	0.03%	0.004%
76	11.421	1694	1695	1698	rBV	309	265	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
 Data File : VX035222.D
 Acq On : 20 Apr 2023 17:45
 Operator : JC/MD
 Sample : 02378-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	11.451	1698	1700	1702	rVV2	371	355	0.02%	0.003%
78	11.549	1714	1716	1717	rBV	254	109	0.01%	0.001%
79	11.701	1739	1741	1747	rVB	497	639	0.04%	0.006%
80	11.756	1748	1750	1753	rBV3	352	334	0.02%	0.003%
81	11.969	1783	1785	1788	rBV	1749	2092	0.14%	0.019%
82	12.024	1788	1794	1805	rVV	762692	1001230	68.99%	9.247%
83	12.317	1837	1842	1858	rBV	772322	1011786	69.72%	9.345%
84	12.707	1905	1906	1907	rBV	387	187	0.01%	0.002%
85	12.762	1912	1915	1918	rBV3	1098	1236	0.09%	0.011%
86	13.183	1983	1984	1987	rBV	179	185	0.01%	0.002%
87	13.231	1991	1992	1995	rBV2	232	238	0.02%	0.002%
88	13.274	1997	1999	2000	rBV	224	137	0.01%	0.001%
89	13.329	2007	2008	2010	rBV	279	181	0.01%	0.002%
90	13.396	2017	2019	2021	rBV2	321	248	0.02%	0.002%
91	13.506	2035	2037	2040	rVB3	340	406	0.03%	0.004%
92	13.548	2040	2044	2047	rBV	249	397	0.03%	0.004%
93	13.591	2047	2051	2058	rBV3	5417	7553	0.52%	0.070%
94	13.786	2078	2083	2084	rBV3	401	534	0.04%	0.005%
95	13.908	2101	2103	2104	rBV3	367	252	0.02%	0.002%
96	13.969	2110	2113	2117	rVB2	1033	1230	0.08%	0.011%
97	14.091	2131	2133	2135	rBV2	251	213	0.01%	0.002%
98	14.128	2135	2139	2143	rVV3	931	1437	0.10%	0.013%
99	14.298	2166	2167	2170	rBV2	288	311	0.02%	0.003%
100	14.914	2266	2268	2269	rBV2	422	232	0.02%	0.002%


Sum of corrected areas: 10827353

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035222.D
Acq On : 20 Apr 2023 17:45
Operator : JC/MD
Sample : 02378-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

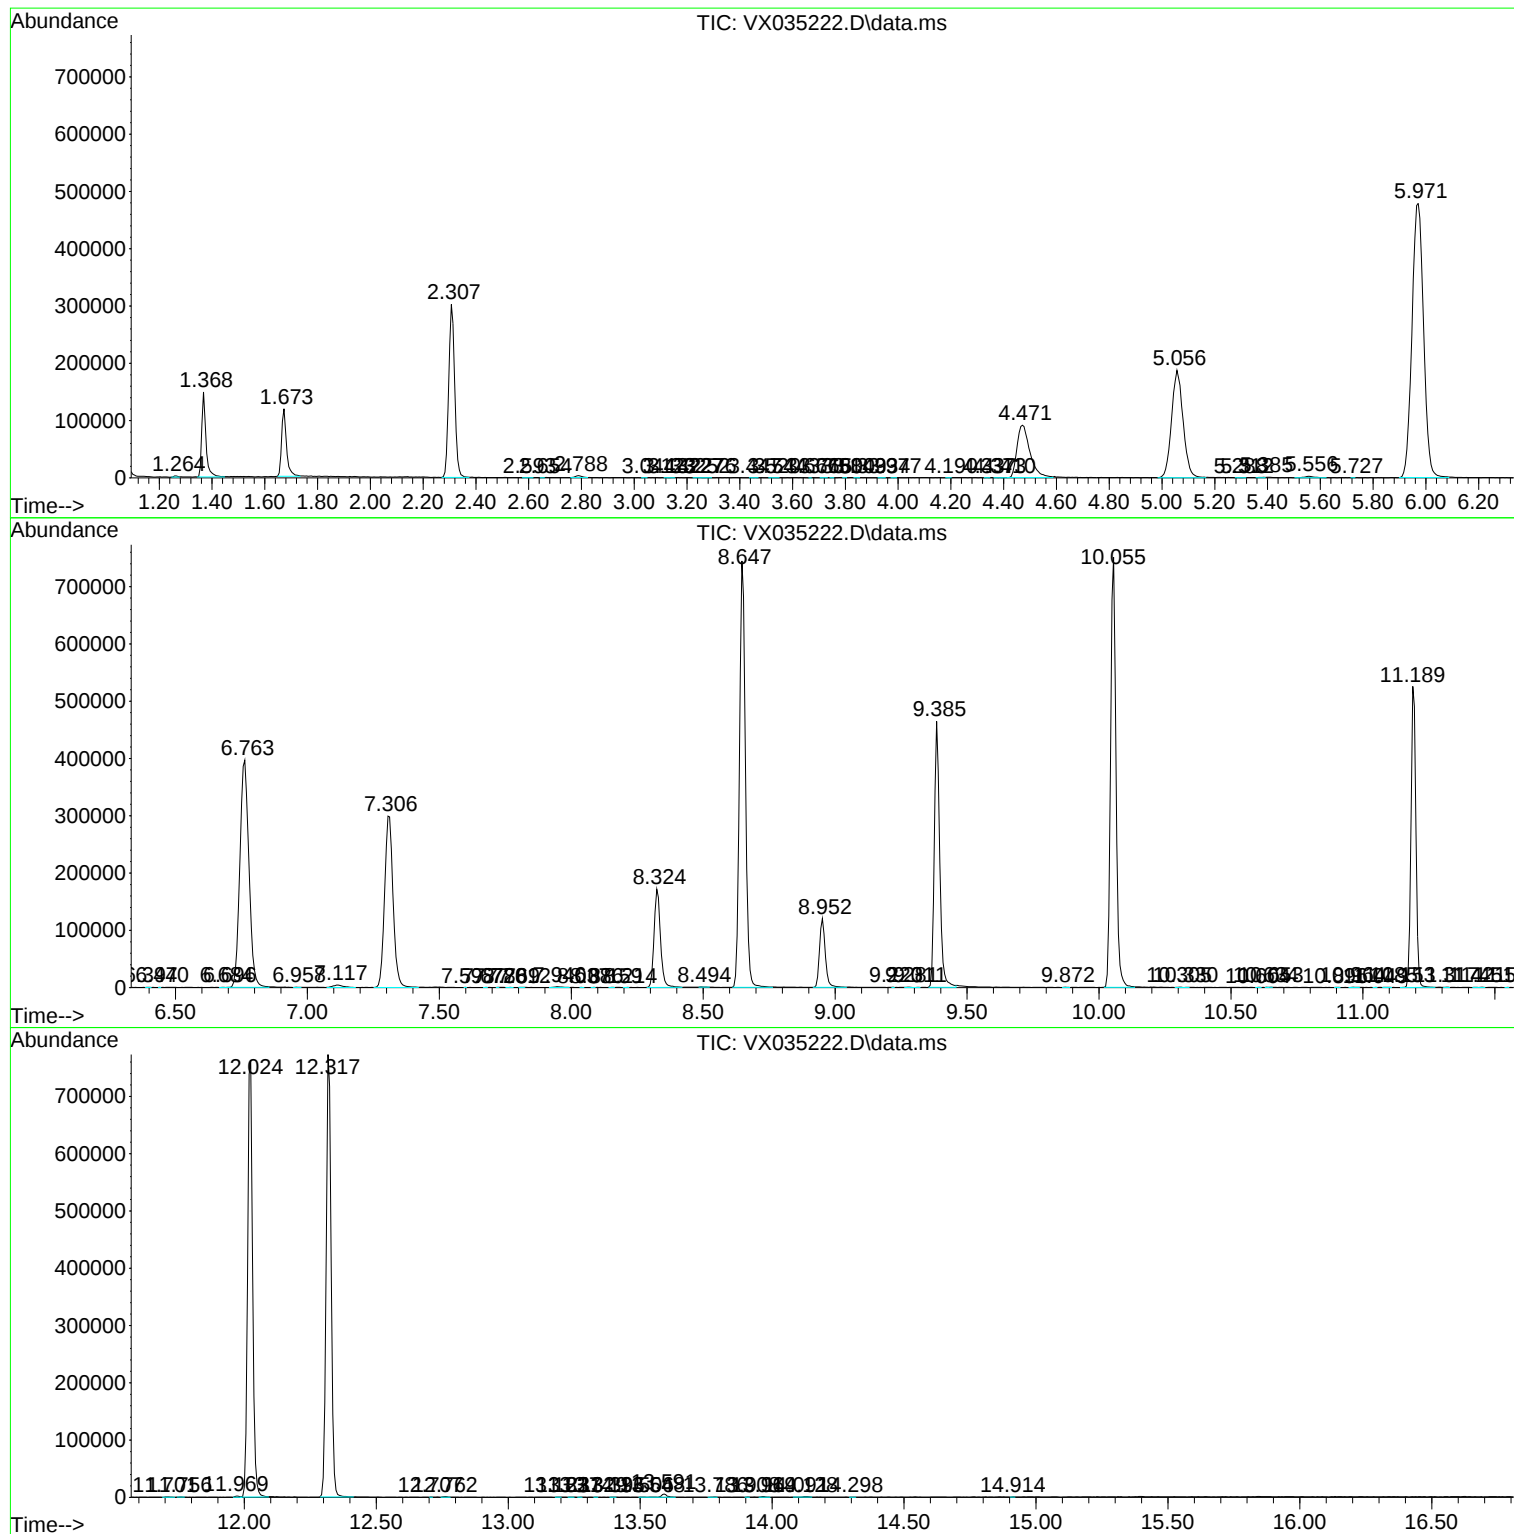

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035222.D
Acq On : 20 Apr 2023 17:45
Operator : JC/MD
Sample : 02378-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035222.D
Acq On : 20 Apr 2023 17:45
Operator : JC/MD
Sample : 02378-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc