
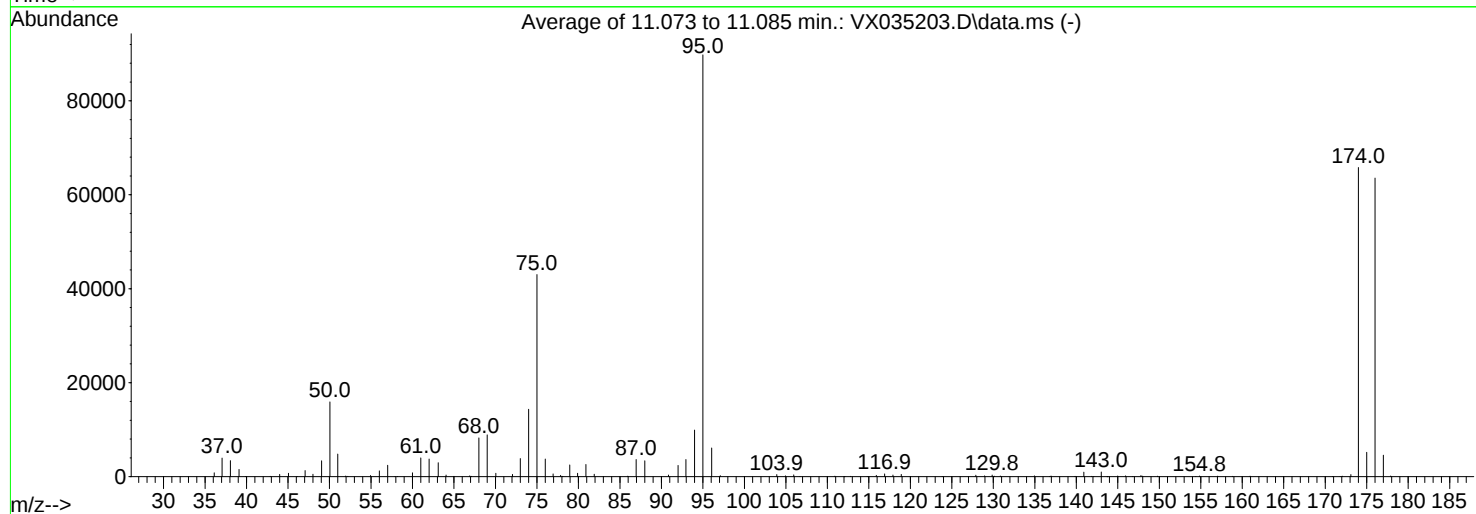


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042023\
Data File : VX035203.D
Acq On : 20 Apr 2023 09:07
Operator : JC/MD
Sample : BFB625
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB625

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
Title : VOC Analysis
Last Update : Tue Apr 25 03:03:54 2023

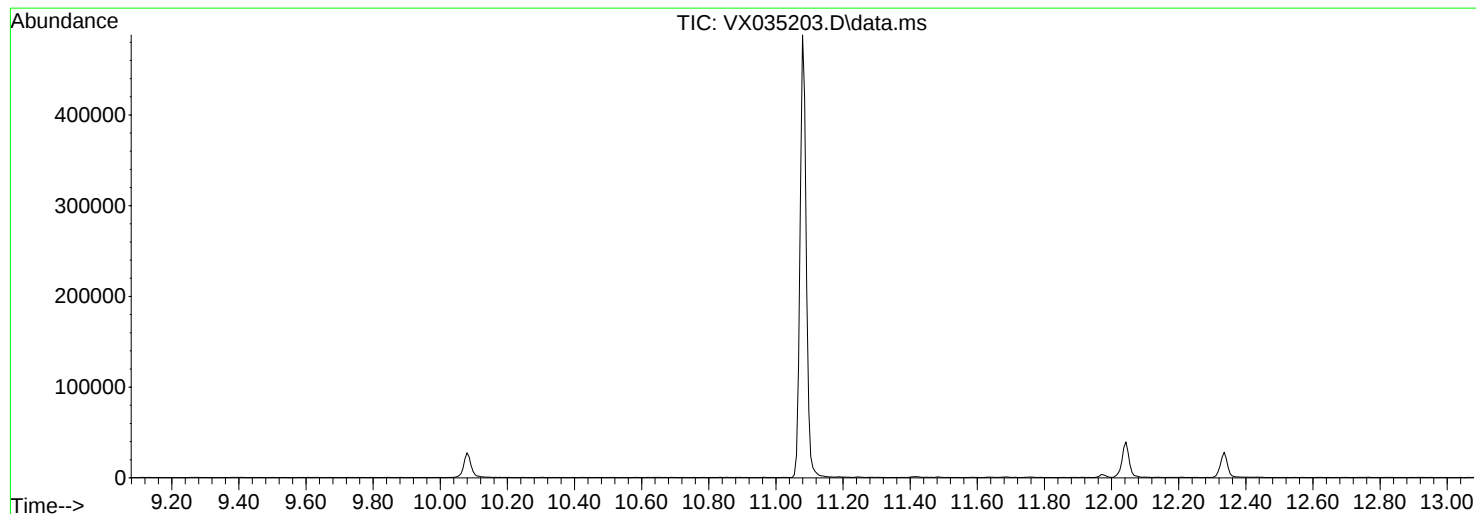

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	15911	PASS
75	95	30	80	47.9	43003	PASS
95	95	100	100	100.0	89784	PASS
96	95	5	9	6.8	6093	PASS
173	174	0.00	2	0.7	429	PASS
174	95	50	120	73.3	65800	PASS
175	174	5	9	7.9	5174	PASS
176	174	95	101	96.6	63544	PASS
177	176	5	9	7.2	4576	PASS

m/z	Abundance
40.00	223.0
43.40	53.0
44.00	174.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625

m/z	Abundance
36.10	672.0
37.10	3819.0
38.10	3289.0
39.10	1435.0
39.90	158.0
42.80	113.0
44.00	547.0
45.10	751.0
47.10	1084.0
48.00	361.0
49.00	3026.0
50.10	14152.0
51.00	4315.0
51.90	193.0
55.00	112.0
56.00	1155.0
57.00	2191.0
57.90	69.0
60.00	828.0
61.00	3209.0
62.00	3364.0
63.10	2905.0
64.00	391.0
65.00	54.0
66.90	232.0
68.00	7492.0
69.00	8028.0
70.00	592.0
72.00	406.0
73.00	3189.0
74.00	11976.0
75.00	36424.0
76.00	3388.0
77.00	453.0
77.80	370.0
78.90	1925.0
79.90	711.0
80.90	2075.0
81.90	498.0
85.80	58.0
87.00	3623.0
88.00	2839.0
91.00	341.0
92.00	1886.0
92.90	3084.0
94.00	7940.0
95.00	74160.0
96.00	4979.0
97.10	189.0
103.90	394.0
105.00	104.0
106.00	398.0
106.70	64.0
111.00	93.0
112.80	84.0
116.00	257.0
116.90	445.0
118.00	218.0
118.90	324.0
123.80	52.0
128.00	208.0
128.90	78.0
129.80	270.0
130.90	75.0
135.10	121.0
136.80	149.0
140.90	563.0
142.10	61.0
143.00	797.0
145.00	73.0
145.90	141.0
147.80	160.0
154.40	97.0
155.00	84.0
157.10	93.0
161.00	61.0
172.00	126.0
173.10	489.0
174.00	45808.0
175.00	3692.0
176.00	43552.0
177.00	3502.0
177.90	92.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625

m/z	Abundance
36.10	961.0
37.10	4589.0
38.00	3891.0
39.10	1760.0
40.10	158.0
42.90	105.0
44.00	816.0
45.00	822.0
46.10	83.0
47.10	1705.0
48.00	726.0
49.10	4093.0
50.00	18960.0
51.00	5893.0
52.00	268.0
54.90	269.0
56.00	1446.0
57.00	2818.0
58.20	127.0
60.00	875.0
61.00	5085.0
62.00	4455.0
63.10	3435.0
64.00	305.0
65.00	107.0
66.90	237.0
68.00	9763.0
69.00	10168.0
70.00	836.0
72.00	543.0
73.00	4524.0
74.00	17704.0
75.00	52600.0
76.00	4169.0
77.00	815.0
77.90	488.0
79.00	2967.0
79.90	785.0
80.90	3248.0
81.90	576.0
83.00	63.0
85.90	203.0
86.90	4081.0
88.00	3926.0
90.80	368.0
92.00	2642.0
93.00	4068.0
94.00	12069.0
95.00	107080.0
96.10	7346.0
97.10	317.0
103.80	552.0
105.00	243.0
105.90	466.0
106.70	86.0
110.90	150.0
112.00	54.0
112.80	90.0
114.80	80.0
115.80	281.0
116.90	684.0
117.80	448.0
119.00	576.0
123.90	57.0
127.80	256.0
128.90	251.0
129.90	394.0
130.70	113.0
131.00	114.0
134.90	244.0
137.00	153.0
139.80	104.0
140.90	1099.0
141.80	155.0
143.00	1082.0
145.00	171.0
146.00	221.0
147.80	285.0
148.00	285.0
149.80	137.0
154.80	156.0
157.00	145.0
158.80	105.0
161.00	188.0
172.10	188.0
174.00	76984.0
175.00	5810.0
176.00	74688.0
177.00	5387.0
177.90	250.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625

m/z	Abundance
36.10	802.0
37.00	3475.0
38.00	3087.0
39.10	1417.0
40.00	187.0
44.10	638.0
45.00	568.0
46.10	80.0
47.00	1078.0
48.00	471.0
49.10	2974.0
50.10	14621.0
51.00	4259.0
52.20	181.0
54.90	297.0
56.00	1128.0
57.00	2234.0
60.00	714.0
61.00	3666.0
62.00	3483.0
63.10	2585.0
64.10	376.0
65.00	58.0
67.10	251.0
68.00	7521.0
69.00	8474.0
70.10	726.0
72.10	492.0
73.00	3878.0
74.00	13369.0
75.00	39984.0
76.00	3649.0
76.90	447.0
78.10	251.0
78.90	2626.0
79.90	639.0
80.90	2491.0
81.90	467.0
86.00	109.0
87.00	3271.0
88.00	3357.0
90.80	323.0
92.00	2599.0
93.00	3801.0
94.00	9762.0
95.00	88112.0
96.00	5953.0
97.00	114.0
104.00	396.0
104.80	142.0
105.90	279.0
110.80	64.0
112.70	52.0
115.00	78.0
115.90	305.0
116.90	602.0
118.00	408.0
118.80	541.0
127.90	450.0
129.00	211.0
129.80	319.0
130.10	353.0
130.80	158.0
135.00	147.0
136.90	235.0
139.90	78.0
140.90	1164.0
141.90	86.0
143.00	1051.0
143.70	54.0
145.00	127.0
146.00	115.0
146.80	116.0
147.80	258.0
149.80	127.0
154.80	168.0
157.10	94.0
158.90	131.0
160.90	114.0
170.90	78.0
171.80	149.0
173.10	799.0
174.00	74608.0
175.00	6019.0
176.00	72392.0
177.00	4839.0
177.90	120.0

Instrument :
MSVOA_X
ClientSampleId :
BFB625