

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX042120\
 Data File : VX015820.D
 Acq On : 22 Apr 2020 02:05
 Operator : JC/SP
 Sample : L2351-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-17A

Quant Time: Apr 22 04:26:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 27 09:35:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	954853	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	1462662	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	1430355	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	813125	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.04	65	529408	39.31	ug/l	0.00
Spiked Amount			Recovery	=	78.62%	
35) Dibromofluoromethane	5.47	113	431772	46.18	ug/l	0.00
Spiked Amount			Recovery	=	92.36%	
50) Toluene-d8	8.70	98	1747953	50.78	ug/l	0.00
Spiked Amount			Recovery	=	101.56%	
62) 4-Bromofluorobenzene	11.12	95	753436	53.86	ug/l	0.00
Spiked Amount			Recovery	=	107.72%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.62	94	299	Below Cal		85
11) Tert butyl alcohol	3.00	59	1994	0.619	ug/l #	30
12) 1,1-Dichloroethene	2.37	96	1922	0.213	ug/l #	7
13) Acrolein	2.27	56	1775	0.967	ug/l	89
16) Acetone	2.42	43	228390	39.474	ug/l	97
17) Carbon Disulfide	2.55	76	29326	1.066	ug/l	100
18) Methyl Acetate	2.75	43	14305	0.969	ug/l	95
20) Methylene Chloride	2.84	84	46348	4.289	ug/l	93
25) 2-Butanone	4.65	43	26662	2.865	ug/l	94
29) Tetrahydrofuran	5.10	42	3347	0.560	ug/l #	61
36) 1,1-Dichloropropene	5.64	75	62434	4.633	ug/l #	52
38) Carbon Tetrachloride	5.64	117	83470	5.718	ug/l #	14
40) Benzene	6.12	78	8487	0.215	ug/l #	73
43) Isopropyl Acetate	6.42	43	319864	10.798	ug/l	98
48) Methyl methacrylate	7.65	41	21375	1.445	ug/l #	19
49) 1,4-Dioxane	7.71	88	1254	4.543	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	310537	18.498	ug/l #	48
54) cis-1,3-Dichloropropene	8.59	75	128973	7.152	ug/l #	48
56) Ethyl methacrylate	9.29	69	3621	0.206	ug/l #	1
57) 1,3-Dichloropropane	9.53	76	22365	1.245	ug/l #	42
59) 2-Hexanone	9.53	43	311560	24.582	ug/l #	53
74) N-amyl acetate	10.81	43	26852	0.906	ug/l #	53
76) 1,2,3-Trichloropropane	11.12	75	363064	21.713	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.12	75	363064	52.099	ug/l #	10
95) Naphthalene	13.82	128	20788	0.346	ug/l #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042120\
Data File : VX015820.D
Acq On : 22 Apr 2020 02:05
Operator : JC/SP
Sample : L2351-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-17A

Quant Time: Apr 22 04:26:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 27 09:35:51 2020
Response via : Initial Calibration

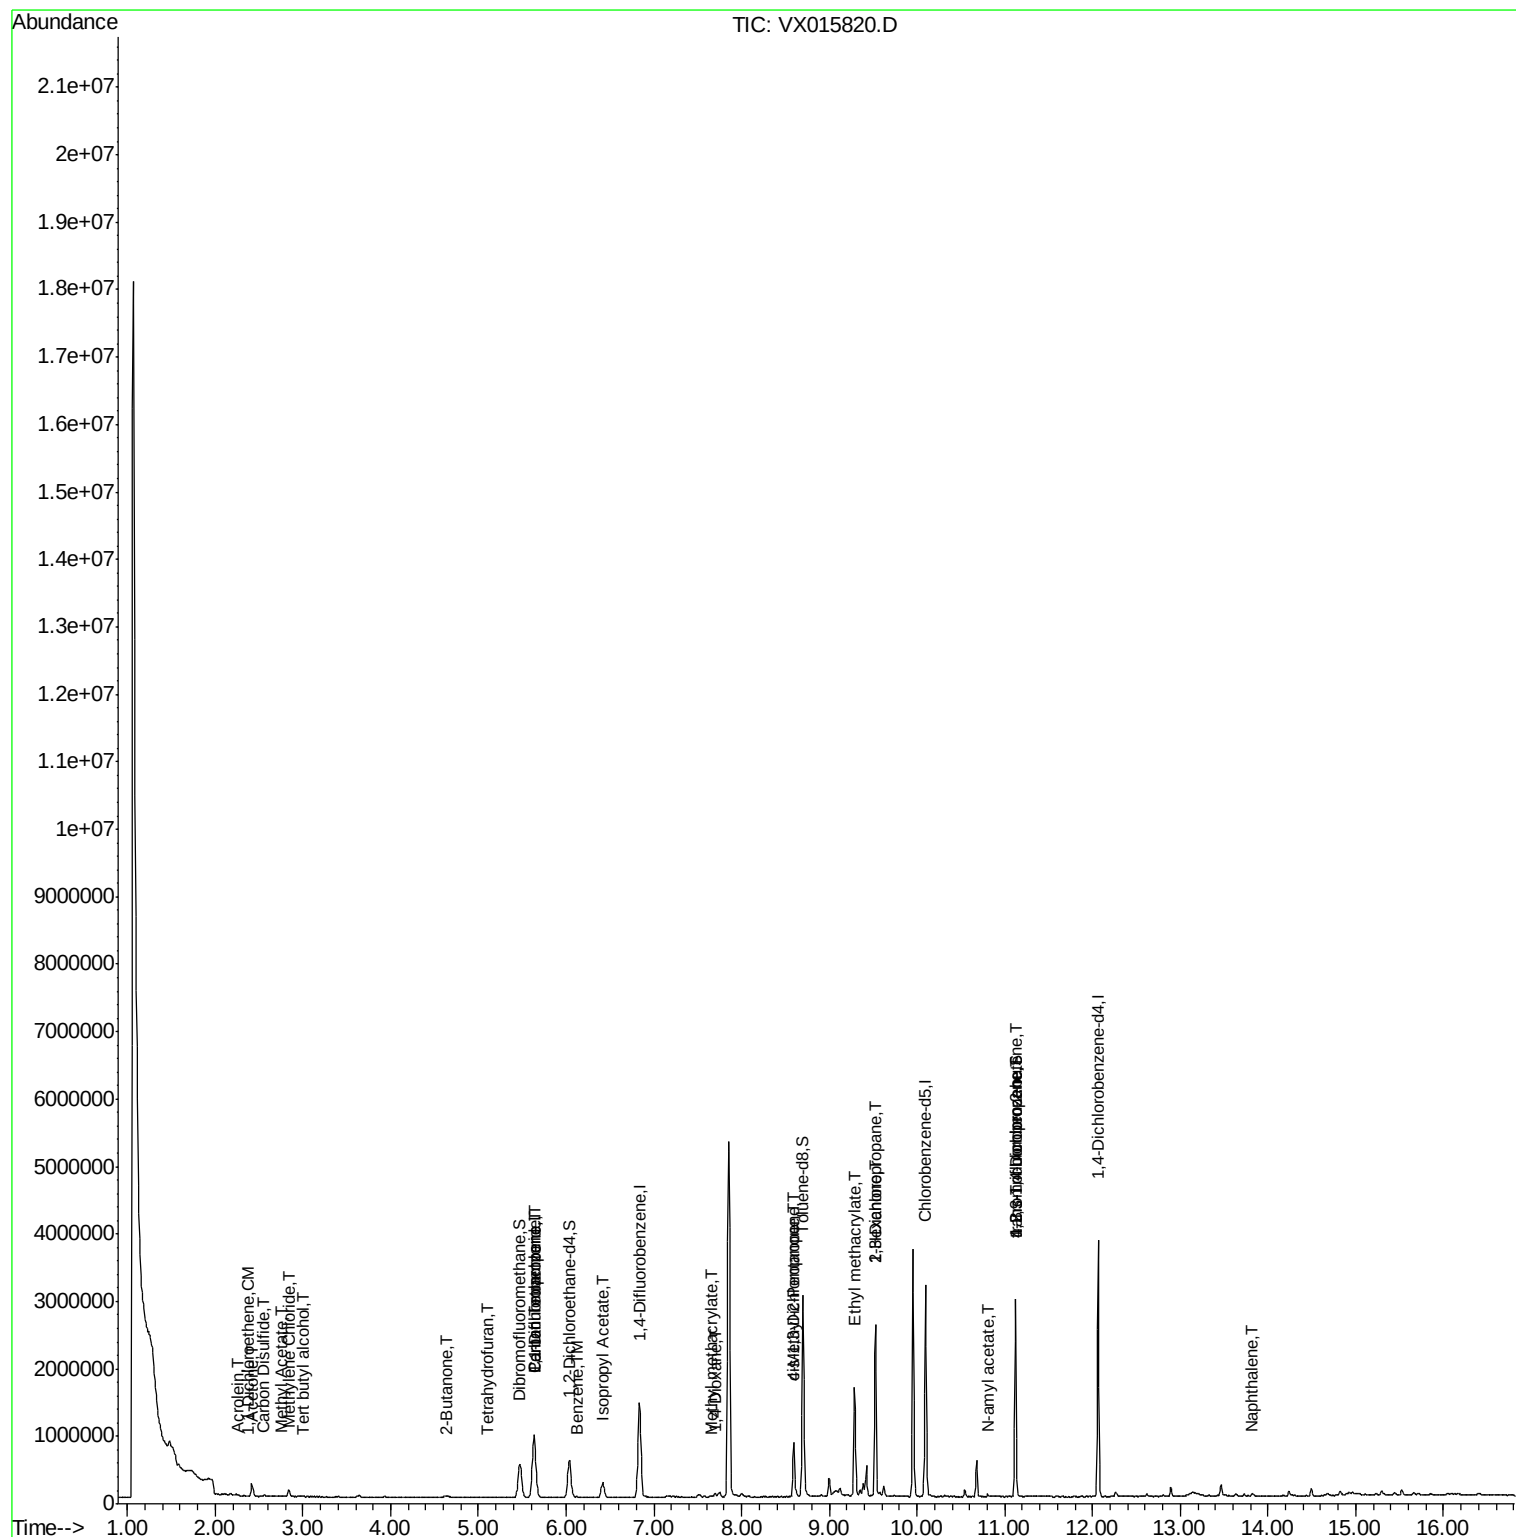



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 779

Delta R.T. 0.01 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :


TP-17A

Tot Ion:168 Resp: 954853

Ion Ratio Lower Upper

168 100

99 52.5 46.4 69.6

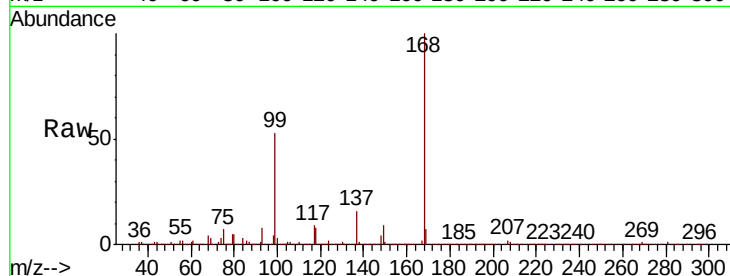

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64



300000

200000

100000

0

Time-->

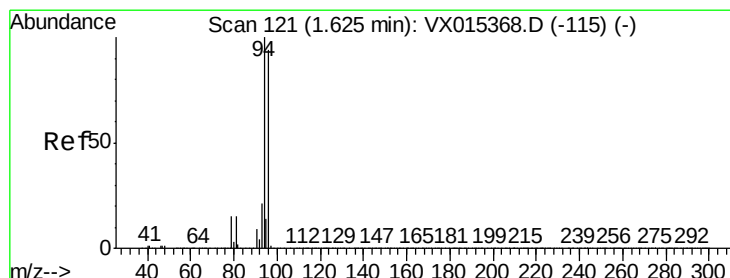

#5

Bromomethane

Concen: Below Cal

RT: 1.62 min Scan# 121

Delta R.T. 0.00 min

Lab File: VX015820.D


Acq: 22 Apr 2020 02:05

Tgt Ion: 94 Resp: 299

Ion Ratio Lower Upper

94 100

96 107.5 74.8 112.2

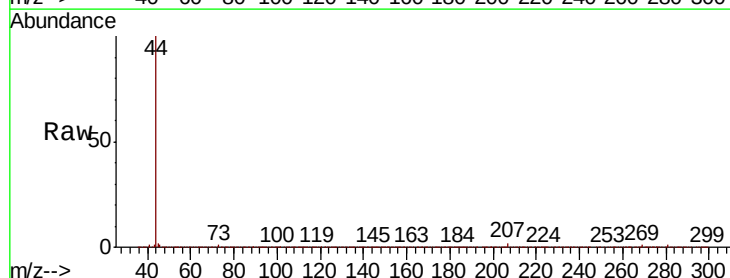

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0


1500


1000

500

0

Time-->







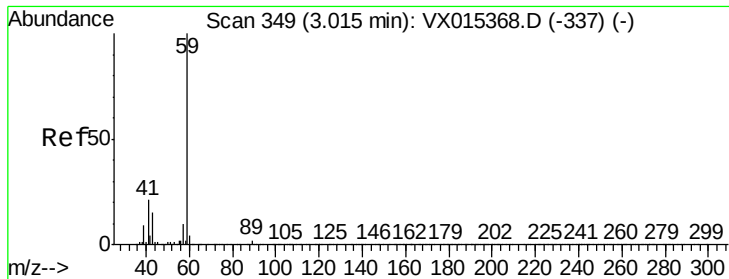

#11
Tert butyl alcohol
Concen: 0.619 ug/l
RT: 3.00 min Scan# 347
Delta R.T. -0.01 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05




Instrument :
MSVOA_X
ClientSampled :
TP-17A


Tot Ion: 59 Resp: 1994
Ion Ratio Lower Upper
59 100
57 36.0 8.1 12.1#

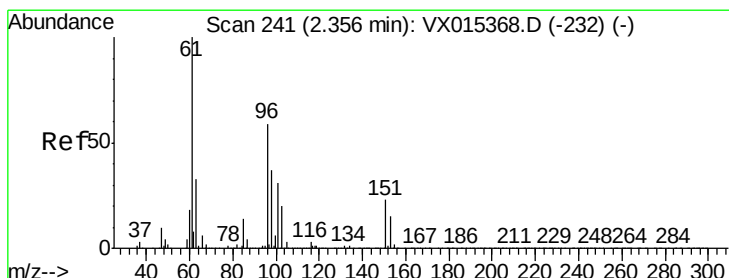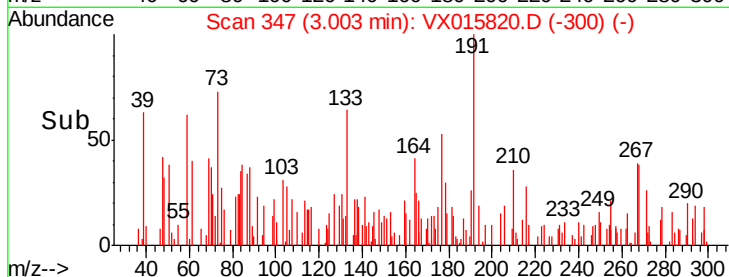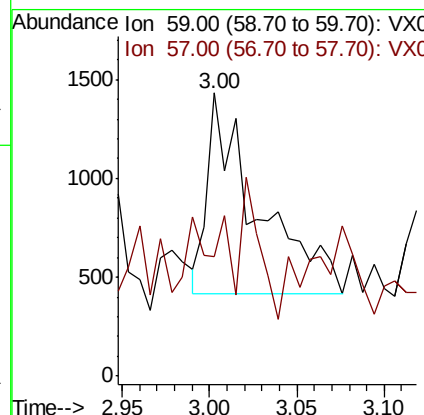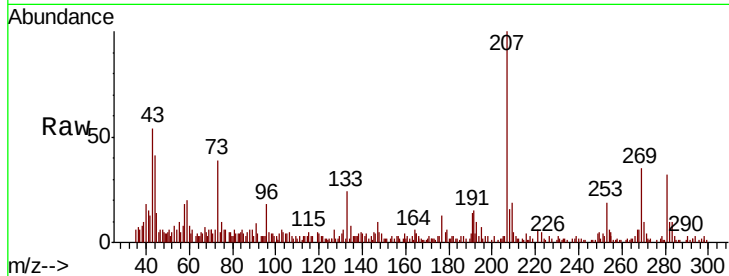

#12
1,1-Dichloroethene
Concen: 0.213 ug/l
RT: 2.37 min Scan# 244
Delta R.T. 0.02 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Tgt Ion: 96 Resp: 1922
Ion Ratio Lower Upper
96 100
61 21.6 135.7 203.5#
98 22.4 50.6 75.8#


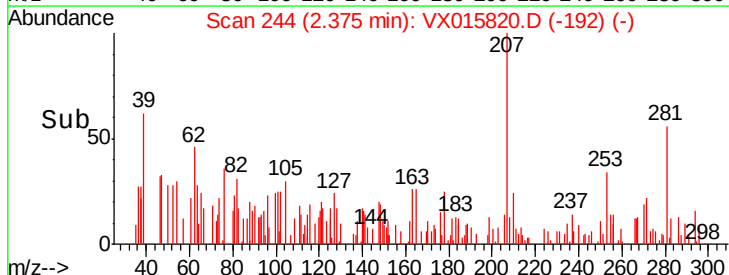
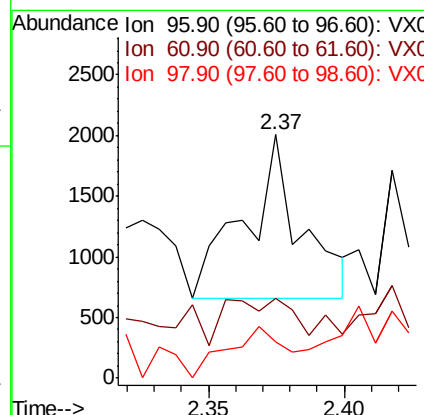
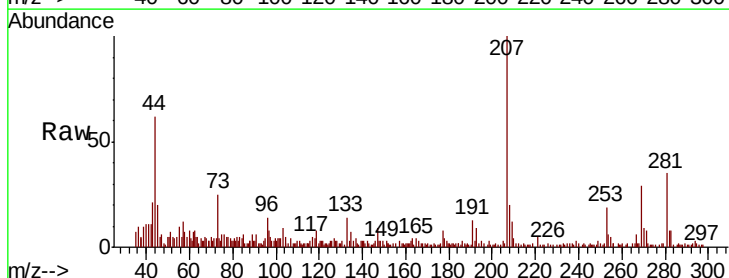


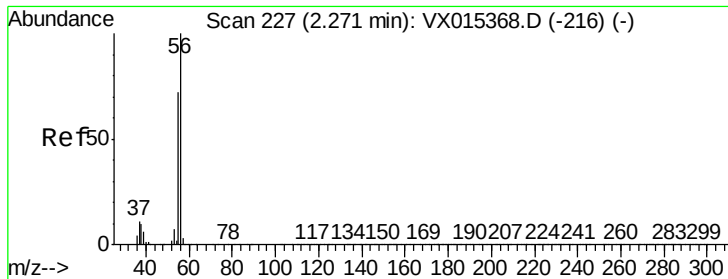

#13
Acrolein
Concen: 0.967 ug/l
RT: 2.27 min Scan# 227
Delta R.T. 0.00 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05




Instrument :
MSVOA_X
ClientSampled :
TP-17A


Tot Ion: 56 Resp: 1775
Ion Ratio Lower Upper
56 100
55 80.2 57.0 85.4

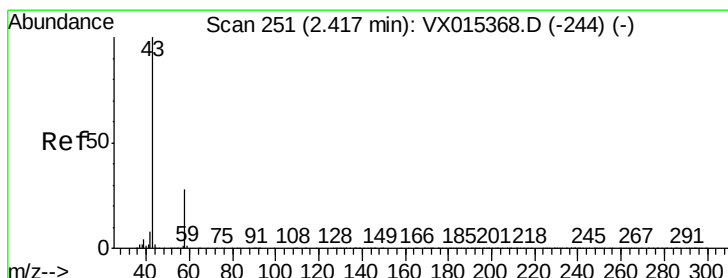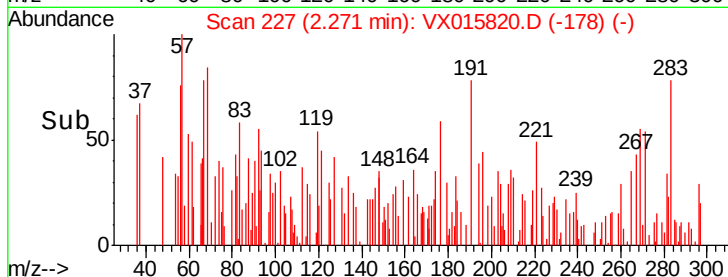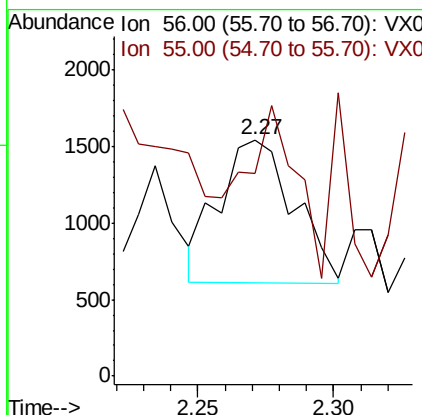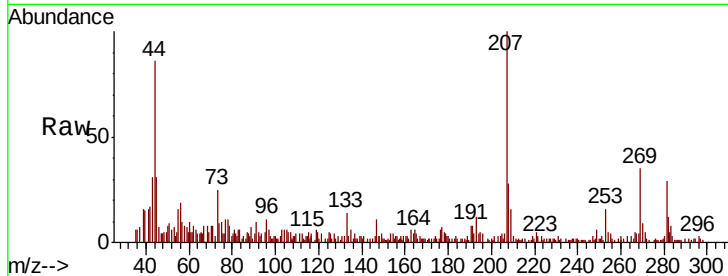

#16
Acetone
Concen: 39.474 ug/l
RT: 2.42 min Scan# 251
Delta R.T. 0.00 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Tgt Ion: 43 Resp: 228390
Ion Ratio Lower Upper
43 100
58 29.2 22.1 33.1


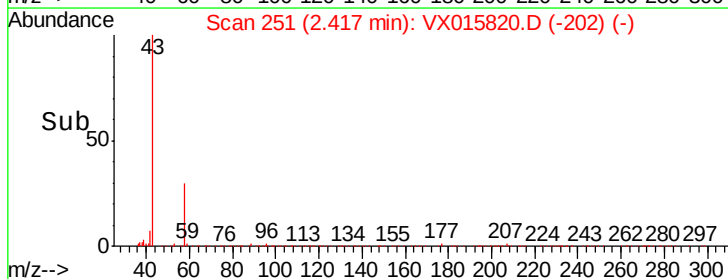
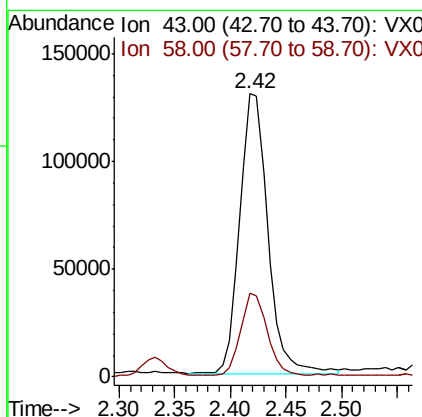
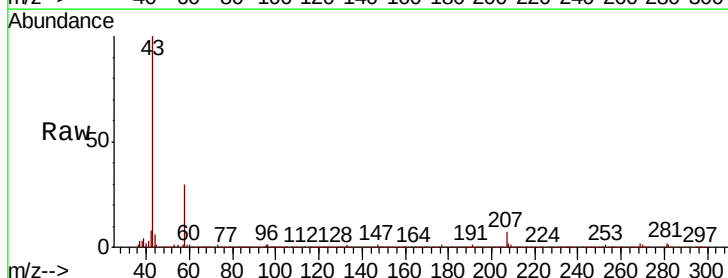




#17
Carbon Disulfide
Concen: 1.066 ug/l
RT: 2.55 min Scan# 273
Delta R.T. 0.00 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05




Instrument :
MSVOA_X
ClientSampleId :
TP-17A


Tot Ion: 76 Resp: 29326
Ion Ratio Lower Upper
76 100
78 8.8 7.1 10.7

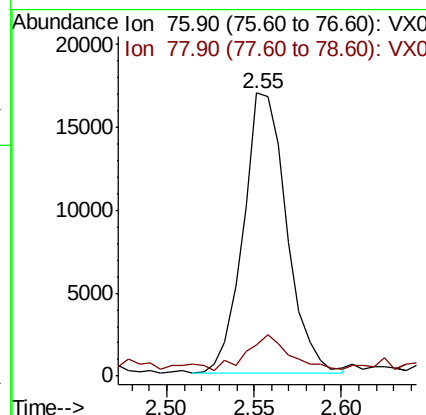

#18
Methyl Acetate
Concen: 0.969 ug/l
RT: 2.75 min Scan# 305
Delta R.T. -0.01 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Tgt Ion: 43 Resp: 14305
Ion Ratio Lower Upper
43 100
74 18.2 16.5 24.7


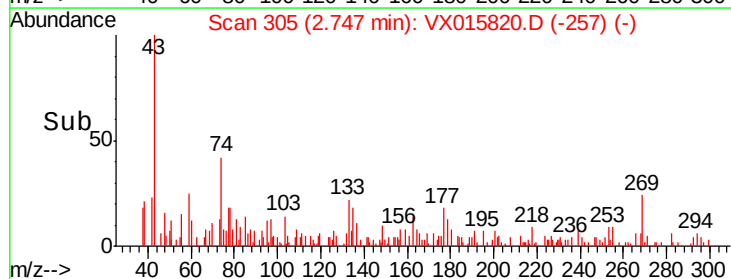
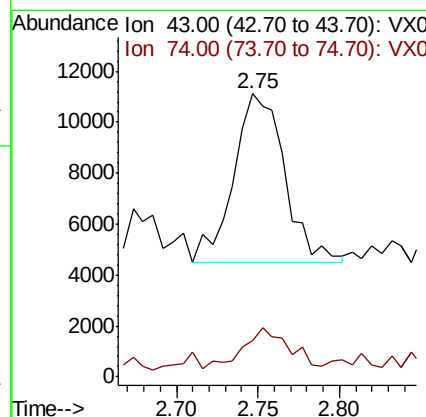



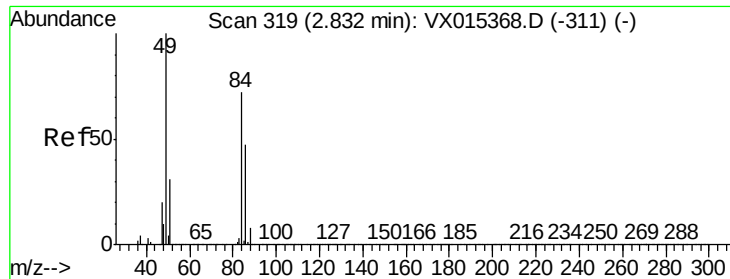

#20
Methvlene Chloride
Concen: 4.289 ug/l
RT: 2.84 min Scan# 320
Delta R.T. 0.01 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05




Instrument :
MSVOA_X
ClientSampleId :
TP-17A


Tot Ion:	84	Resp:	46348
Ion	Ratio	Lower	Upper
84	100		
49	131.1	111.3	166.9
51	44.1	34.0	51.0
86	55.7	52.5	78.7

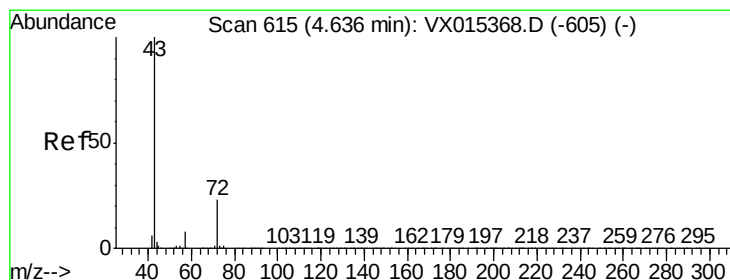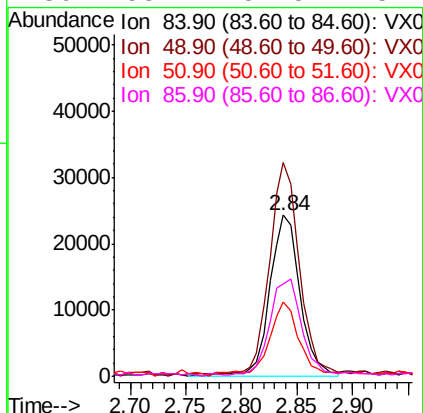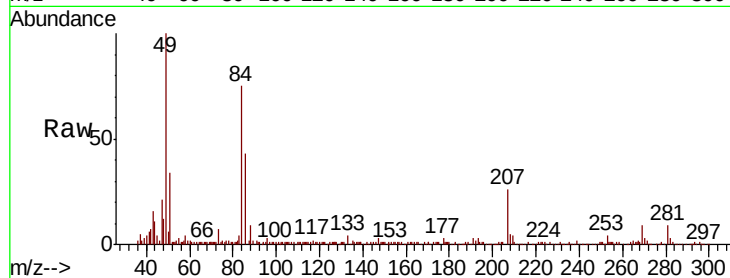

#25
2-Butanone
Concen: 2.865 ug/l
RT: 4.65 min Scan# 617
Delta R.T. 0.01 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Tgt Ion:	43	Resp:	26662
Ion	Ratio	Lower	Upper
43	100		
72	26.5	19.0	28.4

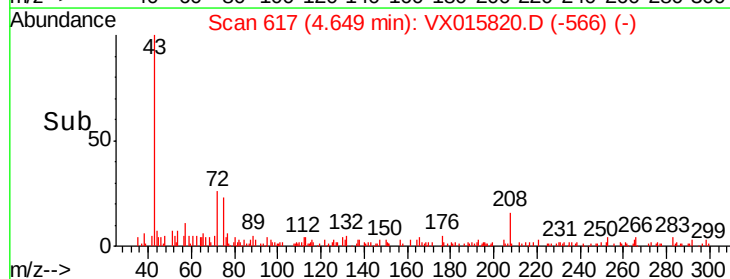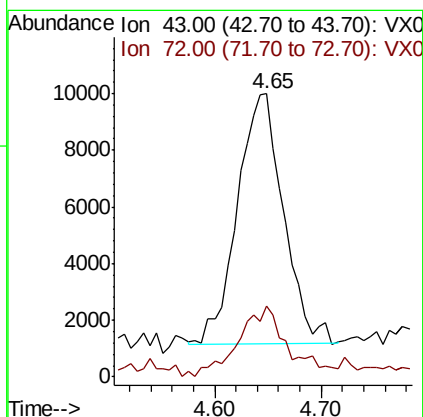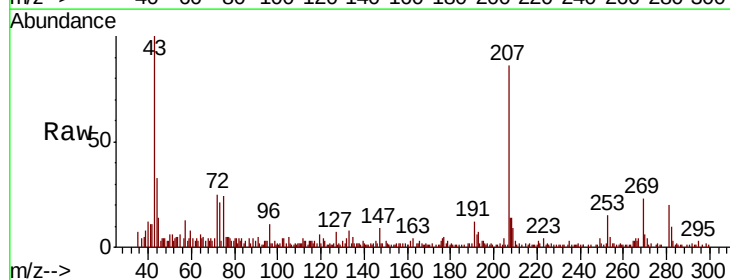

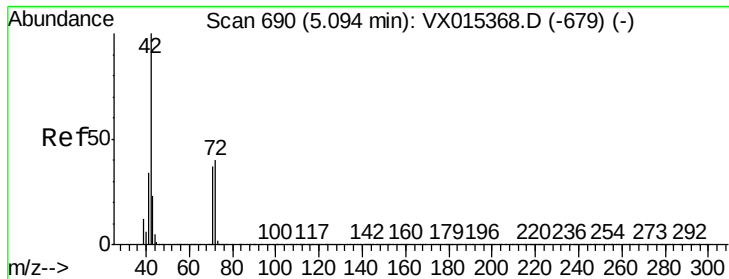

#29

Tetrahydrofuran

Concen: 0.560 ug/l

RT: 5.10 min Scan# 691

Delta R.T. 0.01 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :

TP-17A


Tot Ion: 42 Resp: 3347

Ion Ratio Lower Upper

42 100

72 85.2 31.7 47.5#




71 36.4 29.6 44.4

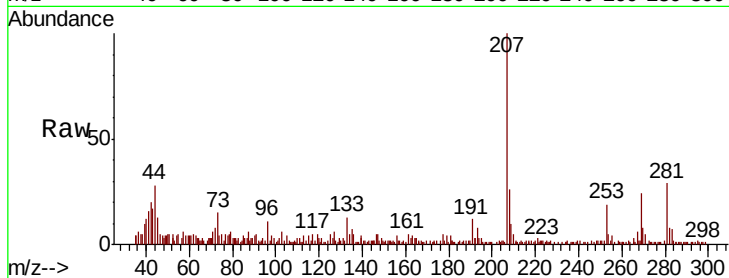

Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

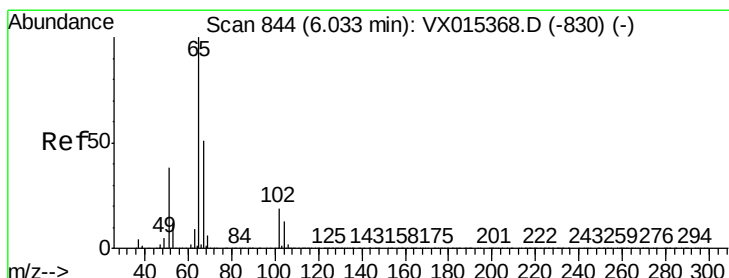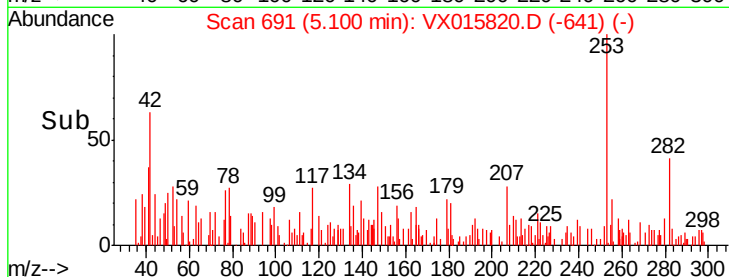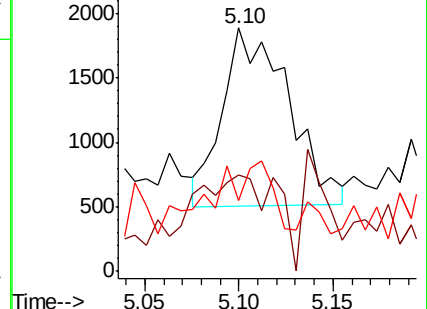

#33

1,2-Dichloroethane-d4

Concen: 39.311 ug/l

RT: 6.04 min Scan# 845

Delta R.T. 0.01 min

Lab File: VX015820.D


Acq: 22 Apr 2020 02:05

Tgt Ion: 65 Resp: 529408

Ion Ratio Lower Upper



65 100


67 51.7 0.0 102.6

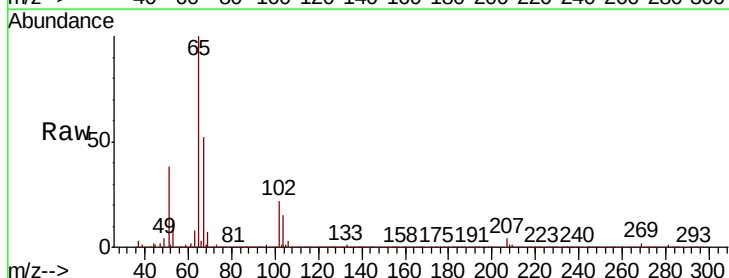

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

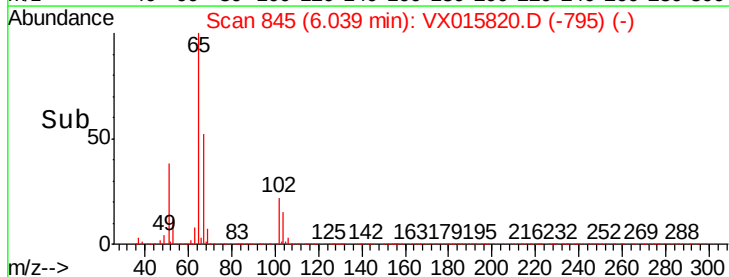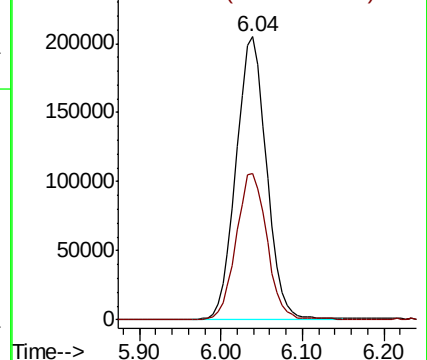



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 976

Delta R.T. 0.00 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :

TP-17A


Tot Ion:114 Resp: 1462662

Ion Ratio Lower Upper

114 100

63 21.2 0.0 44.2




88 15.8 0.0 33.8

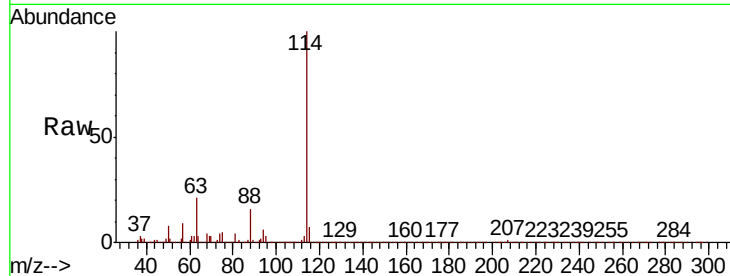

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

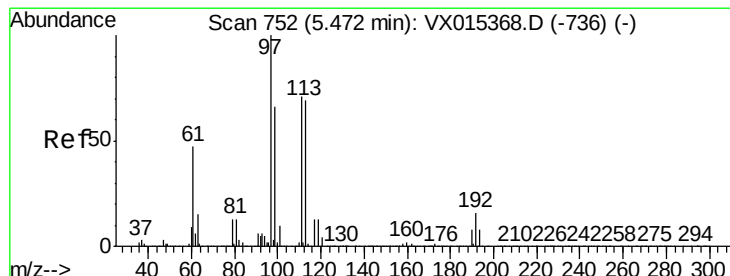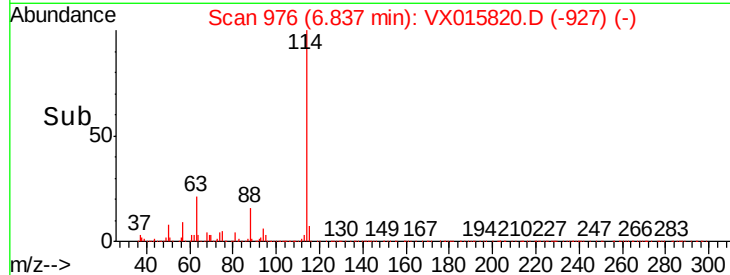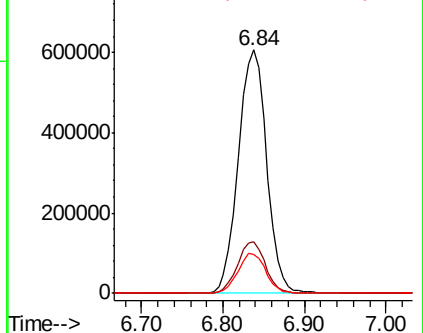

#35

Dibromofluoromethane

Concen: 46.180 ug/l

RT: 5.47 min Scan# 752

Delta R.T. 0.00 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05


Tgt Ion:113 Resp: 431772

Ion Ratio Lower Upper

113 100

111 101.6 81.5 122.3



192 23.7 17.8 26.6

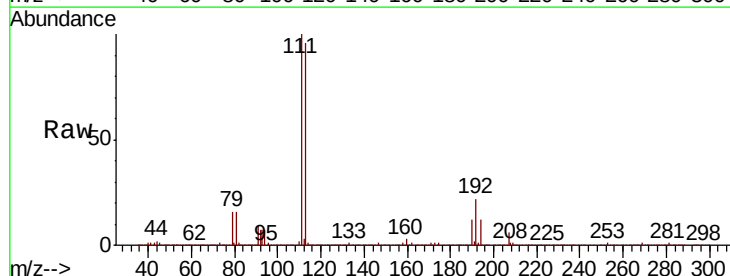


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

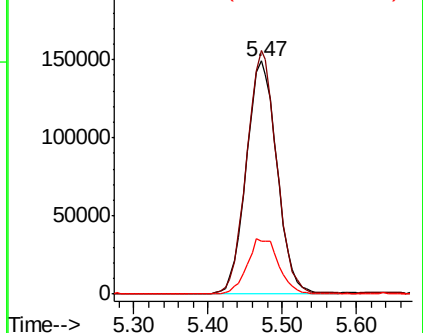

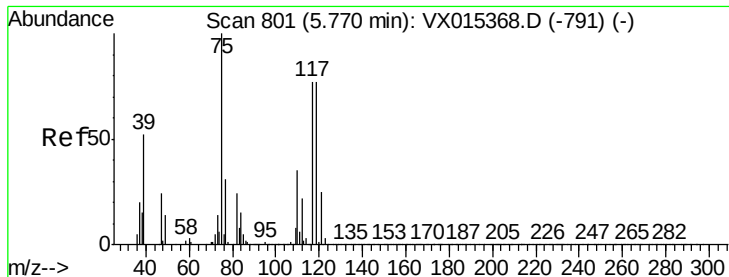

#36

1,1-Dichloropropene

Concen: 4.633 ug/l

RT: 5.64 min Scan# 779

Delta R.T. -0.13 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :

TP-17A


Tot Ion: 75 Resp: 62434

Ion Ratio Lower Upper


75 100

110 10.5 17.1 51.3#

77 0.0 24.6 36.8#


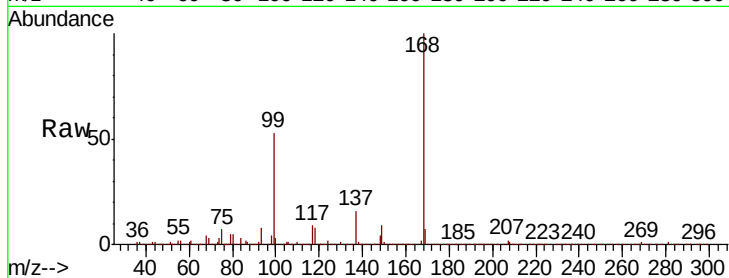


Abundance Ion 74.90 (74.60 to 75.60): VX015820.D (-752) (-)

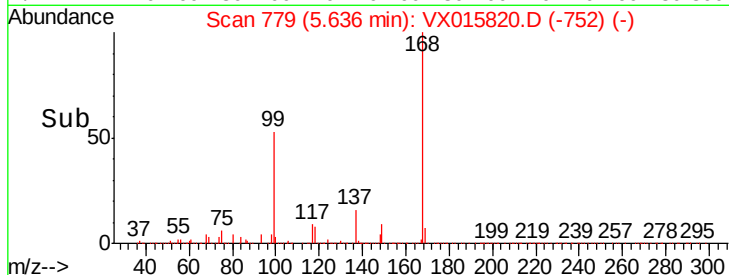

Ion 109.90 (109.60 to 110.60): VX015820.D (-752) (-)

Ion 76.90 (76.60 to 77.60): VX015820.D (-752) (-)

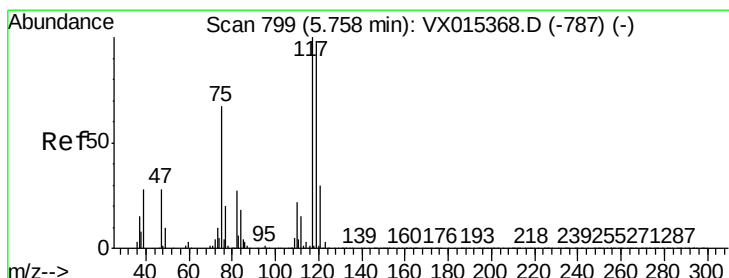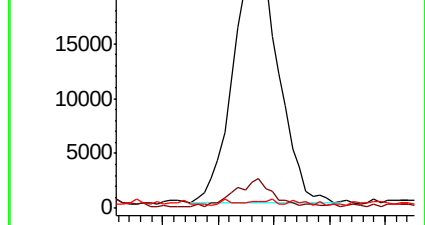

#38

Carbon Tetrachloride

Concen: 5.718 ug/l

RT: 5.64 min Scan# 779

Delta R.T. -0.12 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05


Tgt Ion: 117 Resp: 83470

Ion Ratio Lower Upper


117 100

119 3.6 78.0 117.0#

121 0.0 23.8 35.8#

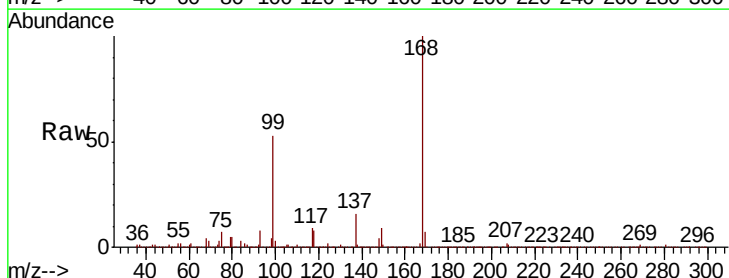



Abundance Ion 116.80 (116.50 to 117.50): VX015820.D (-750) (-)

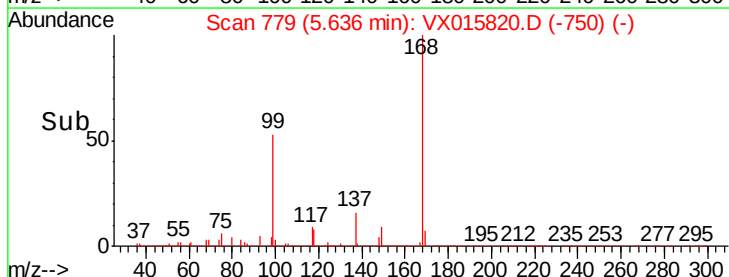

Ion 118.80 (118.50 to 119.50): VX015820.D (-750) (-)

Ion 120.80 (120.50 to 121.50): VX015820.D (-750) (-)

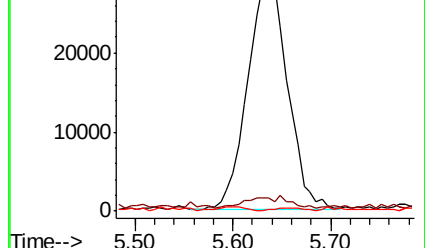



#40

Benzene

Concen: 0.215 ug/l

RT: 6.12 min Scan# 858

Delta R.T. 0.00 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampled :





TP-17A

Tot Ion: 78 Resp: 8487

Ion Ratio Lower Upper

78 100

77 11.1 19.8 29.8#

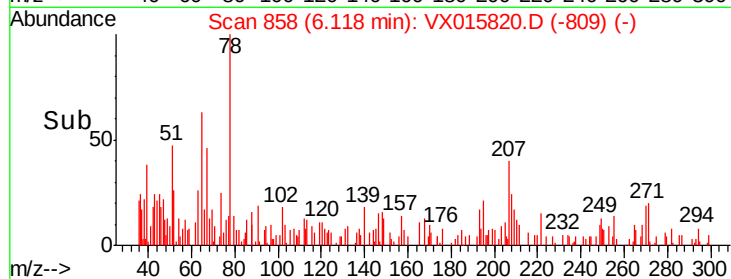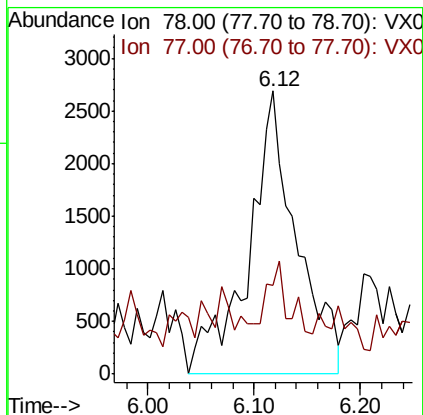

#43

Isopropyl Acetate

Concen: 10.798 ug/l

RT: 6.42 min Scan# 907

Delta R.T. 0.00 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05




Tgt Ion: 43 Resp: 319864


Ion Ratio Lower Upper

43 100

61 19.5 14.8 22.2

87 12.2 9.4 14.0

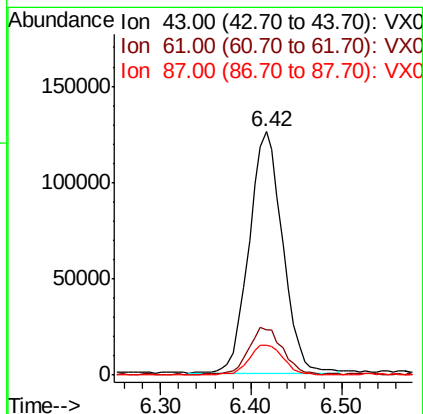



#48

Methvl methacrylate

Concen: 1.445 ug/l

RT: 7.65 min Scan# 1110

Delta R.T. -0.10 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :

TP-17A


Tot Ion: 41 Resp: 21375

Ion Ratio Lower Upper

41 100

69 2.1 56.7 85.1#




39 0.0 46.5 69.7#

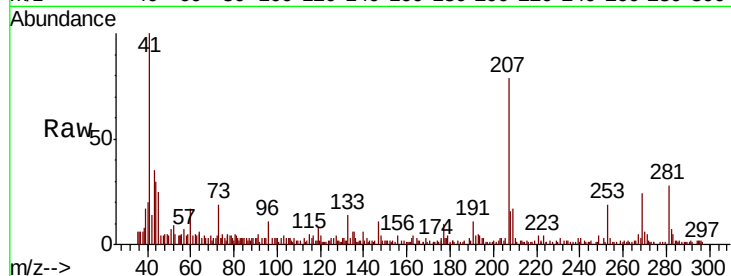

Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

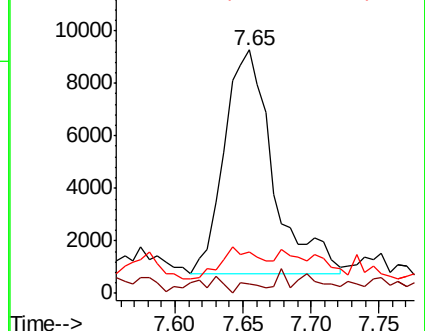

#49

1,4-Dioxane

Concen: 4.543 ug/l

RT: 7.71 min Scan# 1119

Delta R.T. -0.01 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05


Tgt Ion: 88 Resp: 1254

Ion Ratio Lower Upper

88 100

43 0.0 30.1 45.1#



58 258.5 60.6 90.8#




Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




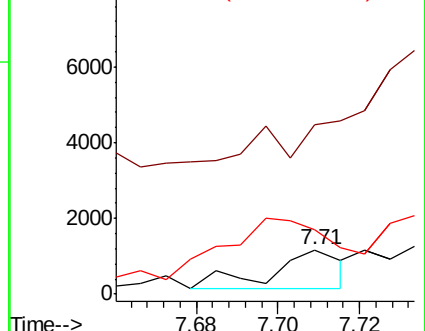




#50
Toluene-d8
Concen: 50.778 ug/l
RT: 8.70 min Scan# 1281
Delta R.T. 0.00 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05




Instrument :
MSVOA_X
ClientSampleId :
TP-17A


Tot Ion: 98 Resp: 1747953
Ion Ratio Lower Upper
98 100
100 67.9 53.5 80.3

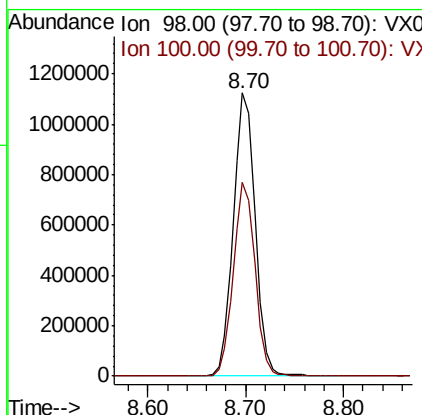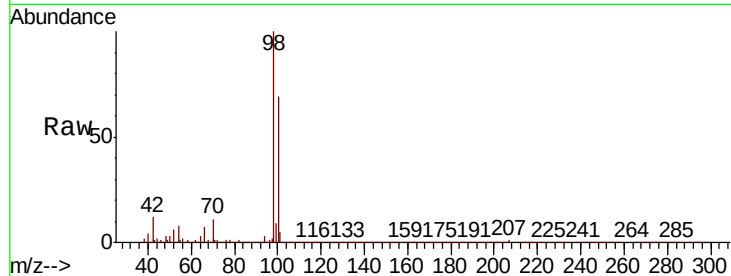

#51
4-Methyl-2-Pentanone
Concen: 18.498 ug/l
RT: 8.59 min Scan# 1264
Delta R.T. -0.03 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Tgt Ion: 43 Resp: 310537
Ion Ratio Lower Upper
43 100
58 6.1 29.7 44.5#

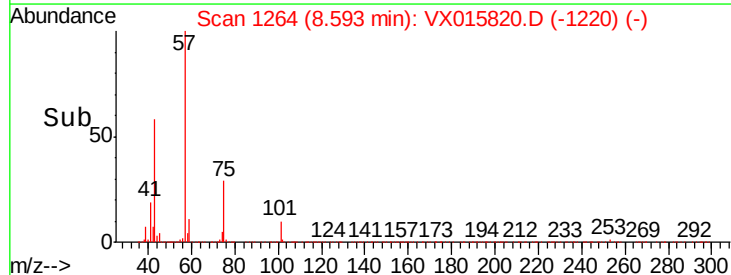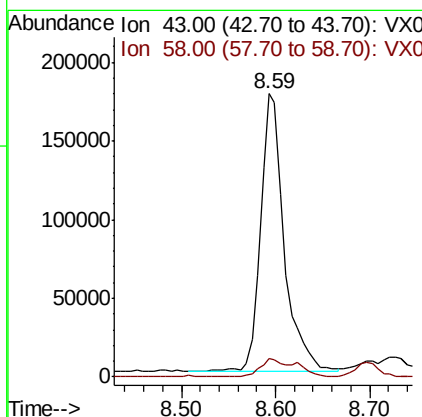




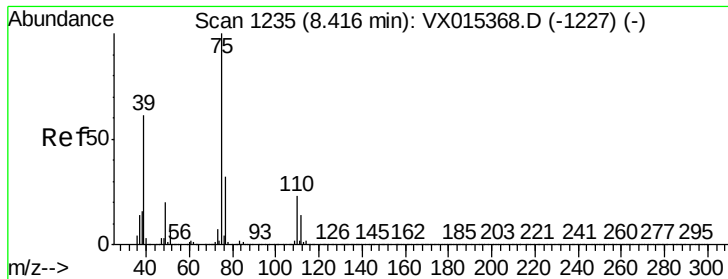


#54

cis-1,3-Dichloropropene
 Concen: 7.152 ug/l
 RT: 8.59 min Scan# 1264
 Delta R.T. 0.18 min
 Lab File: VX015820.D
 Acq: 22 Apr 2020 02:05

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-17A




Tot Ion	Ratio	Lower	Upper
75	100		
77	0.3	25.8	38.6#
39	23.0	49.0	73.4#

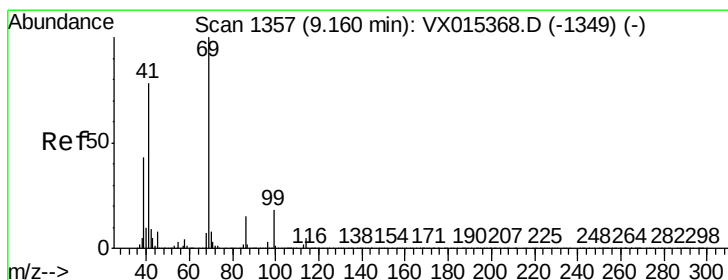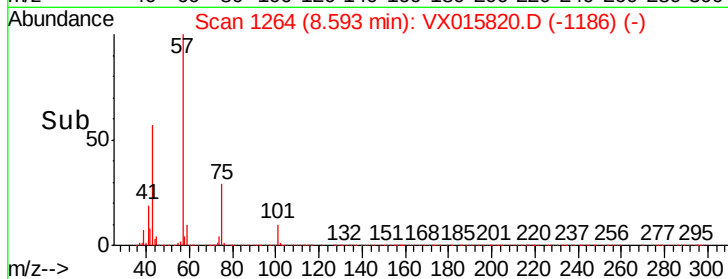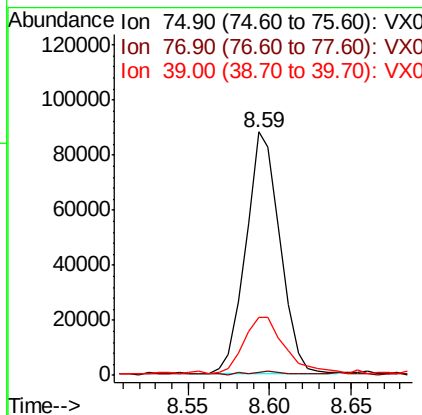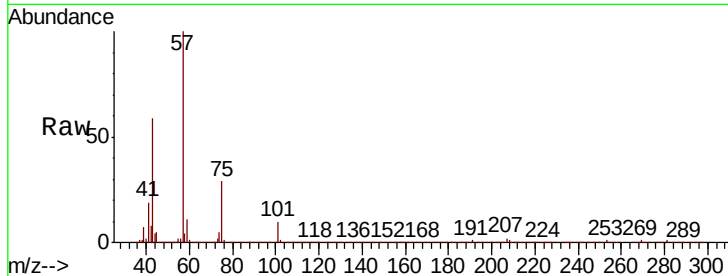


#56

Ethyl methacrylate
 Concen: 0.206 ug/l
 RT: 9.29 min Scan# 1379
 Delta R.T. 0.13 min
 Lab File: VX015820.D
 Acq: 22 Apr 2020 02:05

Tgt Ion	Ratio	Lower	Upper
69	100		
41	6329.6	61.6	92.4#
39	2349.3	34.0	51.0#

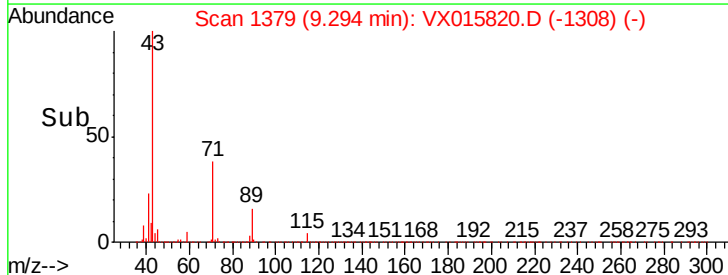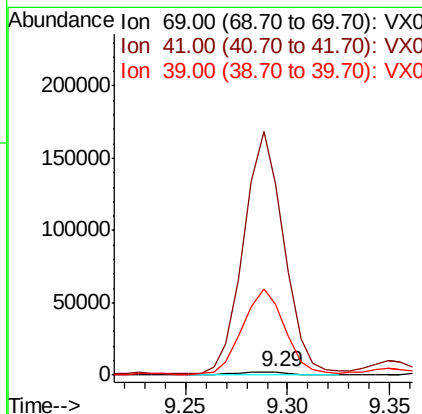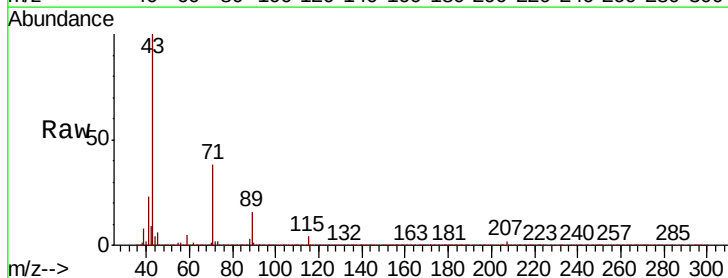



#57

1,3-Dichloropropane

Concen: 1.245 ug/l

RT: 9.53 min Scan# 1417

Delta R.T. 0.17 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :





TP-17A

Tot Ion: 76 Resp: 22365

Ion Ratio Lower Upper

76 100

78 0.0 25.8 38.8#

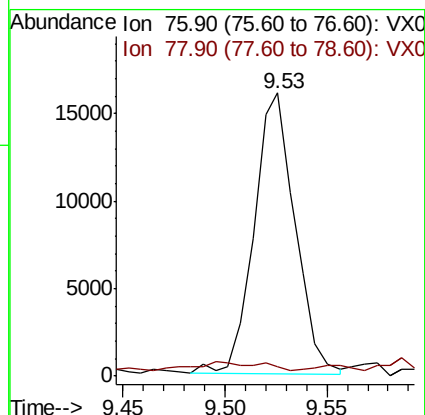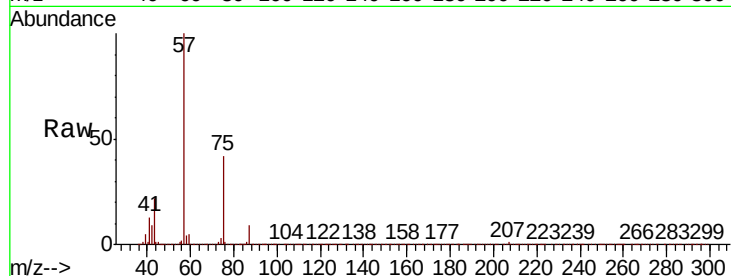

#59

2-Hexanone

Concen: 24.582 ug/l

RT: 9.53 min Scan# 1417

Delta R.T. 0.05 min

Lab File: VX015820.D




Acq: 22 Apr 2020 02:05


Tgt Ion: 43 Resp: 311560

Ion Ratio Lower Upper

43 100

58 18.6 25.6 76.6#

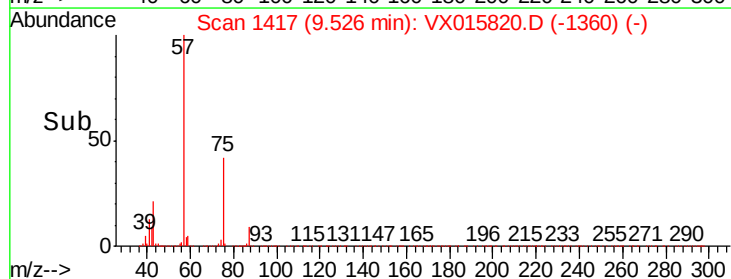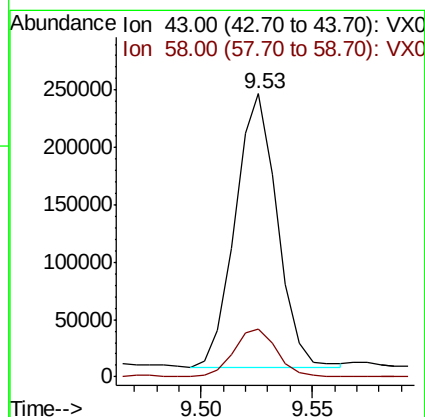



#62

4-Bromofluorobenzene

Concen: 53.857 ug/l

RT: 11.12 min Scan# 1679

Delta R.T. 0.00 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :

TP-17A


Tot Ion: 95 Resp: 753436

Ion Ratio Lower Upper

95 100

174 84.4 0.0 158.6

176 82.4 0.0 159.0

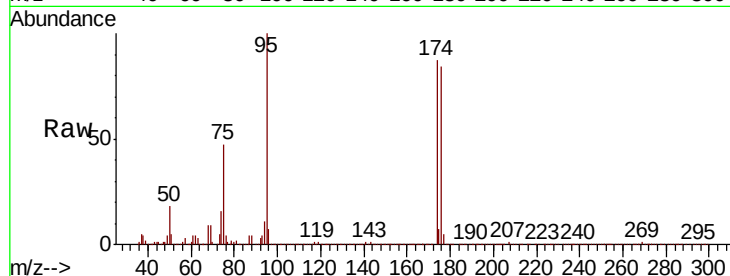


Abundance Ion 94.90 (94.60 to 95.60): VX015820.D (-1669) (-)

Ion 173.80 (173.50 to 174.50): VX015820.D (-1669) (-)

Ion 175.80 (175.50 to 176.50): VX015820.D (-1669) (-)

Time-->




Abundance Ion 94.90 (94.60 to 95.60): VX015820.D (-1669) (-)

Ion 173.80 (173.50 to 174.50): VX015820.D (-1669) (-)

Ion 175.80 (175.50 to 176.50): VX015820.D (-1669) (-)

Time-->

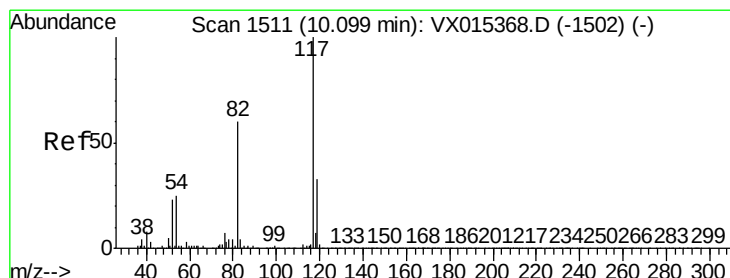

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1511

Delta R.T. 0.00 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05


Tgt Ion: 117 Resp: 1430355

Ion Ratio Lower Upper

117 100

82 55.8 47.8 71.8

119 32.2 26.8 40.2

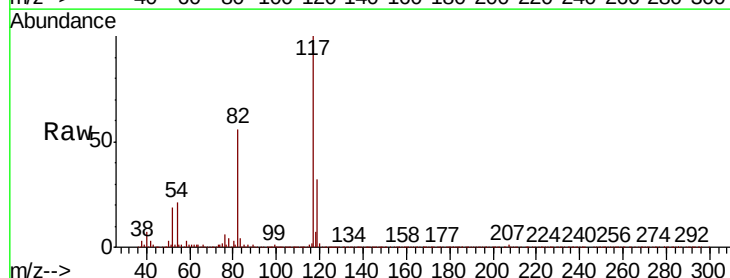


Abundance Ion 116.90 (116.60 to 117.60): VX015820.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX015820.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX015820.D (-1462) (-)

Time-->




Abundance Ion 116.90 (116.60 to 117.60): VX015820.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX015820.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX015820.D (-1462) (-)

Time-->







#72

1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1833
Delta R.T. 0.00 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Instrument :
MSVOA_X
ClientSampleId :
TP-17A




Tot Ion	Ratio	Lower	Upper
152	100		
115	55.3	39.0	116.9
150	153.9	0.0	340.8

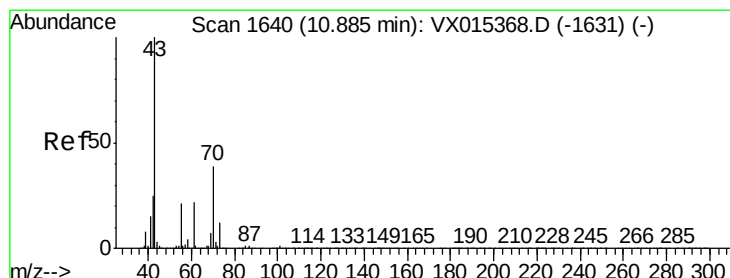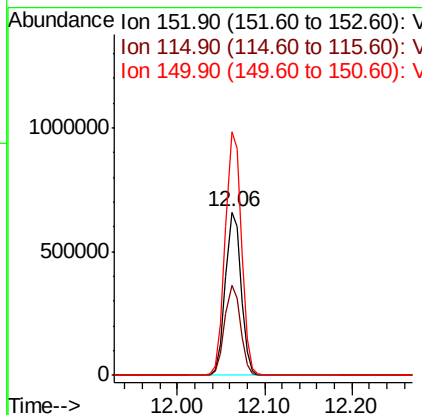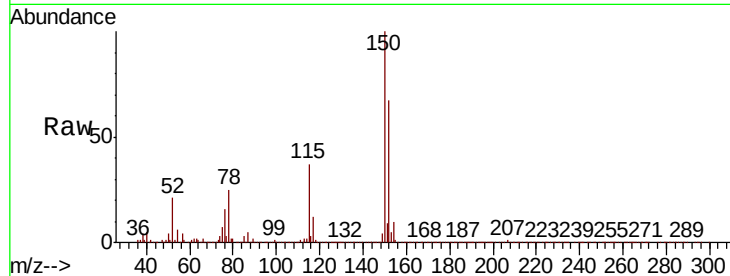


#74

N-amyl acetate
Concen: 0.906 ug/l
RT: 10.81 min Scan# 1627
Delta R.T. -0.08 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Tgt Ion	Ratio	Lower	Upper
43	100		
70	1.7	30.2	45.4#
55	5.9	16.8	25.2#
61	4.1	18.2	27.2#

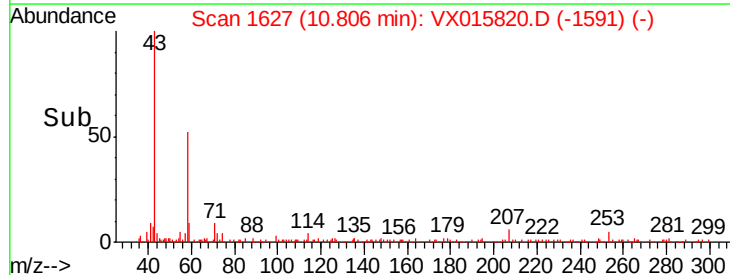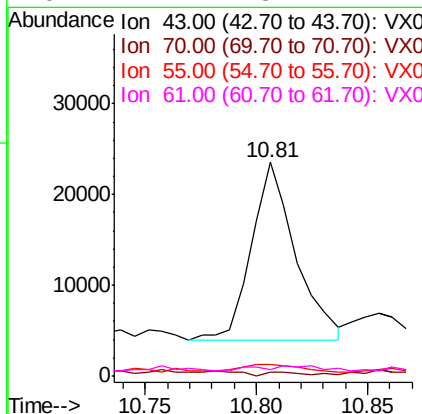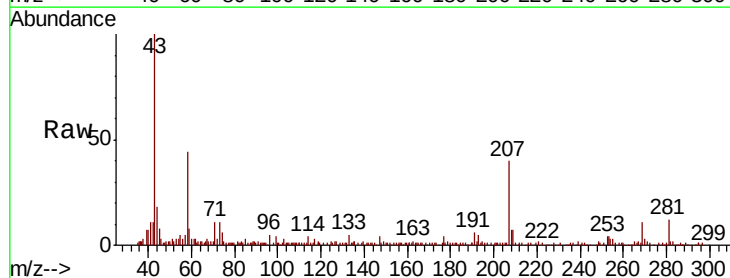



#76

1,2,3-Trichloropropane

Concen: 21.713 ug/l

RT: 11.12 min Scan# 1679

Delta R.T. -0.16 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05

Instrument :

MSVOA_X

ClientSampleId :





TP-17A

Tot Ion: 75 Resp: 363064

Ion Ratio Lower Upper

75 100

77 1.4 21.2 63.6#

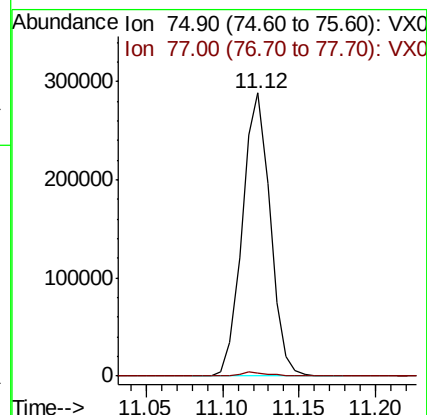

#81

trans-1,4-Dichloro-2-butene

Concen: 52.099 ug/l

RT: 11.12 min Scan# 1679

Delta R.T. 0.06 min

Lab File: VX015820.D

Acq: 22 Apr 2020 02:05




Tgt Ion: 75 Resp: 363064


Ion Ratio Lower Upper

75 100

53 0.2 80.1 120.1#

89 0.0 36.1 54.1#

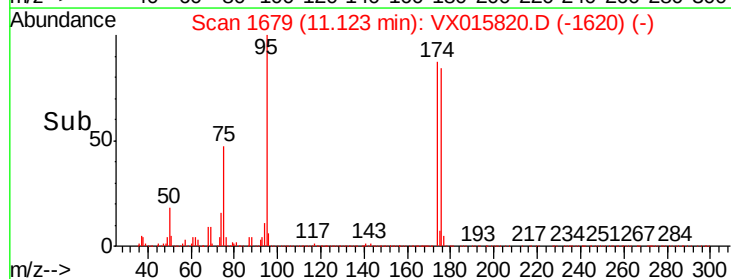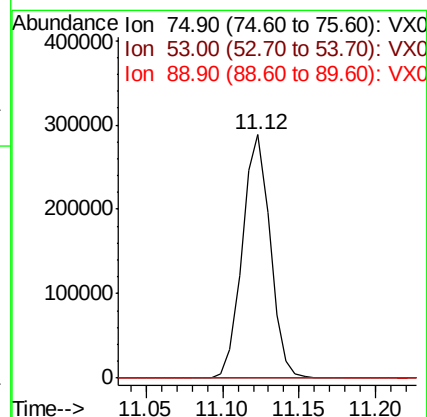


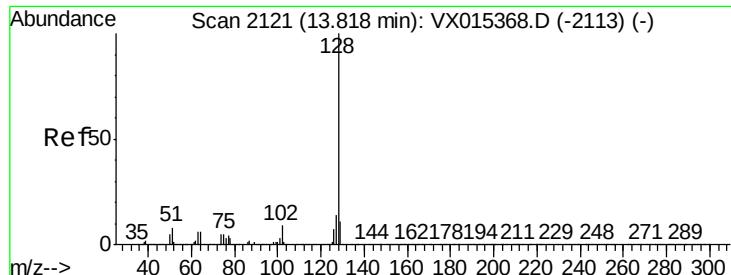

#95
Naphthalene
Concen: 0.346 ug/l
RT: 13.82 min Scan# 2121
Delta R.T. 0.00 min
Lab File: VX015820.D
Acq: 22 Apr 2020 02:05

Instrument :
MSVOA_X
ClientSampleId :
TP-17A

Tot Ion	Ratio	Lower	Upper
128	100		
127	20.6	10.6	15.8#
129	17.4	8.8	13.2#

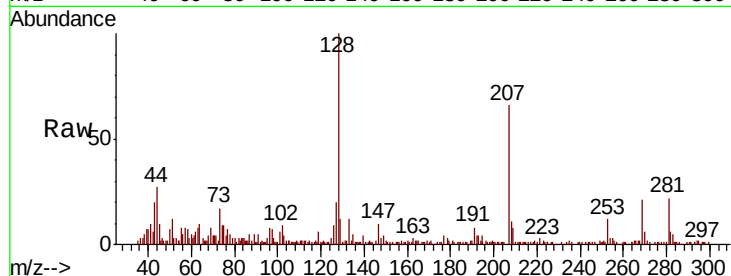

Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

