

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042120\
 Data File : VX015807.D
 Acq On : 21 Apr 2020 20:03
 Operator : JC/SP
 Sample : L2344-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-2

Quant Time: Apr 22 06:33:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 27 09:35:51 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	1011790	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	1568204	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	1517454	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	859020	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.04	65	560383	39.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	78.54%	
35) Dibromofluoromethane	5.47	113	446141	44.51	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.02%	
50) Toluene-d8	8.70	98	1893931	51.32	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.64%	
62) 4-Bromofluorobenzene	11.12	95	794803	52.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.98%	
Target Compounds						
16) Acetone	2.42	43	176433	28.778	ug/l	97
17) Carbon Disulfide	2.56	76	43738	1.501	ug/l #	94
20) Methylene Chloride	2.84	84	46566	4.066	ug/l	95
43) Isopropyl Acetate	6.42	43	296487	9.335	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042120\
Data File : VX015807.D
Acq On : 21 Apr 2020 20:03
Operator : JC/SP
Sample : L2344-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-2

Quant Time: Apr 22 06:33:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 27 09:35:51 2020
Response via : Initial Calibration

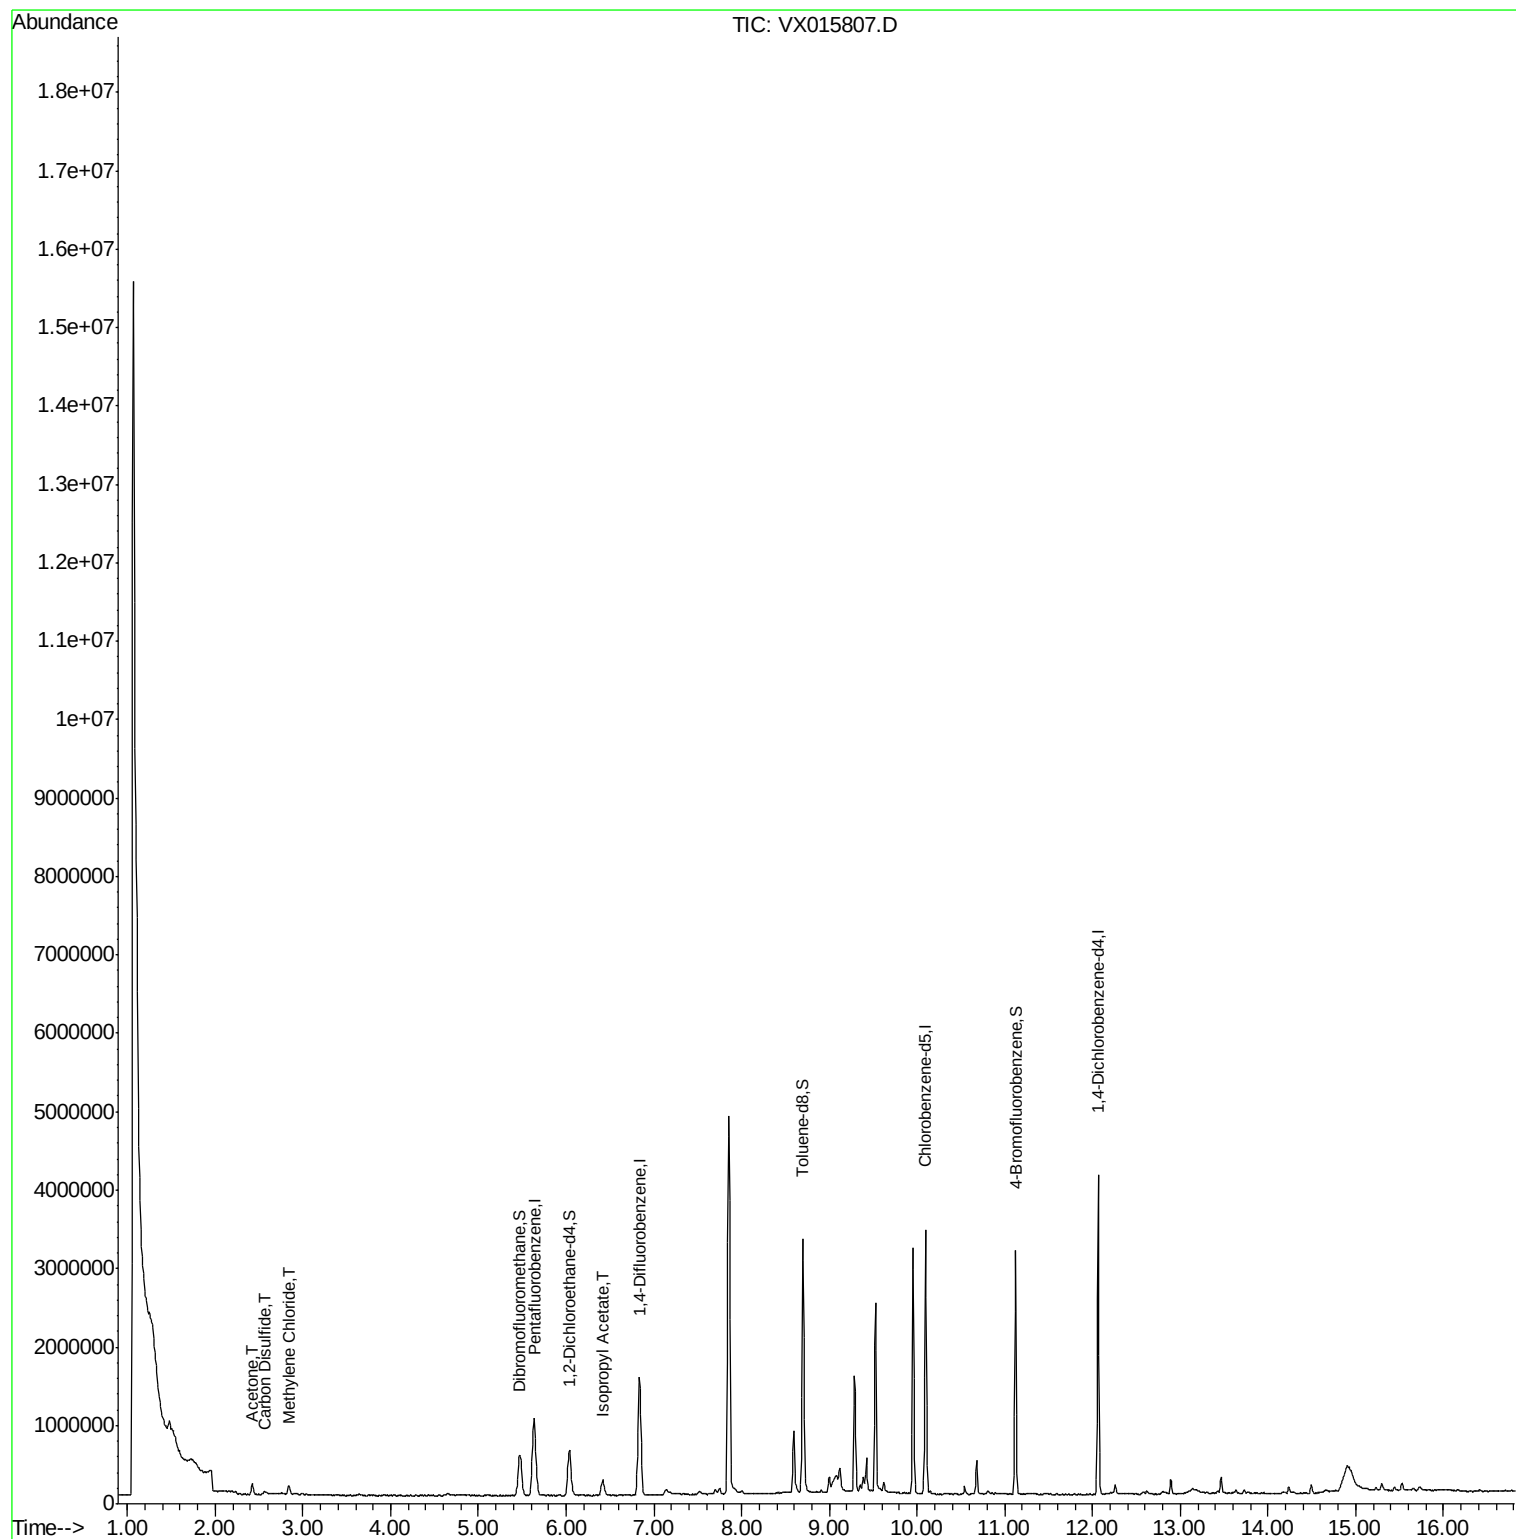

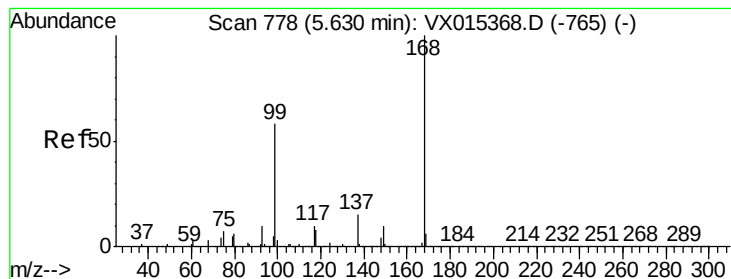

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 779

Delta R.T. 0.01 min

Lab File: VX015807.D

Acq: 21 Apr 2020 20:03

Instrument :

MSVOA_X

ClientSampleId :


TP-2

Tot Ion:168 Resp: 1011790

Ion Ratio Lower Upper

168 100

99 52.0 46.4 69.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64

400000

300000



200000

100000

0

5.50 5.60 5.70 5.80

Time-->

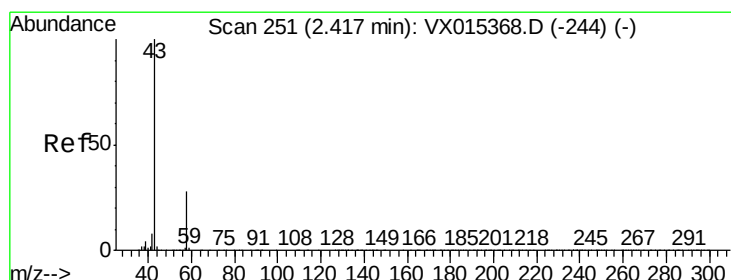

#16

Acetone

Concen: 28.778 ug/l

RT: 2.42 min Scan# 252

Delta R.T. 0.01 min

Lab File: VX015807.D


Acq: 21 Apr 2020 20:03

Tgt Ion: 43 Resp: 176433

Ion Ratio Lower Upper

43 100

58 29.2 22.1 33.1



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.42

100000

80000

60000


40000


20000

0

2.35 2.40 2.45 2.50

Time-->





#17

Carbon Disulfide

Concen: 1.501 ug/l

RT: 2.56 min Scan# 274

Delta R.T. 0.01 min

Lab File: VX015807.D

Acq: 21 Apr 2020 20:03

Instrument :

MSVOA_X

ClientSampleId :


TP-2

Tot Ion: 76 Resp: 43738

Ion Ratio Lower Upper

76 100

78 6.7 7.1 10.7#

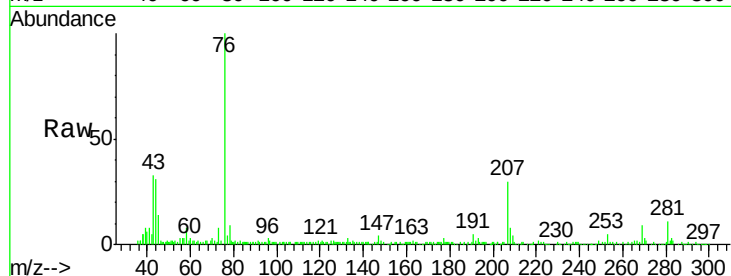

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

2.56

30000

25000

20000



15000

10000

5000

0

Time-->



#20

Methylene Chloride

Concen: 4.066 ug/l

RT: 2.84 min Scan# 320

Delta R.T. 0.01 min

Lab File: VX015807.D

Acq: 21 Apr 2020 20:03

Tgt Ion: 84 Resp: 46566


Ion Ratio Lower Upper

84 100

49 134.1 111.3 166.9

51 42.4 34.0 51.0

86 57.8 52.5 78.7



Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

50000

40000


30000


20000

10000

0

Time-->









#33
 1,2-Dichloroethane-d4
 Concen: 39.269 ug/l
 RT: 6.04 min Scan# 845
 Delta R.T. 0.01 min
 Lab File: VX015807.D
 Acq: 21 Apr 2020 20:03




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-2


Tot Ion: 65 Resp: 560383
 Ion Ratio Lower Upper
 65 100
 67 51.9 0.0 102.6

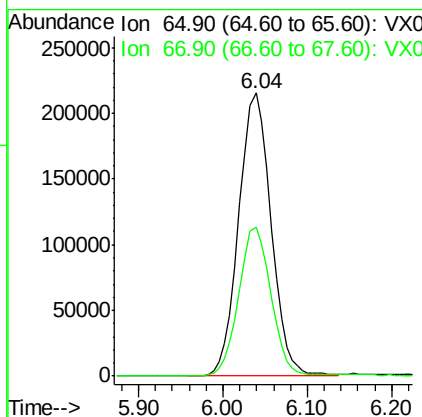

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.84 min Scan# 976
 Delta R.T. 0.00 min
 Lab File: VX015807.D
 Acq: 21 Apr 2020 20:03

Tgt Ion: 114 Resp: 1568204
 Ion Ratio Lower Upper
 114 100
 63 20.5 0.0 44.2
 88 15.9 0.0 33.8



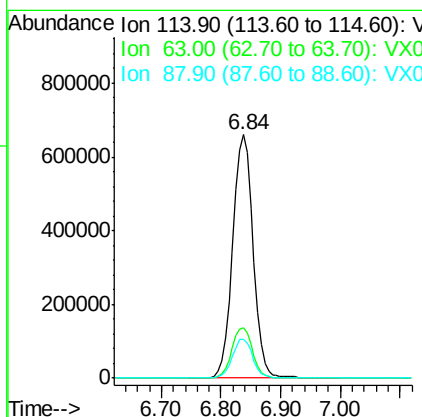



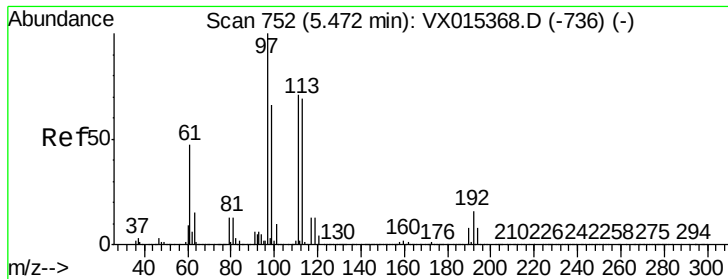

#35
 Dibromofluoromethane
 Concen: 44.506 ug/l
 RT: 5.47 min Scan# 752
 Delta R.T. 0.00 min
 Lab File: VX015807.D
 Acq: 21 Apr 2020 20:03




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-2


Tot Ion	Ratio	Lower	Upper
113	100		
111	104.5	81.5	122.3
192	24.2	17.8	26.6

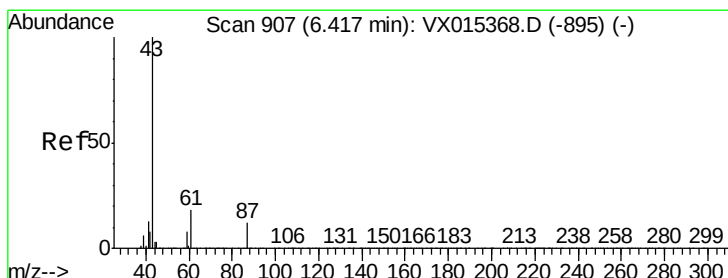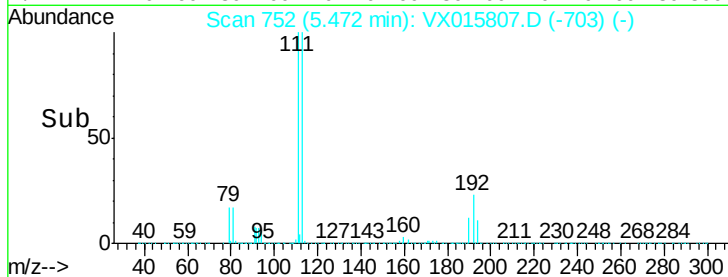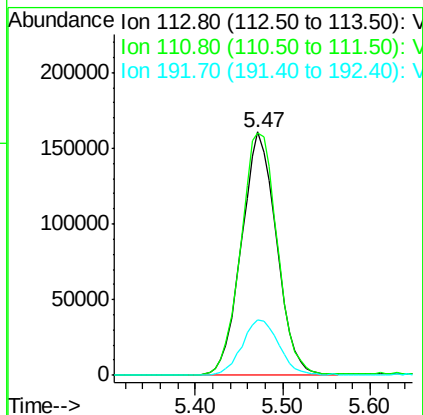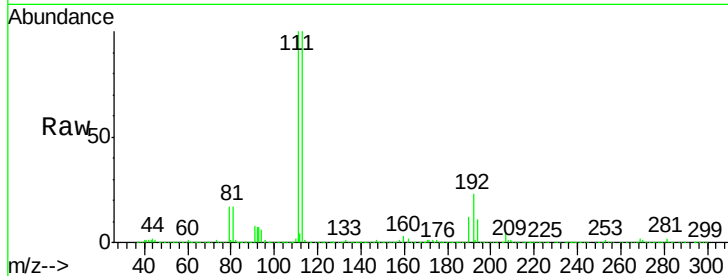

#43
 Isopropyl Acetate
 Concen: 9.335 ug/l
 RT: 6.42 min Scan# 907
 Delta R.T. 0.00 min
 Lab File: VX015807.D
 Acq: 21 Apr 2020 20:03

Tgt Ion	Ratio	Lower	Upper
43	100		
61	19.7	14.8	22.2
87	12.8	9.4	14.0


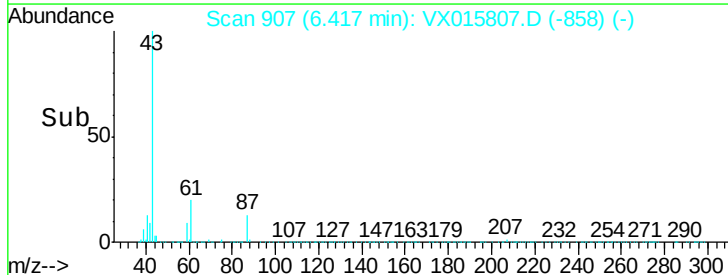
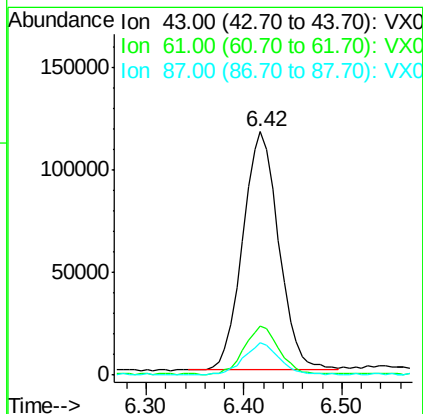
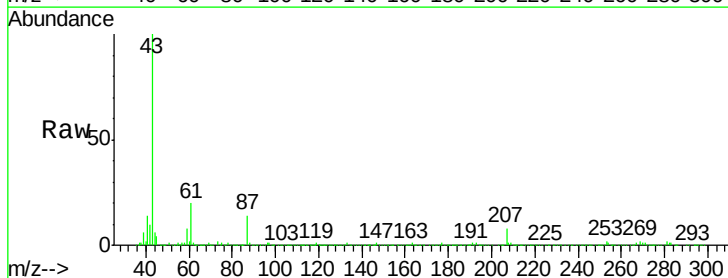




#50
Toluene-d8
Concen: 51.316 ug/l
RT: 8.70 min Scan# 1281
Delta R.T. 0.00 min
Lab File: VX015807.D
Acq: 21 Apr 2020 20:03




Instrument :
MSVOA_X
ClientSampleId :
TP-2


Tot Ion: 98 Resp: 1893931
Ion Ratio Lower Upper
98 100
100 66.2 53.5 80.3

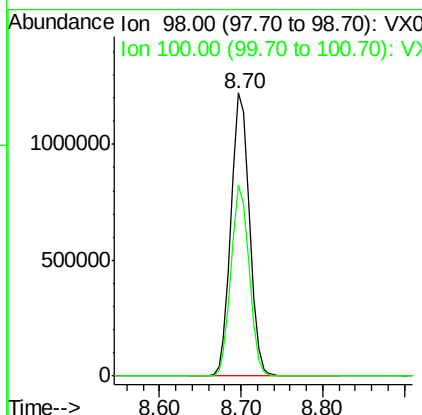

#62
4-Bromofluorobenzene
Concen: 52.990 ug/l
RT: 11.12 min Scan# 1679
Delta R.T. 0.00 min
Lab File: VX015807.D
Acq: 21 Apr 2020 20:03

Tgt Ion: 95 Resp: 794803
Ion Ratio Lower Upper
95 100
174 85.8 0.0 158.6
176 82.7 0.0 159.0



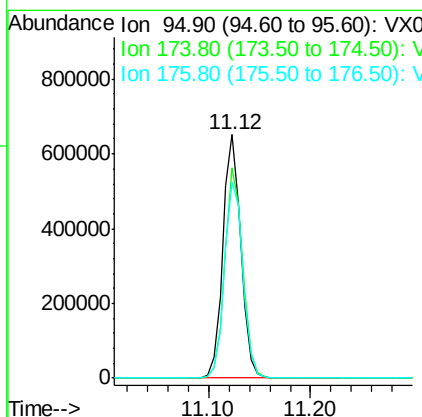



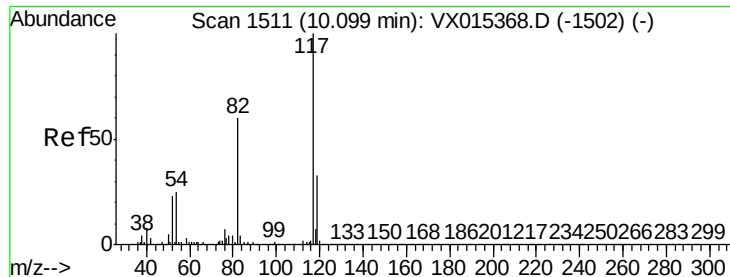

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1511
Delta R.T. 0.00 min
Lab File: VX015807.D
Acq: 21 Apr 2020 20:03

Instrument :
MSVOA_X
ClientSampled :
TP-2

Tot Ion:117 Resp: 1517454
Ion Ratio Lower Upper
117 100
82 54.0 47.8 71.8
119 31.5 26.8 40.2

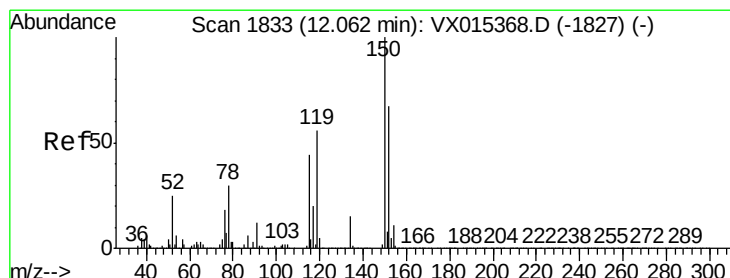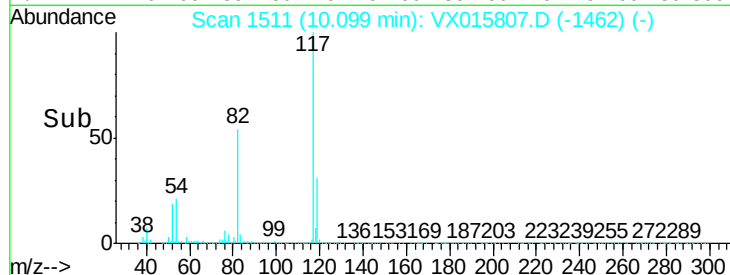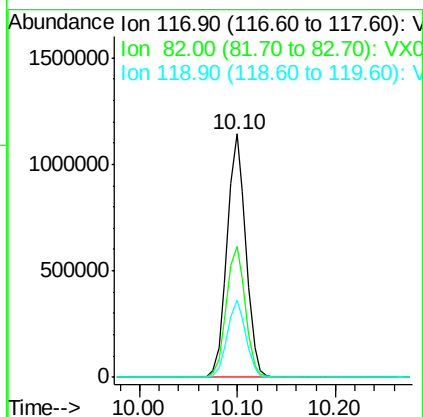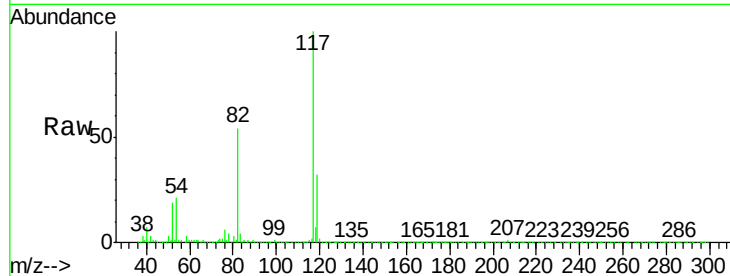

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1833
Delta R.T. 0.00 min
Lab File: VX015807.D
Acq: 21 Apr 2020 20:03

Tgt Ion:152 Resp: 859020
Ion Ratio Lower Upper
152 100
115 55.2 39.0 116.9
150 155.8 0.0 340.8

