


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX042120\
 Data File : VX015782.D
 Acq On : 21 Apr 2020 10:05
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
 Title : SW846 8260
 Last Update : Fri Mar 27 09:35:51 2020

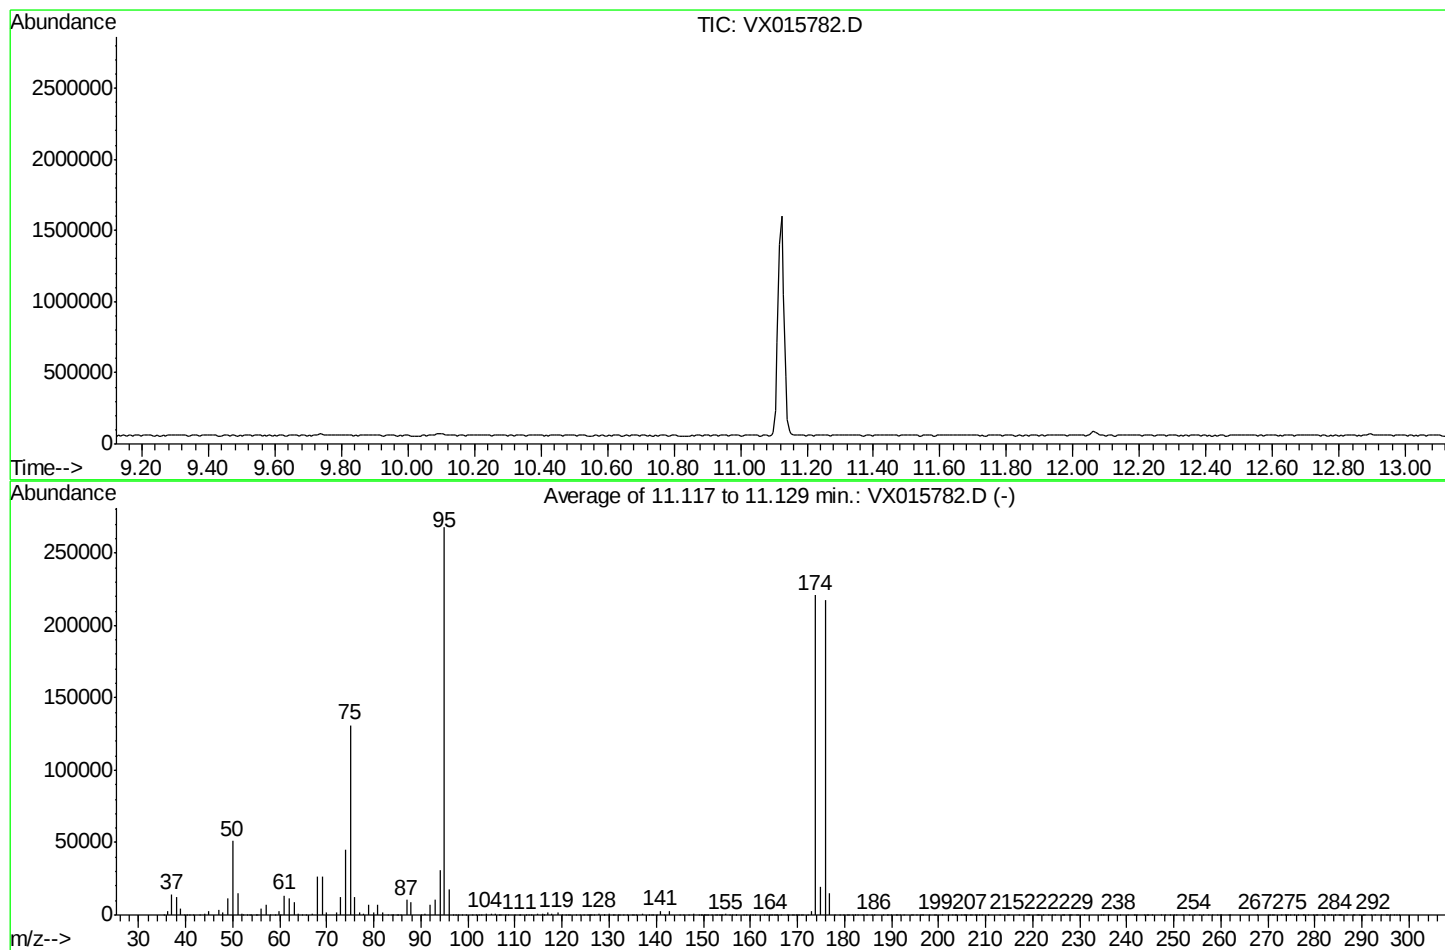

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1669

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	51224	PASS
75	95	30	60	48.9	130929	PASS
95	95	100	100	100.0	267824	PASS
96	95	5	9	6.7	17920	PASS
173	174	0.00	2	1.0	2275	PASS
174	95	50	100	82.4	220703	PASS
175	174	5	9	8.7	19114	PASS
176	174	95	101	98.8	217984	PASS
177	176	5	9	6.7	14708	PASS