


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX042120\
 Data File : VX015810.D
 Acq On : 21 Apr 2020 21:33
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
 Title : SW846 8260
 Last Update : Fri Mar 27 09:35:51 2020

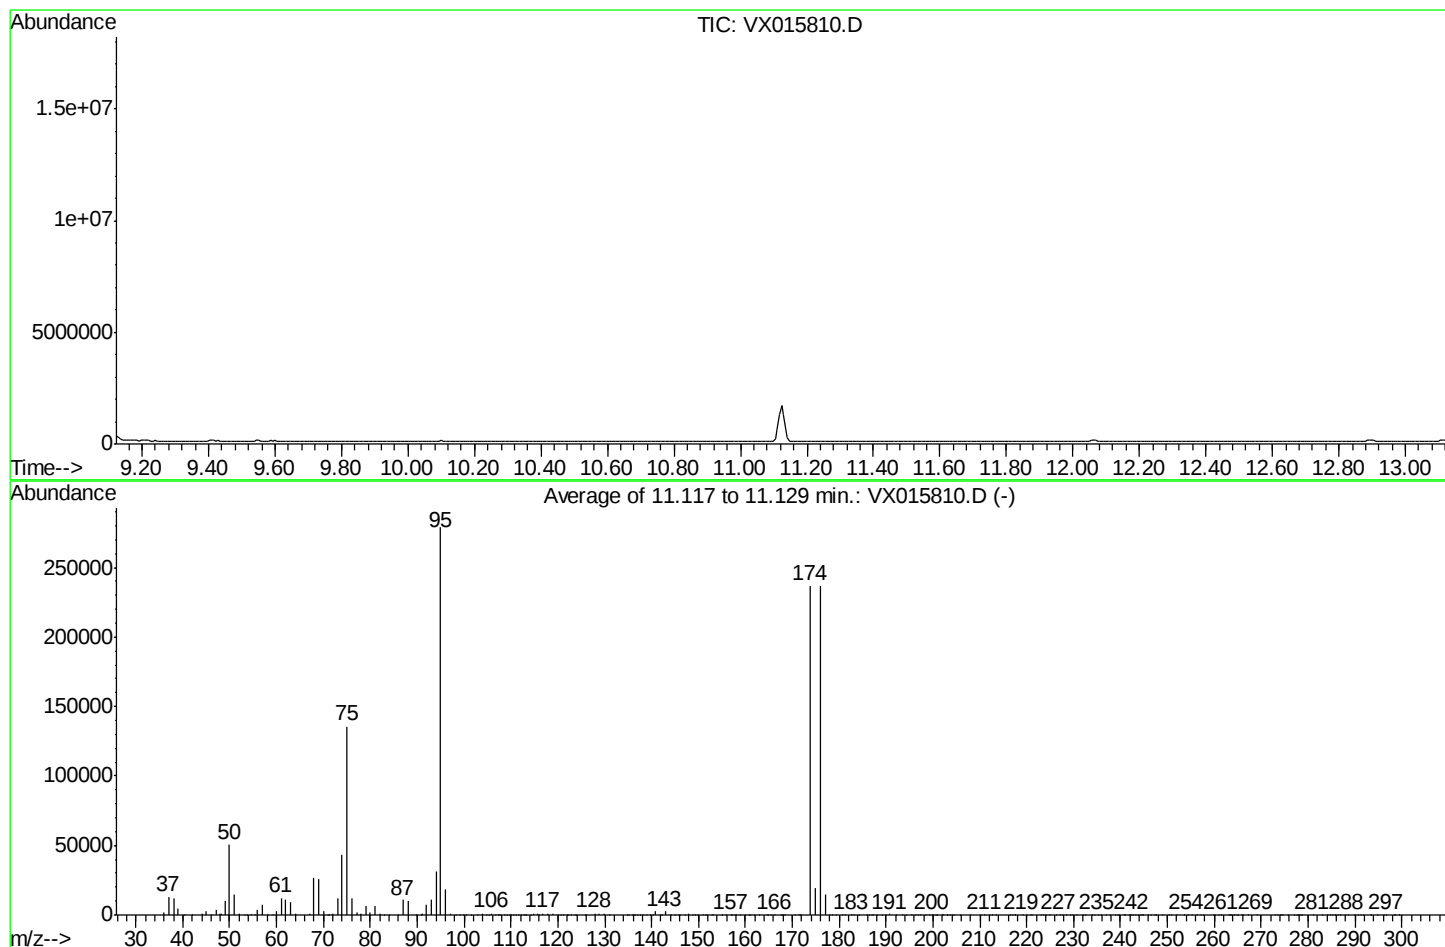

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1666

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	50628	PASS
75	95	30	60	48.5	135420	PASS
95	95	100	100	100.0	278957	PASS
96	95	5	9	6.6	18400	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.9	236928	PASS
175	174	5	9	8.1	19152	PASS
176	174	95	101	99.9	236601	PASS
177	176	5	9	6.3	14819	PASS