

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042121\
 Data File : VX021797.D
 Acq On : 21 Apr 2021 16:57
 Operator : JC/MD
 Sample : M2079-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-12DL

Quant Time: Apr 22 08:59:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 20 13:46:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	162083	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	283352	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.098	117	259943	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	124522	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	94913	51.62	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.24%
35) Dibromofluoromethane	5.464	113	89205	49.23	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.46%
50) Toluene-d8	8.696	98	342056	49.09	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.18%
62) 4-Bromofluorobenzene	11.116	95	124722	47.93	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.86%

Target Compounds					Qvalue	
3) Chloromethane	1.319	50	1499	1.03	ug/l	90
5) Bromomethane	1.648	94	258	0.32	ug/l #	21
6) Chloroethane	1.721	64	440	0.37	ug/l	95
11) Tert butyl alcohol	3.020	59	586	1.46	ug/l #	52
13) Acrolein	2.227	56	345	1.06	ug/l #	14
16) Acetone	2.422	43	1956	3.09	ug/l	93
19) Methyl tert-butyl Ether	3.166	73	3064	0.59	ug/l #	57
20) Methylene Chloride	2.837	84	1168	0.62	ug/l #	86
25) 2-Butanone	4.635	43	773	0.72	ug/l #	45
31) Cyclohexane	5.544	56	3302	1.28	ug/l	94
36) 1,1-Dichloropropene	5.623	75	11442	4.57	ug/l #	49
38) Carbon Tetrachloride	5.629	117	15455	5.64	ug/l #	16
39) Methylcyclohexane	7.440	83	1594	0.49	ug/l #	91
40) Benzene	6.111	78	177665	23.81	ug/l	98
42) 1,2-Dichloroethane	6.159	62	4984	2.06	ug/l	95
51) 4-Methyl-2-Pentanone	8.610	43	584	0.25	ug/l	94
52) Toluene	8.763	92	21575	4.46	ug/l	99
58) 2-Chloroethyl Vinyl ether	8.226	63	1011	0.69	ug/l #	45
67) Ethyl Benzene	10.232	91	126249	13.59	ug/l	98
68) m/p-Xylenes	10.342	106	37713	10.49	ug/l	99
69) o-Xylene	10.683	106	18334	5.29	ug/l	98
70) Styrene	10.683	104	1718	0.29	ug/l #	1
73) Isopropylbenzene	11.000	105	10405	1.19	ug/l	99
76) 1,2,3-Trichloropropane	11.116	75	56740	22.98	ug/l #	39
78) n-propylbenzene	11.341	91	14704	1.52	ug/l	98
79) 2-Chlorotoluene	11.439	91	2952	0.52	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.488	105	28424	3.84	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.116	75	56740	52.84	ug/l #	12
82) 4-Chlorotoluene	11.488	91	3287	0.50	ug/l #	45
84) 1,2,4-Trimethylbenzene	11.787	105	79136	10.59	ug/l	98
85) sec-Butylbenzene	11.787	105	79136	9.34	ug/l #	57
89) n-Butylbenzene	12.360	91	2794	0.41	ug/l #	16
90) Hexachloroethane	12.683	117	2489	1.70	ug/l #	9
95) Naphthalene	13.817	128	22164	2.64	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042121\
Data File : VX021797.D
Acq On : 21 Apr 2021 16:57
Operator : JC/MD
Sample : M2079-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-12DL

Quant Time: Apr 22 08:59:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 20 13:46:22 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042121\
Data File : VX021797.D
Acq On : 21 Apr 2021 16:57
Operator : JC/MD
Sample : M2079-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-12DL

Quant Time: Apr 22 08:59:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 20 13:46:22 2021
Response via : Initial Calibration




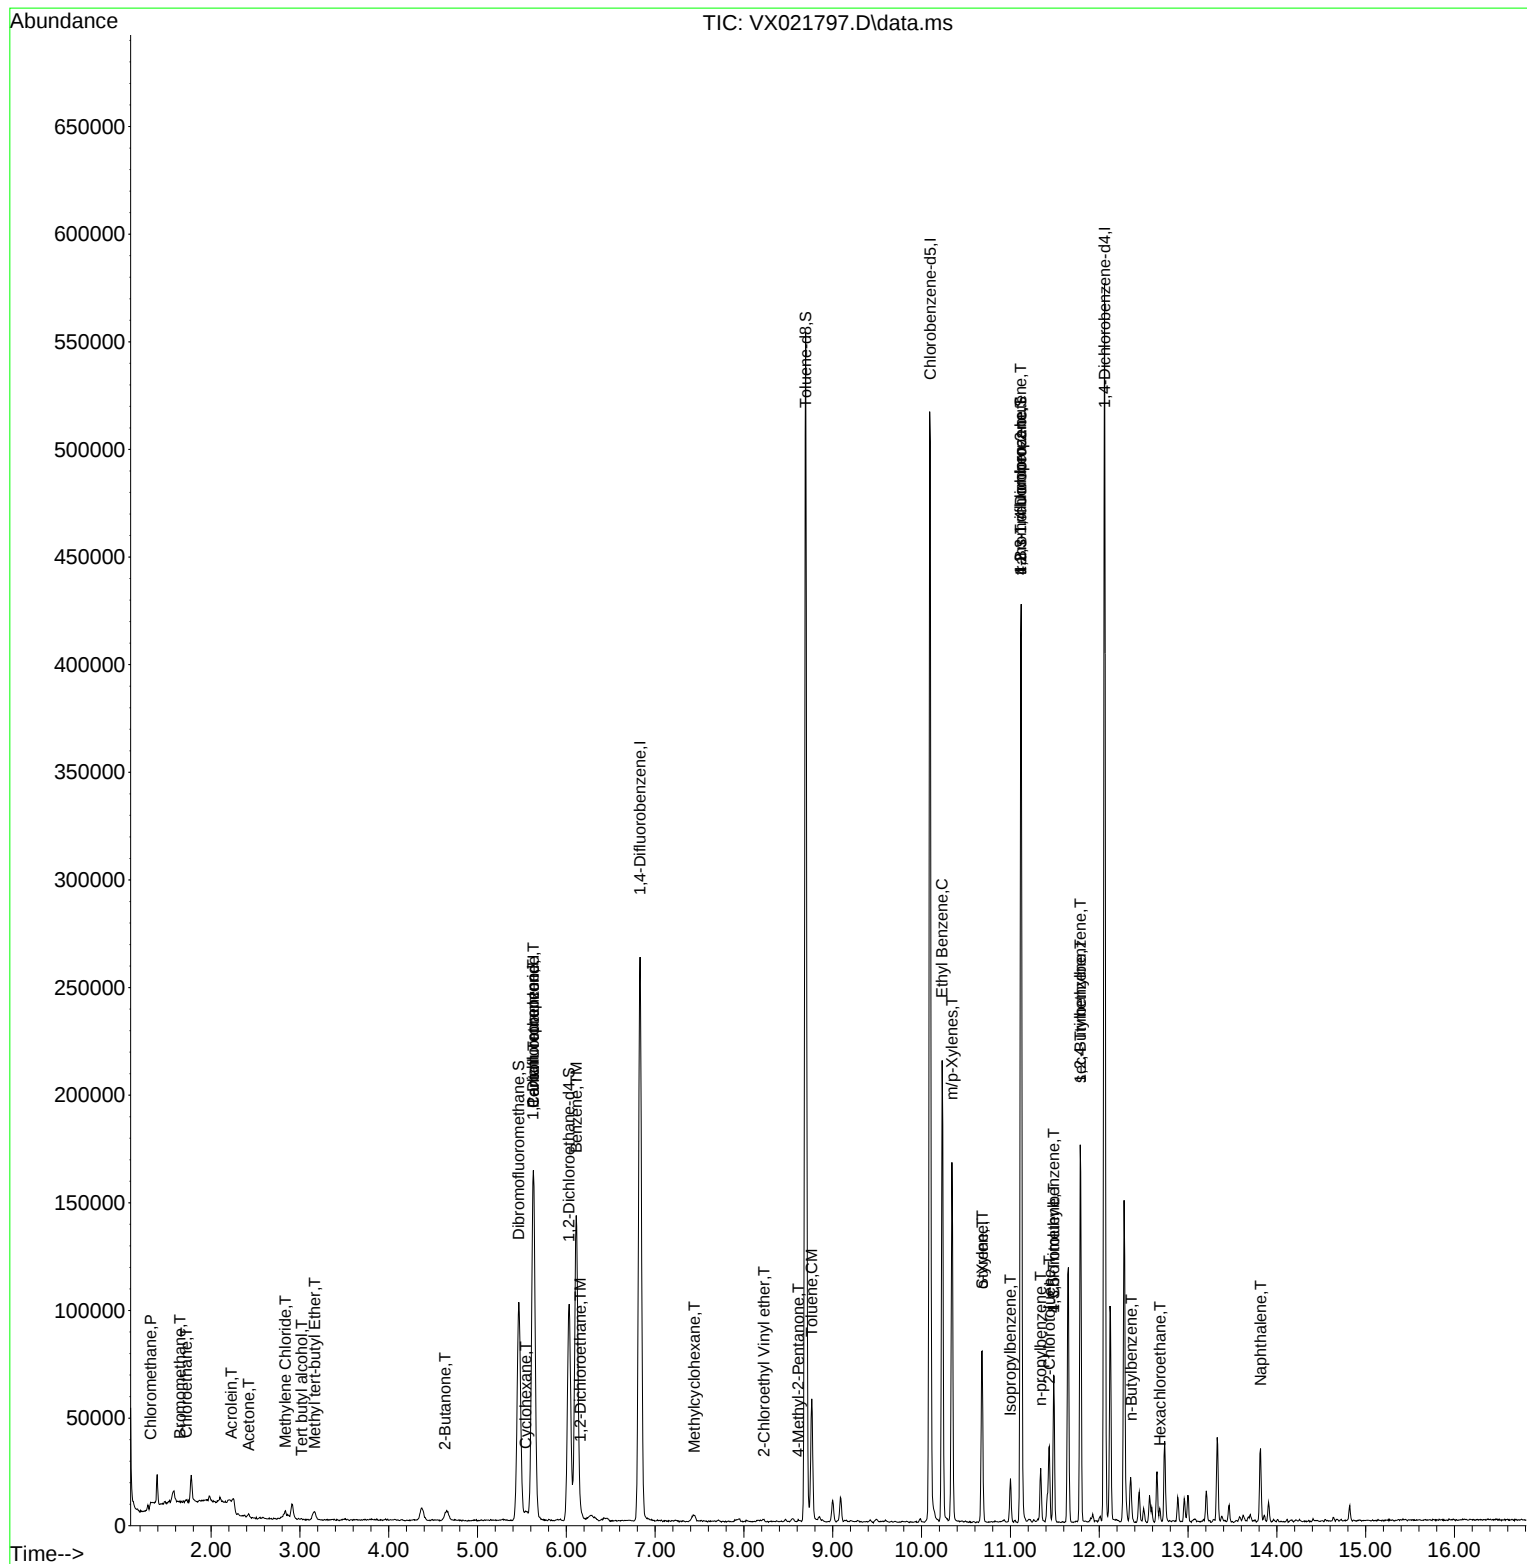




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion:168 Resp: 162083
Ion Ratio Lower Upper
168 100
99 57.0 45.8 68.6

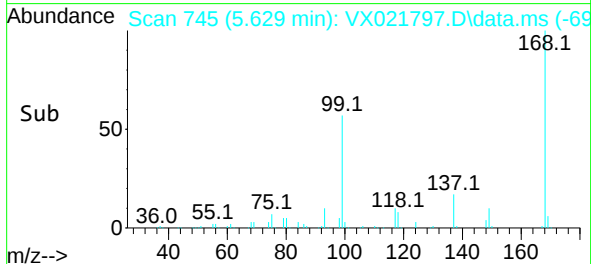

#3
Chloromethane
Concen: 1.03 ug/l
RT: 1.319 min Scan# 38
Delta R.T. 0.006 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 50 Resp: 1499
Ion Ratio Lower Upper
50 100
52 38.6 26.4 39.6


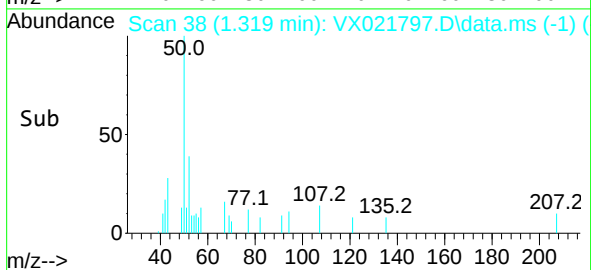

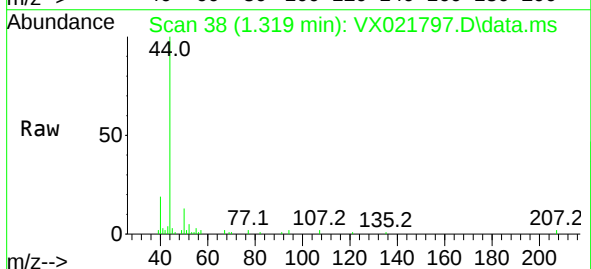


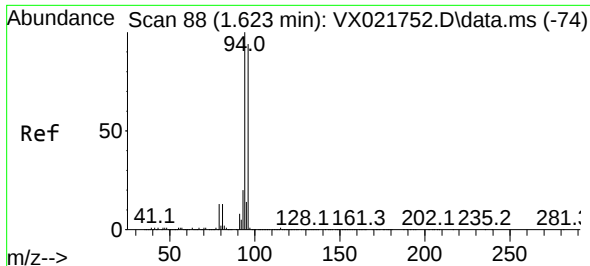

#5
Bromomethane
Concen: 0.32 ug/l
RT: 1.648 min Scan# 92
Delta R.T. 0.025 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampled :
MW-12DL


Tgt Ion: 94 Resp: 258
Ion Ratio Lower Upper
94 100
96 172.5 76.4 114.6#

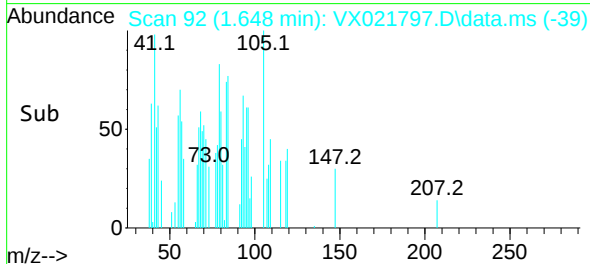

#6
Chloroethane
Concen: 0.37 ug/l
RT: 1.721 min Scan# 104
Delta R.T. 0.012 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 64 Resp: 440
Ion Ratio Lower Upper
64 100
66 34.5 25.4 38.0

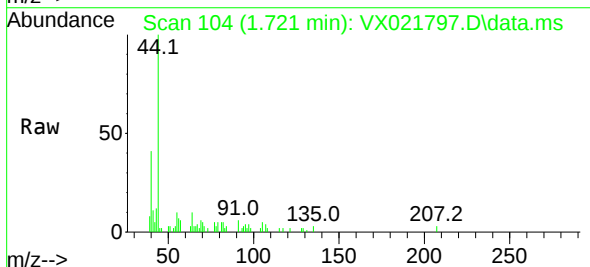







#11

Tert butyl alcohol
Concen: 1.46 ug/l
RT: 3.020 min Scan# 317
Delta R.T. 0.007 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Instrument :
MSVOA_X
ClientSampled :
MW-12DL




Tgt Ion: 59 Resp: 586
Ion Ratio Lower Upper
59 100
57 27.5 7.8 11.8#

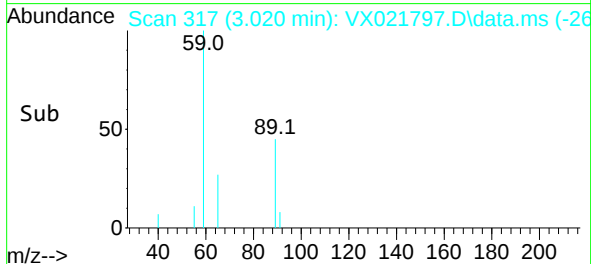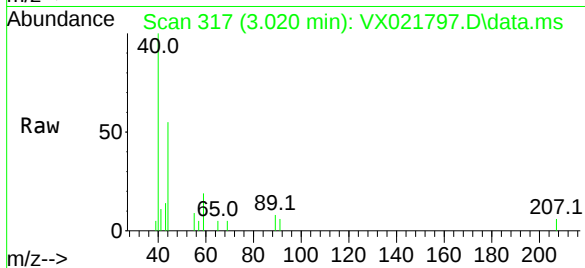


#13

Acrolein
Concen: 1.06 ug/l
RT: 2.227 min Scan# 187
Delta R.T. -0.049 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 56 Resp: 345
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#


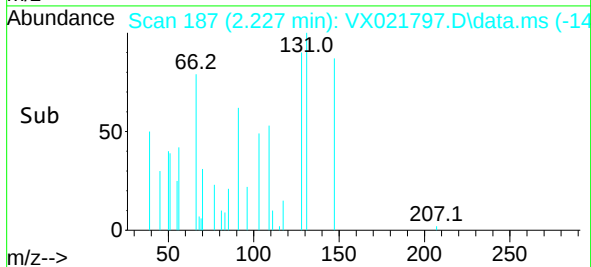

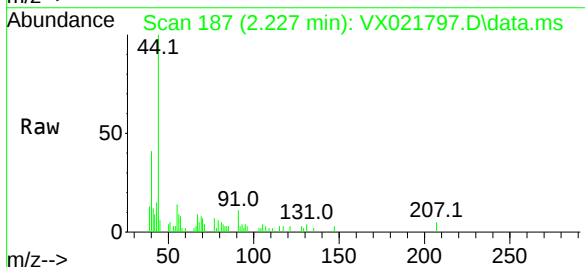




#16
Acetone
Concen: 3.09 ug/l
RT: 2.422 min Scan# 219
Delta R.T. 0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion: 43 Resp: 1956
Ion Ratio Lower Upper
43 100
58 38.6 27.8 41.8

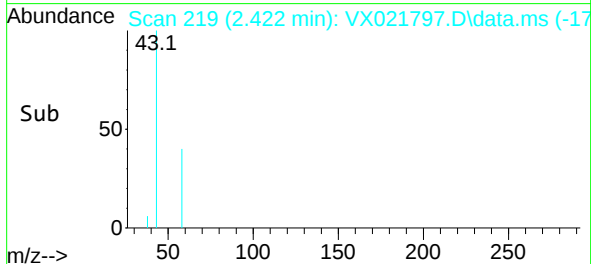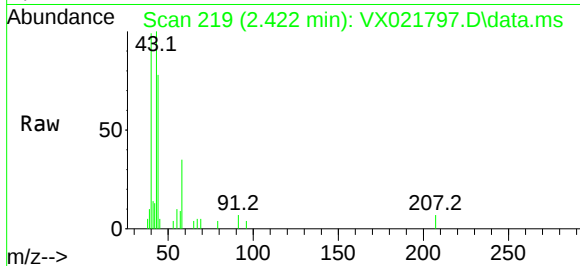

#19
Methyl tert-butyl Ether
Concen: 0.59 ug/l
RT: 3.166 min Scan# 341
Delta R.T. 0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 73 Resp: 3064
Ion Ratio Lower Upper
73 100
57 41.9 17.1 25.7#




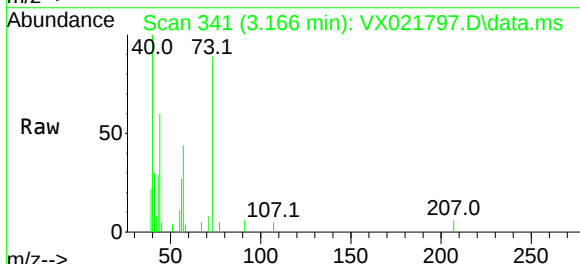


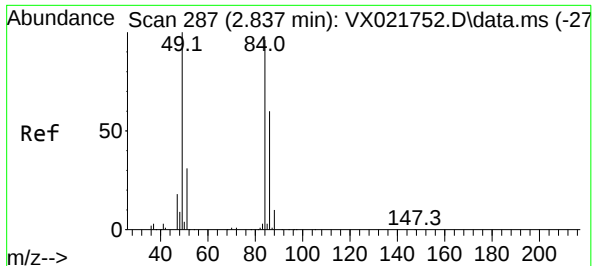

#20
Methylene Chloride
Concen: 0.62 ug/l
RT: 2.837 min Scan# 287
Delta R.T. -0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion:	84	Resp:	1168
Ion	Ratio	Lower	Upper
84	100		
49	123.1	88.6	132.8
51	38.2	27.0	40.6
86	79.3	50.3	75.5#

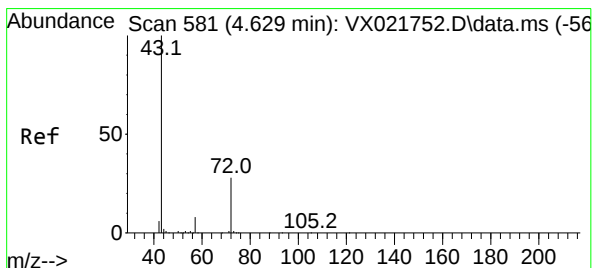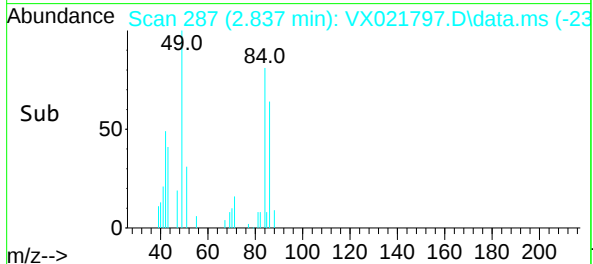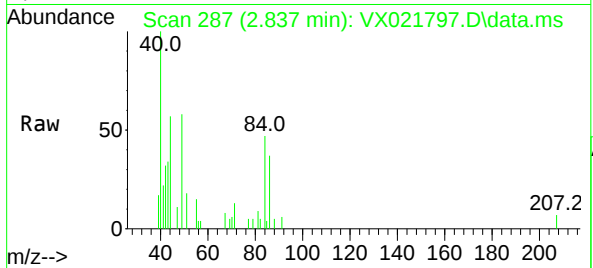

#25
2-Butanone
Concen: 0.72 ug/l
RT: 4.635 min Scan# 582
Delta R.T. 0.006 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion:	43	Resp:	773
Ion	Ratio	Lower	Upper
43	100		
72	0.0	23.7	35.5#


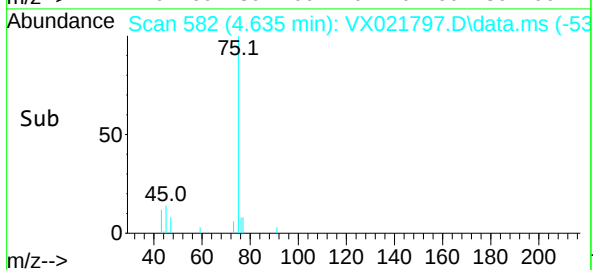

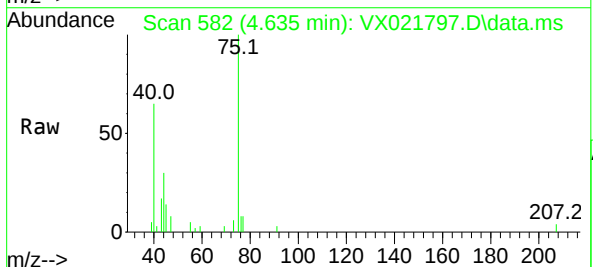


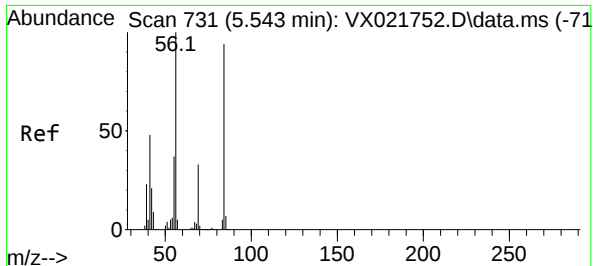

#31
Cyclohexane
Concen: 1.28 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.001 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion: 56 Resp: 3302
Ion Ratio Lower Upper
56 100
69 26.6 25.3 37.9
84 85.1 71.4 107.0

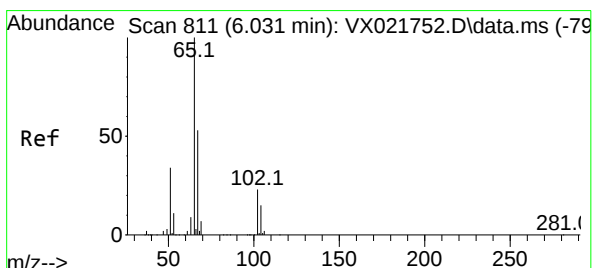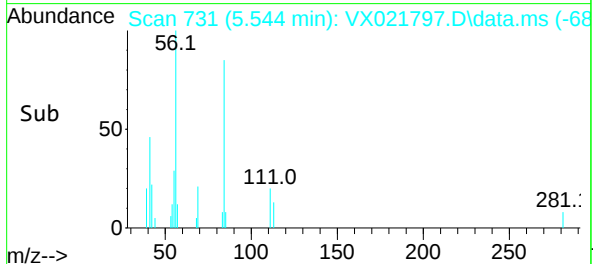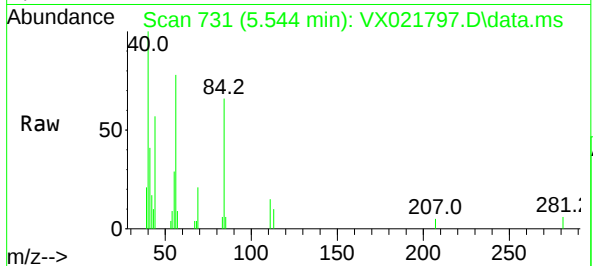

#33
1,2-Dichloroethane-d4
Concen: 51.62 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 65 Resp: 94913
Ion Ratio Lower Upper
65 100
67 54.6 0.0 105.4


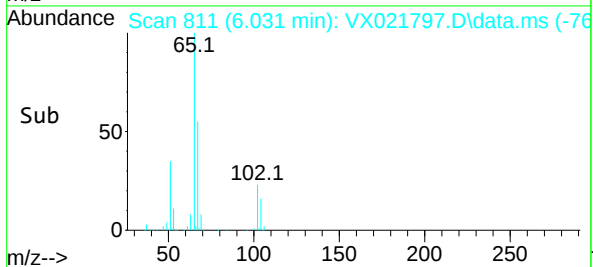

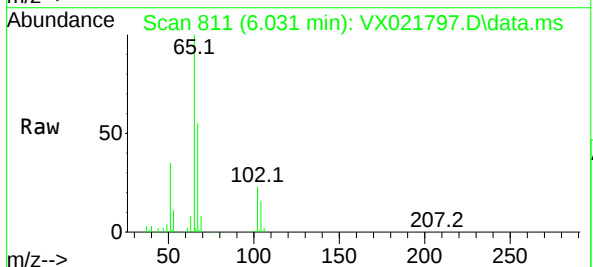




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. 0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion:114 Resp: 283352
Ion Ratio Lower Upper
114 100
63 19.2 0.0 40.8
88 15.4 0.0 32.8

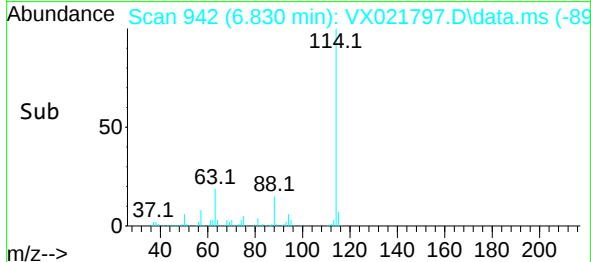

#35
Dibromofluoromethane
Concen: 49.23 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57


Tgt Ion:113 Resp: 89205
Ion Ratio Lower Upper
113 100
111 102.1 81.9 122.9
192 19.5 16.7 25.1

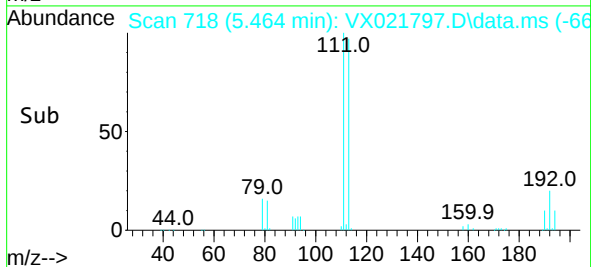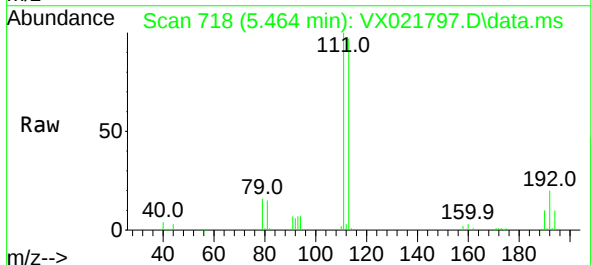






#36
1,1-Dichloropropene
Concen: 4.57 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.146 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57


Instrument :
MSVOA_X
ClientSampled :
MW-12DL

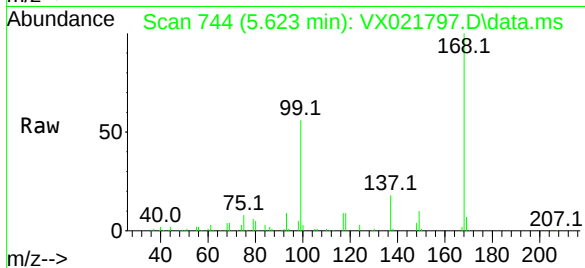



Tgt Ion: 75 Resp: 11442
Ion Ratio Lower Upper
75 100
110 8.9 18.1 54.4#
77 0.0 25.3 37.9#

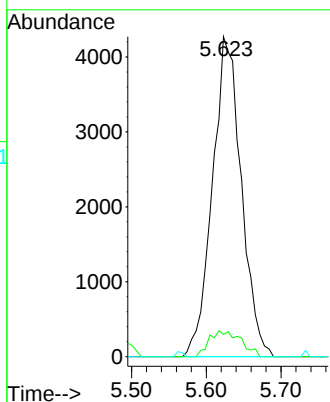


#38
Carbon Tetrachloride
Concen: 5.64 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.122 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

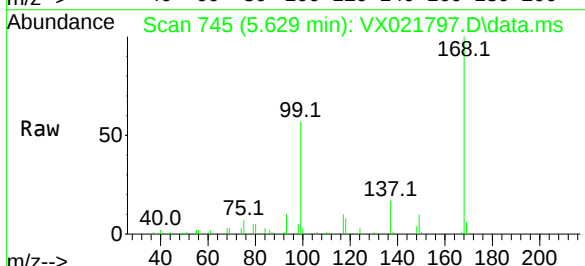

Tgt Ion: 117 Resp: 15455
Ion Ratio Lower Upper
117 100
119 4.7 76.2 114.2#
121 0.0 24.8 37.2#

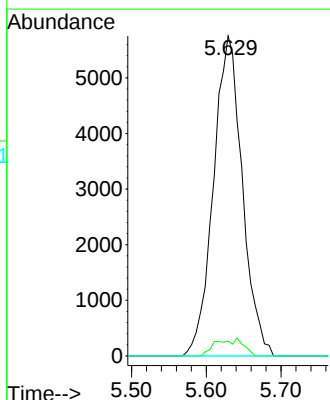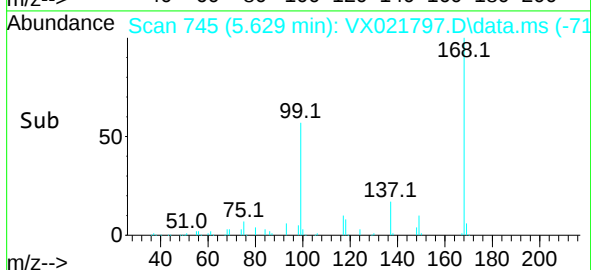



#39

Methylcyclohexane

Concen: 0.49 ug/l

RT: 7.440 min Scan# 1042





Delta R.T. 0.001 min

Lab File: VX021797.D

Acq: 21 Apr 2021 16:57

Tgt Ion:	83	Resp:	1594
Ion	Ratio	Lower	Upper
83	100		
55	70.6	58.9	88.3
98	36.2	38.1	57.1#

Instrument :
MSVOA_X
ClientSampleId :
MW-12DL

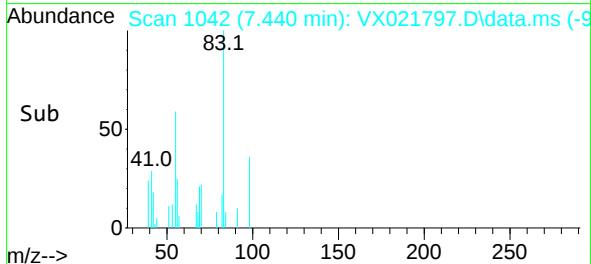

#40

Benzene

Concen: 23.81 ug/l




RT: 6.111 min Scan# 824


Delta R.T. 0.001 min

Lab File: VX021797.D

Acq: 21 Apr 2021 16:57

Tgt Ion:	78	Resp:	177665
Ion	Ratio	Lower	Upper
78	100		
77	22.5	18.9	28.3

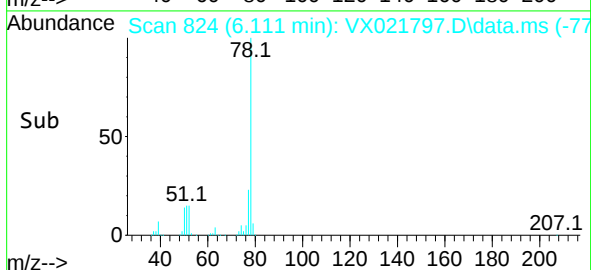



#42

1,2-Dichloroethane

Concen: 2.06 ug/l

RT: 6.159 min Scan# 832

Delta R.T. 0.000 min

Lab File: VX021797.D





Acq: 21 Apr 2021 16:57

Tgt Ion: 62 Resp: 4984

Ion Ratio Lower Upper

62 100

98 8.4 0.0 20.2



#50

Toluene-d8

Concen: 49.09 ug/l

RT: 8.696 min Scan# 1248

Delta R.T. 0.001 min

Lab File: VX021797.D




Acq: 21 Apr 2021 16:57


Tgt Ion: 98 Resp: 342056

Ion Ratio Lower Upper

98 100

100 65.2 51.9 77.9


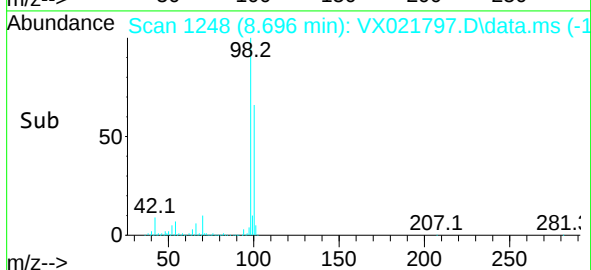






#51
4-Methyl-2-Pentanone
Concen: 0.25 ug/l
RT: 8.610 min Scan# 1234
Delta R.T. -0.006 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion: 43 Resp: 584
Ion Ratio Lower Upper
43 100
58 40.4 35.4 53.0

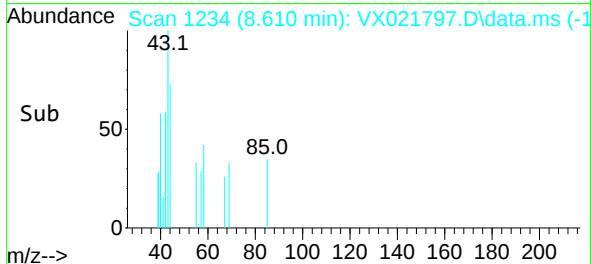

#52
Toluene
Concen: 4.46 ug/l
RT: 8.763 min Scan# 1259
Delta R.T. 0.001 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 92 Resp: 21575
Ion Ratio Lower Upper
92 100
91 173.3 137.1 205.7


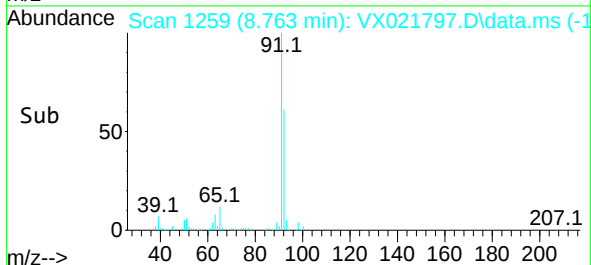

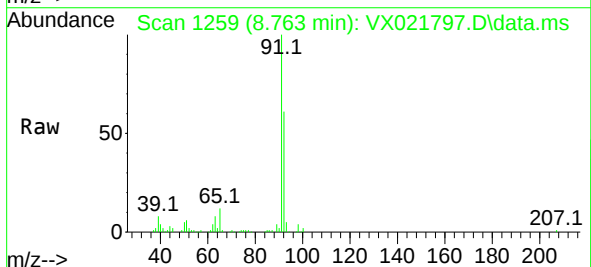




#58
2-Chloroethyl Vinyl ether
Concen: 0.69 ug/l
RT: 8.226 min Scan# 1171
Delta R.T. -0.061 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampled :
MW-12DL


Tgt Ion: 63 Resp: 1011
Ion Ratio Lower Upper
63 100
106 0.0 23.5 35.3#

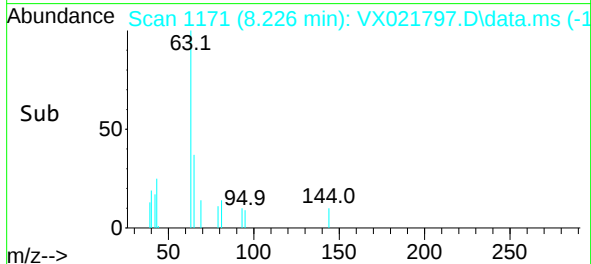

#62
4-Bromofluorobenzene
Concen: 47.93 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 95 Resp: 124722
Ion Ratio Lower Upper
95 100
174 79.1 0.0 154.6
176 76.6 0.0 155.8


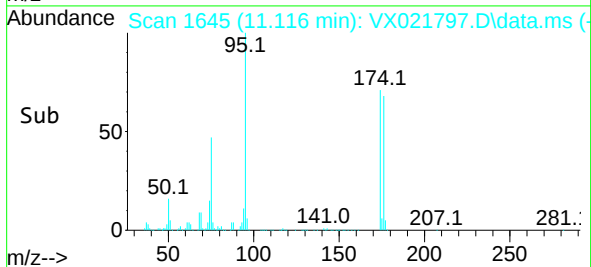

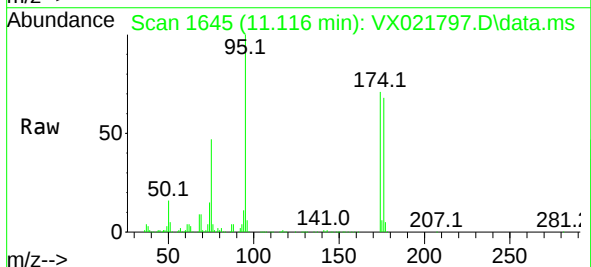




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.098 min Scan# 1478
Delta R.T. 0.007 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion:117 Resp: 259943
Ion Ratio Lower Upper
117 100
82 50.9 47.4 71.2
119 32.4 26.6 39.8

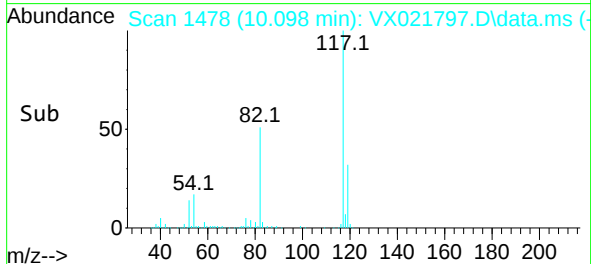

#67
Ethyl Benzene
Concen: 13.59 ug/l
RT: 10.232 min Scan# 1500
Delta R.T. -0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 91 Resp: 126249
Ion Ratio Lower Upper
91 100
106 31.9 24.6 37.0


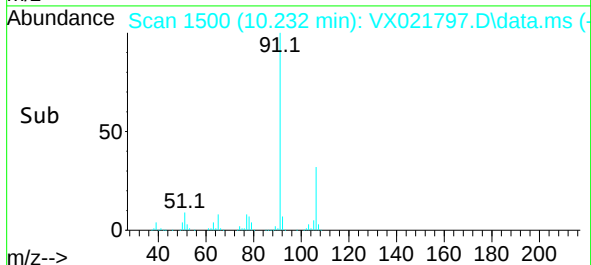

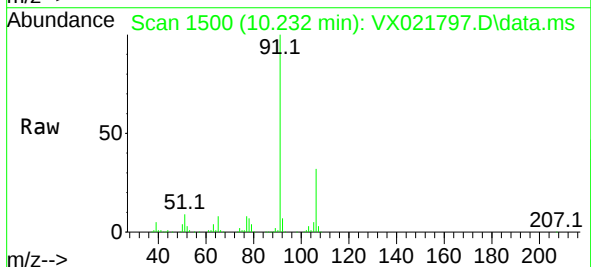




#68
m/p-Xylenes
Concen: 10.49 ug/l
RT: 10.342 min Scan# 1518
Delta R.T. 0.001 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion:106 Resp: 37713
Ion Ratio Lower Upper
106 100
91 204.7 162.8 244.2

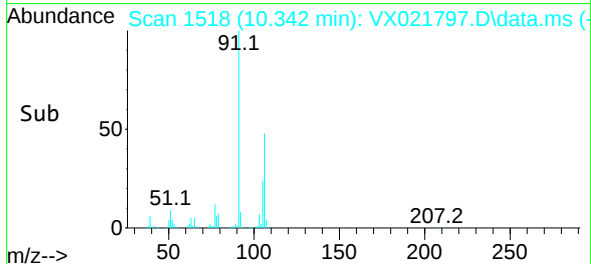

#69
o-Xylene
Concen: 5.29 ug/l
RT: 10.683 min Scan# 1574
Delta R.T. 0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion:106 Resp: 18334
Ion Ratio Lower Upper
106 100
91 218.7 108.1 324.2

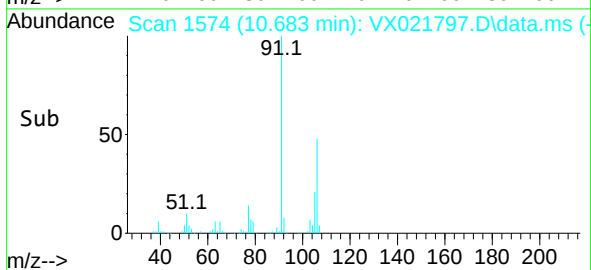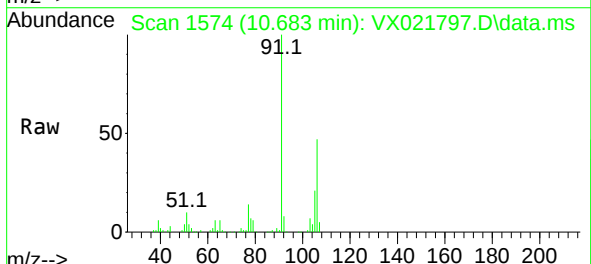



#70

Styrene

Concen: 0.29 ug/l

RT: 10.683 min Scan# 1574

Delta R.T. -0.012 min

Lab File: VX021797.D

Acq: 21 Apr 2021 16:57

Tgt Ion:104 Resp: 1718

Ion Ratio Lower Upper

104 100

78 169.4 40.0 60.0#





103 162.0 43.4 65.0#

Instrument :

MSVOA_X

ClientSampled :

MW-12DL

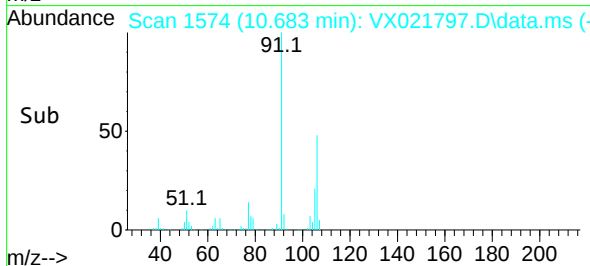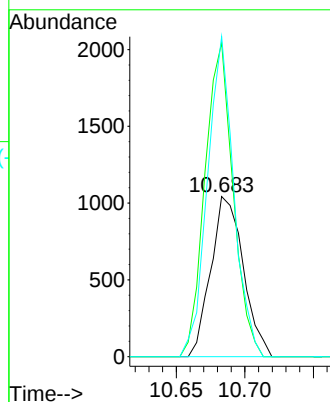

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.061 min Scan# 1800

Delta R.T. -0.000 min

Lab File: VX021797.D

Acq: 21 Apr 2021 16:57




Tgt Ion:152 Resp: 124522


Ion Ratio Lower Upper

152 100

115 58.5 41.1 123.3

150 155.5 0.0 349.0

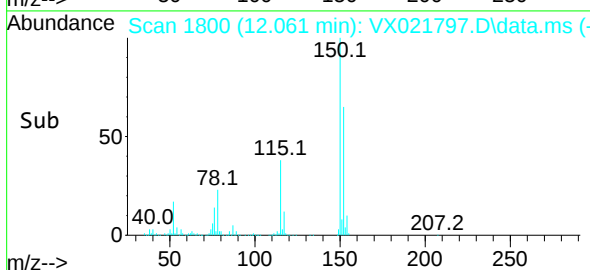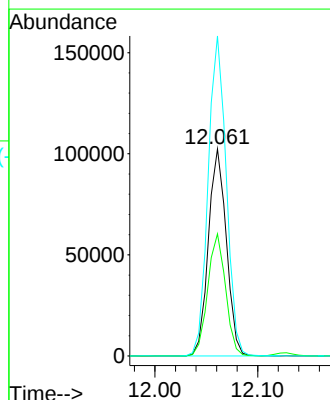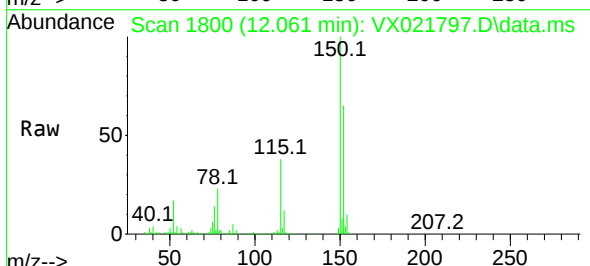



#73

Isopropylbenzene

Concen: 1.19 ug/l

RT: 11.000 min Scan# 1626

Delta R.T. 0.000 min

Lab File: VX021797.D





Acq: 21 Apr 2021 16:57

Tgt Ion:105 Resp: 10405

Ion Ratio Lower Upper

105 100

120 25.9 13.2 39.6

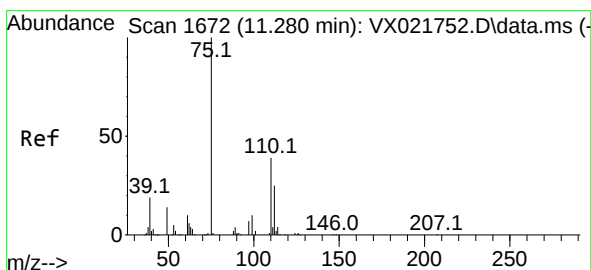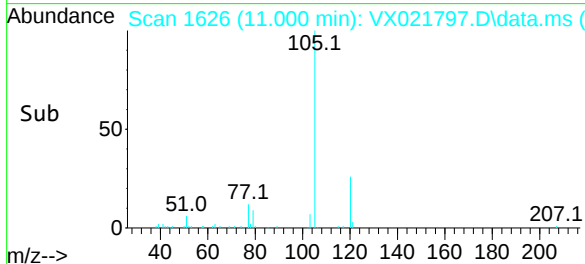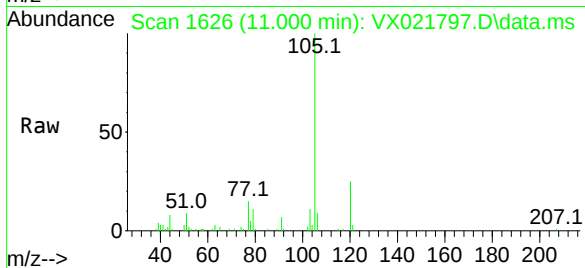

#76

1,2,3-Trichloropropane

Concen: 22.98 ug/l

RT: 11.116 min Scan# 1645

Delta R.T. -0.164 min

Lab File: VX021797.D




Acq: 21 Apr 2021 16:57


Tgt Ion: 75 Resp: 56740

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

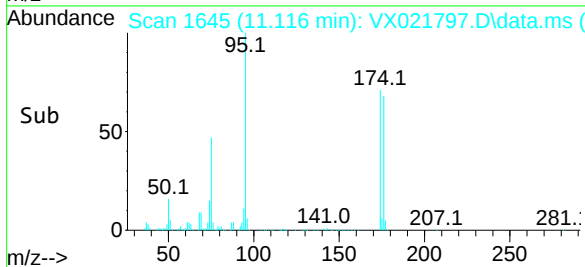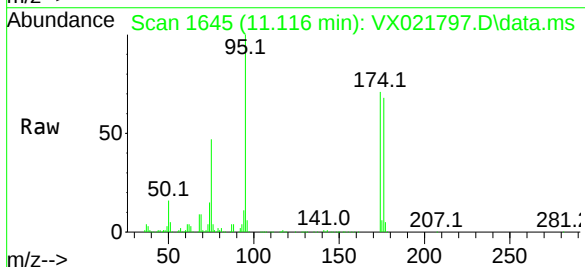



#78

n-propylbenzene

Concen: 1.52 ug/l

RT: 11.341 min Scan# 1682

Delta R.T. 0.000 min

Lab File: VX021797.D





Acq: 21 Apr 2021 16:57

Tgt Ion: 91 Resp: 14704

Ion Ratio Lower Upper

91 100

120 21.9 11.5 34.5

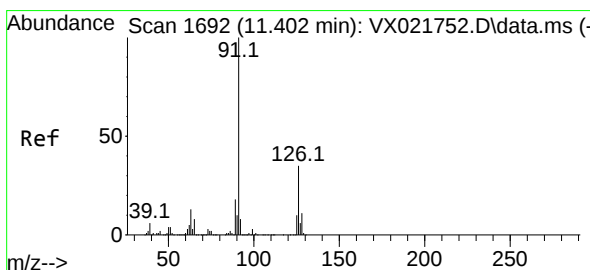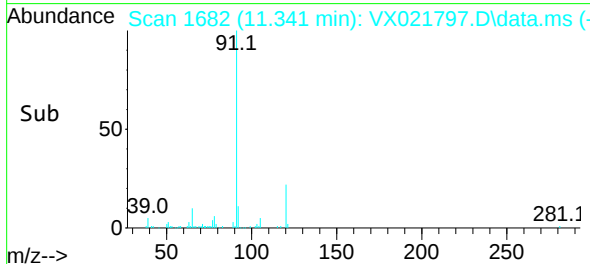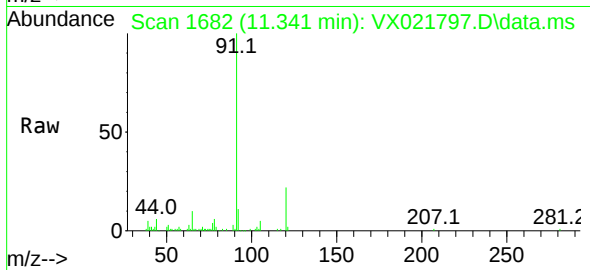

#79

2-Chlorotoluene

Concen: 0.52 ug/l

RT: 11.439 min Scan# 1698

Delta R.T. 0.037 min

Lab File: VX021797.D




Acq: 21 Apr 2021 16:57


Tgt Ion: 91 Resp: 2952

Ion Ratio Lower Upper

91 100

126 0.0 16.6 49.8#


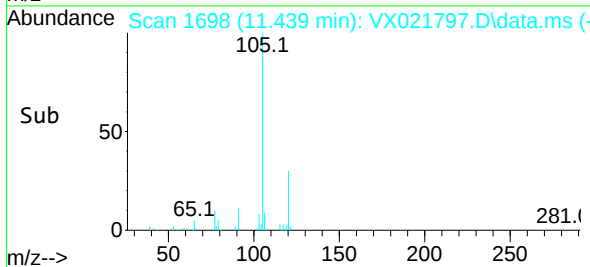

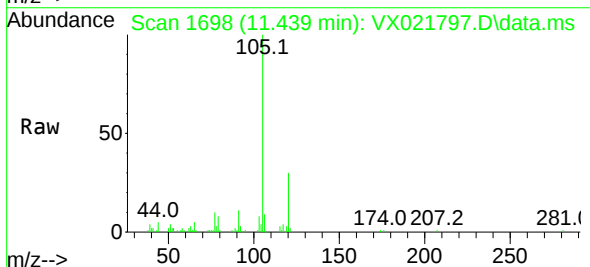


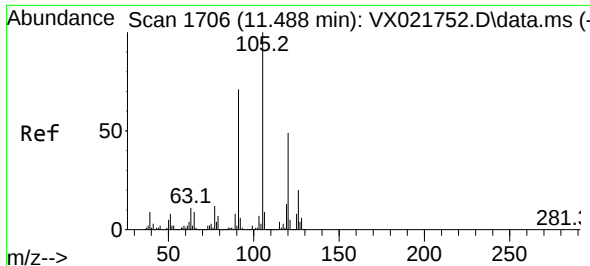

#80
1,3,5-Trimethylbenzene
Concen: 3.84 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.000 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampled :
MW-12DL


Tgt Ion:105 Resp: 28424
Ion Ratio Lower Upper
105 100
120 49.8 23.8 71.5

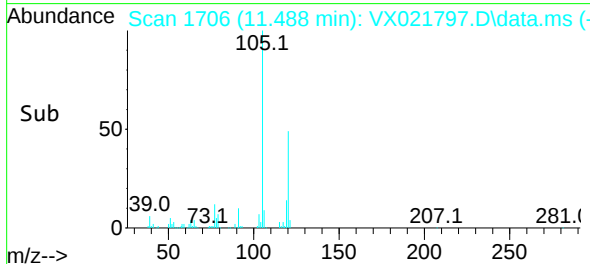

#81
trans-1,4-Dichloro-2-butene
Concen: 52.84 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. 0.061 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 75 Resp: 56740
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


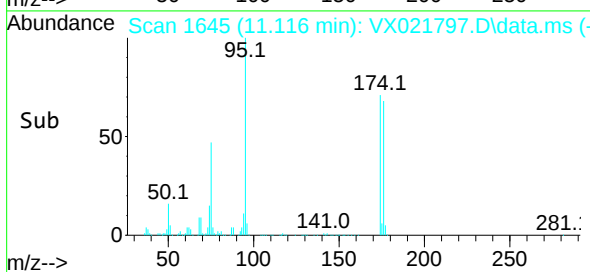

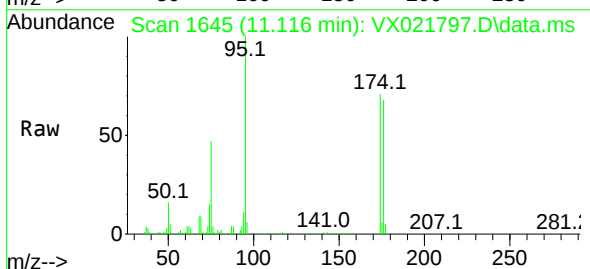


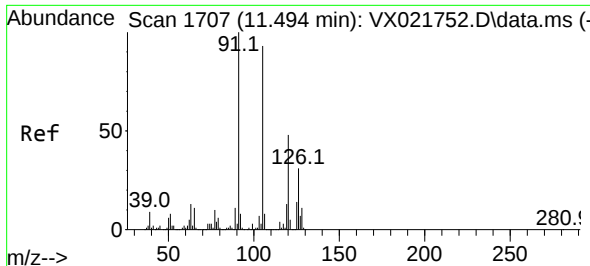

#82
4-Chlorotoluene
Concen: 0.50 ug/l
RT: 11.488 min Scan# 1706
Delta R.T. -0.006 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57




Instrument :
MSVOA_X
ClientSampleId :
MW-12DL


Tgt Ion: 91 Resp: 3287
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

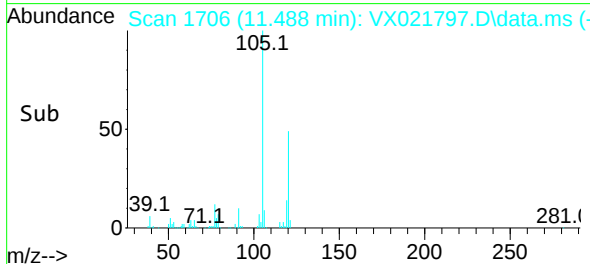

#84
1,2,4-Trimethylbenzene
Concen: 10.59 ug/l
RT: 11.787 min Scan# 1755
Delta R.T. 0.001 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion: 105 Resp: 79136
Ion Ratio Lower Upper
105 100
120 46.2 22.4 67.3

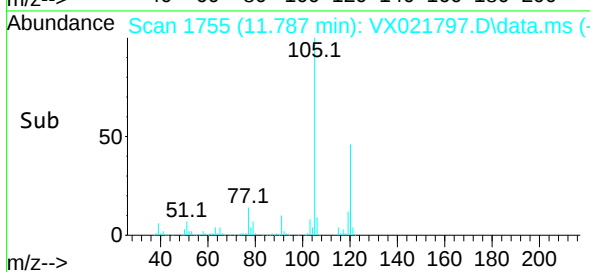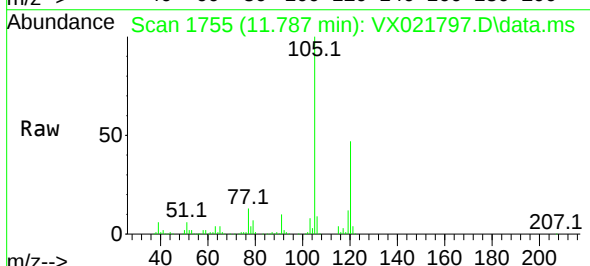



#85

sec-Butylbenzene

Concen: 9.34 ug/l

RT: 11.787 min Scan# 1755

Delta R.T. -0.140 min

Lab File: VX021797.D





Acq: 21 Apr 2021 16:57

Tgt Ion:105 Resp: 79136

Ion Ratio Lower Upper

105 100

134 0.0 10.0 29.8#

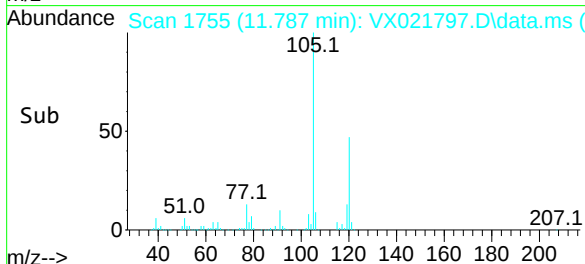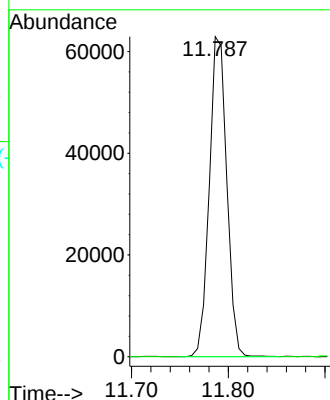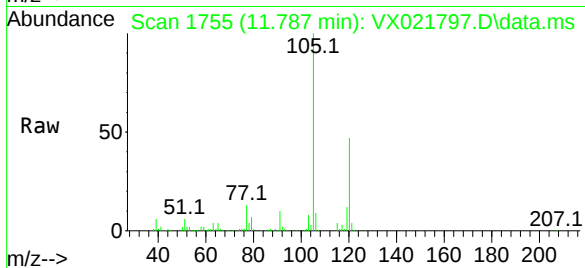

#89

n-Butylbenzene

Concen: 0.41 ug/l

RT: 12.360 min Scan# 1849

Delta R.T. -0.012 min

Lab File: VX021797.D

Acq: 21 Apr 2021 16:57




Tgt Ion: 91 Resp: 2794


Ion Ratio Lower Upper

91 100

92 27.1 27.4 82.0#

134 117.6 13.2 39.5#


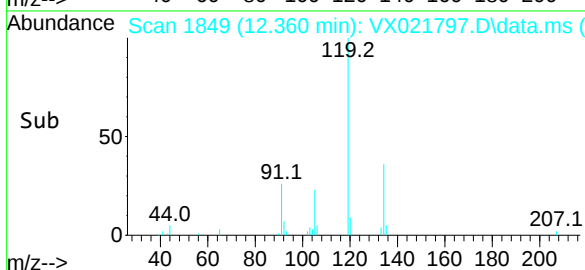
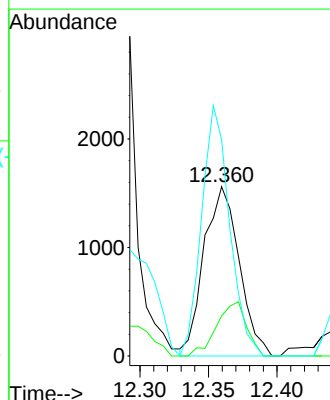
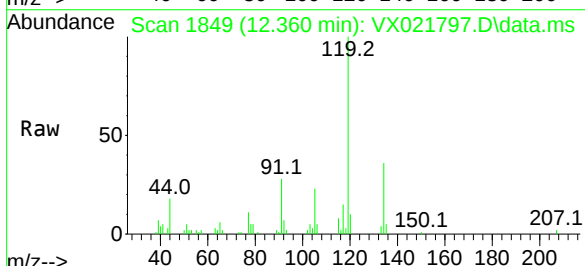




#90
Hexachloroethane
Concen: 1.70 ug/l
RT: 12.683 min Scan# 1902
Delta R.T. 0.104 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Instrument :
MSVOA_X
ClientSampled :
MW-12DL

Tgt Ion:117 Resp: 2489
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#



#95
Naphthalene
Concen: 2.64 ug/l
RT: 13.817 min Scan# 2088
Delta R.T. 0.001 min
Lab File: VX021797.D
Acq: 21 Apr 2021 16:57

Tgt Ion:128 Resp: 22164
Ion Ratio Lower Upper
128 100
127 13.2 10.3 15.5
129 11.2 8.8 13.2

