

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
 Data File : VX028266.D
 Acq On : 22 Apr 2022 01:40
 Operator : JC/MD
 Sample : N2452-05ME
 Misc : 5.96g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-3ME

Quant Time: Apr 22 06:30:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	557857	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	861831	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	766461	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	410983	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	278121	38.236	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	76.480%
35) Dibromofluoromethane	5.391	113	262383	43.412	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	86.820%
50) Toluene-d8	8.653	98	966889	41.652	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	83.300%
62) 4-Bromofluorobenzene	11.085	95	362962	40.893	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	81.780%

Target Compounds				Qvalue		
3) Chloromethane	1.288	50	628	Below Cal	#	85
5) Bromomethane	1.605	94	2138	Below Cal		84
6) Chloroethane	1.770	64	309	Below Cal	#	48
8) Diethyl Ether	2.050	74	105	Below Cal		55
10) Methyl Iodide	2.441	142	2577	5.608	ug/l	91
11) Tert butyl alcohol	2.947	59	21046	5.388	ug/l	# 75
13) Acrolein	2.252	56	317	0.356	ug/l	100
16) Acetone	2.422	43	9950	3.100	ug/l	# 83
17) Carbon Disulfide	2.489	76	2562	0.222	ug/l	100
18) Methyl Acetate	2.721	43	18765	2.902	ug/l	99
20) Methylene Chloride	2.782	84	3860	0.715	ug/l	97
31) Cyclohexane	5.471	56	16485	1.860	ug/l	98
36) 1,1-Dichloropropene	5.550	75	35818	4.543	ug/l	# 50
38) Carbon Tetrachloride	5.556	117	51222	5.755	ug/l	# 15
39) Methylcyclohexane	7.379	83	108138	10.871	ug/l	96
40) Benzene	6.044	78	4741	0.205	ug/l	99
51) 4-Methyl-2-Pentanone	8.598	43	7728	0.925	ug/l	# 41
52) Toluene	8.720	92	11912	0.743	ug/l	96
55) 1,1,2-Trichloroethane	9.104	97	41743	6.408	ug/l	# 20
56) Ethyl methacrylate	9.104	69	8541	0.904	ug/l	# 1
59) 2-Hexanone	9.385	43	44615	6.894	ug/l	# 23
67) Ethyl Benzene	10.201	91	37645	1.374	ug/l	94
68) m/p-Xylenes	10.305	106	85900	7.702	ug/l	95
69) o-Xylene	10.647	106	87584	7.877	ug/l	96
70) Styrene	10.647	104	5082	0.282	ug/l	# 1
71) Bromoform	10.823	173	74	3.588	ug/l	# 29
73) Isopropylbenzene	10.964	105	145241	5.142	ug/l	98
74) N-amyl acetate	10.854	43	66344	6.795	ug/l	# 1
75) 1,1,2,2-Tetrachloroethane	11.220	83	65608	7.157	ug/l	# 32
76) 1,2,3-Trichloropropane	11.085	75	166880	20.632	ug/l	# 36
78) n-propylbenzene	11.305	91	273049	8.717	ug/l	97
79) 2-Chlorotoluene	11.384	91	59601	3.061	ug/l	# 47
80) 1,3,5-Trimethylbenzene	11.457	105	605644	25.258	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.085	75	166880	61.313	ug/l	# 16
82) 4-Chlorotoluene	11.457	91	64836	2.890	ug/l	# 48
83) tert-Butylbenzene	11.713	119	26170	1.069	ug/l	89

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
 Data File : VX028266.D
 Acq On : 22 Apr 2022 01:40
 Operator : JC/MD
 Sample : N2452-05ME
 Misc : 5.96g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-3ME

Quant Time: Apr 22 06:30:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


84) 1,2,4-Trimethylbenzene	11.756	105	1487976	62.426	ug/l	95
85) sec-Butylbenzene	11.890	105	223052	7.551	ug/l	97
86) p-Isopropyltoluene	12.012	119	179883	7.059	ug/l	97
89) n-Butylbenzene	12.335	91	283483	13.547	ug/l #	39
90) Hexachloroethane	12.536	117	34900	9.149	ug/l #	10
91) 1,2-Dichlorobenzene	12.341	146	8713	0.634	ug/l #	76
92) 1,2-Dibromo-3-Chloropr...	12.927	75	4679	2.295	ug/l #	10
95) Naphthalene	13.780	128	555498	20.416	ug/l #	91
96) 1,2,3-Trichlorobenzene	13.975	180	9121	1.138	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028266.D
Acq On : 22 Apr 2022 01:40
Operator : JC/MD
Sample : N2452-05ME
Misc : 5.96g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME

Quant Time: Apr 22 06:30:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




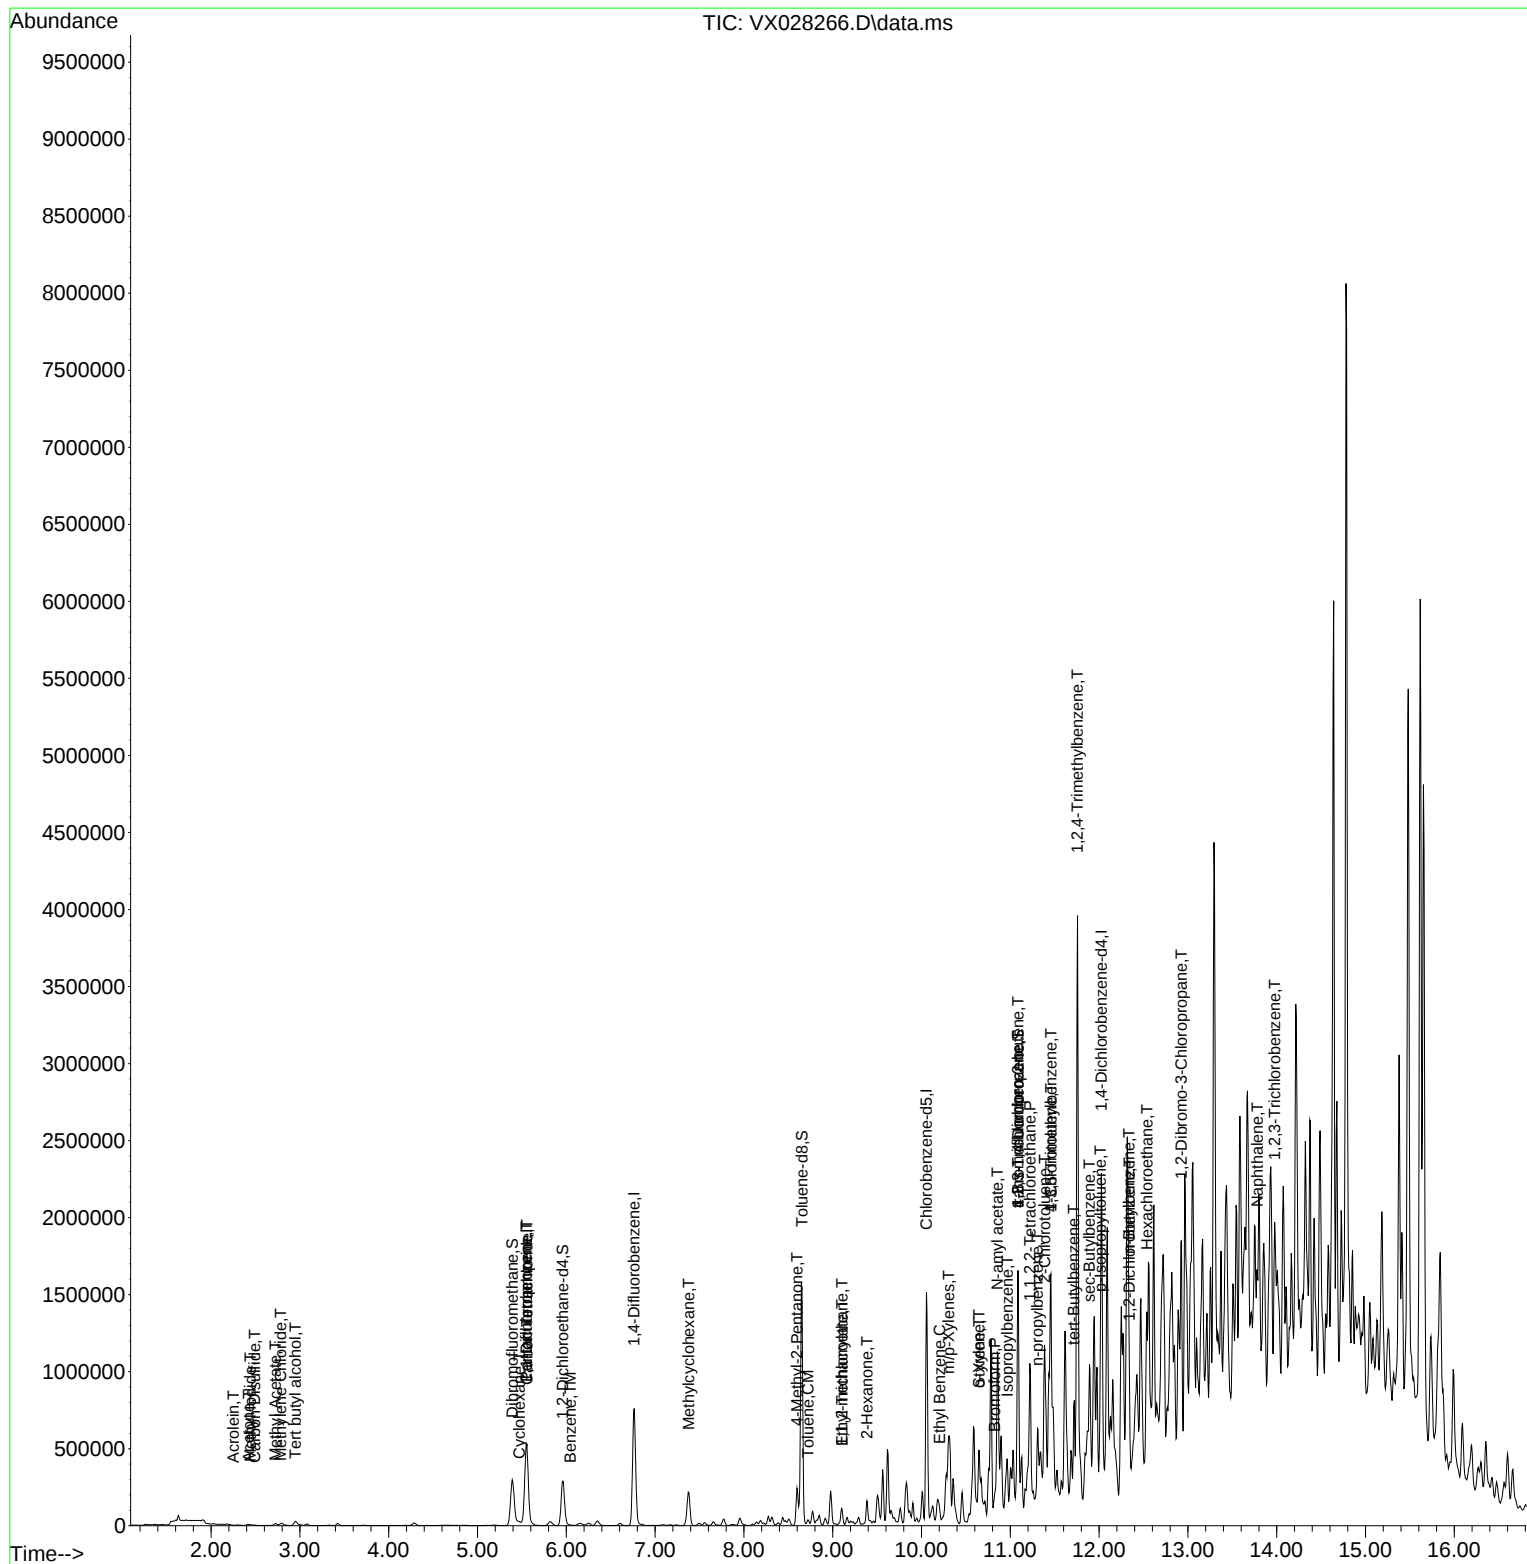




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME

Tgt Ion:168 Resp: 557857
Ion Ratio Lower Upper
168 100
99 50.1 41.7 62.5

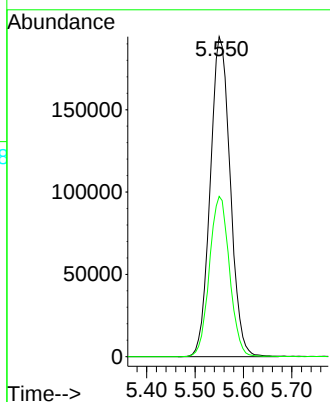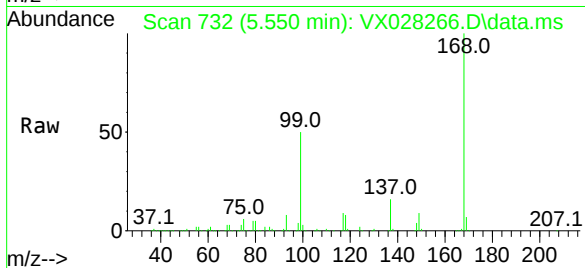

#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. -0.006 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 50 Resp: 628
Ion Ratio Lower Upper
50 100
52 41.6 26.4 39.6#


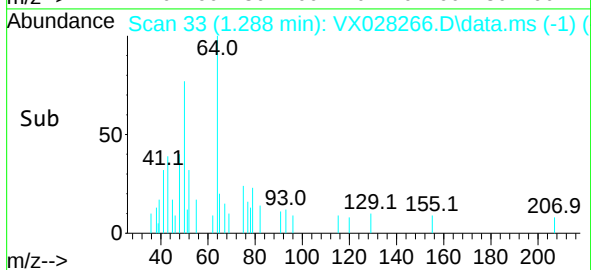
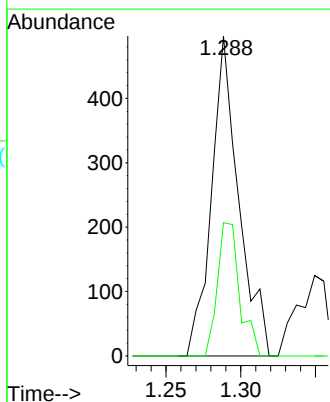
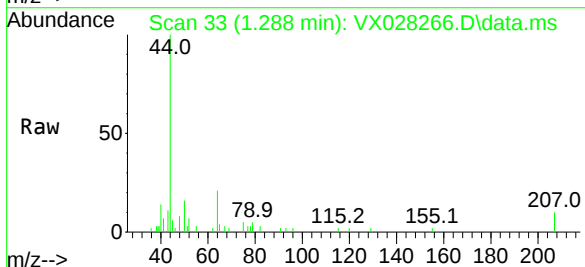




#5
Bromomethane
Concen: Below Cal
RT: 1.605 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 94 Resp: 2138
Ion Ratio Lower Upper
94 100
96 109.9 75.3 112.9

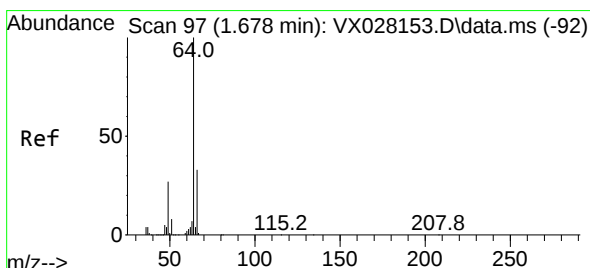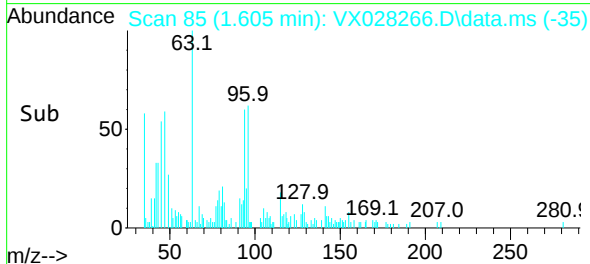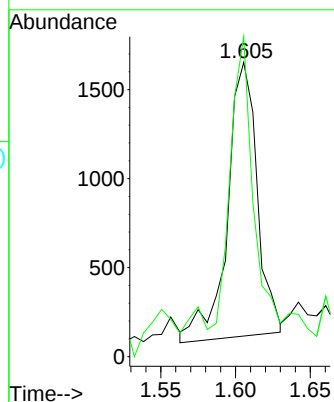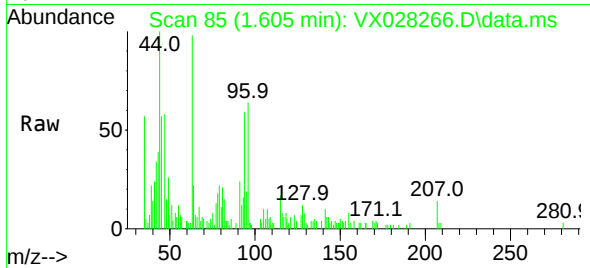

#6
Chloroethane
Concen: Below Cal
RT: 1.770 min Scan# 112
Delta R.T. 0.092 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 64 Resp: 309
Ion Ratio Lower Upper
64 100
66 2.6 25.3 37.9


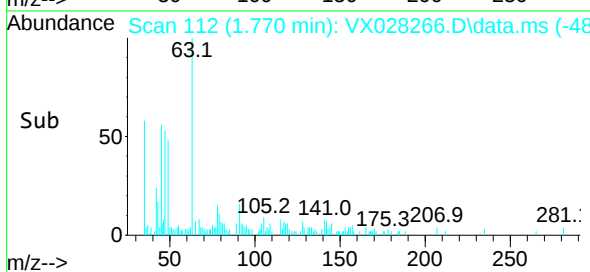
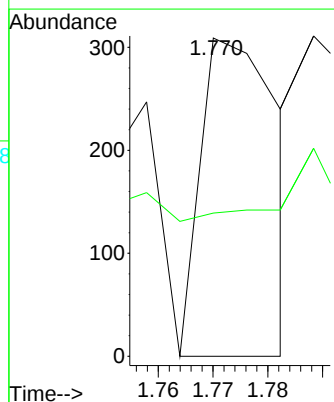
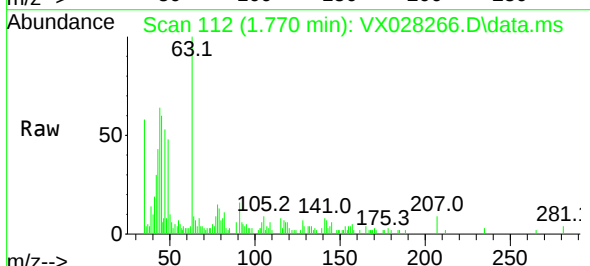




#8
Diethyl Ether
Concen: Below Cal
RT: 2.050 min Scan# 11
Delta R.T. -0.080 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 74 Resp: 105
Ion Ratio Lower Upper
74 100
45 124.8 42.0 126.0

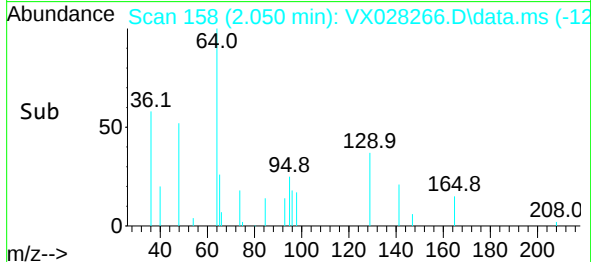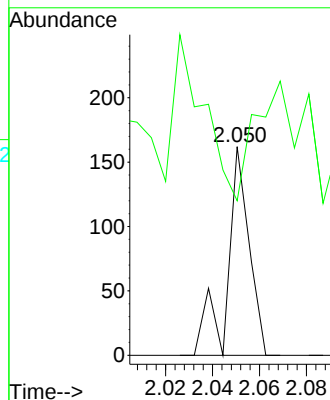

#10
Methyl Iodide
Concen: 5.608 ug/l
RT: 2.441 min Scan# 222
Delta R.T. -0.012 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 142 Resp: 2577
Ion Ratio Lower Upper
142 100
127 49.2 33.9 50.9
141 13.4 11.4 17.2

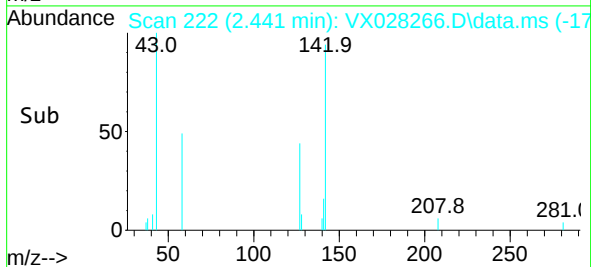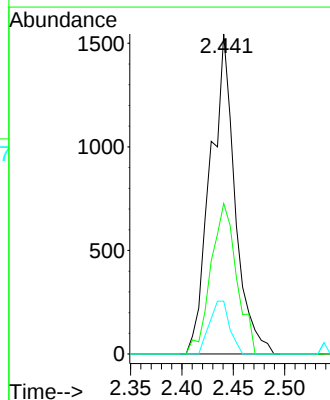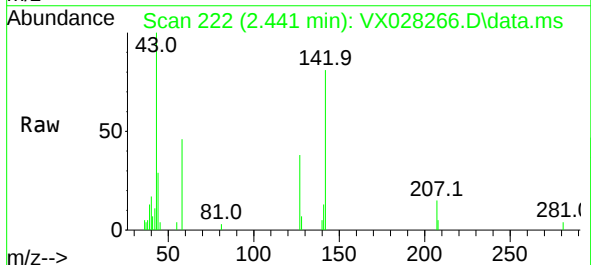

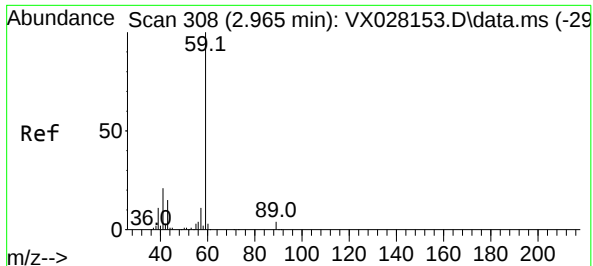

#11

Tert butyl alcohol

Concen: 5.388 ug/l

RT: 2.947 min Scan# 308

Delta R.T. -0.018 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40

Instrument :

MSVOA_X

ClientSampleId :





WC-15-1-3ME

Tgt Ion: 59 Resp: 21046

Ion Ratio Lower Upper

59 100

57 1.1 8.3 12.5#

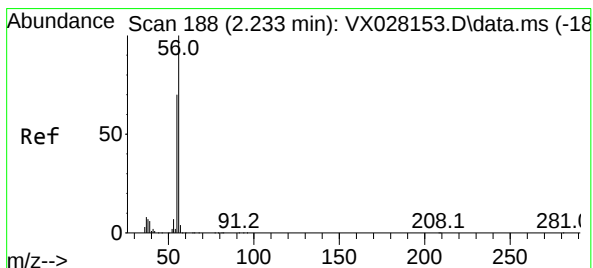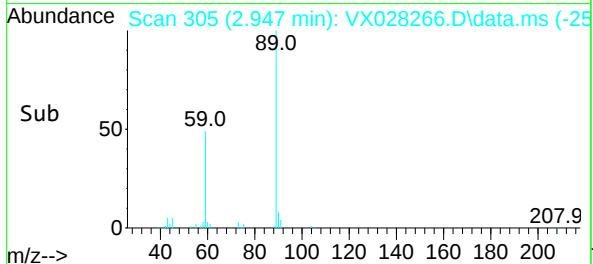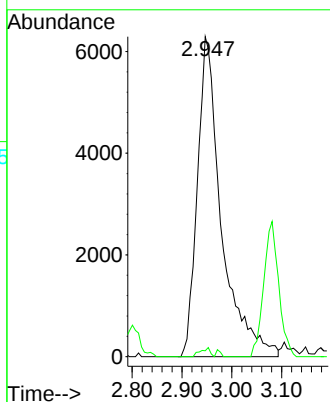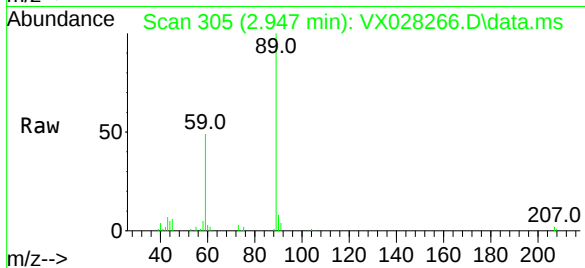

#13

Acrolein

Concen: 0.356 ug/l

RT: 2.252 min Scan# 191

Delta R.T. 0.019 min

Lab File: VX028266.D




Acq: 22 Apr 2022 01:40


Tgt Ion: 56 Resp: 317

Ion Ratio Lower Upper

56 100

55 69.1 55.0 82.6


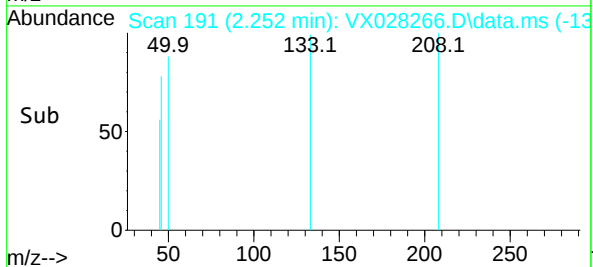
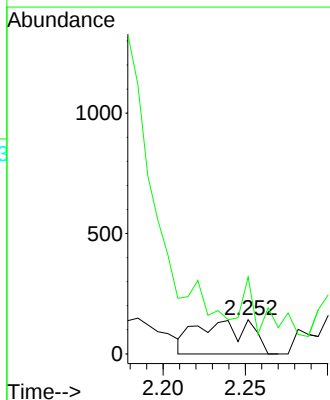
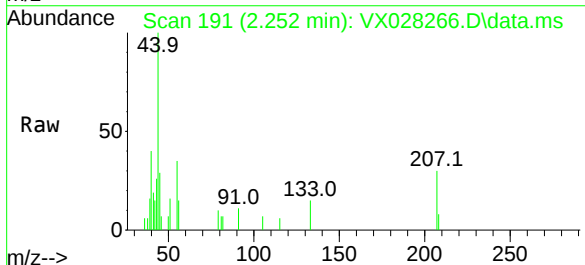


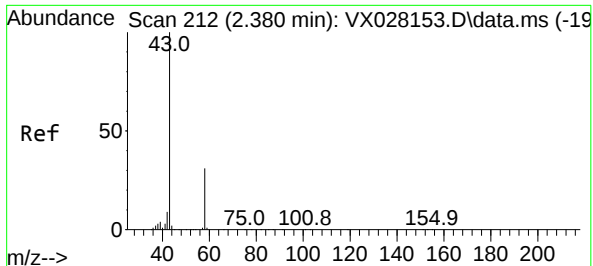

#16
Acetone
Concen: 3.100 ug/l
RT: 2.422 min Scan# 21
Delta R.T. 0.042 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 43 Resp: 9950
Ion Ratio Lower Upper
43 100
58 26.1 28.8 43.2#

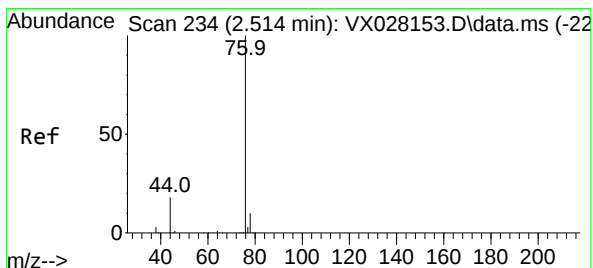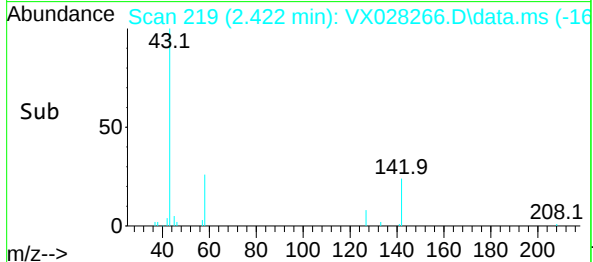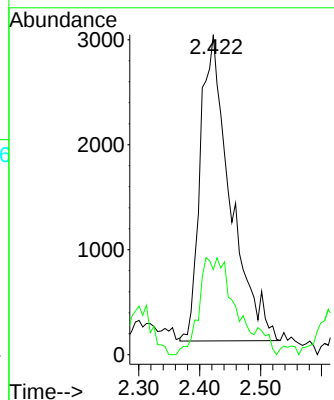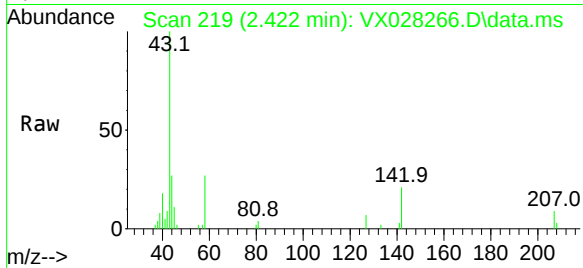

#17
Carbon Disulfide
Concen: 0.222 ug/l
RT: 2.489 min Scan# 230
Delta R.T. -0.025 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 76 Resp: 2562
Ion Ratio Lower Upper
76 100
78 8.9 7.2 10.8


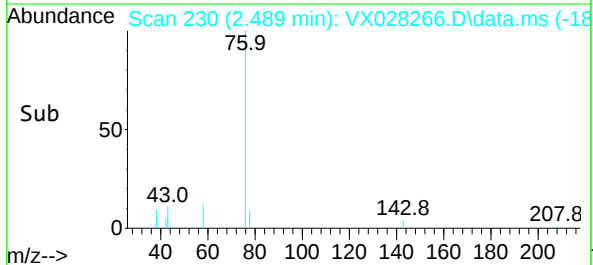
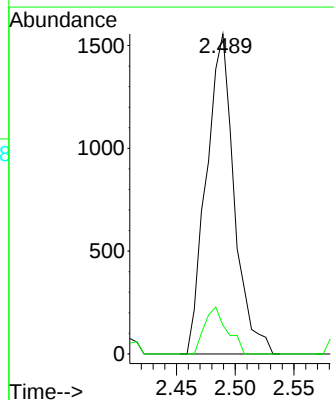
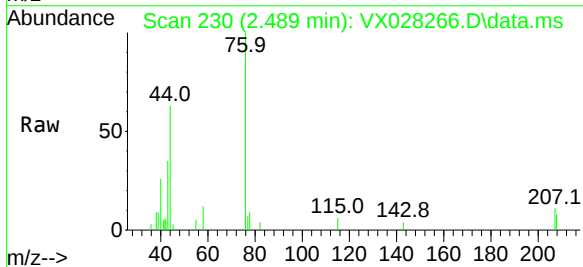




#18
Methyl Acetate
Concen: 2.902 ug/l
RT: 2.721 min Scan# 207
Delta R.T. 0.018 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 43 Resp: 18765
Ion Ratio Lower Upper
43 100
74 29.0 22.8 34.2

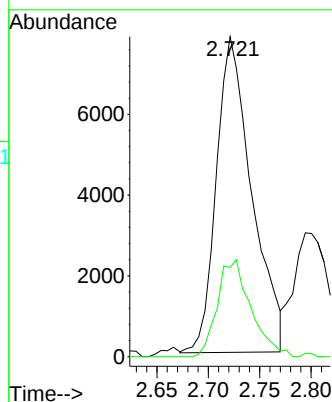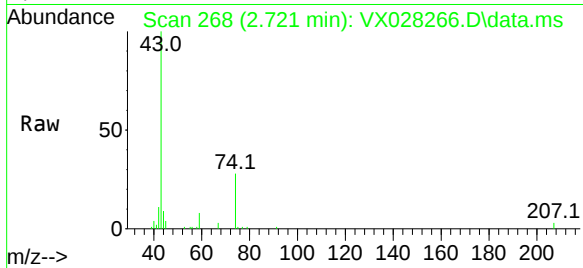

#20
Methylene Chloride
Concen: 0.715 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.006 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40


Tgt Ion: 84 Resp: 3860
Ion Ratio Lower Upper
84 100
49 109.4 85.5 128.3
51 35.4 26.6 39.8
86 67.4 51.5 77.3

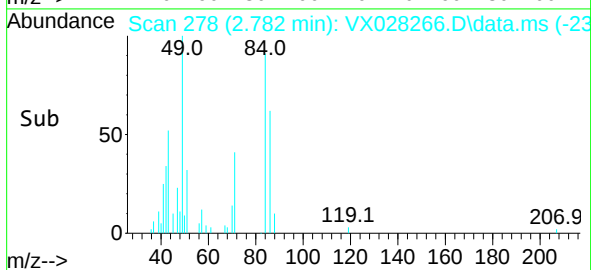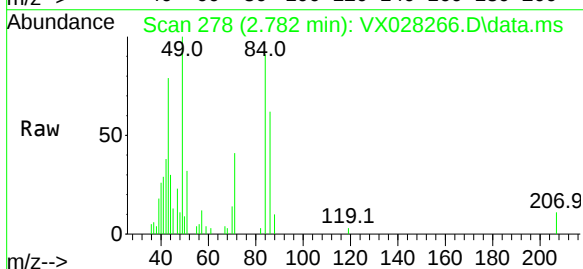






#31
Cyclohexane
Concen: 1.860 ug/l
RT: 5.471 min Scan# 719
Delta R.T. 0.001 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME



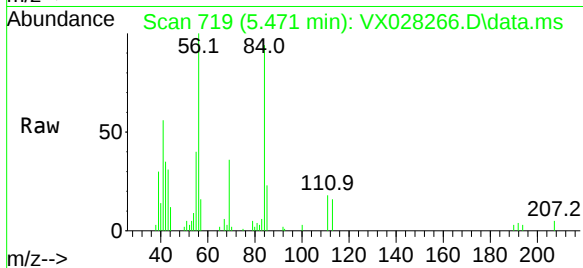



Tgt Ion: 56 Resp: 16485
Ion Ratio Lower Upper
56 100
69 34.0 26.7 40.1
84 94.3 77.2 115.8

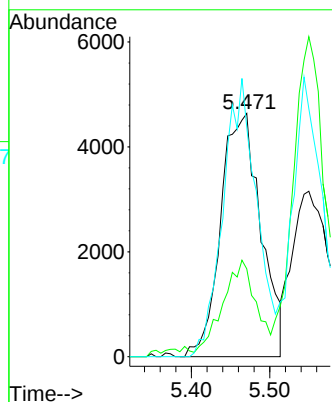

#33
1,2-Dichloroethane-d4
Concen: 38.236 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 65 Resp: 278121
Ion Ratio Lower Upper
65 100
67 52.6 0.0 107.4




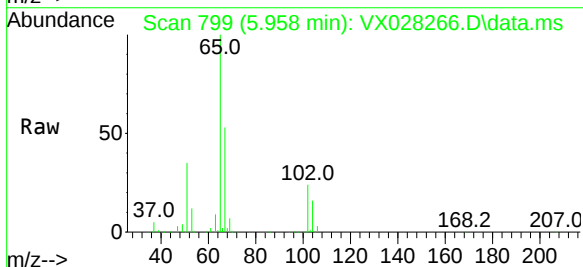




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: VX028266.D
 Acq: 22 Apr 2022 01:40




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-3ME


Tgt Ion:114 Resp: 861831
 Ion Ratio Lower Upper
 114 100
 63 16.9 0.0 36.8
 88 14.8 0.0 32.4

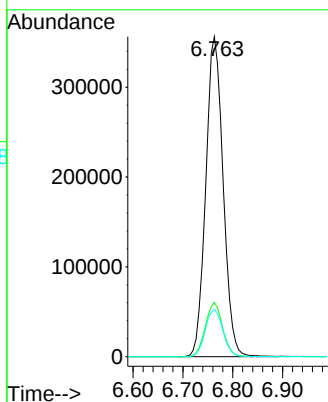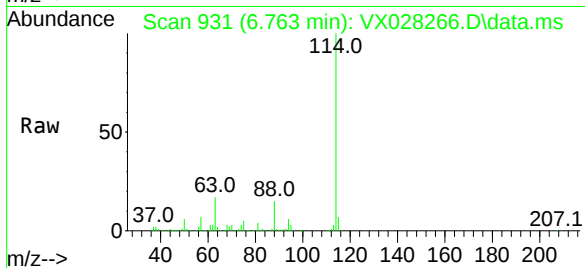

#35
 Dibromofluoromethane
 Concen: 43.412 ug/l
 RT: 5.391 min Scan# 706
 Delta R.T. 0.006 min
 Lab File: VX028266.D
 Acq: 22 Apr 2022 01:40

Tgt Ion:113 Resp: 262383
 Ion Ratio Lower Upper
 113 100
 111 102.5 82.8 124.2
 192 22.3 16.9 25.3


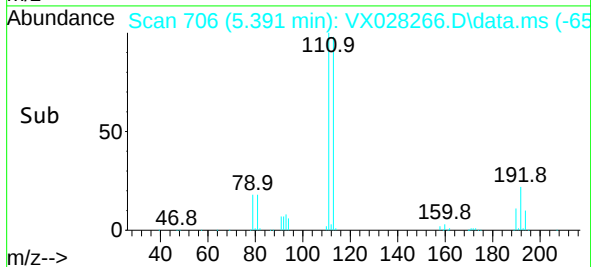
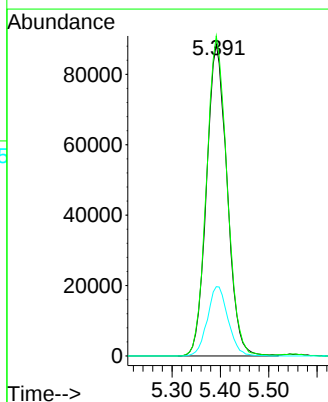
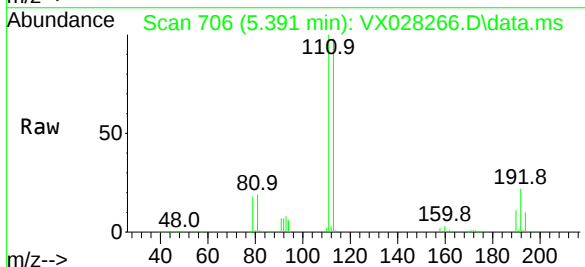




#36
1,1-Dichloropropene
Concen: 4.543 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.146 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 75 Resp: 35818
Ion Ratio Lower Upper
75 100
110 10.3 18.3 54.8#
77 0.0 24.8 37.2#

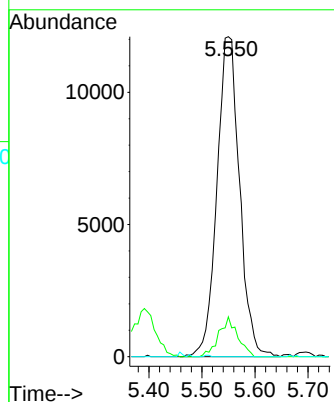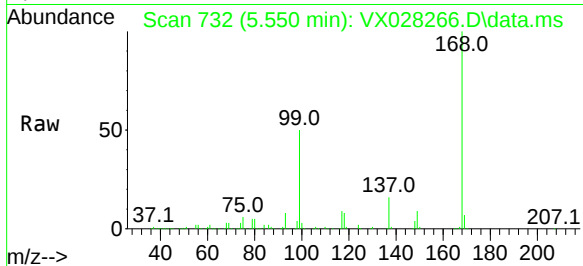

#38
Carbon Tetrachloride
Concen: 5.755 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 117 Resp: 51222
Ion Ratio Lower Upper
117 100
119 4.4 77.3 115.9#
121 0.0 24.2 36.2#

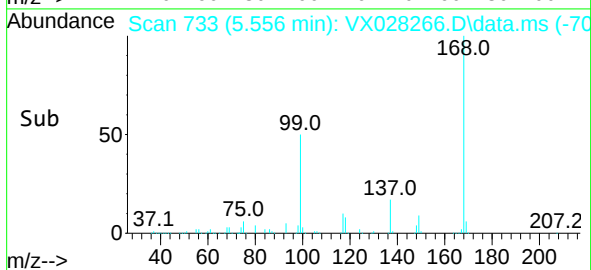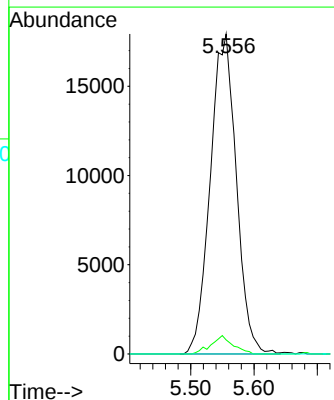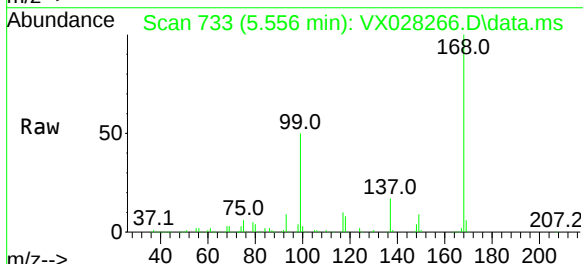

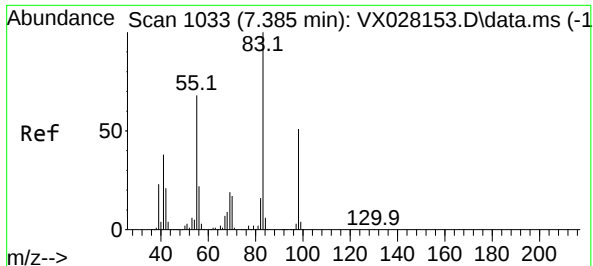

#39

Methylcyclohexane

Concen: 10.871 ug/l

RT: 7.379 min Scan# 1032

Delta R.T. -0.006 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40

Instrument :

MSVOA_X

ClientSampleId :

WC-15-1-3ME





Tgt Ion: 83 Resp: 108138

Ion Ratio Lower Upper

83 100

55 66.6 54.6 81.8

98 51.3 37.4 56.2

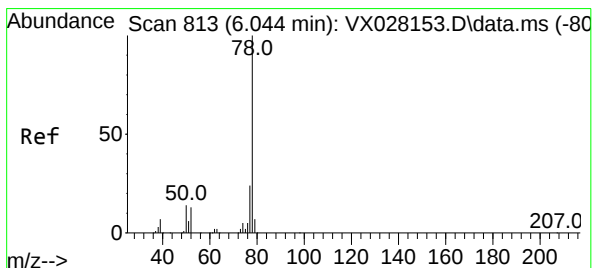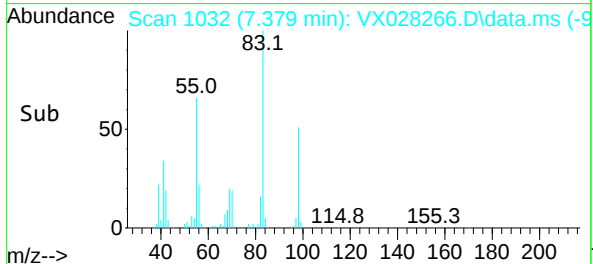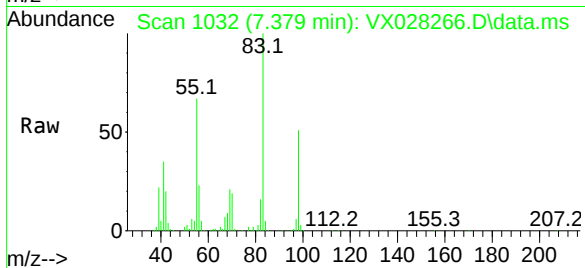

#40

Benzene

Concen: 0.205 ug/l

RT: 6.044 min Scan# 813

Delta R.T. -0.000 min

Lab File: VX028266.D




Acq: 22 Apr 2022 01:40


Tgt Ion: 78 Resp: 4741

Ion Ratio Lower Upper

78 100

77 24.6 19.3 28.9


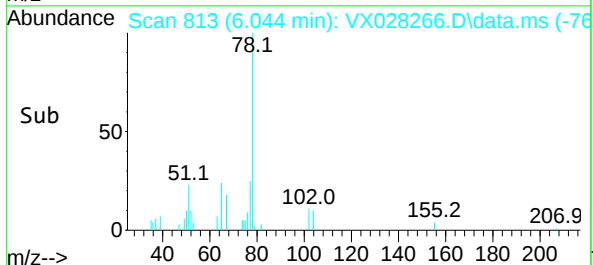
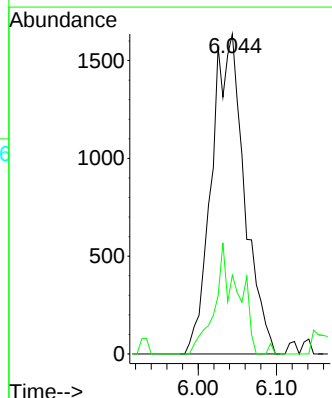
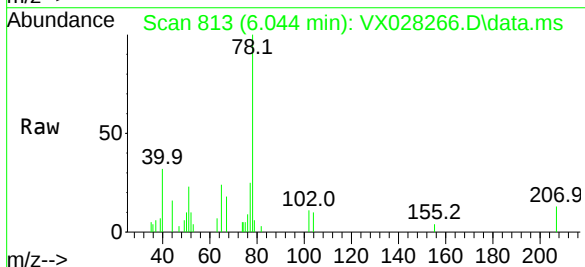




#50
Toluene-d8
Concen: 41.652 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 98 Resp: 966889
Ion Ratio Lower Upper
98 100
100 66.4 52.6 78.8

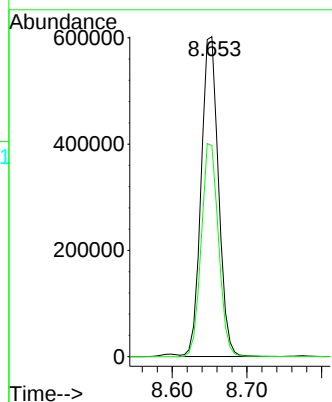

#51
4-Methyl-2-Pentanone
Concen: 0.925 ug/l
RT: 8.598 min Scan# 1232
Delta R.T. 0.024 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 43 Resp: 7728
Ion Ratio Lower Upper
43 100
58 6.4 36.1 54.1#


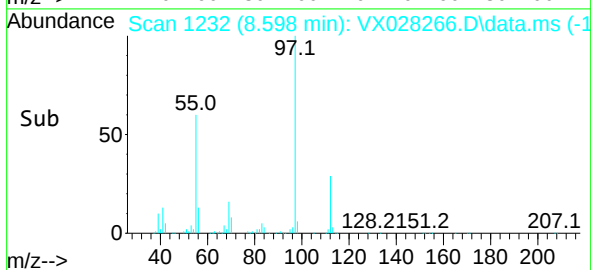
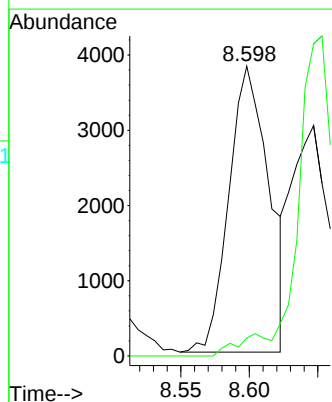
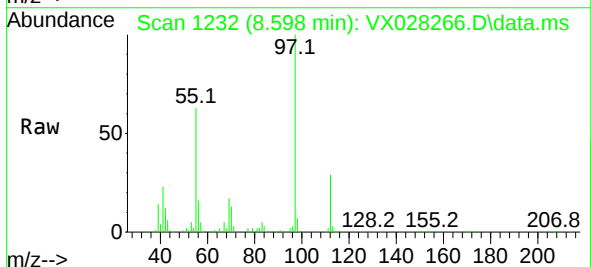




#52
Toluene
Concen: 0.743 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 92 Resp: 11912
Ion Ratio Lower Upper
92 100
91 166.5 137.5 206.3

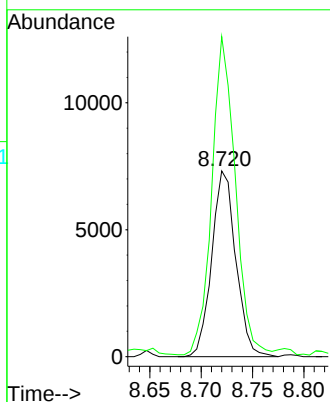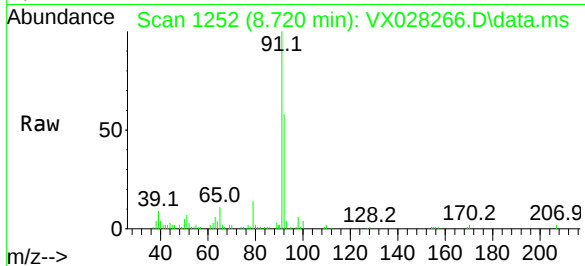

#55
1,1,2-Trichloroethane
Concen: 6.408 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.049 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 97 Resp: 41743
Ion Ratio Lower Upper
97 100
83 8.2 66.2 99.4#
85 0.6 42.9 64.3#
99 0.4 49.0 73.6#


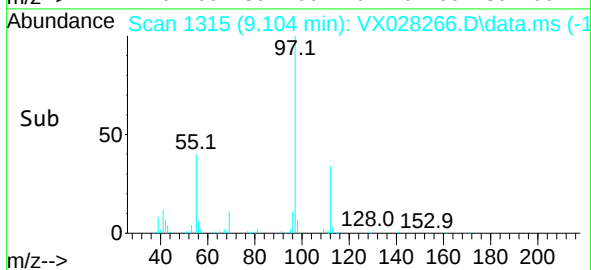
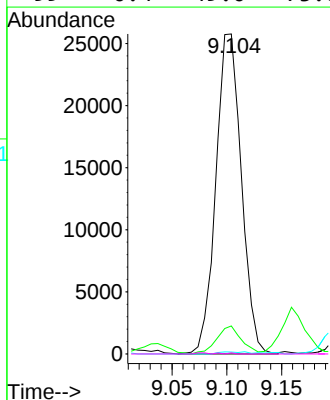
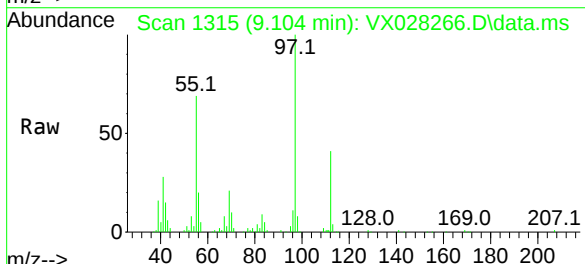




#56
Ethyl methacrylate
Concen: 0.904 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.012 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 69 Resp: 8541
Ion Ratio Lower Upper
69 100
41 145.9 43.8 65.6#
39 84.6 22.2 33.2#

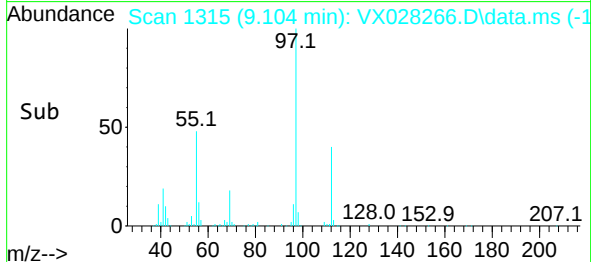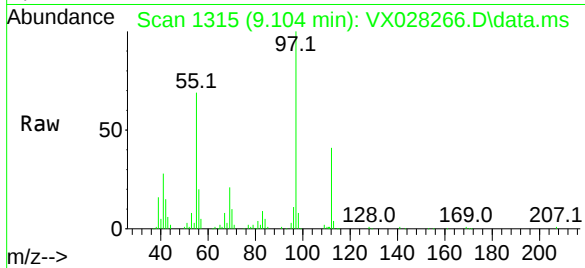

#59
2-Hexanone
Concen: 6.894 ug/l
RT: 9.385 min Scan# 1361
Delta R.T. -0.048 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 43 Resp: 44615
Ion Ratio Lower Upper
43 100
58 3.8 31.9 95.7#


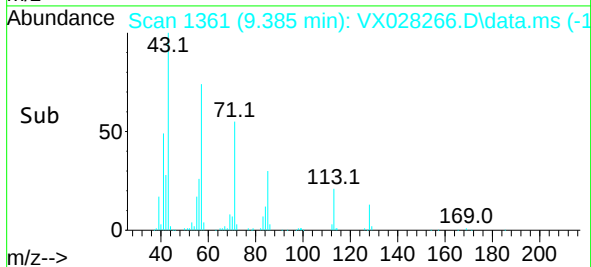

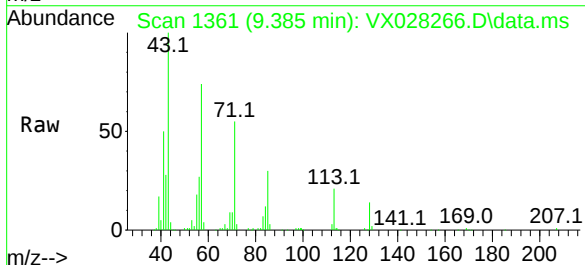




#62
4-Bromofluorobenzene
Concen: 40.893 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 95 Resp: 362962
Ion Ratio Lower Upper
95 100
174 88.3 0.0 163.0
176 85.0 0.0 155.0

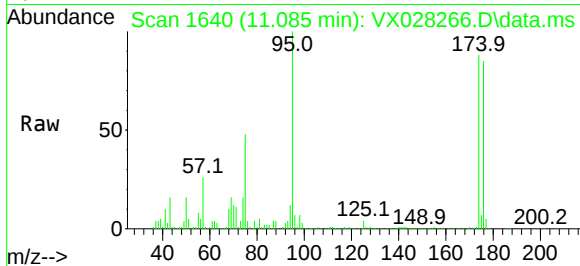

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 117 Resp: 766461
Ion Ratio Lower Upper
117 100
82 50.8 41.8 62.8
119 32.9 24.8 37.2

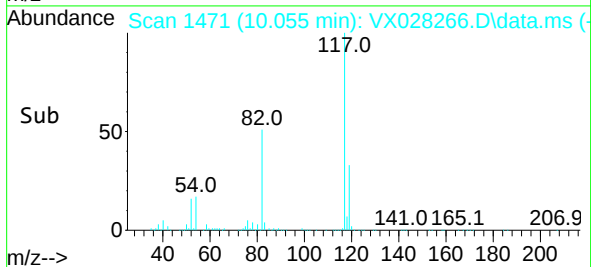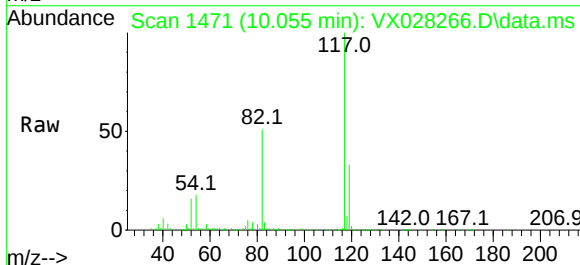



#67

Ethyl Benzene

Concen: 1.374 ug/l

RT: 10.201 min Scan# 1495

Delta R.T. 0.006 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40

Instrument :

MSVOA_X

ClientSampleId :





WC-15-1-3ME

Tgt Ion: 91 Resp: 37645

Ion Ratio Lower Upper

91 100

106 34.0 24.6 36.8

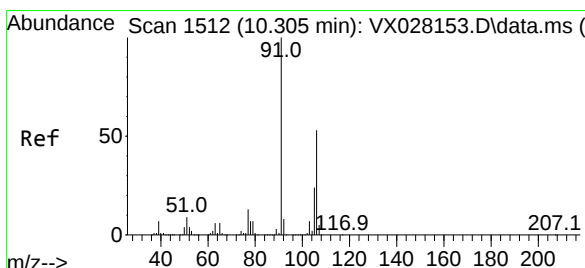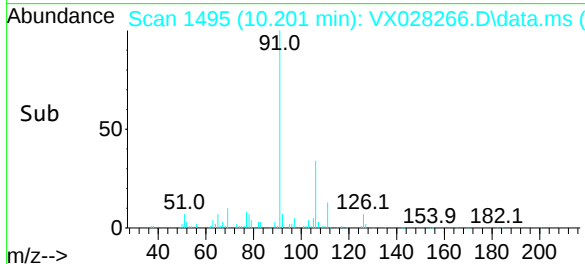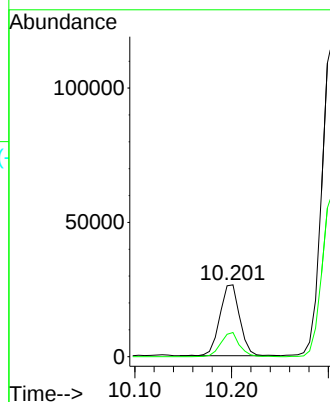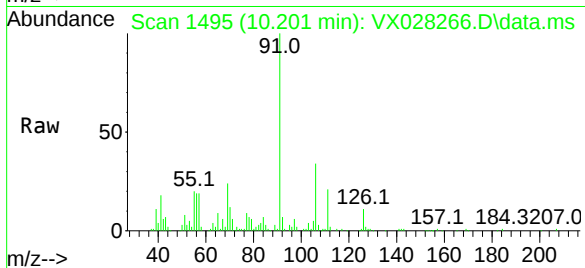

#68

m/p-Xylenes

Concen: 7.702 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.000 min

Lab File: VX028266.D




Acq: 22 Apr 2022 01:40


Tgt Ion: 106 Resp: 85900

Ion Ratio Lower Upper

106 100

91 193.6 160.4 240.6


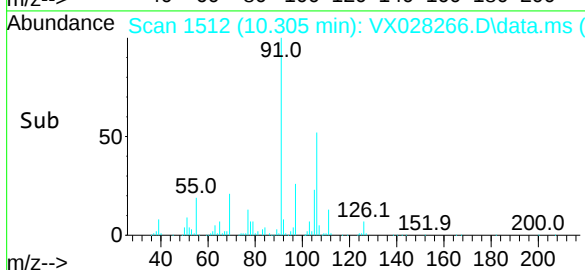
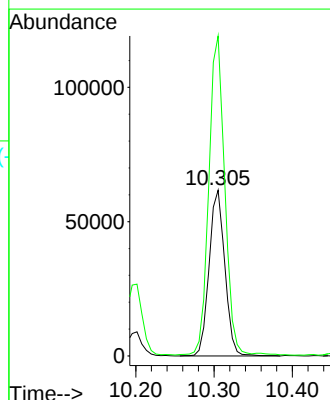
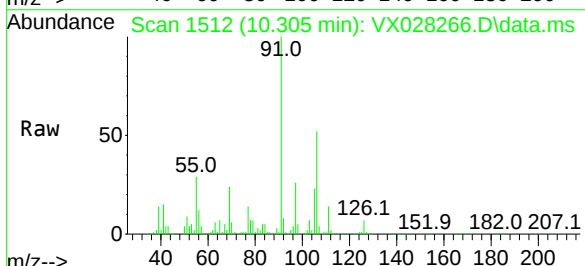




#69
o-Xylene
Concen: 7.877 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion:106 Resp: 87584
Ion Ratio Lower Upper
106 100
91 206.5 106.1 318.1



#70
Styrene
Concen: 0.282 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. -0.013 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion:104 Resp: 5082
Ion Ratio Lower Upper
104 100
78 255.0 38.6 57.8#
103 259.1 43.8 65.8#


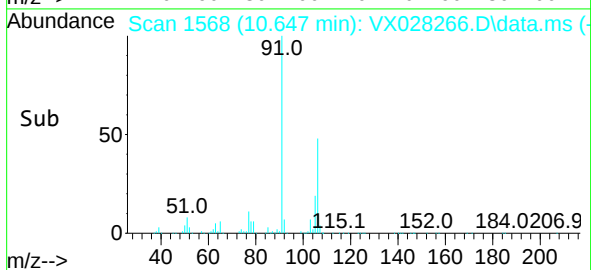

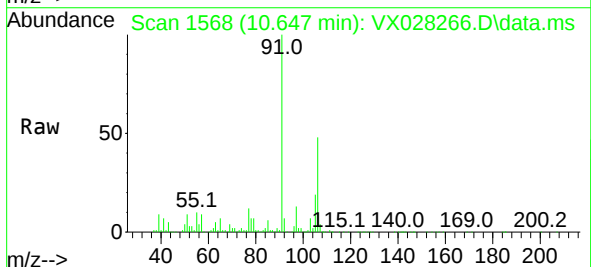




#71
Bromoform
Concen: 3.588 ug/l
RT: 10.823 min Scan# 11
Delta R.T. 0.024 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion:173 Resp: 74
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.2#
254 0.0 0.1 0.1#

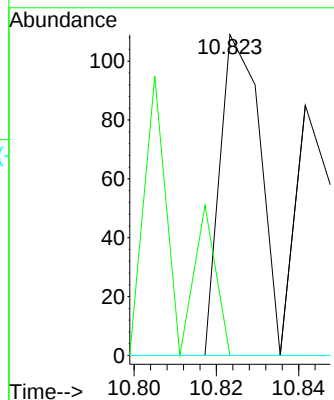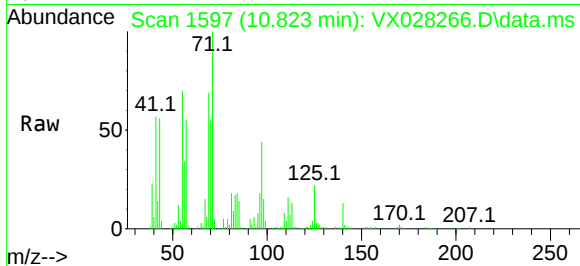

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion:152 Resp: 410983
Ion Ratio Lower Upper
152 100
115 58.3 37.5 112.7
150 156.2 0.0 338.2


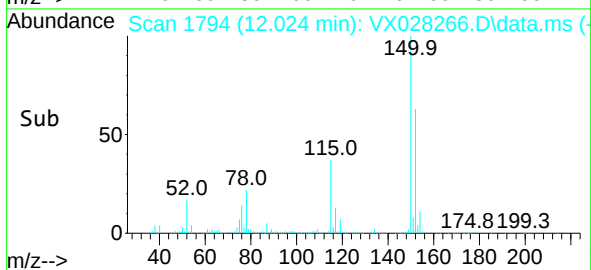
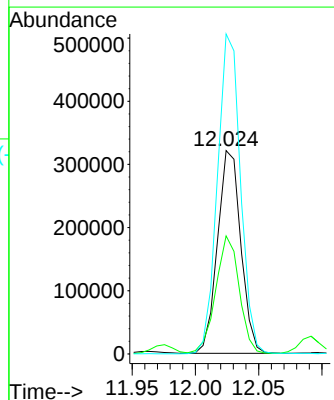
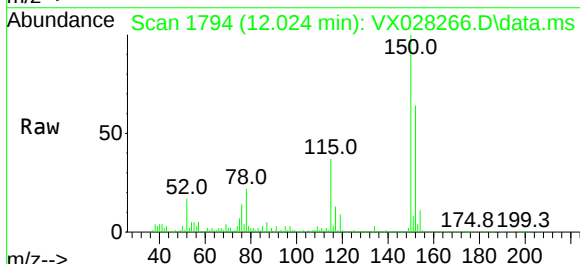




#73
Isopropylbenzene
Concen: 5.142 ug/l
RT: 10.964 min Scan# 1602
Delta R.T. 0.001 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion:105 Resp: 145241
Ion Ratio Lower Upper
105 100
120 28.2 13.5 40.5

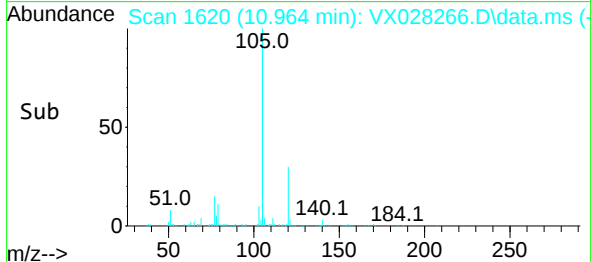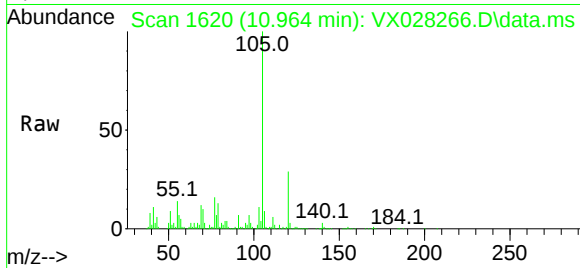

#74
N-ethyl acetate
Concen: 6.795 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.006 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 43 Resp: 66344
Ion Ratio Lower Upper
43 100
70 96.2 42.5 63.7#
55 365.9 23.1 34.7#
61 0.0 22.8 34.2#


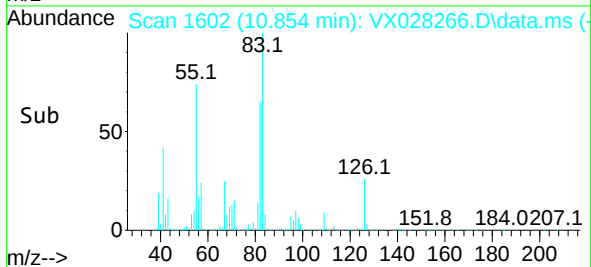

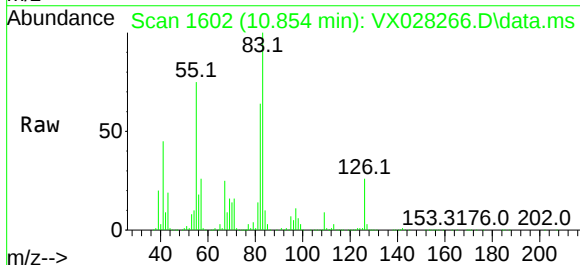


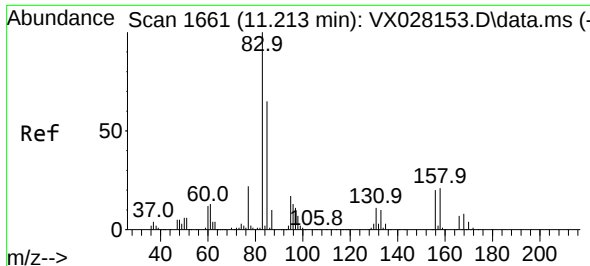

#75
 1,1,2,2-Tetrachloroethane
 Concen: 7.157 ug/l
 RT: 11.220 min Scan# 1640
 Delta R.T. 0.007 min
 Lab File: VX028266.D
 Acq: 22 Apr 2022 01:40




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-3ME


Tgt Ion: 83 Resp: 65608
 Ion Ratio Lower Upper
 83 100
 131 0.3 5.1 15.3#
 85 6.6 32.6 97.7#

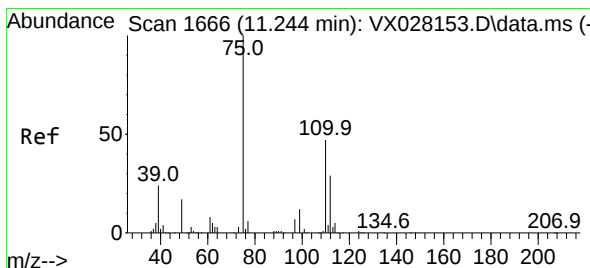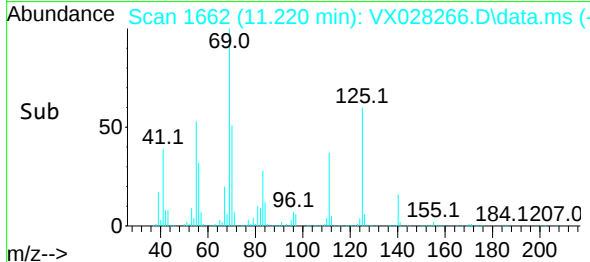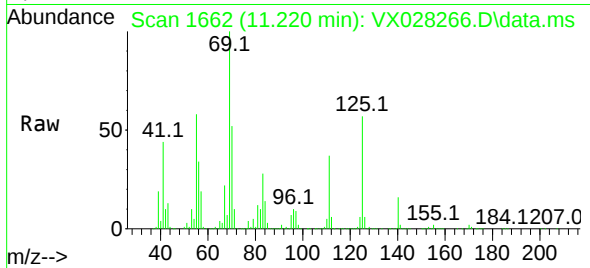

#76
 1,2,3-Trichloropropane
 Concen: 20.632 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX028266.D
 Acq: 22 Apr 2022 01:40

Tgt Ion: 75 Resp: 166880
 Ion Ratio Lower Upper
 75 100
 77 0.0 19.4 58.2#


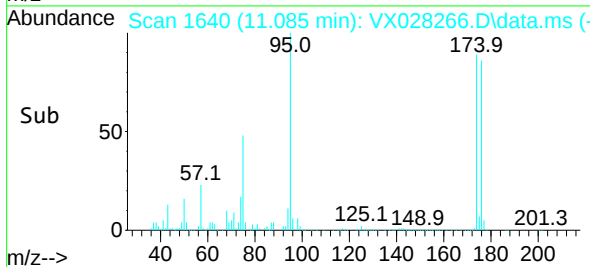

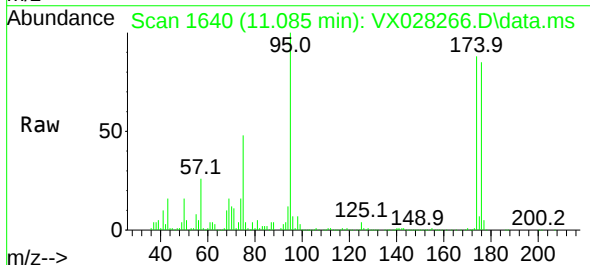


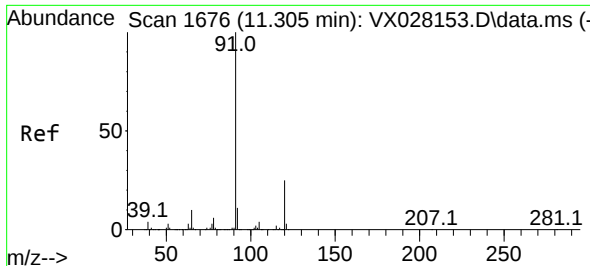

#78
n-propylbenzene
Concen: 8.717 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 91 Resp: 273049
Ion Ratio Lower Upper
91 100
120 24.8 11.6 34.8

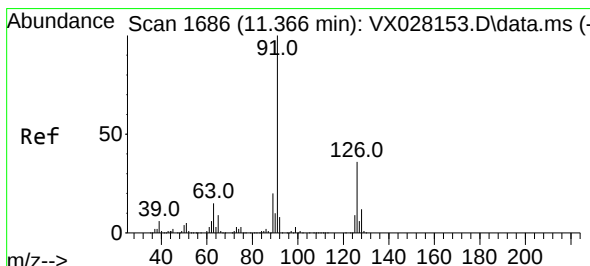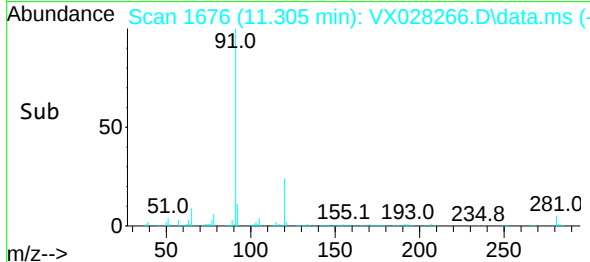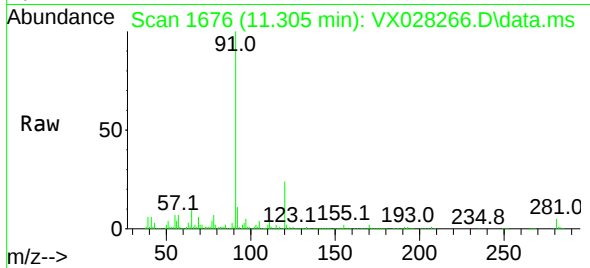

#79
2-Chlorotoluene
Concen: 3.061 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 91 Resp: 59601
Ion Ratio Lower Upper
91 100
126 3.8 17.3 51.9#


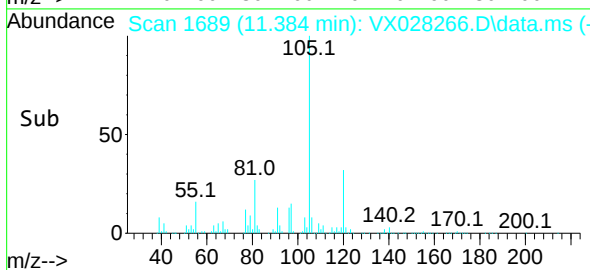

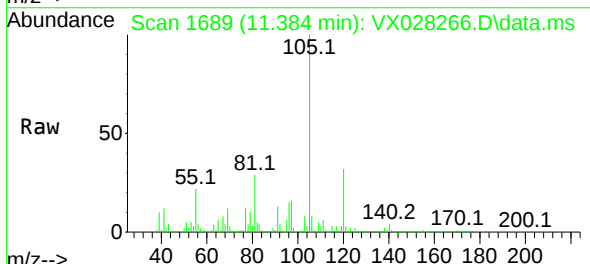




#80
 1,3,5-Trimethylbenzene
 Concen: 25.258 ug/l
 RT: 11.457 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX028266.D
 Acq: 22 Apr 2022 01:40




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-3ME


Tgt Ion:105 Resp: 605644
 Ion Ratio Lower Upper
 105 100
 120 51.2 24.3 72.9

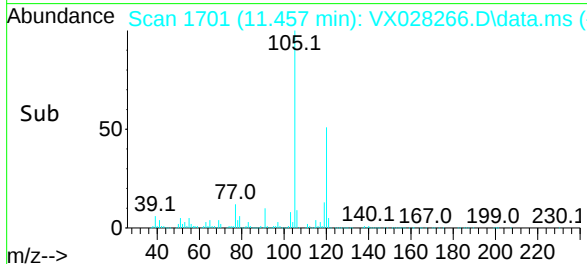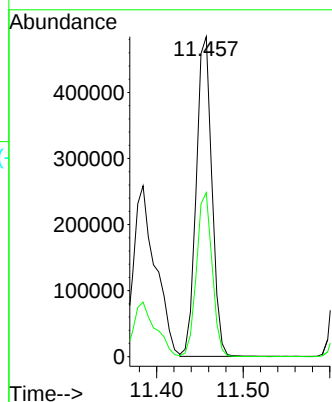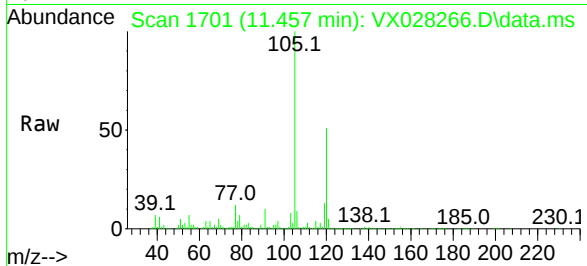

#81
 trans-1,4-Dichloro-2-butene
 Concen: 61.313 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. 0.067 min
 Lab File: VX028266.D
 Acq: 22 Apr 2022 01:40

Tgt Ion: 75 Resp: 166880
 Ion Ratio Lower Upper
 75 100
 53 1.9 69.0 103.4#
 89 0.1 37.0 55.6#

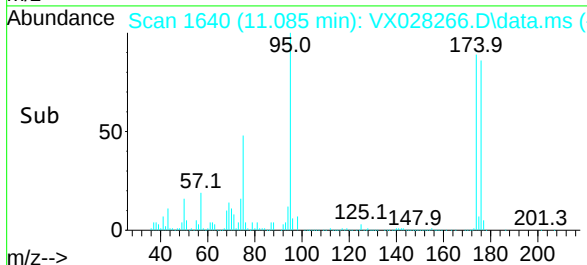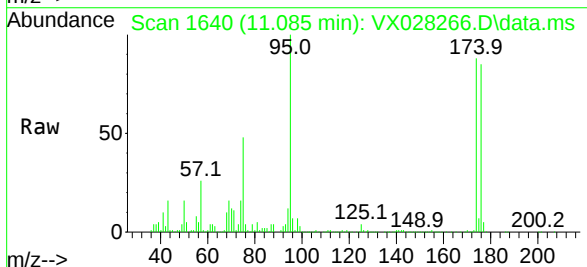



#82

4-Chlorotoluene

Concen: 2.890 ug/l

RT: 11.457 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40

Instrument :

MSVOA_X

ClientSampleId :





WC-15-1-3ME

Tgt Ion: 91 Resp: 64836

Ion Ratio Lower Upper

91 100

126 1.9 14.9 44.5#

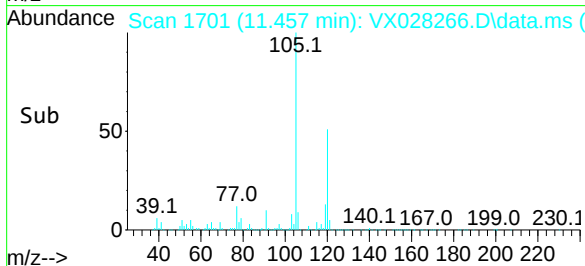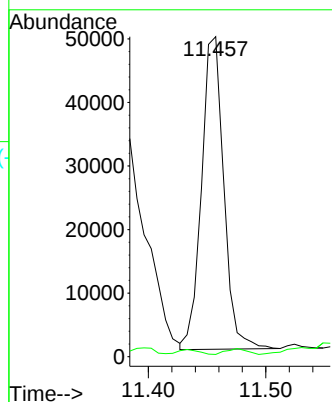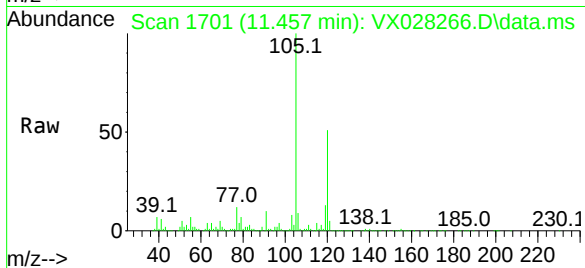

#83

tert-Butylbenzene

Concen: 1.069 ug/l

RT: 11.713 min Scan# 1743

Delta R.T. -0.006 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40




Tgt Ion: 119 Resp: 26170


Ion Ratio Lower Upper

119 100

91 63.4 26.9 80.6

134 26.0 11.4 34.2

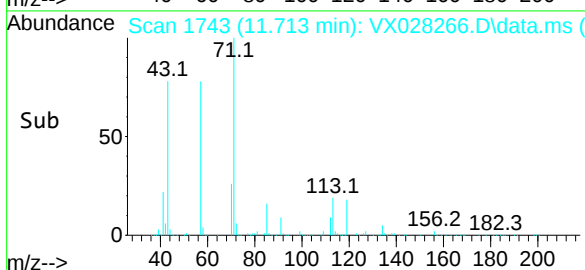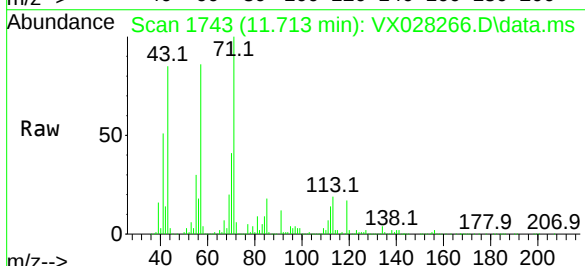

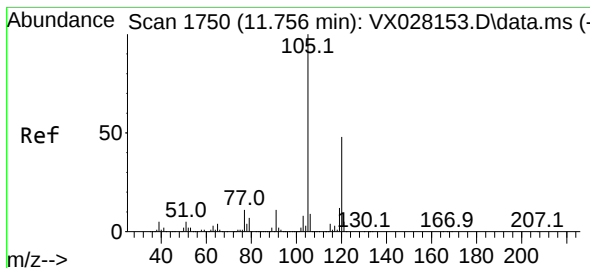

#84

1,2,4-Trimethylbenzene

Concen: 62.426 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.000 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40

Instrument :

MSVOA_X

ClientSampleId :





WC-15-1-3ME

Tgt Ion:105 Resp: 1487976

Ion Ratio Lower Upper

105 100

120 48.6 22.6 67.8

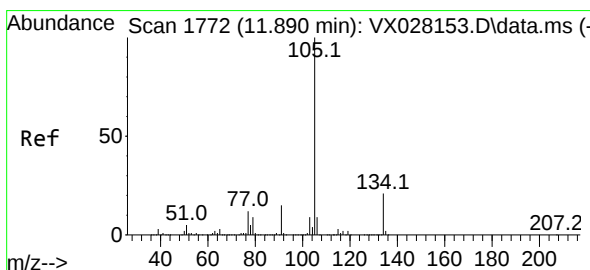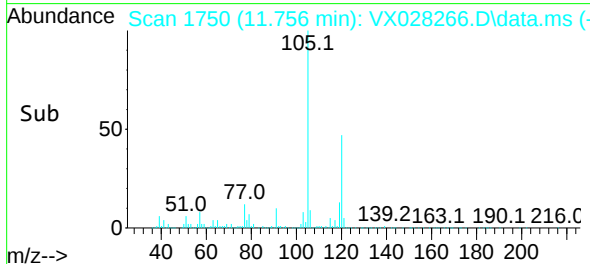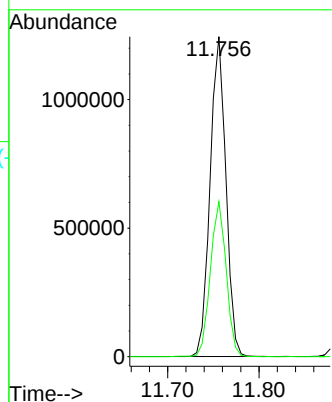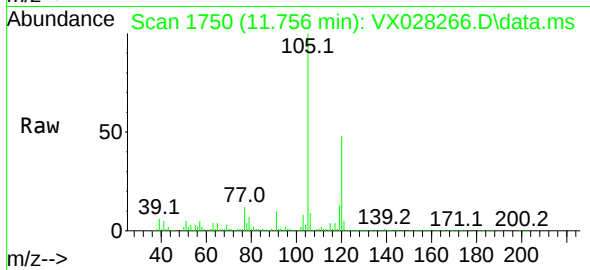

#85

sec-Butylbenzene

Concen: 7.551 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX028266.D




Acq: 22 Apr 2022 01:40


Tgt Ion:105 Resp: 223052

Ion Ratio Lower Upper

105 100

134 21.6 10.2 30.4


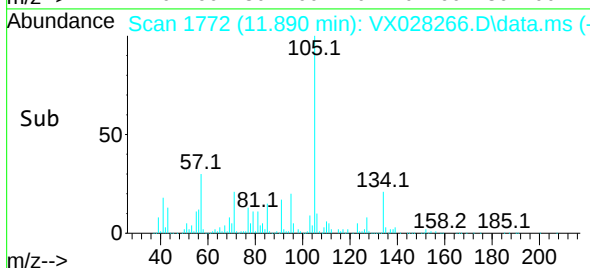

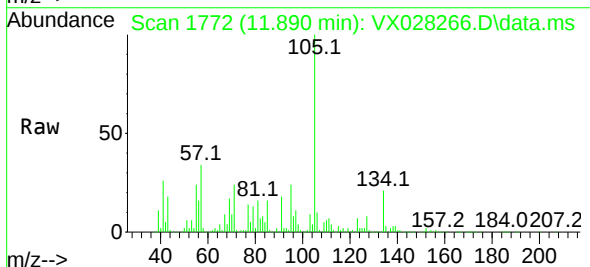


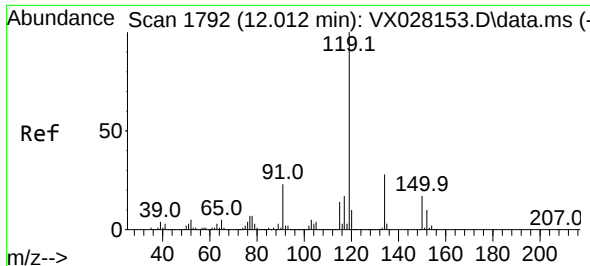

#86
p-Isopropyltoluene
Concen: 7.059 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion:119 Resp: 179883
Ion Ratio Lower Upper
119 100
134 27.5 13.0 39.0
91 23.8 11.3 33.9

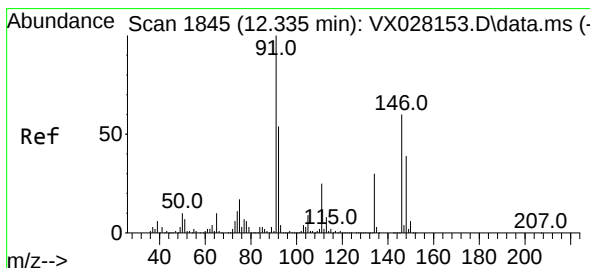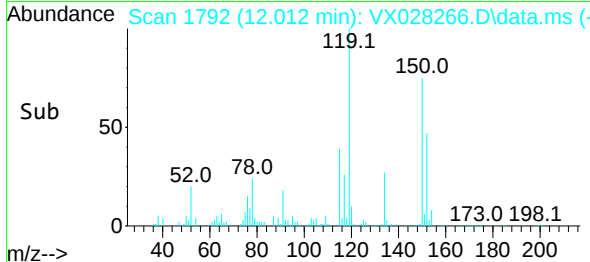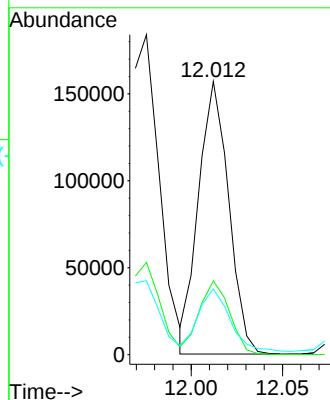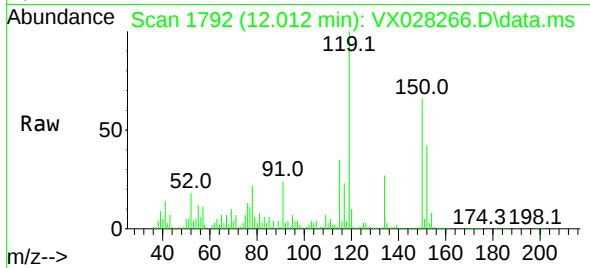

#89
n-Butylbenzene
Concen: 13.547 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40

Tgt Ion: 91 Resp: 283483
Ion Ratio Lower Upper
91 100
92 37.2 27.8 83.3
134 97.1 13.3 39.8#

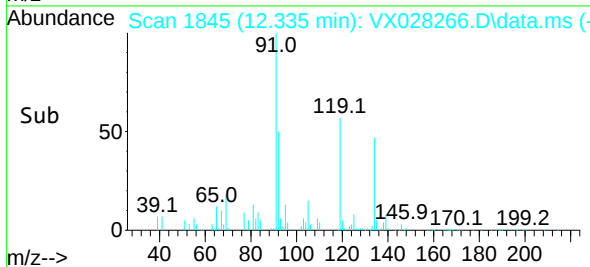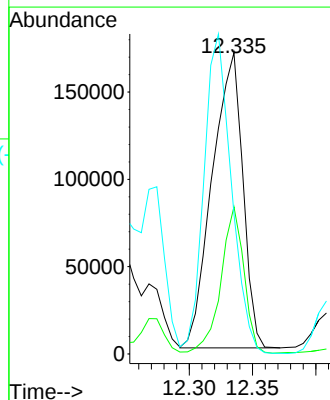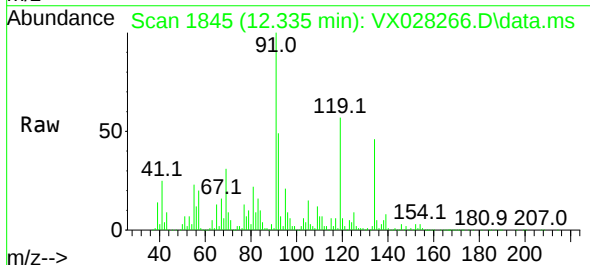



#90

Hexachloroethane

Concen: 9.149 ug/l

RT: 12.536 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40

Instrument :

MSVOA_X

ClientSampleId :





WC-15-1-3ME

Tgt Ion:117 Resp: 34900

Ion Ratio Lower Upper

117 100

201 0.0 39.5 118.5#

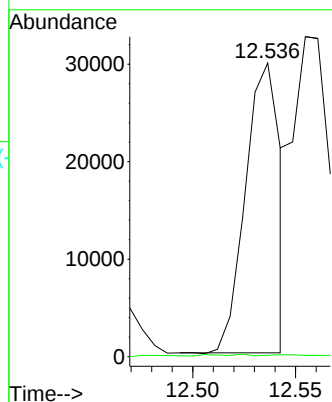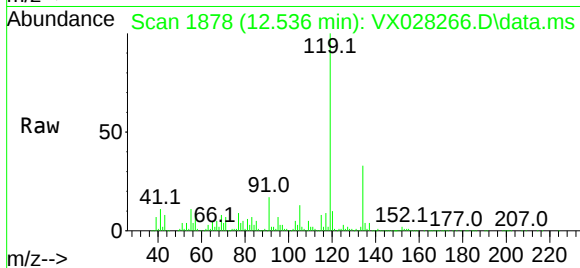

#91

1,2-Dichlorobenzene

Concen: 0.634 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.006 min

Lab File: VX028266.D

Acq: 22 Apr 2022 01:40




Tgt Ion:146 Resp: 8713


Ion Ratio Lower Upper

146 100

111 79.5 21.0 63.0#

148 66.6 32.6 97.7


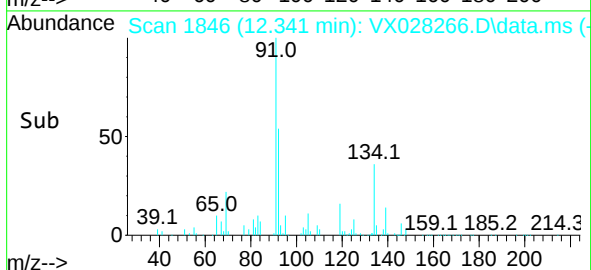

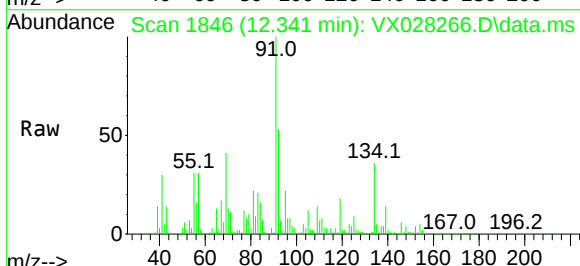




#92
1,2-Dibromo-3-Chloropropane
Concen: 2.295 ug/l
RT: 12.927 min Scan# 1942
Delta R.T. -0.018 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40




Instrument :
MSVOA_X
ClientSampleId :
WC-15-1-3ME


Tgt Ion: 75 Resp: 4679
Ion Ratio Lower Upper
75 100
155 20.7 47.0 141.2#
157 4.9 57.9 173.6#

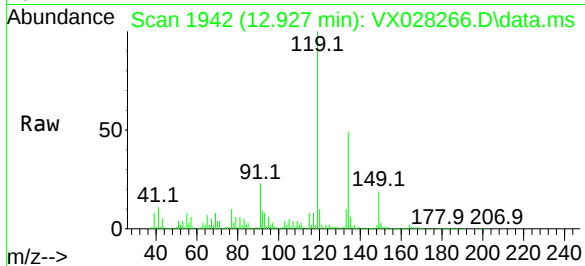

#95
Naphthalene
Concen: 20.416 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.000 min
Lab File: VX028266.D
Acq: 22 Apr 2022 01:40


Tgt Ion:128 Resp: 555498
Ion Ratio Lower Upper
128 100
127 16.0 10.2 15.4#
129 14.4 8.7 13.1#

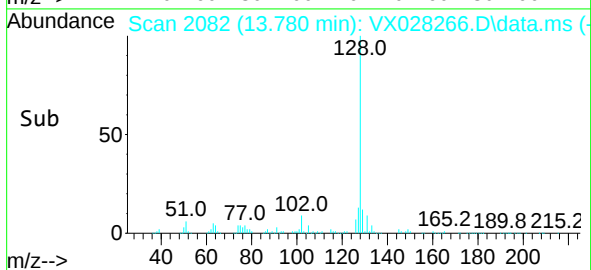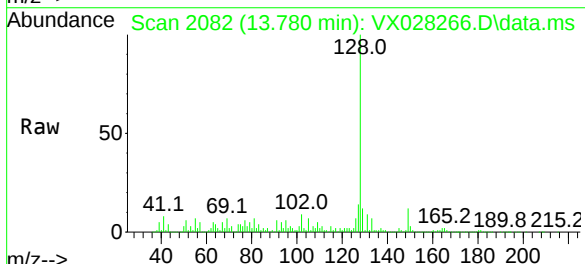



#96
 1,2,3-Trichlorobenzene
 Concen: 1.138 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX028266.D
 Acq: 22 Apr 2022 01:40

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-15-1-3ME



Tgt Ion:180 Resp: 9121
 Ion Ratio Lower Upper
 180 100
 182 10.3 50.0 149.8#
 145 3256.8 16.2 48.5#

