

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
 Data File : VX028232.D
 Acq On : 21 Apr 2022 11:37
 Operator : JC/MD
 Sample : VX0421MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0421MBL01

Quant Time: Apr 21 16:40:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	376898	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	646309	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	616420	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	285557	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	228490	46.495	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	92.980%
35) Dibromofluoromethane	5.385	113	212602	46.906	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	93.820%
50) Toluene-d8	8.647	98	767090	44.064	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	88.120%
62) 4-Bromofluorobenzene	11.079	95	277478	41.687	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	83.380%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028232.D
Acq On : 21 Apr 2022 11:37
Operator : JC/MD
Sample : VX0421MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0421MBL01

Quant Time: Apr 21 16:40:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




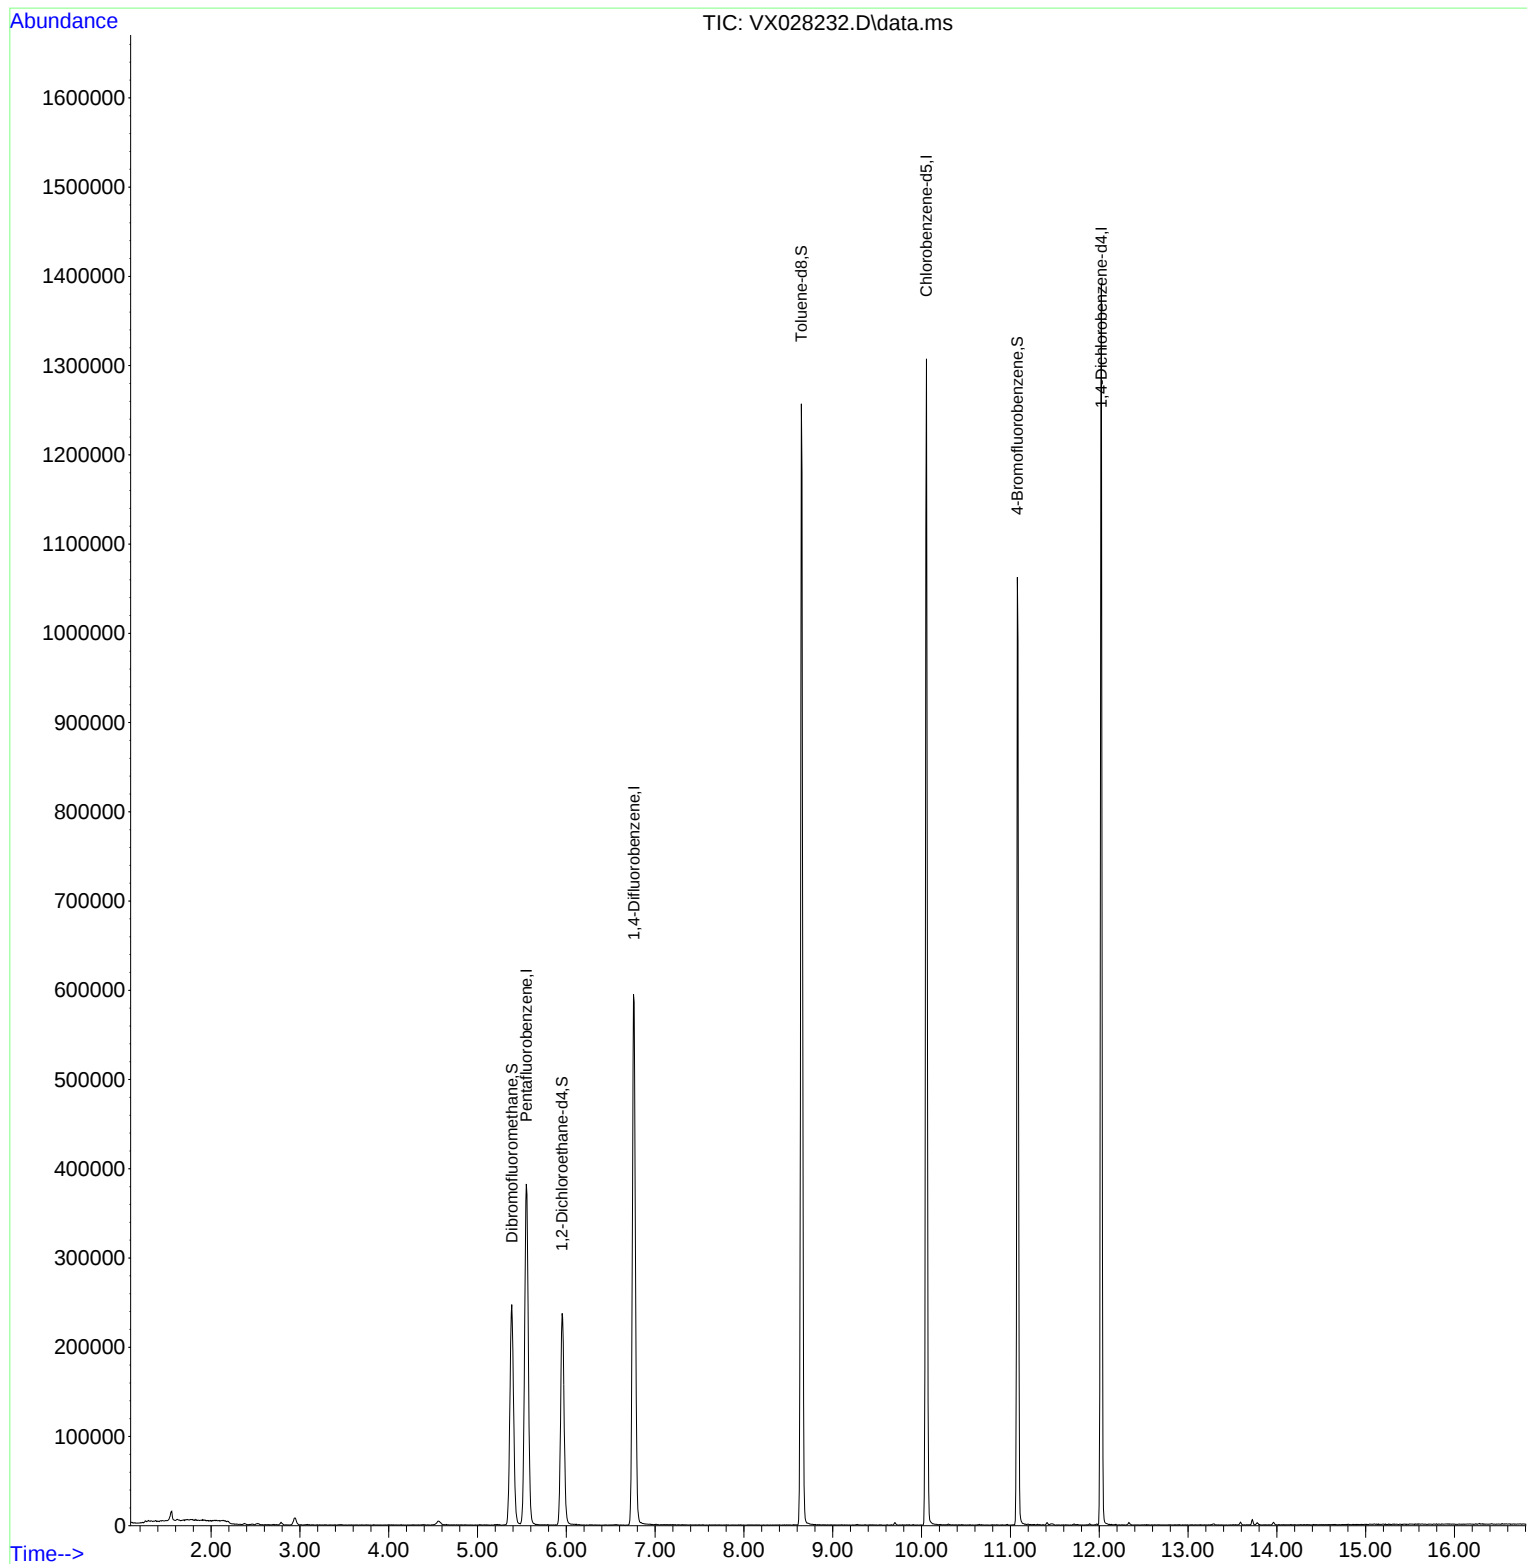


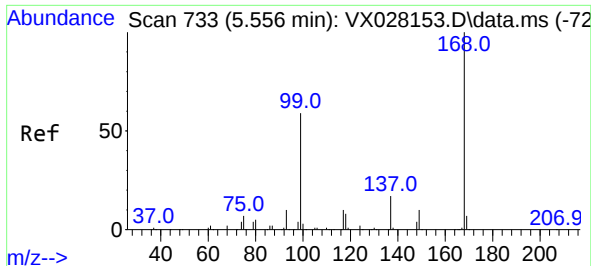

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37




Instrument :
MSVOA_X
ClientSampleId :
VX0421MBL01


Tgt Ion:168 Resp: 376898
Ion Ratio Lower Upper
168 100
99 57.1 41.7 62.5

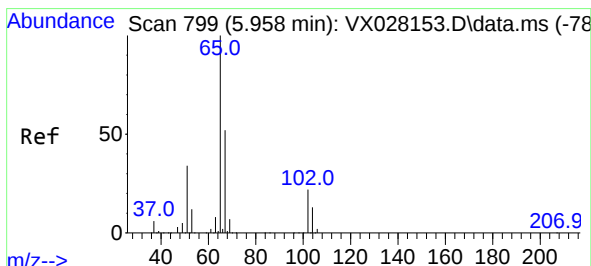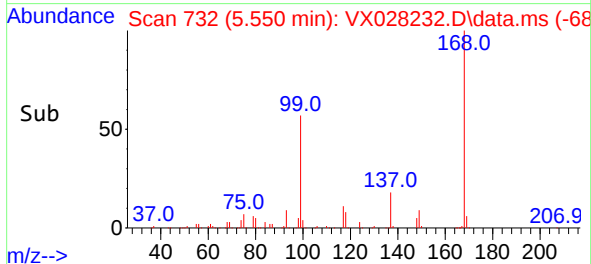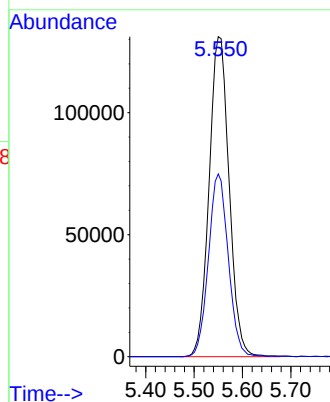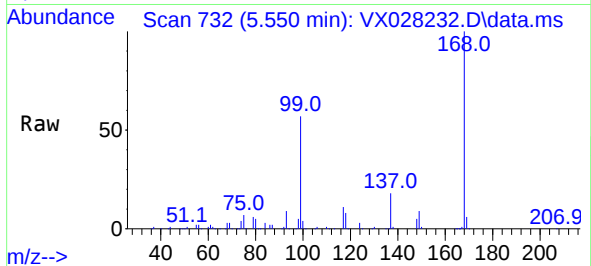

#33
1,2-Dichloroethane-d4
Concen: 46.495 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37


Tgt Ion: 65 Resp: 228490
Ion Ratio Lower Upper
65 100
67 51.8 0.0 107.4

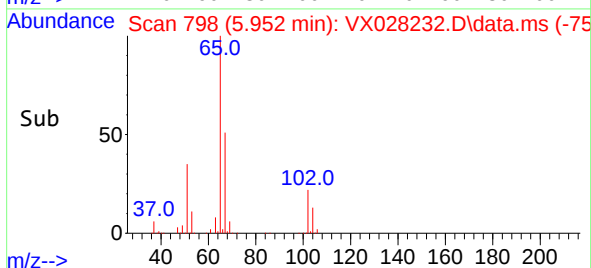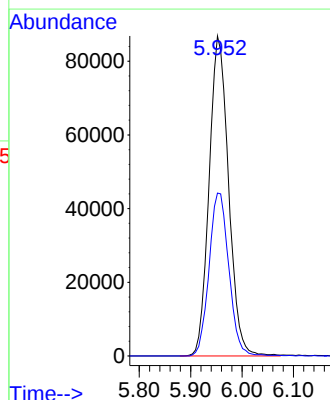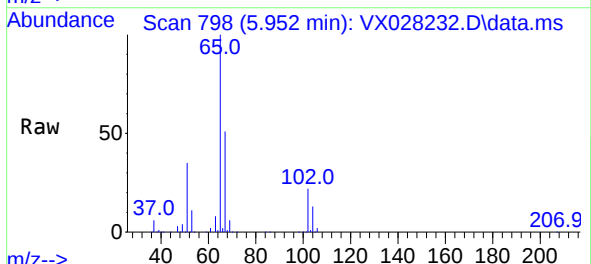



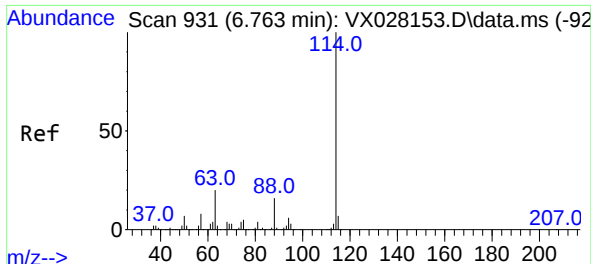


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37

Instrument :
MSVOA_X
ClientSampleId :
VX0421MBL01



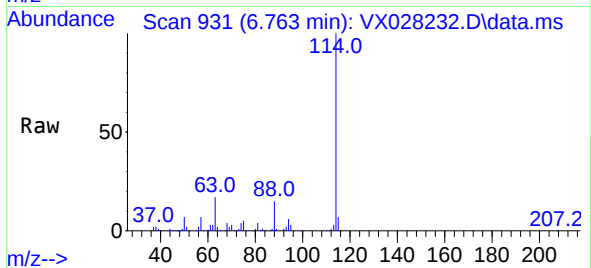



Tgt Ion:114 Resp: 646309
Ion Ratio Lower Upper
114 100
63 17.4 0.0 36.8
88 15.0 0.0 32.4

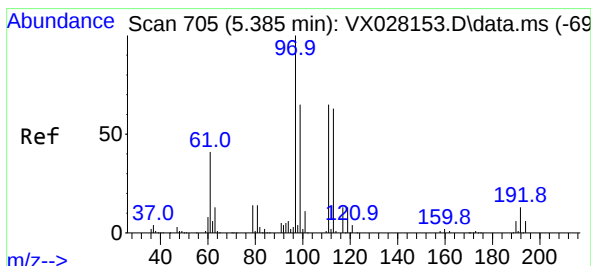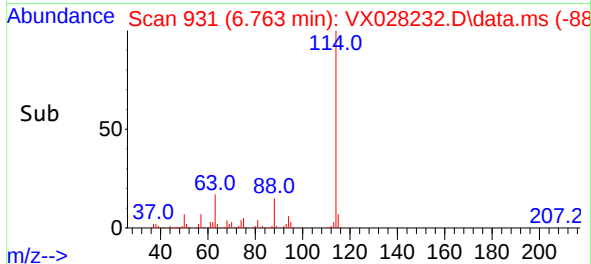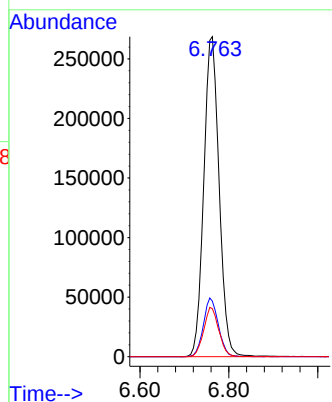

#35
Dibromofluoromethane
Concen: 46.906 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37

Tgt Ion:113 Resp: 212602
Ion Ratio Lower Upper
113 100
111 101.7 82.8 124.2
192 19.5 16.9 25.3


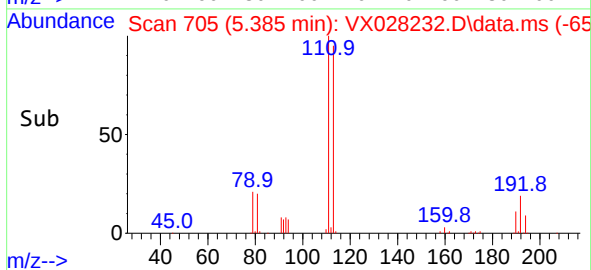
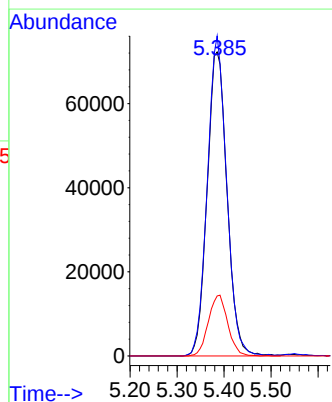
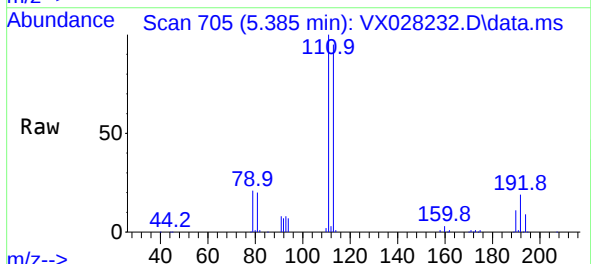


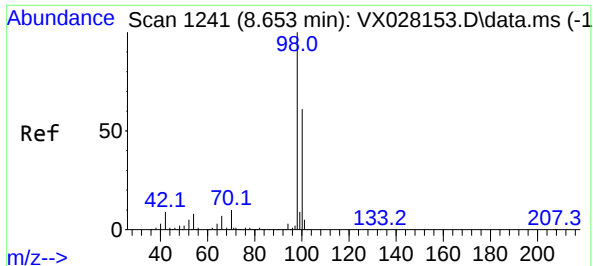

#50
Toluene-d8
Concen: 44.064 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37




Instrument :
MSVOA_X
ClientSampleId :
VX0421MBL01


Tgt Ion: 98 Resp: 767090
Ion Ratio Lower Upper
98 100
100 66.2 52.6 78.8

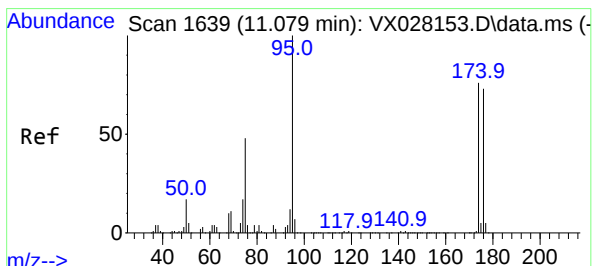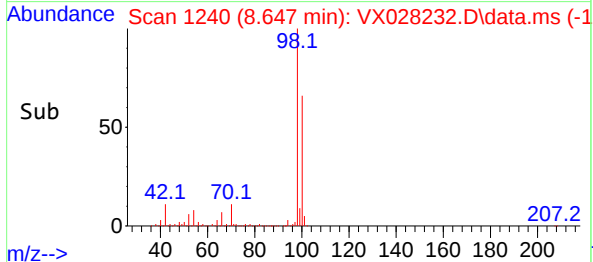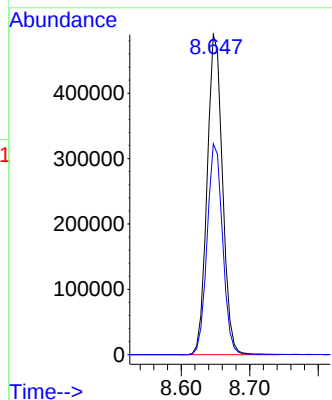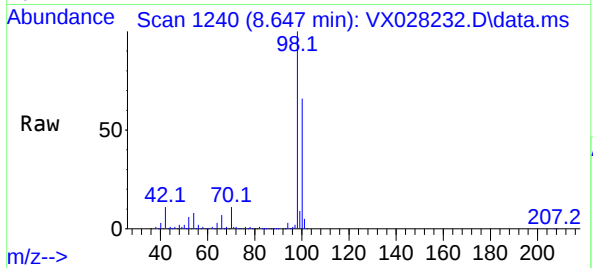

#62
4-Bromofluorobenzene
Concen: 41.687 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37

Tgt Ion: 95 Resp: 277478
Ion Ratio Lower Upper
95 100
174 83.4 0.0 163.0
176 81.8 0.0 155.0


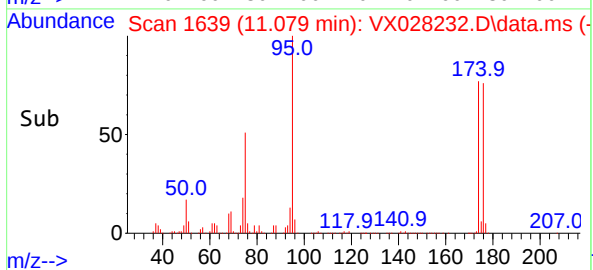
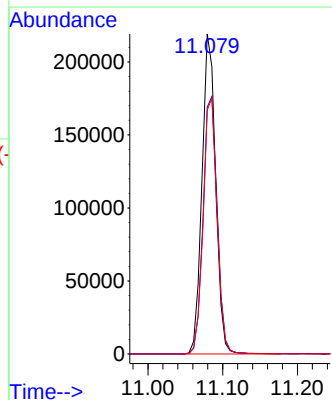
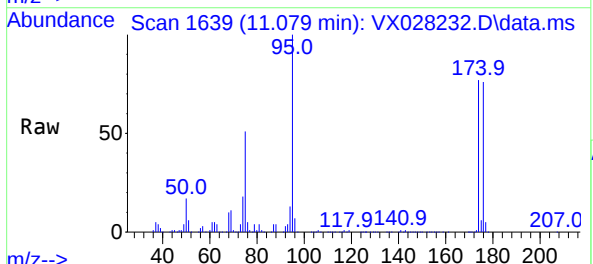


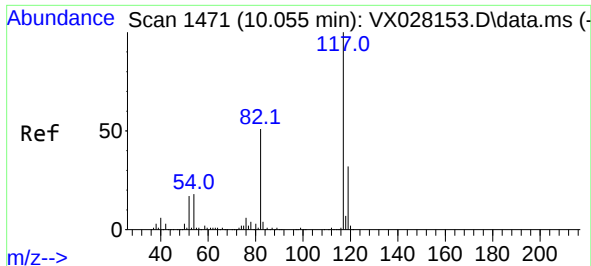

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37

Instrument :
MSVOA_X
ClientSampleId :
VX0421MBL01

Tgt Ion:117 Resp: 616420
Ion Ratio Lower Upper
117 100
82 51.2 41.8 62.8
119 32.8 24.8 37.2

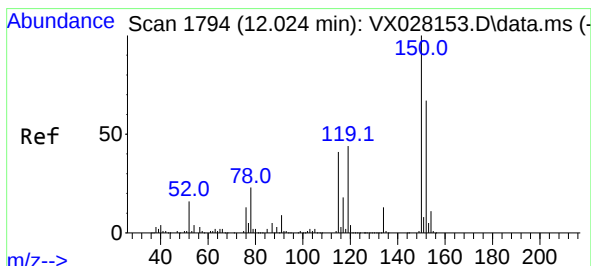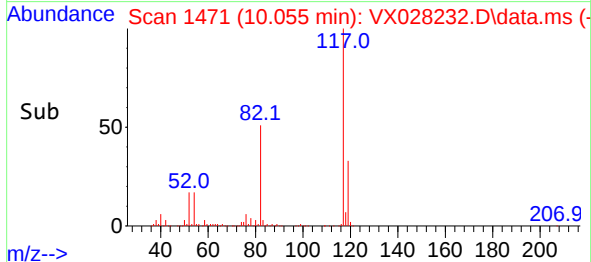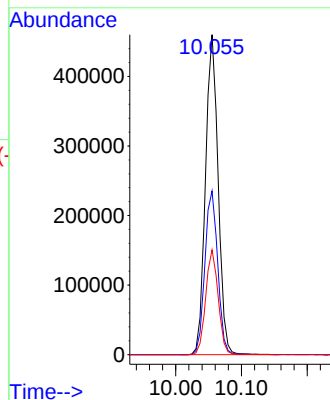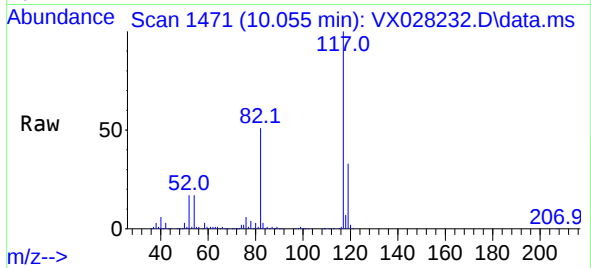

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028232.D
Acq: 21 Apr 2022 11:37

Tgt Ion:152 Resp: 285557
Ion Ratio Lower Upper
152 100
115 59.9 37.5 112.7
150 157.6 0.0 338.2

