

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
 Data File : VX028247.D
 Acq On : 21 Apr 2022 17:33
 Operator : JC/MD
 Sample : N2459-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31584

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Title : SW846 8260

Signal : TIC: VX028247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	693	706	722	rBV2	293441	858585	36.00%	6.923%
2	5.556	722	733	750	rVB	389089	1108657	46.49%	8.939%
3	5.958	787	799	818	rBV2	294800	789035	33.09%	6.362%
4	6.763	920	931	946	rBV	613871	1464359	61.41%	11.807%
5	8.653	1234	1241	1250	rBV	1529839	2384693	100.00%	19.228%
6	10.055	1465	1471	1490	rBV	1416013	1833932	76.90%	14.787%
7	11.079	1634	1639	1651	rBV	1281535	1679270	70.42%	13.540%
8	12.024	1788	1794	1801	rBV	1459428	1798852	75.43%	14.505%
9	13.585	2046	2050	2055	rBV2	17467	30011	1.26%	0.242%
10	13.664	2060	2063	2069	rVB3	17008	29865	1.25%	0.241%
11	13.853	2089	2094	2100	rVB3	17282	27801	1.17%	0.224%
12	13.926	2100	2106	2111	rBV3	30140	45668	1.92%	0.368%
13	14.213	2148	2153	2162	rBV3	36344	64931	2.72%	0.524%
14	14.371	2175	2179	2184	rVB2	30641	39572	1.66%	0.319%
15	14.481	2192	2197	2202	rBV2	32185	48352	2.03%	0.390%
16	14.615	2215	2219	2222	rBV3	20559	30110	1.26%	0.243%
17	14.670	2225	2228	2233	rVB2	22697	34337	1.44%	0.277%
18	14.822	2245	2253	2255	rBV3	23725	38684	1.62%	0.312%
19	14.902	2262	2266	2272	rBV3	20680	40600	1.70%	0.327%
20	15.182	2305	2312	2320	rBV3	23994	54650	2.29%	0.441%


Sum of corrected areas: 12401964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028247.D
Acq On : 21 Apr 2022 17:33
Operator : JC/MD
Sample : N2459-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31584

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

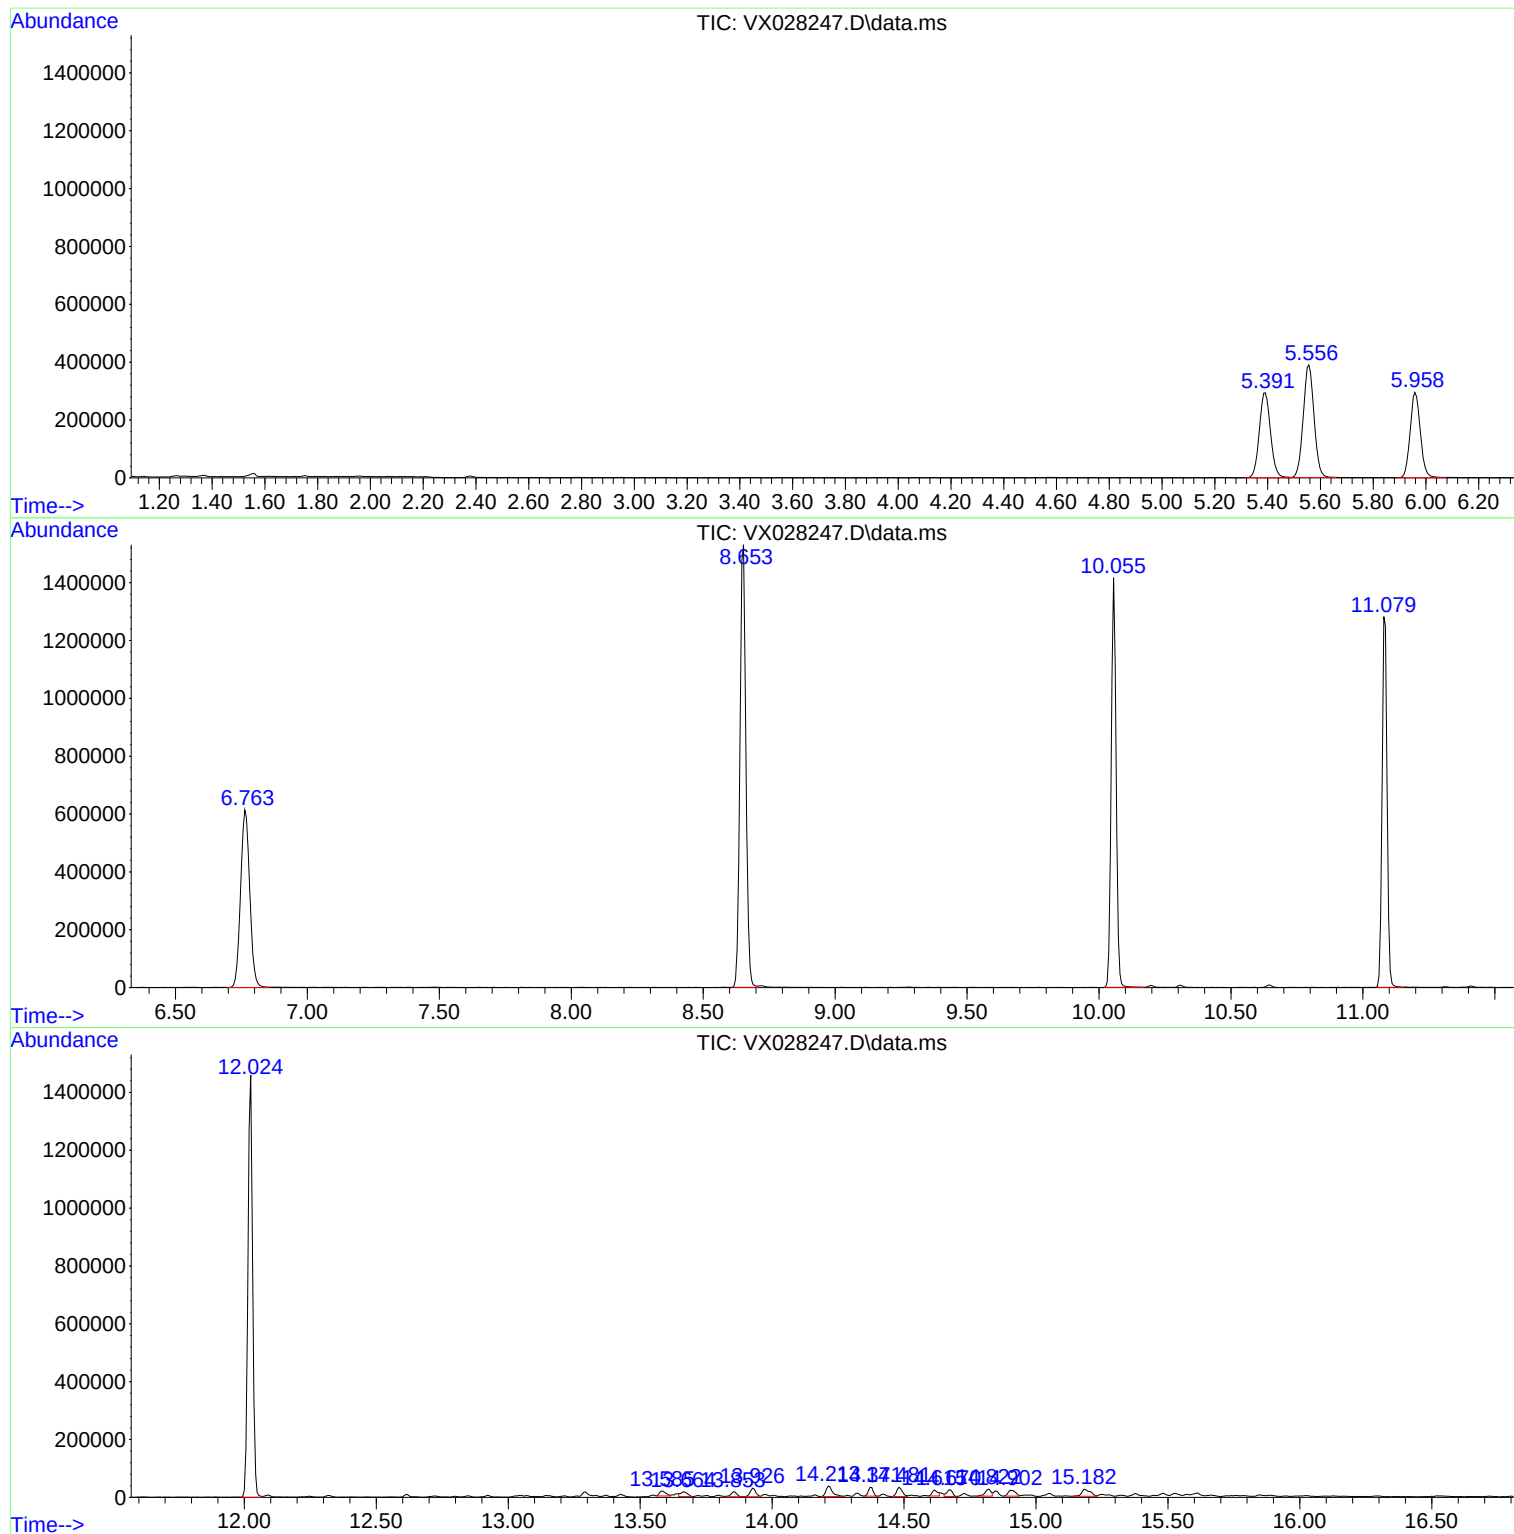

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028247.D
Acq On : 21 Apr 2022 17:33
Operator : JC/MD
Sample : N2459-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31584

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028247.D
Acq On : 21 Apr 2022 17:33
Operator : JC/MD
Sample : N2459-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
31584

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------