

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028257.D
Acq On : 21 Apr 2022 21:25
Operator : JC/MD
Sample : N2511-11 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1592

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M

Title : SW846 8260

Signal : TIC: VX028257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	25	32	47	rBV2	25517	121281	5.18%	1.017%
2	1.569	72	79	82	rBV4	13684	26714	1.14%	0.224%
3	2.947	296	305	313	rBV	23602	57628	2.46%	0.483%
4	5.391	692	706	721	rBV2	288364	842113	35.96%	7.063%
5	5.556	721	733	752	rVB	388758	1114360	47.59%	9.346%
6	5.958	787	799	815	rBV	301013	771960	32.97%	6.474%
7	6.763	920	931	944	rBV	618764	1467262	62.66%	12.305%
8	8.653	1234	1241	1251	rBV	1460827	2341515	100.00%	19.637%
9	10.055	1465	1471	1484	rBV	1355346	1815886	77.55%	15.229%
10	11.086	1634	1640	1654	rBV	1233361	1613787	68.92%	13.534%
11	12.024	1788	1794	1804	rBV	1420845	1751210	74.79%	14.687%




Sum of corrected areas: 11923716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028257.D
Acq On : 21 Apr 2022 21:25
Operator : JC/MD
Sample : N2511-11 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1592

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

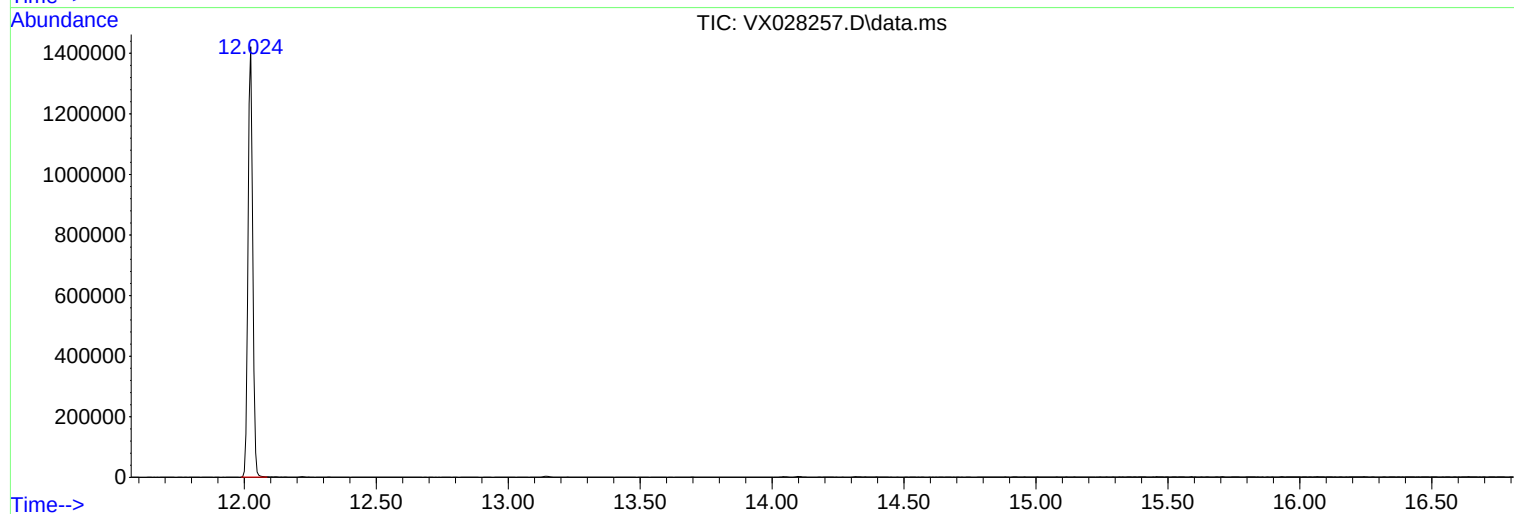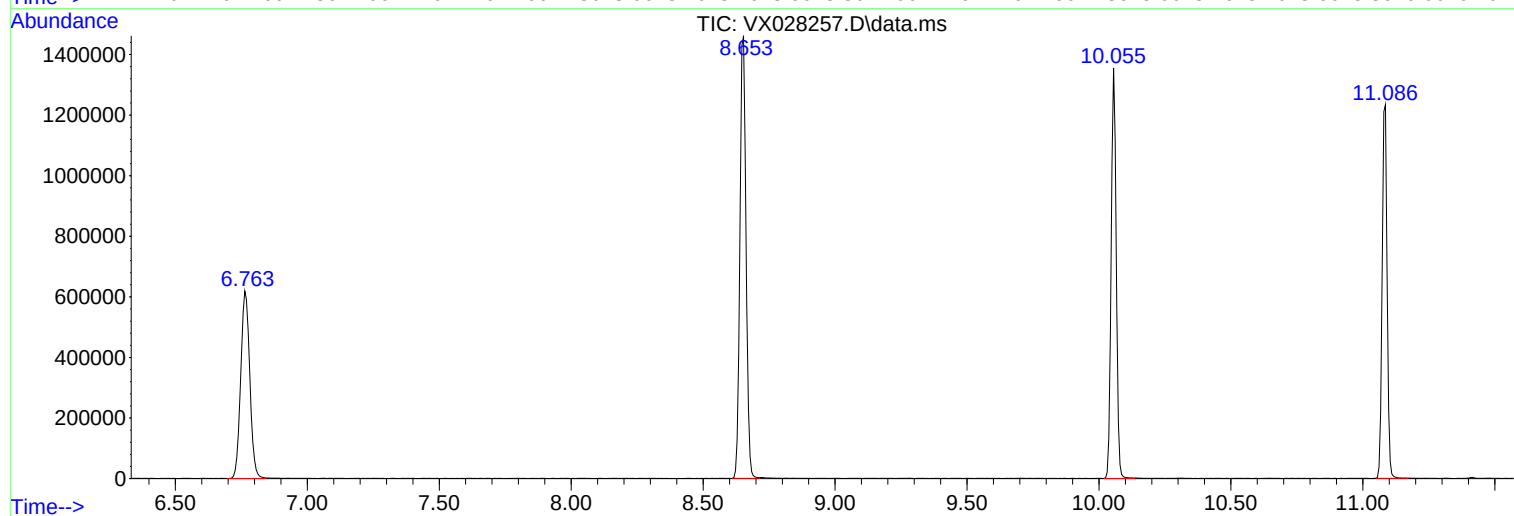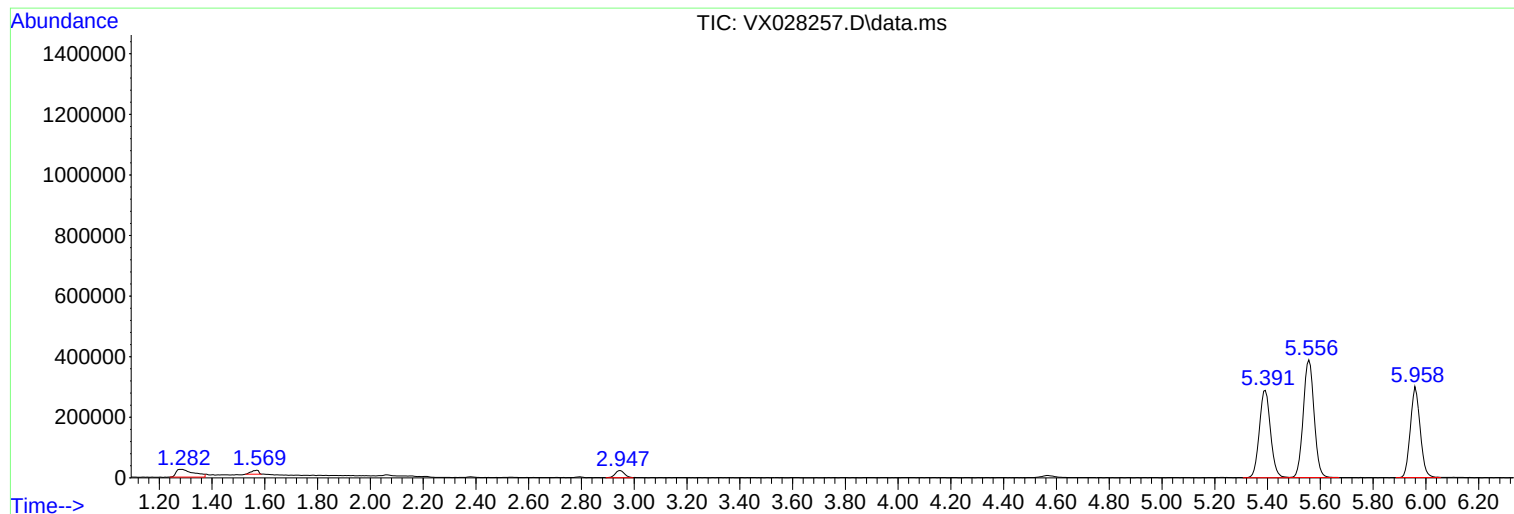

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028257.D
Acq On : 21 Apr 2022 21:25
Operator : JC/MD
Sample : N2511-11 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1592










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.282	5.44 ug/l	121281	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	83
2			2-Aminoethyl hydrogen sulfate	141	C2H7N04S	000926-39-6	74
3			Aminomethanesulfonic acid	111	CH5N03S	013881-91-9	64
4			4,6-Diamino-5-pyrimidinyl hydrog...	206	C4H6N4O4S	071525-41-2	9
5			2,4,6-Triamino-5-pyrimidinyl hyd...	221	C4H7N5O4S	071552-23-3	9

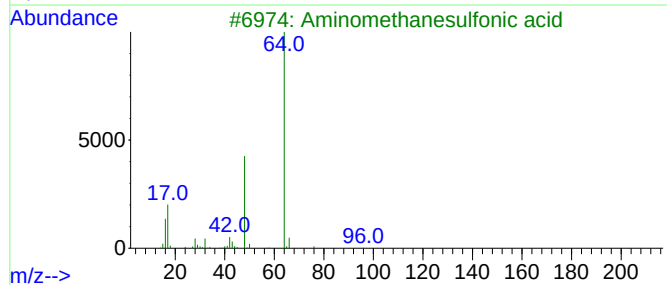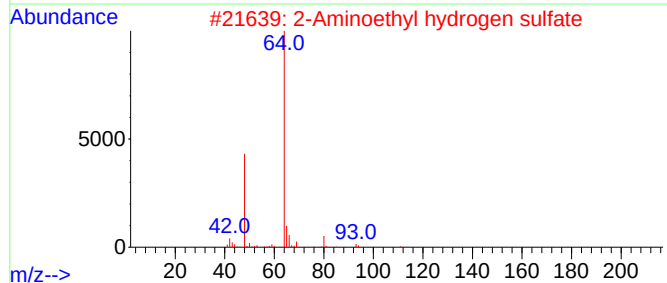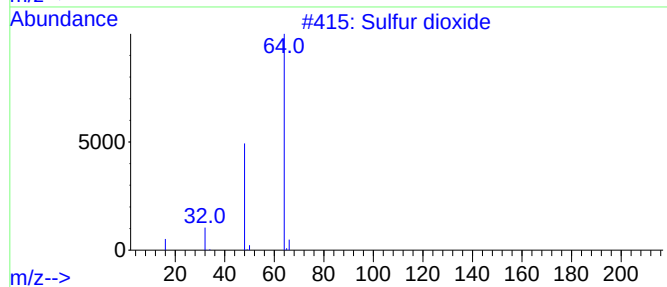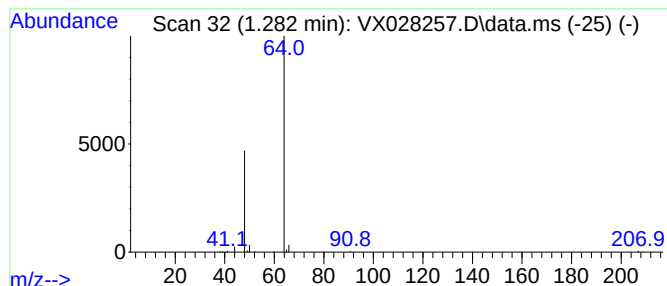

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042122\
Data File : VX028257.D
Acq On : 21 Apr 2022 21:25
Operator : JC/MD
Sample : N2511-11 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1592

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.282	5.4	ug/l	121281	1	5.556	1114360	50.0