



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042123\
Data File : VX035225.D
Acq On : 21 Apr 2023 08:43
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Title : SW846 8260
Last Update : Sat Apr 01 01:50:18 2023

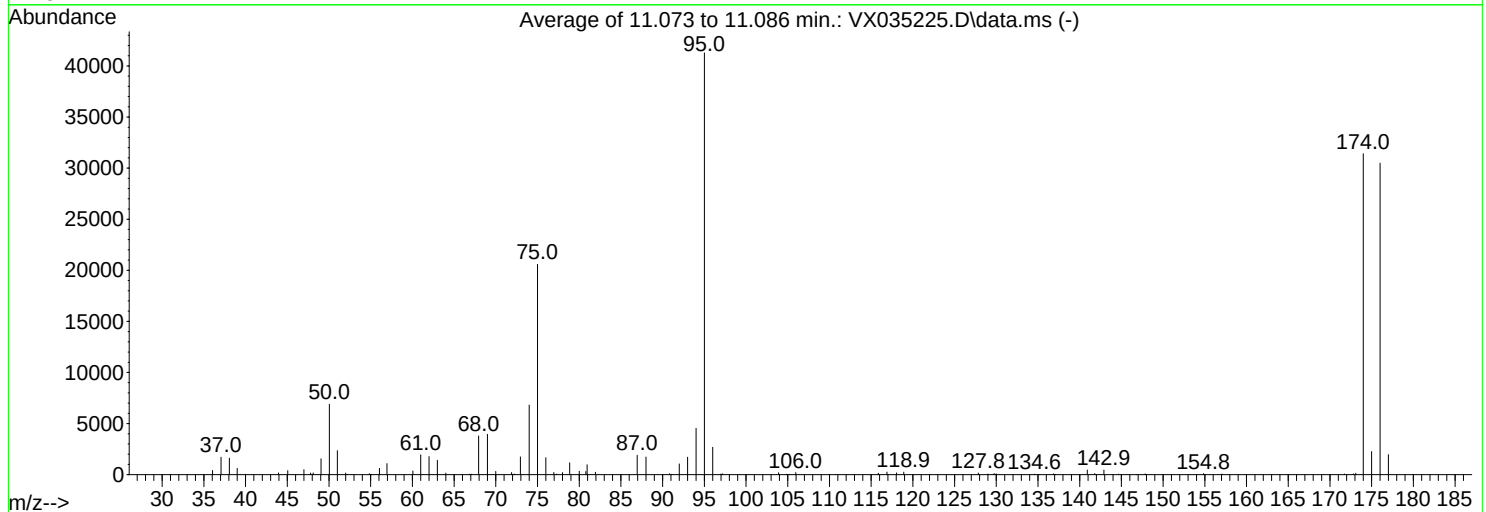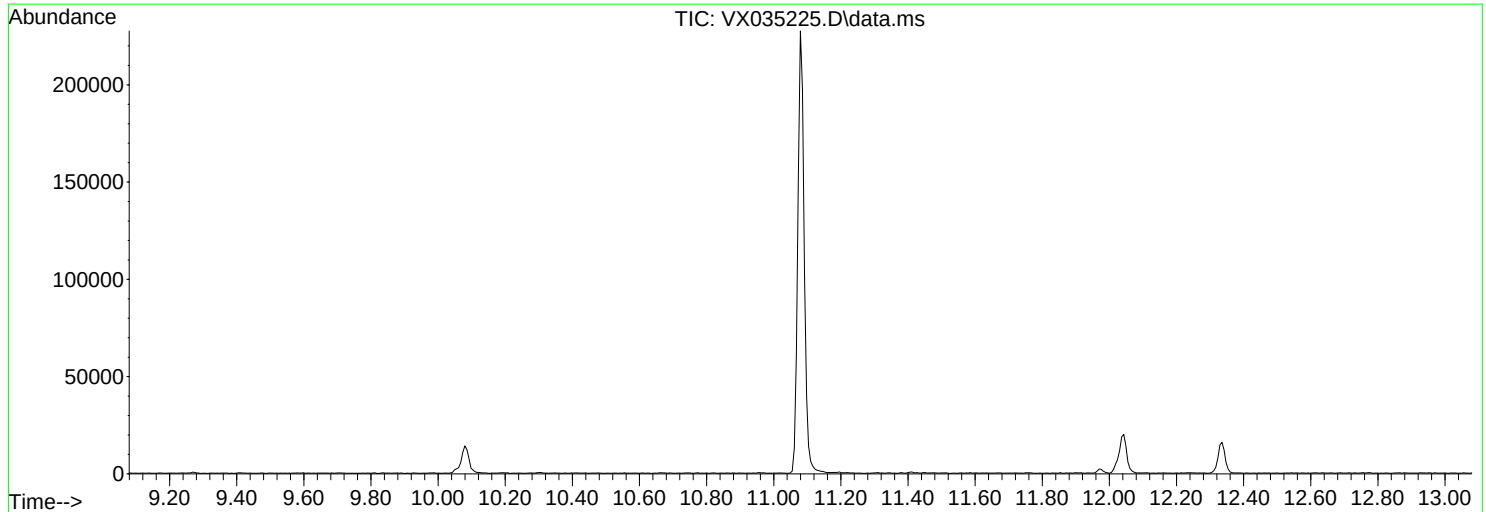

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	6886	PASS
75	95	30	60	49.8	20576	PASS
95	95	100	100	100.0	41280	PASS
96	95	5	9	6.5	2681	PASS
173	174	0.00	2	0.4	134	PASS
174	95	50	100	76.1	31408	PASS
175	174	5	9	7.2	2261	PASS
176	174	95	101	97.1	30493	PASS
177	176	5	9	6.4	1958	PASS