


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX042220\
 Data File : VX015856.D
 Acq On : 22 Apr 2020 21:32
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042220W.M
 Title : SW846 8260
 Last Update : Thu Apr 23 04:36:12 2020

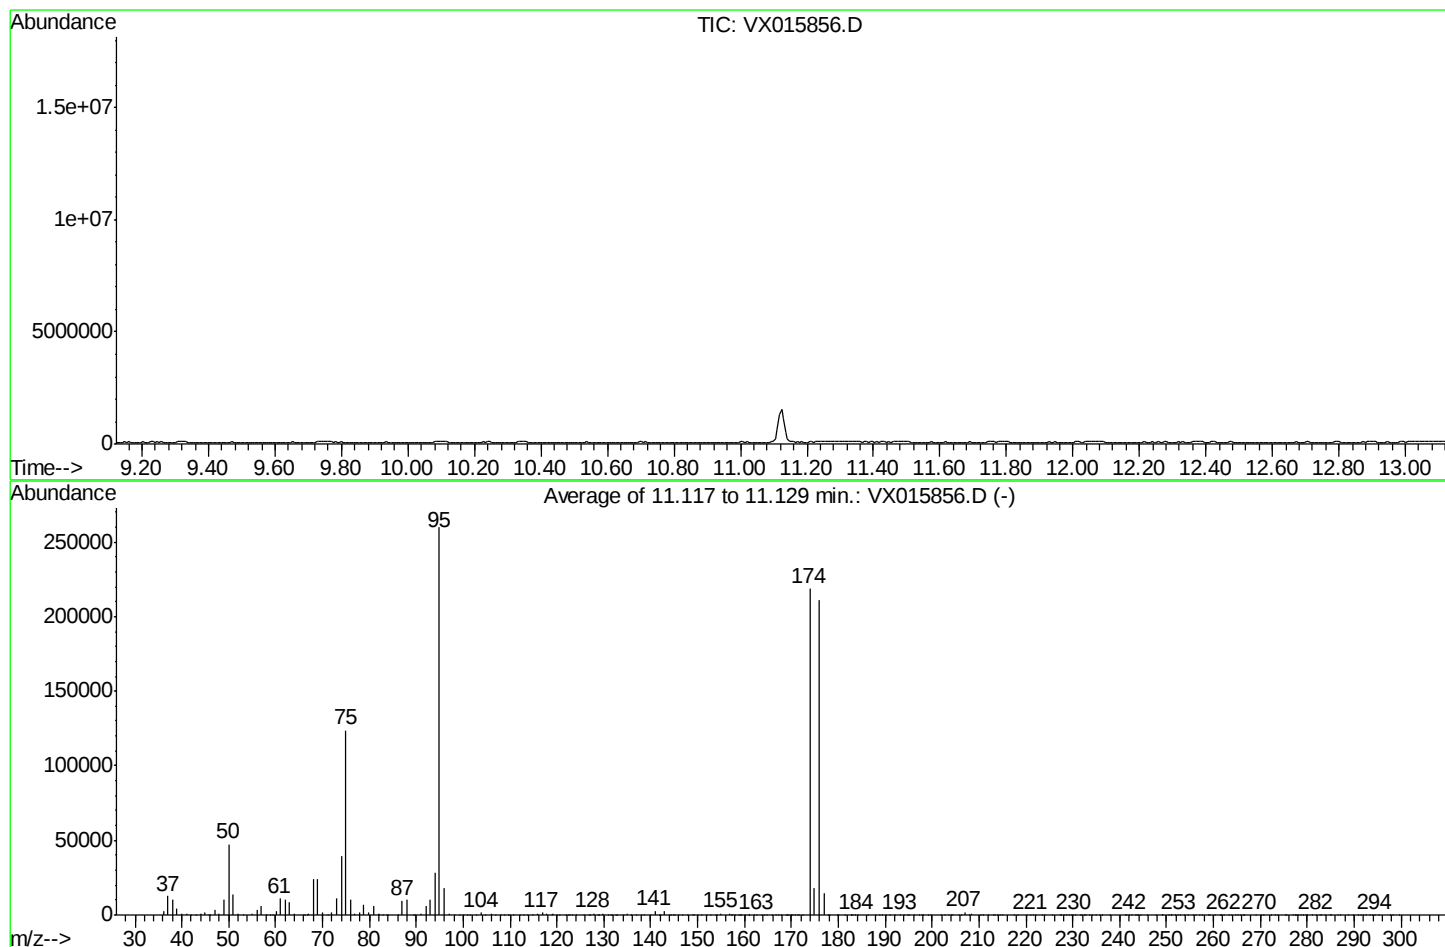

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1669

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	47345	PASS
75	95	30	60	47.7	123939	PASS
95	95	100	100	100.0	259818	PASS
96	95	5	9	7.1	18356	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.1	218585	PASS
175	174	5	9	8.1	17654	PASS
176	174	95	101	96.5	210952	PASS
177	176	5	9	6.9	14539	PASS