

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
 Data File : VX021819.D
 Acq On : 22 Apr 2021 16:11
 Operator : JC/MD
 Sample : M2135-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210421085-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Title : SW846 8260

Signal : TIC: VX021819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.380	45	48	59	rVB	25295	37751	3.57%	0.486%
2	2.166	173	177	184	rVB	31115	44222	4.18%	0.569%
3	2.428	214	220	230	rVB2	26299	48385	4.58%	0.622%
4	3.008	306	315	327	rBV	85125	181343	17.15%	2.332%
5	4.648	572	584	599	rBV	141375	460903	43.59%	5.928%
6	5.087	646	656	670	rBV	146397	440982	41.71%	5.671%
7	5.465	706	718	730	rBV	102571	291180	27.54%	3.745%
8	5.629	734	745	757	rVB	153342	430863	40.75%	5.541%
9	6.031	800	811	820	rBV	96185	250956	23.73%	3.227%
10	6.111	820	824	833	rVB2	10949	27043	2.56%	0.348%
11	6.306	847	856	865	rBV2	5824	15885	1.50%	0.204%
12	6.416	866	874	886	rVB8	4759	15442	1.46%	0.199%
13	6.830	930	942	955	rBV	254241	603930	57.12%	7.767%
14	7.714	1080	1087	1097	rBV	12072	25171	2.38%	0.324%
15	7.952	1121	1126	1134	rBV2	6473	12435	1.18%	0.160%
16	8.696	1240	1248	1254	rBV	548420	859055	81.25%	11.048%
17	8.763	1254	1259	1267	rVB3	18249	35844	3.39%	0.461%
18	8.848	1268	1273	1277	rBV	12792	18363	1.74%	0.236%
19	9.415	1359	1366	1373	rBV	21787	33609	3.18%	0.432%
20	9.531	1380	1385	1391	rVB	20642	28689	2.71%	0.369%
21	10.092	1468	1477	1490	rBV2	586798	1034041	97.80%	13.298%
22	10.238	1496	1501	1506	rBV2	10545	22753	2.15%	0.293%
23	10.342	1512	1518	1524	rVB	64493	94051	8.89%	1.210%
24	10.683	1569	1574	1580	rVB	58454	80842	7.65%	1.040%
25	11.000	1620	1626	1631	rBV	22219	30828	2.92%	0.396%
26	11.122	1640	1646	1652	rBV	507727	676766	64.01%	8.704%
27	11.409	1689	1693	1701	rBV3	15094	33479	3.17%	0.431%
28	11.488	1701	1706	1710	rVB	10727	14412	1.36%	0.185%
29	11.652	1728	1733	1741	rVB	32206	46494	4.40%	0.598%
30	11.787	1745	1755	1760	rBV	43509	60331	5.71%	0.776%
31	11.927	1770	1778	1786	rVB2	28868	43122	4.08%	0.555%
32	12.061	1793	1800	1807	rBV2	739217	1057352	100.00%	13.598%
33	12.128	1807	1811	1816	rBV	28557	39385	3.72%	0.507%
34	12.280	1829	1836	1840	rBV2	73061	98063	9.27%	1.261%
35	12.372	1845	1851	1859	rVB5	13652	28412	2.69%	0.365%
36	12.451	1859	1864	1869	rBV3	13317	23168	2.19%	0.298%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
 Data File : VX021819.D
 Acq On : 22 Apr 2021 16:11
 Operator : JC/MD
 Sample : M2135-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 210421085-02-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Title : SW846 8260

37	12.579	1878	1885	1892	rVB2	8680	21228	2.01%	0.273%
38	12.652	1893	1897	1900	rVB	16347	17545	1.66%	0.226%
39	12.884	1927	1935	1937	rBV6	5766	13073	1.24%	0.168%
40	12.945	1941	1945	1950	rVV2	42515	66777	6.32%	0.859%
41	13.000	1950	1954	1957	rVB3	16884	24834	2.35%	0.319%
42	13.329	2003	2008	2012	rBV2	27374	37593	3.56%	0.483%
43	13.463	2026	2030	2033	rBV2	18200	21958	2.08%	0.282%
44	13.512	2033	2038	2042	rBV2	33726	46068	4.36%	0.592%
45	13.628	2051	2057	2061	rBV6	10480	17552	1.66%	0.226%
46	13.817	2082	2088	2093	rVB	78950	103142	9.75%	1.326%
47	13.908	2096	2103	2108	rBV	7330	14234	1.35%	0.183%
48	13.969	2108	2113	2118	rBV5	13437	26895	2.54%	0.346%
49	14.676	2226	2229	2232	rBV2	20652	30858	2.92%	0.397%
50	14.701	2232	2233	2238	rVB3	17730	17223	1.63%	0.221%
51	14.816	2248	2252	2261	rVB2	22555	33101	3.13%	0.426%
52	16.146	2463	2470	2478	rBV4	6807	13211	1.25%	0.170%
53	16.383	2504	2509	2517	rVB2	13244	24822	2.35%	0.319%




Sum of corrected areas: 7775664

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021819.D
Acq On : 22 Apr 2021 16:11
Operator : JC/MD
Sample : M2135-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210421085-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

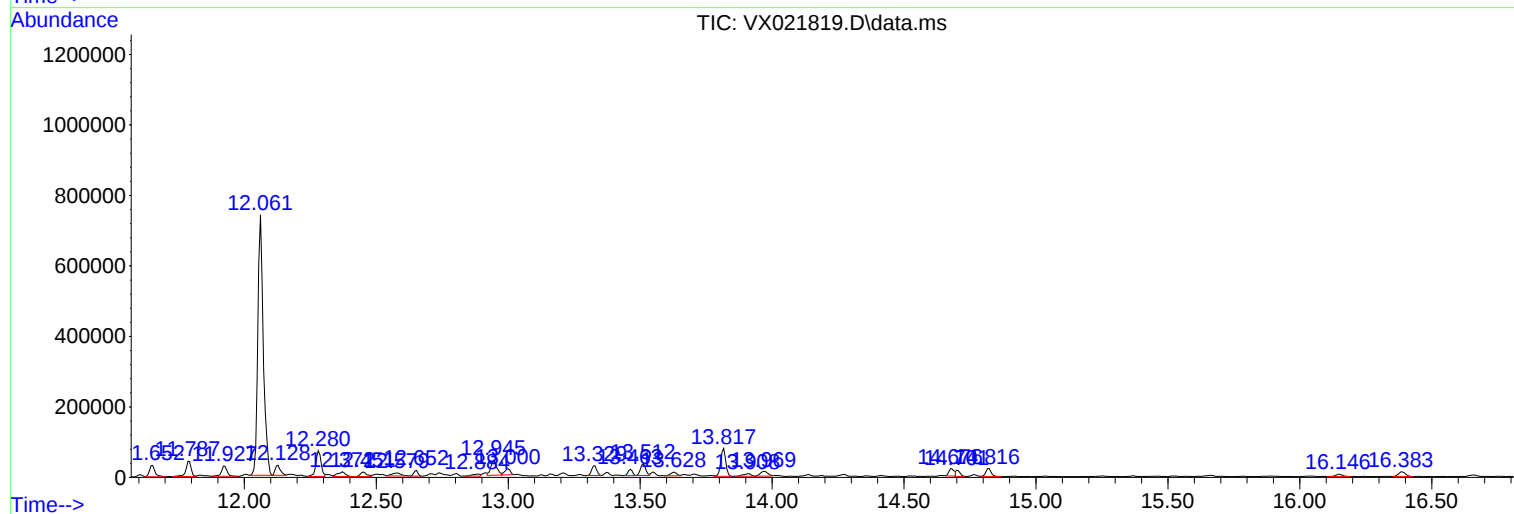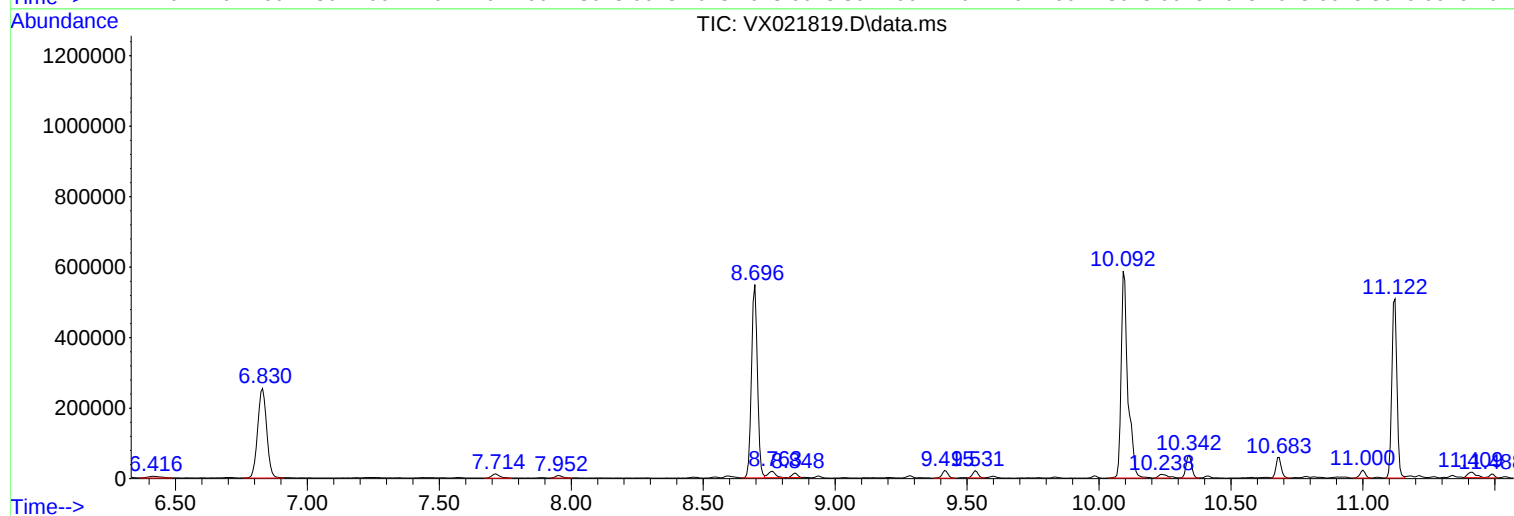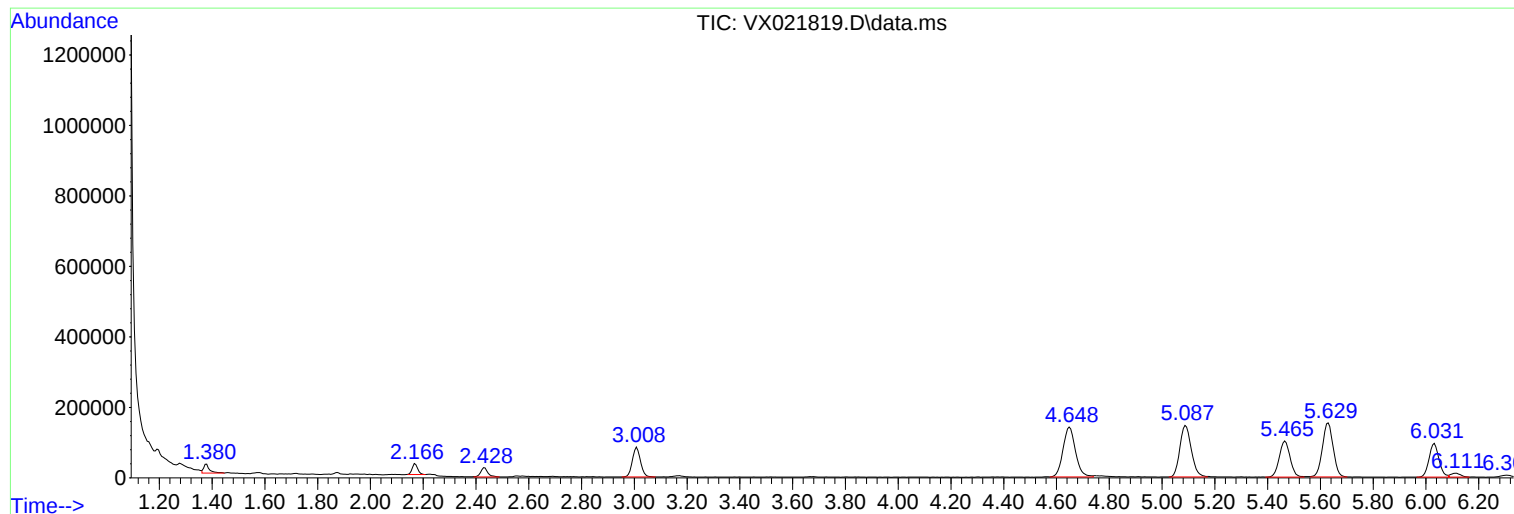

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021819.D
Acq On : 22 Apr 2021 16:11
Operator : JC/MD
Sample : M2135-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210421085-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021819.D
Acq On : 22 Apr 2021 16:11
Operator : JC/MD
Sample : M2135-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
210421085-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
