

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
 Data File : VX021825.D
 Acq On : 22 Apr 2021 18:27
 Operator : JC/MD
 Sample : M2138-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-2-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M

Title : SW846 8260

Signal : TIC: VX021825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.464	708	718	733	rVB	102409	288849	2.17%	1.564%
2	5.629	733	745	758	rBV	154164	427655	3.21%	2.316%
3	6.031	800	811	823	rBV	94917	246065	1.85%	1.333%
4	6.830	932	942	957	rBV	253634	600600	4.51%	3.252%
5	8.695	1241	1248	1261	rBV	547690	854136	6.41%	4.625%
6	9.317	1343	1350	1374	rVB	9117942	13322522	100.00%	72.146%
7	10.091	1471	1477	1491	rBV	589681	821438	6.17%	4.448%
8	11.122	1640	1646	1656	rVB	526702	685291	5.14%	3.711%
9	12.061	1794	1800	1809	rVB	749865	920044	6.91%	4.982%
10	12.579	1879	1885	1891	rVB	235476	299386	2.25%	1.621%




Sum of corrected areas: 18465986

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021825.D
Acq On : 22 Apr 2021 18:27
Operator : JC/MD
Sample : M2138-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

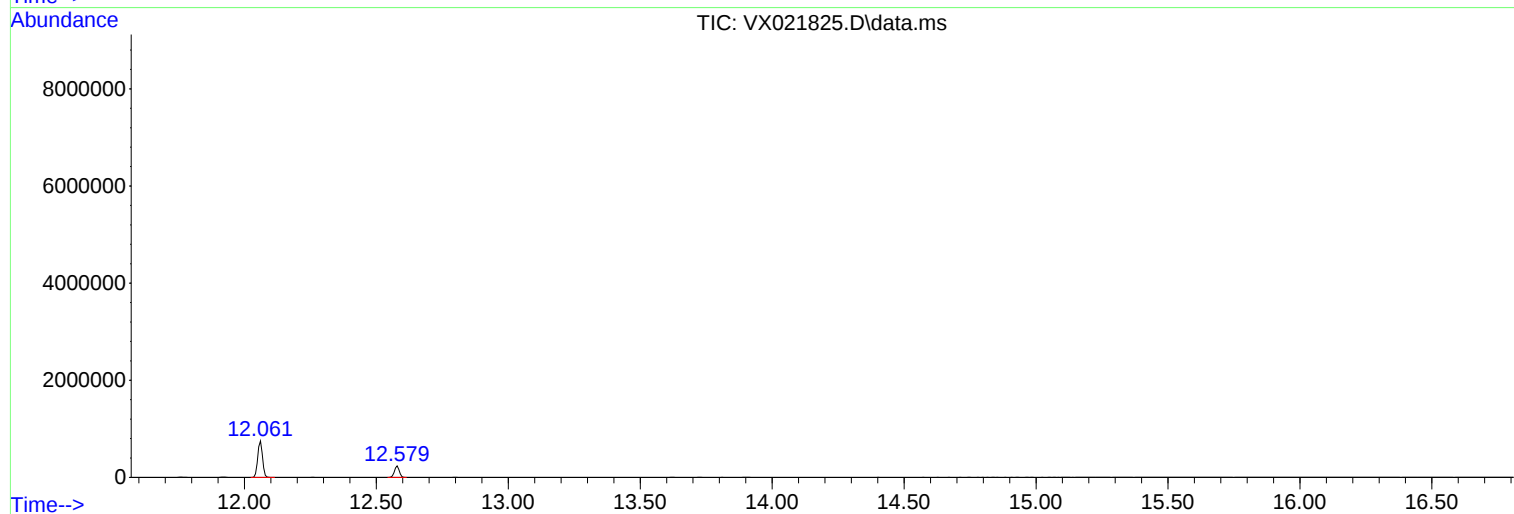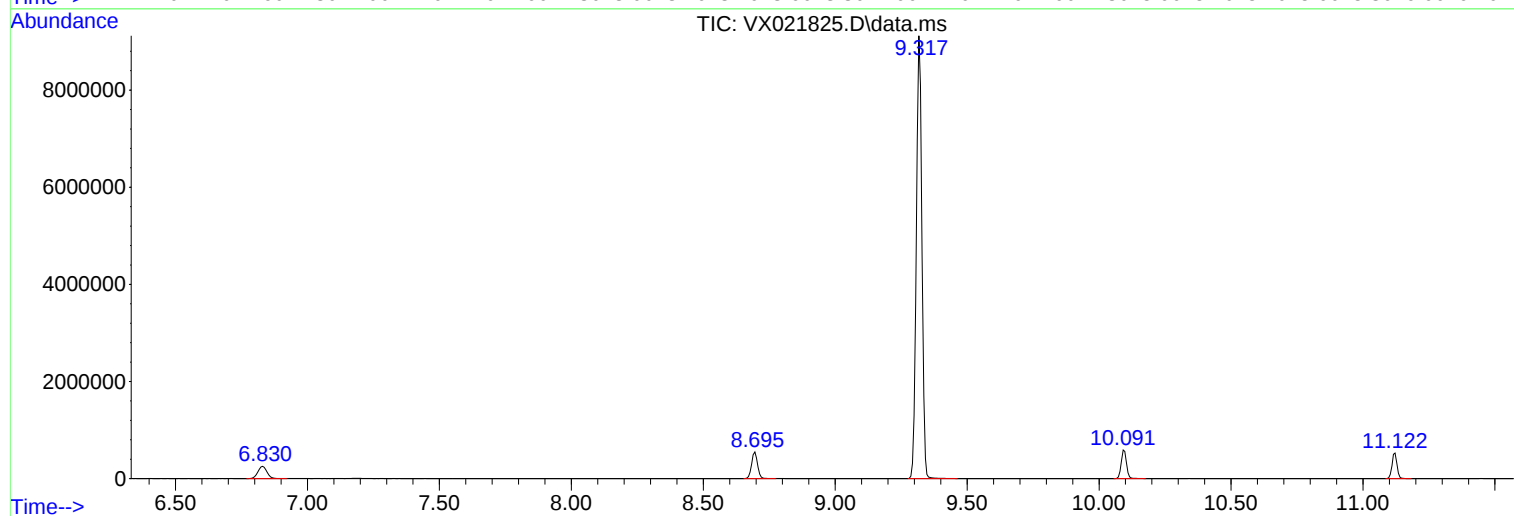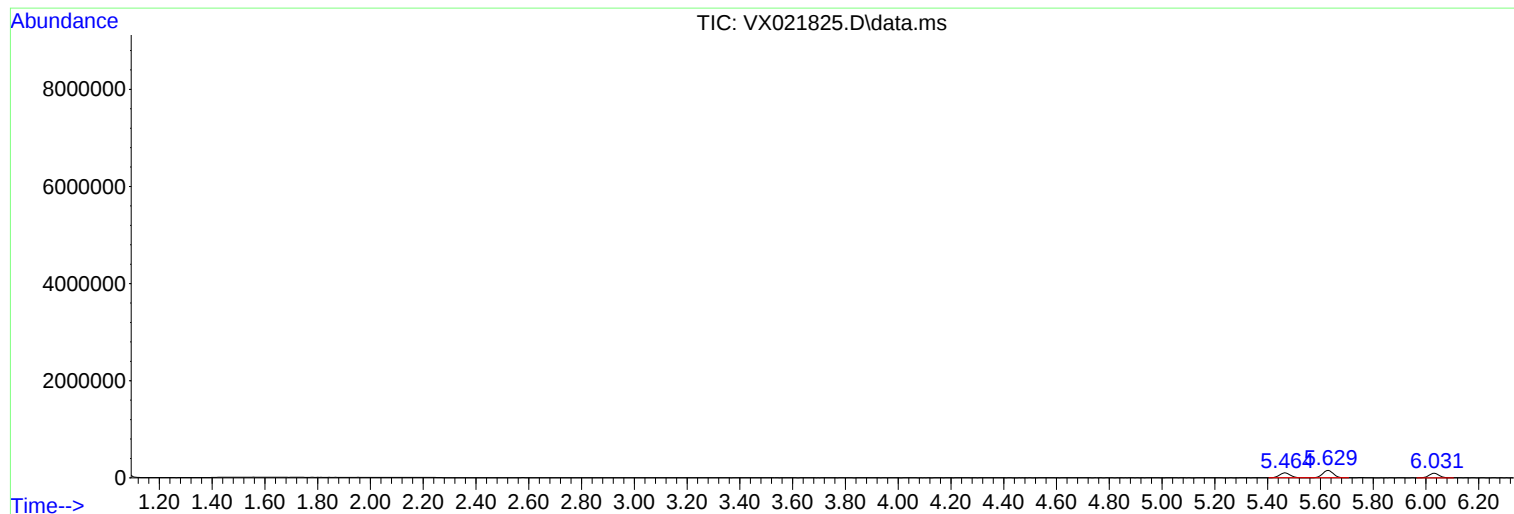

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021825.D
Acq On : 22 Apr 2021 18:27
Operator : JC/MD
Sample : M2138-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021825.D
Acq On : 22 Apr 2021 18:27
Operator : JC/MD
Sample : M2138-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
