

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
 Data File : VX021827.D
 Acq On : 22 Apr 2021 19:13
 Operator : JC/MD
 Sample : M2138-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-2-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M

Title : SW846 8260

Signal : TIC: VX021827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.581	240	245	251	rBV	10514	17443	2.02%	0.379%
2	5.464	707	718	733	rVB2	95478	270096	31.34%	5.861%
3	5.629	733	745	758	rBV	144808	400684	46.49%	8.695%
4	6.031	800	811	824	rBV	87924	231811	26.90%	5.030%
5	6.830	932	942	956	rBV	240807	563861	65.43%	12.236%
6	8.695	1239	1248	1270	rBV	507264	810180	94.01%	17.581%
7	9.317	1344	1350	1358	rVB	26059	39335	4.56%	0.854%
8	10.092	1471	1477	1493	rVB	550318	769902	89.33%	16.707%
9	11.122	1640	1646	1658	rVB	490068	643131	74.62%	13.956%
10	12.061	1794	1800	1810	rVB	701661	861832	100.00%	18.702%




Sum of corrected areas: 4608275

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021827.D
Acq On : 22 Apr 2021 19:13
Operator : JC/MD
Sample : M2138-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

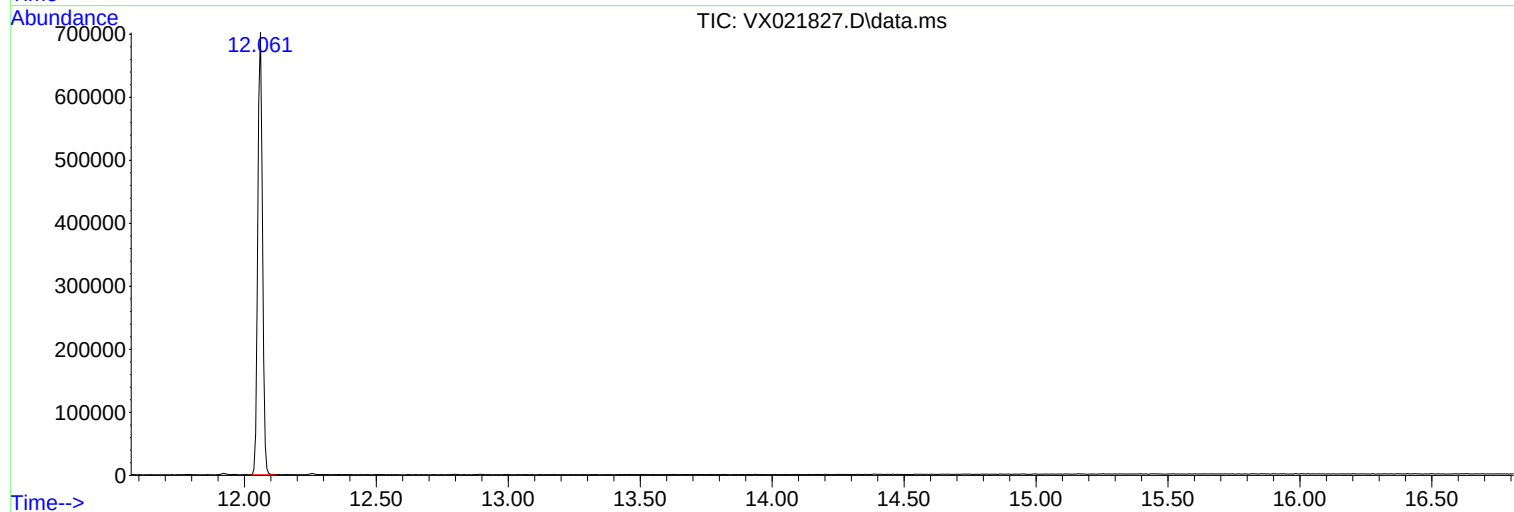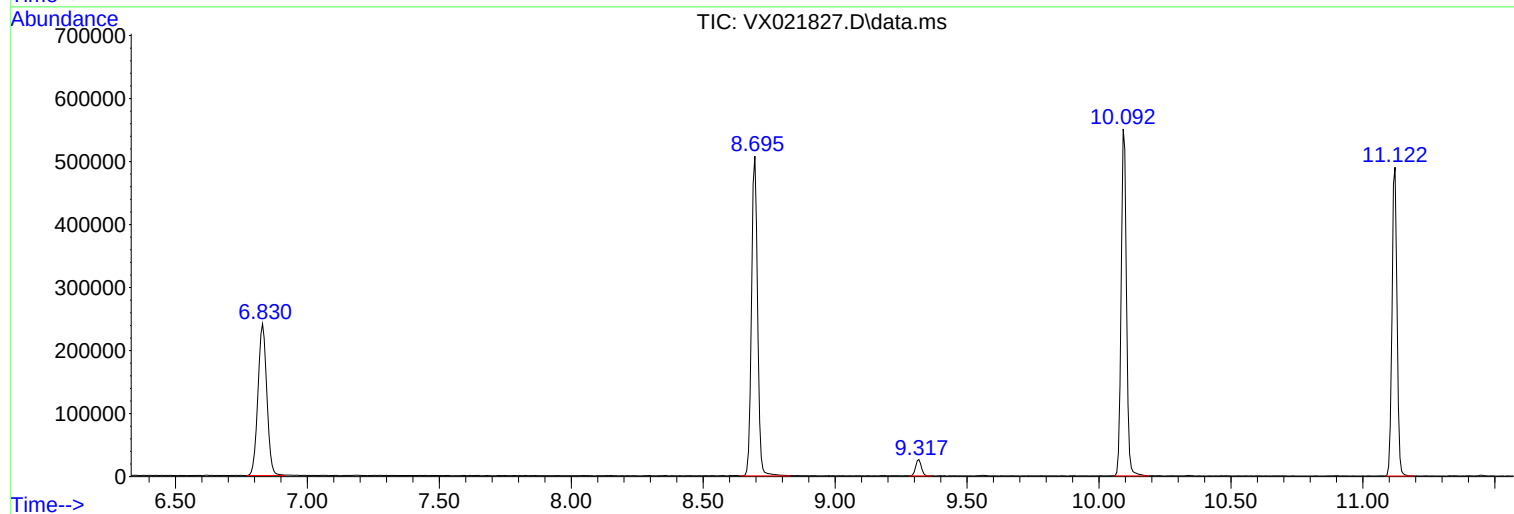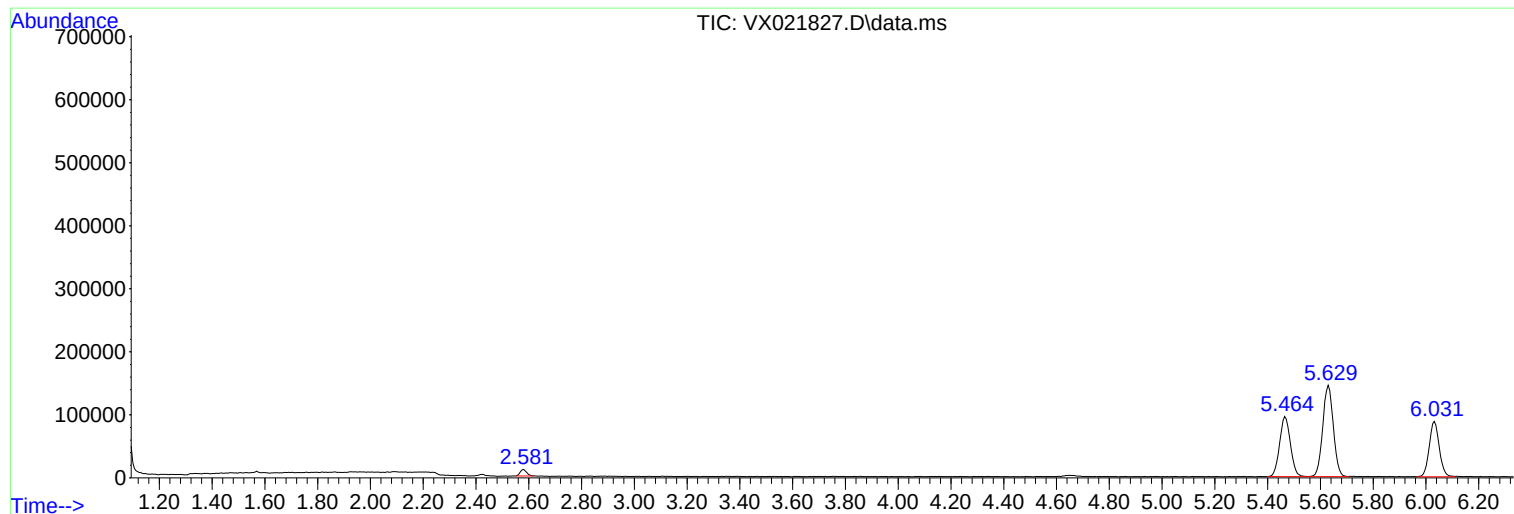

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021827.D
Acq On : 22 Apr 2021 19:13
Operator : JC/MD
Sample : M2138-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
Data File : VX021827.D
Acq On : 22 Apr 2021 19:13
Operator : JC/MD
Sample : M2138-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
