
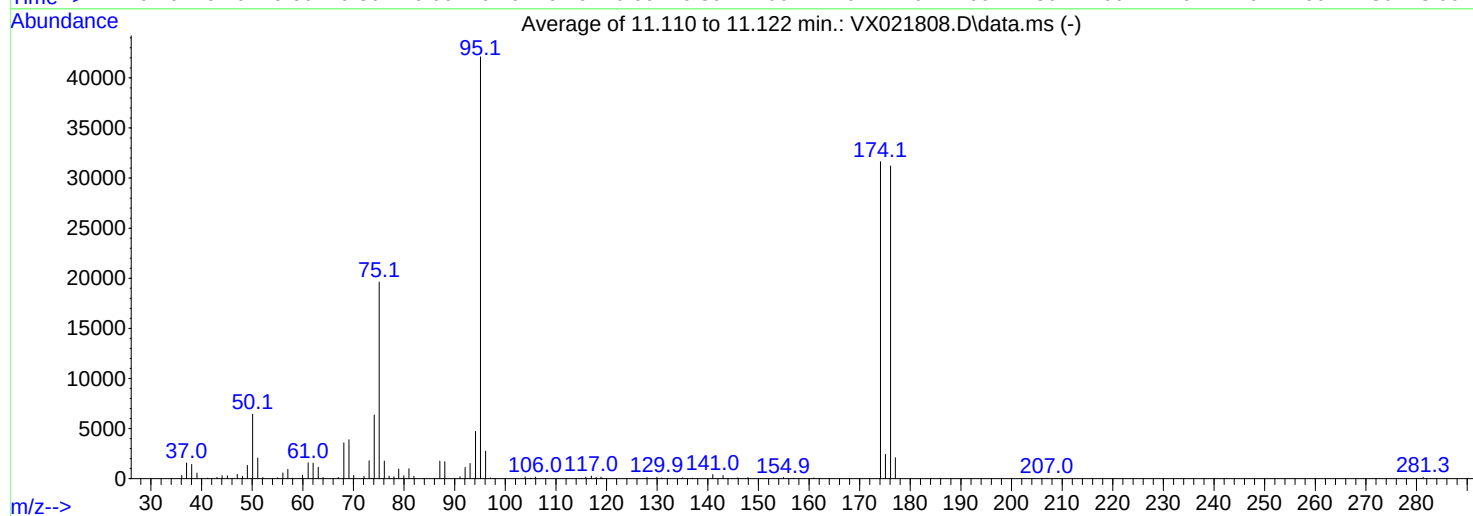


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042221\
 Data File : VX021808.D
 Acq On : 22 Apr 2021 10:16
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Title : SW846 8260
 Last Update : Tue Apr 20 13:46:22 2021

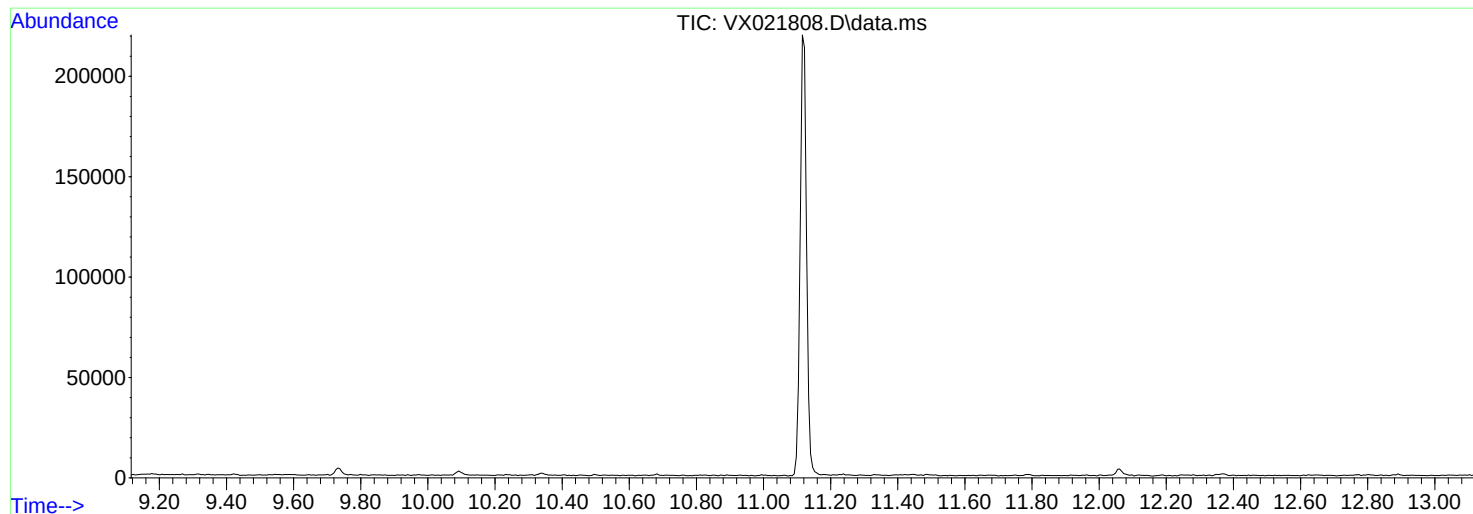

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	6440	PASS
75	95	30	60	46.6	19625	PASS
95	95	100	100	100.0	42099	PASS
96	95	5	9	6.5	2744	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.1	31632	PASS
175	174	5	9	7.7	2432	PASS
176	174	95	101	98.7	31213	PASS
177	176	5	9	6.7	2092	PASS