


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042222\
Data File : VX028271.D
Acq On : 22 Apr 2022 09:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Title : SW846 8260
Last Update : Tue Apr 19 13:38:04 2022

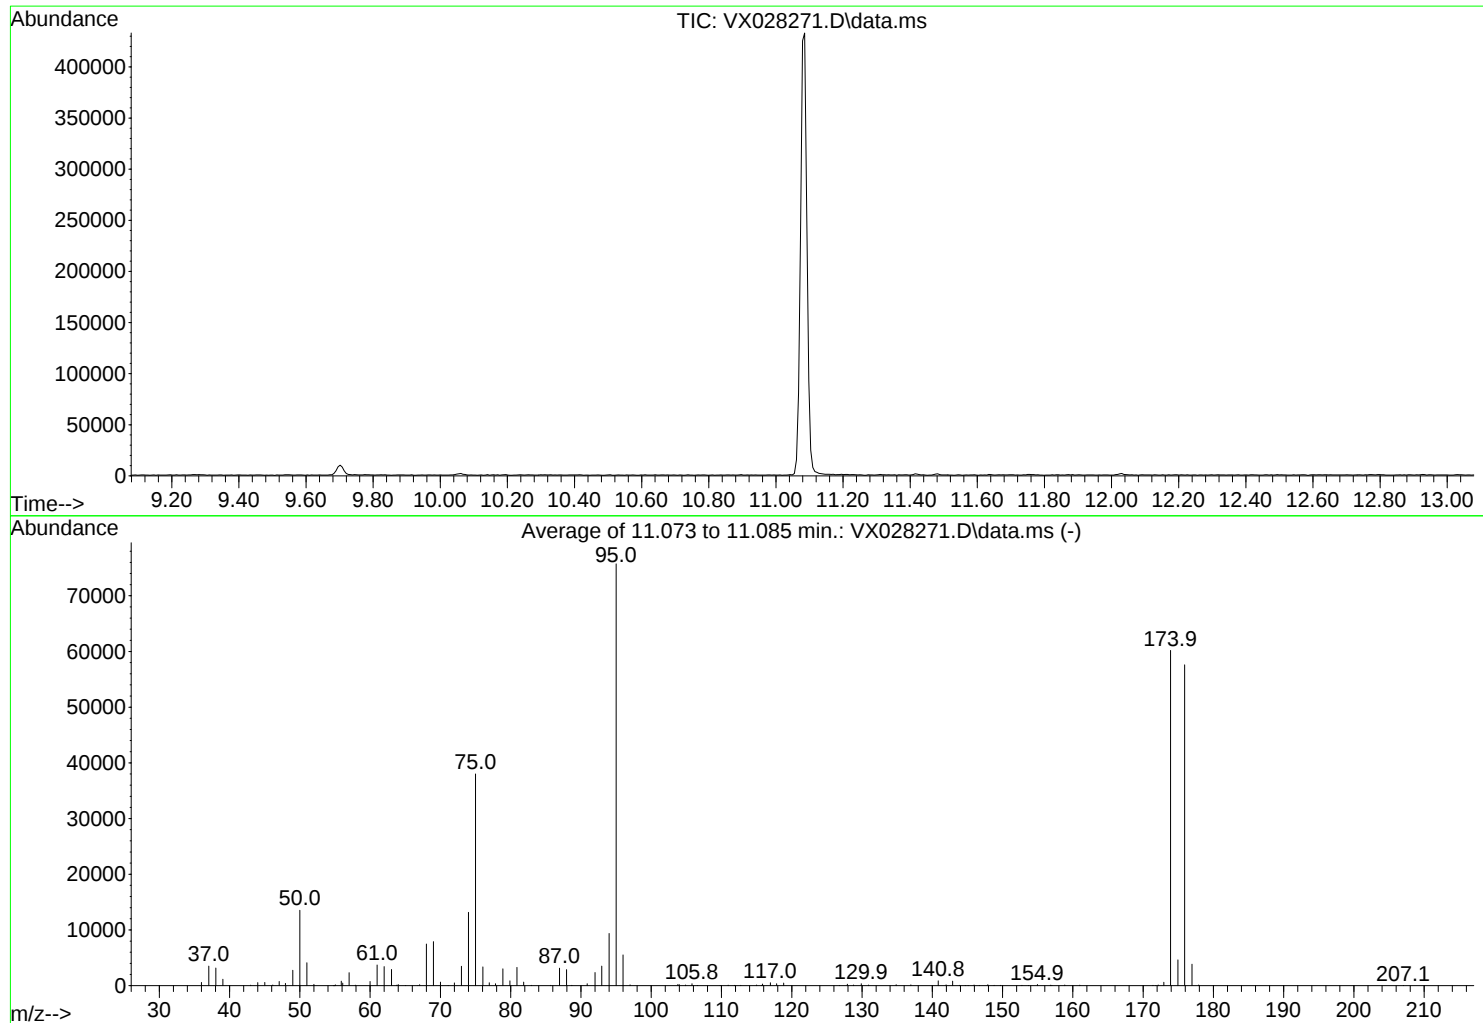

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	13537	PASS
75	95	30	60	50.2	38000	PASS
95	95	100	100	100.0	75736	PASS
96	95	5	9	7.3	5507	PASS
173	174	0.00	2	1.0	610	PASS
174	95	50	100	79.5	60187	PASS
175	174	5	9	7.7	4632	PASS
176	174	95	101	95.7	57595	PASS
177	176	5	9	6.7	3844	PASS