

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042225\
 Data File : VX045876.D
 Acq On : 22 Apr 2025 10:57
 Operator : JC/MD
 Sample : VX0422MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0422MBL01

Quant Time: Apr 23 01:32:43 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	72362	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	143754	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	134942	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	58418	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	69648	52.632	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.260%
35) Dibromofluoromethane	5.373	113	51990	50.974	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.940%
50) Toluene-d8	8.647	98	179619	50.455	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.920%
62) 4-Bromofluorobenzene	11.079	95	69421	53.536	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	107.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042225\
Data File : VX045876.D
Acq On : 22 Apr 2025 10:57
Operator : JC/MD
Sample : VX0422MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0422MBL01

Quant Time: Apr 23 01:32:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




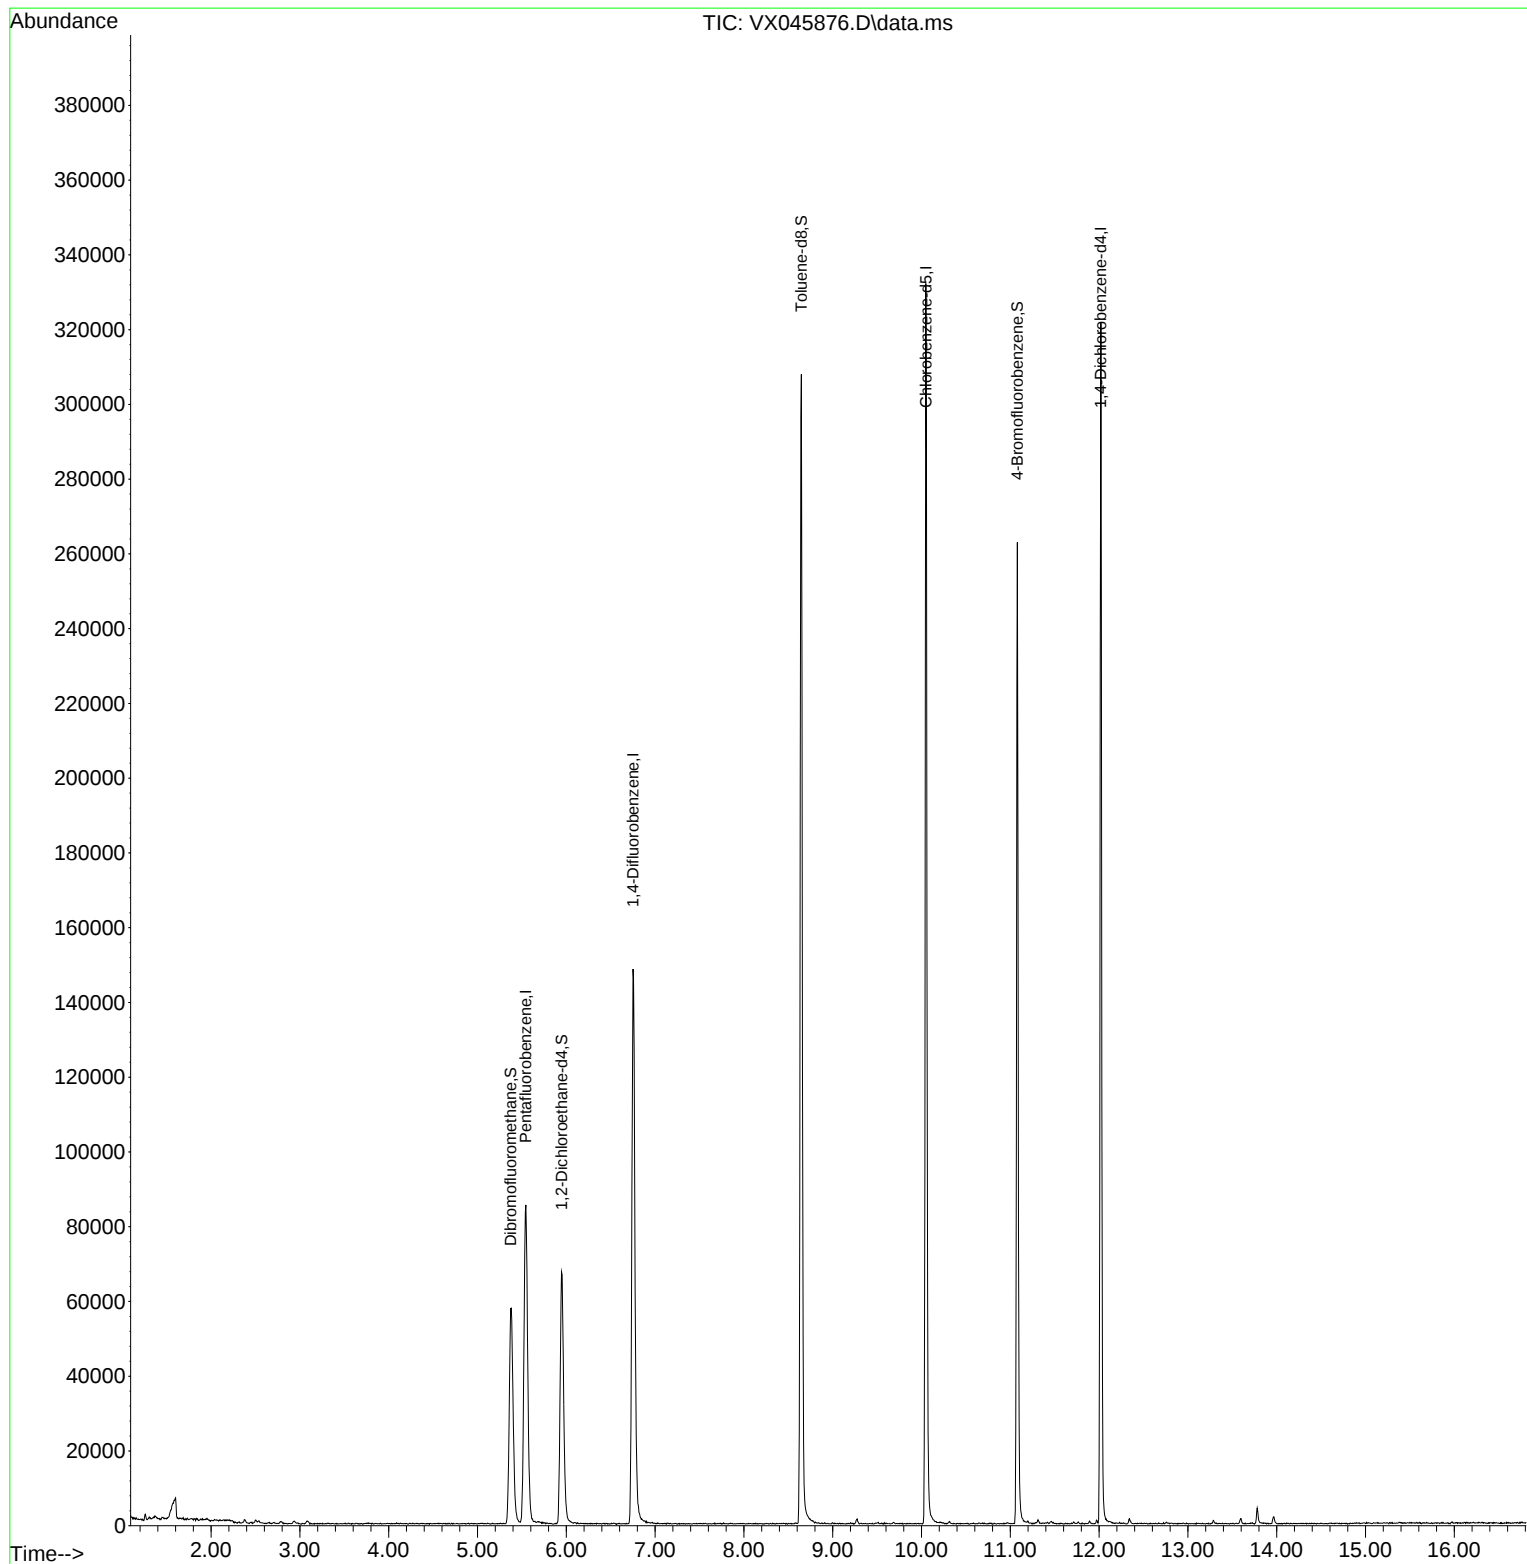


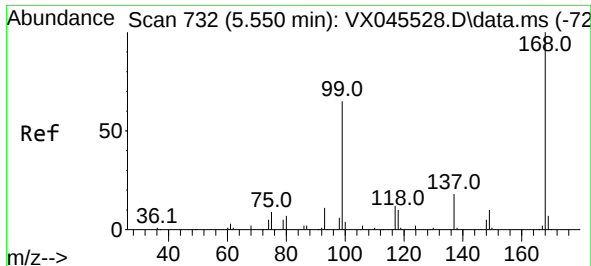

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0422MBL01


Tgt Ion:168 Resp: 72362
Ion Ratio Lower Upper
168 100
99 76.8 52.3 78.5

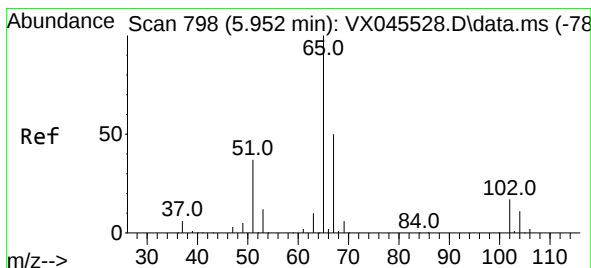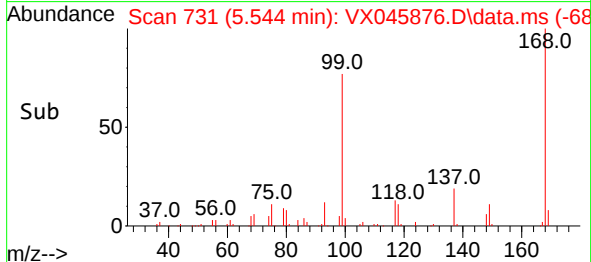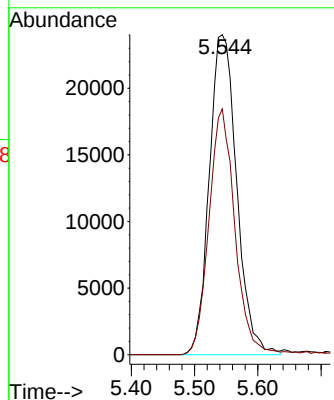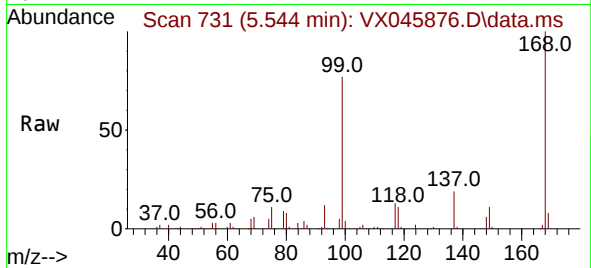

#33
1,2-Dichloroethane-d4
Concen: 52.632 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57

Tgt Ion: 65 Resp: 69648
Ion Ratio Lower Upper
65 100
67 49.3 0.0 99.0


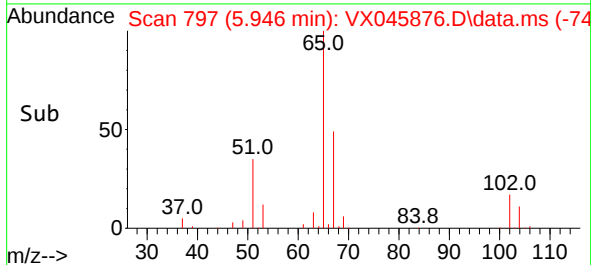
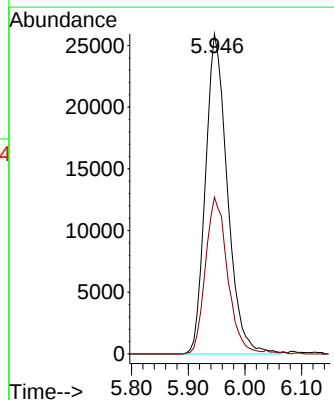
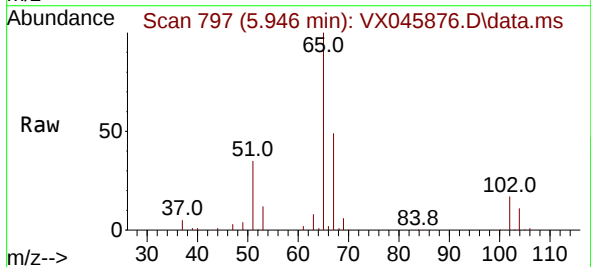


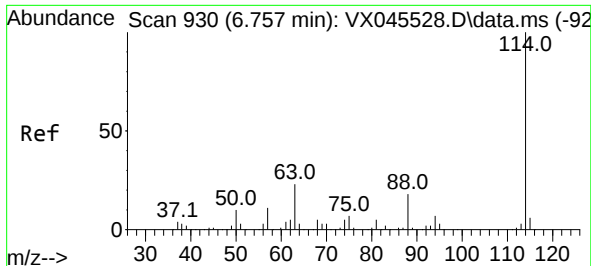

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0422MBL01


Tgt Ion:114 Resp: 143754
Ion Ratio Lower Upper
114 100
63 24.1 0.0 46.8
88 17.7 0.0 35.4

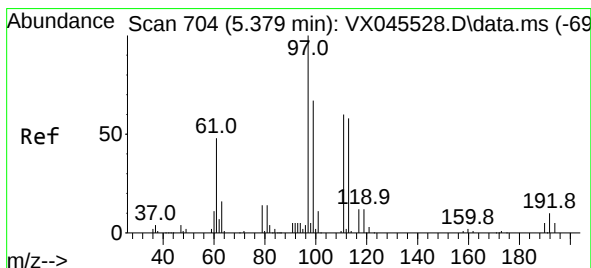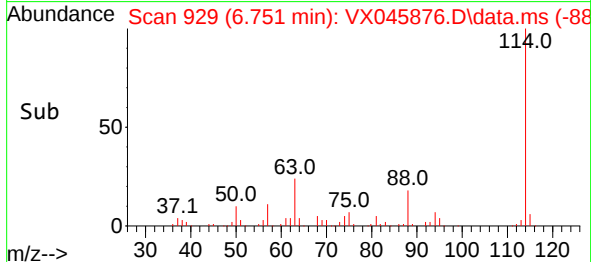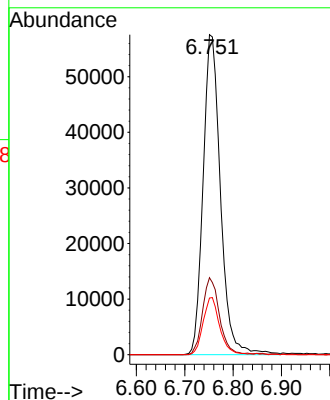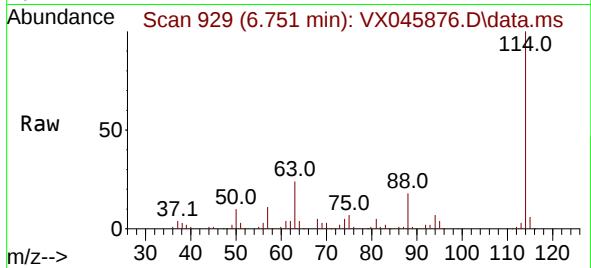

#35
Dibromofluoromethane
Concen: 50.974 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57

Tgt Ion:113 Resp: 51990
Ion Ratio Lower Upper
113 100
111 102.2 81.8 122.6
192 16.5 13.8 20.6


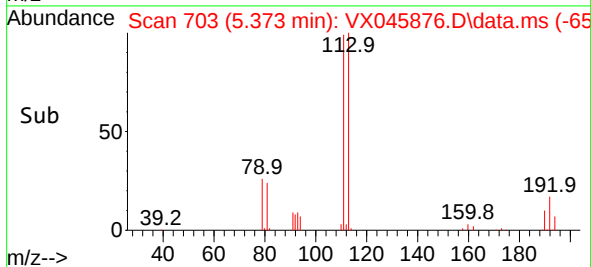
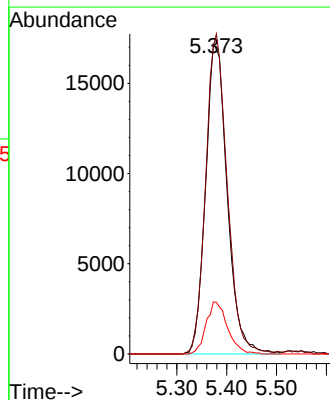
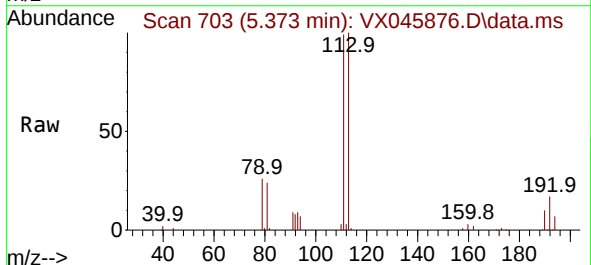


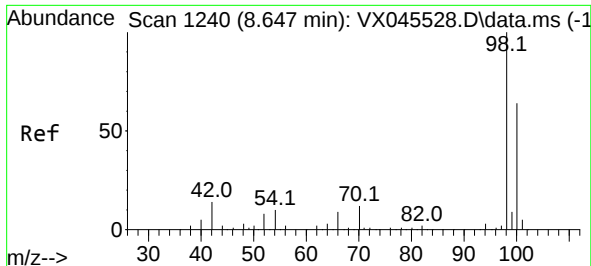

#50
Toluene-d8
Concen: 50.455 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57




Instrument :
MSVOA_X
ClientSampleId :
VX0422MBL01


Tgt Ion: 98 Resp: 179619
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.4

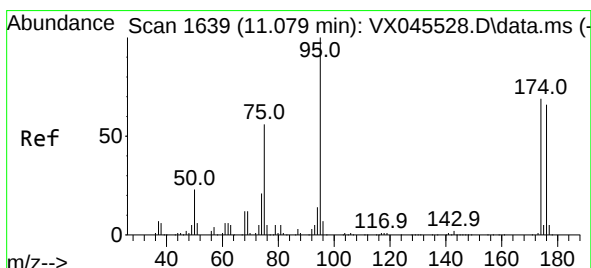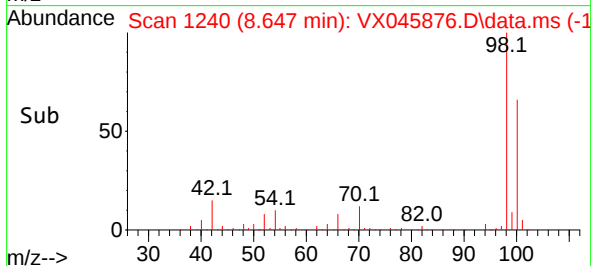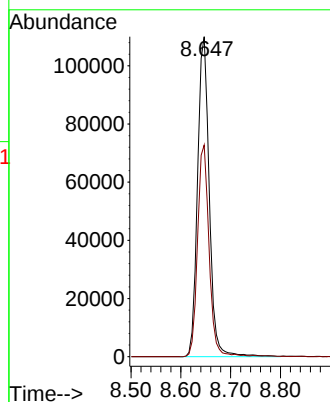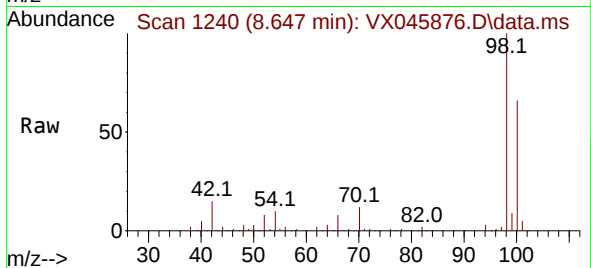

#62
4-Bromofluorobenzene
Concen: 53.536 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57

Tgt Ion: 95 Resp: 69421
Ion Ratio Lower Upper
95 100
174 67.6 0.0 135.8
176 65.4 0.0 131.4


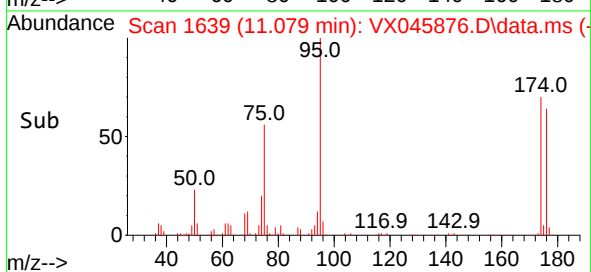
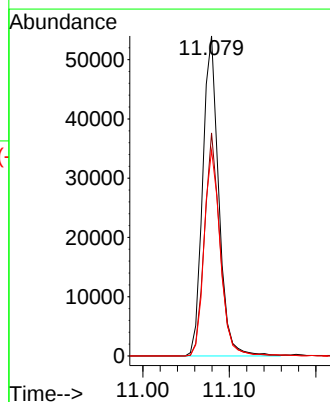
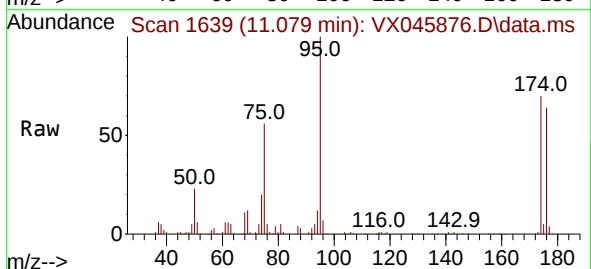


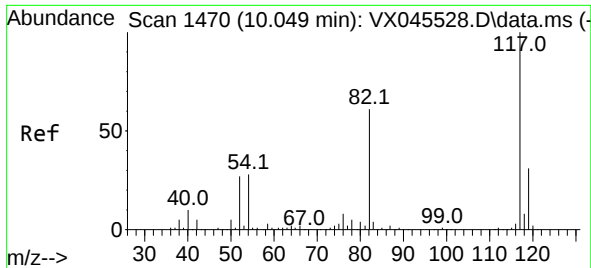

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57

Instrument :
MSVOA_X
ClientSampleId :
VX0422MBL01

Tgt Ion:117 Resp: 134942
Ion Ratio Lower Upper
117 100
82 63.3 49.2 73.8
119 31.7 25.1 37.7

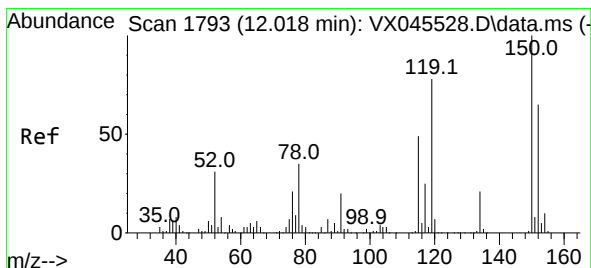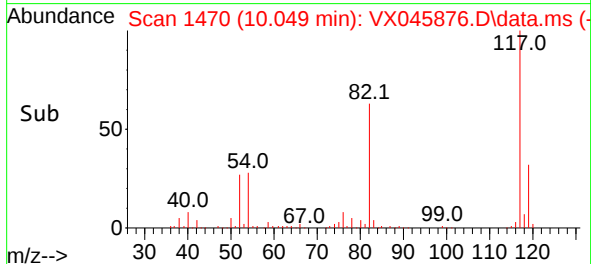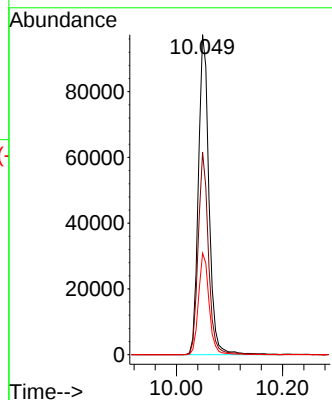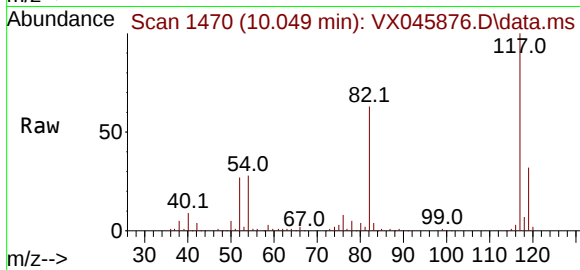

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045876.D
Acq: 22 Apr 2025 10:57

Tgt Ion:152 Resp: 58418
Ion Ratio Lower Upper
152 100
115 66.5 46.9 140.7
150 159.3 0.0 349.4

