

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042225\
 Data File : VX045877.D
 Acq On : 22 Apr 2025 11:20
 Operator : JC/MD
 Sample : VX0422WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0422WBL01

Quant Time: Apr 23 01:32:55 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	68849	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	131344	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	120785	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	49782	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	65353	51.906	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	103.820%
35) Dibromofluoromethane	5.379	113	47028	50.465	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.940%
50) Toluene-d8	8.647	98	163738	50.340	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.680%
62) 4-Bromofluorobenzene	11.079	95	60979	51.469	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	102.940%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042225\
Data File : VX045877.D
Acq On : 22 Apr 2025 11:20
Operator : JC/MD
Sample : VX0422WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0422WBL01

Quant Time: Apr 23 01:32:55 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




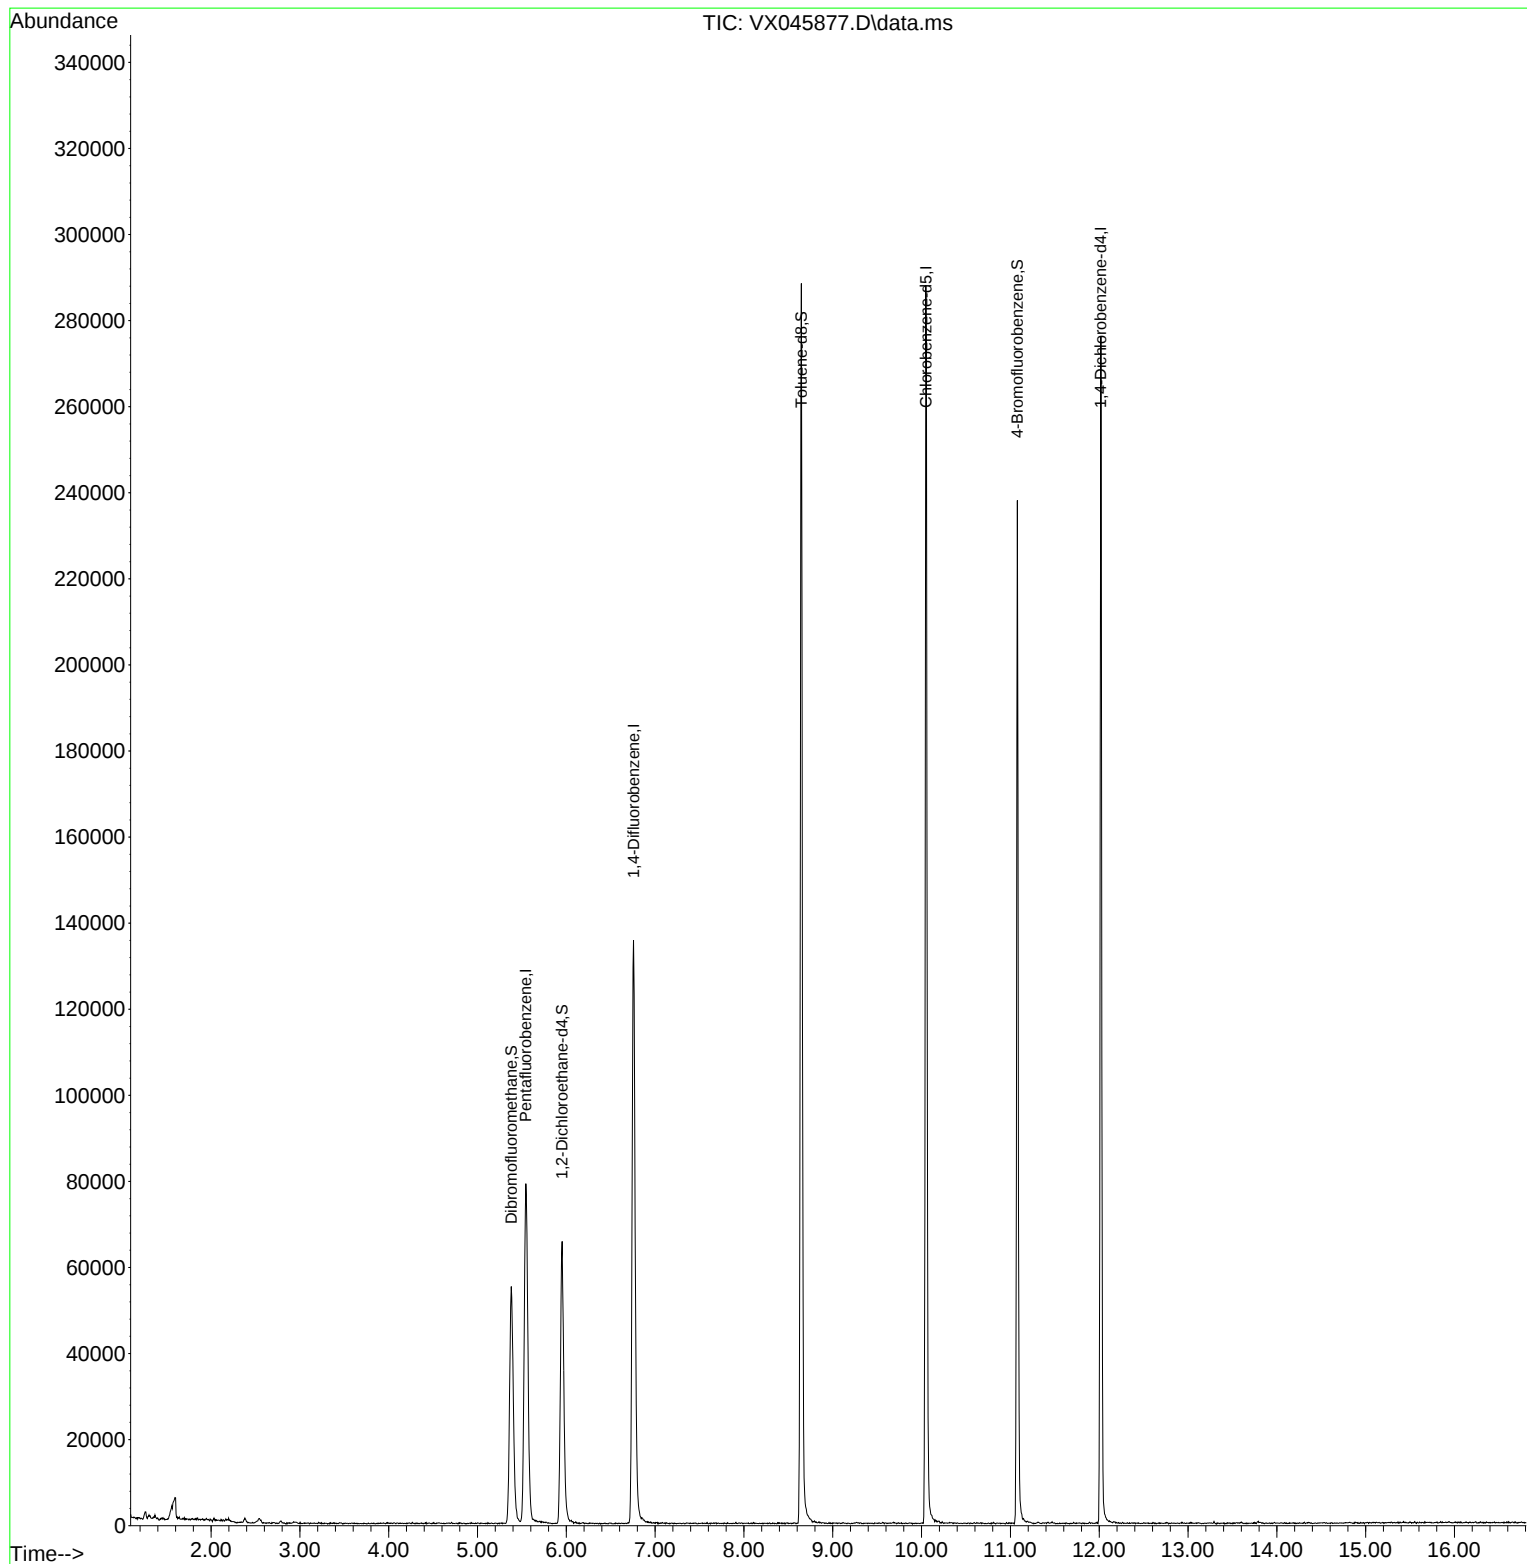




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20




Instrument :
MSVOA_X
ClientSampleId :
VX0422WBL01

Tgt Ion:168 Resp: 68849
Ion Ratio Lower Upper
168 100
99 74.7 52.3 78.5

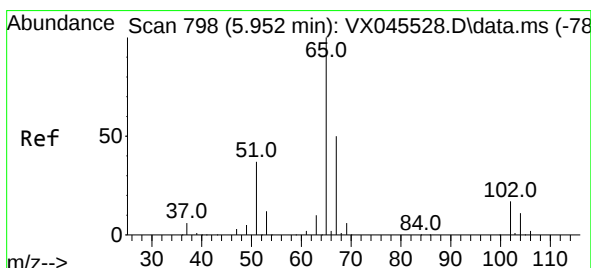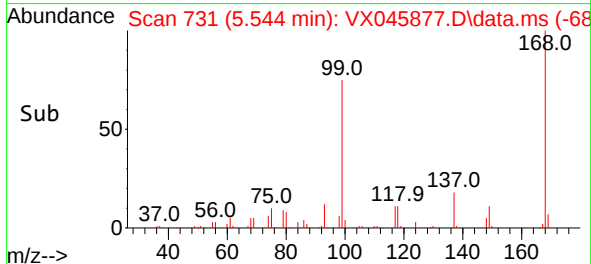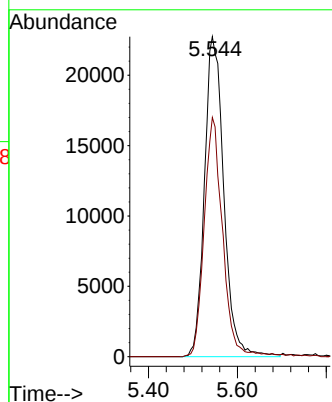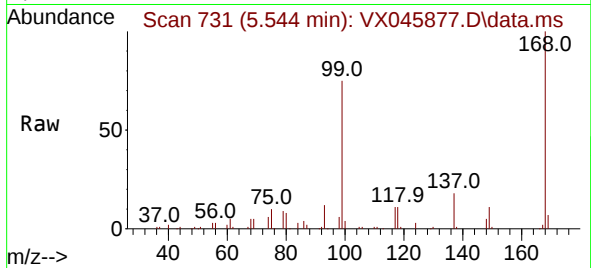

#33
1,2-Dichloroethane-d4
Concen: 51.906 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20

Tgt Ion: 65 Resp: 65353
Ion Ratio Lower Upper
65 100
67 48.7 0.0 99.0

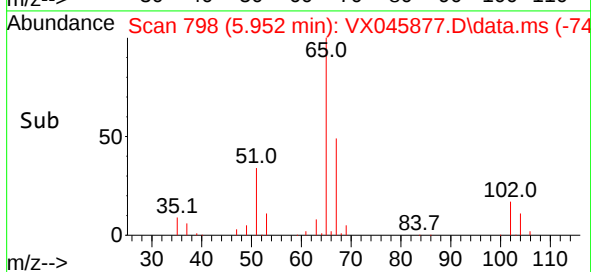
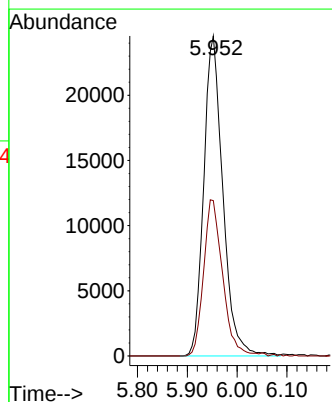
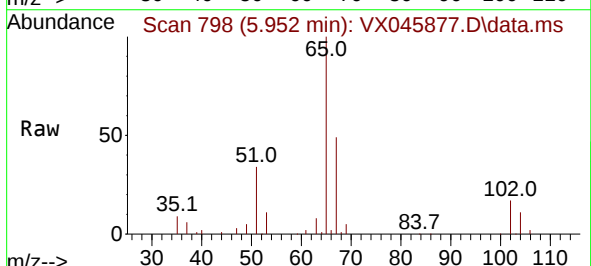




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 913
Delta R.T. 0.000 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20




Instrument :
MSVOA_X
ClientSampleId :
VX0422WBL01


Tgt Ion:114 Resp: 131344
Ion Ratio Lower Upper
114 100
63 23.5 0.0 46.8
88 16.2 0.0 35.4

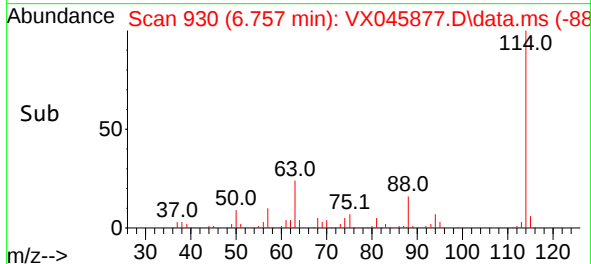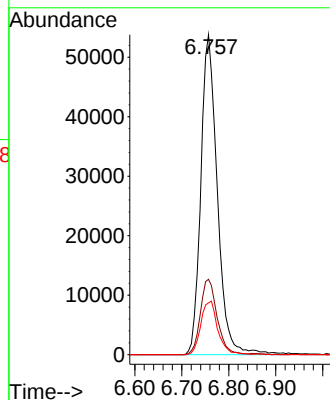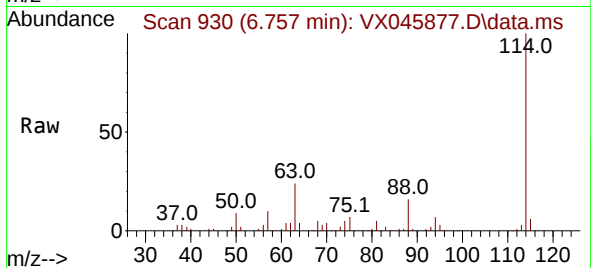

#35
Dibromofluoromethane
Concen: 50.465 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20

Tgt Ion:113 Resp: 47028
Ion Ratio Lower Upper
113 100
111 103.1 81.8 122.6
192 16.8 13.8 20.6

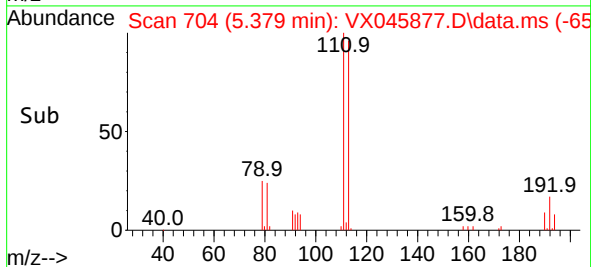
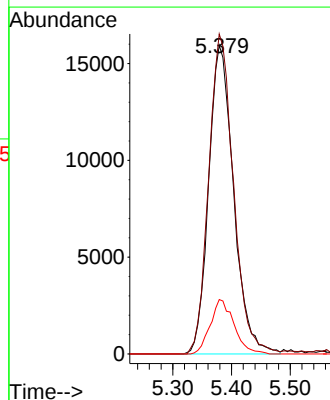
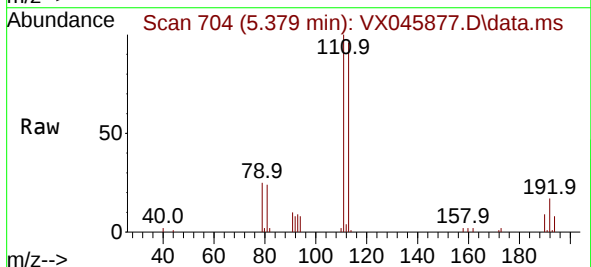


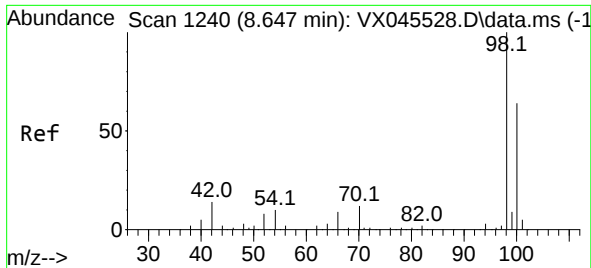

#50
Toluene-d8
Concen: 50.340 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20




Instrument :
MSVOA_X
ClientSampleId :
VX0422WBL01


Tgt Ion: 98 Resp: 163738
Ion Ratio Lower Upper
98 100
100 64.7 52.2 78.4

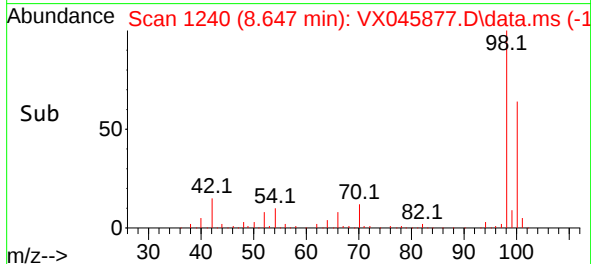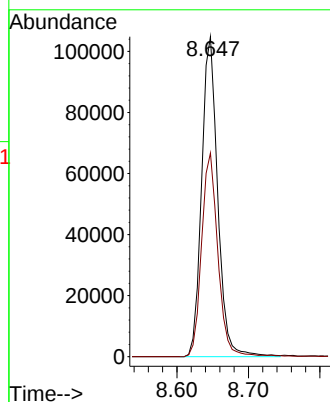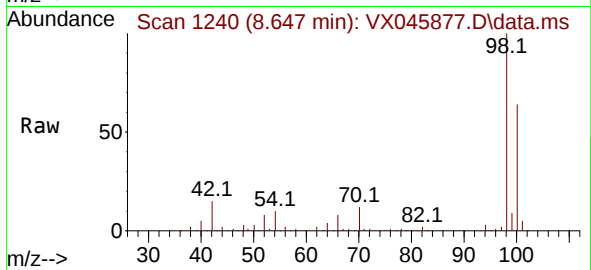

#62
4-Bromofluorobenzene
Concen: 51.469 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20

Tgt Ion: 95 Resp: 60979
Ion Ratio Lower Upper
95 100
174 67.1 0.0 135.8
176 65.1 0.0 131.4


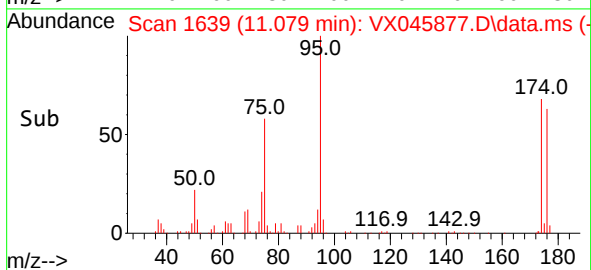
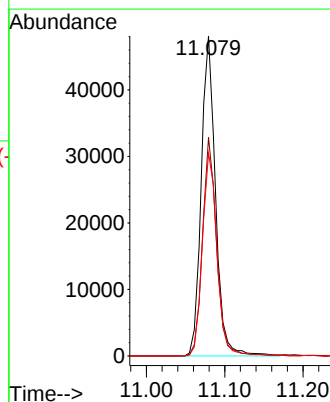
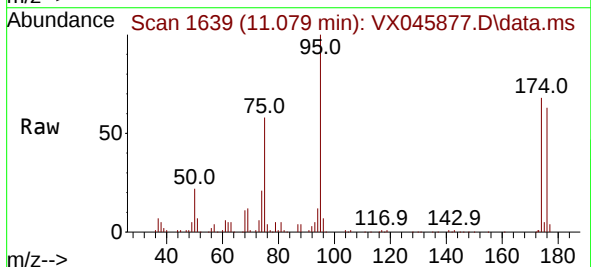


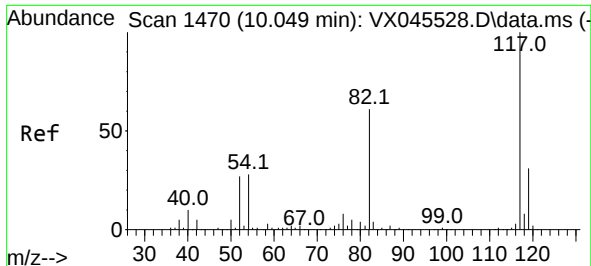

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20

Instrument :
MSVOA_X
ClientSampleId :
VX0422WBL01

Tgt Ion:117 Resp: 120785
Ion Ratio Lower Upper
117 100
82 62.4 49.2 73.8
119 31.6 25.1 37.7

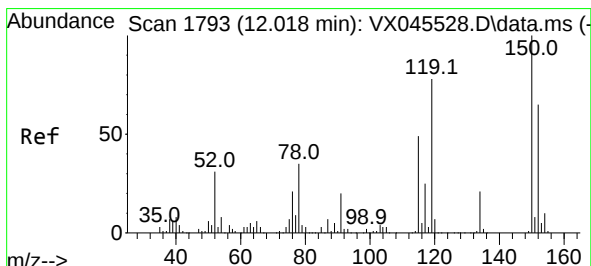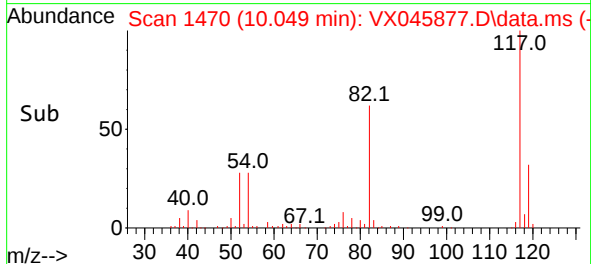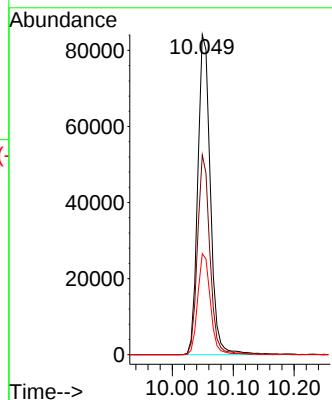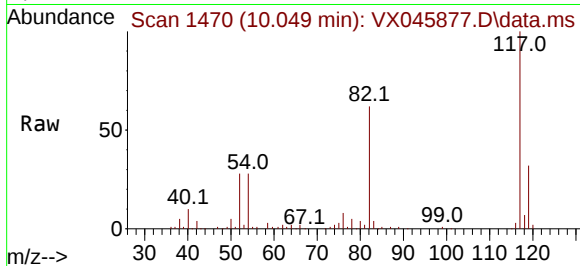

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045877.D
Acq: 22 Apr 2025 11:20

Tgt Ion:152 Resp: 49782
Ion Ratio Lower Upper
152 100
115 65.9 46.9 140.7
150 158.5 0.0 349.4

