

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042319\
 Data File : VX009114.D
 Acq On : 23 Apr 2019 12:33
 Operator : JC/SP
 Sample : K2537-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SS036MW002-190422

Quant Time: Apr 24 05:16:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 17 06:47:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	244672	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	397070	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	343980	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	146292	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	164845	47.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.62%	
35) Dibromofluoromethane	5.50	113	121872	47.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.64%	
50) Toluene-d8	8.71	98	493552	48.56	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.12%	
62) 4-Bromofluorobenzene	11.13	95	162165	45.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.40%	


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042319\
Data File : VX009114.D
Acq On : 23 Apr 2019 12:33
Operator : JC/SP
Sample : K2537-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SS036MW002-190422

Quant Time: Apr 24 05:16:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 17 06:47:58 2019
Response via : Initial Calibration

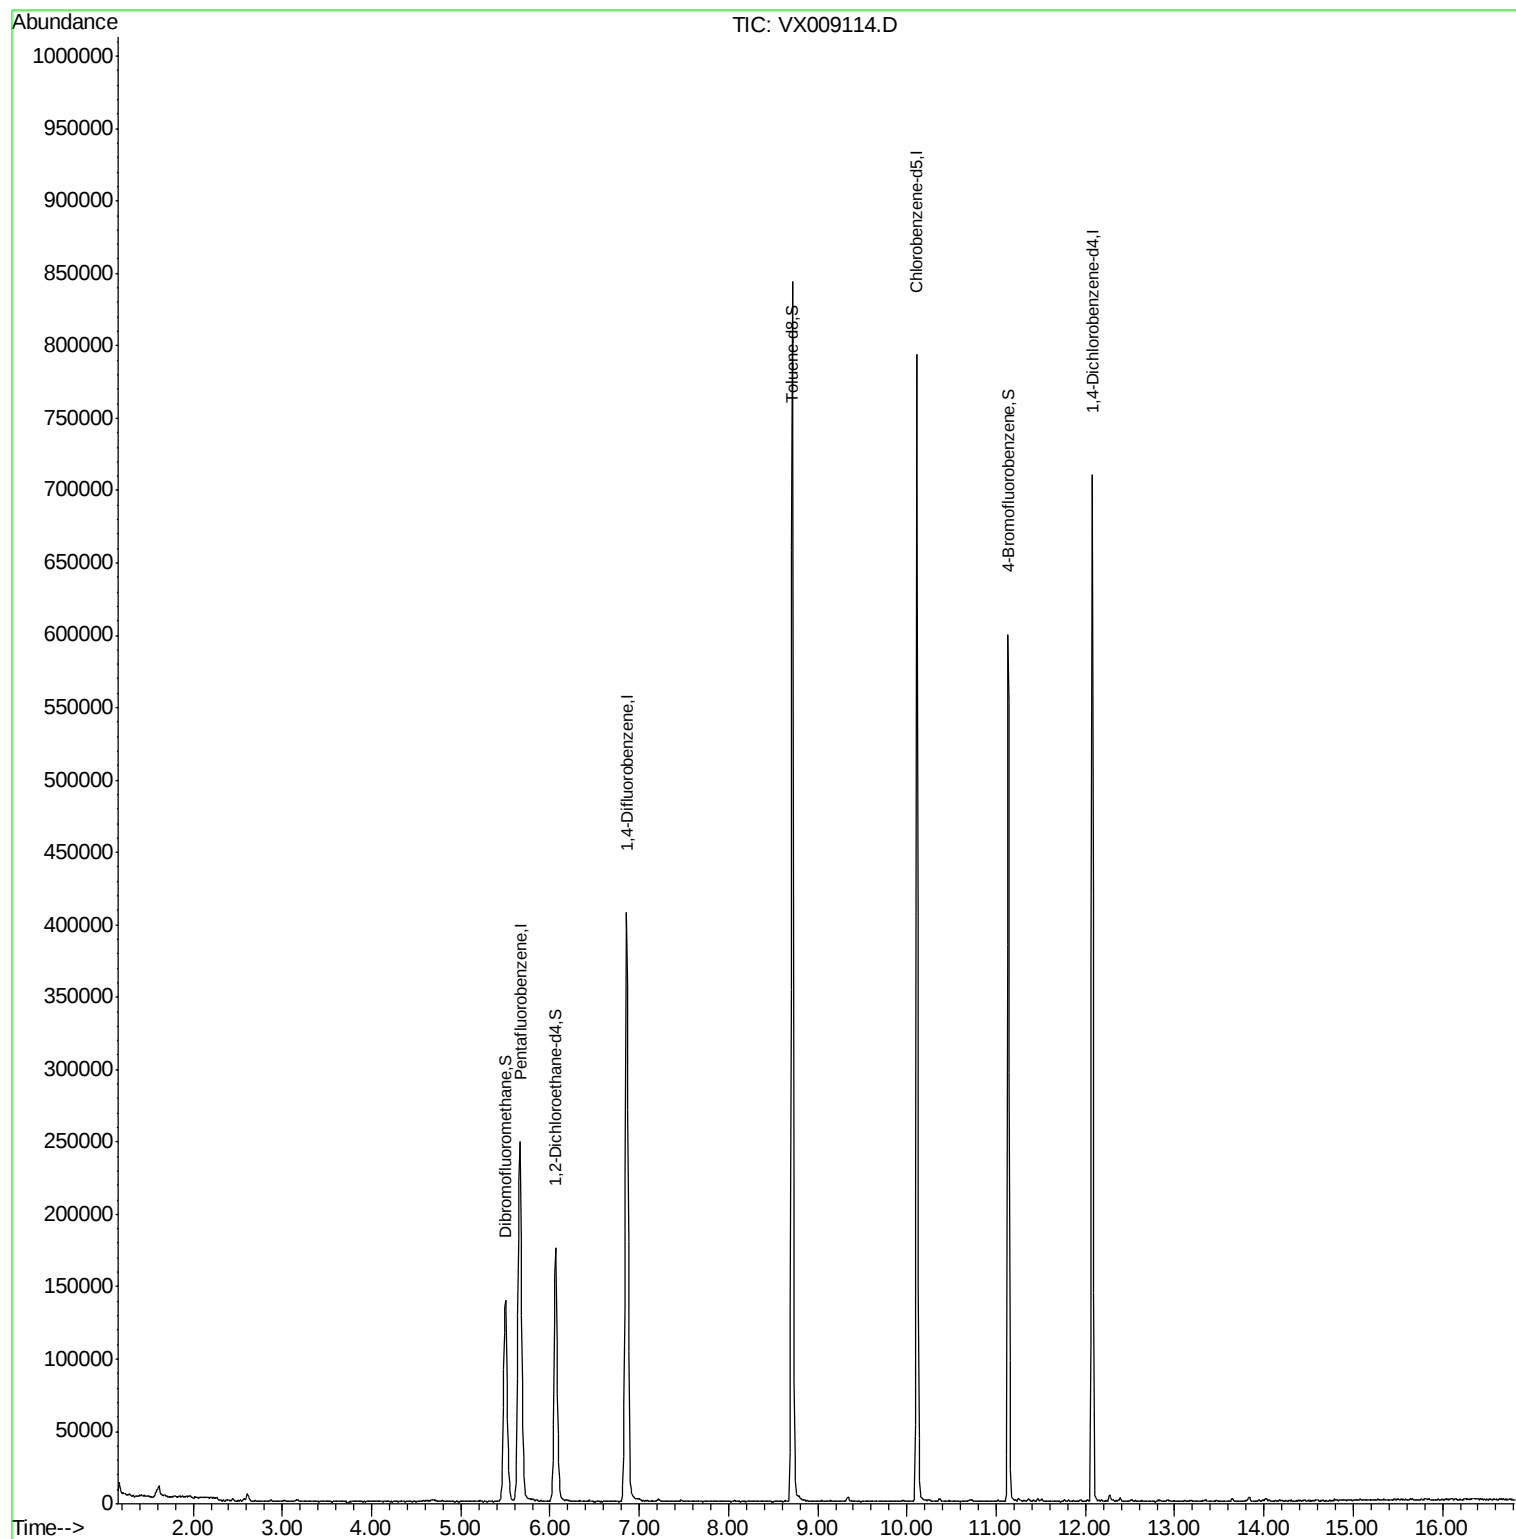



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX009114.D

Acq: 23 Apr 2019 12:33

Instrument :

MSVOA_X

ClientSampleId :


SS036MW002-190422

Tot Ion:168 Resp: 244672

Ion Ratio Lower Upper

168 100

99 55.3 43.0 64.6

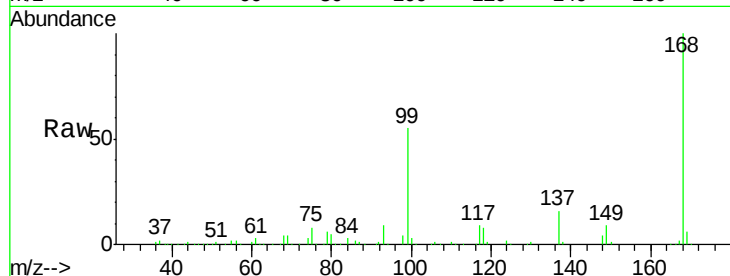

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

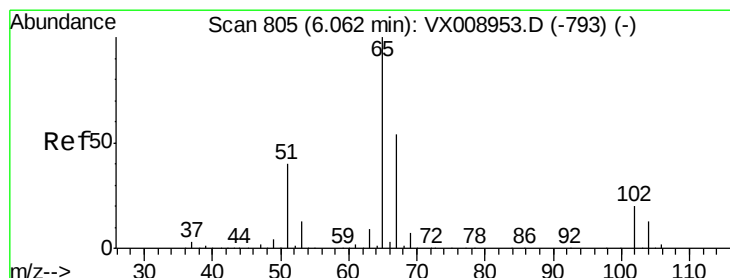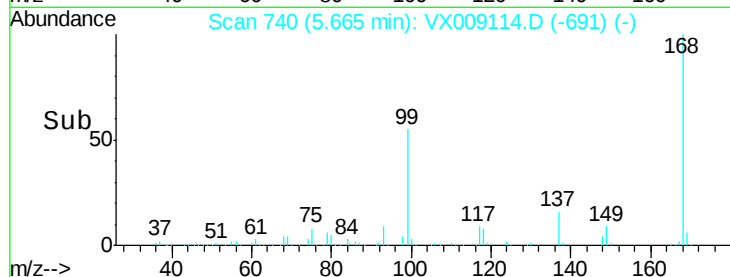

#33

1,2-Dichloroethane-d4

Concen: 47.807 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX009114.D


Acq: 23 Apr 2019 12:33

Tgt Ion: 65 Resp: 164845

Ion Ratio Lower Upper

65 100

67 53.1 0.0 108.6

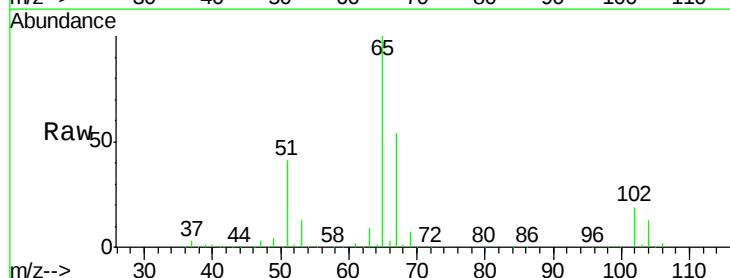

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06


60000


40000

20000

0

Time--> 6.00 6.20




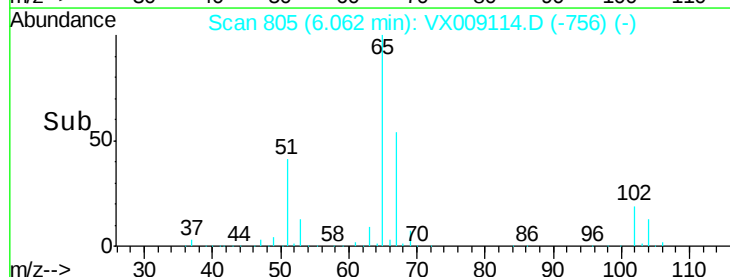


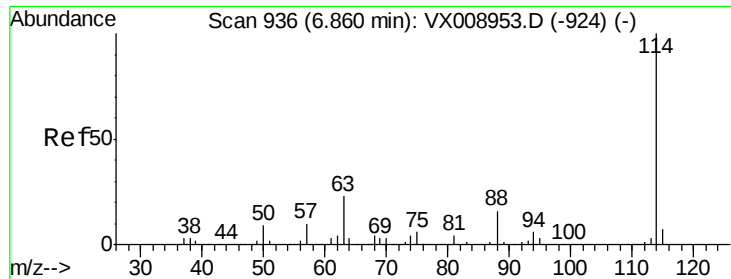

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX009114.D
 Acq: 23 Apr 2019 12:33




Instrument :
 MSVOA_X
 ClientSampleId :
 SS036MW002-190422


Tot Ion:114 Resp: 397070
 Ion Ratio Lower Upper
 114 100
 63 23.5 0.0 46.0
 88 17.0 0.0 32.6

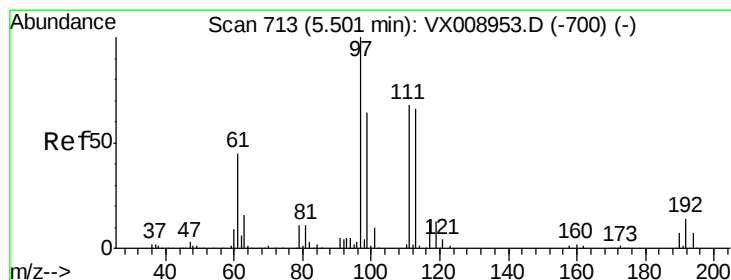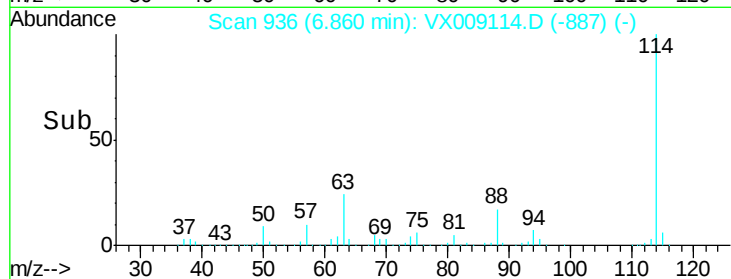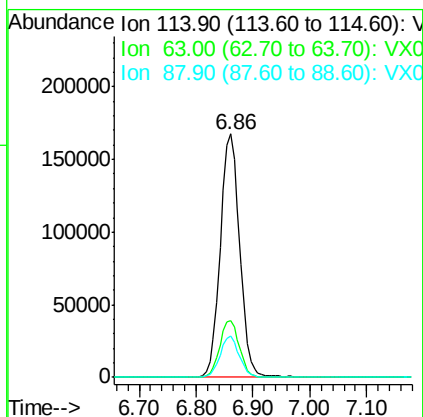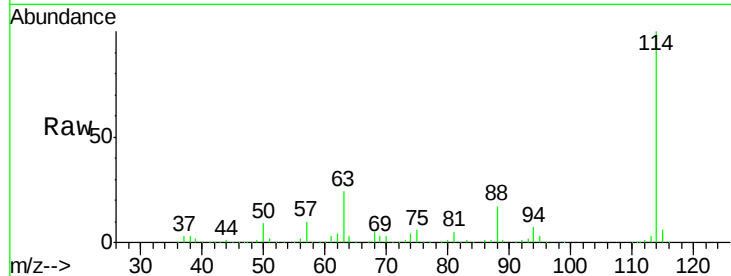

#35
 Dibromofluoromethane
 Concen: 47.825 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX009114.D
 Acq: 23 Apr 2019 12:33

Tgt Ion:113 Resp: 121872
 Ion Ratio Lower Upper
 113 100
 111 100.7 82.9 124.3
 192 20.5 17.4 26.0


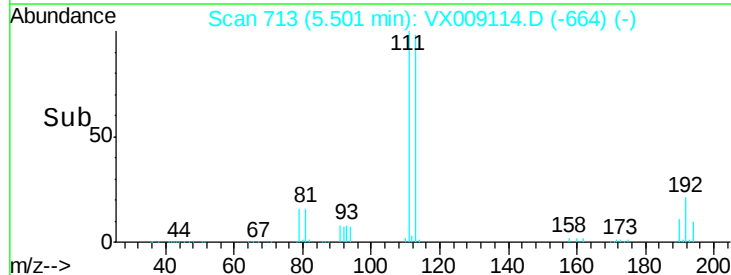
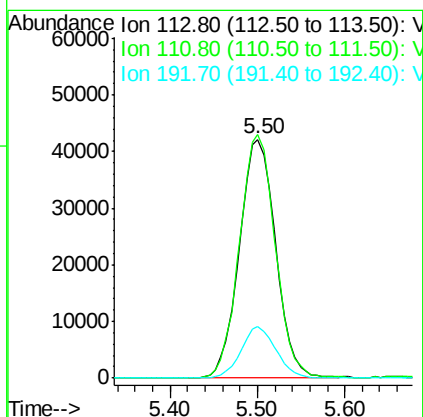
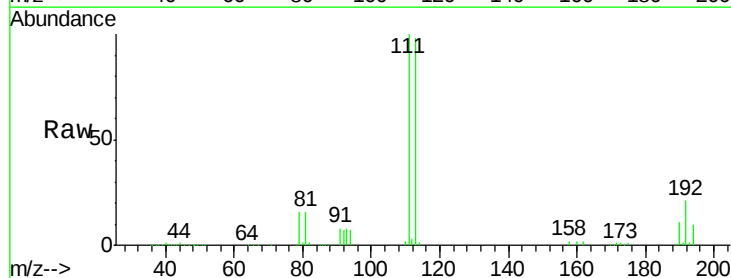


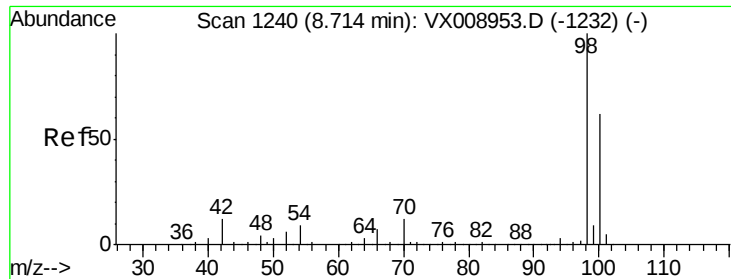

#50
Toluene-d8
Concen: 48.565 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX009114.D
Acq: 23 Apr 2019 12:33




Instrument :
MSVOA_X
ClientSampleId :
SS036MW002-190422


Tot Ion: 98 Resp: 493552
Ion Ratio Lower Upper
98 100
100 64.4 51.4 77.2

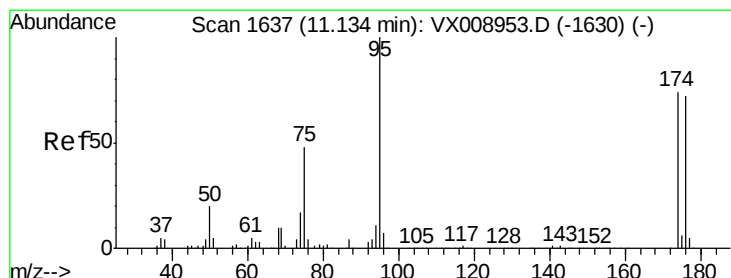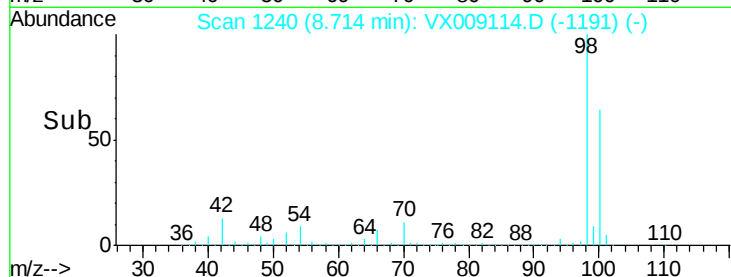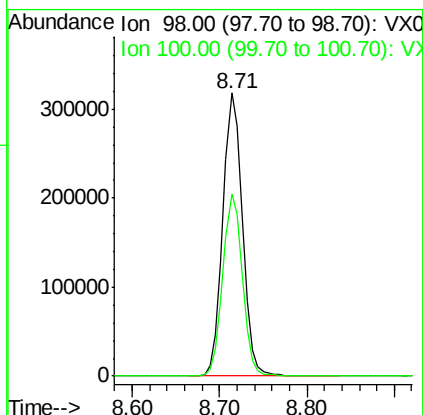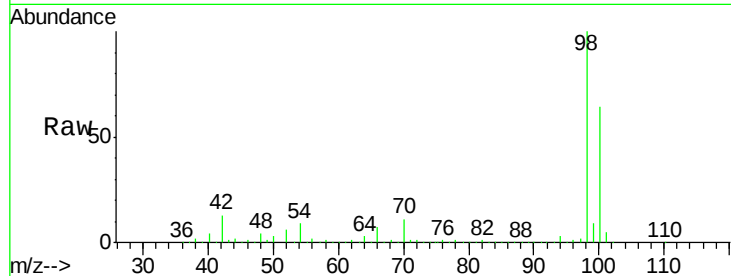

#62
4-Bromofluorobenzene
Concen: 45.203 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX009114.D
Acq: 23 Apr 2019 12:33

Tgt Ion: 95 Resp: 162165
Ion Ratio Lower Upper
95 100
174 79.9 0.0 159.6
176 76.5 0.0 154.8

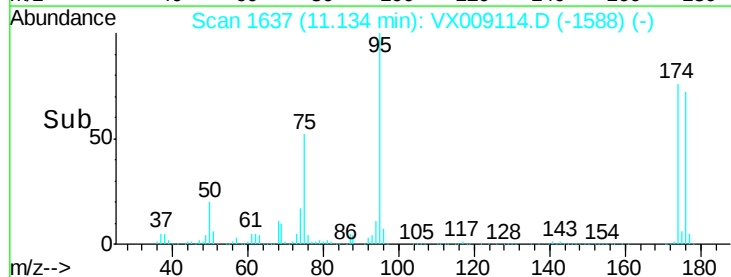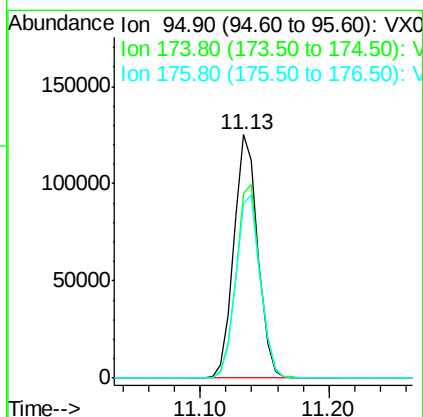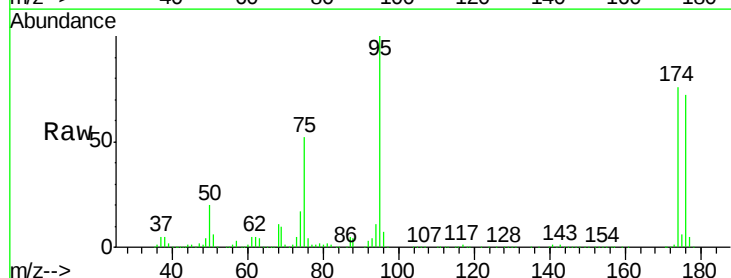


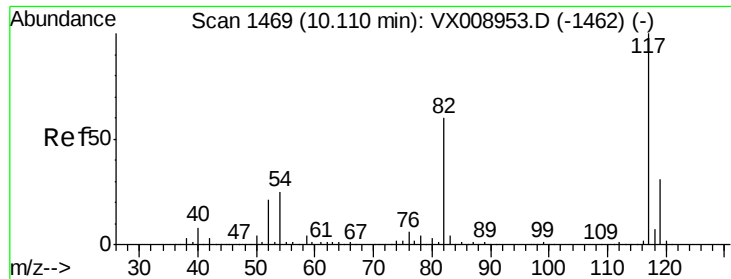




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX009114.D
Acq: 23 Apr 2019 12:33

Instrument :
MSVOA_X
ClientSampleId :
SS036MW002-190422

Tot Ion:117 Resp: 343980
Ion Ratio Lower Upper
117 100
82 60.4 48.2 72.4
119 31.6 25.0 37.6

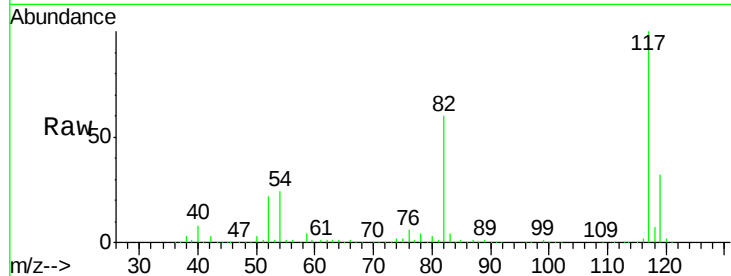


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

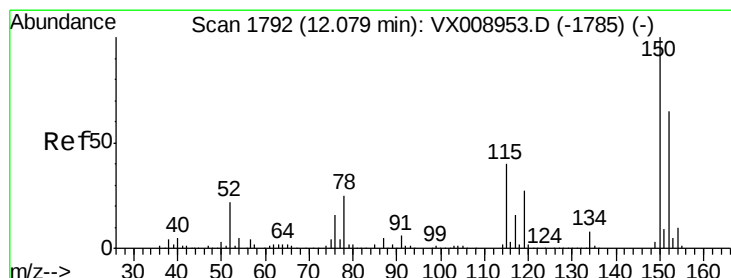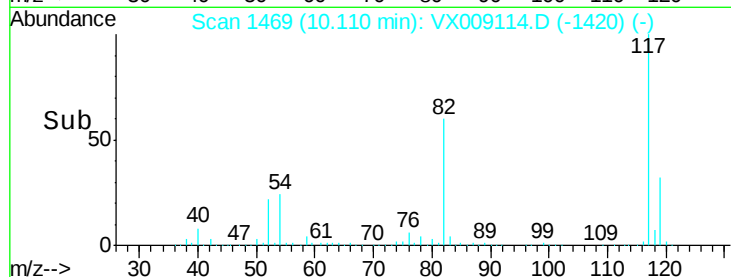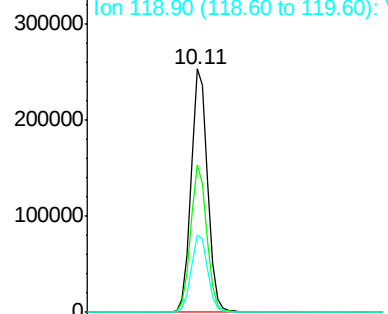

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX009114.D
Acq: 23 Apr 2019 12:33

Tgt Ion:152 Resp: 146292
Ion Ratio Lower Upper
152 100
115 59.1 41.4 124.2
150 155.9 0.0 349.8

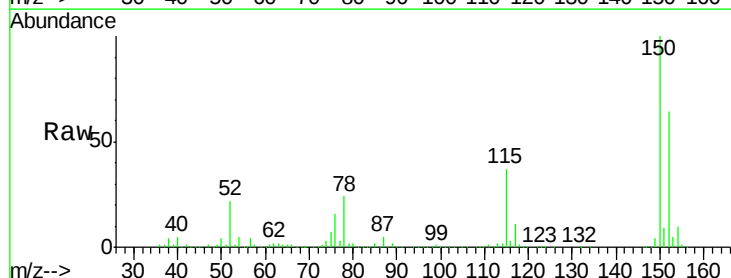

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

