

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
 Data File : VX021840.D
 Acq On : 23 Apr 2021 14:28
 Operator : JC/MD
 Sample : M2138-03DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-2-PDDL

Quant Time: Apr 26 04:03:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 20 13:46:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.629	168	177466	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.830	114	291773	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.092	117	258951	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	119634	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.031	65	95996	47.68	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	95.36%		
35) Dibromofluoromethane	5.464	113	92520	49.58	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	99.16%		
50) Toluene-d8	8.695	98	344556	48.03	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.06%		
62) 4-Bromofluorobenzene	11.116	95	120838	45.10	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.20%		
Target Compounds						Qvalue
3) Chloromethane	1.313	50	1414	0.93	ug/l	97
5) Bromomethane	1.642	94	458	0.51	ug/l	83
10) Methyl Iodide	2.495	142	268	8.32	ug/l #	88
11) Tert butyl alcohol	2.995	59	476	1.08	ug/l	95
13) Acrolein	2.282	56	94	0.26	ug/l #	1
15) Acrylonitrile	3.111	53	323	0.36	ug/l #	69
16) Acetone	2.422	43	748	1.08	ug/l	91
17) Carbon Disulfide	2.550	76	1549	0.33	ug/l #	92
18) Methyl Acetate	2.764	43	552	0.29	ug/l #	47
20) Methylene Chloride	2.837	84	632	0.30	ug/l #	81
29) Tetrahydrofuran	5.105	42	163	0.21	ug/l #	46
31) Cyclohexane	5.629	56	3199	1.13	ug/l #	1
36) 1,1-Dichloropropene	5.629	75	11597	4.50	ug/l #	49
38) Carbon Tetrachloride	5.763	117	578	0.20	ug/l #	60
44) Trichloroethene	7.190	130	480	0.21	ug/l	76
51) 4-Methyl-2-Pentanone	8.616	43	585	0.24	ug/l #	52
55) 1,1,2-Trichloroethane	9.317	97	1507	0.74	ug/l #	1
59) 2-Hexanone	9.470	43	542	0.30	ug/l #	46
60) Dibromochloromethane	9.317	129	186700	75.15	ug/l #	11
64) Tetrachloroethene	9.317	164	194402	96.01	ug/l	98
76) 1,2,3-Trichloropropane	11.116	75	54527	22.98	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.116	75	54527	52.85	ug/l #	12
82) 4-Chlorotoluene	11.494	91	1330	0.21	ug/l	94
87) 1,3-Dichlorobenzene	12.012	146	875	0.23	ug/l	93
88) 1,4-Dichlorobenzene	12.012	146	875	0.23	ug/l	93
89) n-Butylbenzene	12.372	91	2401	0.37	ug/l	92
90) Hexachloroethane	12.579	117	4335	3.08	ug/l	98
93) 1,2,4-Trichlorobenzene	13.627	180	1127	0.42	ug/l	96
94) Hexachlorobutadiene	13.762	225	576	0.44	ug/l	94
95) Naphthalene	13.816	128	2231	0.28	ug/l	96
96) 1,2,3-Trichlorobenzene	13.999	180	837	0.33	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
Data File : VX021840.D
Acq On : 23 Apr 2021 14:28
Operator : JC/MD
Sample : M2138-03DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL

Quant Time: Apr 26 04:03:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 20 13:46:22 2021
Response via : Initial Calibration




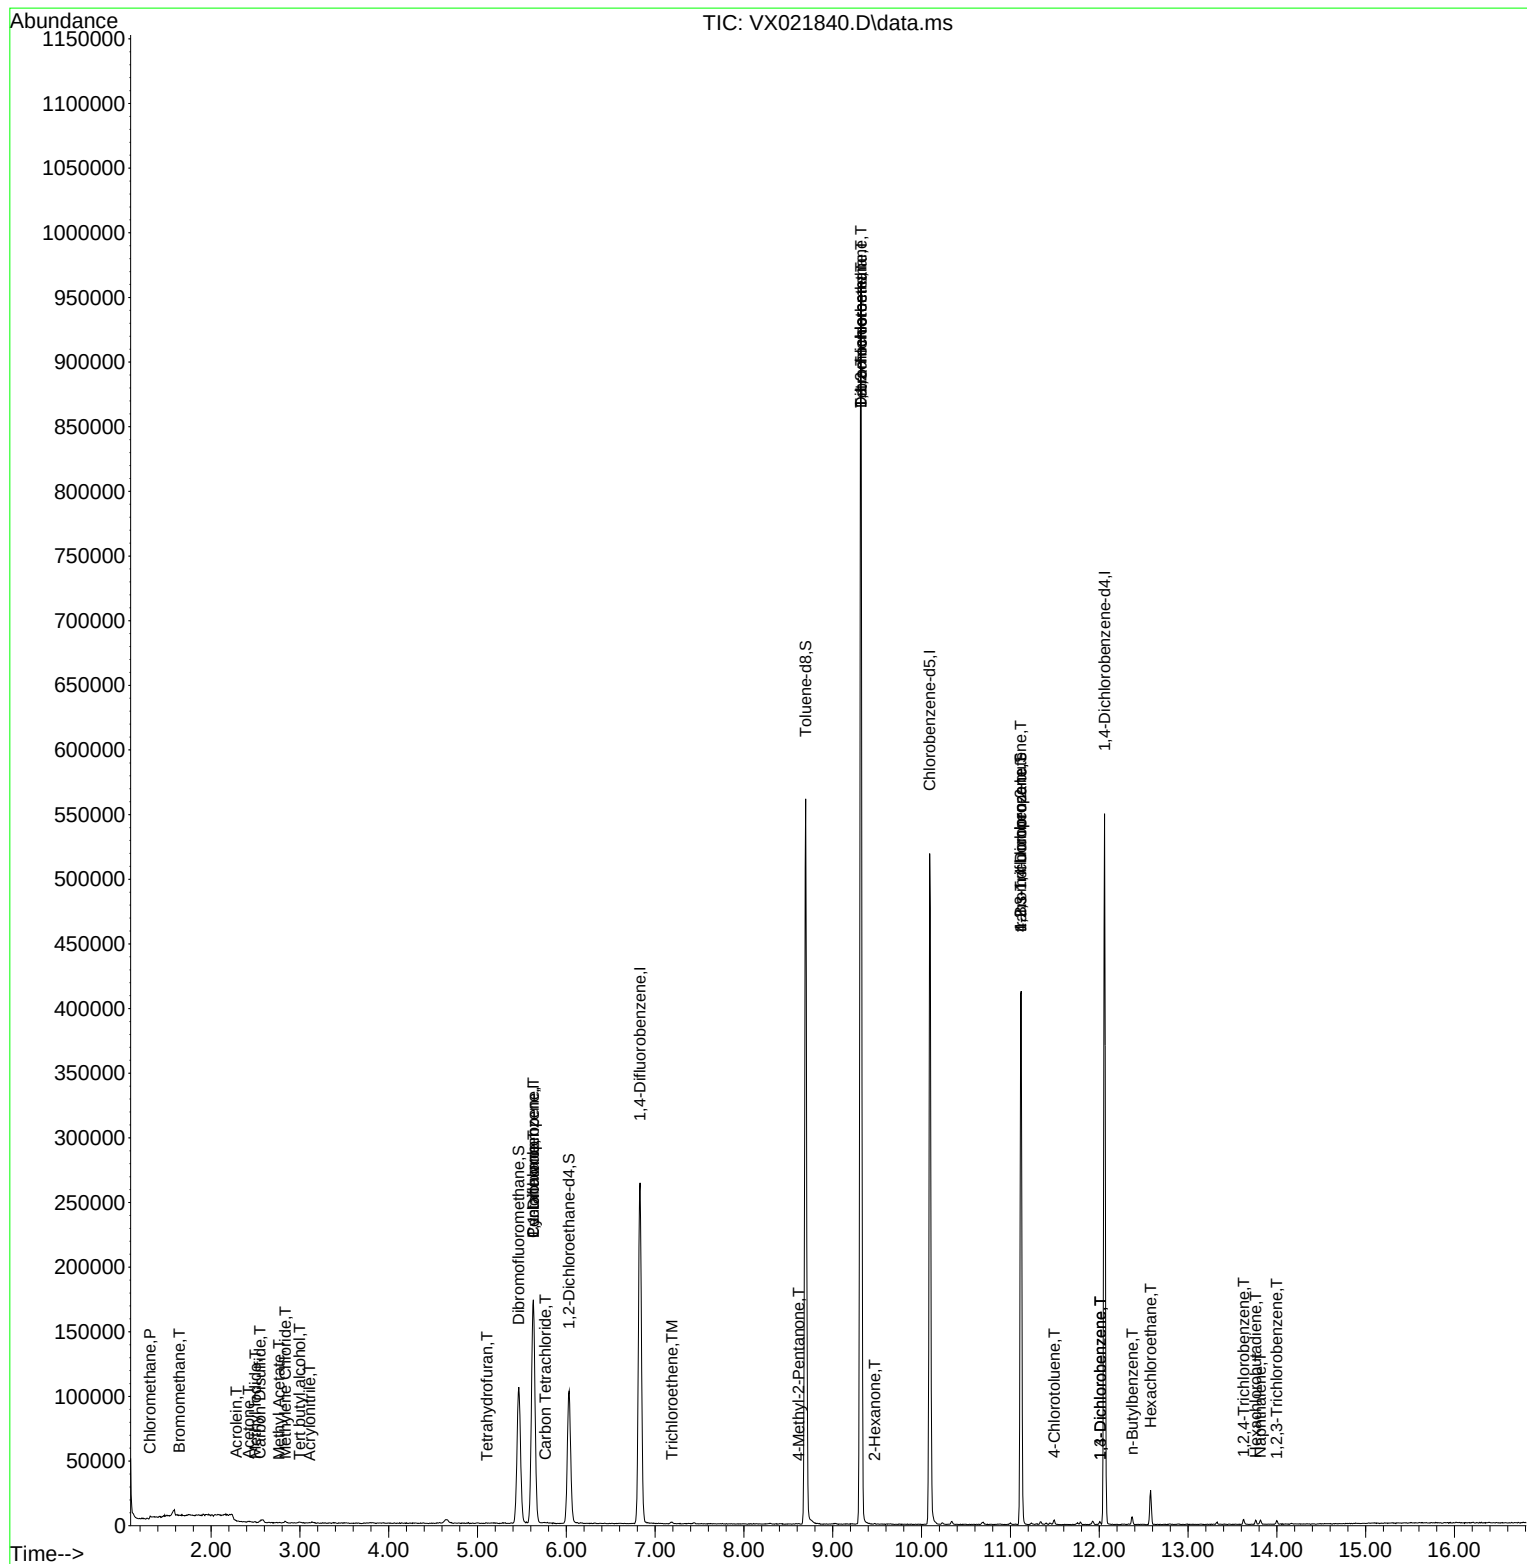




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion:168 Resp: 177466
Ion Ratio Lower Upper
168 100
99 52.3 45.8 68.6

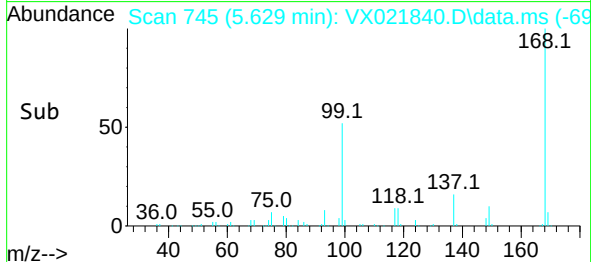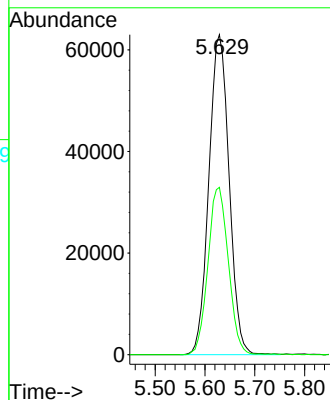

#3
Chloromethane
Concen: 0.93 ug/l
RT: 1.313 min Scan# 37
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 50 Resp: 1414
Ion Ratio Lower Upper
50 100
52 34.8 26.4 39.6


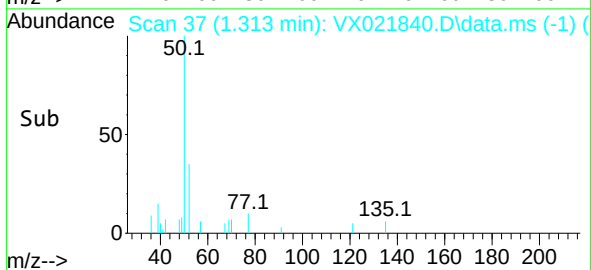
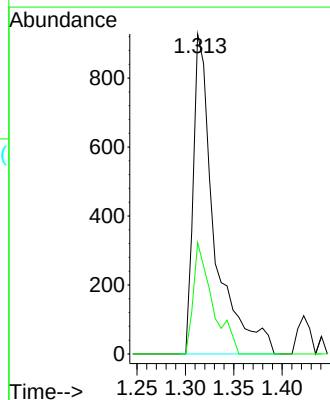
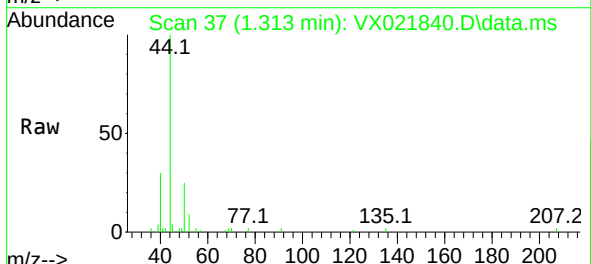


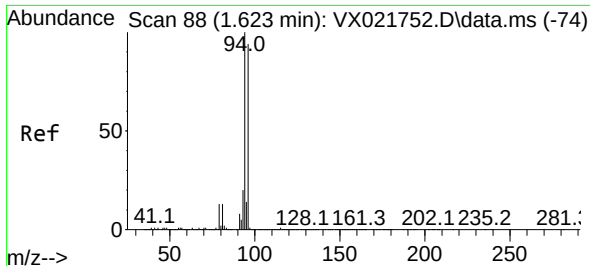

#5
Bromomethane
Concen: 0.51 ug/l
RT: 1.642 min Scan# 91
Delta R.T. 0.019 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 94 Resp: 458
Ion Ratio Lower Upper
94 100
96 78.5 76.4 114.6

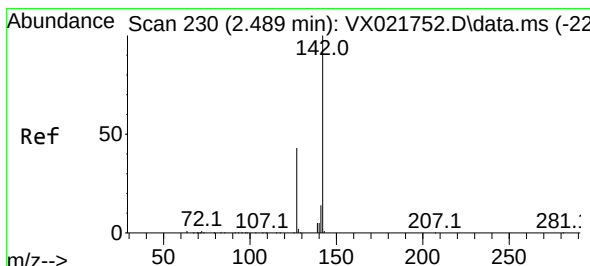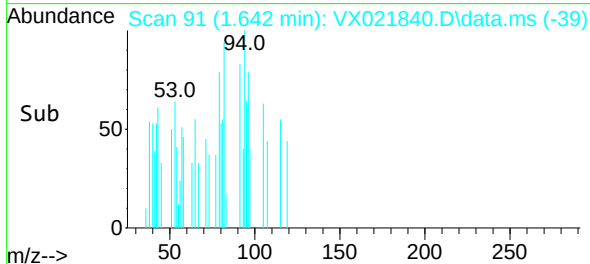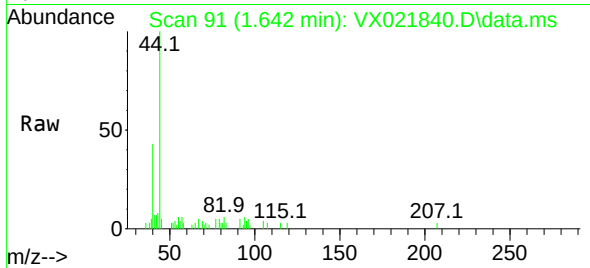

#10
Methyl Iodide
Concen: 8.32 ug/l
RT: 2.495 min Scan# 231
Delta R.T. 0.006 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 142 Resp: 268
Ion Ratio Lower Upper
142 100
127 39.2 33.3 49.9
141 0.0 11.4 17.0#

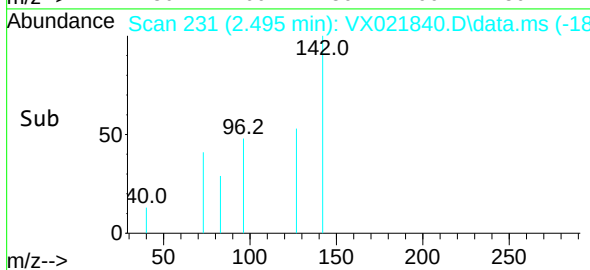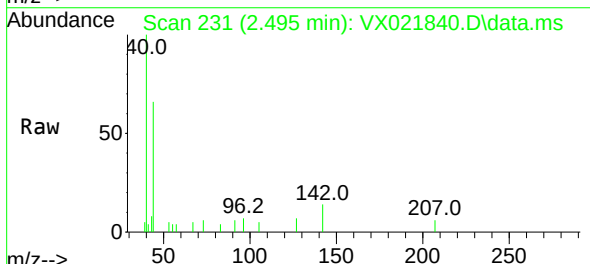







#11

Tert butyl alcohol
Concen: 1.08 ug/l
RT: 2.995 min Scan# 313
Delta R.T. -0.018 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL




Tgt Ion: 59 Resp: 476
Ion Ratio Lower Upper
59 100
57 11.6 7.8 11.8

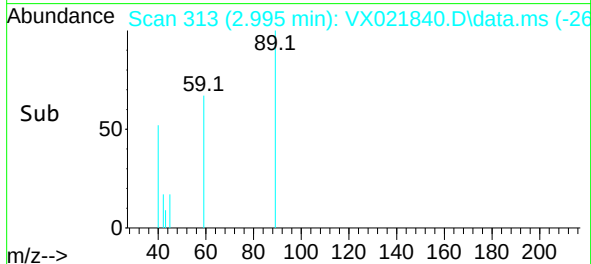


#13

Acrolein
Concen: 0.26 ug/l
RT: 2.282 min Scan# 196
Delta R.T. 0.006 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 56 Resp: 94
Ion Ratio Lower Upper
56 100
55 222.3 56.4 84.6#


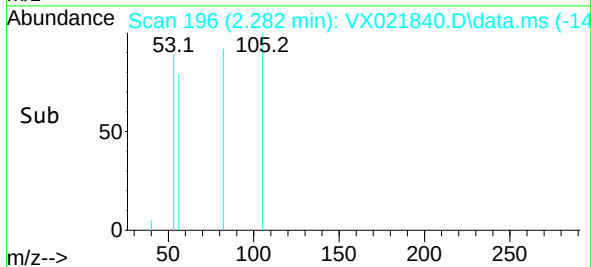

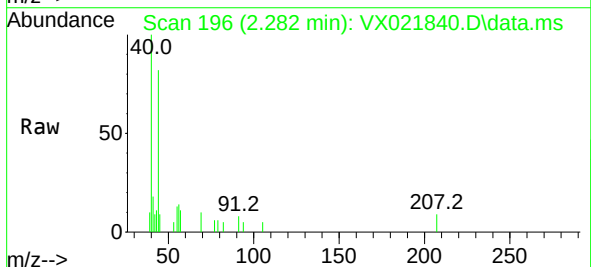


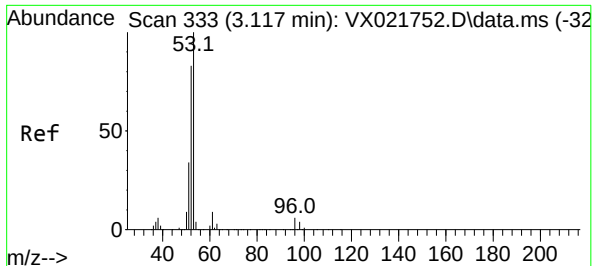

#15
Acrylonitrile
Concen: 0.36 ug/l
RT: 3.111 min Scan# 332
Delta R.T. -0.006 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 53 Resp: 323
Ion Ratio Lower Upper
53 100
52 65.0 65.3 97.9#
51 0.0 28.2 42.2#

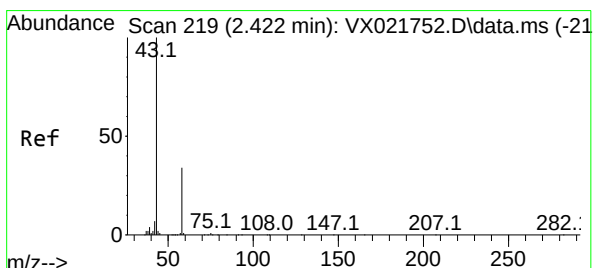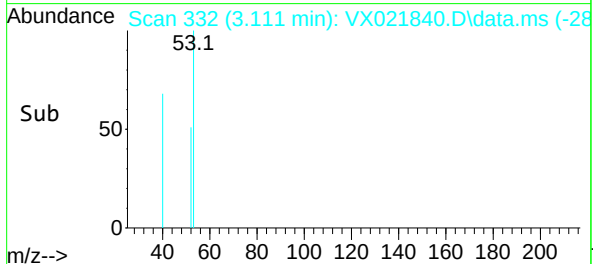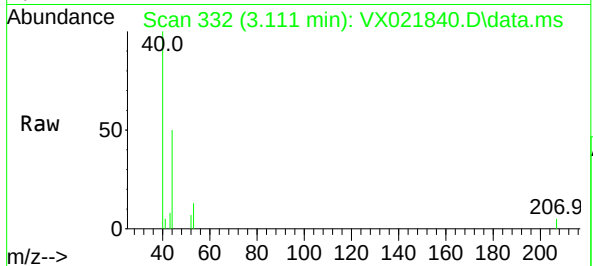

#16
Acetone
Concen: 1.08 ug/l
RT: 2.422 min Scan# 219
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 43 Resp: 748
Ion Ratio Lower Upper
43 100
58 39.9 27.8 41.8


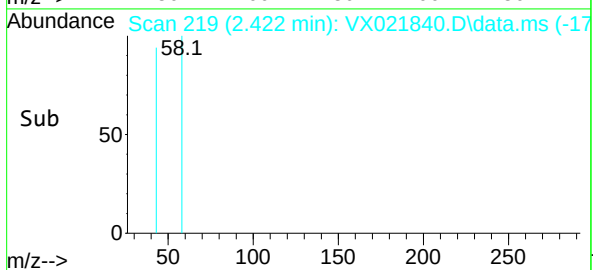

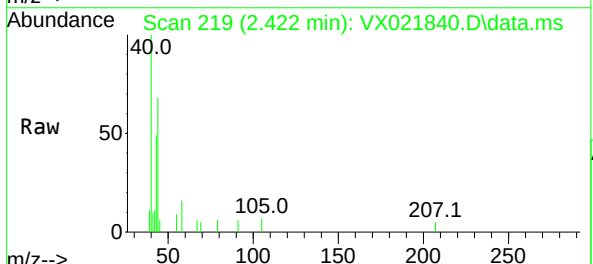




#17
Carbon Disulfide
Concen: 0.33 ug/l
RT: 2.550 min Scan# 240
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 76 Resp: 1549
Ion Ratio Lower Upper
76 100
78 11.9 7.2 10.8#

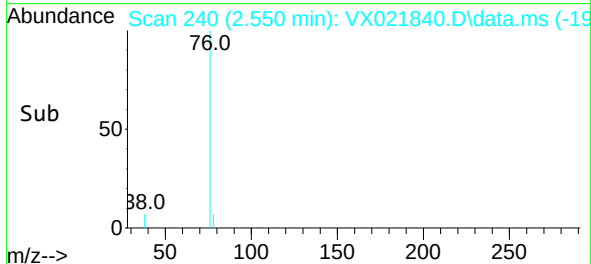

#18
Methyl Acetate
Concen: 0.29 ug/l
RT: 2.764 min Scan# 275
Delta R.T. 0.013 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 43 Resp: 552
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

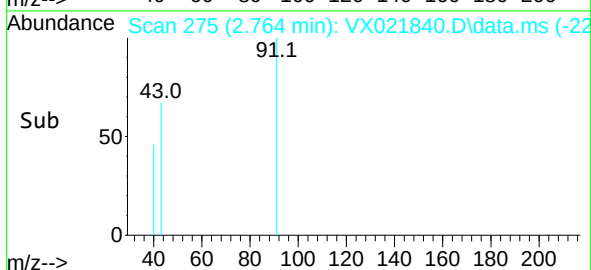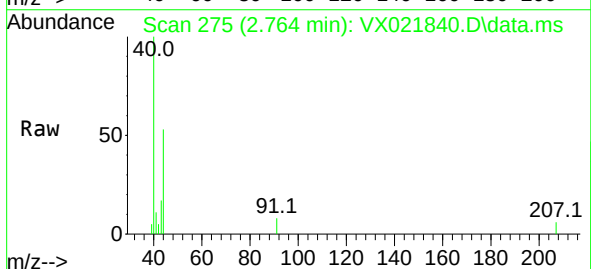

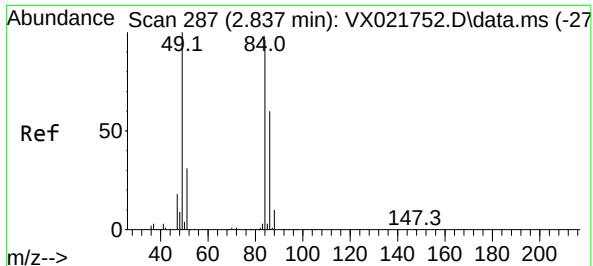

#20

Methylene Chloride

Concen: 0.30 ug/l

RT: 2.837 min Scan# 287

Delta R.T. -0.000 min

Lab File: VX021840.D

Acq: 23 Apr 2021 14:28

Tgt Ion: 84 Resp: 632





Ion Ratio Lower Upper

84 100

49 88.9 88.6 132.8

51 33.8 27.0 40.6

86 43.4 50.3 75.5#

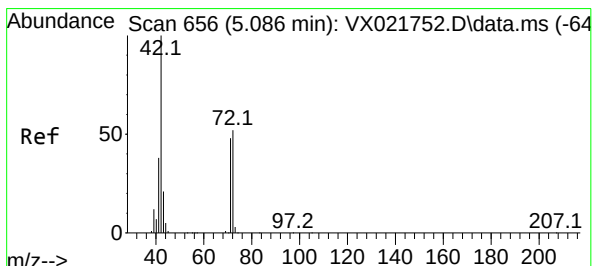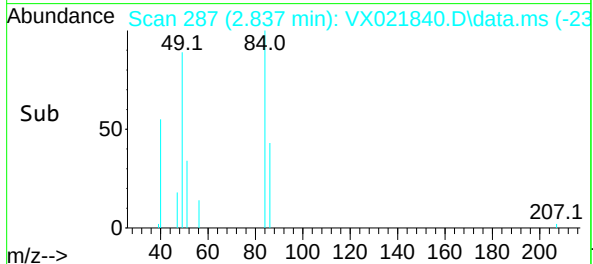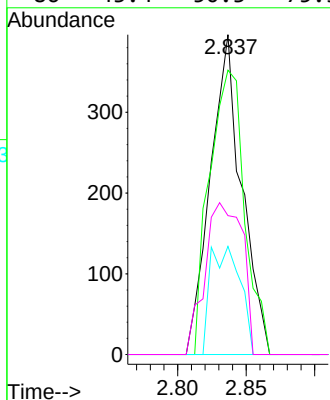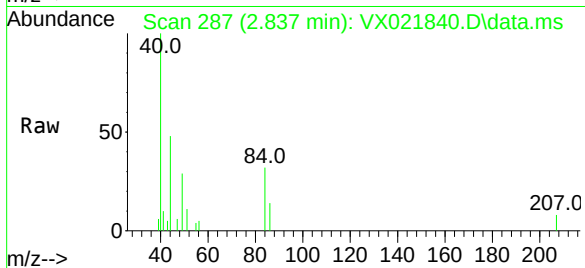

#29

Tetrahydrofuran

Concen: 0.21 ug/l

RT: 5.105 min Scan# 659

Delta R.T. 0.019 min

Lab File: VX021840.D

Acq: 23 Apr 2021 14:28




Tgt Ion: 42 Resp: 163


Ion Ratio Lower Upper

42 100

72 0.0 41.7 62.5#


71 25.8 38.4 57.6#

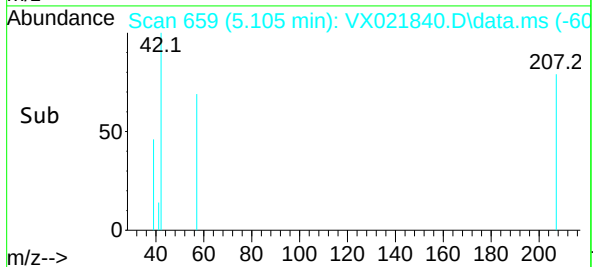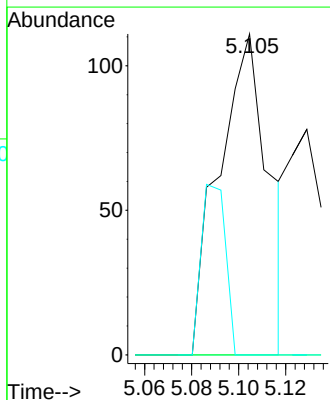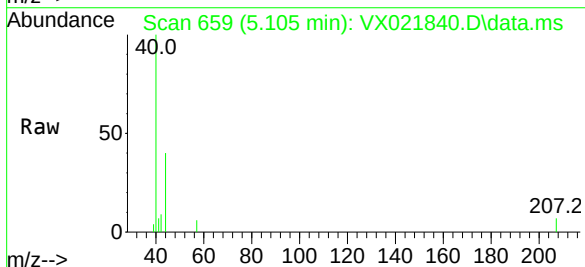



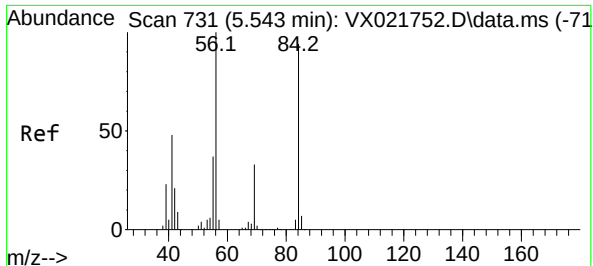


#31
Cyclohexane
Concen: 1.13 ug/l
RT: 5.629 min Scan# 745
Delta R.T. 0.086 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28


Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL

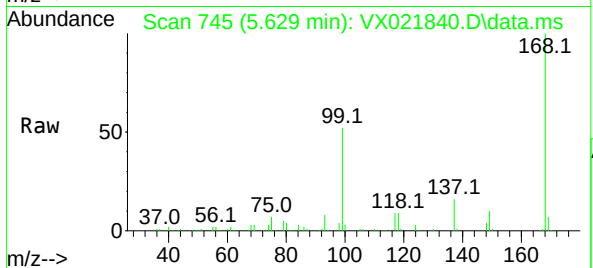



Tgt Ion: 56 Resp: 3199
Ion Ratio Lower Upper
56 100
69 207.9 25.3 37.9#
84 182.7 71.4 107.0#

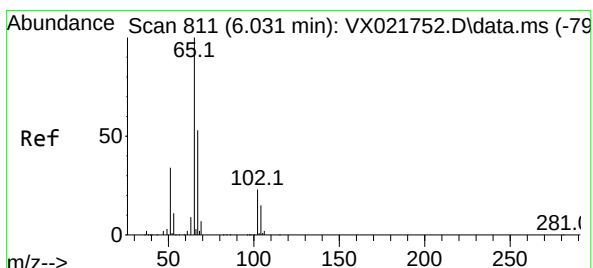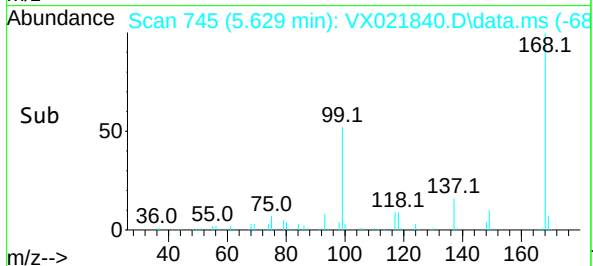


#33
1,2-Dichloroethane-d4
Concen: 47.68 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

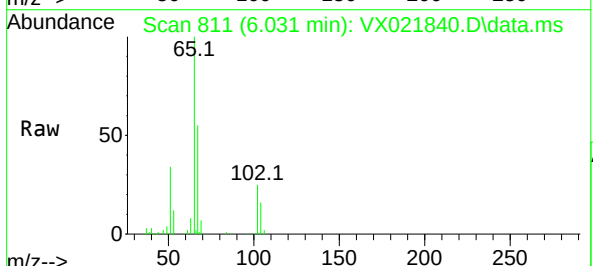


Tgt Ion: 65 Resp: 95996
Ion Ratio Lower Upper
65 100
67 55.1 0.0 105.4

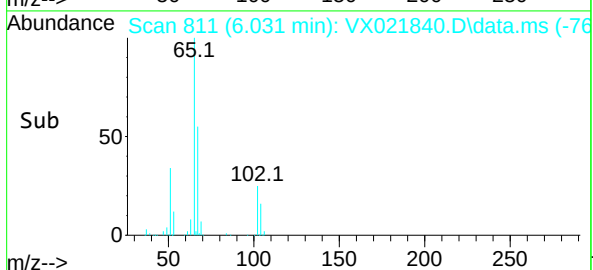






#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.830 min Scan# 942
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28


Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL





Tgt Ion:114 Resp: 291773
Ion Ratio Lower Upper
114 100
63 18.4 0.0 40.8
88 15.2 0.0 32.8

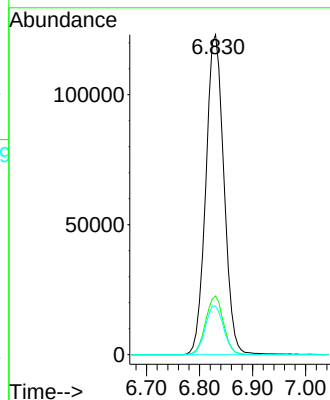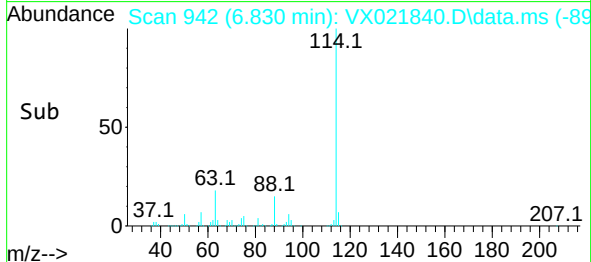


#35
Dibromofluoromethane
Concen: 49.58 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

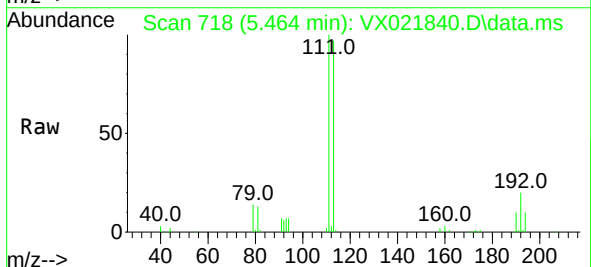


Tgt Ion:113 Resp: 92520
Ion Ratio Lower Upper
113 100
111 103.8 81.9 122.9
192 20.9 16.7 25.1

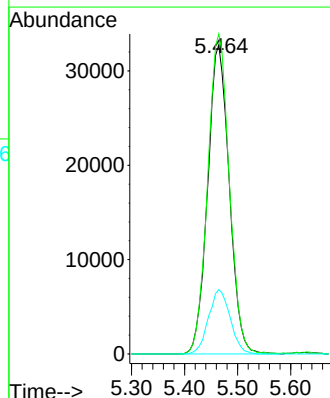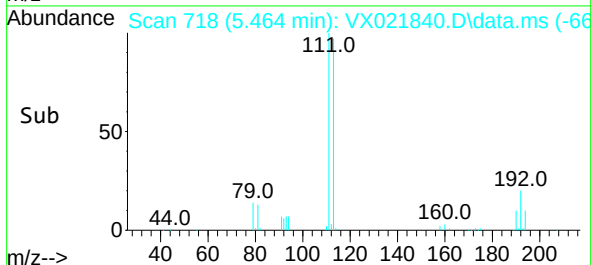






#36
1,1-Dichloropropene
Concen: 4.50 ug/l
RT: 5.629 min Scan# 745
Delta R.T. -0.140 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL







Tgt Ion: 75 Resp: 11597
Ion Ratio Lower Upper
75 100
110 9.5 18.1 54.4#
77 0.0 25.3 37.9#



#38
Carbon Tetrachloride
Concen: 0.20 ug/l
RT: 5.763 min Scan# 767
Delta R.T. 0.012 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 117 Resp: 578
Ion Ratio Lower Upper
117 100
119 47.1 76.2 114.2#
121 37.4 24.8 37.2#


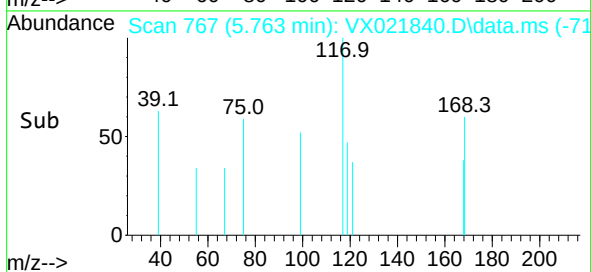

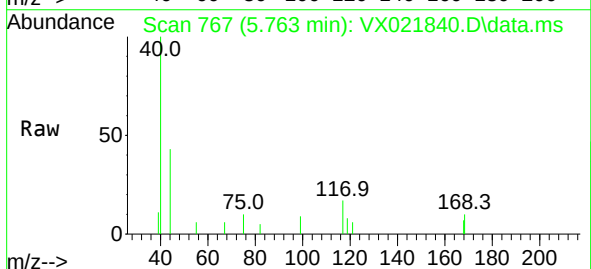


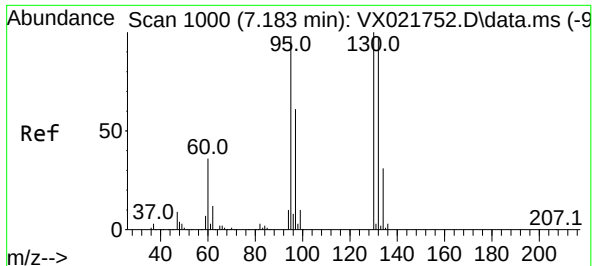

#44
Trichloroethene
Concen: 0.21 ug/l
RT: 7.190 min Scan# 1001
Delta R.T. 0.007 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion:130 Resp: 480
Ion Ratio Lower Upper
130 100
95 75.1 0.0 198.0

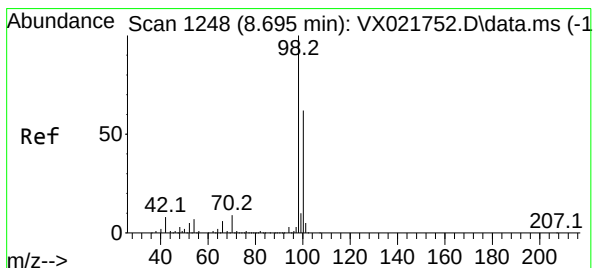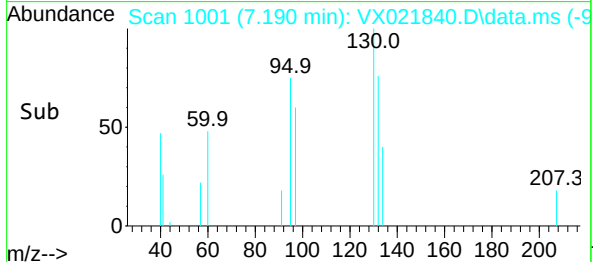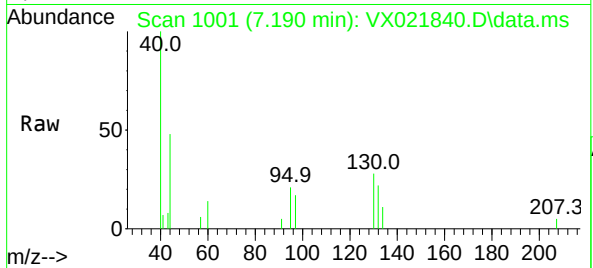

#50
Toluene-d8
Concen: 48.03 ug/l
RT: 8.695 min Scan# 1248
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 98 Resp: 344556
Ion Ratio Lower Upper
98 100
100 64.9 51.9 77.9


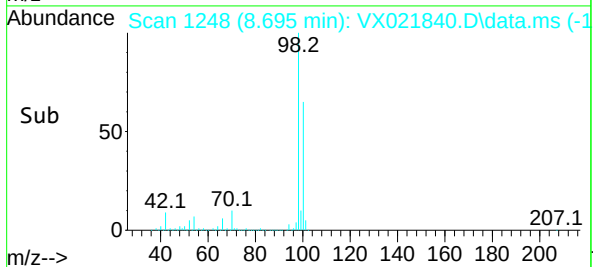

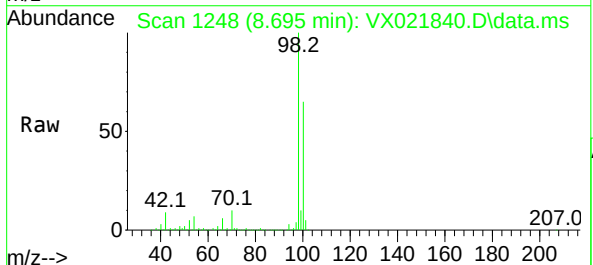




#51
4-Methyl-2-Pentanone
Concen: 0.24 ug/l
RT: 8.616 min Scan# 1235
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 43 Resp: 585
Ion Ratio Lower Upper
43 100
58 13.2 35.4 53.0#

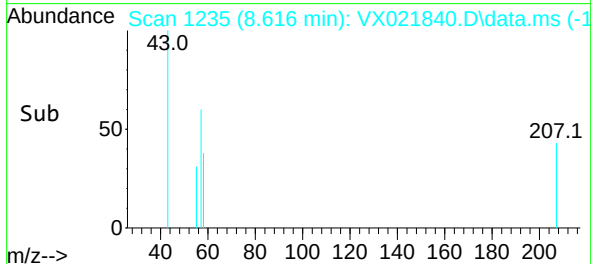

#55
1,1,2-Trichloroethane
Concen: 0.74 ug/l
RT: 9.317 min Scan# 1350
Delta R.T. 0.122 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 97 Resp: 1507
Ion Ratio Lower Upper
97 100
83 276.7 69.3 103.9#
85 27.3 44.3 66.5#
99 15.8 50.3 75.5#


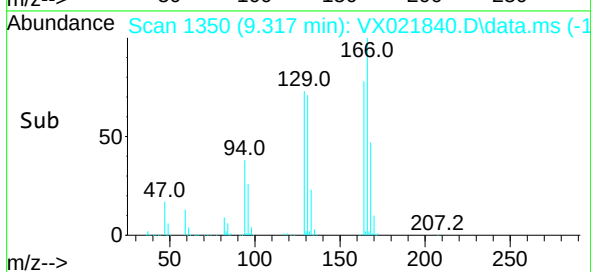

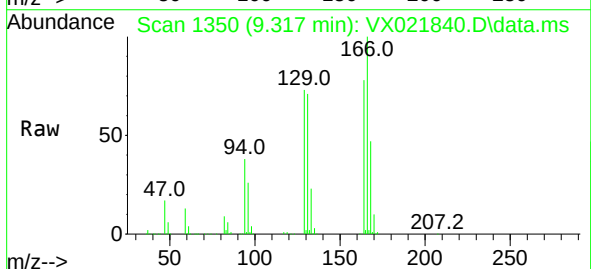




#59
2-Hexanone
Concen: 0.30 ug/l
RT: 9.470 min Scan# 1375
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 43 Resp: 542
Ion Ratio Lower Upper
43 100
58 20.1 30.9 92.8#

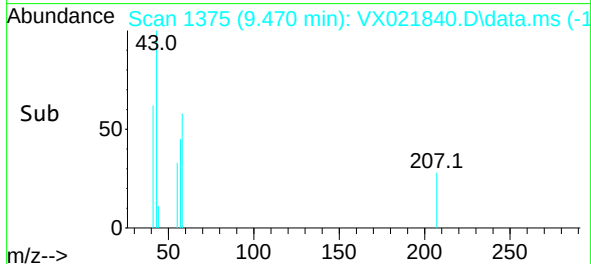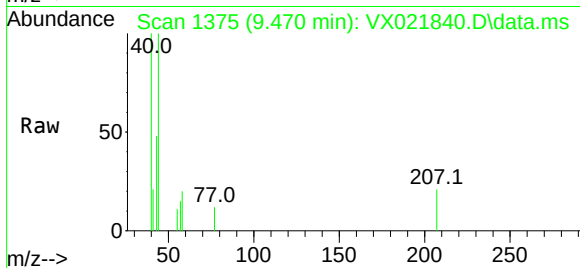

#60
Dibromochloromethane
Concen: 75.15 ug/l
RT: 9.317 min Scan# 1350
Delta R.T. -0.244 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 129 Resp: 186700
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#


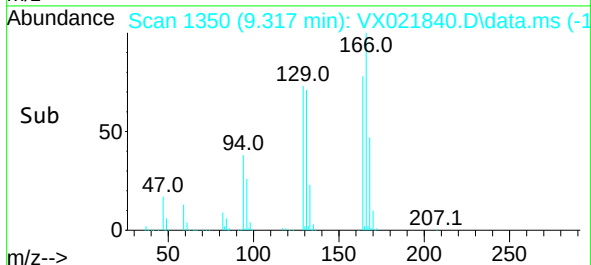

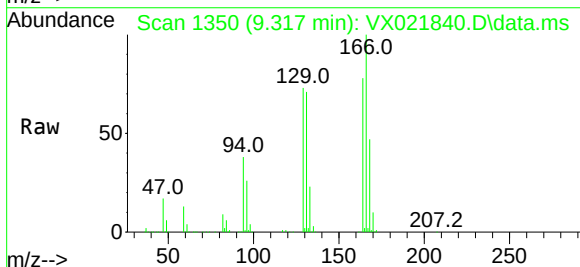




#62
4-Bromofluorobenzene
Concen: 45.10 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 95 Resp: 120838
Ion Ratio Lower Upper
95 100
174 81.7 0.0 154.6
176 79.8 0.0 155.8

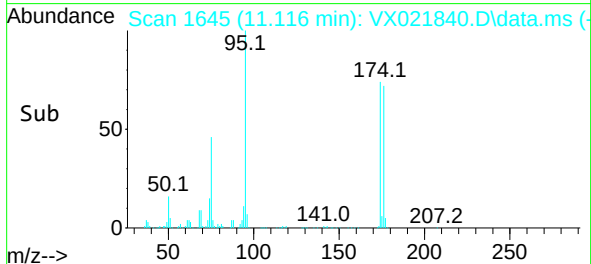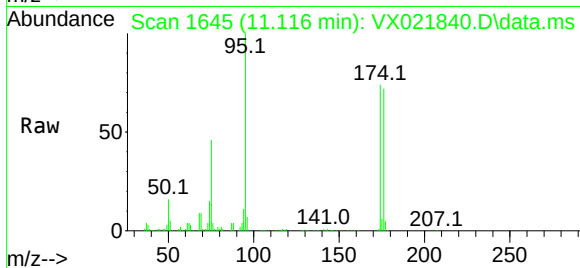

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.092 min Scan# 1477
Delta R.T. 0.001 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 117 Resp: 258951
Ion Ratio Lower Upper
117 100
82 52.5 47.4 71.2
119 32.2 26.6 39.8


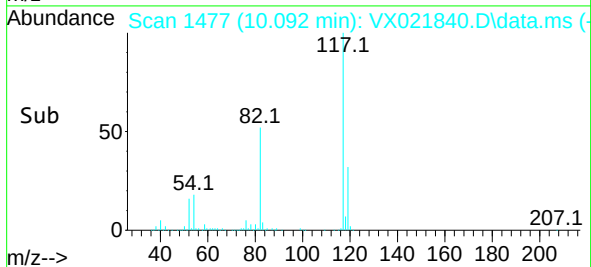

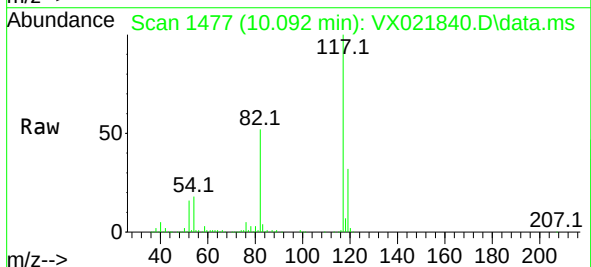




#64
Tetrachloroethene
Concen: 96.01 ug/l
RT: 9.317 min Scan# 1350
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion:164 Resp: 194402
Ion Ratio Lower Upper
164 100
166 127.7 103.4 155.2
129 93.3 70.8 106.2
131 90.5 72.5 108.7

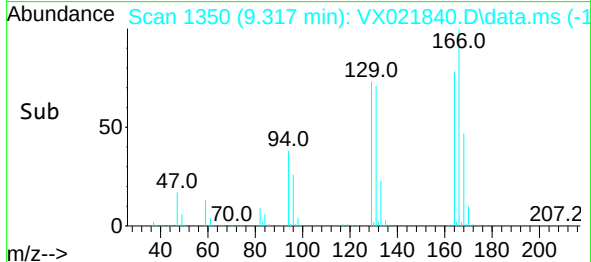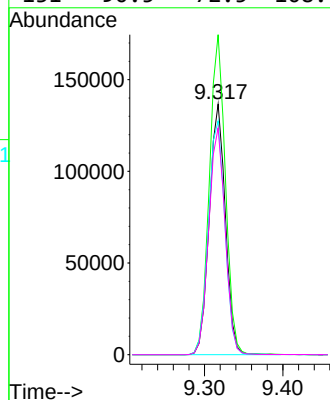

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion:152 Resp: 119634
Ion Ratio Lower Upper
152 100
115 58.5 41.1 123.3
150 156.9 0.0 349.0


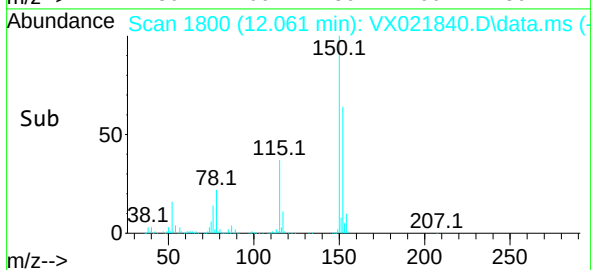
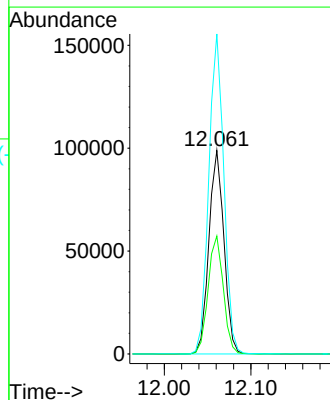
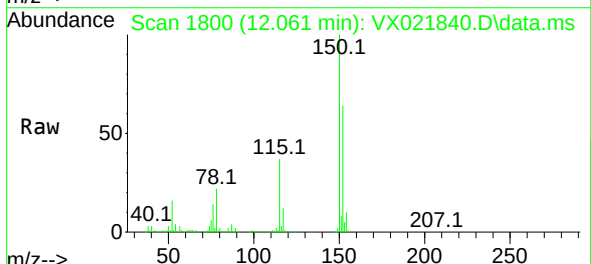


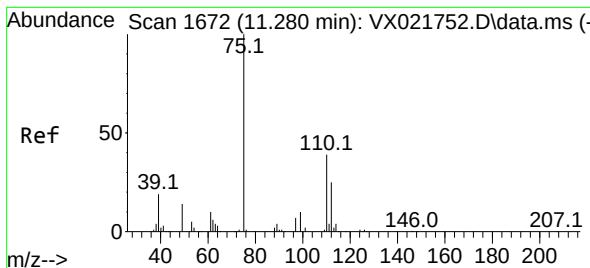

#76
1,2,3-Trichloropropane
Concen: 22.98 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.164 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 75 Resp: 54527
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

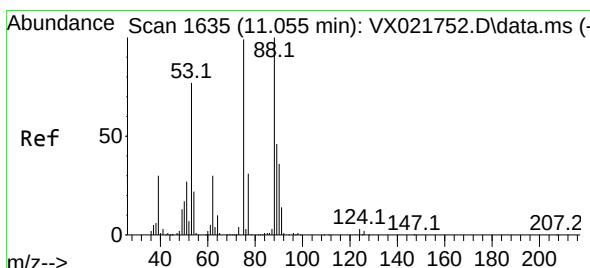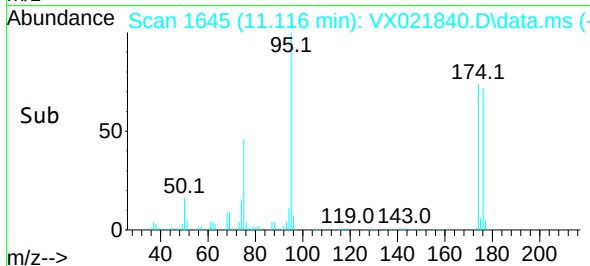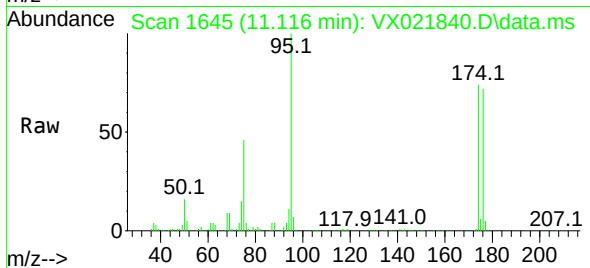

#81
trans-1,4-Dichloro-2-butene
Concen: 52.85 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. 0.061 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 75 Resp: 54527
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


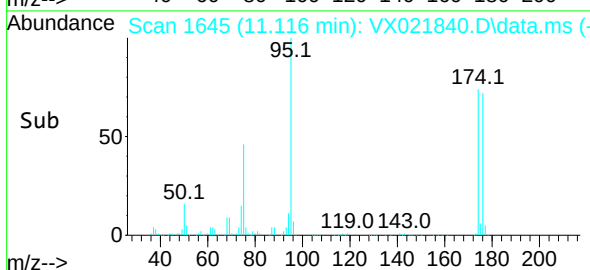

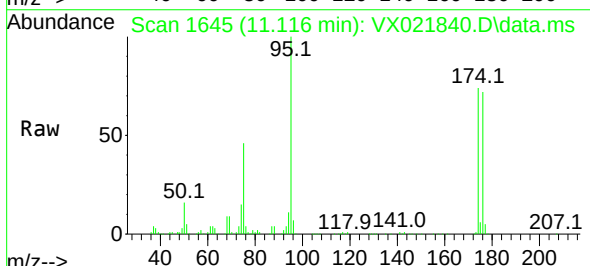


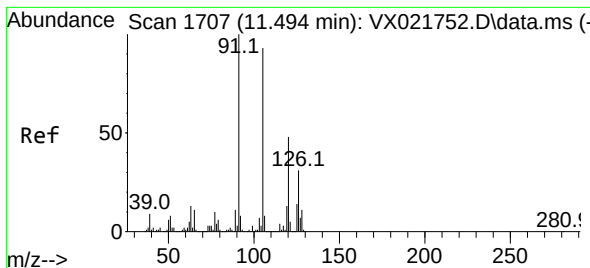

#82
4-Chlorotoluene
Concen: 0.21 ug/l
RT: 11.494 min Scan# 1707
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion: 91 Resp: 1330
Ion Ratio Lower Upper
91 100
126 26.3 14.9 44.5

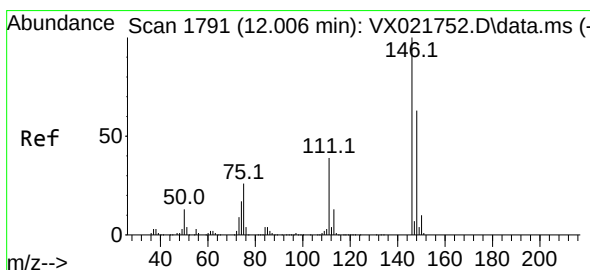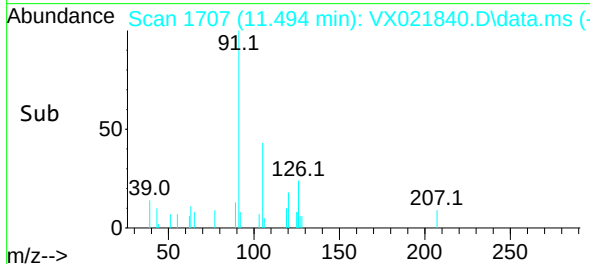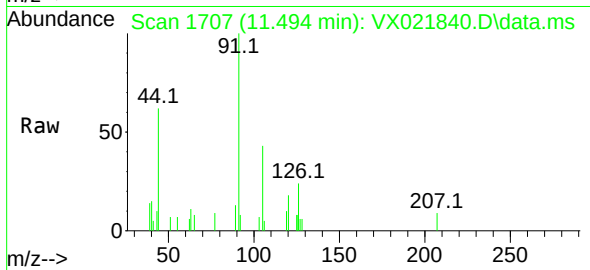

#87
1,3-Dichlorobenzene
Concen: 0.23 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.006 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion: 146 Resp: 875
Ion Ratio Lower Upper
146 100
111 31.2 20.2 60.5
148 66.1 31.9 95.7


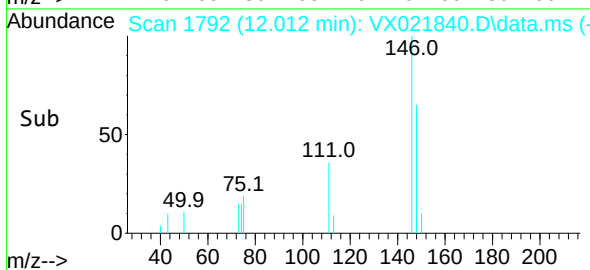

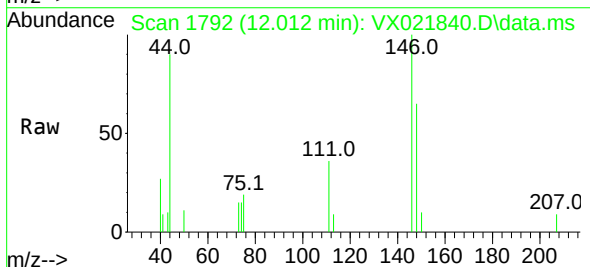




#88
1,4-Dichlorobenzene
Concen: 0.23 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.067 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion:	146	Resp:	875
Ion Ratio	Lower	Upper	
146	100		
111	31.2	19.6	58.8
148	66.1	31.6	95.0

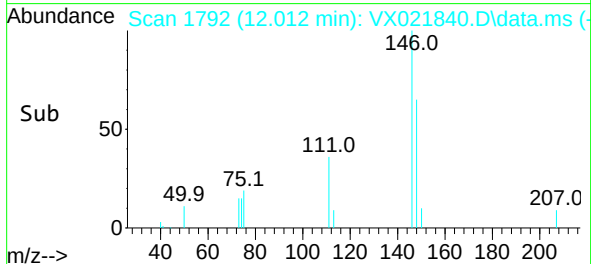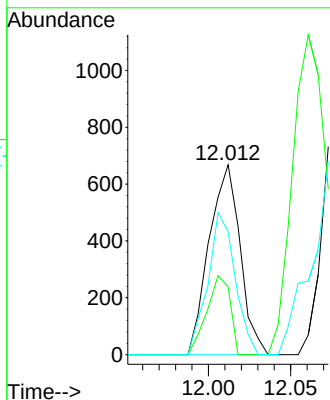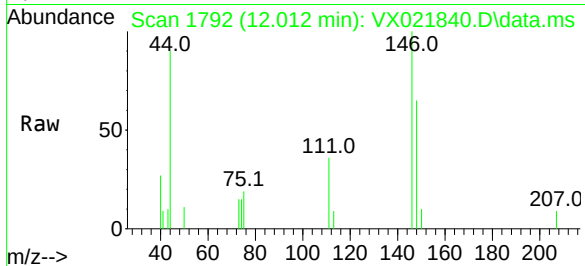

#89
n-Butylbenzene
Concen: 0.37 ug/l
RT: 12.372 min Scan# 1851
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion:	91	Resp:	2401
Ion Ratio	Lower	Upper	
91	100		
92	47.3	27.4	82.0
134	24.2	13.2	39.5


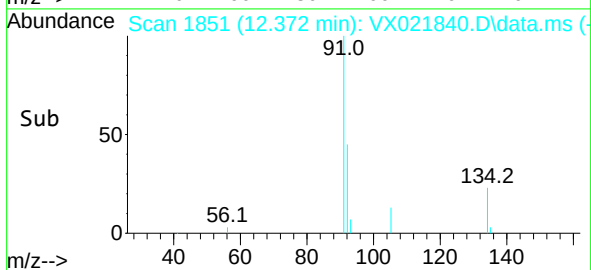
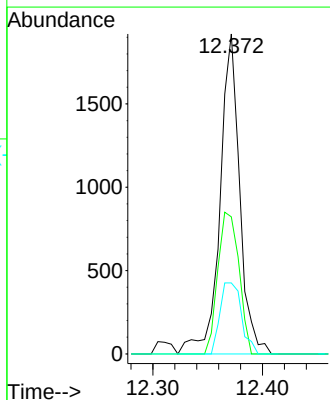
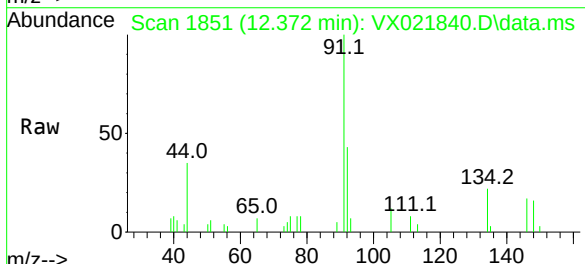




#90
Hexachloroethane
Concen: 3.08 ug/l
RT: 12.579 min Scan# 1885
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion:117 Resp: 4335
Ion Ratio Lower Upper
117 100
201 82.6 40.4 121.2



#93
1,2,4-Trichlorobenzene
Concen: 0.42 ug/l
RT: 13.627 min Scan# 2057
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28

Tgt Ion:180 Resp: 1127
Ion Ratio Lower Upper
180 100
182 93.5 47.7 143.1
145 34.7 15.0 45.0


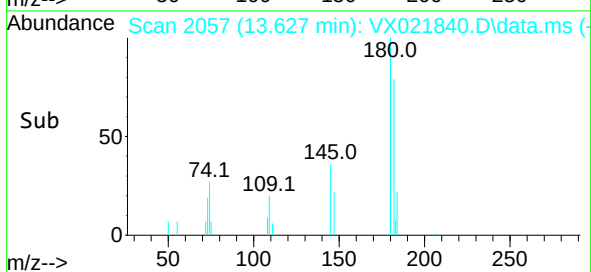






#94
Hexachlorobutadiene
Concen: 0.44 ug/l
RT: 13.762 min Scan# 2079
Delta R.T. -0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28




Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PDDL


Tgt Ion:225	Resp:	576
Ion	Ratio	Lower Upper
225	100	
223	57.6	31.1 93.2
227	58.5	31.6 95.0

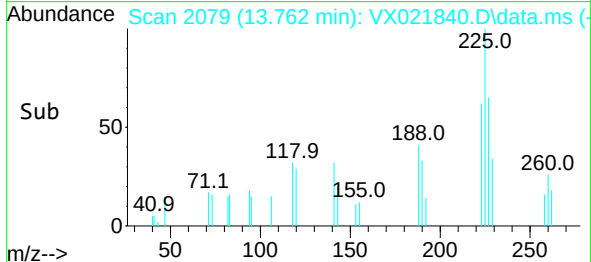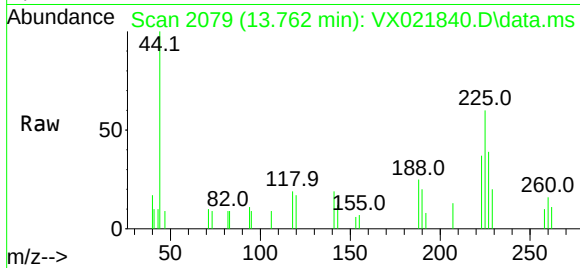

#95
Naphthalene
Concen: 0.28 ug/l
RT: 13.816 min Scan# 2088
Delta R.T. 0.000 min
Lab File: VX021840.D
Acq: 23 Apr 2021 14:28


Tgt Ion:128	Resp:	2231
Ion	Ratio	Lower Upper
128	100	
127	11.6	10.3 15.5
129	12.4	8.8 13.2

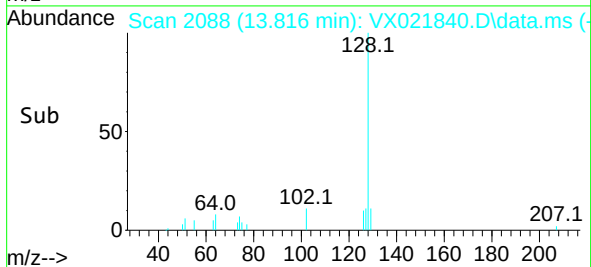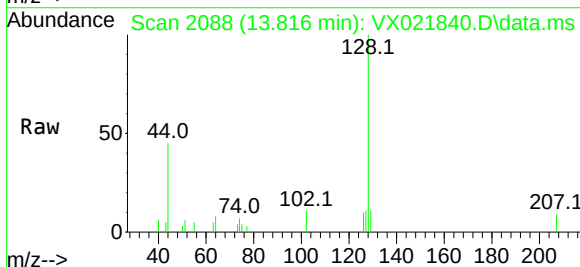



#96
 1,2,3-Trichlorobenzene
 Concen: 0.33 ug/l
 RT: 13.999 min Scan# 2118
 Delta R.T. 0.000 min
 Lab File: VX021840.D
 Acq: 23 Apr 2021 14:28

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-2-PDDL

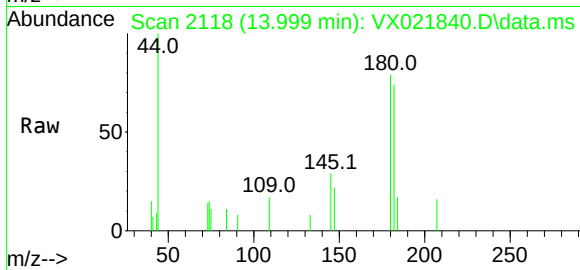

Tgt Ion:	180	Resp:	837
Ion	Ratio	Lower	Upper
180	100		
182	99.5	47.6	142.9
145	30.5	16.1	48.3

