

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
 Data File : VX021837.D
 Acq On : 23 Apr 2021 13:10
 Operator : JC/MD
 Sample : VX0423WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0423WBL01

Quant Time: Apr 26 04:02:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 20 13:46:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.623	168	165129	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.824	114	274844	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.092	117	243996	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.061	152	114522	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.025	65	90660	48.40	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	96.80%
35) Dibromofluoromethane	5.465	113	87680	49.89	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.78%
50) Toluene-d8	8.690	98	326639	48.33	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.66%
62) 4-Bromofluorobenzene	11.116	95	114845	45.51	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.02%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
Data File : VX021837.D
Acq On : 23 Apr 2021 13:10
Operator : JC/MD
Sample : VX0423WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0423WBL01

Quant Time: Apr 26 04:02:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 20 13:46:22 2021
Response via : Initial Calibration




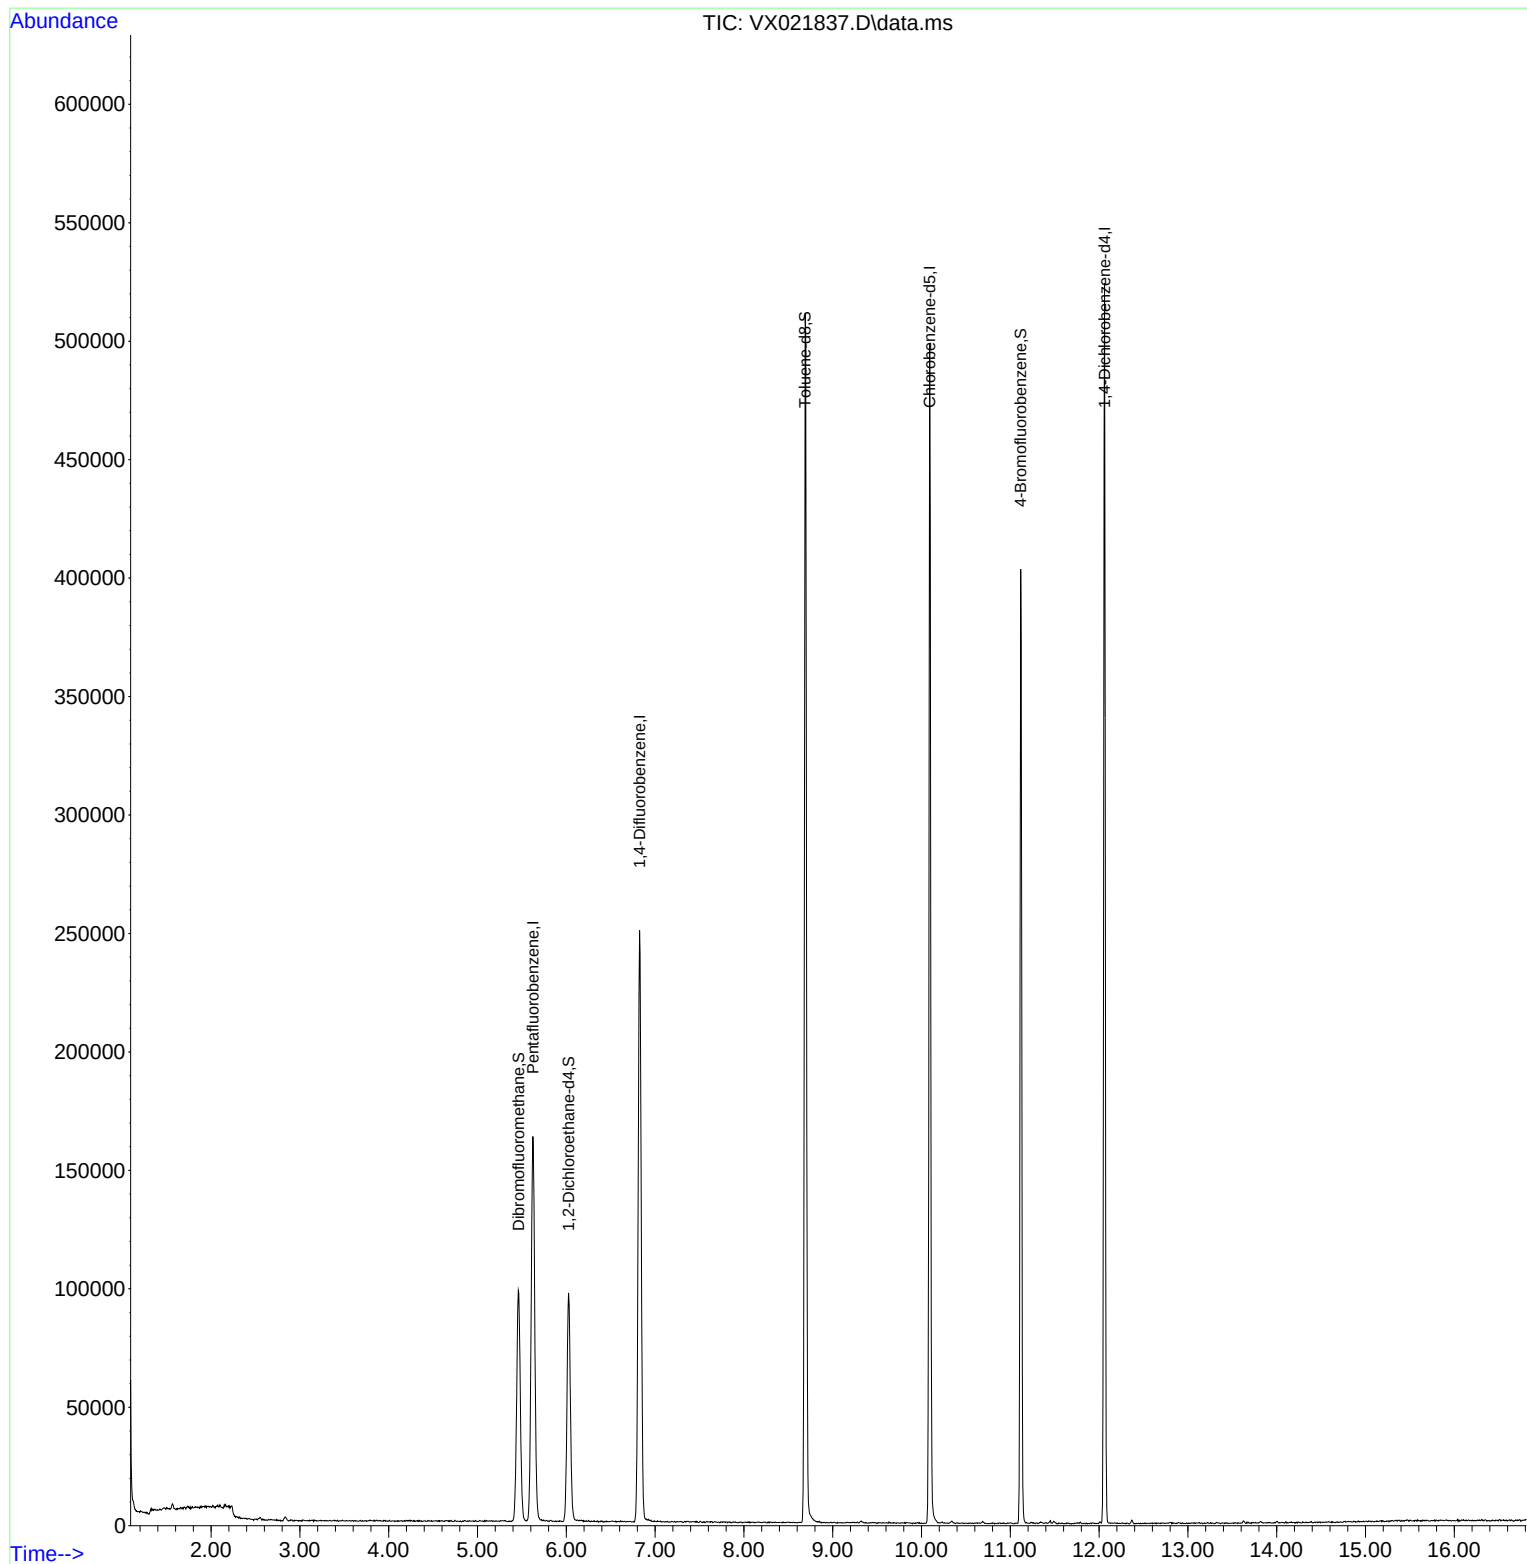


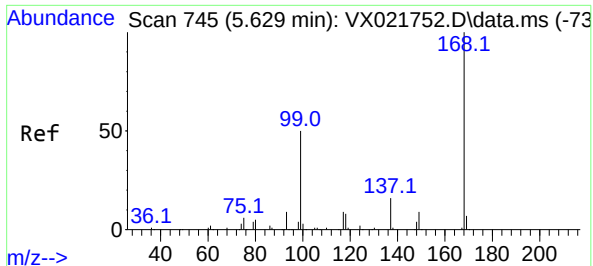

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.623 min Scan# 744
Delta R.T. -0.006 min
Lab File: VX021837.D
Acq: 23 Apr 2021 13:10




Instrument :
MSVOA_X
ClientSampleId :
VX0423WBL01


Tgt Ion:168 Resp: 165129
Ion Ratio Lower Upper
168 100
99 54.2 45.8 68.6

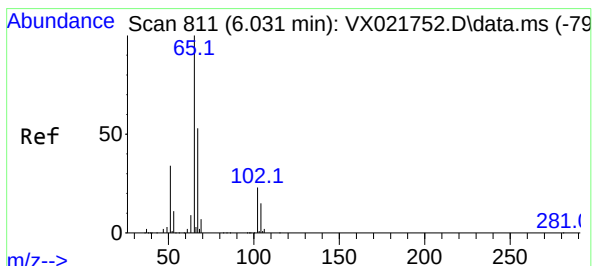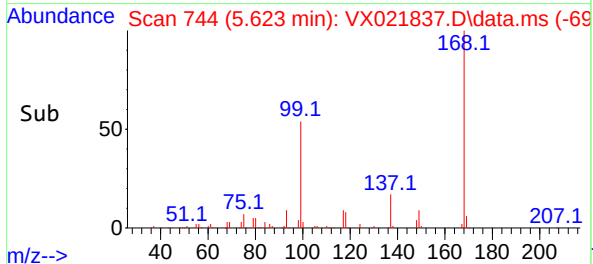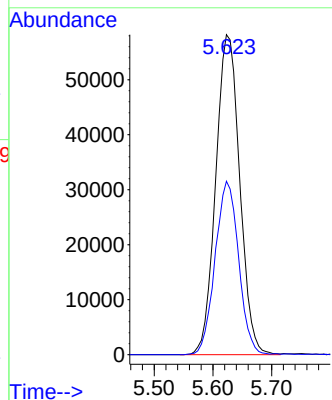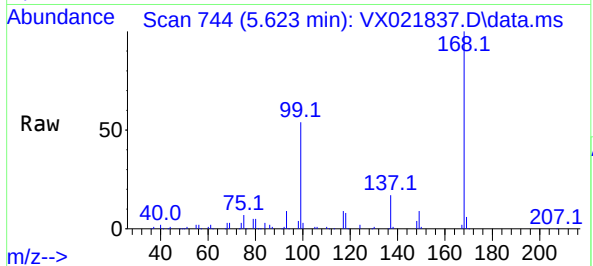

#33
1,2-Dichloroethane-d4
Concen: 48.40 ug/l
RT: 6.025 min Scan# 810
Delta R.T. -0.006 min
Lab File: VX021837.D
Acq: 23 Apr 2021 13:10

Tgt Ion: 65 Resp: 90660
Ion Ratio Lower Upper
65 100
67 55.1 0.0 105.4

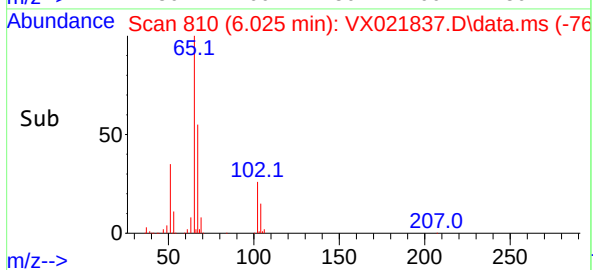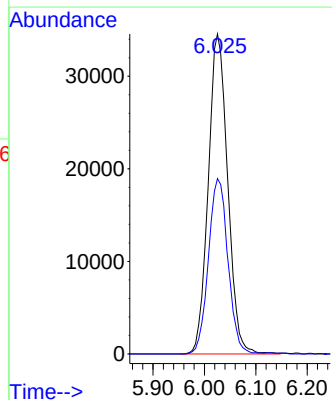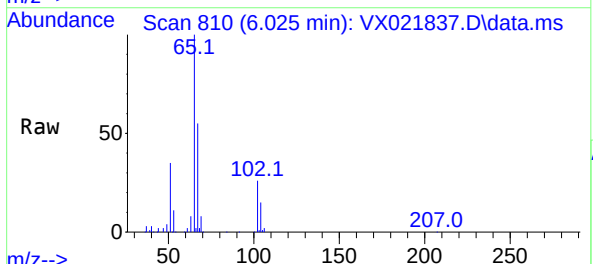

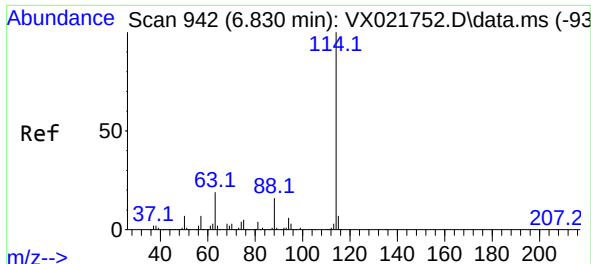

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.824 min Scan# 941

Delta R.T. -0.006 min

Lab File: VX021837.D

Acq: 23 Apr 2021 13:10





Tgt Ion:114 Resp: 274844

Ion Ratio Lower Upper

114 100

63 18.6 0.0 40.8

88 16.0 0.0 32.8

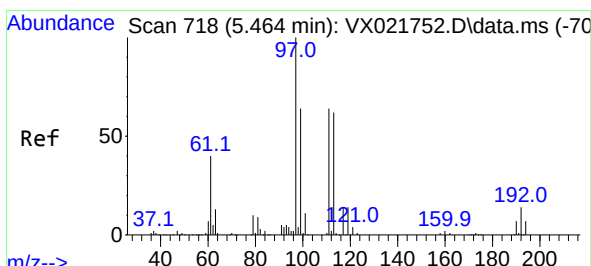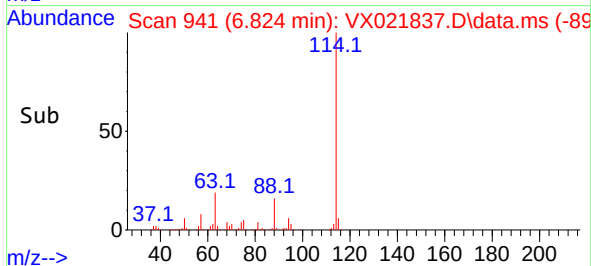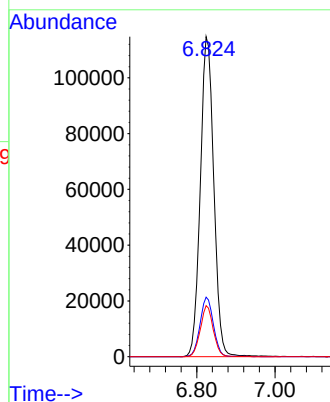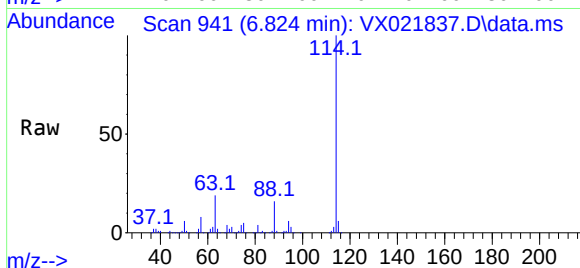

#35

Dibromofluoromethane

Concen: 49.89 ug/l

RT: 5.465 min Scan# 718

Delta R.T. 0.001 min

Lab File: VX021837.D

Acq: 23 Apr 2021 13:10




Tgt Ion:113 Resp: 87680


Ion Ratio Lower Upper

113 100

111 102.9 81.9 122.9

192 20.0 16.7 25.1


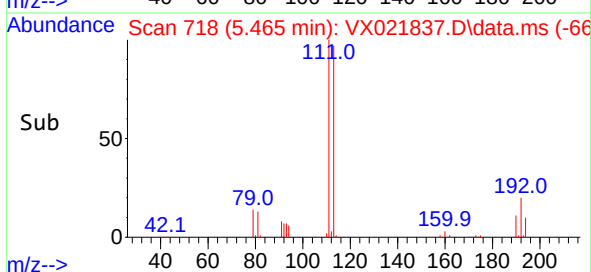
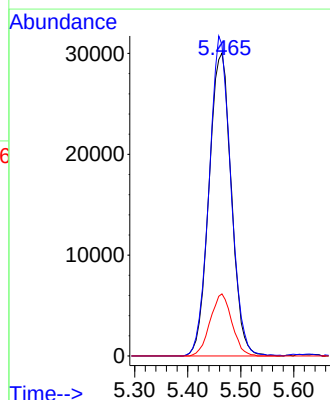
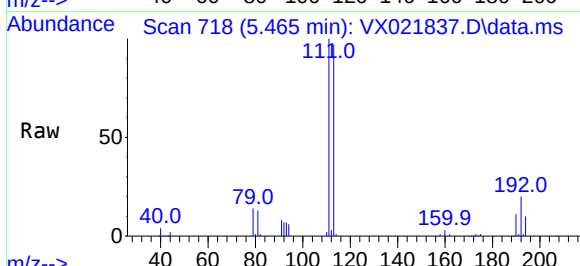


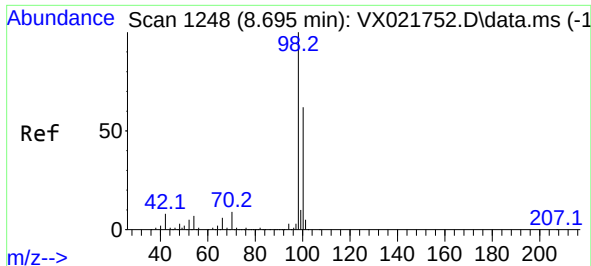

#50
Toluene-d8
Concen: 48.33 ug/l
RT: 8.690 min Scan# 1247
Delta R.T. -0.005 min
Lab File: VX021837.D
Acq: 23 Apr 2021 13:10




Instrument :
MSVOA_X
ClientSampleId :
VX0423WBL01


Tgt Ion: 98 Resp: 326639
Ion Ratio Lower Upper
98 100
100 65.9 51.9 77.9

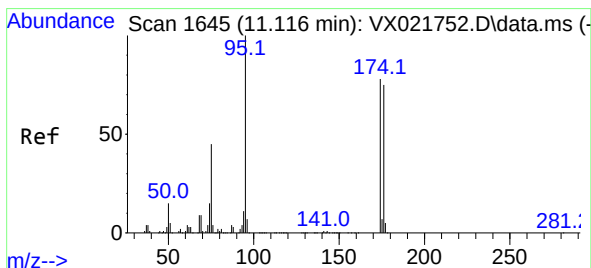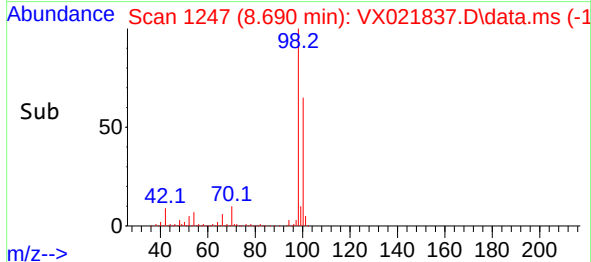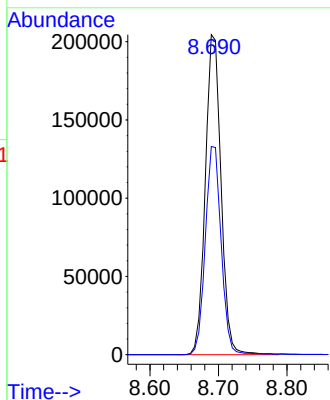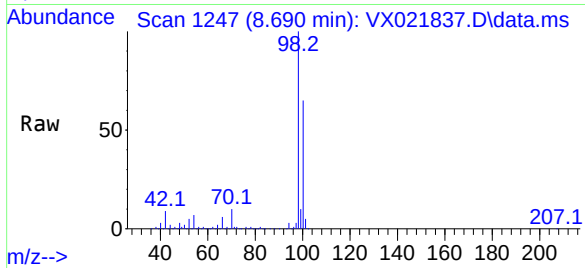

#62
4-Bromofluorobenzene
Concen: 45.51 ug/l
RT: 11.116 min Scan# 1645
Delta R.T. -0.000 min
Lab File: VX021837.D
Acq: 23 Apr 2021 13:10

Tgt Ion: 95 Resp: 114845
Ion Ratio Lower Upper
95 100
174 80.9 0.0 154.6
176 79.0 0.0 155.8


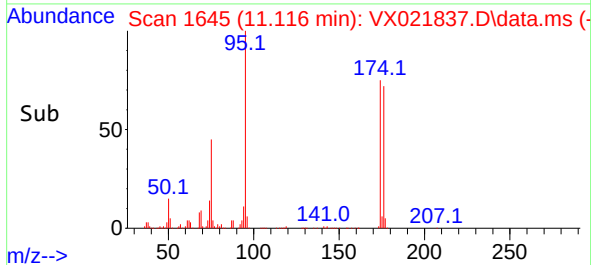
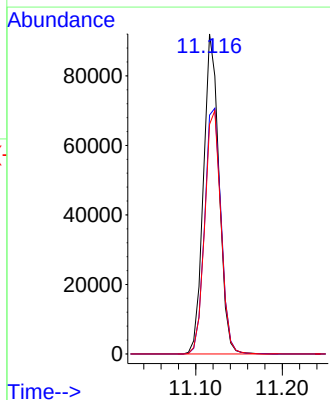
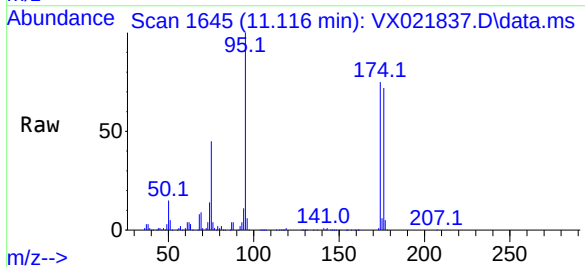


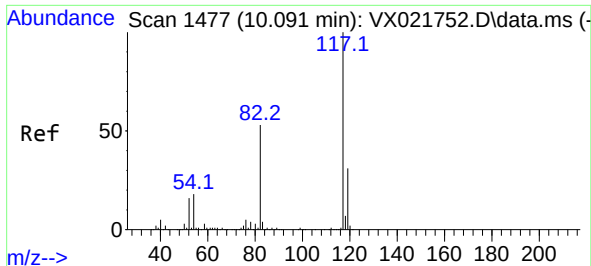

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.092 min Scan# 1477
Delta R.T. 0.001 min
Lab File: VX021837.D
Acq: 23 Apr 2021 13:10

Instrument :
MSVOA_X
ClientSampleId :
VX0423WBL01

Tgt Ion:117 Resp: 243996
Ion Ratio Lower Upper
117 100
82 52.0 47.4 71.2
119 31.8 26.6 39.8

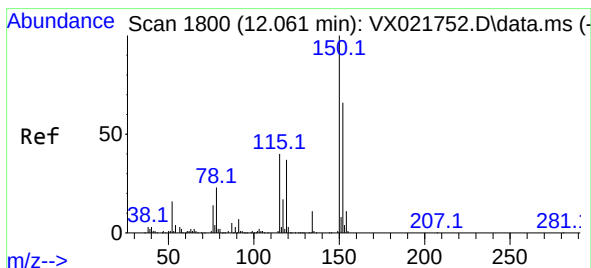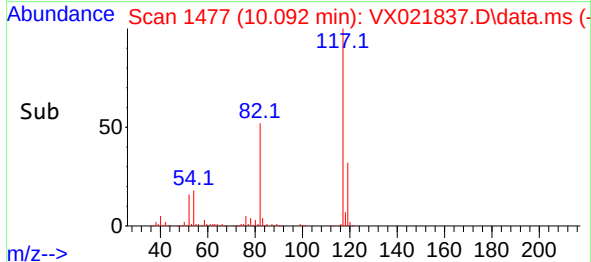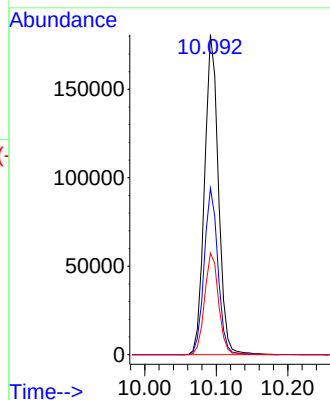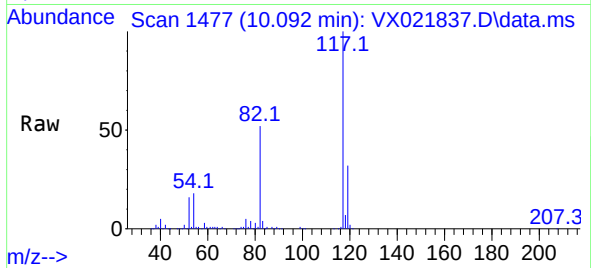

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.061 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VX021837.D
Acq: 23 Apr 2021 13:10

Tgt Ion:152 Resp: 114522
Ion Ratio Lower Upper
152 100
115 57.0 41.1 123.3
150 156.6 0.0 349.0

