

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
 Data File : VX021843.D
 Acq On : 23 Apr 2021 15:37
 Operator : JC/MD
 Sample : M2138-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-2-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M

Title : SW846 8260

Signal : TIC: VX021843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.581	240	245	251	rVB	5167	9909	1.09%	0.206%
2	5.464	707	718	734	rBV2	107588	308554	33.96%	6.414%
3	5.629	734	745	756	rBV	179384	497350	54.74%	10.338%
4	6.031	800	811	826	rBV	104629	275536	30.33%	5.728%
5	6.830	932	942	957	rBV	278316	653107	71.88%	13.576%
6	8.695	1241	1248	1266	rBV	581060	908578	100.00%	18.886%
7	9.317	1344	1350	1355	rBV	19055	28062	3.09%	0.583%
8	10.091	1471	1477	1496	rBV	535493	762213	83.89%	15.844%
9	11.122	1640	1646	1656	rBV	460680	599837	66.02%	12.469%
10	12.061	1794	1800	1808	rBV	631728	767591	84.48%	15.956%




Sum of corrected areas: 4810737

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
Data File : VX021843.D
Acq On : 23 Apr 2021 15:37
Operator : JC/MD
Sample : M2138-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

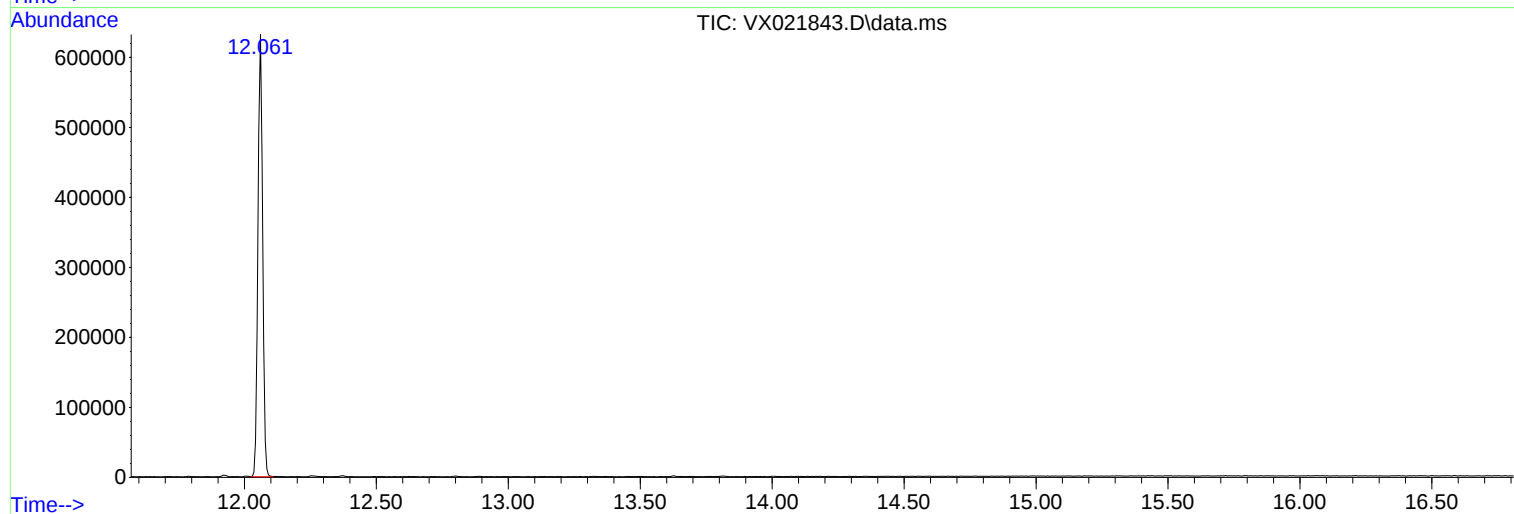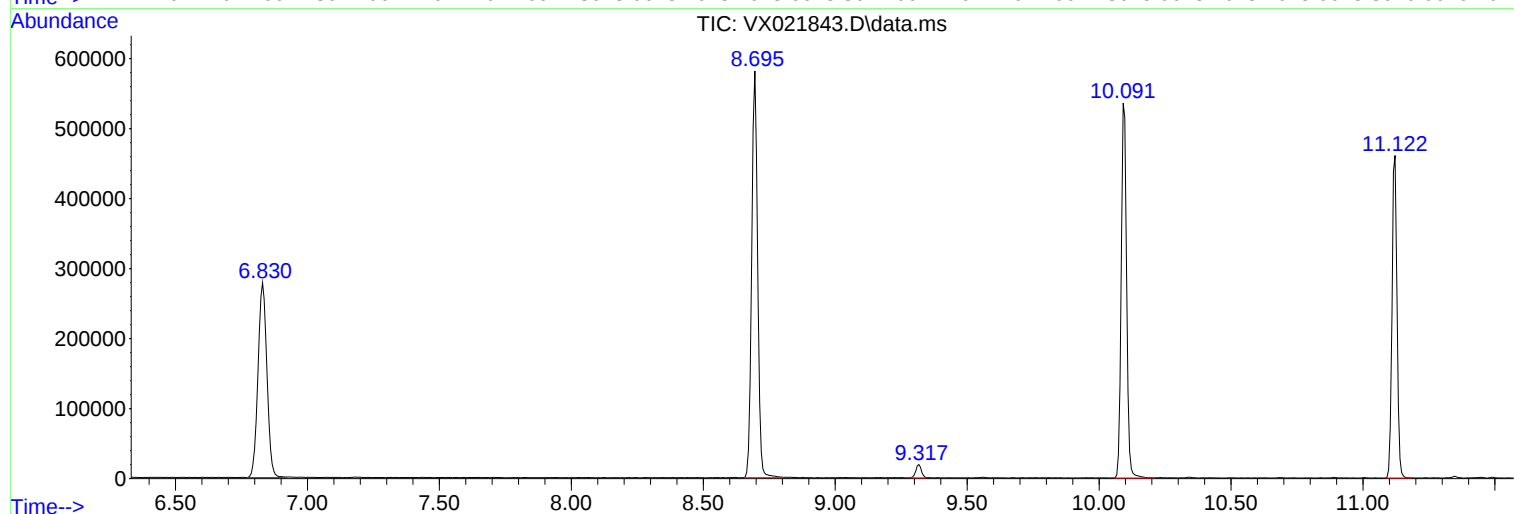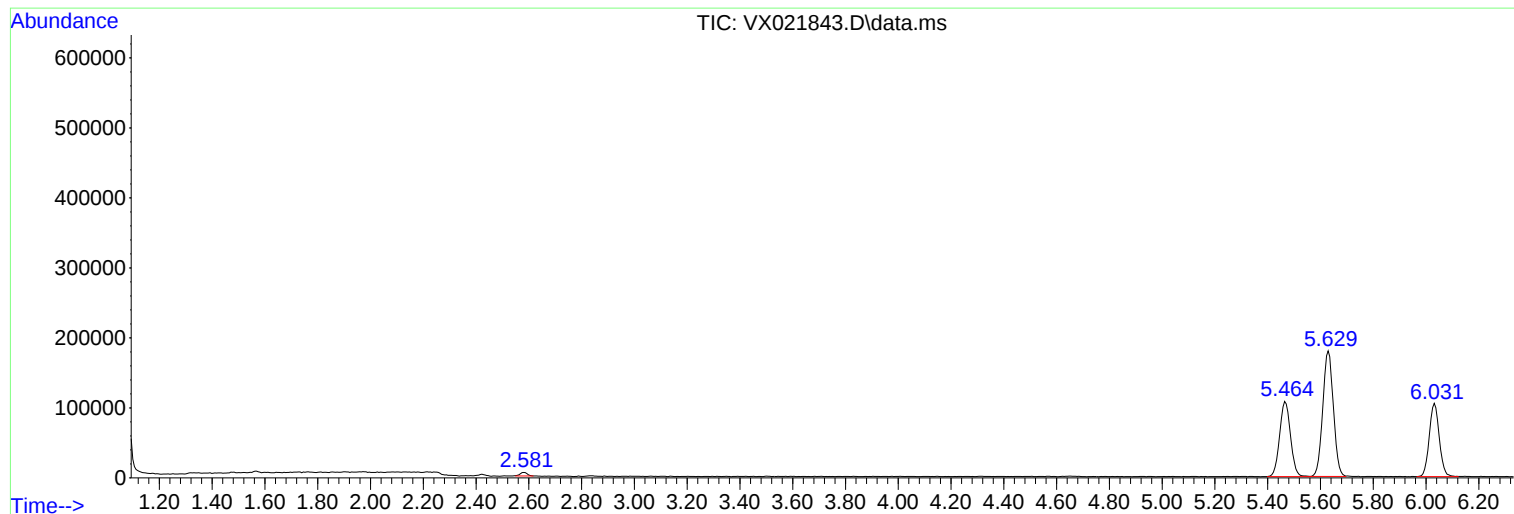

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
Data File : VX021843.D
Acq On : 23 Apr 2021 15:37
Operator : JC/MD
Sample : M2138-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042321\
Data File : VX021843.D
Acq On : 23 Apr 2021 15:37
Operator : JC/MD
Sample : M2138-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-2-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042021W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
