

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042324\
 Data File : VX041212.D
 Acq On : 23 Apr 2024 13:27
 Operator : JC/MD
 Sample : P2233-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 24 01:46:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 23 05:30:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	195400	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	286694	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	217316	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	131174	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	101436	54.534	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 109.060%	
35) Dibromofluoromethane	5.379	113	90198	51.721	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.440%	
50) Toluene-d8	8.647	98	318688	54.164	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 108.320%	
62) 4-Bromofluorobenzene	11.079	95	117436	54.075	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 108.160%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.294	50	651	0.389	ug/l	99
5) Bromomethane	1.599	94	1080	1.146	ug/l	83
6) Chloroethane	1.648	64	294	0.462	ug/l #	66
9) 1,1,2-Trichlorotrifluo...	2.313	101	896	0.587	ug/l #	87
10) Methyl Iodide	2.441	142	737	0.401	ug/l #	72
11) Tert butyl alcohol	3.002	59	92	0.276	ug/l #	78
12) 1,1-Dichloroethene	2.307	96	3275	2.300	ug/l	93
13) Acrolein	2.252	56	336	0.899	ug/l #	14
16) Acetone	2.398	43	4679	6.911	ug/l #	73
17) Carbon Disulfide	2.508	76	1262	0.424	ug/l	99
18) Methyl Acetate	2.721	43	806	0.402	ug/l #	75
20) Methylene Chloride	2.788	84	1633	0.988	ug/l	87
24) 1,1-Dichloroethane	3.605	63	29456	10.535	ug/l	99
25) 2-Butanone	4.605	43	249	0.215	ug/l #	51
27) cis-1,2-Dichloroethene	4.495	96	7422	3.805	ug/l	81
28) Bromochloromethane	5.099	49	1706	1.608	ug/l #	16
30) Chloroform	5.093	83	23092	7.695	ug/l	96
31) Cyclohexane	5.550	56	3057	1.221	ug/l #	5
36) 1,1-Dichloropropene	5.544	75	11484	5.147	ug/l #	51
38) Carbon Tetrachloride	5.550	117	16513	6.626	ug/l #	15
39) Methylcyclohexane	7.123	83	3360	1.135	ug/l #	1
42) 1,2-Dichloroethane	6.092	62	3684	1.542	ug/l	94
44) Trichloroethene	7.123	130	322340	160.883	ug/l	86
47) Bromodichloromethane	7.824	83	1593	0.701	ug/l #	90
49) 1,4-Dioxane	7.696	88	308	7.671	ug/l #	76
52) Toluene	8.720	92	43320	9.976	ug/l	96
53) t-1,3-Dichloropropene	8.726	75	532	0.239	ug/l #	1
60) Dibromochloromethane	9.525	129	502	0.257	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	56422	26.697	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	56422	75.320	ug/l #	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042324\
Data File : VX041212.D
Acq On : 23 Apr 2024 13:27
Operator : JC/MD
Sample : P2233-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 24 01:46:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 23 05:30:28 2024
Response via : Initial Calibration




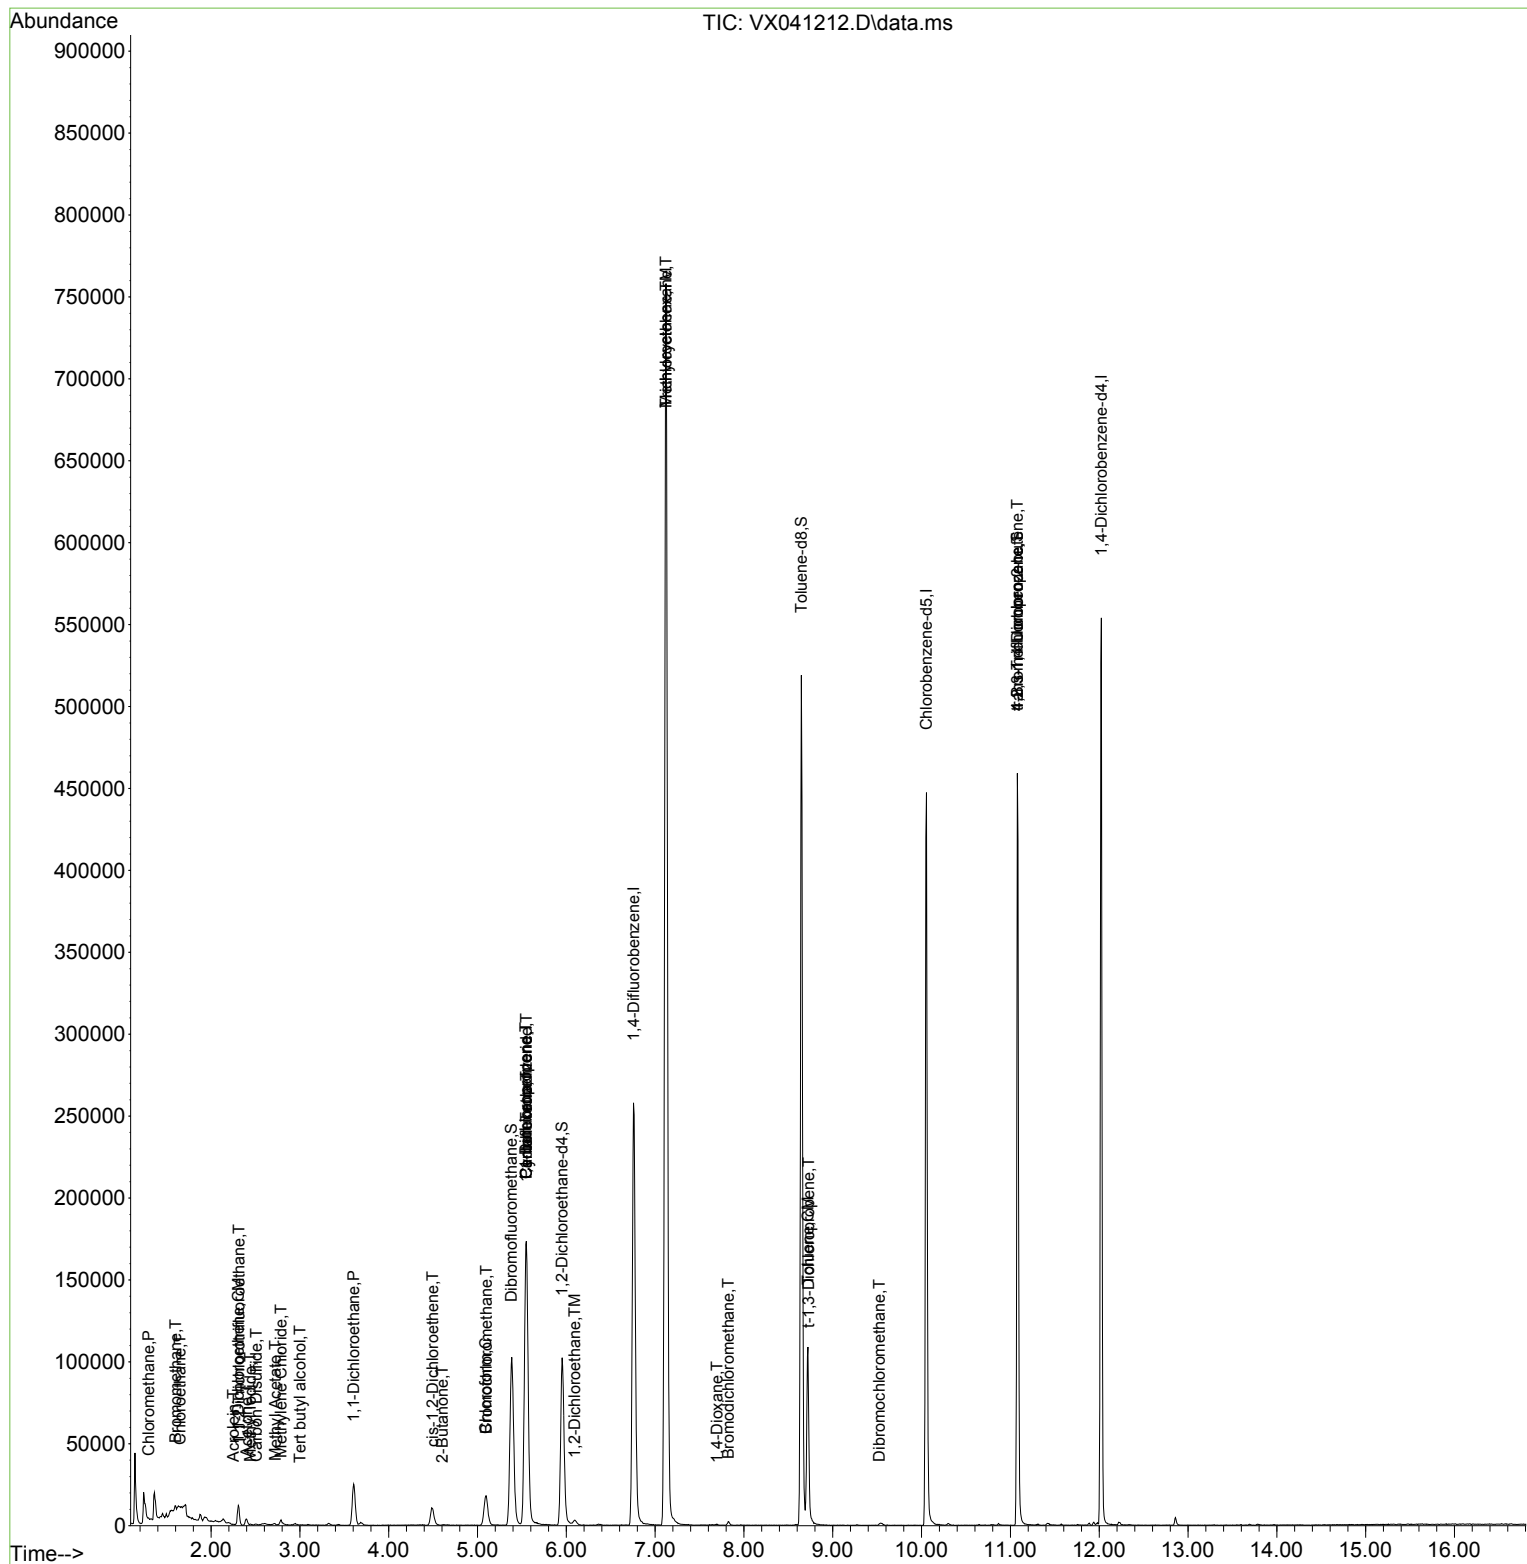




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 195400
Ion Ratio Lower Upper
168 100
99 47.9 56.6 85.0#



#3
Chloromethane
Concen: 0.389 ug/l
RT: 1.294 min Scan# 34
Delta R.T. -0.006 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Tgt Ion: 50 Resp: 651
Ion Ratio Lower Upper
50 100
52 32.5 25.5 38.3

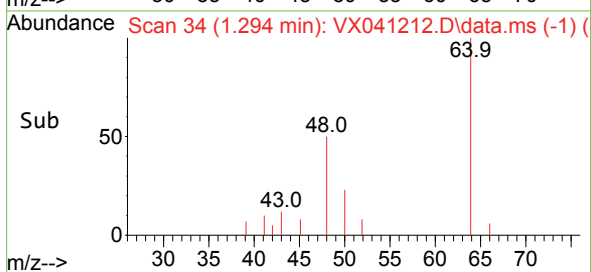

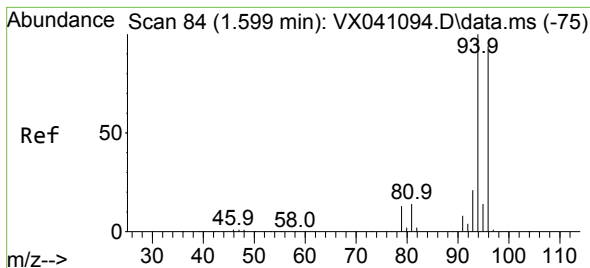

#5

Bromomethane

Concen: 1.146 ug/l

RT: 1.599 min Scan# 84

Delta R.T. -0.000 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 94 Resp: 1080

Ion Ratio Lower Upper

94 100

96 76.8 74.6 111.8

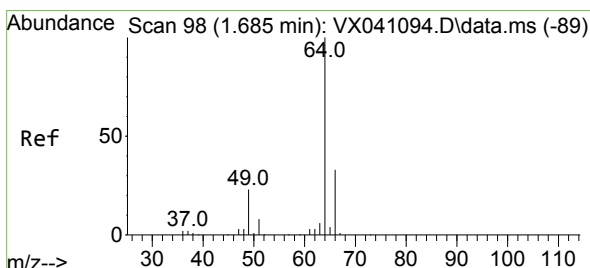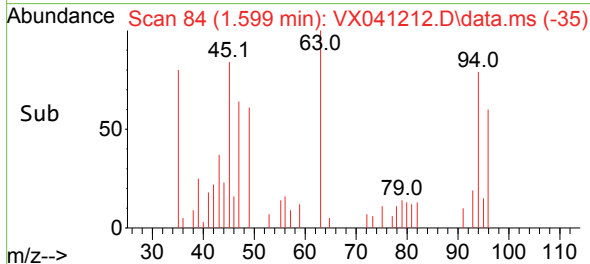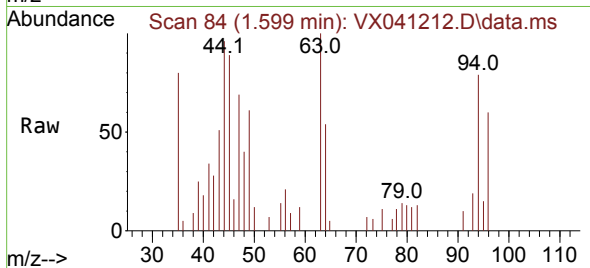

#6

Chloroethane

Concen: 0.462 ug/l

RT: 1.648 min Scan# 92

Delta R.T. -0.018 min

Lab File: VX041212.D




Acq: 23 Apr 2024 13:27


Tgt Ion: 64 Resp: 294

Ion Ratio Lower Upper

64 100


66 50.3 25.1 37.7#

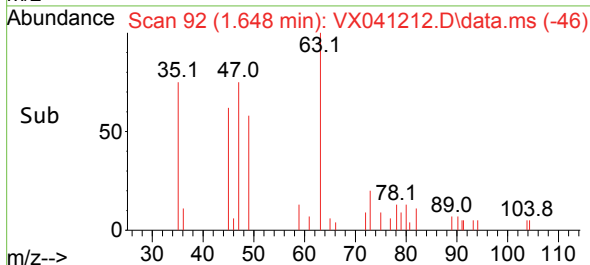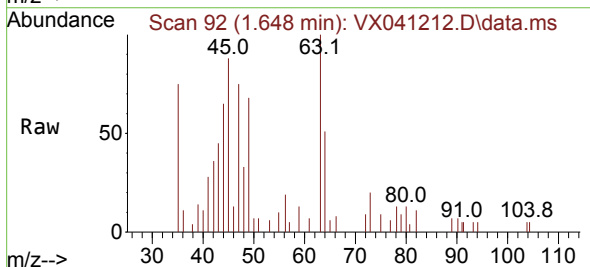



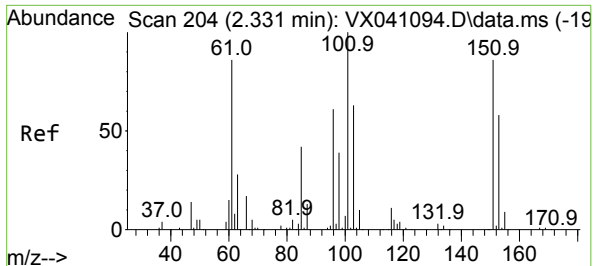


#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.587 ug/l
RT: 2.313 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:101 Resp: 896
Ion Ratio Lower Upper
101 100
85 36.2 37.0 55.6#
151 82.4 58.6 87.8

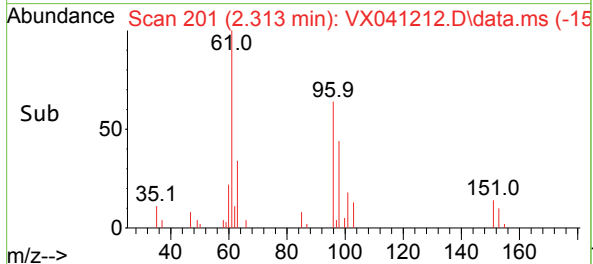

#10
Methyl Iodide
Concen: 0.401 ug/l
RT: 2.441 min Scan# 222
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Tgt Ion:142 Resp: 737
Ion Ratio Lower Upper
142 100
127 33.8 41.6 62.4#
141 0.0 11.6 17.4#

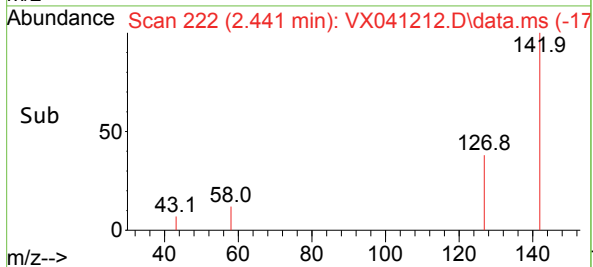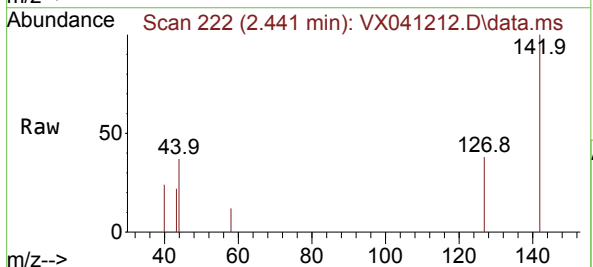



#11

Tert butyl alcohol

Concen: 0.276 ug/l

RT: 3.002 min Scan# 314

Delta R.T. -0.061 min


Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 59 Resp: 92

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#



#12

1,1-Dichloroethene

Concen: 2.300 ug/l

RT: 2.307 min Scan# 200

Delta R.T. -0.000 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27




Tgt Ion: 96 Resp: 3275


Ion Ratio Lower Upper

96 100

61 170.5 144.6 216.8

98 67.5 50.4 75.6



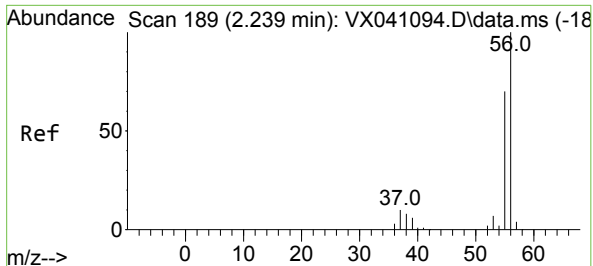

#13

Acrolein

Concen: 0.899 ug/l

RT: 2.252 min Scan# 191

Delta R.T. 0.012 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 336

Ion Ratio Lower Upper

56 100

55 0.0 57.1 85.7#

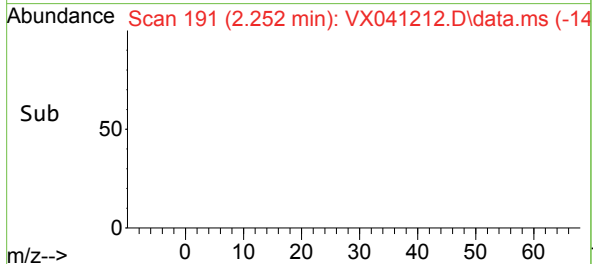

#16

Acetone

Concen: 6.911 ug/l

RT: 2.398 min Scan# 215

Delta R.T. -0.000 min

Lab File: VX041212.D




Acq: 23 Apr 2024 13:27


Tgt Ion: 43 Resp: 4679

Ion Ratio Lower Upper

43 100

58 41.7 21.9 32.9#

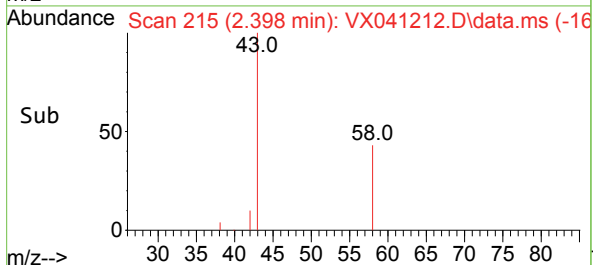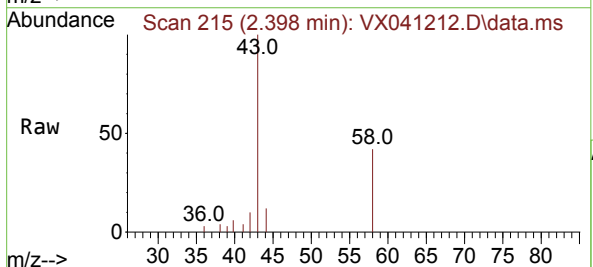



#17

Carbon Disulfide

Concen: 0.424 ug/l

RT: 2.508 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 1262

Ion Ratio Lower Upper

76 100

78 9.0 7.0 10.6



#18

Methyl Acetate

Concen: 0.402 ug/l

RT: 2.721 min Scan# 268

Delta R.T. 0.012 min

Lab File: VX041212.D




Acq: 23 Apr 2024 13:27


Tgt Ion: 43 Resp: 806

Ion Ratio Lower Upper

43 100


74 10.5 17.8 26.8#








#20
Methylene Chloride
Concen: 0.988 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:	84	Resp:	1633
Ion	Ratio	Lower	Upper
84	100		
49	112.1	103.6	155.4
51	34.5	33.8	50.6
86	55.1	49.4	74.0



#24
1,1-Dichloroethane
Concen: 10.535 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27


Tgt Ion:	63	Resp:	29456
Ion	Ratio	Lower	Upper
63	100		
98	7.0	3.3	9.8
100	4.7	2.1	6.5








#25
2-Butanone
Concen: 0.215 ug/l
RT: 4.605 min Scan# 51
Delta R.T. 0.037 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 43 Resp: 249
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#



#27
cis-1,2-Dichloroethene
Concen: 3.805 ug/l
RT: 4.495 min Scan# 559
Delta R.T. 0.012 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Tgt Ion: 96 Resp: 7422
Ion Ratio Lower Upper
96 100
61 121.6 0.0 312.2
98 65.6 0.0 129.0









#28
Bromochloromethane
Concen: 1.608 ug/l
RT: 5.099 min Scan# 61
Delta R.T. 0.195 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 49 Resp: 1706
Ion Ratio Lower Upper
49 100
129 0.0 0.0 3.8
130 0.0 57.5 86.3#



#30
Chloroform
Concen: 7.695 ug/l
RT: 5.093 min Scan# 657
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27


Tgt Ion: 83 Resp: 23092
Ion Ratio Lower Upper
83 100
85 59.9 50.3 75.5





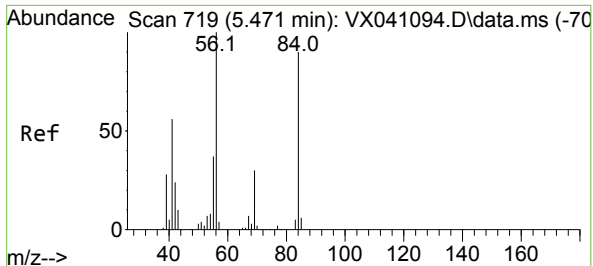


#31
Cyclohexane
Concen: 1.221 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.085 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 3057
Ion Ratio Lower Upper
56 100
69 156.1 23.4 35.2#
84 123.1 65.9 98.9#

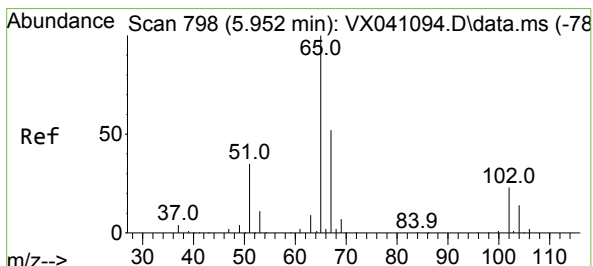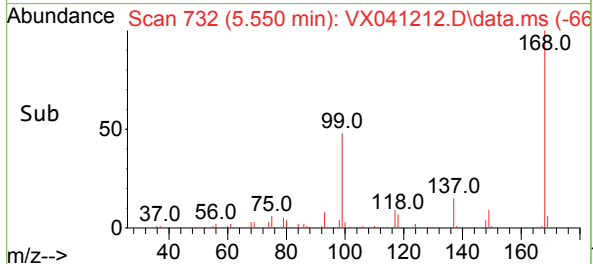

#33
1,2-Dichloroethane-d4
Concen: 54.534 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Tgt Ion: 65 Resp: 101436
Ion Ratio Lower Upper
65 100
67 50.6 0.0 100.2


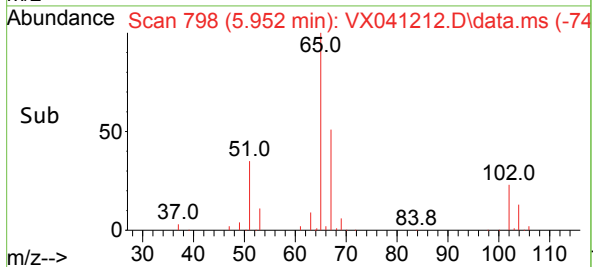

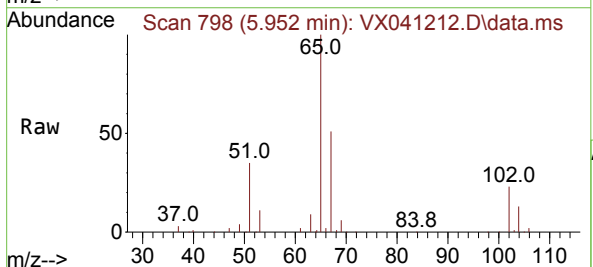


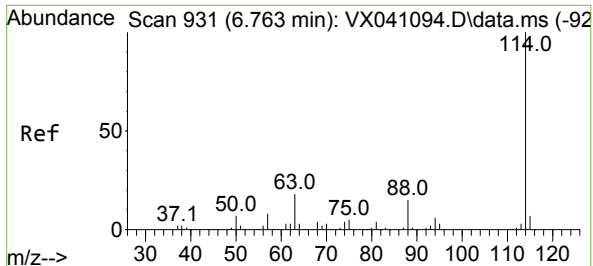

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 286694
Ion Ratio Lower Upper
114 100
63 18.9 0.0 45.0
88 14.9 0.0 36.6

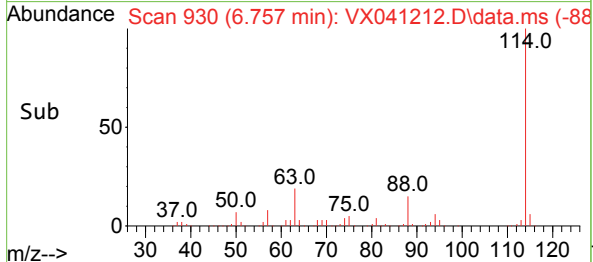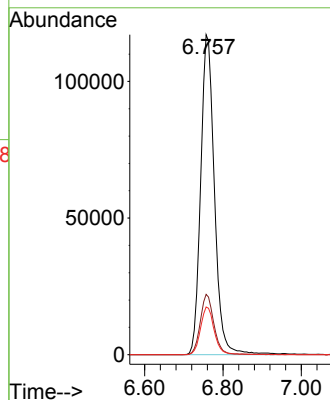

#35
Dibromofluoromethane
Concen: 51.721 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27


Tgt Ion:113 Resp: 90198
Ion Ratio Lower Upper
113 100
111 101.4 82.9 124.3
192 26.2 13.3 19.9#

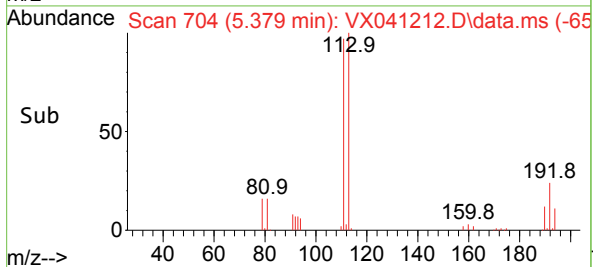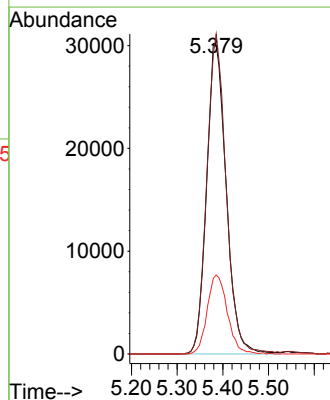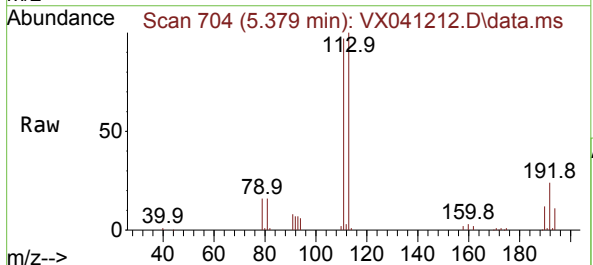






#36
1,1-Dichloropropene
Concen: 5.147 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 11484
Ion Ratio Lower Upper
75 100
110 9.4 17.0 50.9#
77 0.0 24.7 37.1#



#38
Carbon Tetrachloride
Concen: 6.626 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.122 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27


Tgt Ion: 117 Resp: 16513
Ion Ratio Lower Upper
117 100
119 5.3 78.2 117.2#
121 0.0 24.4 36.6#

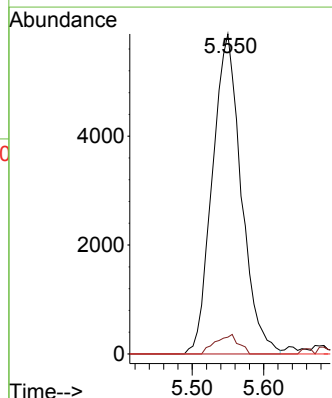






#39
Methylcyclohexane
Concen: 1.135 ug/l
RT: 7.123 min Scan# 90
Delta R.T. -0.250 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 83 Resp: 3360
Ion Ratio Lower Upper
83 100
55 0.0 64.6 97.0#
98 197.9 36.7 55.1#

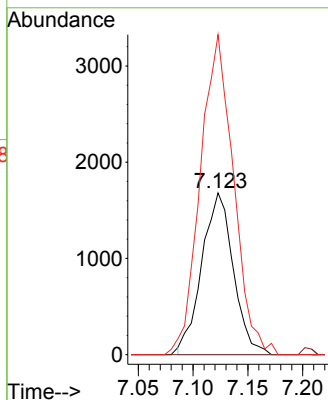

#42
1,2-Dichloroethane
Concen: 1.542 ug/l
RT: 6.092 min Scan# 821
Delta R.T. 0.006 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Tgt Ion: 62 Resp: 3684
Ion Ratio Lower Upper
62 100
98 10.3 0.0 16.0

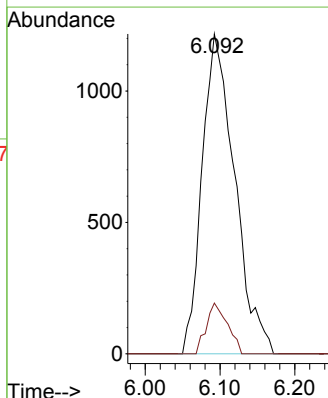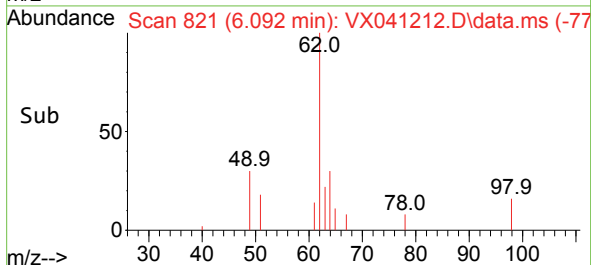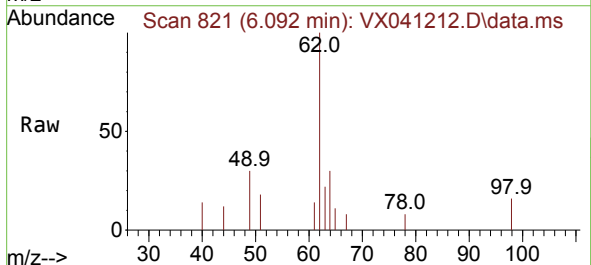



#44

Trichloroethene

Concen: 160.883 ug/l

RT: 7.123 min Scan# 990

Delta R.T. -0.000 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:130 Resp: 322340

Ion Ratio Lower Upper

130 100

95 88.4 0.0 204.4

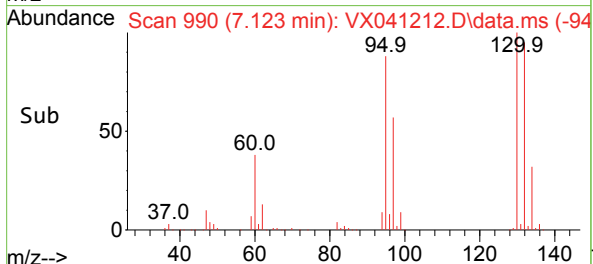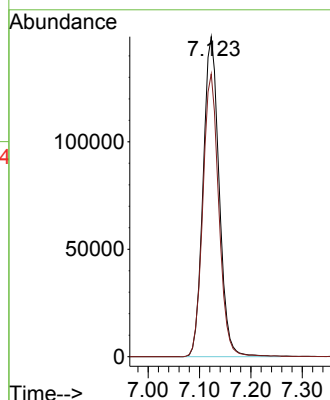

#47

Bromodichloromethane

Concen: 0.701 ug/l

RT: 7.824 min Scan# 1105

Delta R.T. -0.000 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27




Tgt Ion: 83 Resp: 1593


Ion Ratio Lower Upper

83 100

85 70.3 49.8 74.6


127 11.3 7.1 10.7#

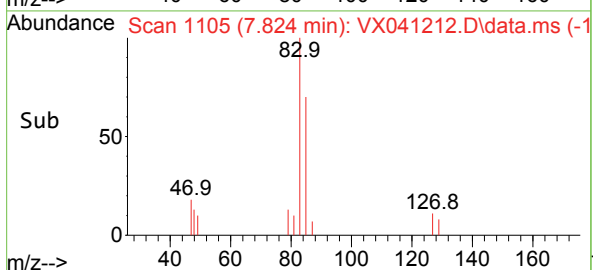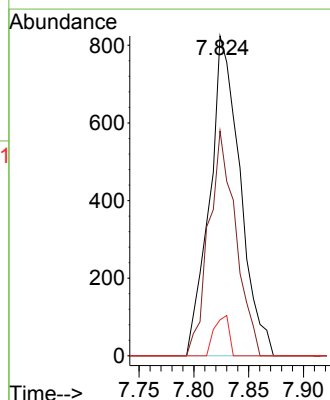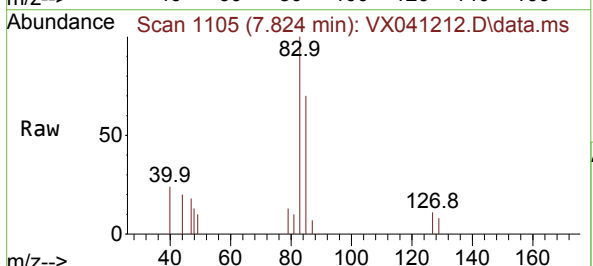






#49
1,4-Dioxane
Concen: 7.671 ug/l
RT: 7.696 min Scan# 1084
Delta R.T. 0.018 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 88 Resp: 308
Ion Ratio Lower Upper
88 100
43 31.8 0.0 0.0#
58 54.2 60.1 90.1#

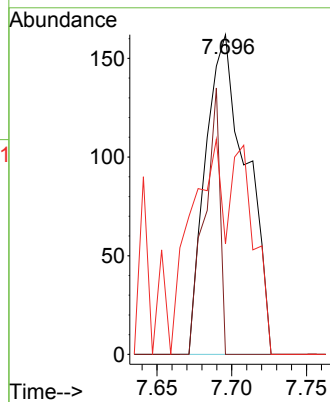

#50
Toluene-d8
Concen: 54.164 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Tgt Ion: 98 Resp: 318688
Ion Ratio Lower Upper
98 100
100 66.3 53.1 79.7


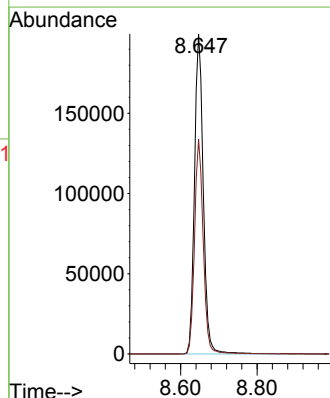






#52
Toluene
Concen: 9.976 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 43320
Ion Ratio Lower Upper
92 100
91 172.7 134.2 201.2

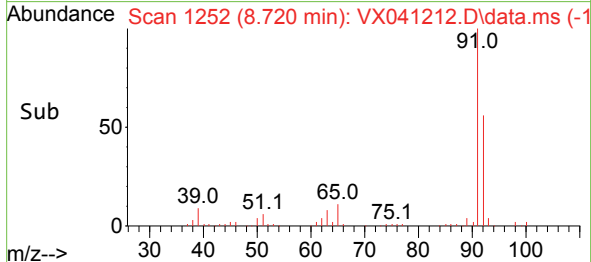

#53
t-1,3-Dichloropropene
Concen: 0.239 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. -0.250 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27


Tgt Ion: 75 Resp: 532
Ion Ratio Lower Upper
75 100
77 89.8 25.7 38.5#

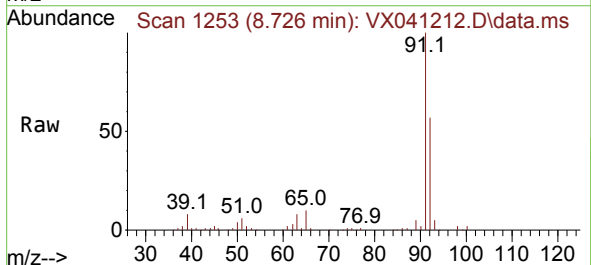






#60
Dibromochloromethane
Concen: 0.257 ug/l
RT: 9.525 min Scan# 1384
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:129 Resp: 502
Ion Ratio Lower Upper
129 100
127 79.1 38.8 116.4

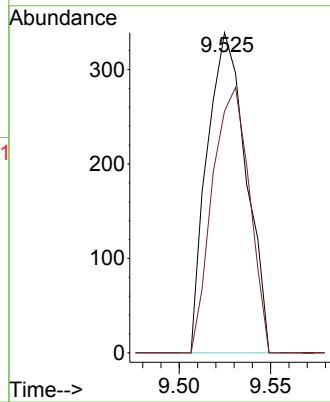

#62
4-Bromofluorobenzene
Concen: 54.075 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX041212.D
Acq: 23 Apr 2024 13:27

Tgt Ion: 95 Resp: 117436
Ion Ratio Lower Upper
95 100
174 99.9 0.0 135.6
176 97.6 0.0 131.0

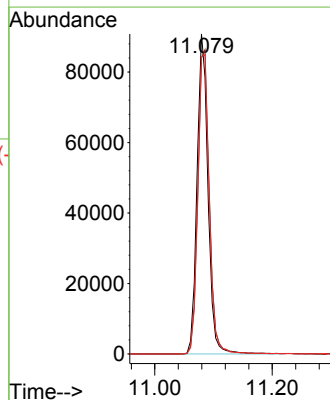



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:117 Resp: 217316

Ion Ratio Lower Upper

117 100

82 49.7 46.2 69.4

119 32.5 25.5 38.3

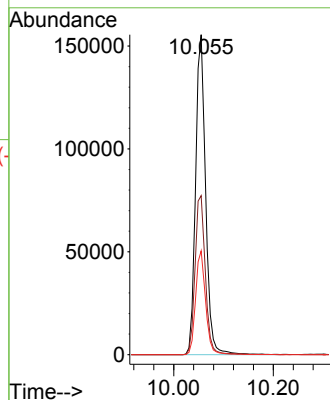

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27




Tgt Ion:152 Resp: 131174


Ion Ratio Lower Upper

152 100

115 52.6 43.3 129.9

150 154.6 0.0 345.0

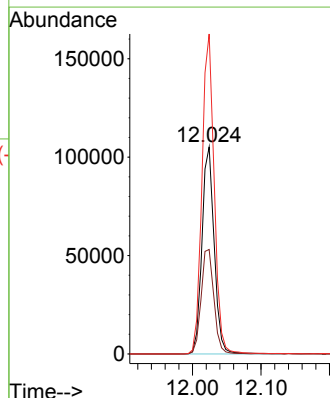



#76

1,2,3-Trichloropropane

Concen: 26.697 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 56422

Ion Ratio Lower Upper

75 100

77 0.9 19.1 57.5#



#81

trans-1,4-Dichloro-2-butene

Concen: 75.320 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX041212.D

Acq: 23 Apr 2024 13:27

Tgt Ion: 75 Resp: 56422

Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#

