

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042324\
 Data File : VX041210.D
 Acq On : 23 Apr 2024 12:41
 Operator : JC/MD
 Sample : P2207-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUR-1288

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
 Title : SW846 8260

Signal : TIC: VX041210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	33	rBV2	20820	35963	4.44%	0.708%
2	1.453	56	60	68	rBV	64542	96354	11.90%	1.897%
3	1.538	68	74	78	rVV	8099	17693	2.18%	0.348%
4	2.294	192	198	207	rBV	104689	200884	24.80%	3.956%
5	2.392	208	214	228	rVB2	32181	88937	10.98%	1.751%
6	2.940	297	304	314	rBV	7696	19345	2.39%	0.381%
7	4.239	509	517	526	rBV2	8990	27665	3.42%	0.545%
8	5.385	693	705	721	rBV2	96777	289153	35.70%	5.694%
9	5.550	721	732	750	rVV	169197	487855	60.24%	9.606%
10	5.952	789	798	820	rBV	98046	262665	32.43%	5.172%
11	6.757	921	930	946	rBV	247088	604916	74.69%	11.911%
12	6.891	946	952	959	rVB6	3029	8559	1.06%	0.169%
13	8.647	1232	1240	1250	rBV	505805	809904	100.00%	15.948%
14	9.000	1293	1298	1308	rBV	18338	29723	3.67%	0.585%
15	9.537	1378	1386	1401	rBV4	8244	24607	3.04%	0.485%
16	10.055	1465	1471	1489	rBV	524127	732413	90.43%	14.422%
17	11.079	1634	1639	1655	rBV	451396	592703	73.18%	11.671%
18	11.689	1735	1739	1748	rBV2	5709	8270	1.02%	0.163%
19	11.988	1783	1788	1789	rBV2	9981	11354	1.40%	0.224%
20	12.024	1789	1794	1806	rVB	546797	710003	87.67%	13.981%
21	12.219	1822	1826	1838	rBV2	10489	19509	2.41%	0.384%




Sum of corrected areas: 5078475

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042324\
Data File : VX041210.D
Acq On : 23 Apr 2024 12:41
Operator : JC/MD
Sample : P2207-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1288

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

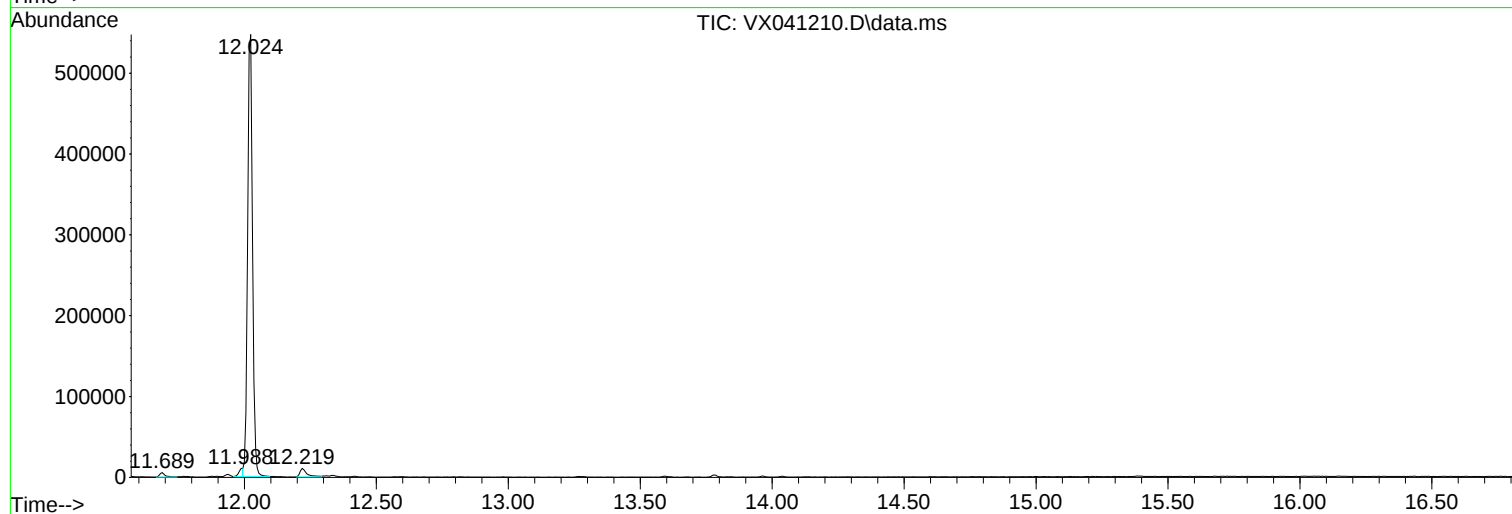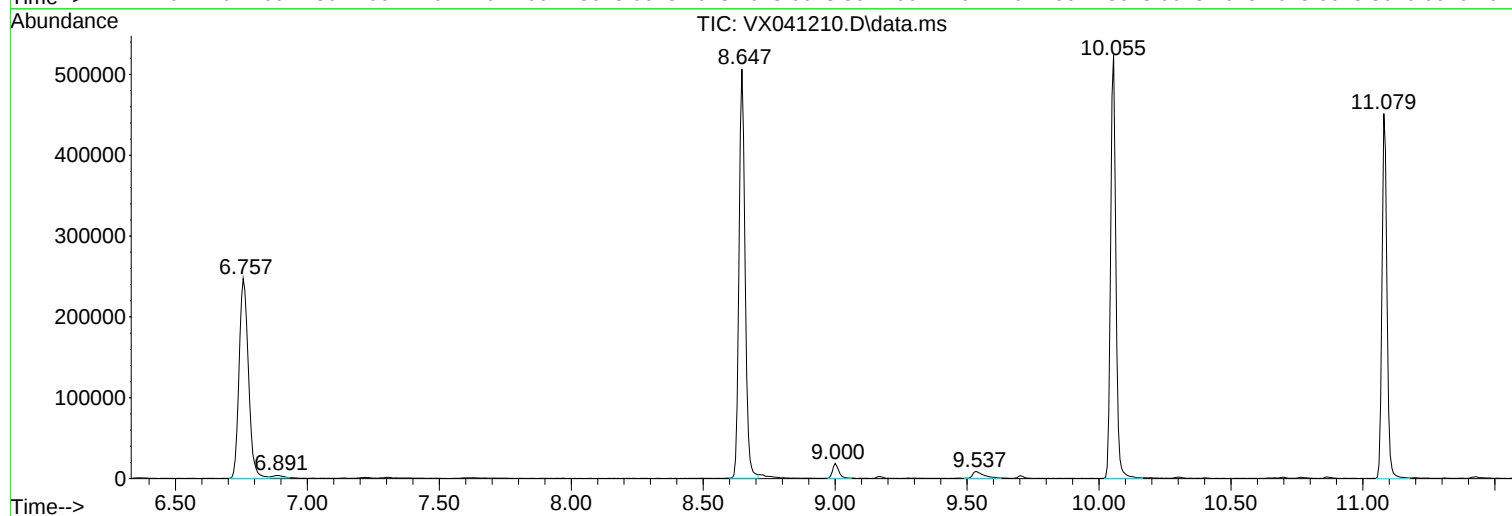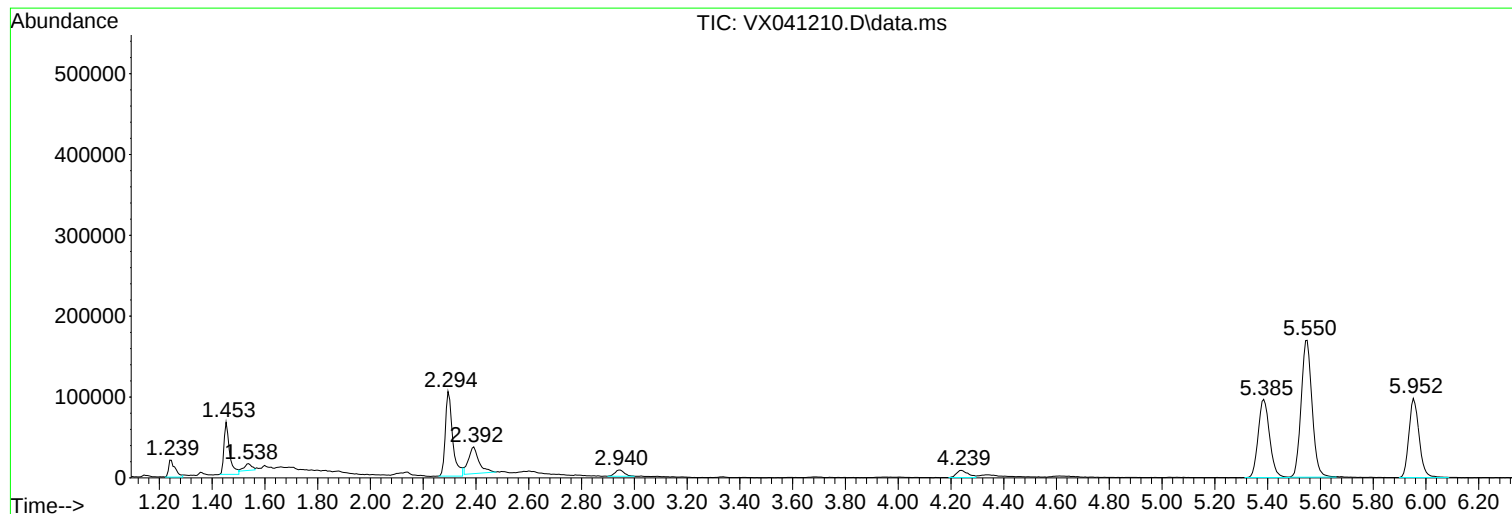

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042324\
Data File : VX041210.D
Acq On : 23 Apr 2024 12:41
Operator : JC/MD
Sample : P2207-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1288










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Propanal Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.294	20.59 ug/l	200884	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanal	58	C3H6O	000123-38-6	78
2			Trimethylene oxide	58	C3H6O	000503-30-0	9
3			Propylene oxide	58	C3H6O	000075-56-9	7
4			Oxirane, methyl-, (S)-	58	C3H6O	016088-62-3	7
5			Glyoxal	58	C2H2O2	000107-22-2	4

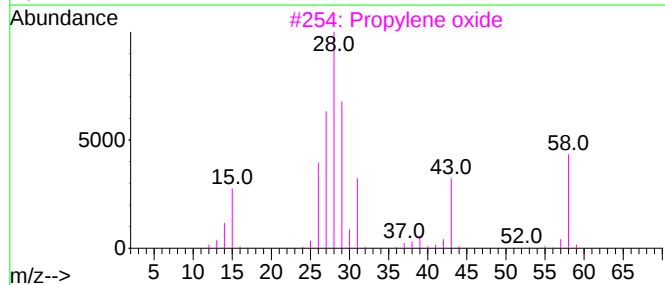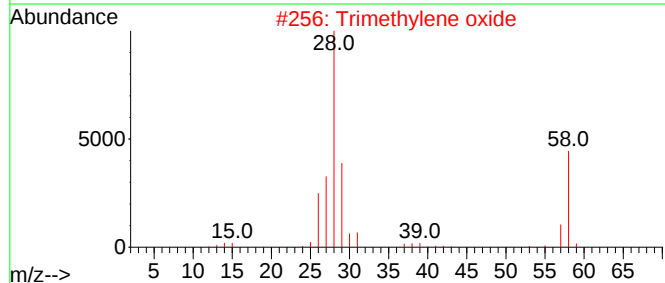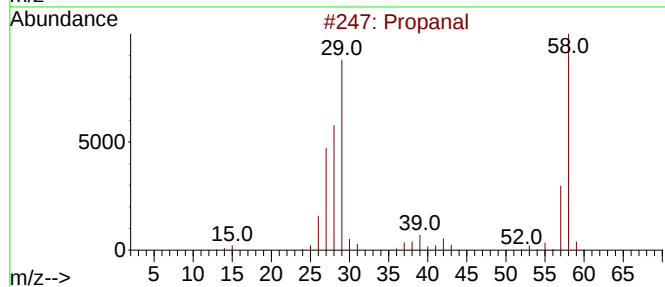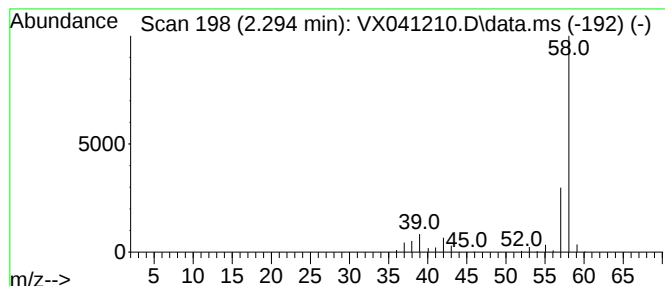

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042324\
Data File : VX041210.D
Acq On : 23 Apr 2024 12:41
Operator : JC/MD
Sample : P2207-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUR-1288

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propanal	2.294	20.6	ug/l	200884	1	5.550	487855	50.0