
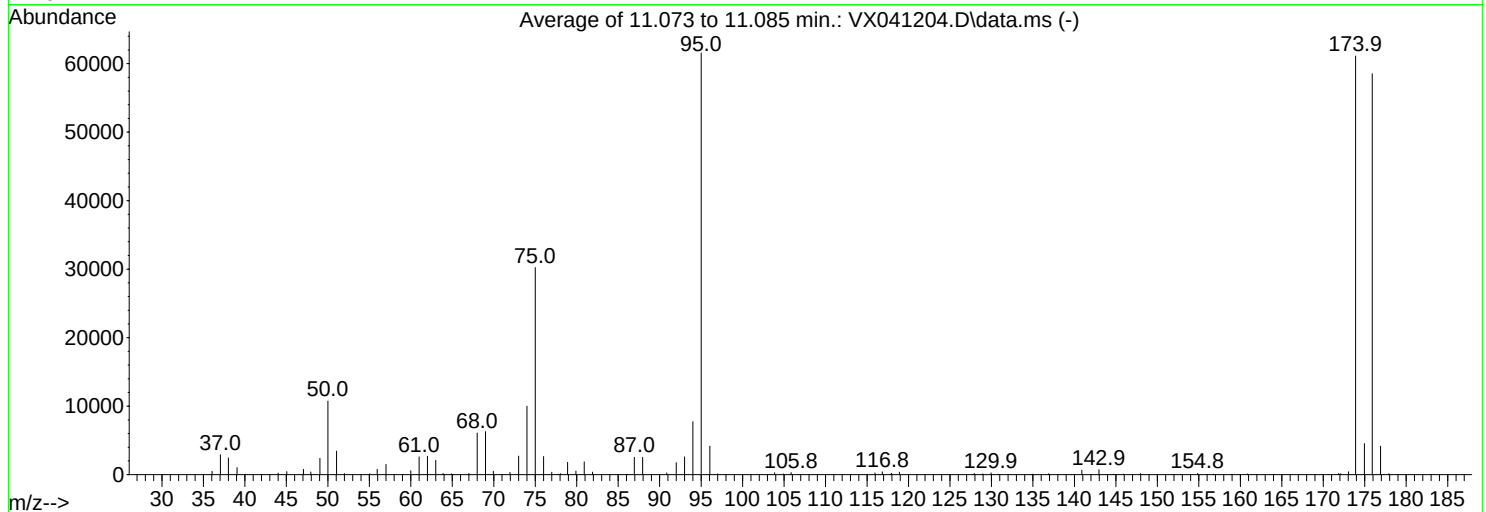


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042324\
Data File : VX041204.D
Acq On : 23 Apr 2024 08:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
Title : SW846 8260
Last Update : Tue Apr 23 05:30:28 2024

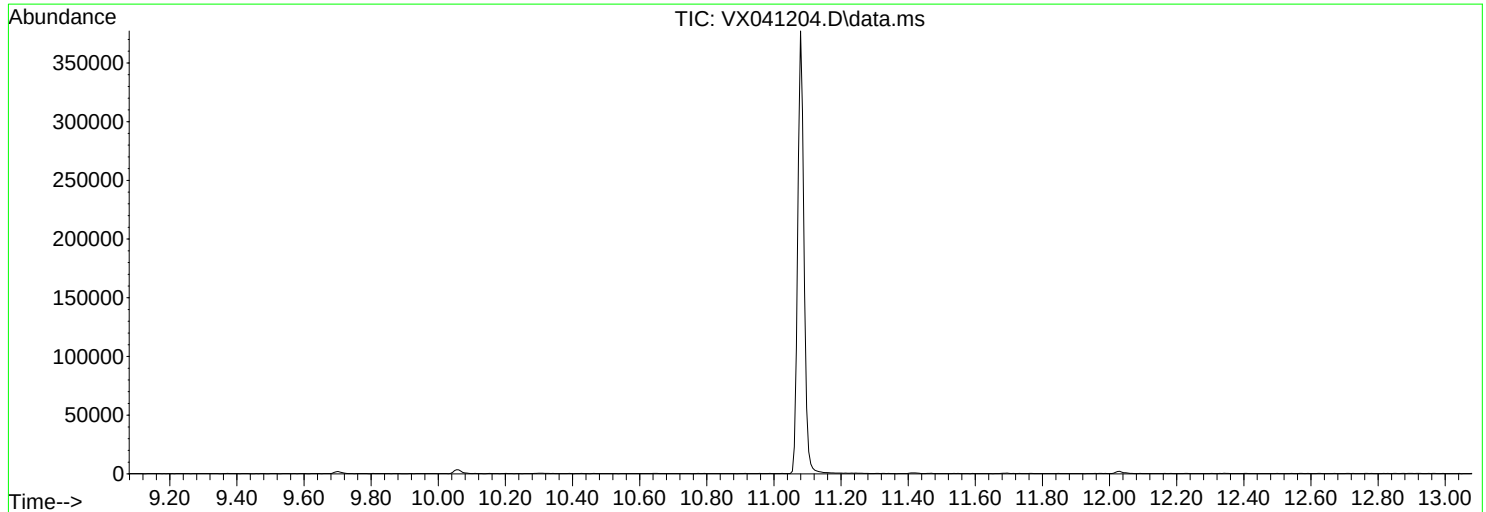

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	10738	PASS
75	95	30	60	49.1	30232	PASS
95	95	100	100	100.0	61576	PASS
96	95	5	9	6.8	4168	PASS
173	174	0.00	2	0.7	410	PASS
174	95	50	100	99.2	61104	PASS
175	174	5	9	7.4	4533	PASS
176	174	95	101	95.8	58541	PASS
177	176	5	9	7.1	4164	PASS