
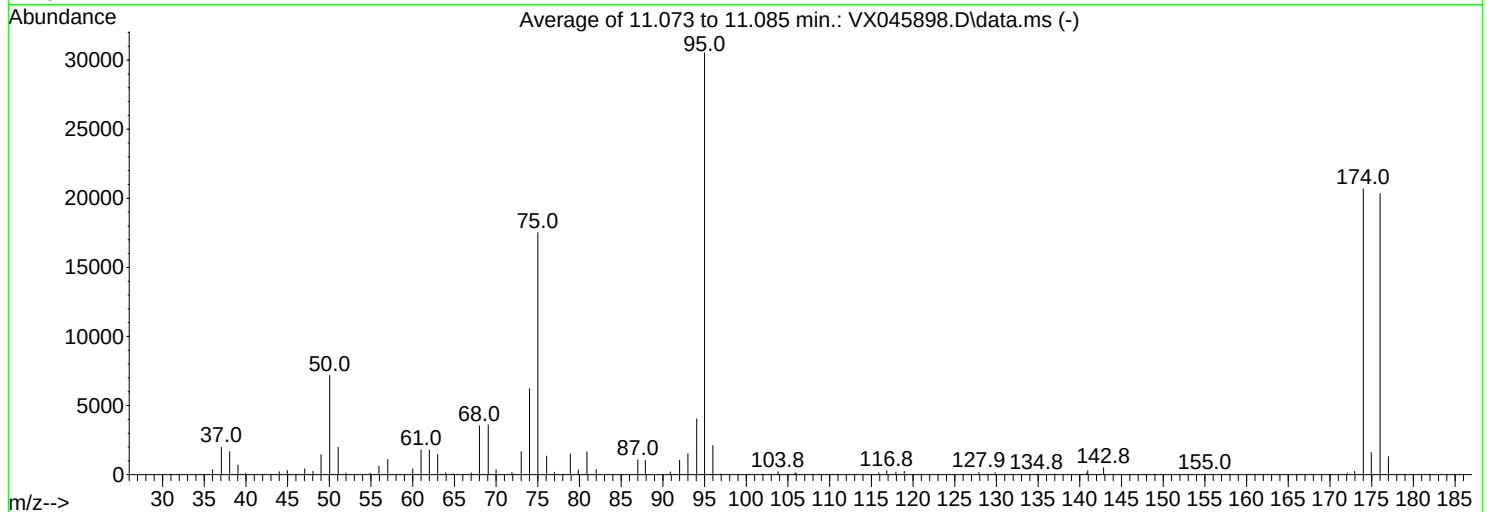


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042325\
Data File : VX045898.D
Acq On : 23 Apr 2025 08:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Title : SW846 8260
Last Update : Wed Apr 02 03:11:43 2025

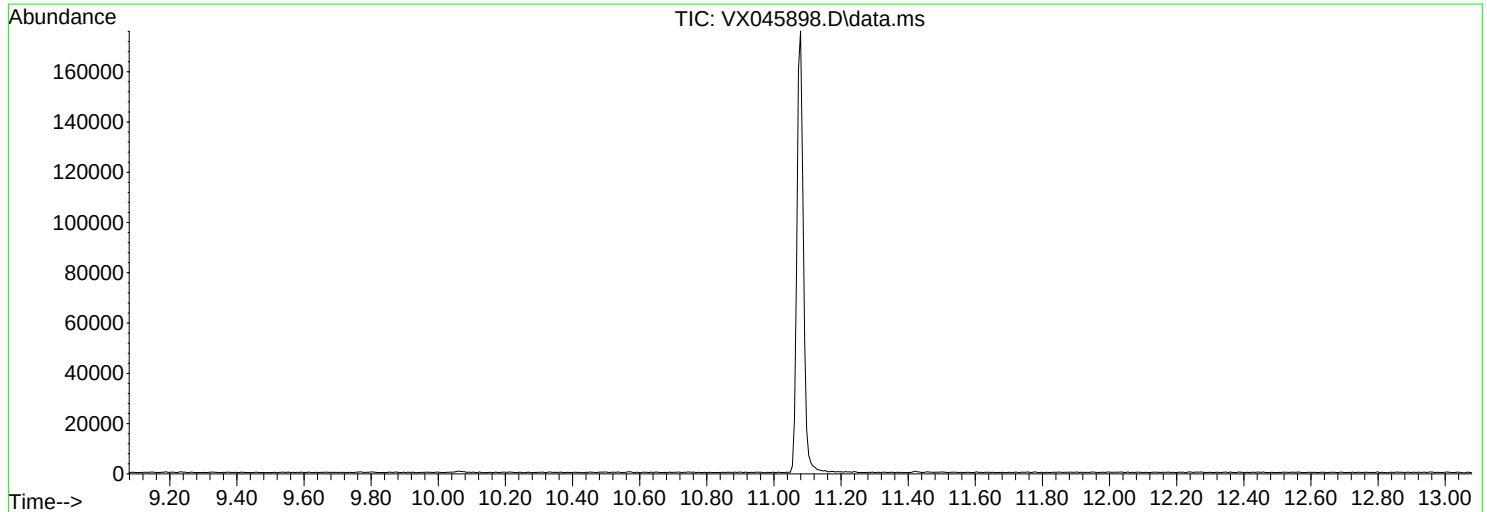

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.5	7175	PASS
75	95	30	60	57.4	17524	PASS
95	95	100	100	100.0	30525	PASS
96	95	5	9	6.9	2111	PASS
173	174	0.00	2	1.2	248	PASS
174	95	50	100	67.7	20680	PASS
175	174	5	9	7.7	1598	PASS
176	174	95	101	98.3	20333	PASS
177	176	5	9	6.4	1306	PASS