

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042419\
 Data File : VX009139.D
 Acq On : 24 Apr 2019 12:50
 Operator : JC/SP
 Sample : K2535-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S37-TB-2019-1

Quant Time: Apr 25 06:03:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 17 06:47:58 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	220996	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	360256	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	304200	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	122471	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	149184	47.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.80%	
35) Dibromofluoromethane	5.50	113	111013	48.02	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.04%	
50) Toluene-d8	8.71	98	443932	48.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.30%	
62) 4-Bromofluorobenzene	11.13	95	141340	43.42	ug/l	0.00
Spiked Amount 50.000			Recovery	=	86.84%	
Target Compounds						
16) Acetone	2.44	43	1882	1.165	ug/l	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042419\
Data File : VX009139.D
Acq On : 24 Apr 2019 12:50
Operator : JC/SP
Sample : K2535-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S37-TB-2019-1

Quant Time: Apr 25 06:03:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 17 06:47:58 2019
Response via : Initial Calibration

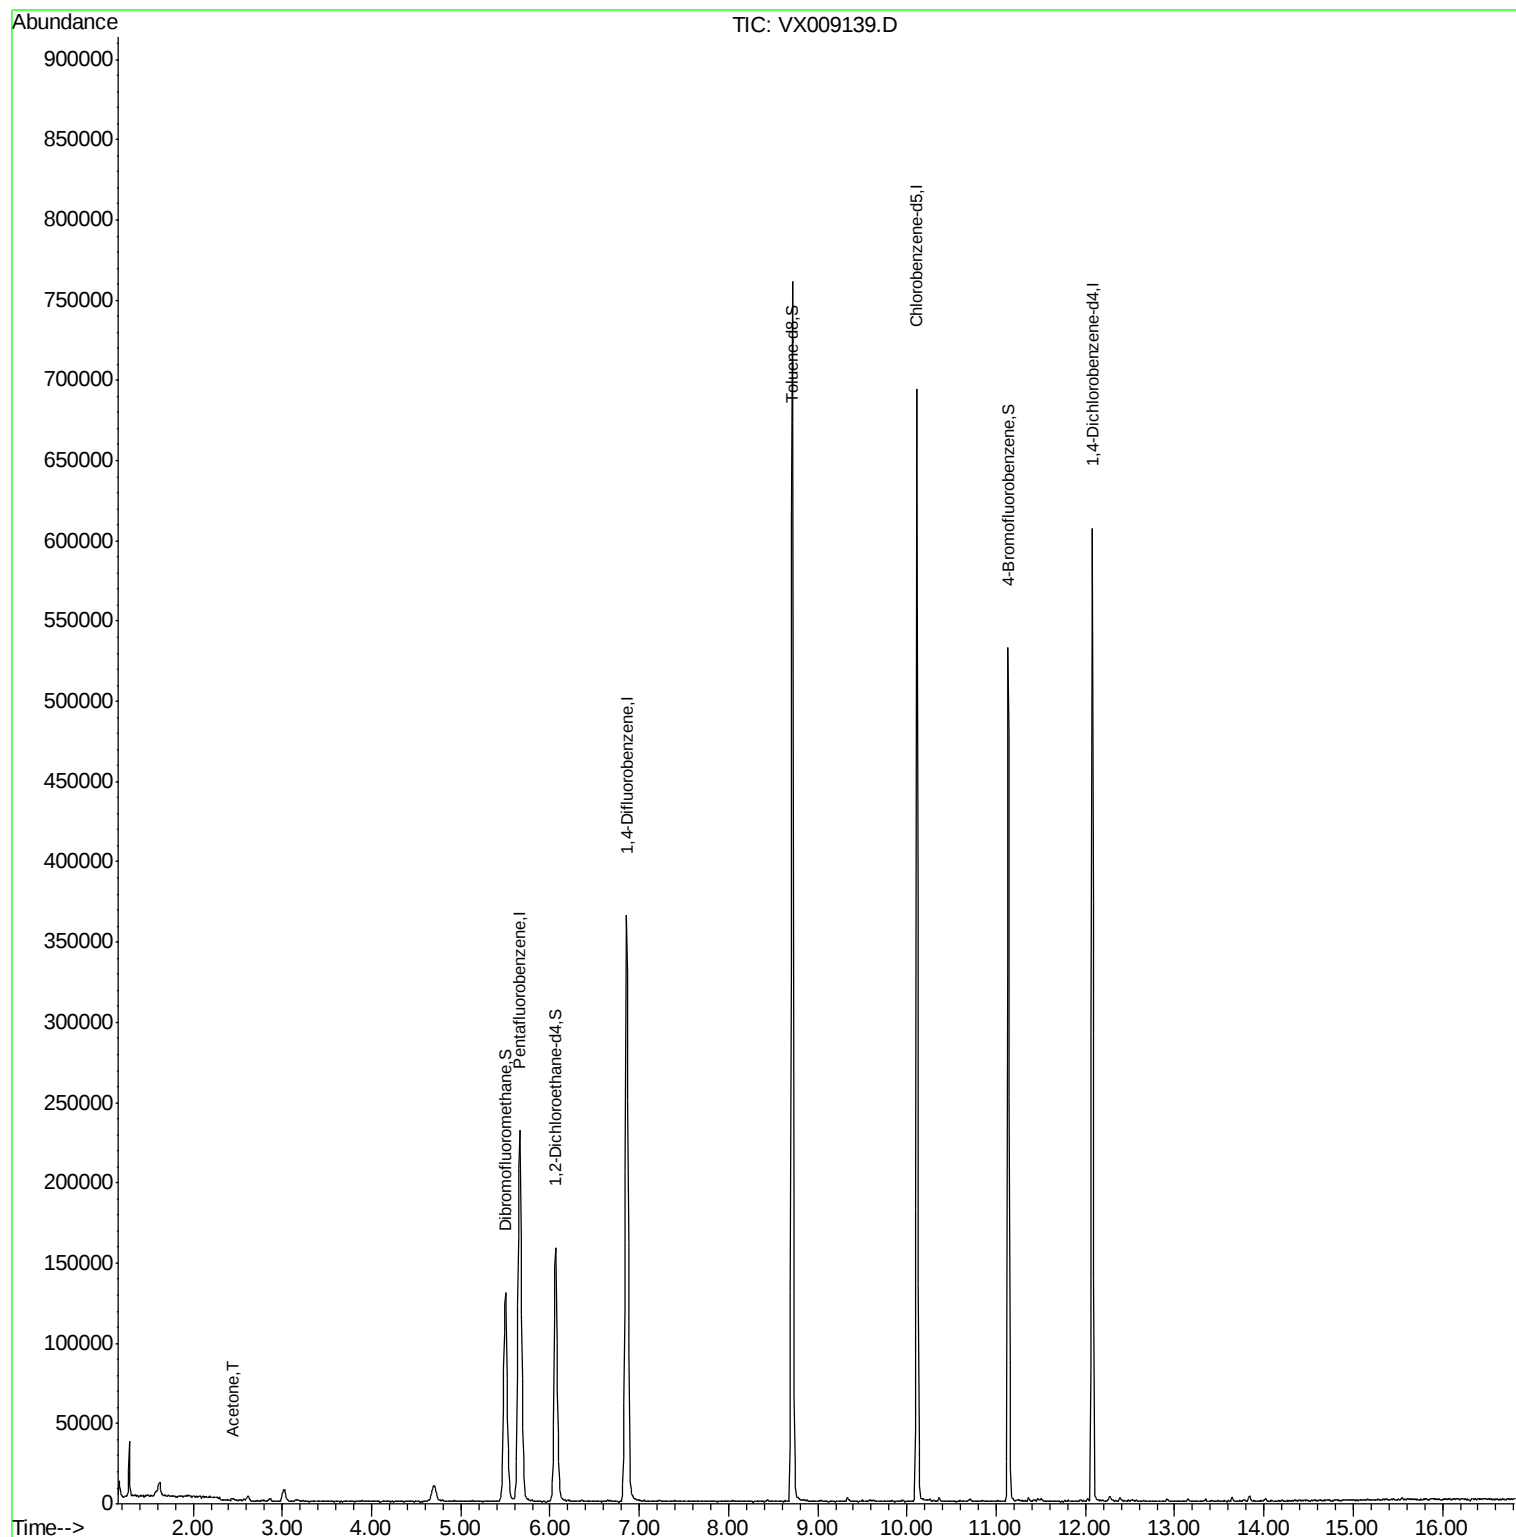

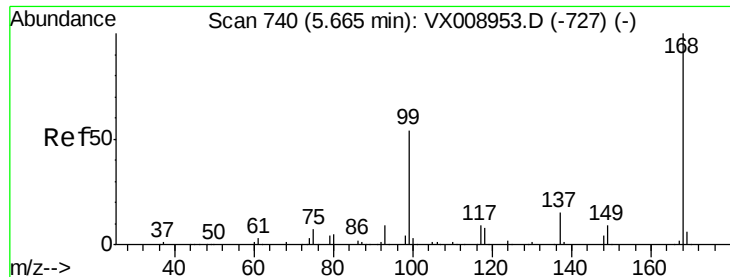

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.01 min

Lab File: VX009139.D

Acq: 24 Apr 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :


S37-TB-2019-1

Tot Ion:168 Resp: 220996

Ion Ratio Lower Upper




168 100

99 56.3 43.0 64.6

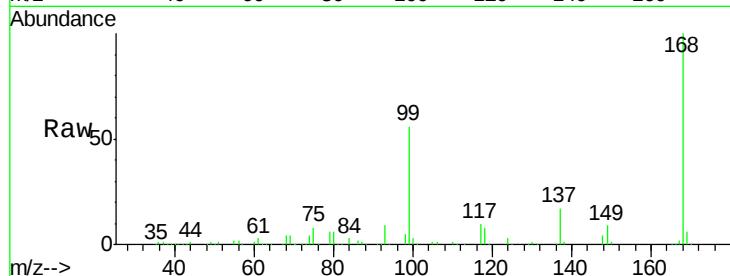

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

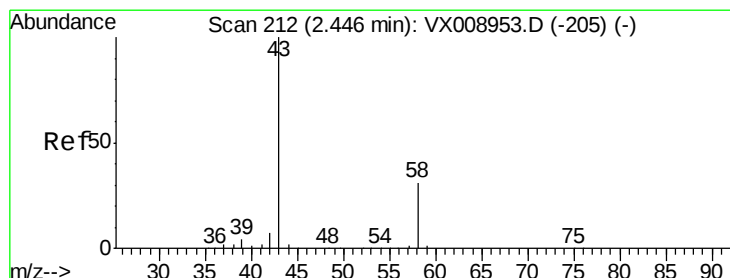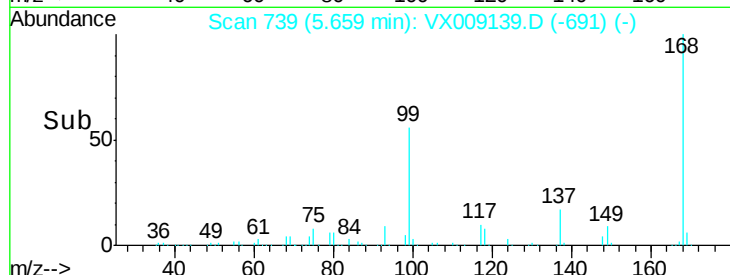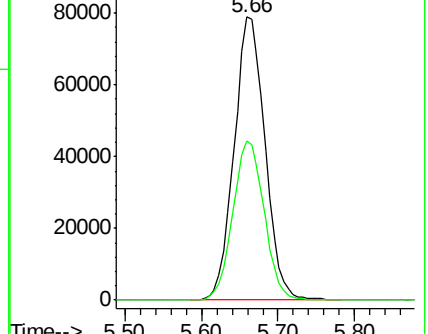

#16

Acetone

Concen: 1.165 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX009139.D


Acq: 24 Apr 2019 12:50

Tgt Ion: 43 Resp: 1882

Ion Ratio Lower Upper



43 100


58 30.6 24.8 37.2

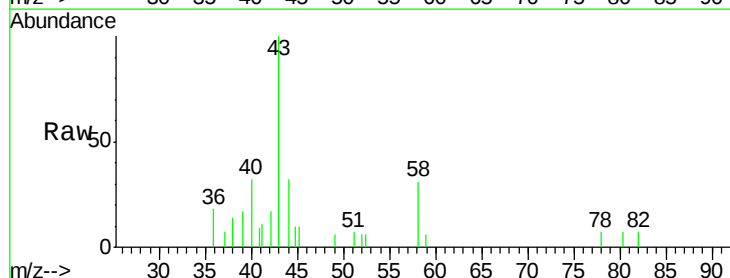

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

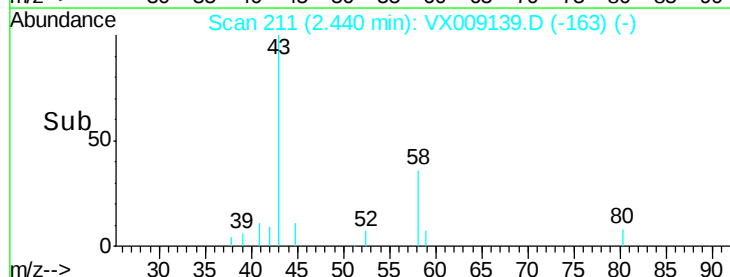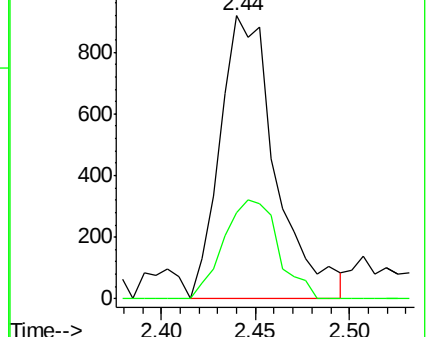

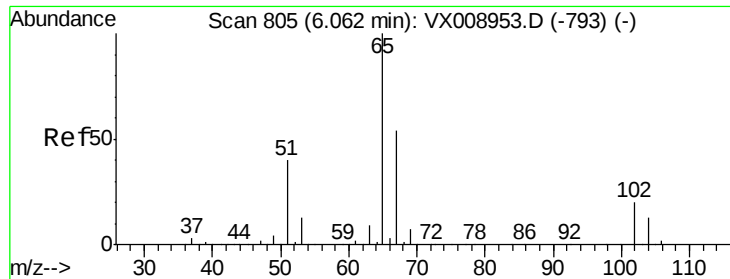

#33

1,2-Dichloroethane-d4

Concen: 47.900 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX009139.D

Acq: 24 Apr 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :


S37-TB-2019-1

Tot Ion: 65 Resp: 149184

Ion Ratio Lower Upper




65 100

67 54.0 0.0 108.6

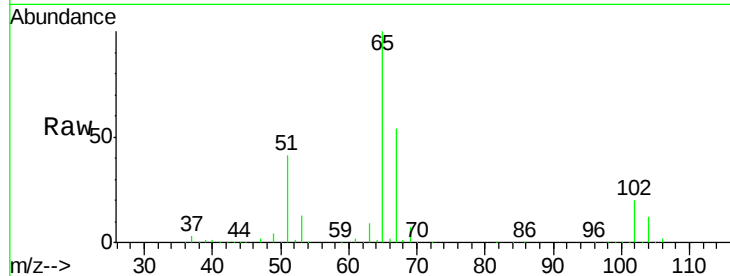

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

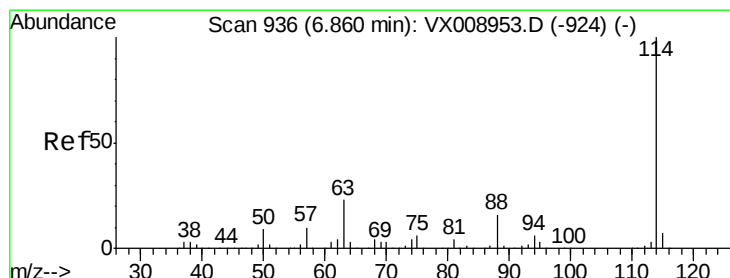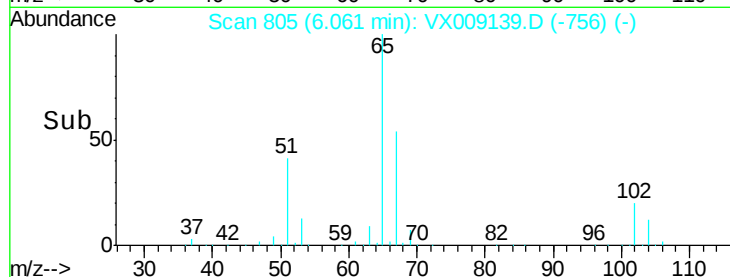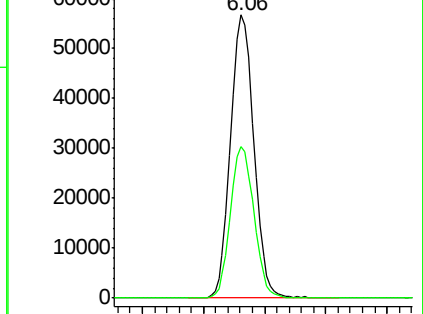

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX009139.D

Acq: 24 Apr 2019 12:50


Tgt Ion: 114 Resp: 360256

Ion Ratio Lower Upper

114 100

63 23.3 0.0 46.0



88 16.8 0.0 32.6

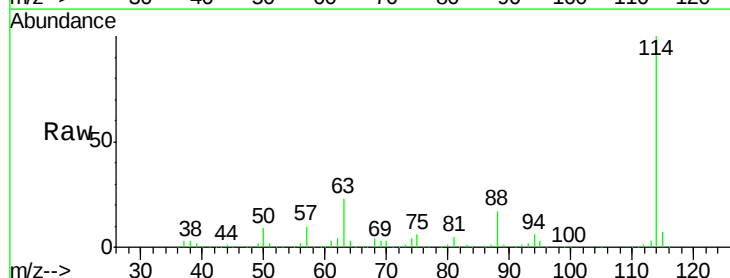


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

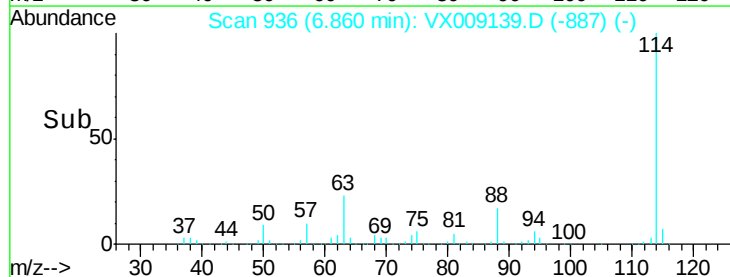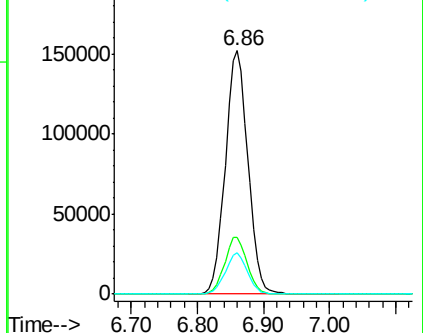

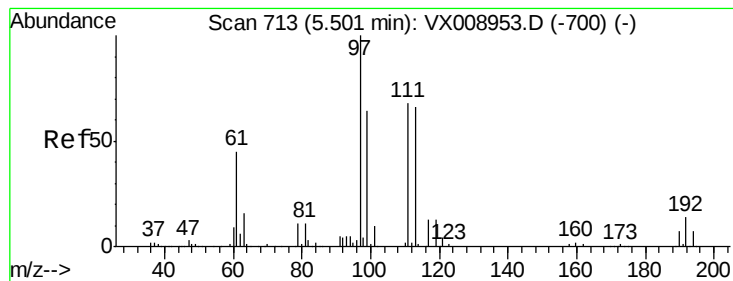

#35

Dibromofluoromethane

Concen: 48.015 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX009139.D

Acq: 24 Apr 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

S37-TB-2019-1


Tot Ion:113 Resp: 111013

Ion Ratio Lower Upper

113 100

111 102.8 82.9 124.3




192 20.9 17.4 26.0

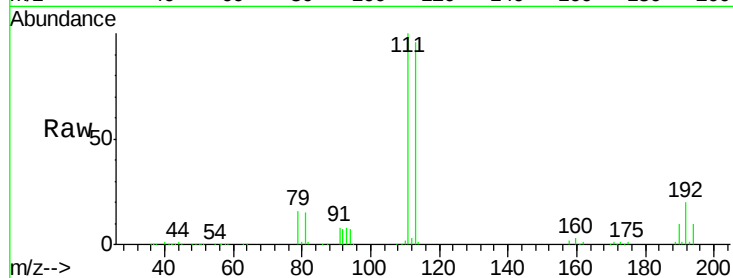

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

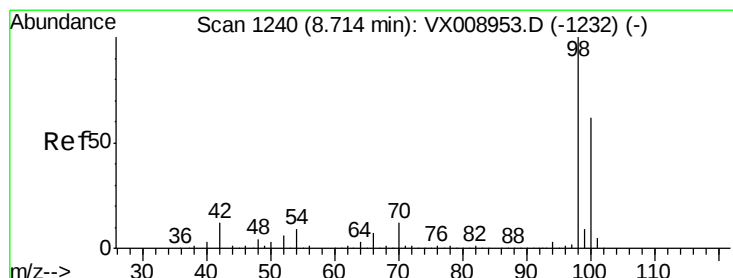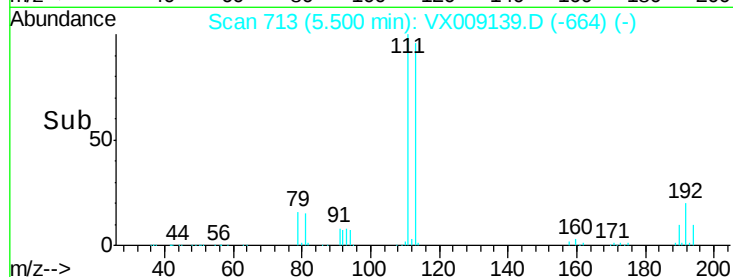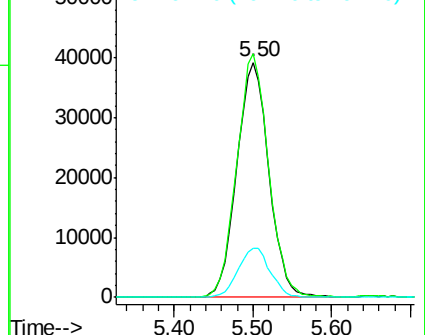

#50

Toluene-d8

Concen: 48.146 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX009139.D


Acq: 24 Apr 2019 12:50

Tgt Ion: 98 Resp: 443932

Ion Ratio Lower Upper



98 100


100 64.5 51.4 77.2

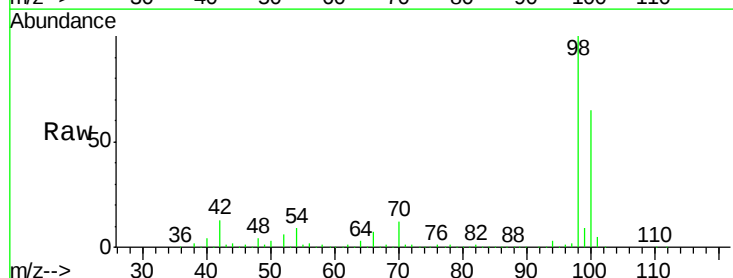

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

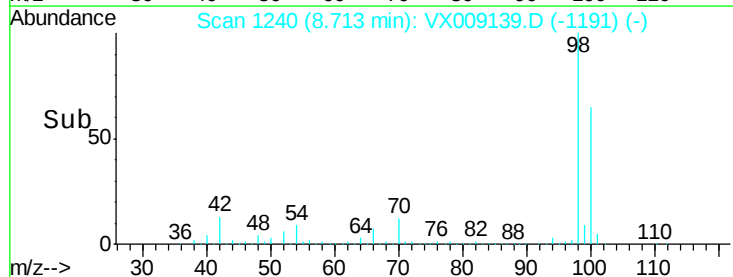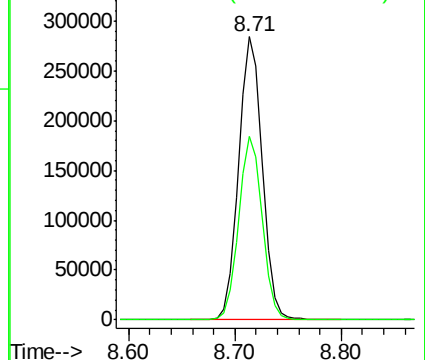

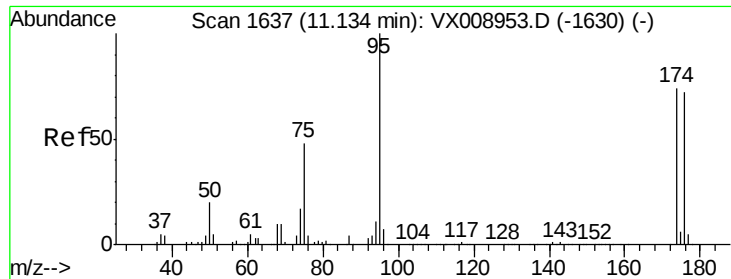

#62

4-Bromofluorobenzene

Concen: 43.424 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX009139.D

Acq: 24 Apr 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

S37-TB-2019-1


Tot Ion: 95 Resp: 141340

Ion Ratio Lower Upper

95 100

174 79.7 0.0 159.6




176 76.8 0.0 154.8

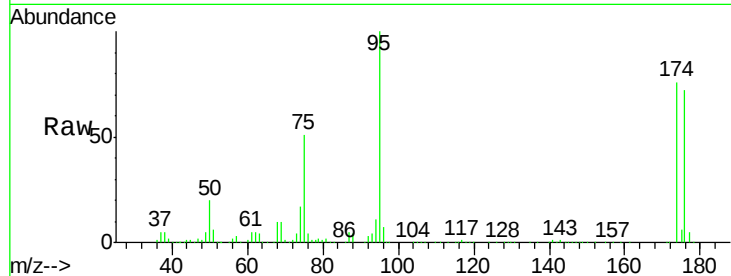

Abundance Ion 94.90 (94.60 to 95.60): VX008953.D (-1630) (-)

Ion 173.80 (173.50 to 174.50): VX008953.D (-1630) (-)

Ion 175.80 (175.50 to 176.50): VX008953.D (-1630) (-)

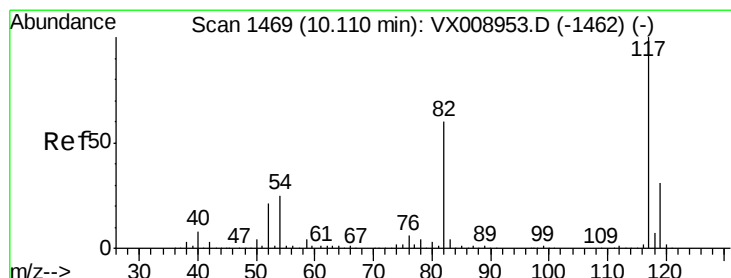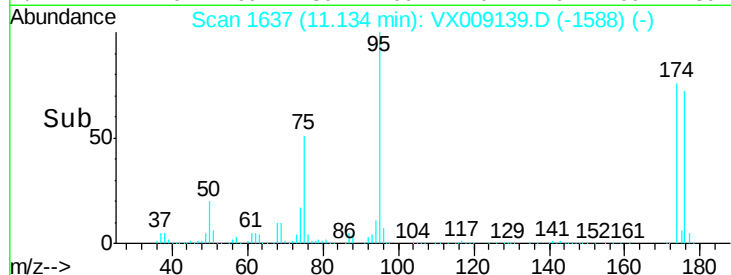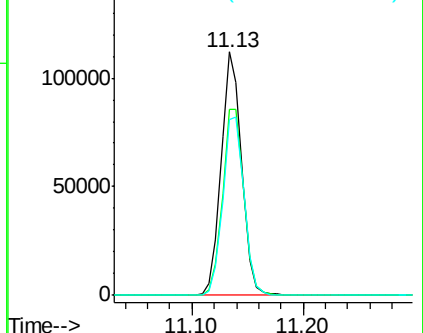

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX009139.D

Acq: 24 Apr 2019 12:50


Tgt Ion: 117 Resp: 304200

Ion Ratio Lower Upper

117 100

82 60.2 48.2 72.4



119 32.1 25.0 37.6

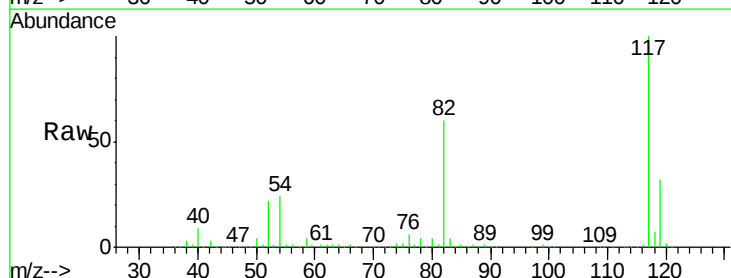


Abundance Ion 116.90 (116.60 to 117.60): VX008953.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX008953.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX008953.D (-1462) (-)

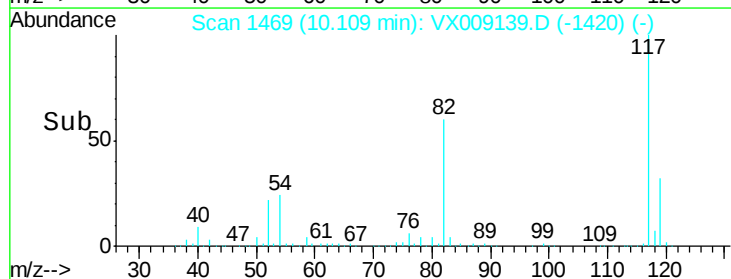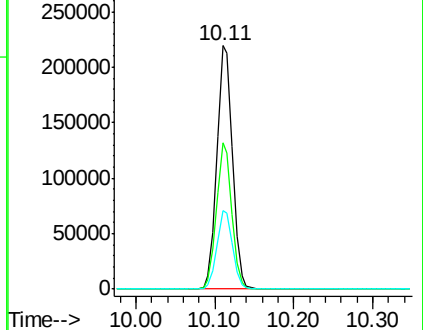

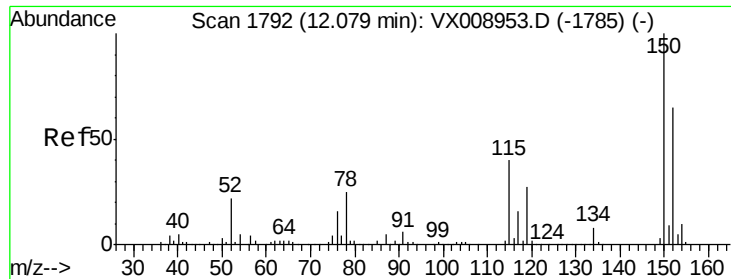

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX009139.D


Acq: 24 Apr 2019 12:50

Instrument :

MSVOA_X

ClientSampleId :

S37-TB-2019-1

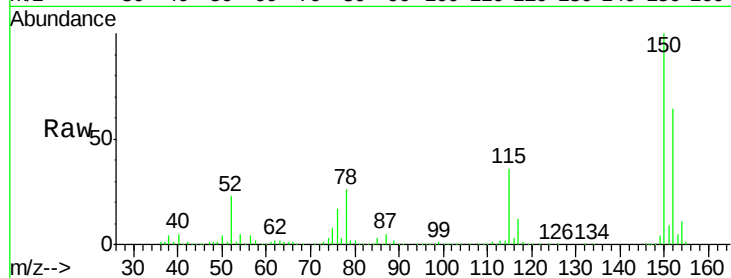


Tot Ion:152 Resp: 122471

Ion Ratio Lower Upper

152 100

115 58.8 41.4 124.2

150 157.3 0.0 349.8

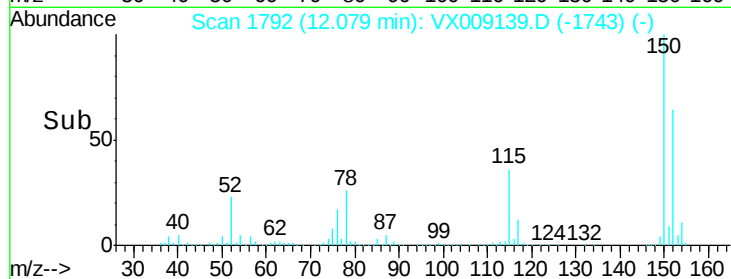

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

