

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042420\  
 Data File : VX015949.D  
 Acq On : 24 Apr 2020 22:23  
 Operator : JC/SP  
 Sample : L2415-03  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SS042MW127-200423

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X042420W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.575       | 236           | 244         | 251          | rBV2     | 11281          | 23376         | 2.92%           | 0.540%        |
| 2         | 5.470       | 706           | 719         | 731          | rBV      | 79881          | 226862        | 28.33%          | 5.244%        |
| 3         | 5.635       | 735           | 746         | 759          | rVV      | 141629         | 395382        | 49.37%          | 9.139%        |
| 4         | 6.037       | 801           | 812         | 826          | rBV      | 95985          | 252628        | 31.55%          | 5.840%        |
| 5         | 6.836       | 931           | 943         | 956          | rBV      | 237568         | 561147        | 70.07%          | 12.971%       |
| 6         | 7.196       | 991           | 1002        | 1009         | rBV7     | 4039           | 10359         | 1.29%           | 0.239%        |
| 7         | 8.695       | 1240          | 1248        | 1264         | rBV      | 508150         | 800816        | 100.00%         | 18.511%       |
| 8         | 9.317       | 1344          | 1350        | 1359         | rVB      | 46911          | 70617         | 8.82%           | 1.632%        |
| 9         | 10.098      | 1472          | 1478        | 1497         | rVB      | 538858         | 713976        | 89.16%          | 16.504%       |
| 10        | 11.122      | 1641          | 1646        | 1657         | rBV      | 437491         | 553016        | 69.06%          | 12.783%       |
| 11        | 12.061      | 1795          | 1800        | 1811         | rBV      | 565760         | 717967        | 89.65%          | 16.596%       |


Sum of corrected areas: 4326146

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042420\  
Data File : VX015949.D  
Acq On : 24 Apr 2020 22:23  
Operator : JC/SP  
Sample : L2415-03  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS042MW127-200423

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X042420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

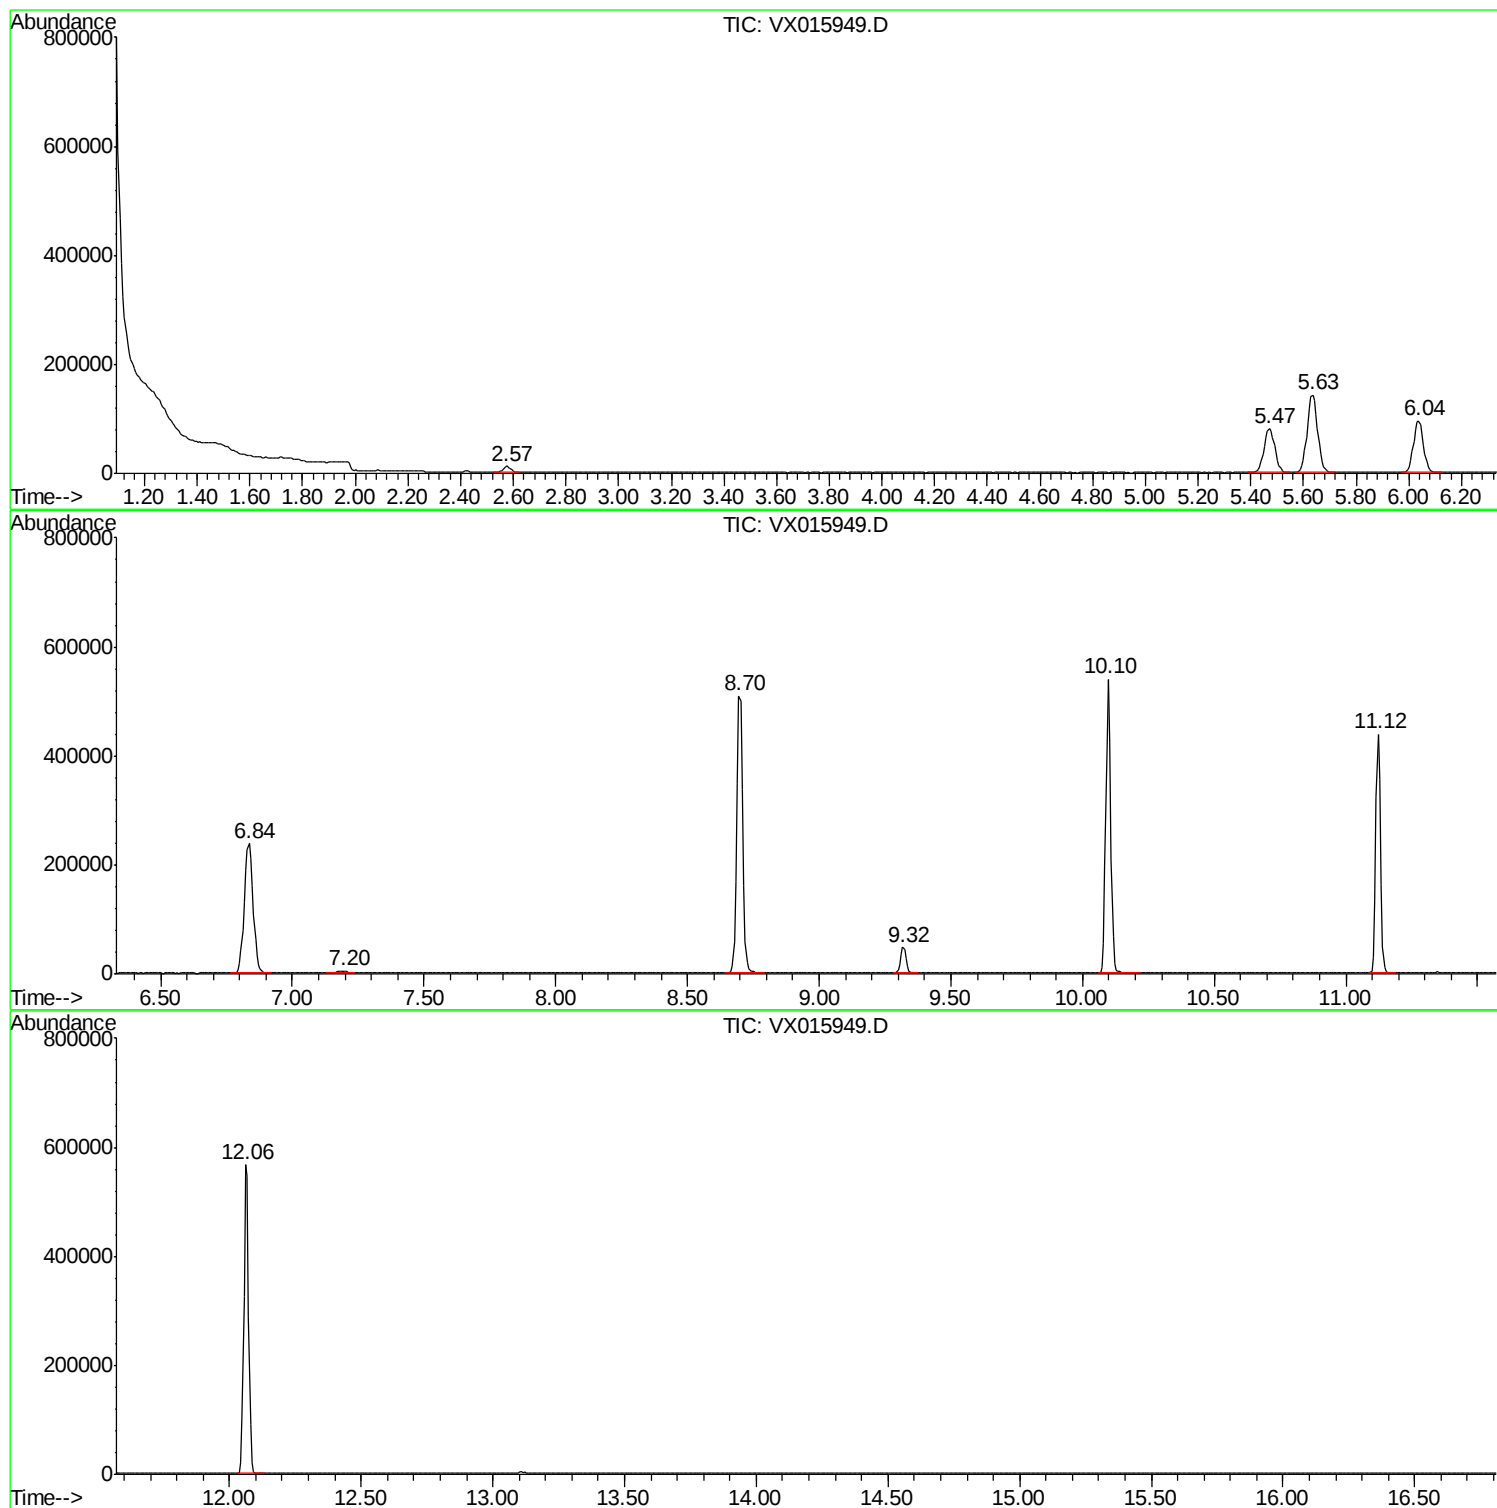

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX042420\  
Data File : VX015949.D  
Acq On : 24 Apr 2020 22:23  
Operator : JC/SP  
Sample : L2415-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS042MW127-200423

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X042420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX042420\  
Data File : VX015949.D  
Acq On : 24 Apr 2020 22:23  
Operator : JC/SP  
Sample : L2415-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS042MW127-200423

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X042420W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |