

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042425\
 Data File : VX045929.D
 Acq On : 24 Apr 2025 15:56
 Operator : JC/MD
 Sample : Q1855-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 2001

Quant Time: Apr 25 02:27:57 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	63160	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	126878	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	117802	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	46552	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	63584	55.050	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 110.100%			
35) Dibromofluoromethane	5.379	113	46325	51.461	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 102.920%			
50) Toluene-d8	8.647	98	160661	51.132	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 102.260%			
62) 4-Bromofluorobenzene	11.079	95	57296	50.062	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 100.120%			
Target Compounds						Qvalue
11) Tert butyl alcohol	2.965	59	922	5.940	ug/l #	72
13) Acrolein	2.233	56	153	0.716	ug/l #	76
16) Acetone	2.380	43	24662	51.998	ug/l	96
18) Methyl Acetate	2.709	43	2501	2.290	ug/l #	89
20) Methylene Chloride	2.788	84	5283	5.950	ug/l	98
25) 2-Butanone	4.586	43	2737	3.942	ug/l	94
29) Tetrahydrofuran	5.025	42	154	0.342	ug/l #	35
31) Cyclohexane	5.544	56	1985	1.401	ug/l #	42
36) 1,1-Dichloropropene	5.550	75	6434	5.294	ug/l #	51
38) Carbon Tetrachloride	5.544	117	7728	5.883	ug/l #	15
40) Benzene	6.037	78	7331	1.975	ug/l	98
43) Isopropyl Acetate	6.342	43	13429	5.785	ug/l	98
48) Methyl methacrylate	7.793	41	49890	41.622	ug/l #	51
51) 4-Methyl-2-Pentanone	8.549	43	40655	26.417	ug/l #	53
52) Toluene	8.720	92	5226	2.327	ug/l	97
53) t-1,3-Dichloropropene	8.958	75	148	2.393	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	14762	11.063	ug/l #	67
57) 1,3-Dichloropropane	9.482	76	1561	1.002	ug/l #	42
59) 2-Hexanone	9.378	43	13114	11.507	ug/l #	28
67) Ethyl Benzene	10.195	91	1119	0.248	ug/l	92
68) m/p-Xylenes	10.305	106	1766	1.077	ug/l	99
69) o-Xylene	10.640	106	1273	0.788	ug/l	90
74) N-amyl acetate	10.774	43	1840	1.032	ug/l #	51
76) 1,2,3-Trichloropropane	11.079	75	32986	29.049	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.457	105	745	0.242	ug/l	81
81) trans-1,4-Dichloro-2-b...	11.079	75	32986	98.590	ug/l #	1
84) 1,2,4-Trimethylbenzene	11.756	105	2146	0.693	ug/l	71
85) sec-Butylbenzene	11.756	105	2146	0.572	ug/l #	58
90) Hexachloroethane	12.414	117	436	0.821	ug/l #	19
95) Naphthalene	13.774	128	65242	20.200	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042425\
Data File : VX045929.D
Acq On : 24 Apr 2025 15:56
Operator : JC/MD
Sample : Q1855-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
2001

Quant Time: Apr 25 02:27:57 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




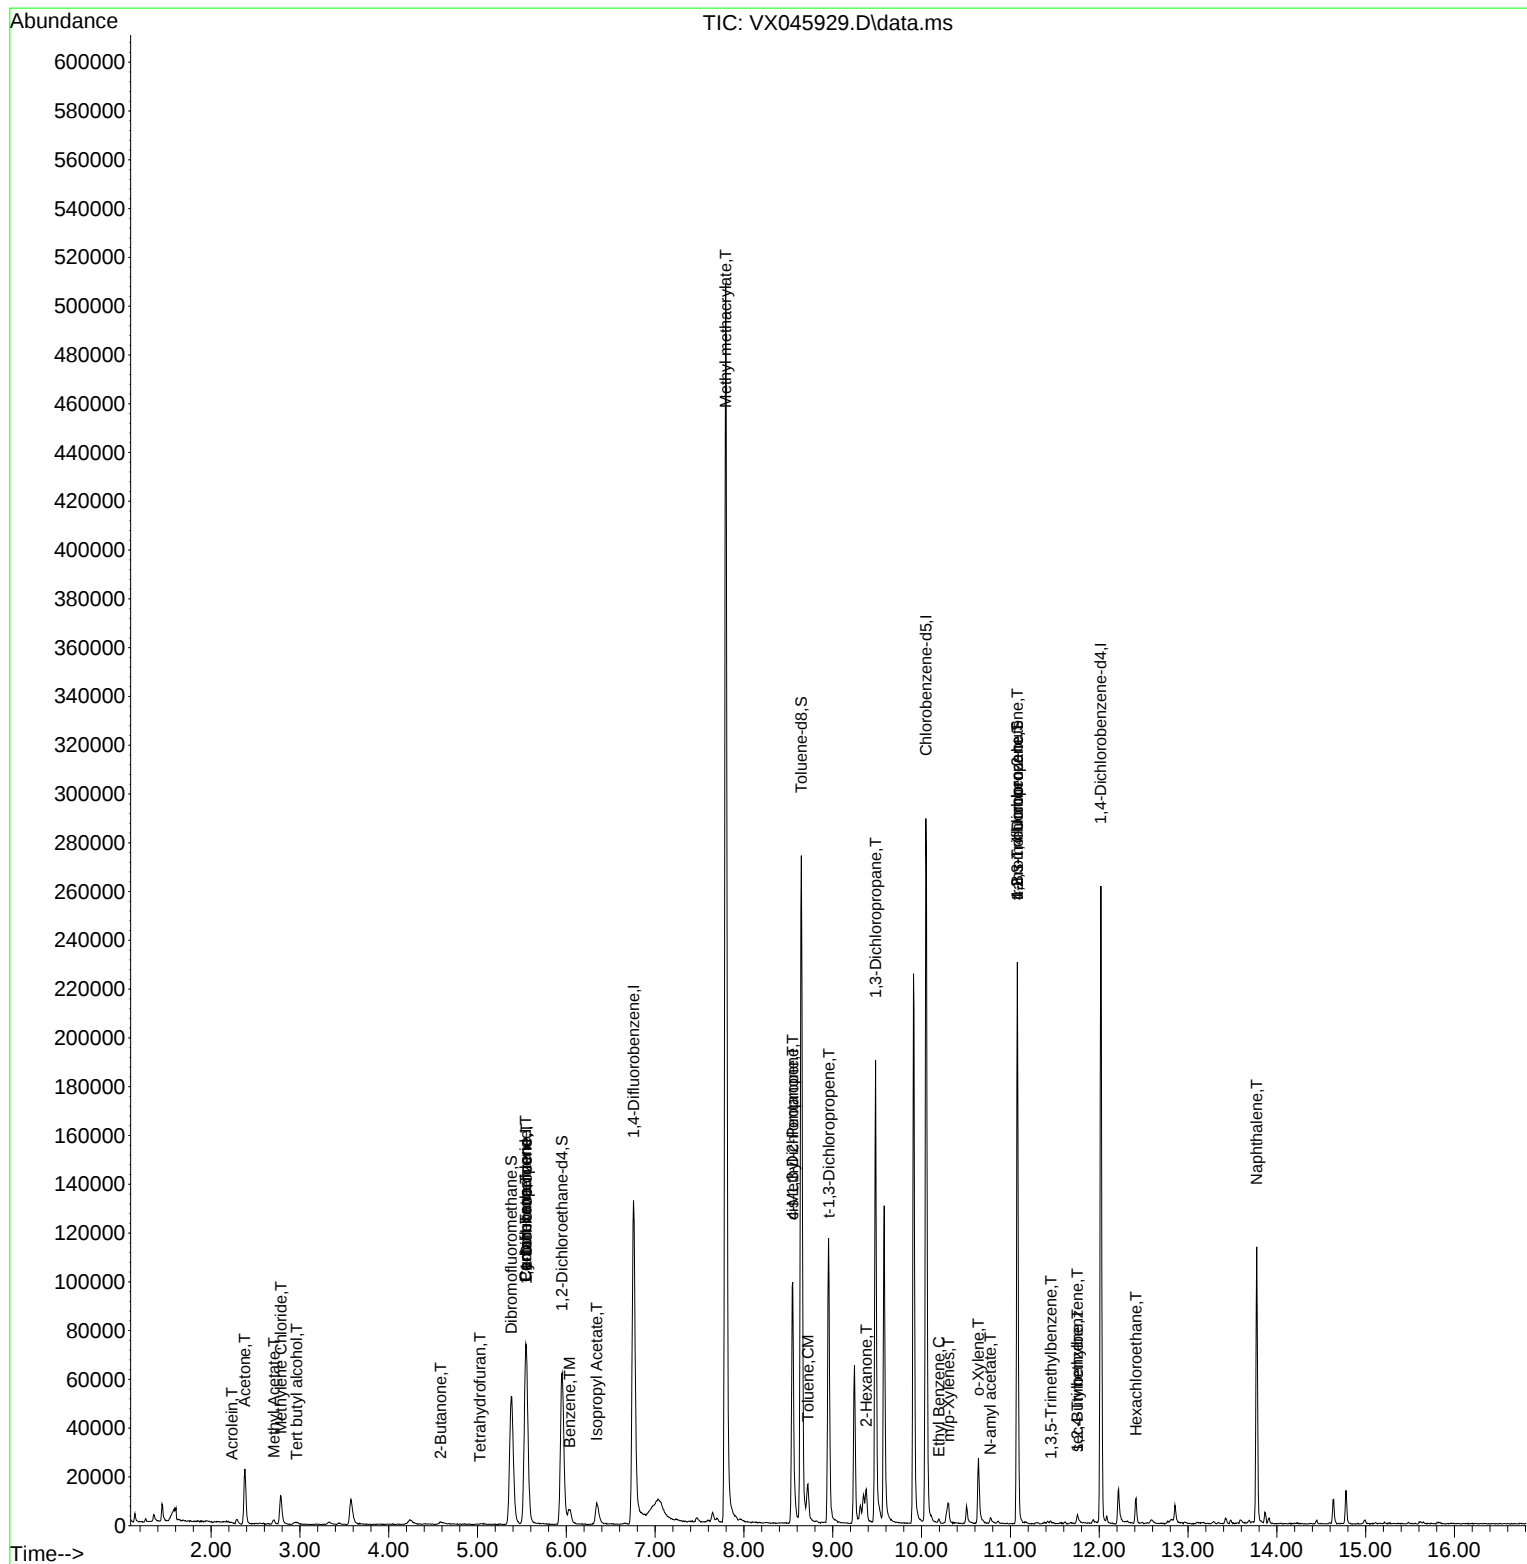




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion:168 Resp: 63160
Ion Ratio Lower Upper
168 100
99 74.8 52.3 78.5



#11
Tert butyl alcohol
Concen: 5.940 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.012 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 59 Resp: 922
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#




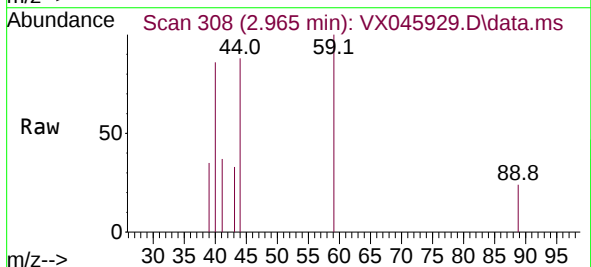




#13
Acrolein
Concen: 0.716 ug/l
RT: 2.233 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion: 56 Resp: 153
Ion Ratio Lower Upper
56 100
55 50.3 56.2 84.2#

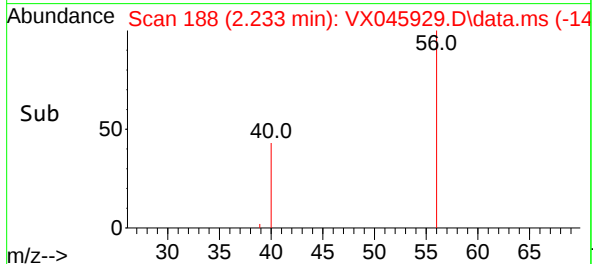

#16
Acetone
Concen: 51.998 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 43 Resp: 24662
Ion Ratio Lower Upper
43 100
58 30.2 22.3 33.5


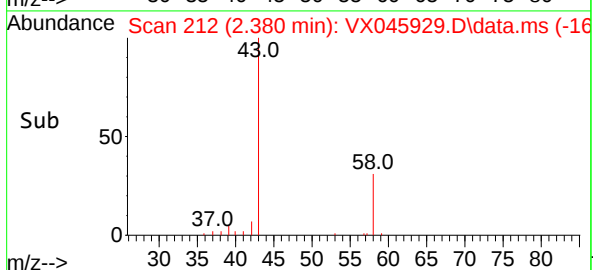






#18
Methyl Acetate
Concen: 2.290 ug/l
RT: 2.709 min Scan# 201
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion: 43 Resp: 2501
Ion Ratio Lower Upper
43 100
74 16.8 17.5 26.3#

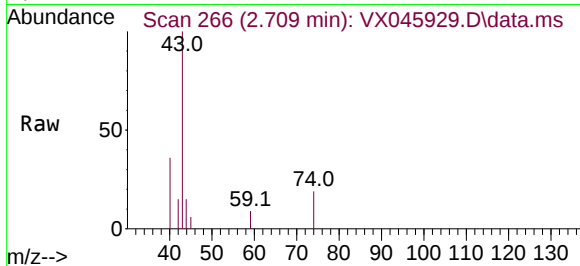

#20
Methylene Chloride
Concen: 5.950 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 84 Resp: 5283
Ion Ratio Lower Upper
84 100
49 137.2 107.5 161.3
51 39.5 33.0 49.6
86 63.4 50.1 75.1

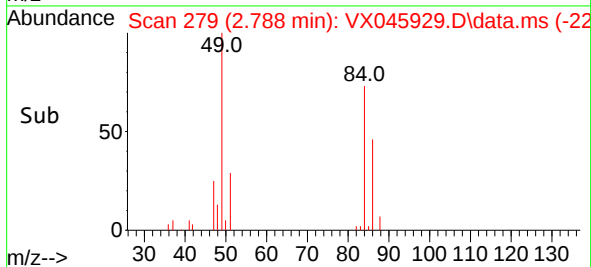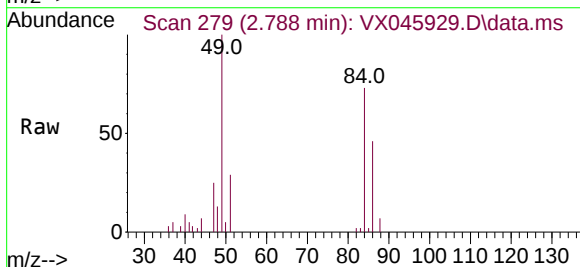



#25

2-Butanone

Concen: 3.942 ug/l

RT: 4.586 min Scan# 51

Delta R.T. 0.030 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Instrument :

MSVOA_X

ClientSampleId :





2001

Tgt Ion: 43 Resp: 2737

Ion Ratio Lower Upper

43 100

72 26.1 18.6 28.0

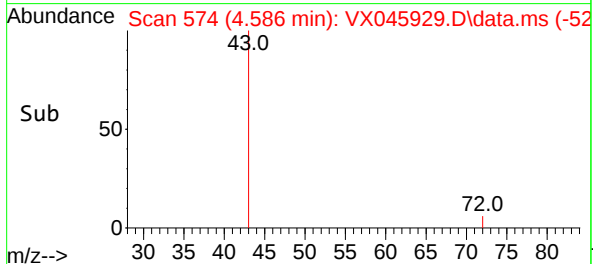

#29

Tetrahydrofuran

Concen: 0.342 ug/l

RT: 5.025 min Scan# 646

Delta R.T. 0.024 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56




Tgt Ion: 42 Resp: 154


Ion Ratio Lower Upper

42 100

72 0.0 33.4 50.0#

71 0.0 31.4 47.0#


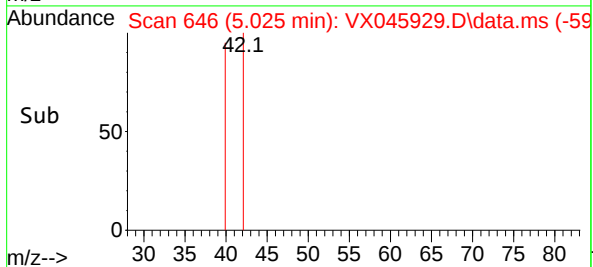

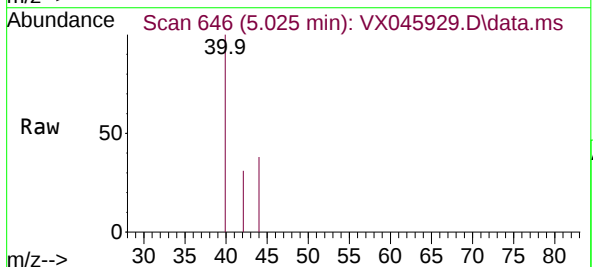




#31
Cyclohexane
Concen: 1.401 ug/l
RT: 5.544 min Scan# 718
Delta R.T. 0.079 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion: 56 Resp: 1985
Ion Ratio Lower Upper
56 100
69 148.4 23.6 35.4#
84 83.7 67.7 101.5

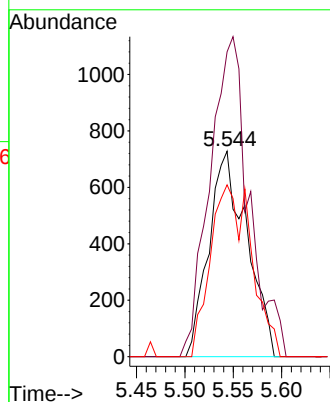

#33
1,2-Dichloroethane-d4
Concen: 55.050 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 65 Resp: 63584
Ion Ratio Lower Upper
65 100
67 50.0 0.0 99.0

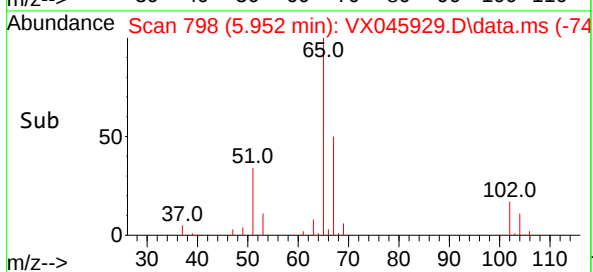
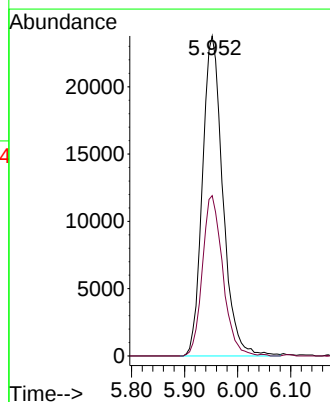
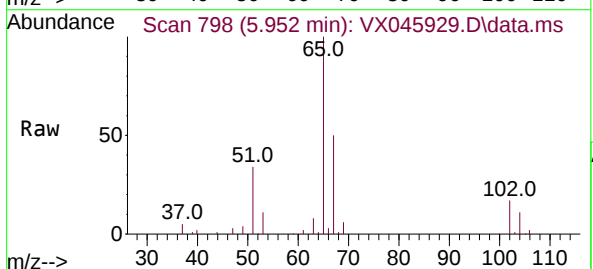




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion:114 Resp: 126878
Ion Ratio Lower Upper
114 100
63 24.2 0.0 46.8
88 17.6 0.0 35.4

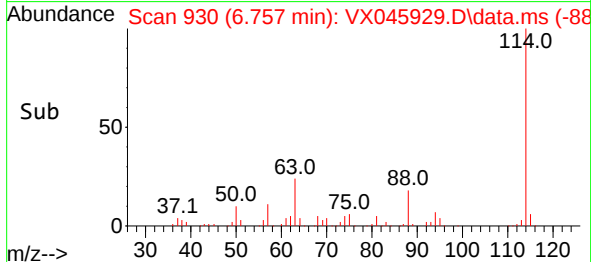

#35
Dibromofluoromethane
Concen: 51.461 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion:113 Resp: 46325
Ion Ratio Lower Upper
113 100
111 101.5 81.8 122.6
192 16.4 13.8 20.6

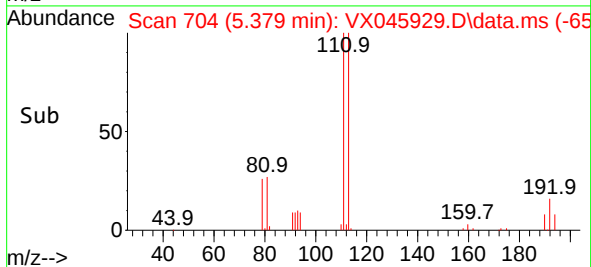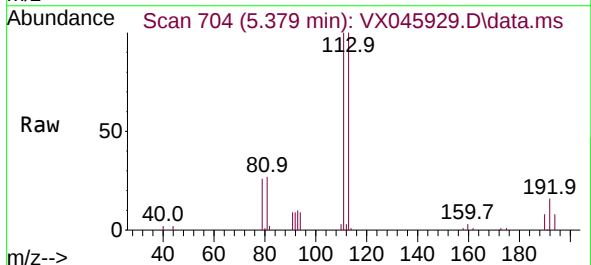



#36

1,1-Dichloropropene

Concen: 5.294 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.134 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Instrument :

MSVOA_X

ClientSampleId :

2001





Tgt Ion: 75 Resp: 6434

Ion Ratio Lower Upper

75 100

110 9.3 16.9 50.6#

77 0.0 25.0 37.4#



#38

Carbon Tetrachloride

Concen: 5.883 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.128 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56




Tgt Ion: 117 Resp: 7728


Ion Ratio Lower Upper

117 100

119 4.5 76.9 115.3#

121 0.0 24.2 36.2#









#40
Benzene
Concen: 1.975 ug/l
RT: 6.037 min Scan# 811
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion: 78 Resp: 7331
Ion Ratio Lower Upper
78 100
77 22.7 19.0 28.6

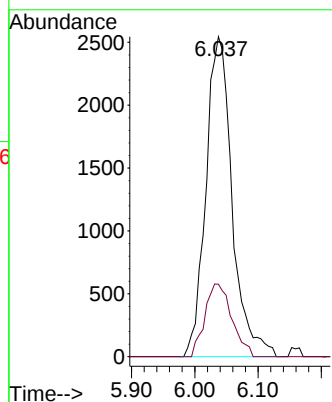

#43
Isopropyl Acetate
Concen: 5.785 ug/l
RT: 6.342 min Scan# 862
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 43 Resp: 13429
Ion Ratio Lower Upper
43 100
61 16.4 14.1 21.1
87 11.3 9.2 13.8


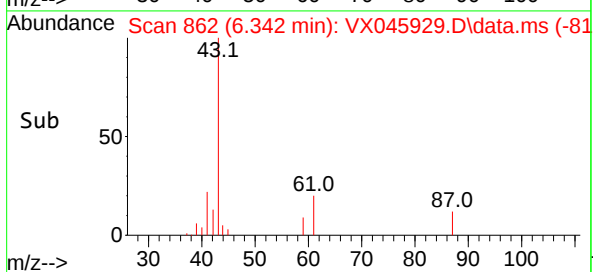
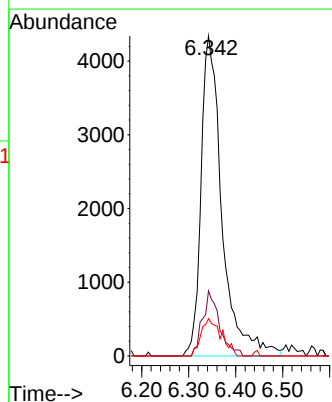





#48
Methyl methacrylate
Concen: 41.622 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.104 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion: 41 Resp: 49890
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 60.2 53.6 80.4



#50
Toluene-d8
Concen: 51.132 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 98 Resp: 160661
Ion Ratio Lower Upper
98 100
100 65.3 52.2 78.4




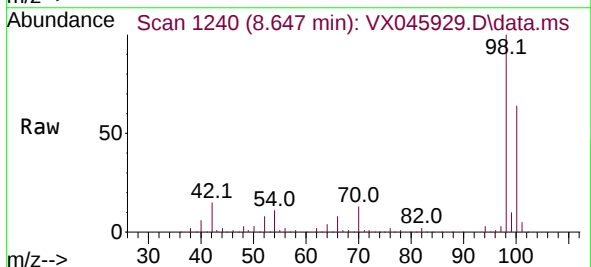




#51
4-Methyl-2-Pentanone
Concen: 26.417 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion: 43 Resp: 40655
Ion Ratio Lower Upper
43 100
58 8.1 28.5 42.7#

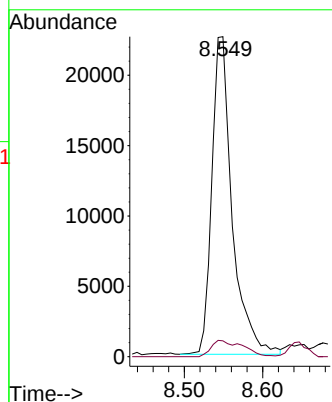

#52
Toluene
Concen: 2.327 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 92 Resp: 5226
Ion Ratio Lower Upper
92 100
91 178.2 138.7 208.1

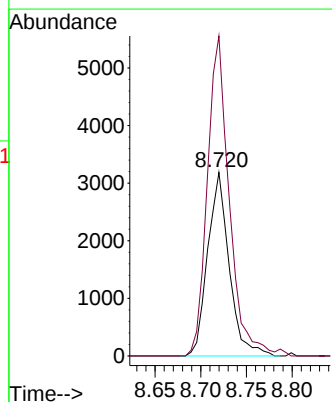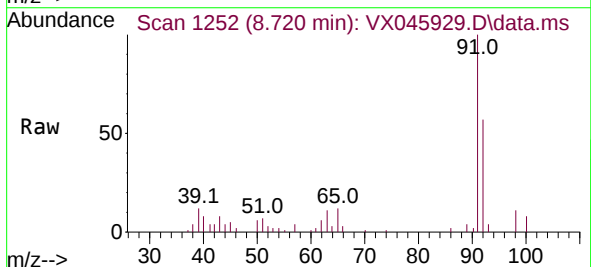



#53

t-1,3-Dichloropropene

Concen: 2.393 ug/l

RT: 8.958 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Instrument :

MSVOA_X

ClientSampleId :





2001

Tgt Ion: 75 Resp: 148

Ion Ratio Lower Upper

75 100

77 0.0 25.4 38.0#

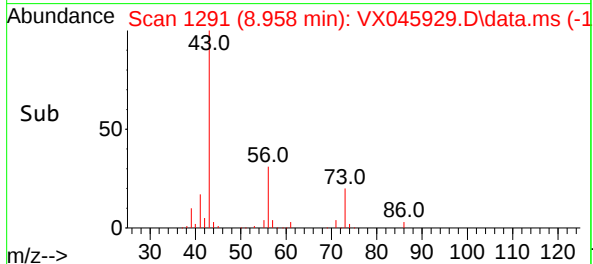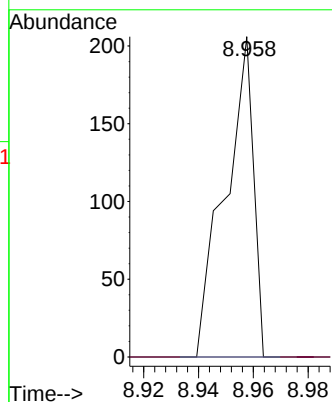

#54

cis-1,3-Dichloropropene

Concen: 11.063 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56




Tgt Ion: 75 Resp: 14762


Ion Ratio Lower Upper

75 100

77 0.0 24.6 36.8#

39 44.2 48.4 72.6#

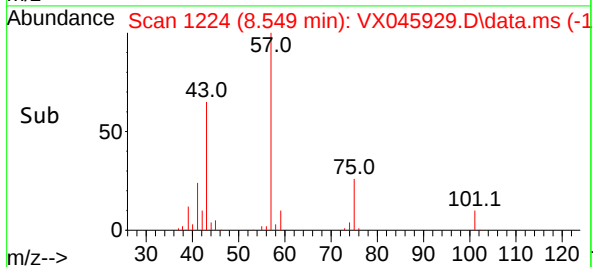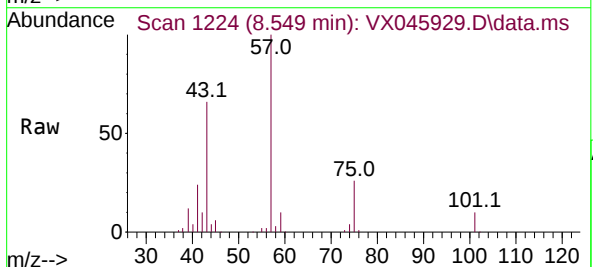



#57

1,3-Dichloropropane

Concen: 1.002 ug/l

RT: 9.482 min Scan# 1

Delta R.T. 0.177 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Instrument :

MSVOA_X

ClientSampleId :





2001

Tgt Ion: 76 Resp: 1561

Ion Ratio Lower Upper

76 100

78 0.0 26.0 39.0#

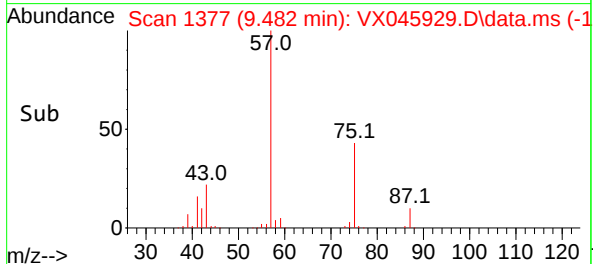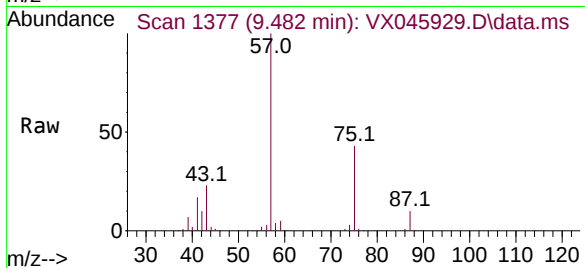

#59

2-Hexanone

Concen: 11.507 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.049 min

Lab File: VX045929.D




Acq: 24 Apr 2025 15:56


Tgt Ion: 43 Resp: 13114

Ion Ratio Lower Upper

43 100

58 0.0 24.9 74.6#

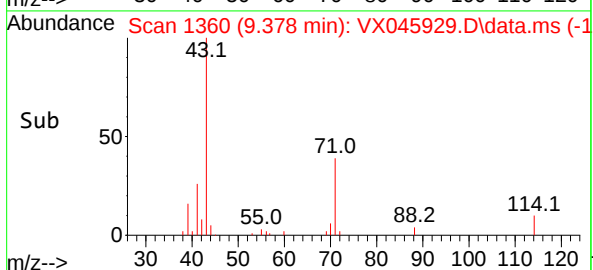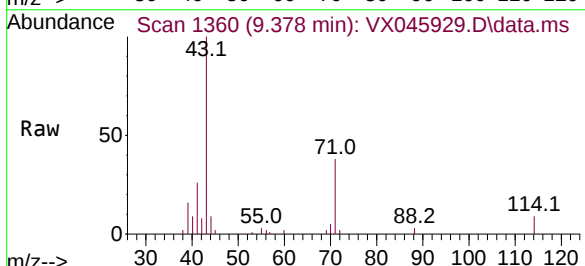



#62

4-Bromofluorobenzene

Concen: 50.062 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Instrument :

MSVOA_X

ClientSampleId :

2001





Tgt Ion: 95 Resp: 57296

Ion Ratio Lower Upper

95 100

174 69.1 0.0 135.8

176 64.5 0.0 131.4

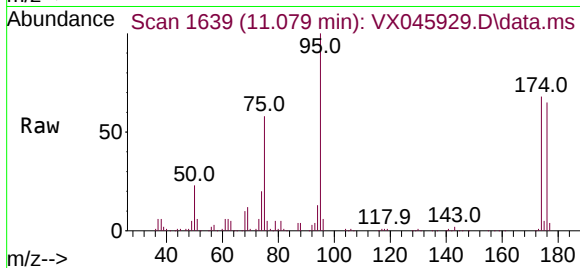

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. -0.000 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56




Tgt Ion: 117 Resp: 117802


Ion Ratio Lower Upper

117 100

82 64.1 49.2 73.8

119 31.5 25.1 37.7


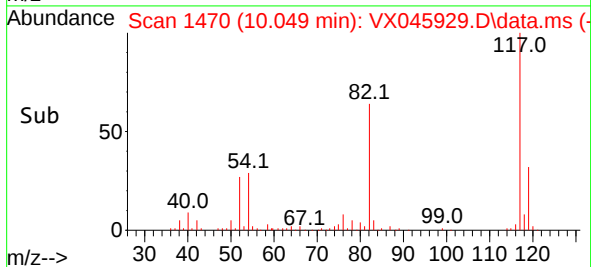

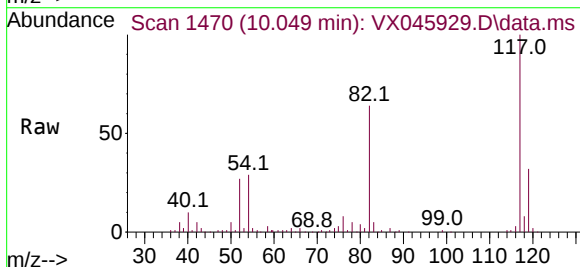




#67
Ethyl Benzene
Concen: 0.248 ug/l
RT: 10.195 min Scan# 1493
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion: 91 Resp: 1119
Ion Ratio Lower Upper
91 100
106 25.5 23.7 35.5



#68
m/p-Xylenes
Concen: 1.077 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 106 Resp: 1766
Ion Ratio Lower Upper
106 100
91 216.9 172.6 258.8

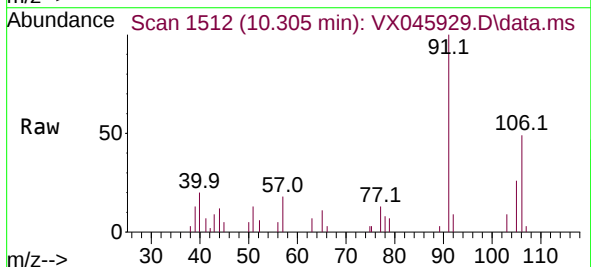



#69

o-Xylene

Concen: 0.788 ug/l

RT: 10.640 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Instrument :

MSVOA_X

ClientSampleId :





2001

Tgt Ion:106 Resp: 1273

Ion Ratio Lower Upper

106 100

91 243.2 113.6 340.6

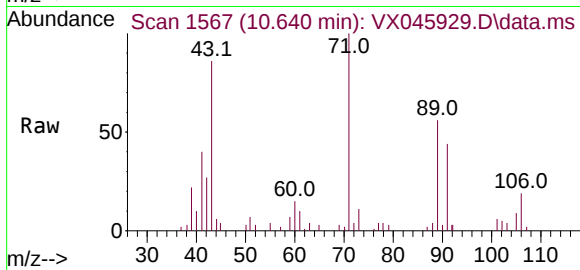

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.000 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56




Tgt Ion:152 Resp: 46552


Ion Ratio Lower Upper

152 100

115 65.5 46.9 140.7

150 159.7 0.0 349.4




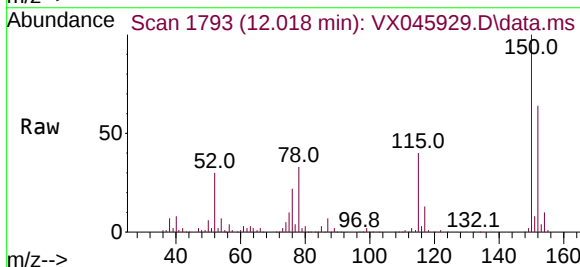




#74
N-amy1 acetate
Concen: 1.032 ug/l
RT: 10.774 min Scan# 1639
Delta R.T. -0.067 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion:	43	Resp:	1840
Ion	Ratio	Lower	Upper
43	100		
70	0.0	30.1	45.1#
55	8.4	18.3	27.5#
61	0.0	17.5	26.3#

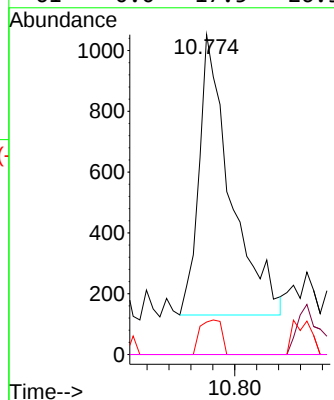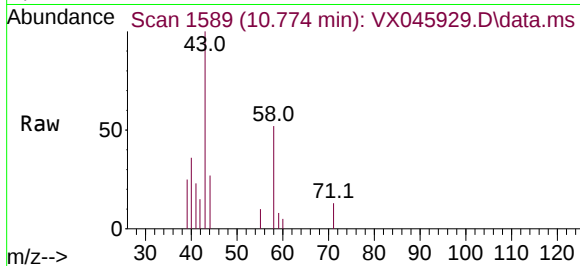

#76
1,2,3-Trichloropropane
Concen: 29.049 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion:	75	Resp:	32986
Ion	Ratio	Lower	Upper
75	100		
77	0.9	20.0	59.9#


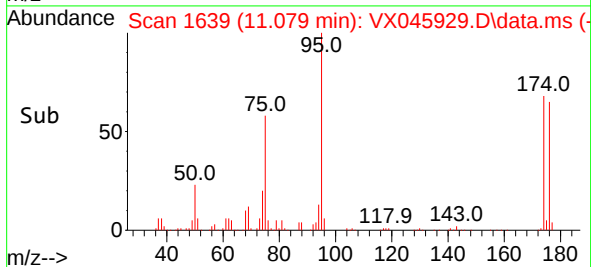
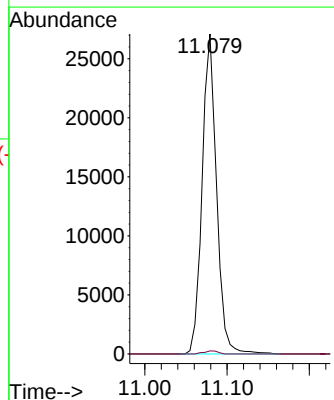
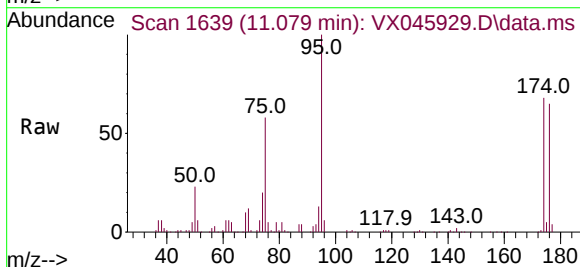




#80
1,3,5-Trimethylbenzene
Concen: 0.242 ug/l
RT: 11.457 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56




Instrument :
MSVOA_X
ClientSampleId :
2001


Tgt Ion:105 Resp: 745
Ion Ratio Lower Upper
105 100
120 33.3 23.0 69.0

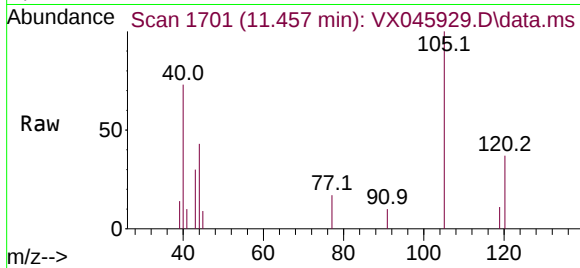

#81
trans-1,4-Dichloro-2-butene
Concen: 98.590 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX045929.D
Acq: 24 Apr 2025 15:56

Tgt Ion: 75 Resp: 32986
Ion Ratio Lower Upper
75 100
53 0.0 101.8 152.6#
89 0.0 37.2 55.8#




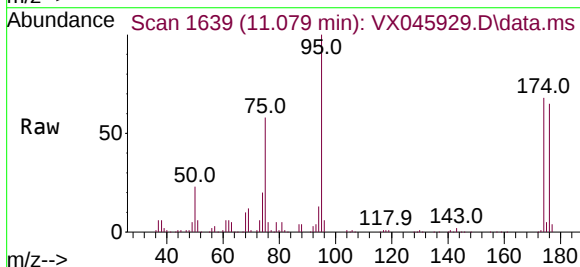




#84
 1,2,4-Trimethylbenzene
 Concen: 0.693 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.006 min
 Lab File: VX045929.D
 Acq: 24 Apr 2025 15:56




Instrument :
 MSVOA_X
 ClientSampleId :
 2001


Tgt Ion:105 Resp: 2146
 Ion Ratio Lower Upper
 105 100
 120 24.7 21.4 64.3

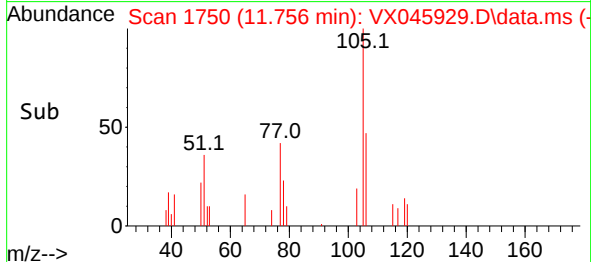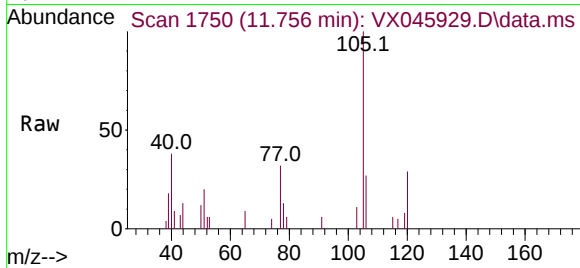

#85
 sec-Butylbenzene
 Concen: 0.572 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.134 min
 Lab File: VX045929.D
 Acq: 24 Apr 2025 15:56

Tgt Ion:105 Resp: 2146
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.6 28.6#

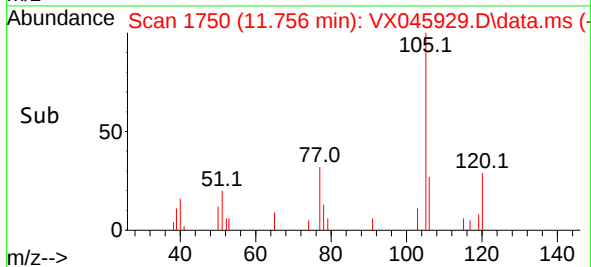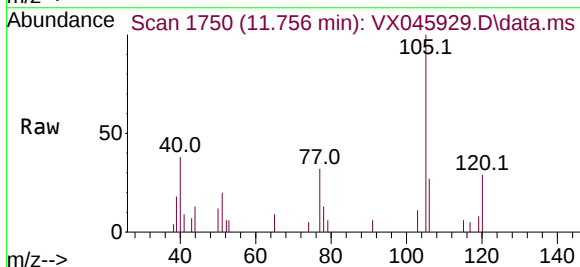



#90

Hexachloroethane

Concen: 0.821 ug/l

RT: 12.414 min Scan# 117

Delta R.T. -0.122 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Instrument :

MSVOA_X

ClientSampleId :





2001

Tgt Ion:117 Resp: 436

Ion Ratio Lower Upper

117 100

201 0.0 31.2 93.6#

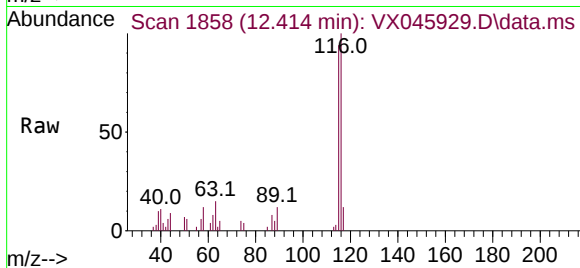

#95

Naphthalene

Concen: 20.200 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. -0.000 min

Lab File: VX045929.D

Acq: 24 Apr 2025 15:56

Tgt Ion:128 Resp: 65242

Ion Ratio Lower Upper

128 100

127 13.3 10.3 15.5

129 11.4 8.6 12.8

