

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042519\
 Data File : VX009161.D
 Acq On : 25 Apr 2019 14:45
 Operator : JC/SP
 Sample : K2555-08
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BLIND-DUPLICATE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.623	66	77	79	rBV9	8179	18954	1.60%	0.317%
2	2.611	233	239	247	rVB	10196	19984	1.69%	0.334%
3	3.013	299	305	316	rVB	5122	13497	1.14%	0.226%
4	4.702	571	582	591	rBV2	3764	11843	1.00%	0.198%
5	5.501	701	713	725	rBV	123349	352269	29.80%	5.892%
6	5.659	728	739	753	rVB	226337	633145	53.56%	10.590%
7	6.061	795	805	818	rBV	155584	408540	34.56%	6.834%
8	6.860	923	936	950	rBV	360597	853932	72.23%	14.283%
9	8.713	1233	1240	1255	rBV	763787	1182220	100.00%	19.775%
10	10.109	1462	1469	1478	rBV	689103	960811	81.27%	16.071%
11	11.134	1632	1637	1652	rBV	553216	714048	60.40%	11.944%
12	12.079	1786	1792	1801	rBV	630463	809230	68.45%	13.536%


Sum of corrected areas: 5978473

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042519\
Data File : VX009161.D
Acq On : 25 Apr 2019 14:45
Operator : JC/SP
Sample : K2555-08
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BLIND-DUPLICATE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

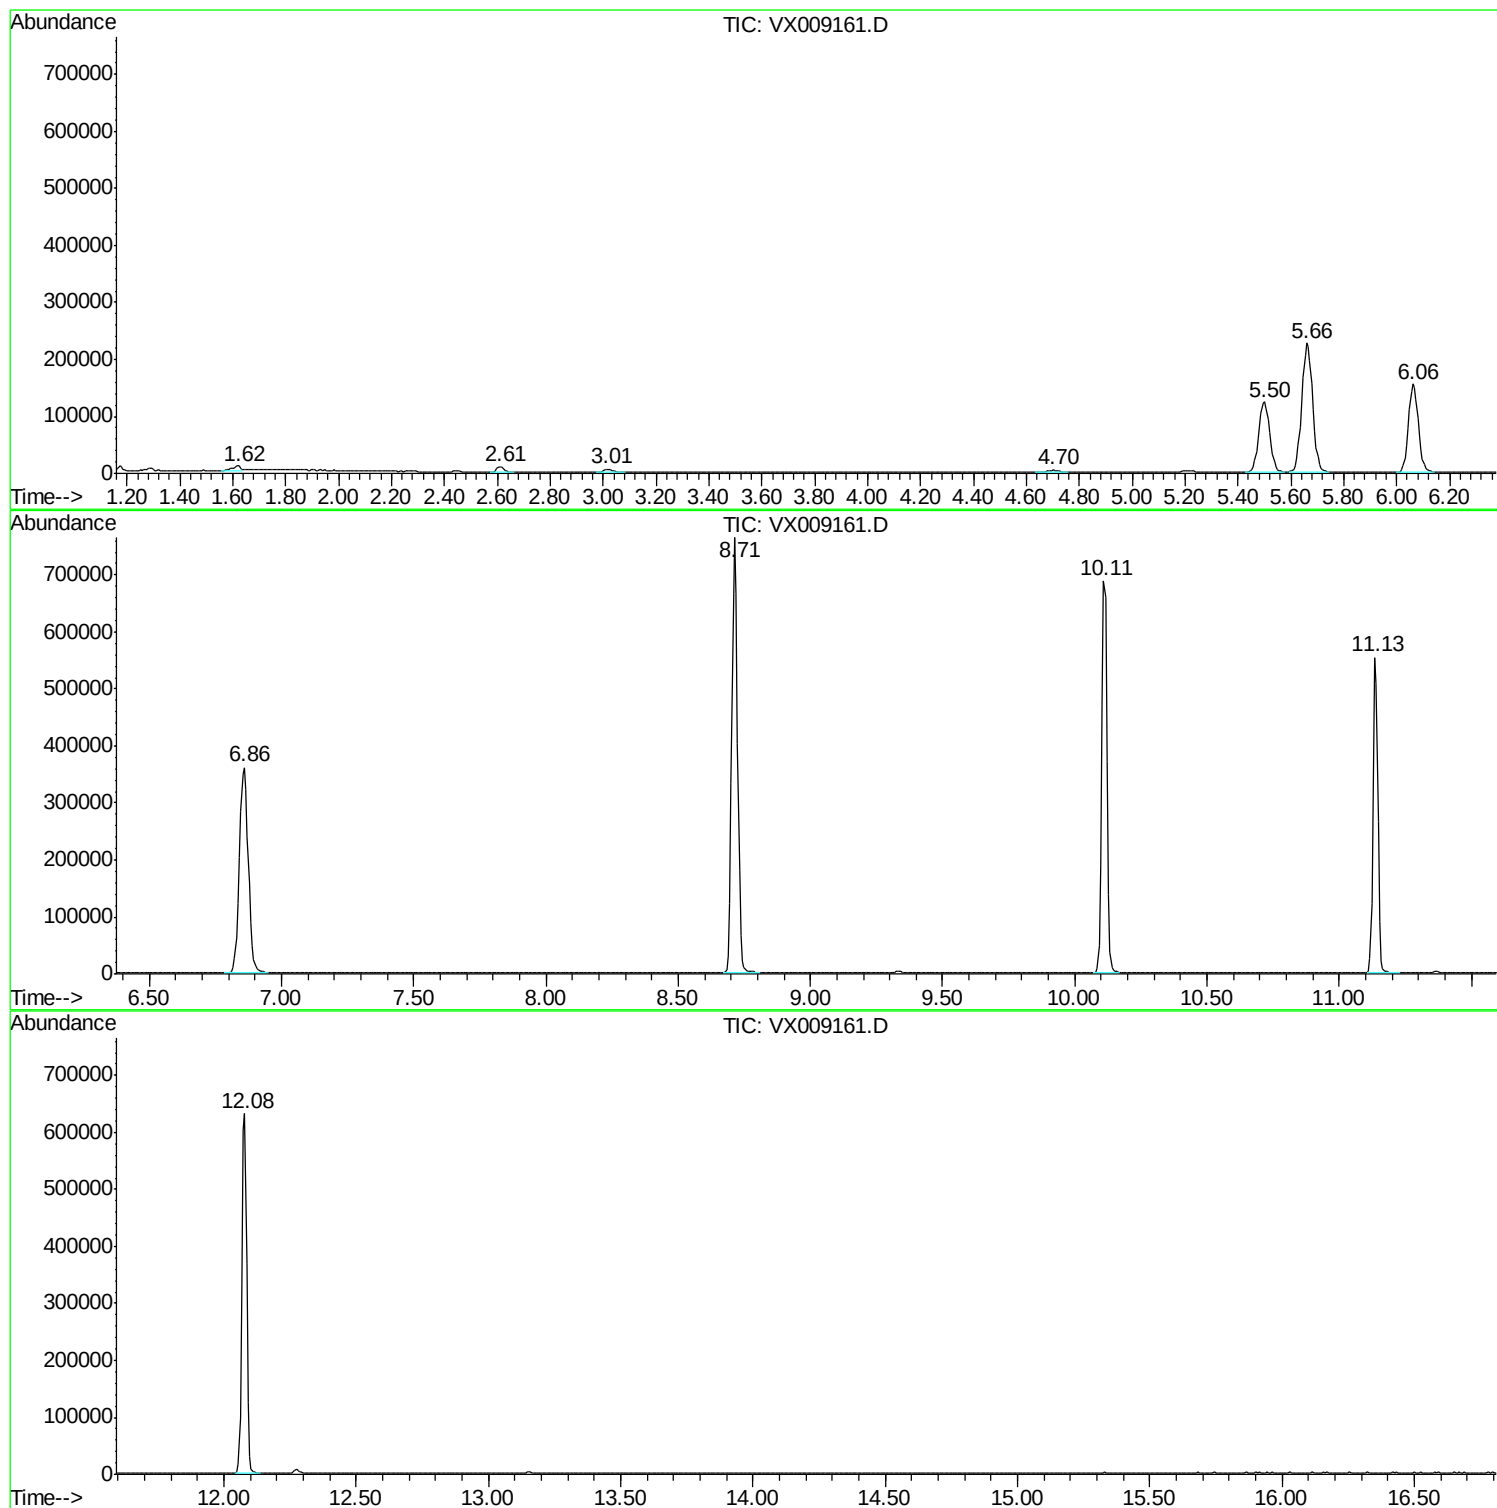

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX042519\
Data File : VX009161.D
Acq On : 25 Apr 2019 14:45
Operator : JC/SP
Sample : K2555-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BLIND-DUPLICATE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX042519\
Data File : VX009161.D
Acq On : 25 Apr 2019 14:45
Operator : JC/SP
Sample : K2555-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BLIND-DUPLICATE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc