

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042522\
 Data File : VX028337.D
 Acq On : 25 Apr 2022 19:31
 Operator : JC/MD
 Sample : N2557-03DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PURGE-WATERDL

Quant Time: Apr 26 08:14:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	400009	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	692068	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	658985	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	312575	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	244200	46.821	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	93.640%		
35) Dibromofluoromethane	5.385	113	219803	45.288	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	90.580%		
50) Toluene-d8	8.653	98	820757	44.030	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	88.060%		
62) 4-Bromofluorobenzene	11.079	95	299132	41.968	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	83.940%		
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.142	85	871	0.337	ug/l	98
3) Chloromethane	1.294	50	526	Below Cal		99
4) Vinyl Chloride	1.374	62	5283	1.310	ug/l #	83
5) Bromomethane	1.611	94	1023	Below Cal		90
6) Chloroethane	1.691	64	244	Below Cal		91
9) 1,1,2-Trichlorotrifluo...	2.331	101	29007	8.955	ug/l	94
10) Methyl Iodide	2.459	142	569	5.349	ug/l #	73
11) Tert butyl alcohol	2.947	59	12658	2.852	ug/l #	78
12) 1,1-Dichloroethene	2.319	96	8149	2.651	ug/l	94
16) Acetone	2.380	43	6210	2.516	ug/l	91
20) Methylene Chloride	2.788	84	1898	0.490	ug/l #	78
21) trans-1,2-Dichloroethene	3.093	96	1036	0.248	ug/l #	92
24) 1,1-Dichloroethane	3.611	63	37750	5.442	ug/l	99
27) cis-1,2-Dichloroethene	4.495	96	284109	56.992	ug/l	84
30) Chloroform	5.092	83	3143	0.377	ug/l	93
31) Cyclohexane	5.556	56	7116	1.120	ug/l #	21
32) 1,1,1-Trichloroethane	5.391	97	27455	3.639	ug/l	97
36) 1,1-Dichloropropene	5.550	75	29283	4.625	ug/l #	50
38) Carbon Tetrachloride	5.556	117	40776	5.705	ug/l #	16
39) Methylcyclohexane	7.129	83	2705	0.339	ug/l #	1
44) Trichloroethene	7.129	130	229723	42.747	ug/l	99
49) 1,4-Dioxane	7.696	88	115	0.896	ug/l #	25
52) Toluene	8.720	92	207443	16.112	ug/l	99
53) t-1,3-Dichloropropene	8.720	75	2454	0.338	ug/l #	1
60) Dibromochloromethane	9.275	129	12459	2.185	ug/l #	9
64) Tetrachloroethene	9.275	164	12892	2.505	ug/l	94
76) 1,2,3-Trichloropropane	11.079	75	148656	24.165	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	148656	71.812	ug/l #	15
90) Hexachloroethane	12.695	117	100	1.841	ug/l #	10
91) 1,2-Dichlorobenzene	12.335	146	8435	0.808	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042522\
Data File : VX028337.D
Acq On : 25 Apr 2022 19:31
Operator : JC/MD
Sample : N2557-03DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL

Quant Time: Apr 26 08:14:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




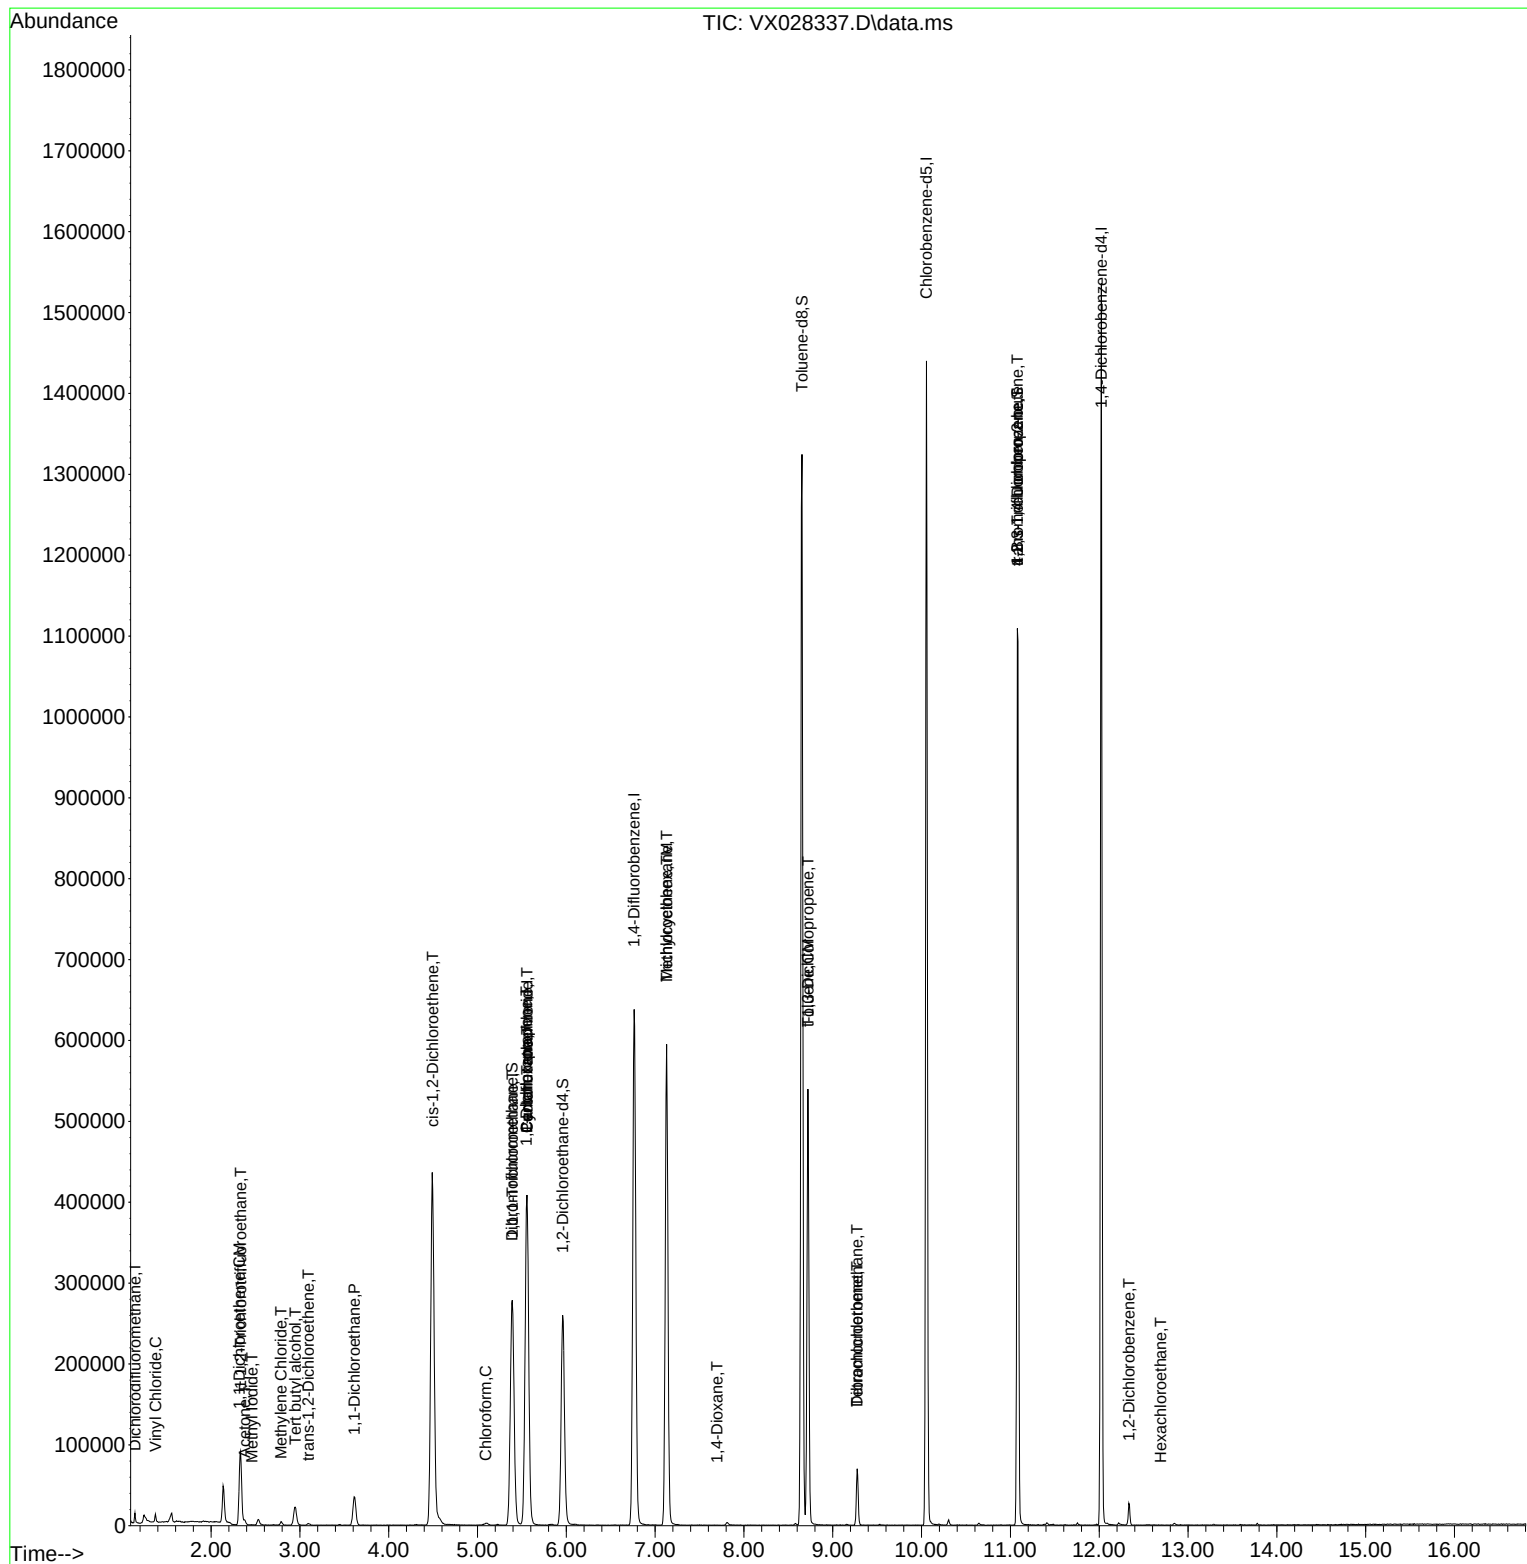




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion:168 Resp: 400009
Ion Ratio Lower Upper
168 100
99 55.9 41.7 62.5

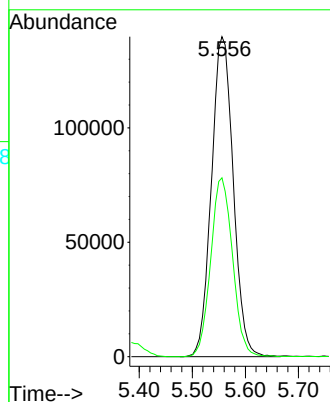

#2
Dichlorodifluoromethane
Concen: 0.337 ug/l
RT: 1.142 min Scan# 9
Delta R.T. -0.024 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 85 Resp: 871
Ion Ratio Lower Upper
85 100
87 31.2 16.2 48.6


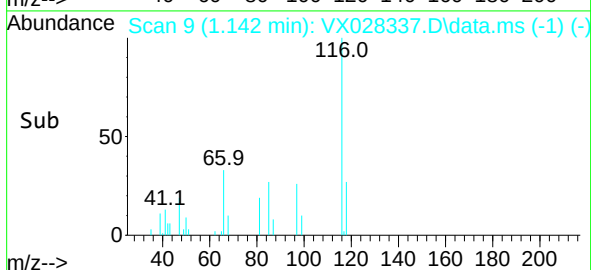
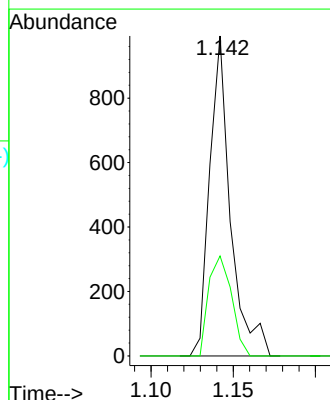
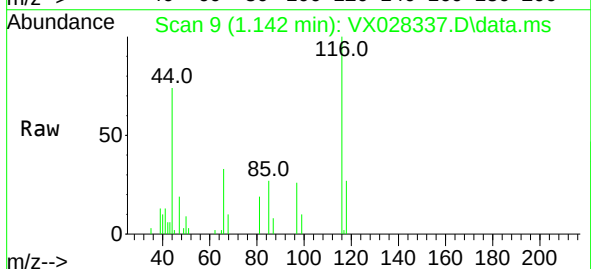


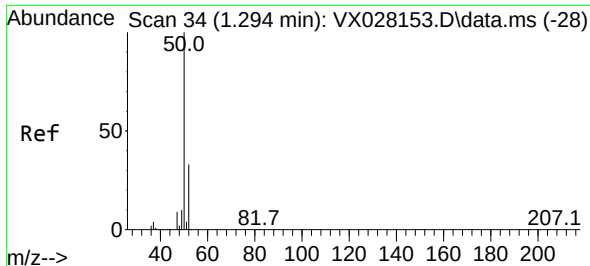

#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 50 Resp: 526
Ion Ratio Lower Upper
50 100
52 32.5 26.4 39.6

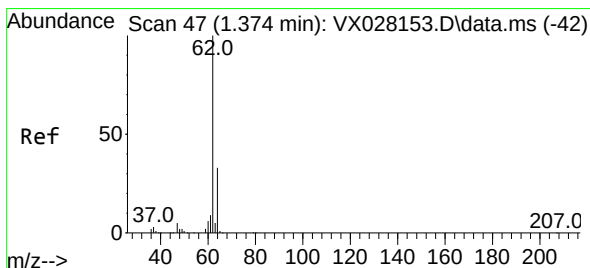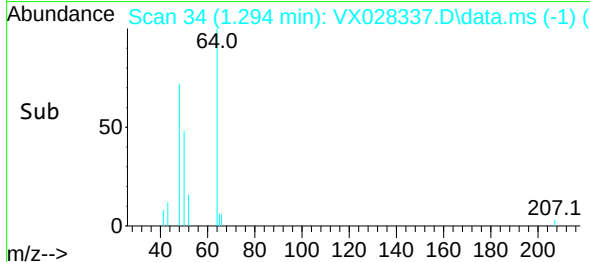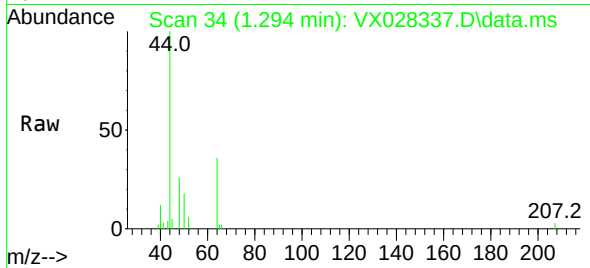

#4
Vinyl Chloride
Concen: 1.310 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 62 Resp: 5283
Ion Ratio Lower Upper
62 100
64 41.4 25.5 38.3#


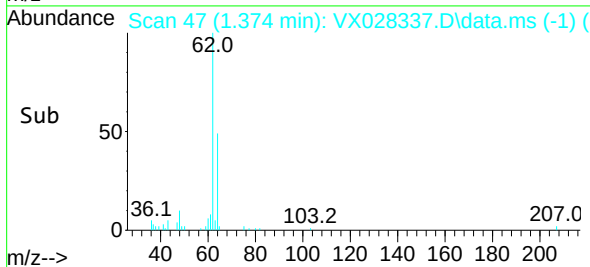

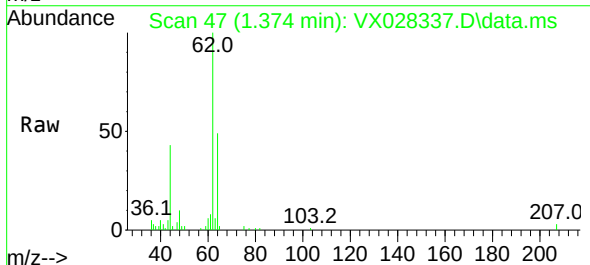


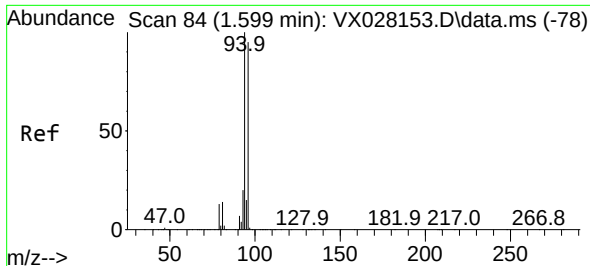

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 80
Delta R.T. 0.012 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 94 Resp: 1023
Ion Ratio Lower Upper
94 100
96 103.9 75.3 112.9

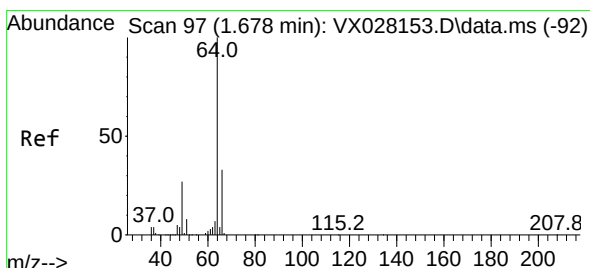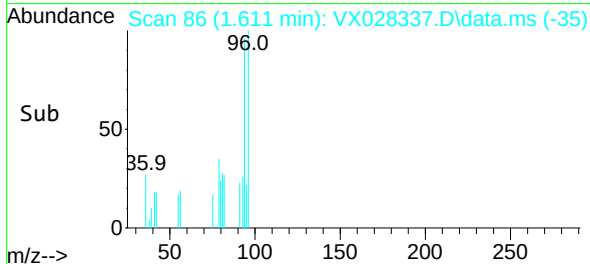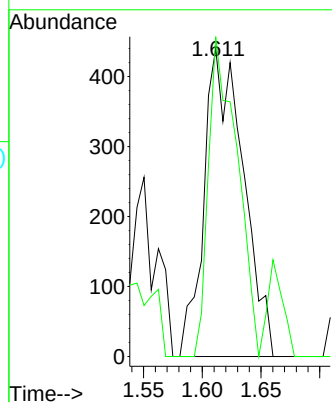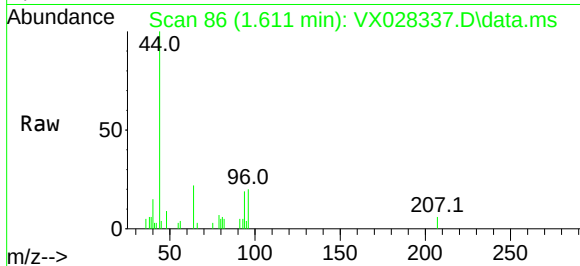

#6
Chloroethane
Concen: Below Cal
RT: 1.691 min Scan# 99
Delta R.T. 0.013 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 64 Resp: 244
Ion Ratio Lower Upper
64 100
66 36.5 25.3 37.9


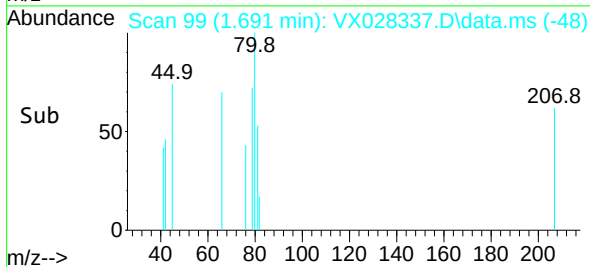
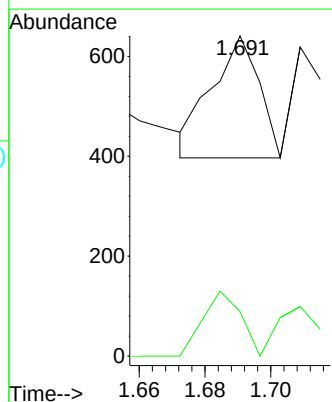
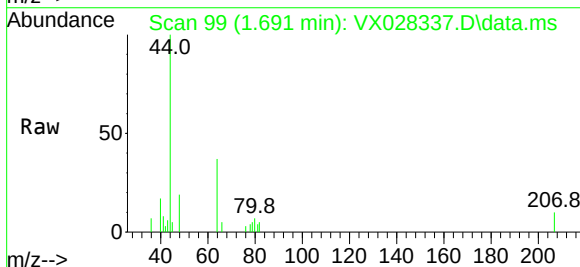




#9
1,1,2-Trichlorotrifluoroethane
Concen: 8.955 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion:101 Resp: 29007
Ion Ratio Lower Upper
101 100
85 47.8 33.5 50.3
151 80.6 61.8 92.6

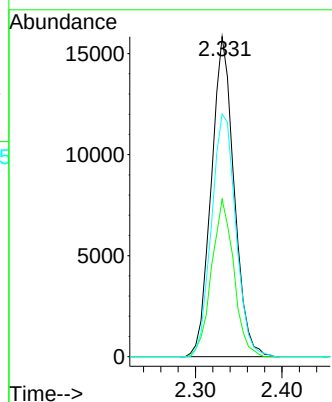

#10
Methyl Iodide
Concen: 5.349 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion:142 Resp: 569
Ion Ratio Lower Upper
142 100
127 26.5 33.9 50.9#
141 0.0 11.4 17.2#


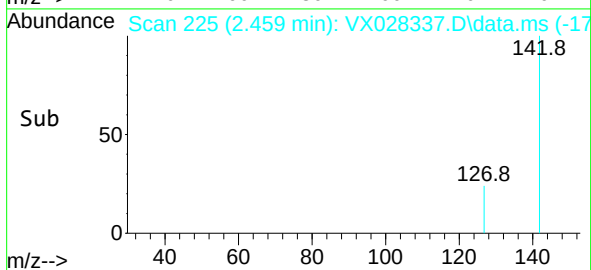

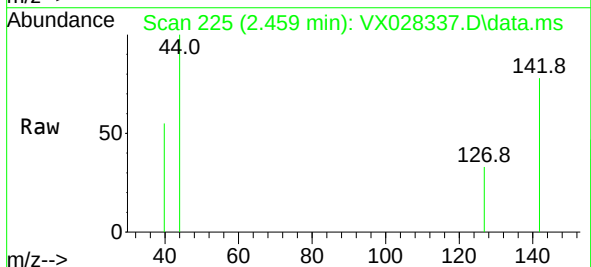


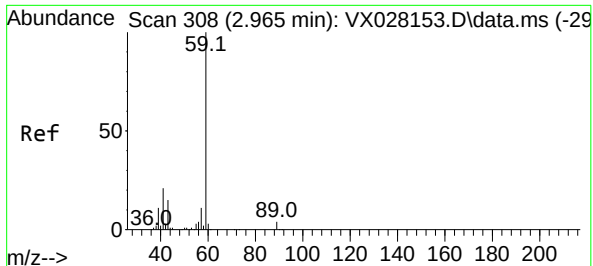

#11
Tert butyl alcohol
Concen: 2.852 ug/l
RT: 2.947 min Scan# 308
Delta R.T. -0.018 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 59 Resp: 12658
Ion Ratio Lower Upper
59 100
57 2.2 8.3 12.5#

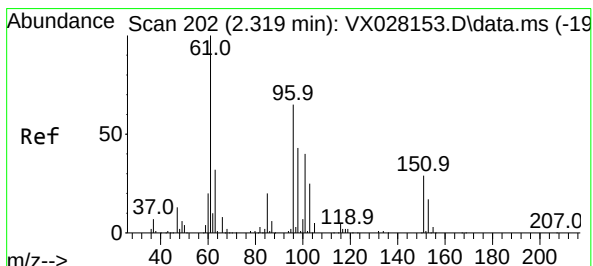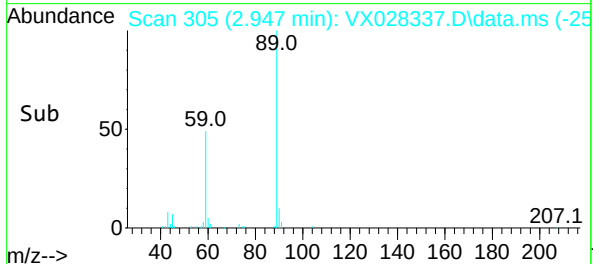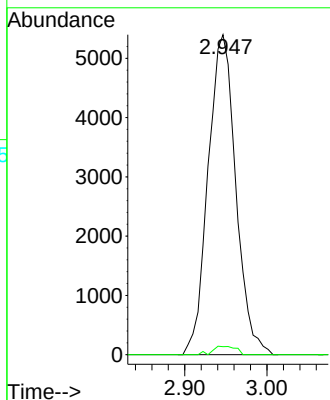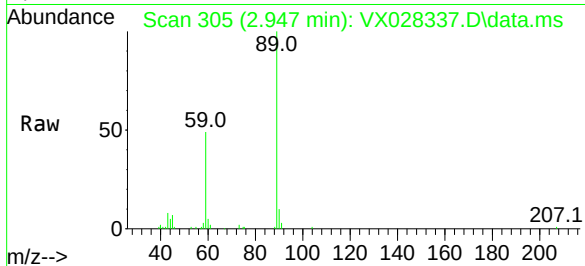

#12
1,1-Dichloroethene
Concen: 2.651 ug/l
RT: 2.319 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 96 Resp: 8149
Ion Ratio Lower Upper
96 100
61 149.4 124.6 187.0
98 69.3 51.0 76.4


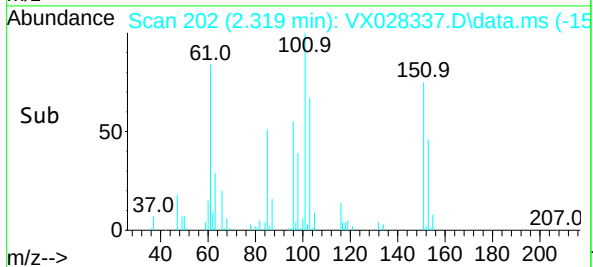
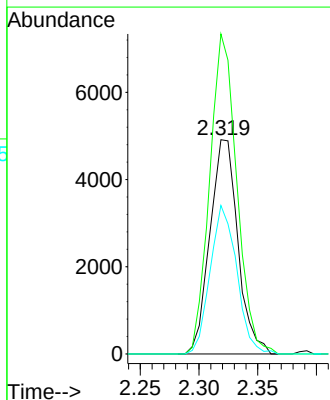
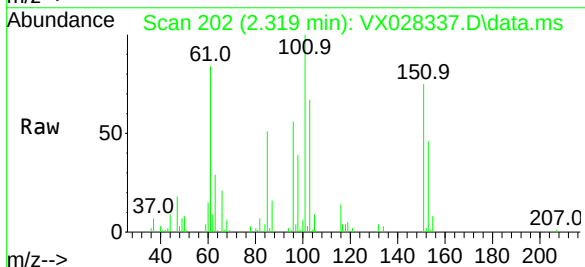


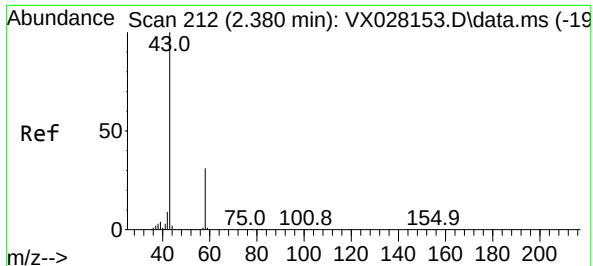

#16
Acetone
Concen: 2.516 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 43 Resp: 6210
Ion Ratio Lower Upper
43 100
58 30.5 28.8 43.2

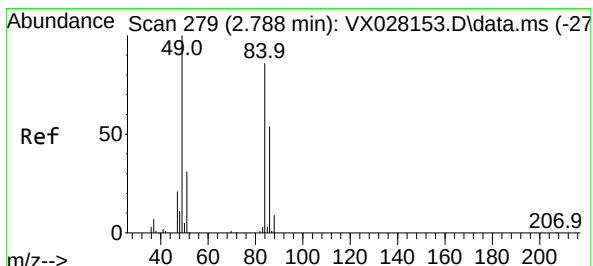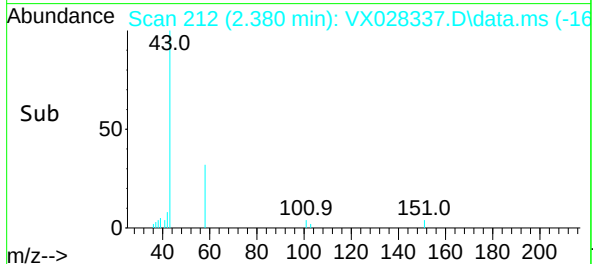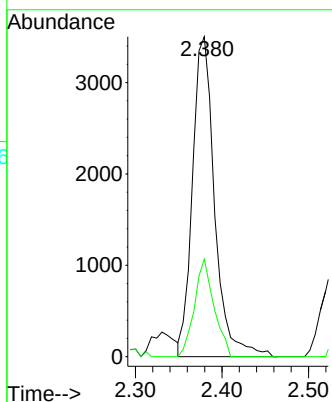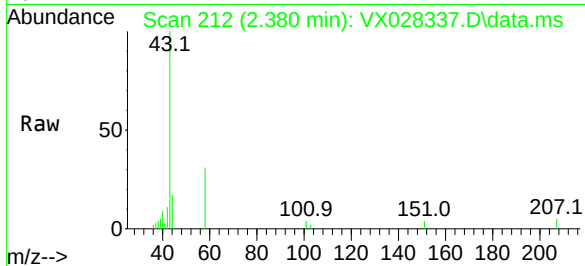

#20
Methylene Chloride
Concen: 0.490 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31


Tgt Ion: 84 Resp: 1898
Ion Ratio Lower Upper
84 100
49 138.6 85.5 128.3#
51 32.8 26.6 39.8
86 49.6 51.5 77.3#

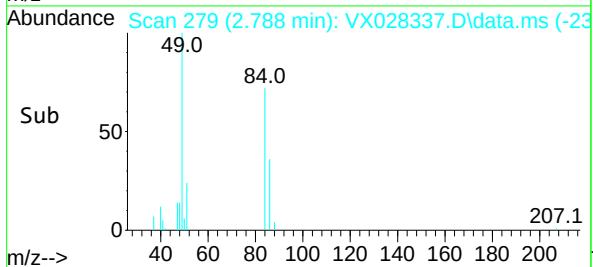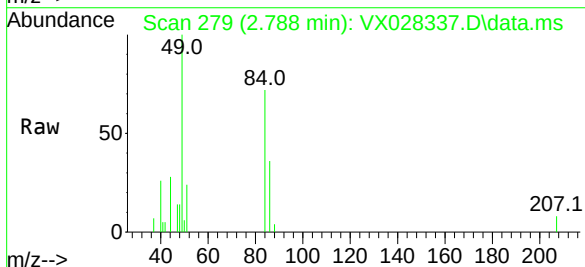






#21
trans-1,2-Dichloroethene
Concen: 0.248 ug/l
RT: 3.093 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL







Tgt Ion: 96 Resp: 1036
Ion Ratio Lower Upper
96 100
61 130.7 105.4 158.2
98 45.3 50.0 75.0#

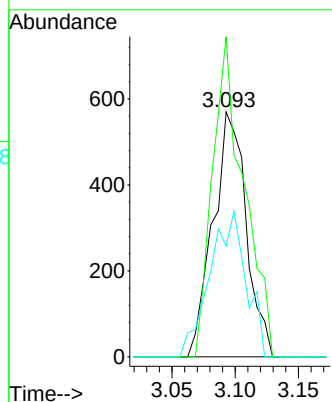

#24
1,1-Dichloroethane
Concen: 5.442 ug/l
RT: 3.611 min Scan# 414
Delta R.T. 0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 63 Resp: 37750
Ion Ratio Lower Upper
63 100
98 8.4 3.9 11.7
100 4.7 2.4 7.2


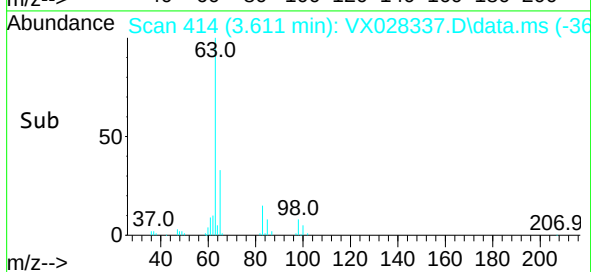
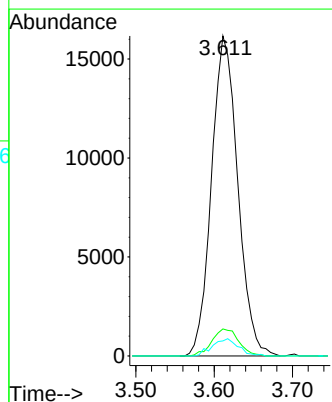





#27
 cis-1,2-Dichloroethene
 Concen: 56.992 ug/l
 RT: 4.495 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: VX028337.D
 Acq: 25 Apr 2022 19:31




Instrument :
 MSVOA_X
 ClientSampleId :
 PURGE-WATERDL


Tgt Ion: 96 Resp: 284109
 Ion Ratio Lower Upper
 96 100
 61 113.9 0.0 283.8
 98 65.8 0.0 129.8

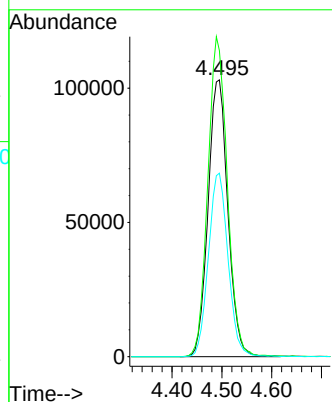

#30
 Chloroform
 Concen: 0.377 ug/l
 RT: 5.092 min Scan# 657
 Delta R.T. -0.007 min
 Lab File: VX028337.D
 Acq: 25 Apr 2022 19:31

Tgt Ion: 83 Resp: 3143
 Ion Ratio Lower Upper
 83 100
 85 60.5 52.7 79.1


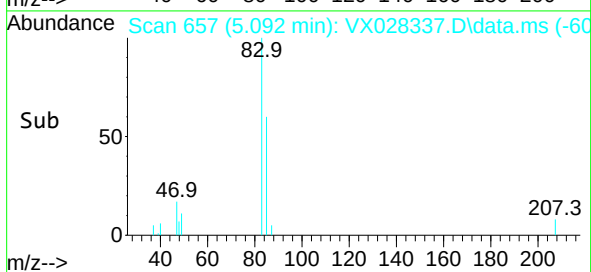
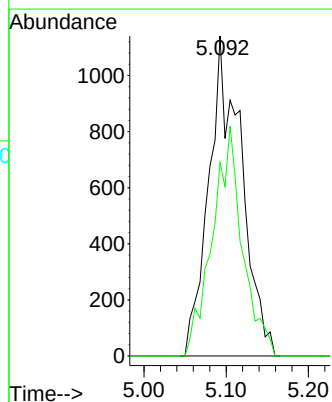



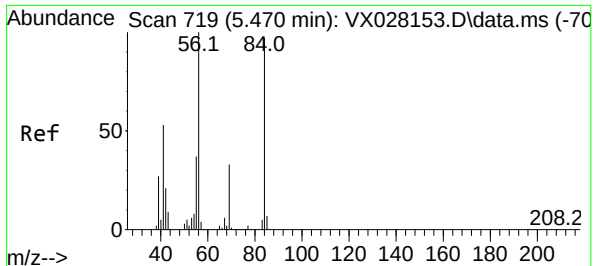

#31
Cyclohexane
Concen: 1.120 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.086 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 56 Resp: 7116
Ion Ratio Lower Upper
56 100
69 164.1 26.7 40.1#
84 123.3 77.2 115.8#

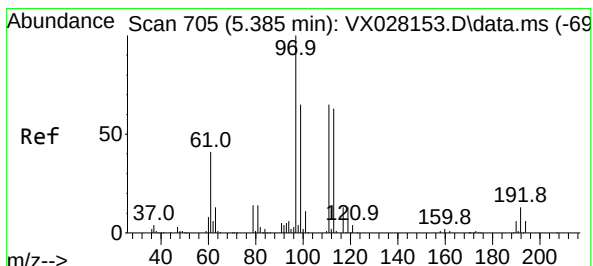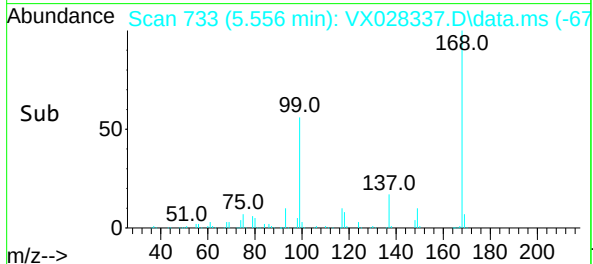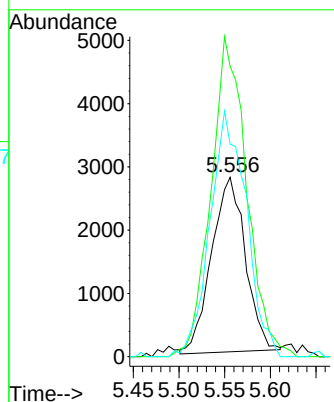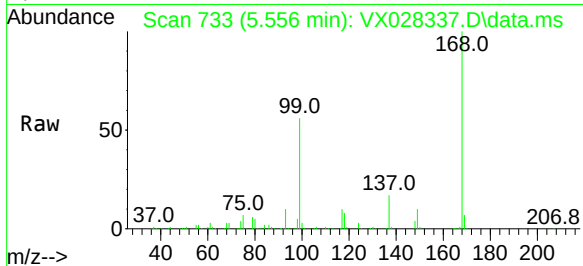

#32
1,1,1-Trichloroethane
Concen: 3.639 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 97 Resp: 27455
Ion Ratio Lower Upper
97 100
99 67.5 51.8 77.6
61 43.5 34.0 51.0


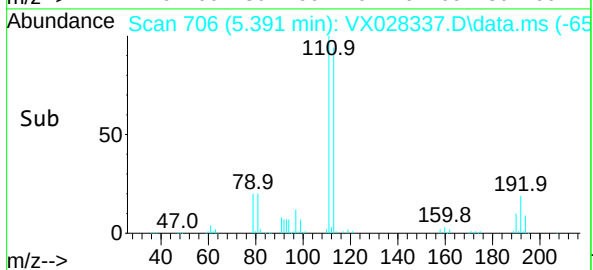
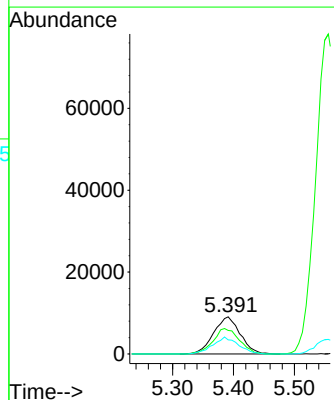
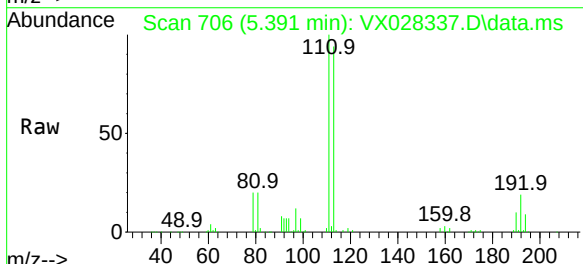




#33
 1,2-Dichloroethane-d4
 Concen: 46.821 ug/l
 RT: 5.958 min Scan# 799
 Delta R.T. 0.000 min
 Lab File: VX028337.D
 Acq: 25 Apr 2022 19:31




Instrument :
 MSVOA_X
 ClientSampleId :
 PURGE-WATERDL


Tgt Ion: 65 Resp: 244200
 Ion Ratio Lower Upper
 65 100
 67 51.3 0.0 107.4

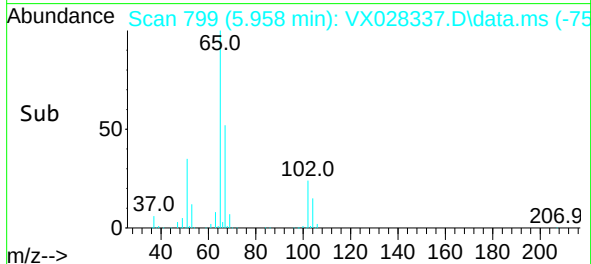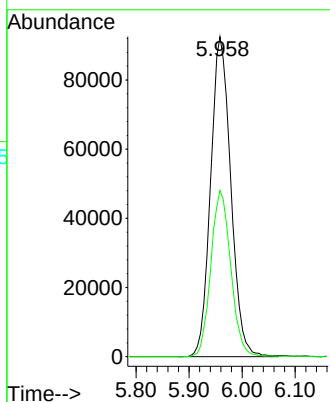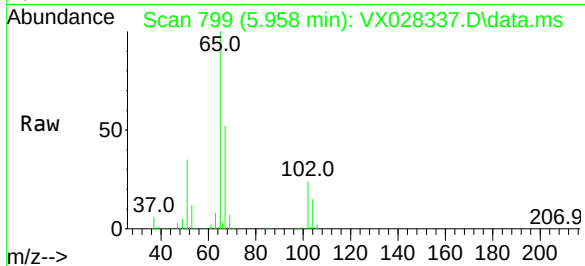

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.000 min
 Lab File: VX028337.D
 Acq: 25 Apr 2022 19:31

Tgt Ion: 114 Resp: 692068
 Ion Ratio Lower Upper
 114 100
 63 17.9 0.0 36.8
 88 15.4 0.0 32.4


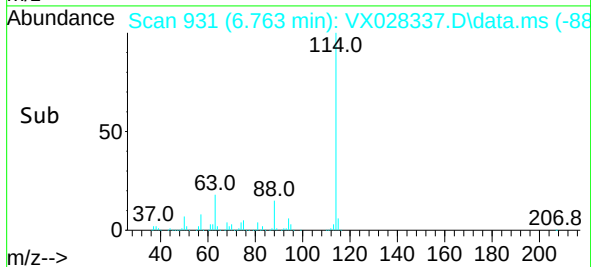
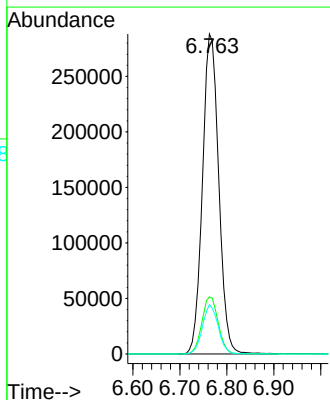
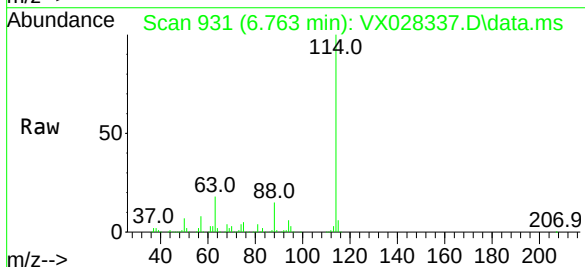


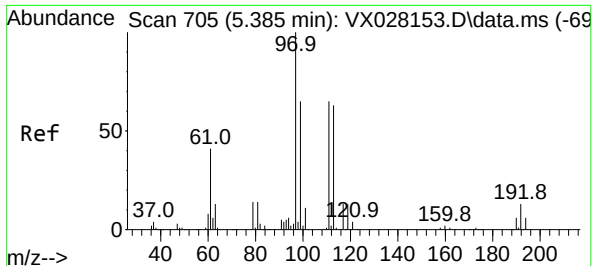

#35
Dibromofluoromethane
Concen: 45.288 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion:113 Resp: 219803
Ion Ratio Lower Upper
113 100
111 103.2 82.8 124.2
192 19.8 16.9 25.3

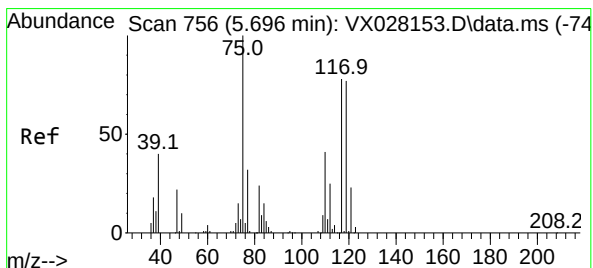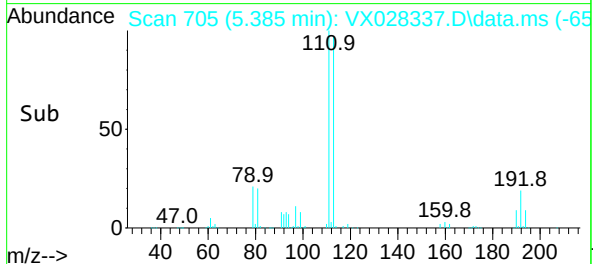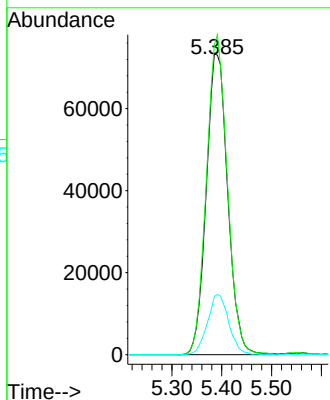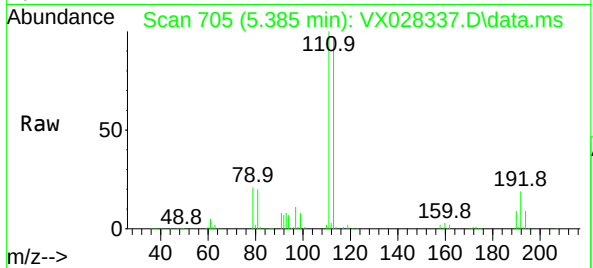

#36
1,1-Dichloropropene
Concen: 4.625 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.146 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31


Tgt Ion: 75 Resp: 29283
Ion Ratio Lower Upper
75 100
110 10.1 18.3 54.8#
77 0.0 24.8 37.2#

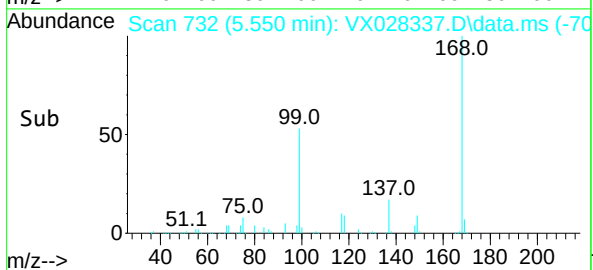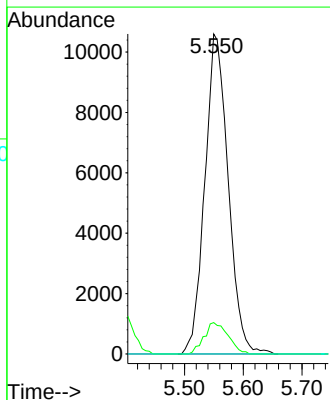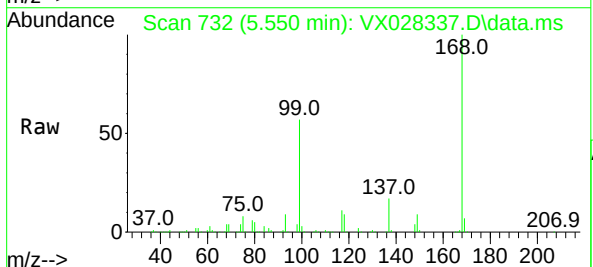






#38
Carbon Tetrachloride
Concen: 5.705 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL







Tgt Ion:117 Resp: 40776
Ion Ratio Lower Upper
117 100
119 5.3 77.3 115.9#
121 0.0 24.2 36.2#

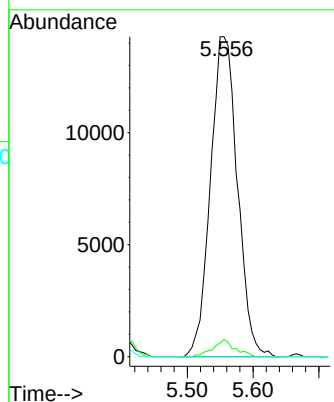

#39
Methylcyclohexane
Concen: 0.339 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.256 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 83 Resp: 2705
Ion Ratio Lower Upper
83 100
55 0.0 54.6 81.8#
98 178.9 37.4 56.2#


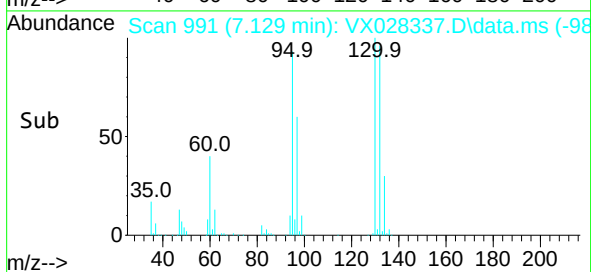
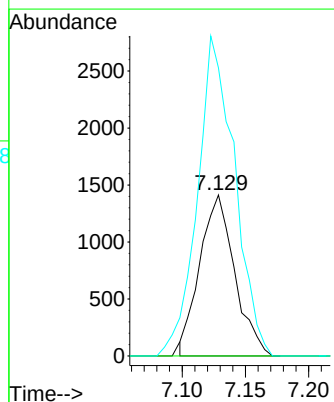



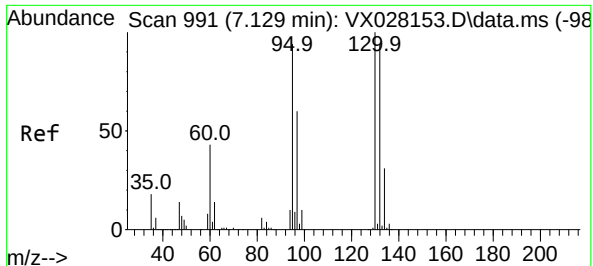

#44
Trichloroethene
Concen: 42.747 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion:130 Resp: 229723
Ion Ratio Lower Upper
130 100
95 93.0 0.0 188.8

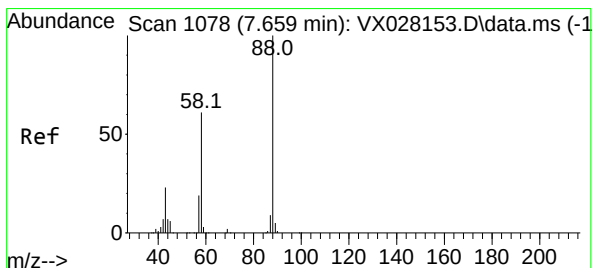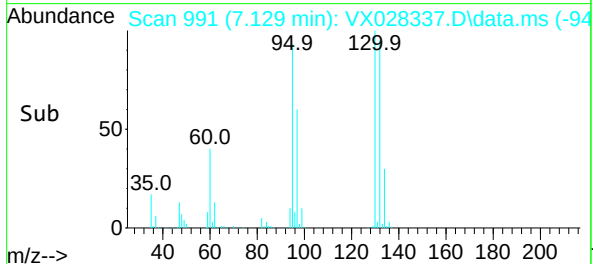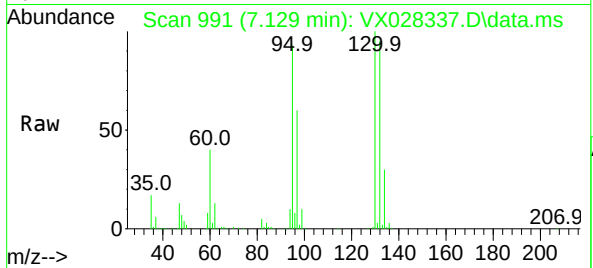

#49
1,4-Dioxane
Concen: 0.896 ug/l
RT: 7.696 min Scan# 1084
Delta R.T. 0.037 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 88 Resp: 115
Ion Ratio Lower Upper
88 100
43 0.0 21.9 32.9#
58 0.0 53.7 80.5#


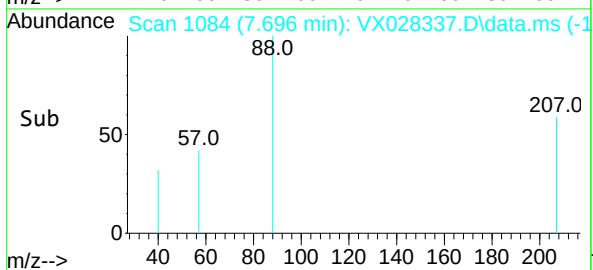

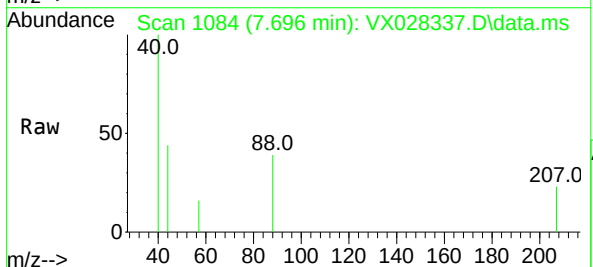




#50
Toluene-d8
Concen: 44.030 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 98 Resp: 820757
Ion Ratio Lower Upper
98 100
100 65.7 52.6 78.8

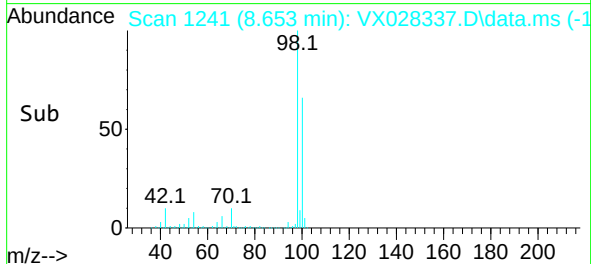

#52
Toluene
Concen: 16.112 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 92 Resp: 207443
Ion Ratio Lower Upper
92 100
91 170.0 137.5 206.3

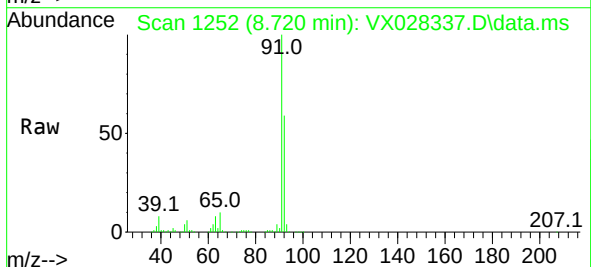

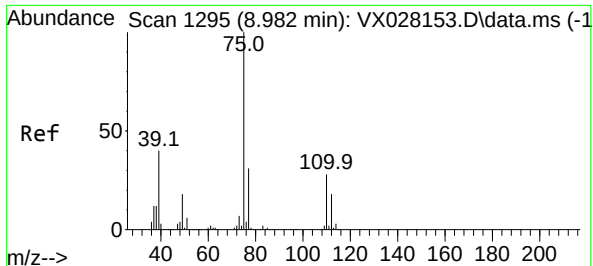

#53

t-1,3-Dichloropropene

Concen: 0.338 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX028337.D

Acq: 25 Apr 2022 19:31

Instrument :

MSVOA_X

ClientSampleId :





PURGE-WATERDL

Tgt Ion: 75 Resp: 2454

Ion Ratio Lower Upper

75 100

77 155.6 25.4 38.0#

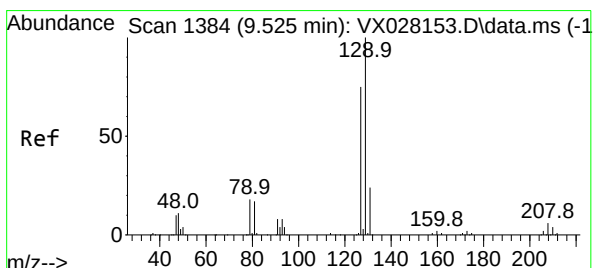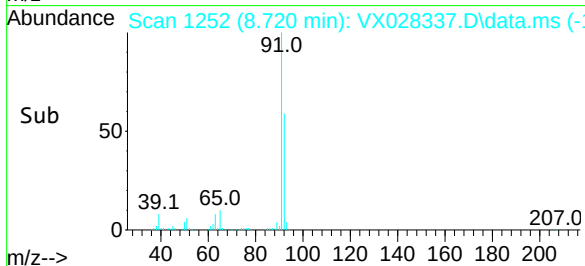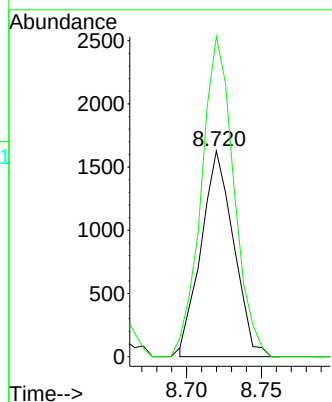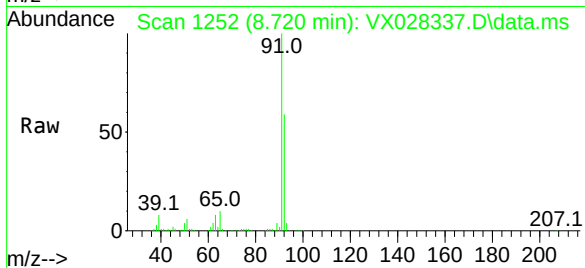

#60

Dibromochloromethane

Concen: 2.185 ug/l

RT: 9.275 min Scan# 1343

Delta R.T. -0.250 min

Lab File: VX028337.D




Acq: 25 Apr 2022 19:31


Tgt Ion: 129 Resp: 12459

Ion Ratio Lower Upper

129 100

127 0.0 40.3 120.8#


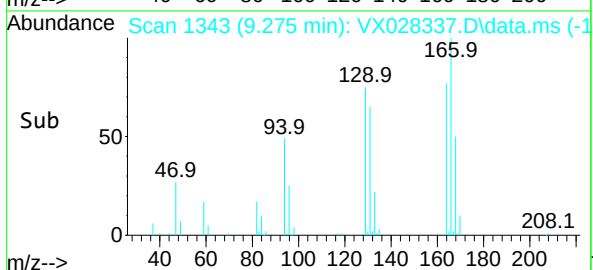

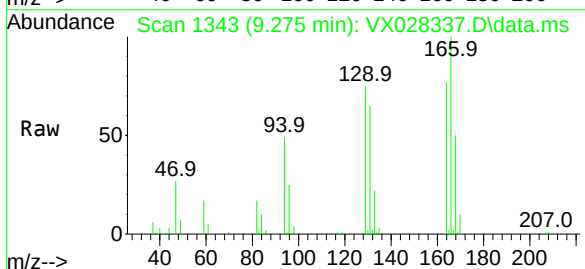




#62
4-Bromofluorobenzene
Concen: 41.968 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 95 Resp: 299132
Ion Ratio Lower Upper
95 100
174 83.4 0.0 163.0
176 80.9 0.0 155.0

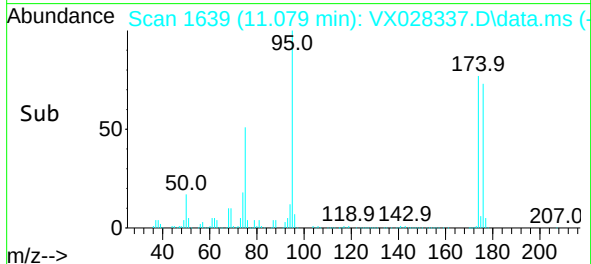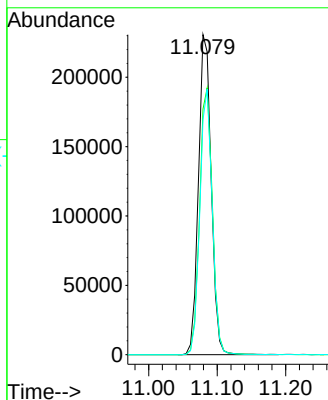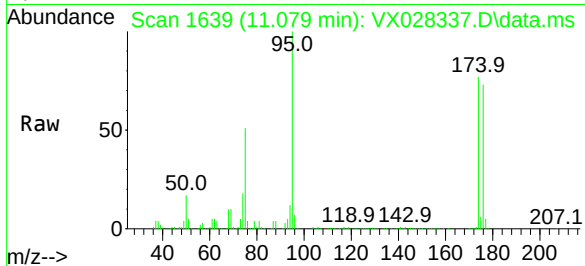

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 117 Resp: 658985
Ion Ratio Lower Upper
117 100
82 52.0 41.8 62.8
119 32.6 24.8 37.2

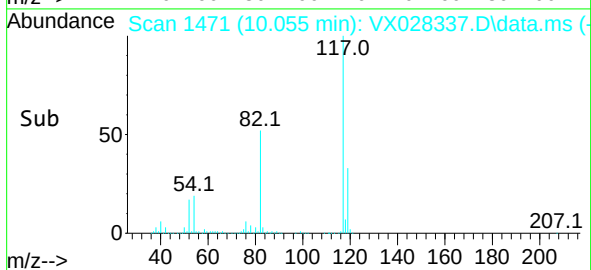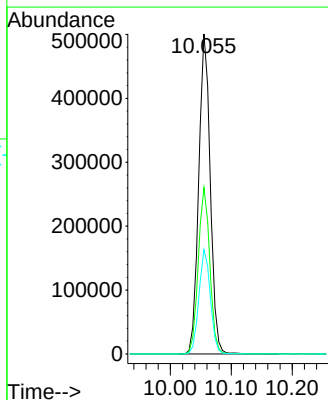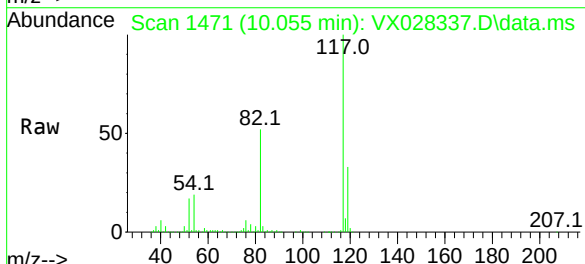







#64
Tetrachloroethene
Concen: 2.505 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL

Tgt Ion:164 Resp: 12892




Ion	Ratio	Lower	Upper
164	100		
166	130.1	101.2	151.8
129	97.7	73.0	109.4
131	84.5	74.2	111.2

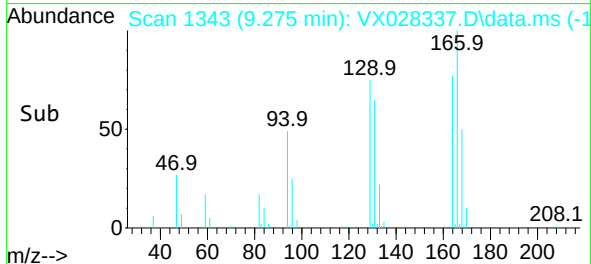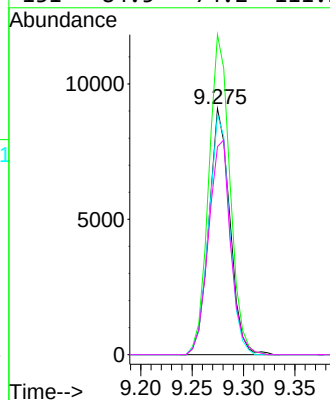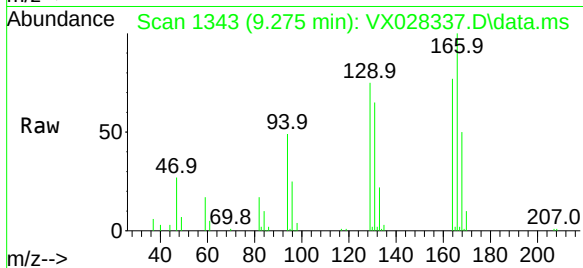


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion:152 Resp: 312575

Ion	Ratio	Lower	Upper
152	100		
115	57.5	37.5	112.7
150	155.2	0.0	338.2


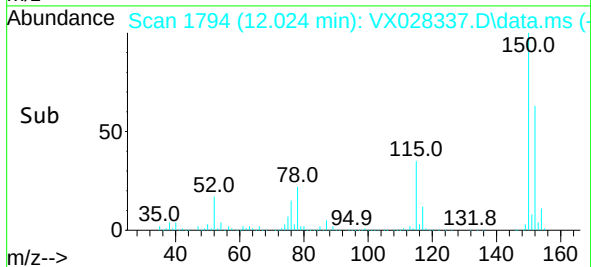
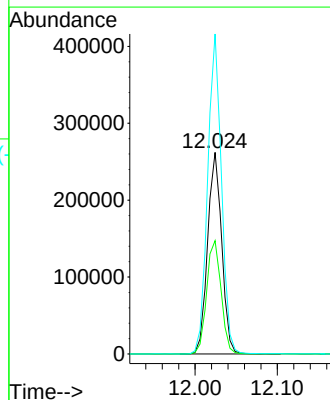
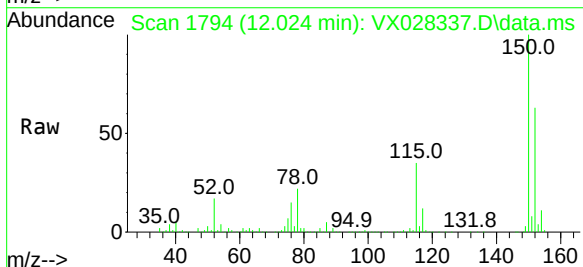


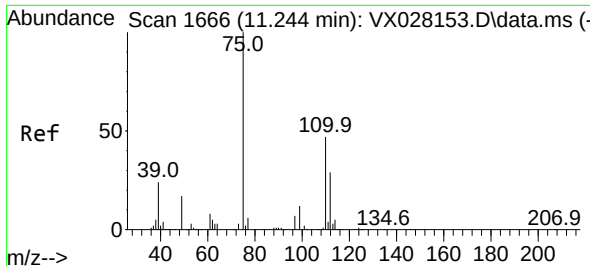

#76
1,2,3-Trichloropropane
Concen: 24.165 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31




Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATERDL


Tgt Ion: 75 Resp: 148656
Ion Ratio Lower Upper
75 100
77 1.0 19.4 58.2#

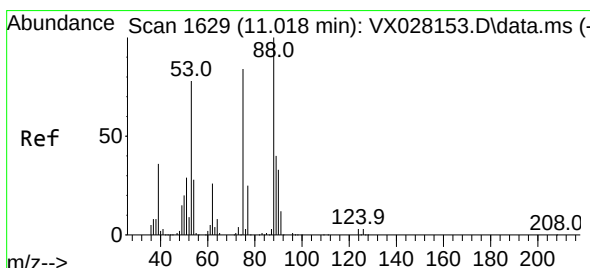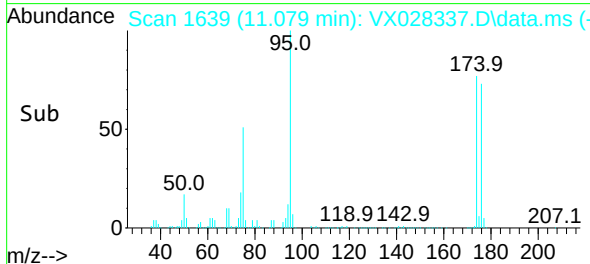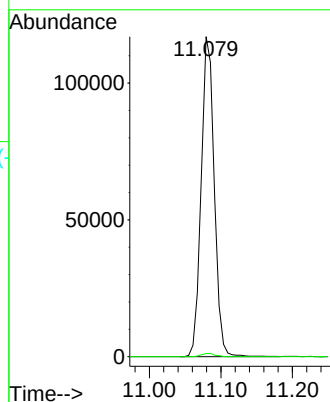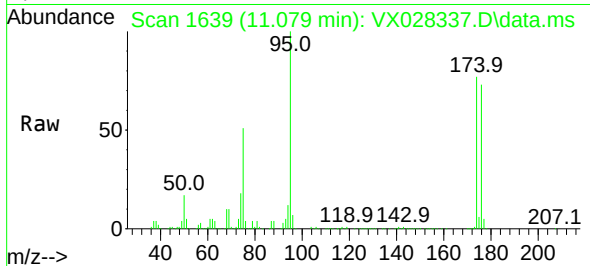

#81
trans-1,4-Dichloro-2-butene
Concen: 71.812 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX028337.D
Acq: 25 Apr 2022 19:31

Tgt Ion: 75 Resp: 148656
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#


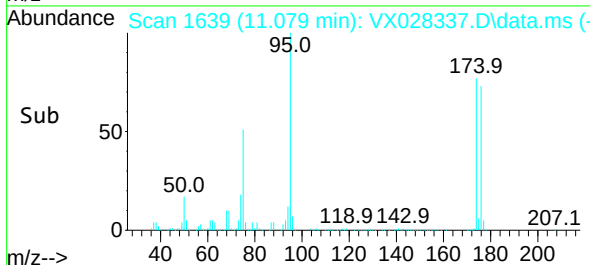
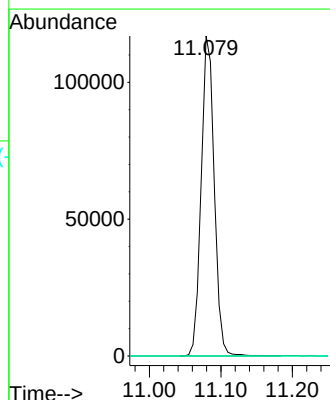
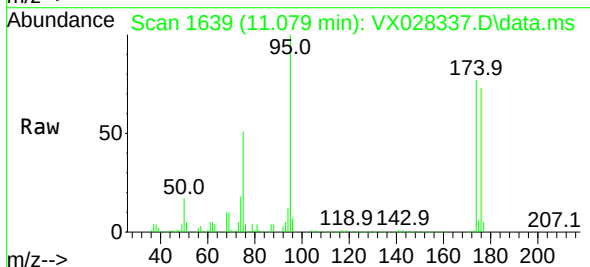




#90
 Hexachloroethane
 Concen: 1.841 ug/l
 RT: 12.695 min Scan# 1904
 Delta R.T. 0.153 min
 Lab File: VX028337.D
 Acq: 25 Apr 2022 19:31

Instrument :
 MSVOA_X
 ClientSampleId :
 PURGE-WATERDL

Tgt Ion:117 Resp: 100
 Ion Ratio Lower Upper
 117 100
 201 0.0 39.5 118.5#

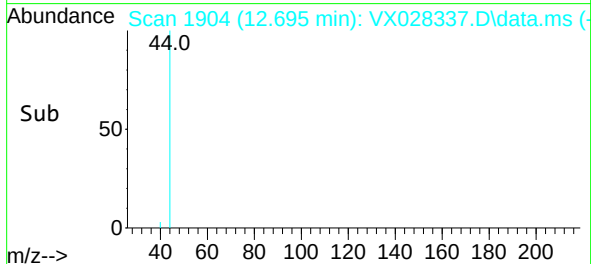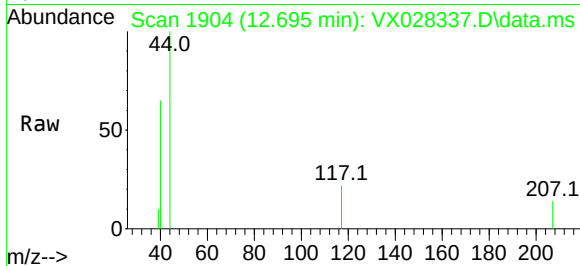

#91
 1,2-Dichlorobenzene
 Concen: 0.808 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.000 min
 Lab File: VX028337.D
 Acq: 25 Apr 2022 19:31

Tgt Ion:146 Resp: 8435
 Ion Ratio Lower Upper
 146 100
 111 42.6 21.0 63.0
 148 68.0 32.6 97.7

