

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042522\
 Data File : VX028327.D
 Acq On : 25 Apr 2022 15:27
 Operator : JC/MD
 Sample : N2557-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PURGE-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Title : SW846 8260

Signal : TIC: VX028327.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.136	165	172	193	rVB	238560	406647	6.45%	1.312%
2	2.331	193	204	218	rBV2	508976	1039347	16.49%	3.354%
3	3.611	403	414	433	rBV	173912	412825	6.55%	1.332%
4	4.489	546	558	583	rBV	2101391	5653936	89.70%	18.247%
5	5.391	689	706	720	rBV	429774	1284210	20.37%	4.145%
6	5.556	720	733	751	rVB	387182	1128828	17.91%	3.643%
7	5.958	789	799	812	rBV	283335	749544	11.89%	2.419%
8	6.763	920	931	947	rBV	621587	1454655	23.08%	4.695%
9	7.129	979	991	1006	rBV	2935850	6303119	100.00%	20.342%
10	8.653	1233	1241	1246	rBV	1496549	2311220	36.67%	7.459%
11	8.720	1246	1252	1269	rVB	2755283	4148704	65.82%	13.389%
12	9.275	1336	1343	1353	rVB	374445	535930	8.50%	1.730%
13	10.055	1464	1471	1482	rBV	1413572	1872101	29.70%	6.042%
14	11.079	1634	1639	1657	rBV	1272326	1642409	26.06%	5.301%
15	12.024	1788	1794	1801	rBV	1536694	1862687	29.55%	6.012%
16	12.335	1839	1845	1853	rVB	141096	178864	2.84%	0.577%




Sum of corrected areas: 30985026

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042522\
Data File : VX028327.D
Acq On : 25 Apr 2022 15:27
Operator : JC/MD
Sample : N2557-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

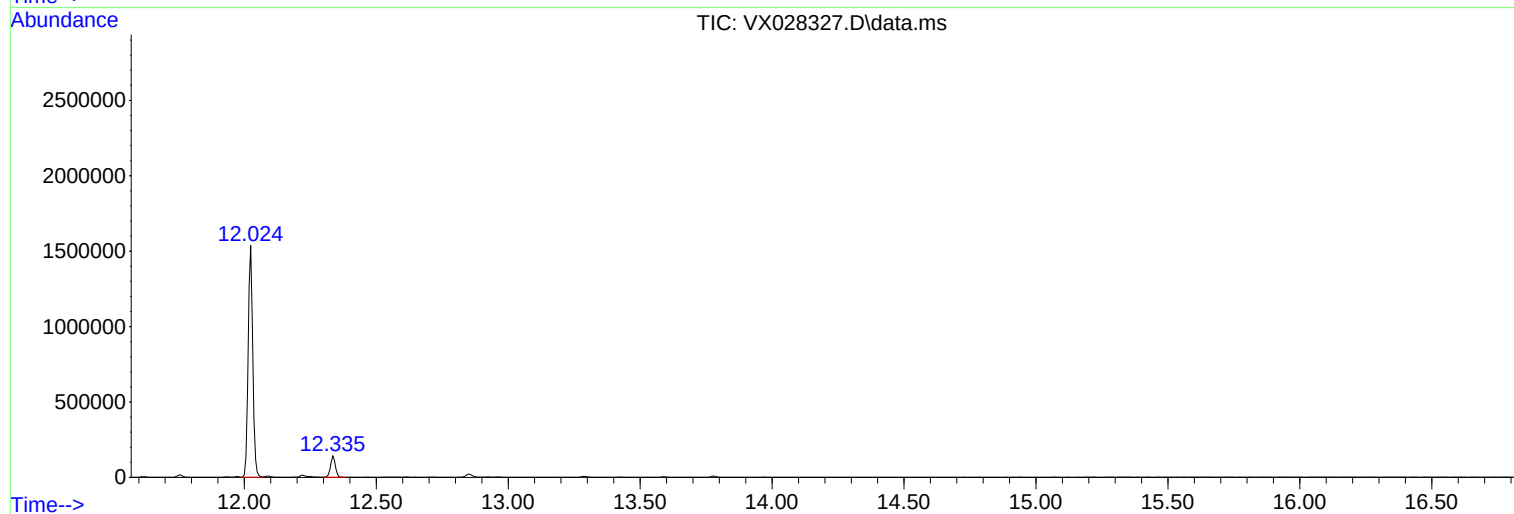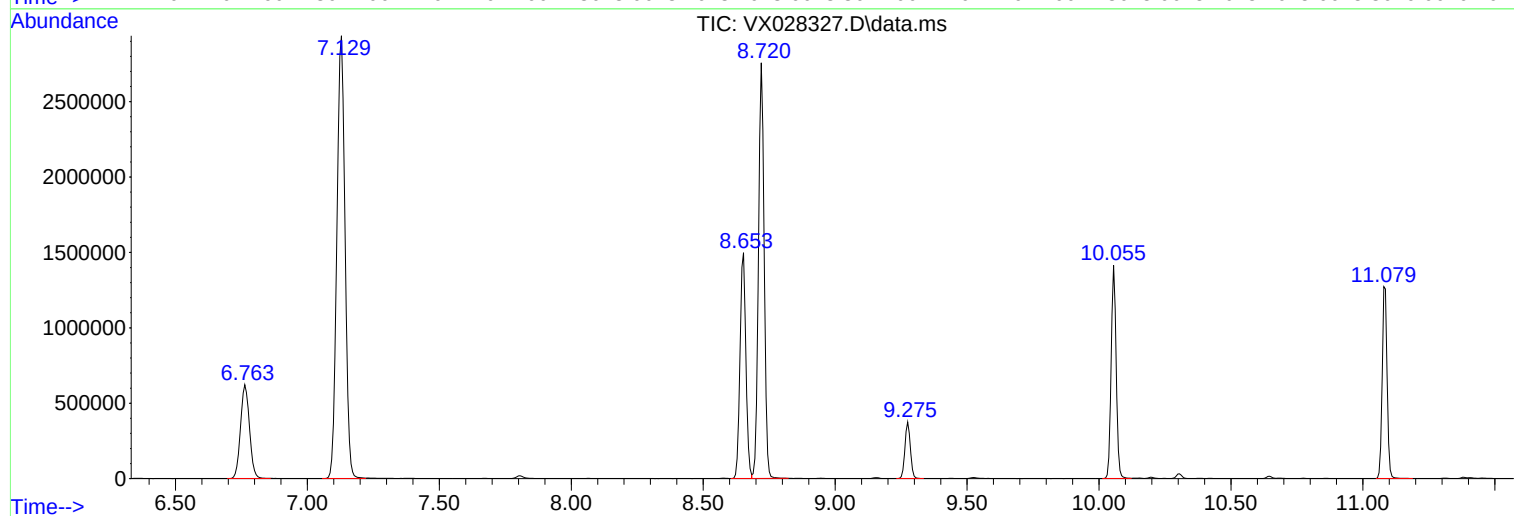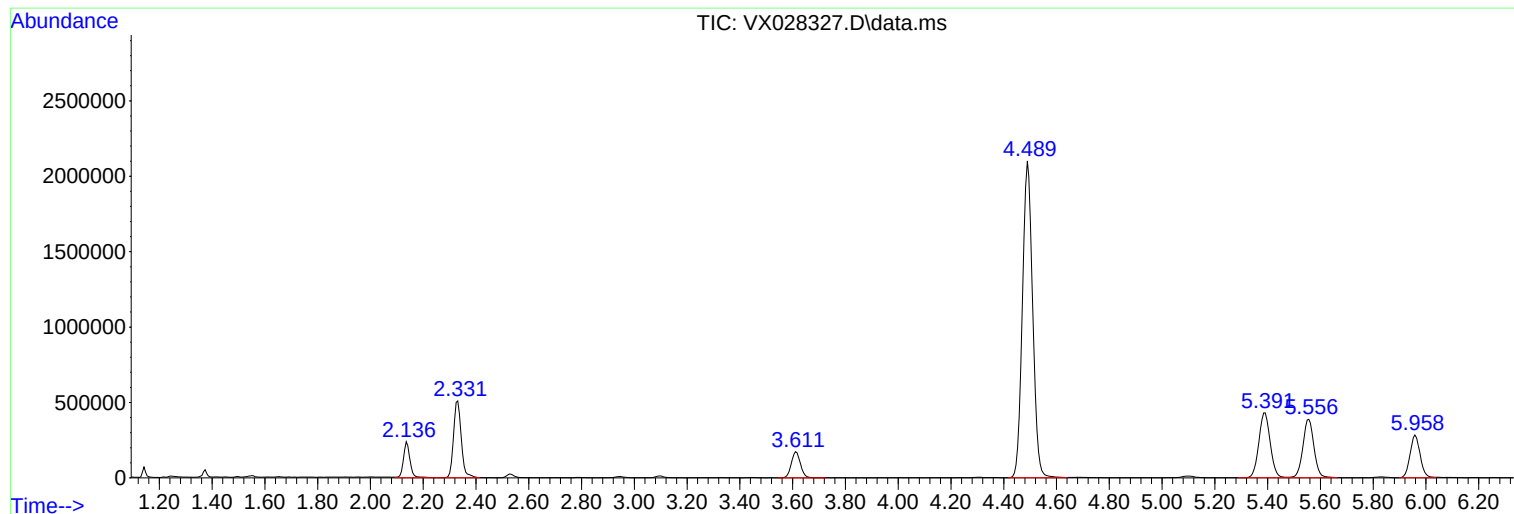

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042522\
Data File : VX028327.D
Acq On : 25 Apr 2022 15:27
Operator : JC/MD
Sample : N2557-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATER









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,2-dichloro-1,1,2-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.136	18.01 ug/l	406647	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	91
2			1-Butyne, 3,3-dimethyl-	82	C6H10	000917-92-0	10
3			Cyclopropane, 1,2-dimethyl-3-met...	82	C6H10	062338-02-7	10
4			1,4-Pentadiene, 3-methyl-	82	C6H10	001115-08-8	9
5			Methyl 2-butynoate	98	C5H6O2	023326-27-4	9

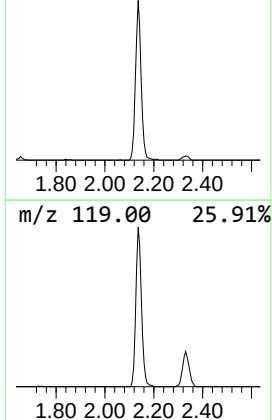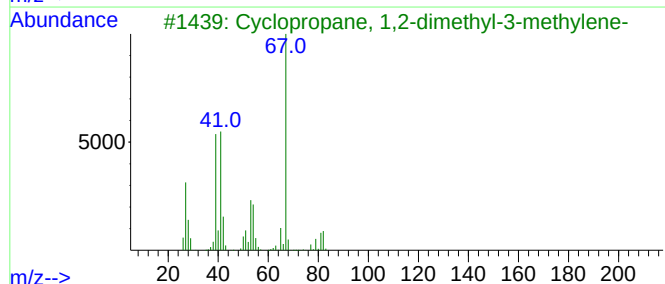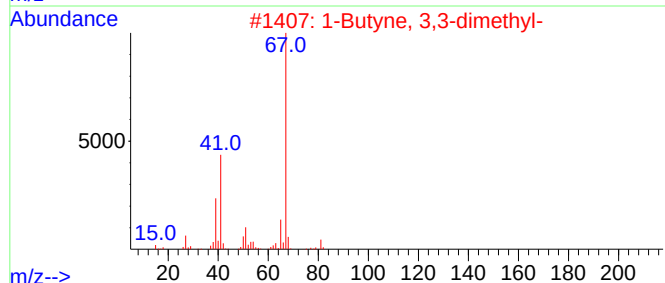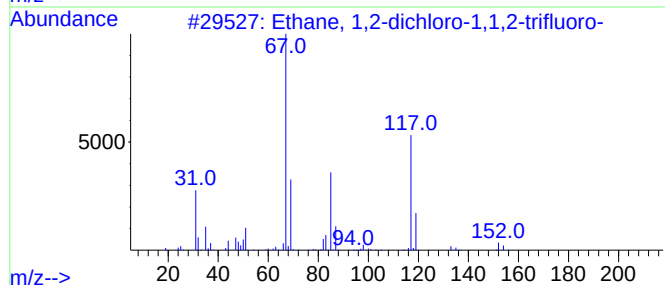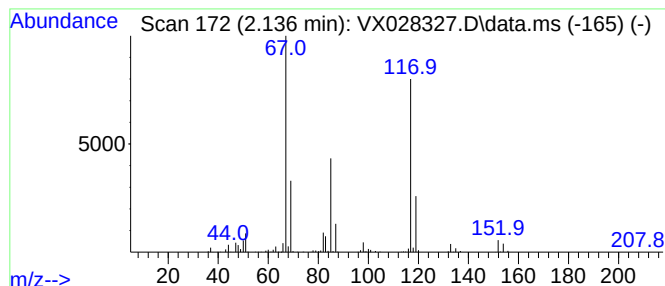

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042522\
Data File : VX028327.D
Acq On : 25 Apr 2022 15:27
Operator : JC/MD
Sample : N2557-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PURGE-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,2-dic...	2.136	18.0	ug/l	406647	1	5.556	1128830	50.0