

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042619\
 Data File : VX009190.D
 Acq On : 26 Apr 2019 15:23
 Operator : JC/SP
 Sample : K2591-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Apr 27 05:32:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 17 06:47:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	211994	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	338551	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	295210	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	125527	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	138288	46.29	ug/l	0.00
Spiked Amount			Recovery	=	92.58%	
35) Dibromofluoromethane	5.50	113	101985	46.94	ug/l	0.00
Spiked Amount			Recovery	=	93.88%	
50) Toluene-d8	8.71	98	425579	49.11	ug/l	0.00
Spiked Amount			Recovery	=	98.22%	
62) 4-Bromofluorobenzene	11.13	95	140329	45.88	ug/l	0.00
Spiked Amount			Recovery	=	91.76%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042619\
Data File : VX009190.D
Acq On : 26 Apr 2019 15:23
Operator : JC/SP
Sample : K2591-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Apr 27 05:32:16 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 17 06:47:58 2019
Response via : Initial Calibration

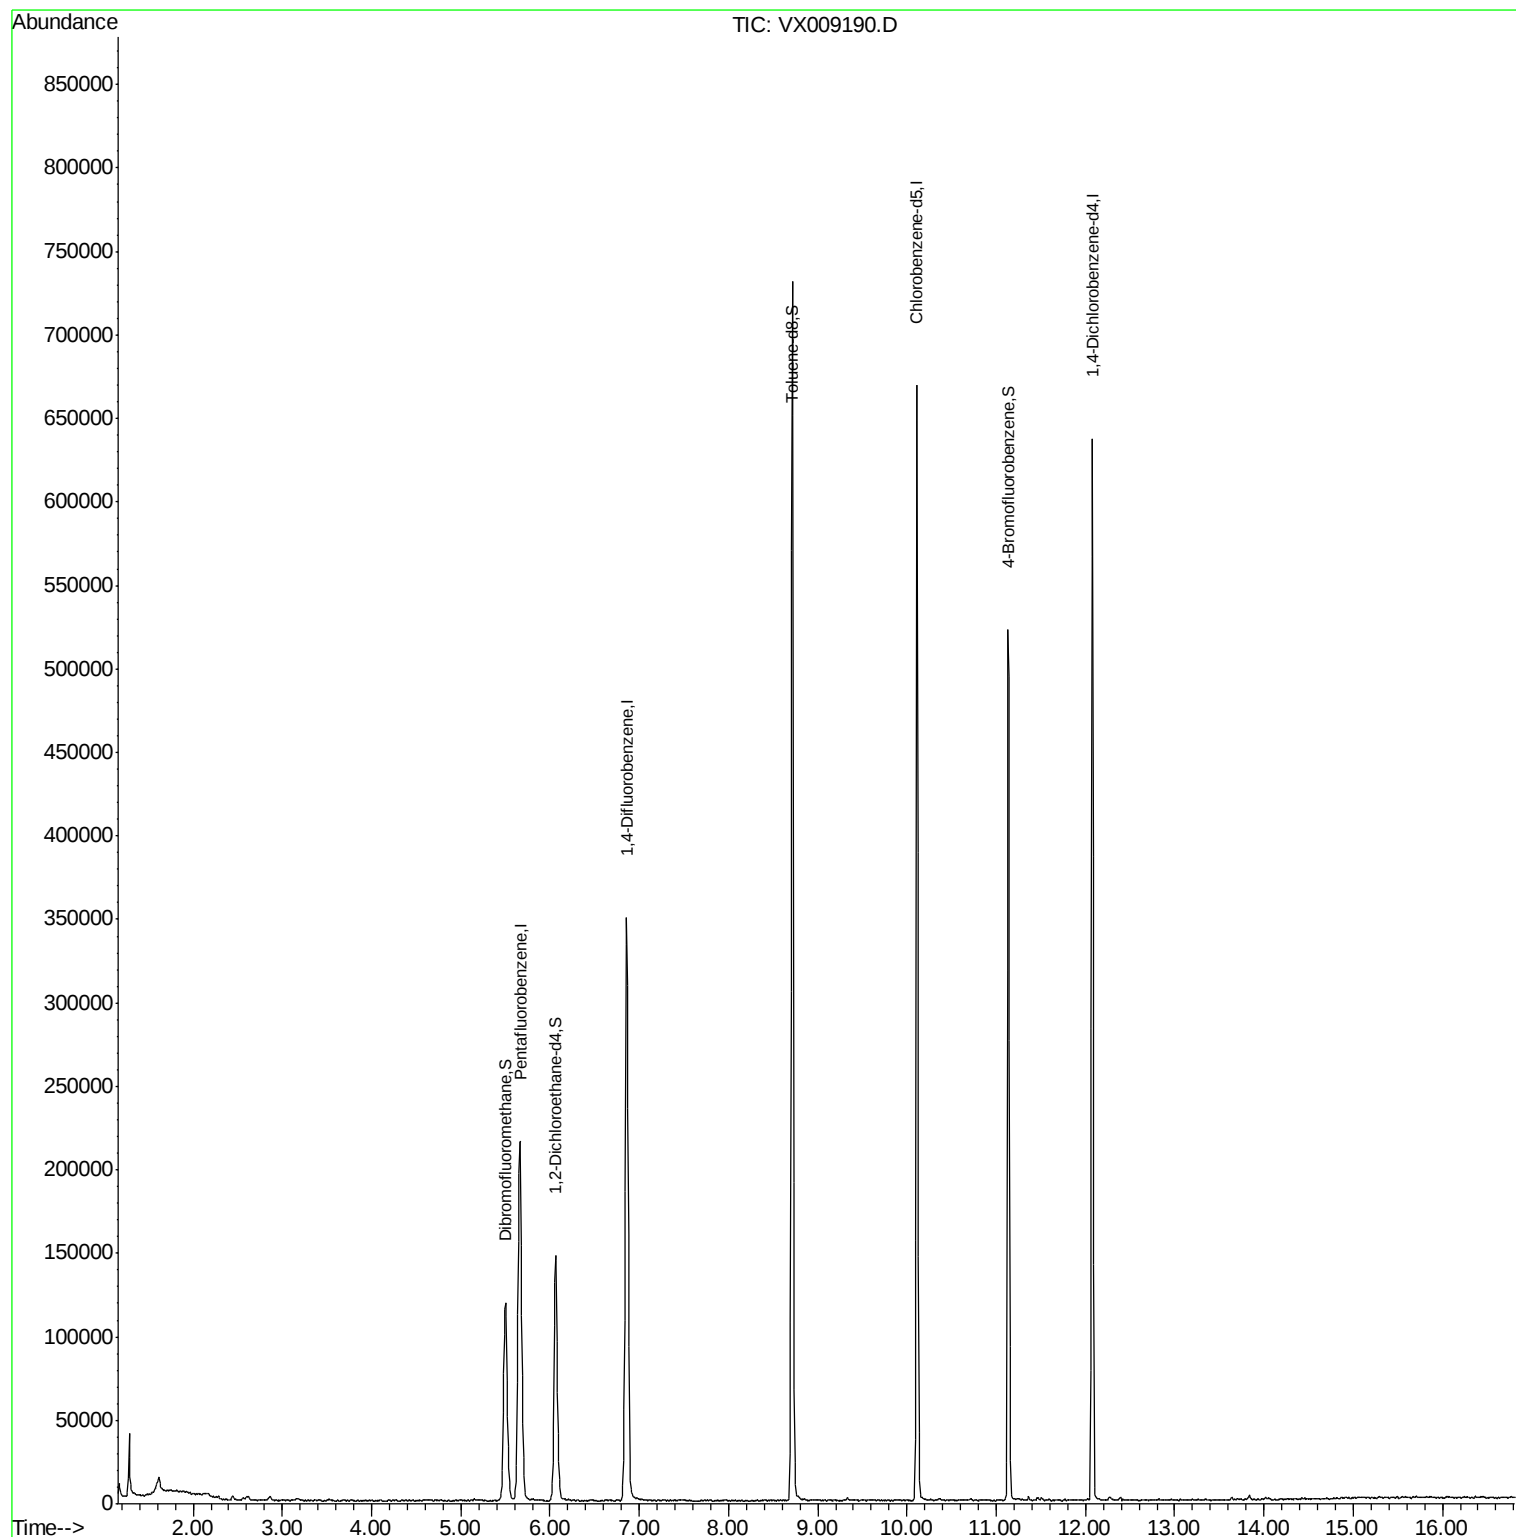

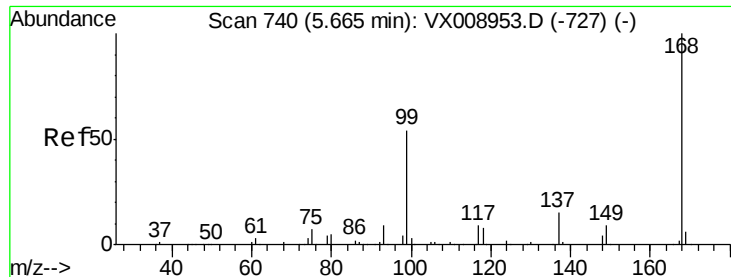

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX009190.D

Acq: 26 Apr 2019 15:23

Instrument :

MSVOA_X

ClientSampleId :


STORAGE-BLANK-SOIL-REF-6

Tot Ion:168 Resp: 211994

Ion Ratio Lower Upper

168 100

99 55.5 43.0 64.6

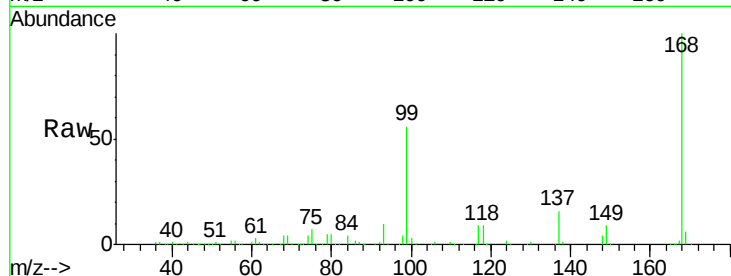

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80

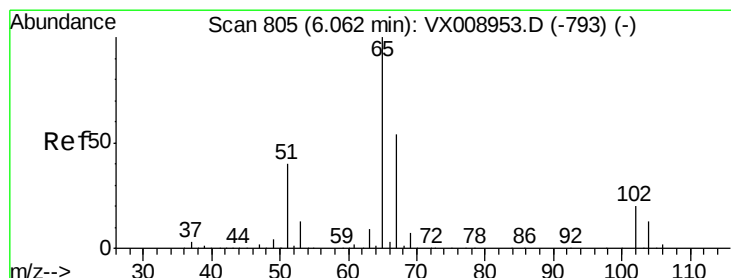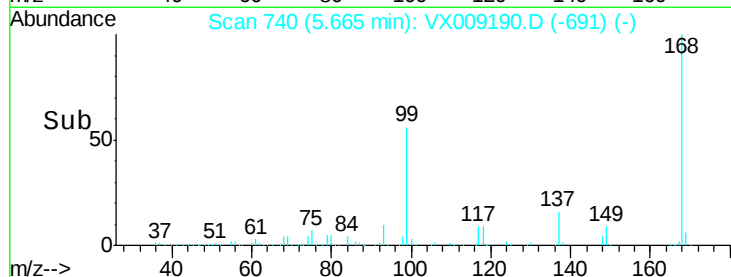

#33

1,2-Dichloroethane-d4

Concen: 46.287 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.01 min

Lab File: VX009190.D


Acq: 26 Apr 2019 15:23

Tgt Ion: 65 Resp: 138288

Ion Ratio Lower Upper

65 100

67 54.2 0.0 108.6

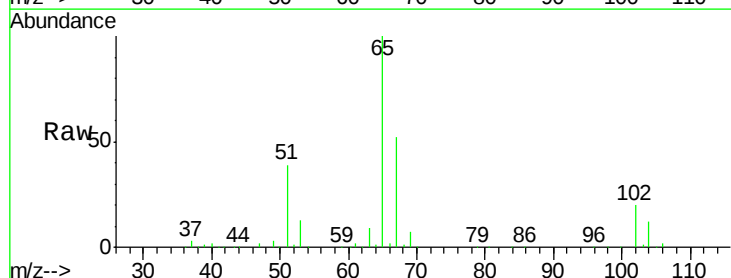

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

60000

50000

40000


30000


20000

10000

0

Time--> 5.90 6.00 6.10 6.20

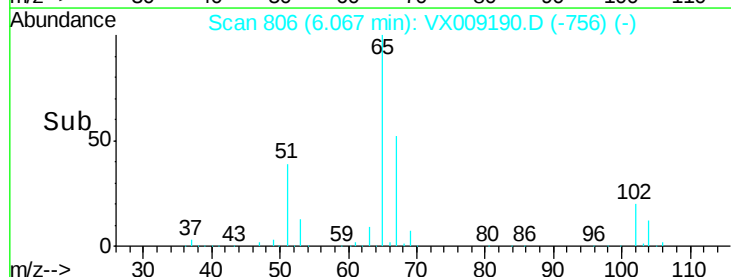


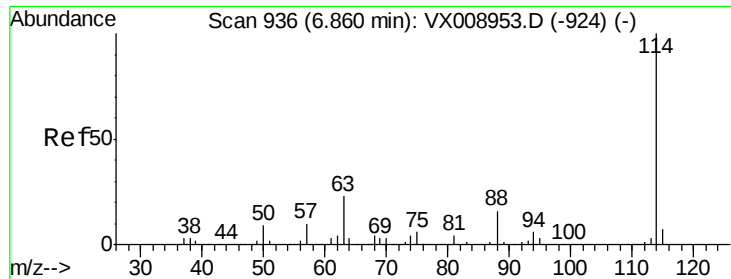


#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX009190.D
 Acq: 26 Apr 2019 15:23

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6



Tot Ion	Ratio	Lower	Upper
114	100		
63	22.5	0.0	46.0
88	16.6	0.0	32.6

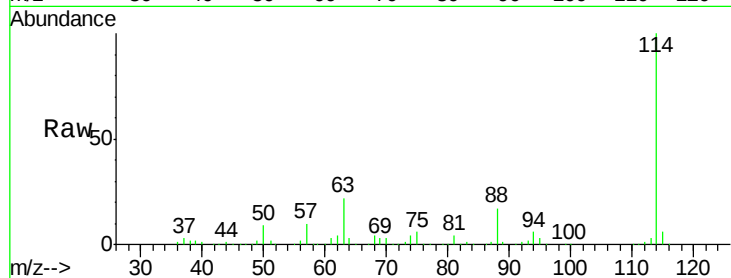

Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX
 Ion 87.90 (87.60 to 88.60): VX

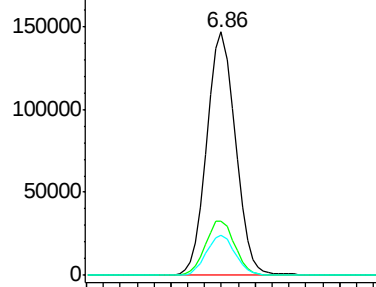


Time--> 6.70 6.80 6.90 7.00

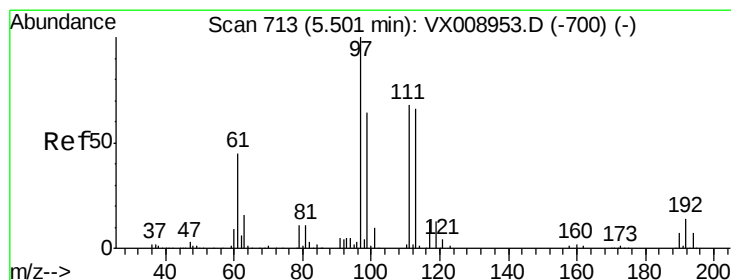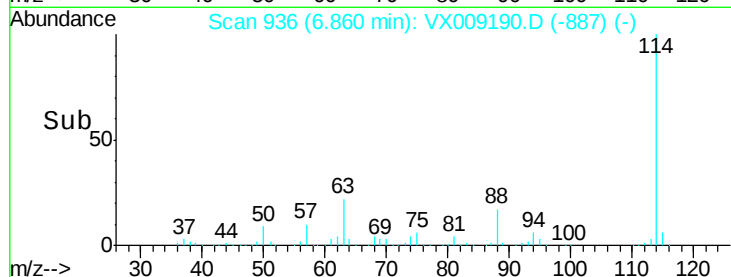


#35
 Dibromofluoromethane
 Concen: 46.938 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX009190.D
 Acq: 26 Apr 2019 15:23


Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.5	82.9	124.3
192	21.4	17.4	26.0

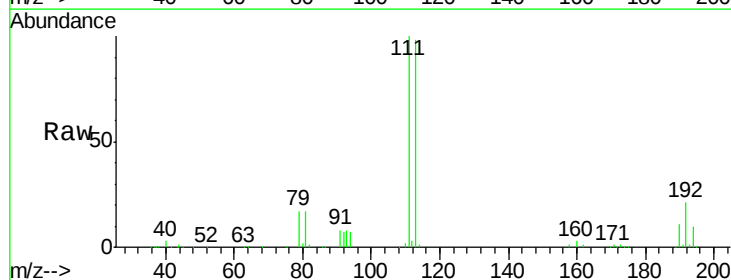


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

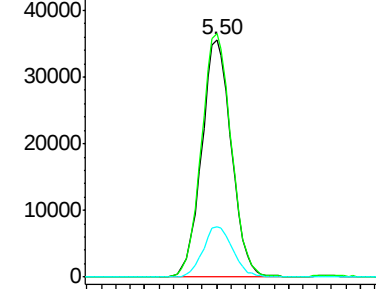

Time--> 5.40 5.50 5.60 5.70




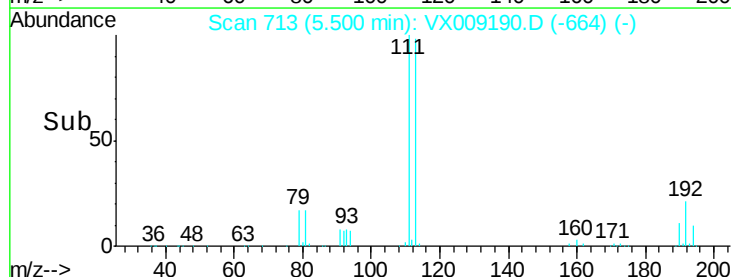


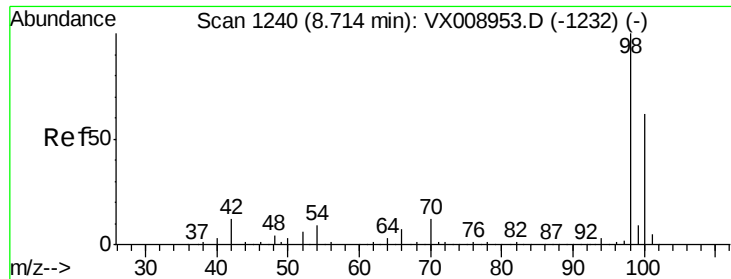

#50
Toluene-d8
Concen: 49.115 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX009190.D
Acq: 26 Apr 2019 15:23




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tot Ion: 98 Resp: 425579
Ion Ratio Lower Upper
98 100
100 63.8 51.4 77.2

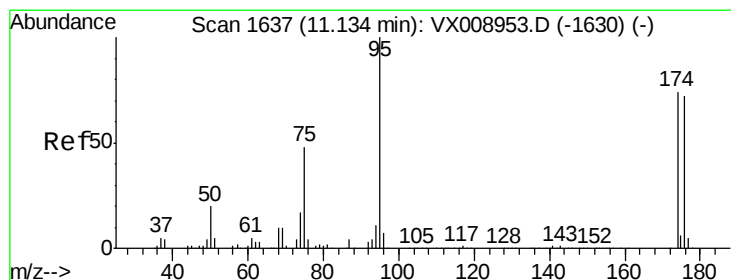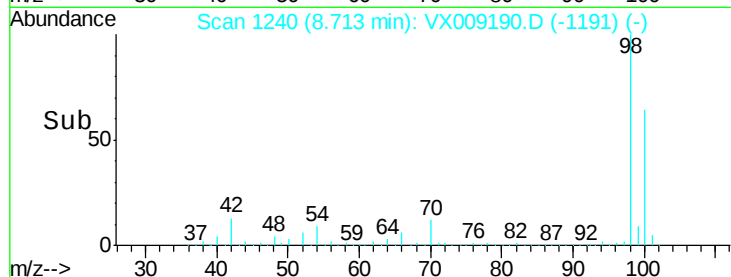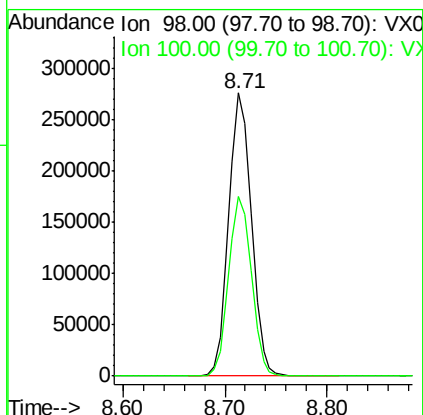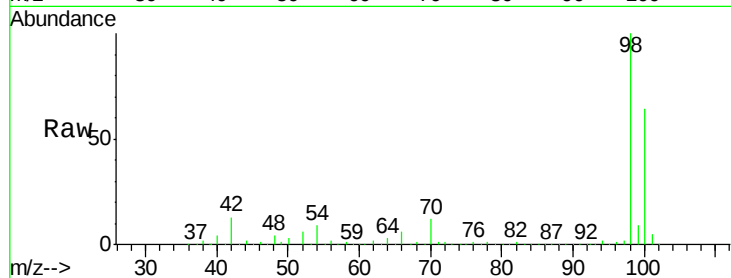

#62
4-Bromofluorobenzene
Concen: 45.878 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX009190.D
Acq: 26 Apr 2019 15:23

Tgt Ion: 95 Resp: 140329
Ion Ratio Lower Upper
95 100
174 81.3 0.0 159.6
176 77.8 0.0 154.8

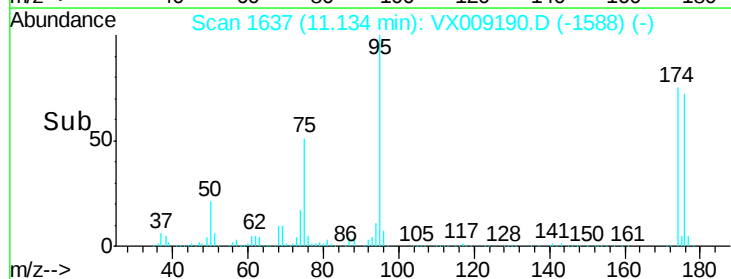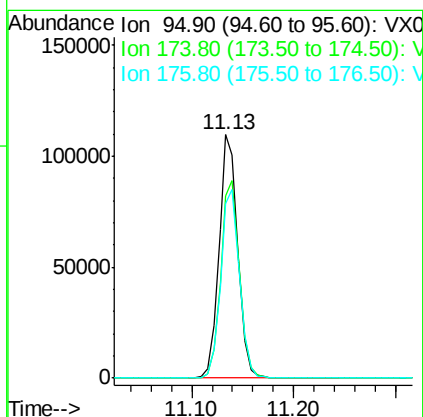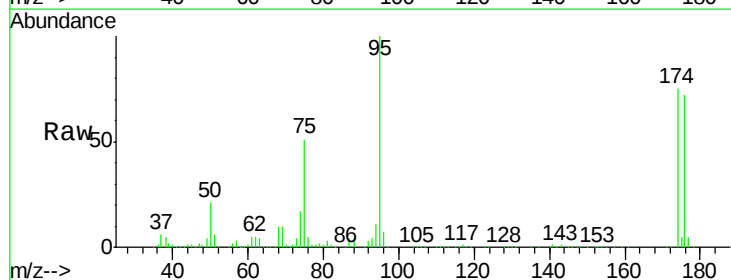


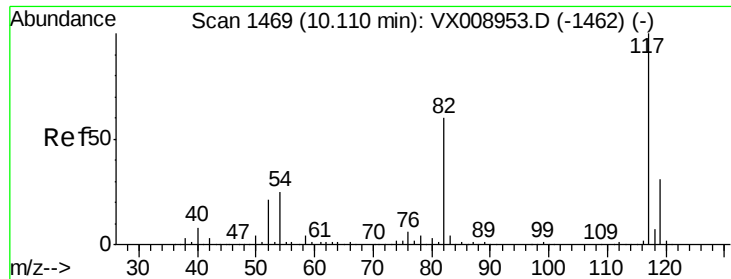




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.01 min
Lab File: VX009190.D
Acq: 26 Apr 2019 15:23

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tot Ion:117 Resp: 295210
Ion Ratio Lower Upper
117 100
82 57.9 48.2 72.4
119 32.8 25.0 37.6

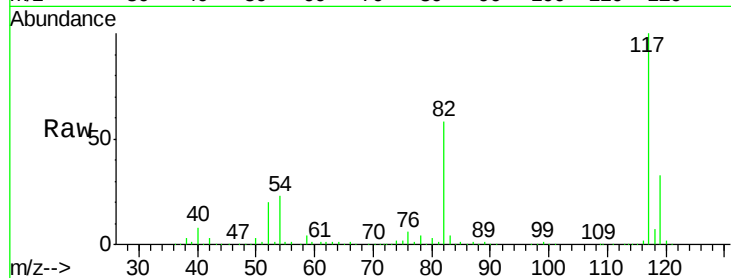


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

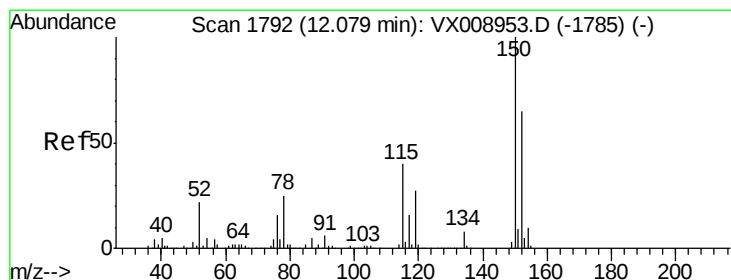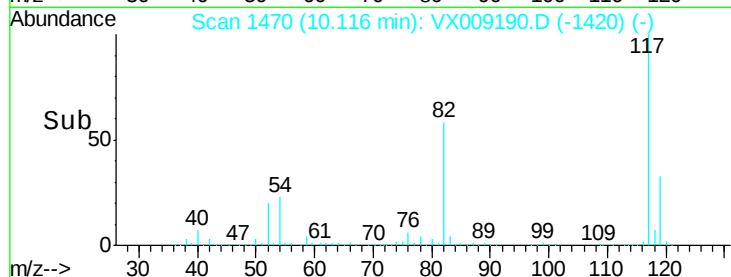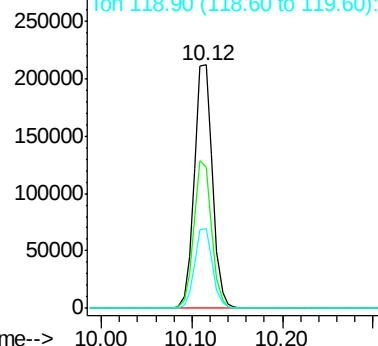

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX009190.D
Acq: 26 Apr 2019 15:23

Tgt Ion:152 Resp: 125527
Ion Ratio Lower Upper
152 100
115 59.0 41.4 124.2
150 155.5 0.0 349.8

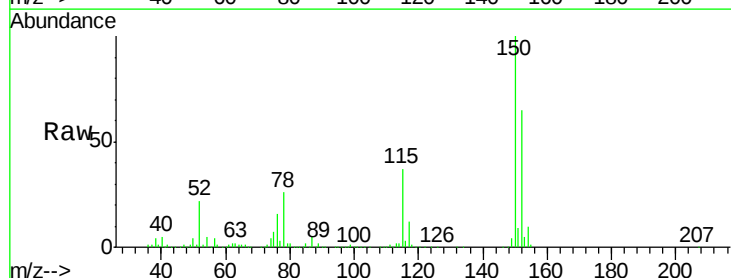

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

