

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042619\
 Data File : VX009187.D
 Acq On : 26 Apr 2019 14:13
 Operator : JC/SP
 Sample : K2565-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S81-0105

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	17	20	23	rBV	23483	32395	2.04%	0.162%
2	1.318	23	27	35	rVV2	35834	116343	7.33%	0.583%
3	1.788	99	104	113	rVB	82633	126790	7.99%	0.635%
4	2.001	134	139	149	rVB	75663	121297	7.64%	0.607%
5	2.391	196	203	208	rBV2	17543	35405	2.23%	0.177%
6	2.842	269	277	280	rBV	36194	74399	4.69%	0.373%
7	2.891	280	285	289	rVV	86665	157137	9.90%	0.787%
8	3.172	320	331	342	rBV	101191	230870	14.54%	1.156%
9	3.525	380	389	403	rVB	68043	158786	10.00%	0.795%
10	4.312	508	518	524	rBV2	11828	33890	2.13%	0.170%
11	4.403	524	533	546	rVB	127057	371544	23.40%	1.861%
12	4.598	557	565	574	rVB	10207	31107	1.96%	0.156%
13	5.501	701	713	719	rBV	120208	344220	21.68%	1.724%
14	5.580	719	726	733	rVV2	100761	316671	19.95%	1.586%
15	5.659	733	739	748	rVB	180449	474180	29.87%	2.375%
16	5.933	769	784	796	rBV4	67074	218612	13.77%	1.095%
17	6.061	796	805	814	rVV	149839	388711	24.48%	1.947%
18	6.141	814	818	827	rVV2	16291	44113	2.78%	0.221%
19	6.263	829	838	846	rVV3	33856	121045	7.62%	0.606%
20	6.354	846	853	862	rVV4	64252	199795	12.58%	1.001%
21	6.458	862	870	883	rVB2	49351	141040	8.88%	0.706%
22	6.860	925	936	946	rBV	342538	814616	51.31%	4.080%
23	7.464	1020	1035	1047	rBV	315756	740817	46.66%	3.710%
24	7.732	1074	1079	1088	rVB	34363	67580	4.26%	0.338%
25	7.848	1090	1098	1107	rBV3	23822	51398	3.24%	0.257%
26	8.055	1122	1132	1143	rVB3	41204	122058	7.69%	0.611%
27	8.177	1144	1152	1160	rBV	61511	131472	8.28%	0.658%
28	8.384	1182	1186	1192	rVB2	22463	41530	2.62%	0.208%
29	8.500	1201	1205	1209	rBV2	20473	34039	2.14%	0.170%
30	8.665	1225	1232	1235	rBV2	84528	156701	9.87%	0.785%
31	8.713	1235	1240	1247	rVV	753492	1190034	74.95%	5.960%
32	8.787	1247	1252	1256	rVV	24498	42525	2.68%	0.213%
33	8.841	1256	1261	1265	rVV	39225	68053	4.29%	0.341%
34	8.908	1269	1272	1278	rVB2	26223	42018	2.65%	0.210%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042619\
 Data File : VX009187.D
 Acq On : 26 Apr 2019 14:13
 Operator : JC/SP
 Sample : K2565-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S81-0105

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
 Title : SW846 8260

35	9.043	1288	1294	1301	rVB	78379	133331	8.40%	0.668%
36	9.165	1306	1314	1319	rBV	41759	69695	4.39%	0.349%
37	9.573	1373	1381	1385	rBV3	35645	66859	4.21%	0.335%
38	9.622	1385	1389	1394	rVB	82208	109758	6.91%	0.550%
39	9.677	1394	1398	1402	rBV	66094	94010	5.92%	0.471%
40	9.890	1426	1433	1441	rBV4	21071	48388	3.05%	0.242%
41	10.109	1464	1469	1476	rVV	683668	916062	57.70%	4.588%
42	10.183	1476	1481	1486	rVV	36193	61611	3.88%	0.309%
43	10.250	1486	1492	1497	rVV	468950	624710	39.35%	3.129%
44	10.359	1501	1510	1516	rVV	289708	465518	29.32%	2.331%
45	10.640	1549	1556	1560	rBV4	31698	68722	4.33%	0.344%
46	10.695	1560	1565	1578	rVB	1195709	1587704	100.00%	7.951%
47	10.835	1584	1588	1593	rVB	52228	69459	4.37%	0.348%
48	10.914	1596	1601	1605	rBV3	27550	46508	2.93%	0.233%
49	11.018	1613	1618	1622	rBV	48812	65888	4.15%	0.330%
50	11.134	1632	1637	1642	rBV	541891	701662	44.19%	3.514%
51	11.274	1657	1660	1669	rVB2	30160	45128	2.84%	0.226%
52	11.359	1669	1674	1678	rBV	55510	74194	4.67%	0.372%
53	11.432	1682	1686	1688	rBV	66852	95044	5.99%	0.476%
54	11.506	1693	1698	1701	rVB	27663	36465	2.30%	0.183%
55	11.664	1719	1724	1733	rBV	601890	744978	46.92%	3.731%
56	11.804	1743	1747	1752	rVB	407961	483203	30.43%	2.420%
57	11.945	1767	1770	1774	rVB	30130	37320	2.35%	0.187%
58	12.024	1775	1783	1786	rBV	91042	114413	7.21%	0.573%
59	12.079	1786	1792	1797	rVV	634742	842465	53.06%	4.219%
60	12.140	1797	1802	1808	rVB	668887	798449	50.29%	3.999%
61	12.231	1813	1817	1823	rVB	28285	40162	2.53%	0.201%
62	12.298	1823	1828	1830	rBV2	207890	269518	16.98%	1.350%
63	12.323	1830	1832	1836	rVV	119765	125653	7.91%	0.629%
64	12.365	1836	1839	1848	rVB3	90174	135176	8.51%	0.677%
65	12.457	1849	1854	1859	rBV3	69428	98356	6.19%	0.493%
66	12.518	1859	1864	1869	rVB	188604	232208	14.63%	1.163%
67	12.585	1869	1875	1877	rBV	76005	102556	6.46%	0.514%
68	12.609	1877	1879	1883	rVV	61562	68001	4.28%	0.341%
69	12.664	1884	1888	1891	rVV	78401	100524	6.33%	0.503%
70	12.700	1891	1894	1898	rVV2	36939	47126	2.97%	0.236%
71	12.755	1898	1903	1911	rVV4	125188	269275	16.96%	1.349%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042619\
 Data File : VX009187.D
 Acq On : 26 Apr 2019 14:13
 Operator : JC/SP
 Sample : K2565-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S81-0105

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
 Title : SW846 8260

72	12.853	1915	1919	1921	rVV2	32183	46883	2.95%	0.235%
73	12.902	1923	1927	1931	rVB2	142344	182948	11.52%	0.916%
74	12.975	1931	1939	1943	rBV	139830	203008	12.79%	1.017%
75	13.018	1943	1946	1952	rVB	93013	121063	7.63%	0.606%
76	13.078	1952	1956	1963	rVB3	42759	71603	4.51%	0.359%
77	13.194	1971	1975	1977	rBV2	51130	69217	4.36%	0.347%
78	13.219	1977	1979	1983	rVV2	32217	42734	2.69%	0.214%
79	13.261	1983	1986	1989	rVB4	23235	30923	1.95%	0.155%
80	13.304	1989	1993	1995	rBV	48150	60624	3.82%	0.304%
81	13.341	1995	1999	2004	rVV2	380751	538359	33.91%	2.696%
82	13.389	2004	2007	2011	rVV2	24437	37619	2.37%	0.188%
83	13.481	2017	2022	2029	rVB	136090	207285	13.06%	1.038%
84	13.560	2030	2035	2038	rBV3	25747	42307	2.66%	0.212%
85	13.597	2038	2041	2044	rVV	30793	39907	2.51%	0.200%
86	13.633	2044	2047	2053	rVV3	89420	176793	11.14%	0.885%
87	13.694	2055	2057	2059	rVV2	39864	52568	3.31%	0.263%
88	13.719	2059	2061	2066	rVB2	62407	77385	4.87%	0.388%
89	13.834	2077	2080	2087	rVB2	76163	137158	8.64%	0.687%
90	13.908	2087	2092	2097	rVB2	45480	78534	4.95%	0.393%
91	13.987	2097	2105	2109	rBV2	66265	108950	6.86%	0.546%
92	14.030	2109	2112	2116	rBV3	25353	34108	2.15%	0.171%
93	14.133	2124	2129	2132	rBV3	24969	39403	2.48%	0.197%
94	14.273	2147	2152	2158	rVB3	60779	117463	7.40%	0.588%
95	14.377	2165	2169	2173	rVV	27693	31707	2.00%	0.159%
96	14.432	2174	2178	2182	rVB	31349	39581	2.49%	0.198%
97	14.536	2191	2195	2204	rBV2	75557	115519	7.28%	0.579%
98	14.670	2214	2217	2219	rBV2	27037	33602	2.12%	0.168%
99	14.840	2241	2245	2249	rVV2	43563	67919	4.28%	0.340%
100	15.548	2356	2361	2366	rBV	20513	31462	1.98%	0.158%


Sum of corrected areas: 19967922

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042619\
Data File : VX009187.D
Acq On : 26 Apr 2019 14:13
Operator : JC/SP
Sample : K2565-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S81-0105

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

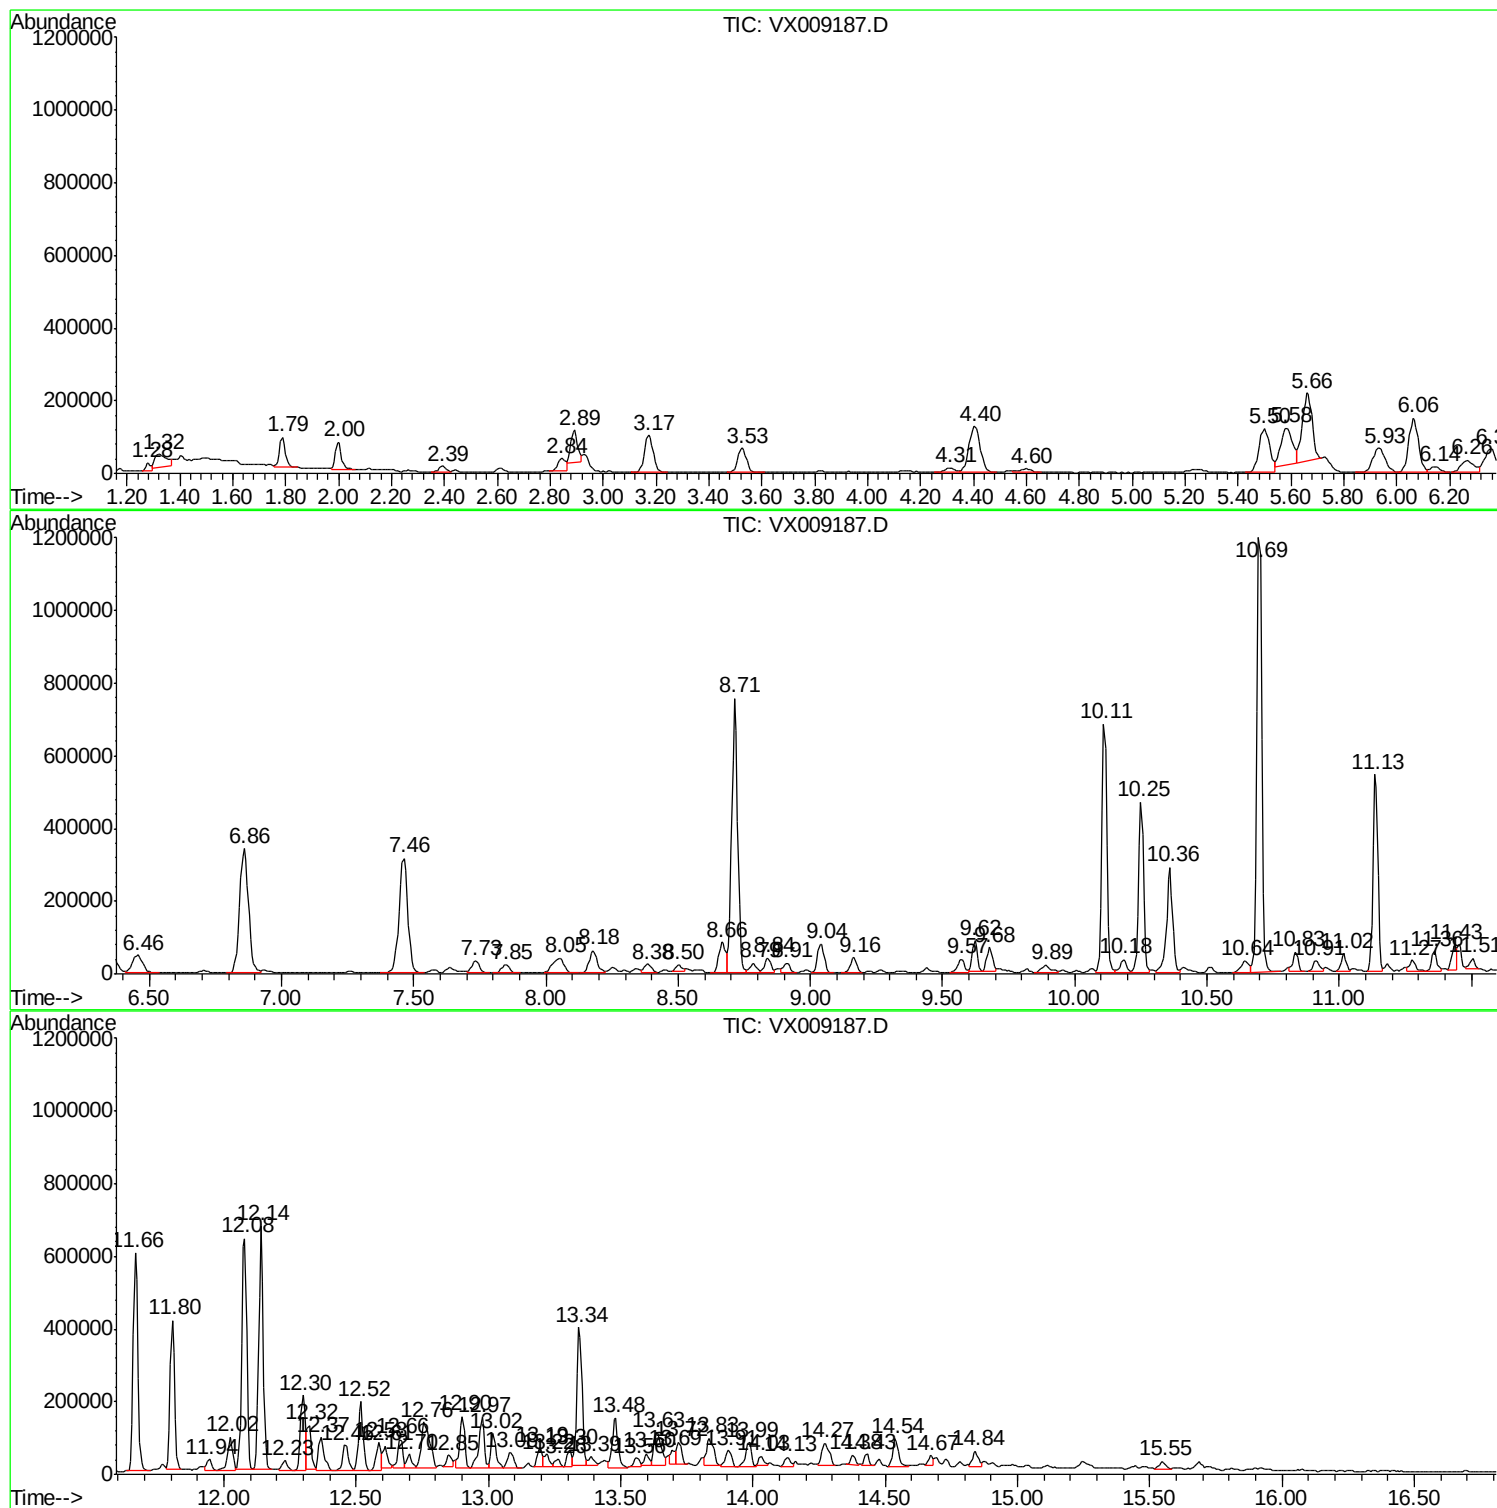

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX042619\
Data File : VX009187.D
Acq On : 26 Apr 2019 14:13
Operator : JC/SP
Sample : K2565-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S81-0105

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX042619\
Data File : VX009187.D
Acq On : 26 Apr 2019 14:13
Operator : JC/SP
Sample : K2565-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S81-0105

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X041519W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc