

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042622\
 Data File : VX028362.D
 Acq On : 26 Apr 2022 20:05
 Operator : JC/MD
 Sample : N2559-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-10D

Quant Time: Apr 27 02:08:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	434641	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	744298	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	741696	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	357682	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	310454	54.781	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 109.560%	
35) Dibromofluoromethane	5.391	113	282437	54.110	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 108.220%	
50) Toluene-d8	8.653	98	1054405	52.594	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 105.180%	
62) 4-Bromofluorobenzene	11.079	95	393047	51.275	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 102.560%	
Target Compounds						
						Qvalue
16) Acetone	2.386	43	21680	11.191	ug/l	# 85
20) Methylene Chloride	2.794	84	21376	5.084	ug/l	97
43) Isopropyl Acetate	6.342	43	30500	2.713	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042622\
Data File : VX028362.D
Acq On : 26 Apr 2022 20:05
Operator : JC/MD
Sample : N2559-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-10D

Quant Time: Apr 27 02:08:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




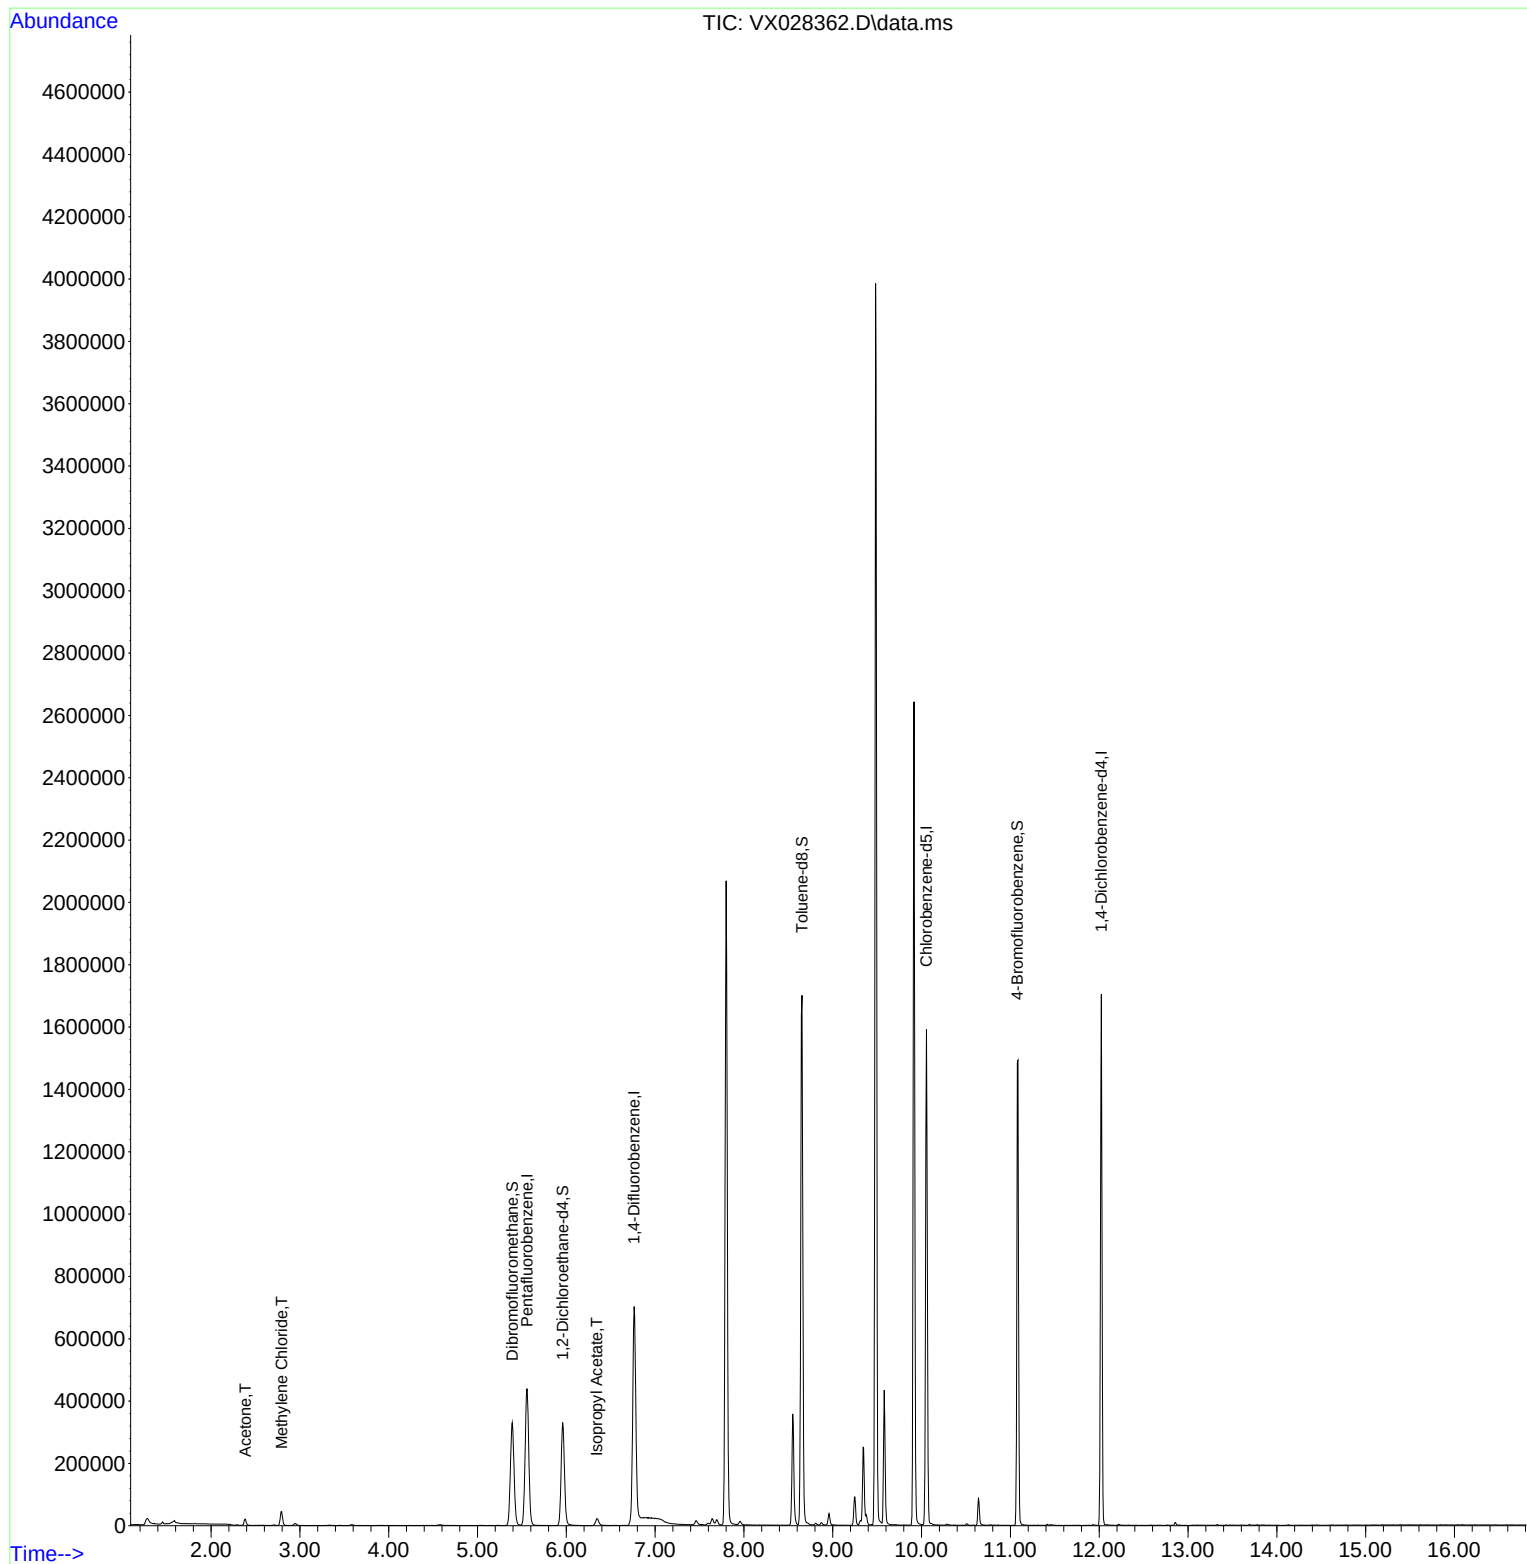




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05




Instrument :
MSVOA_X
ClientSampleId :
MH-10D


Tgt Ion:168 Resp: 434641
Ion Ratio Lower Upper
168 100
99 56.5 41.7 62.5

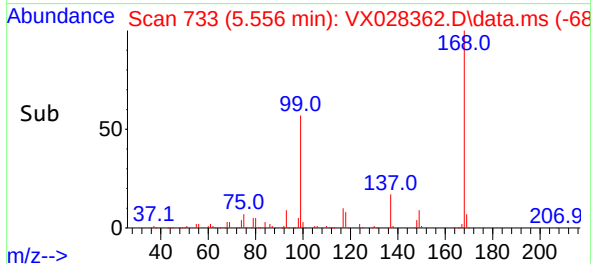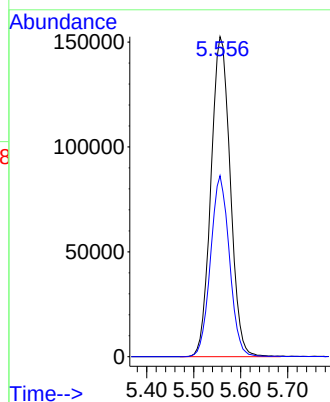

#16
Acetone
Concen: 11.191 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05

Tgt Ion: 43 Resp: 21680
Ion Ratio Lower Upper
43 100
58 27.0 28.8 43.2#

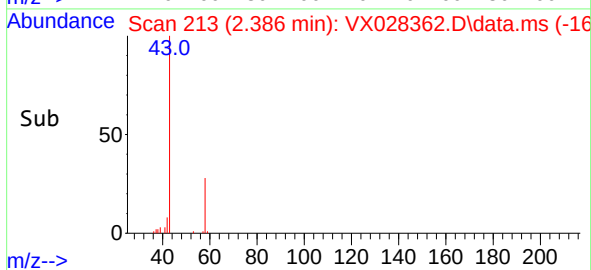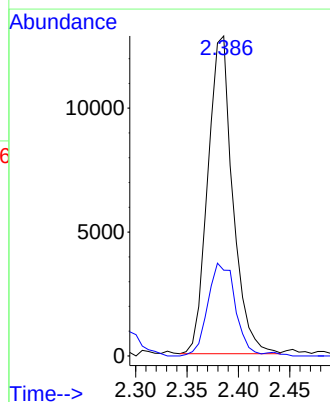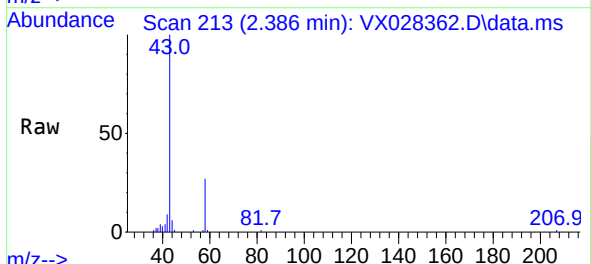




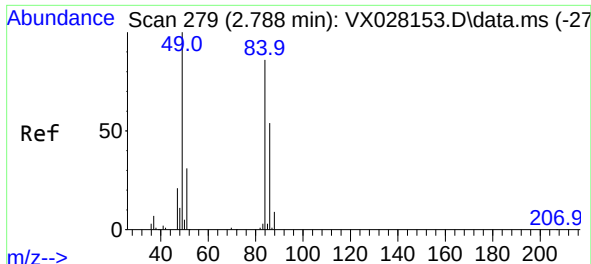


#20
Methylene Chloride
Concen: 5.084 ug/l
RT: 2.794 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05

Instrument :
MSVOA_X
ClientSampleId :
MH-10D

Tgt Ion: 84 Resp: 21376




Ion	Ratio	Lower	Upper
84	100		
49	102.8	85.5	128.3
51	29.1	26.6	39.8
86	63.8	51.5	77.3

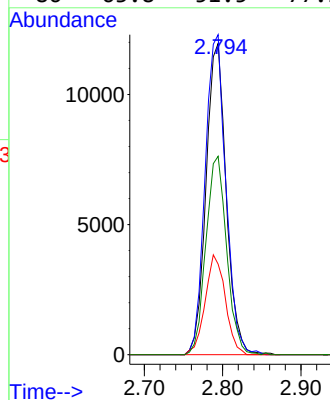


#33
1,2-Dichloroethane-d4
Concen: 54.781 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05

Tgt Ion: 65 Resp: 310454

Ion	Ratio	Lower	Upper
65	100		
67	51.3	0.0	107.4


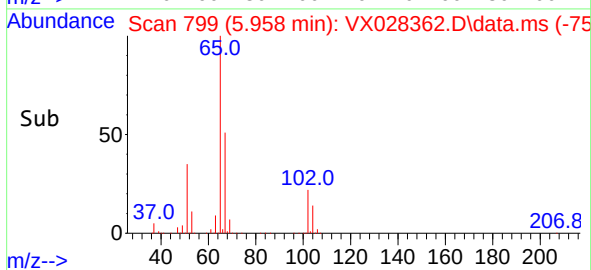
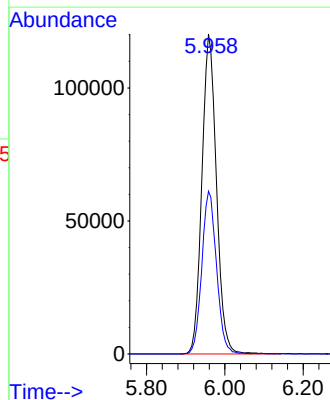
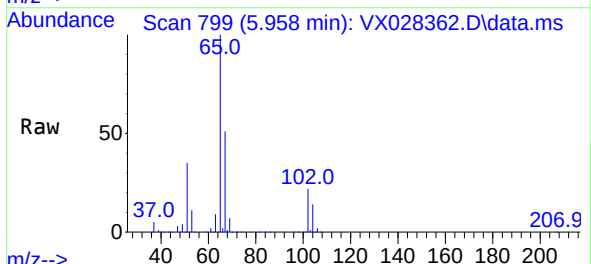




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05




Instrument :
MSVOA_X
ClientSampleId :
MH-10D


Tgt Ion:114 Resp: 744298
Ion Ratio Lower Upper
114 100
63 17.9 0.0 36.8
88 15.4 0.0 32.4

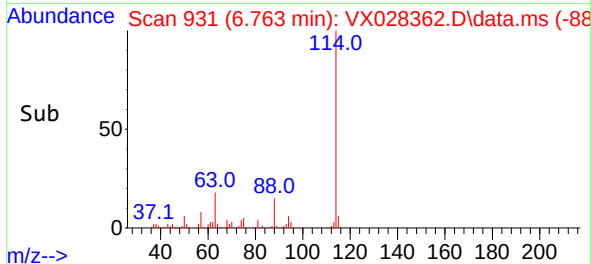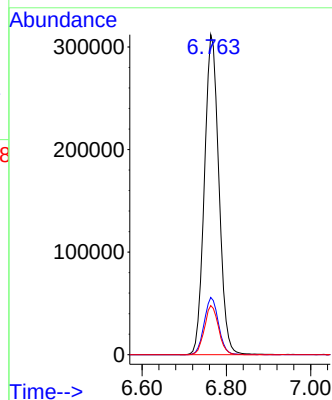

#35
Dibromofluoromethane
Concen: 54.110 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05

Tgt Ion:113 Resp: 282437
Ion Ratio Lower Upper
113 100
111 101.6 82.8 124.2
192 20.3 16.9 25.3


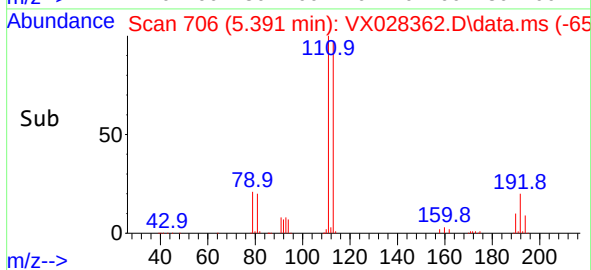
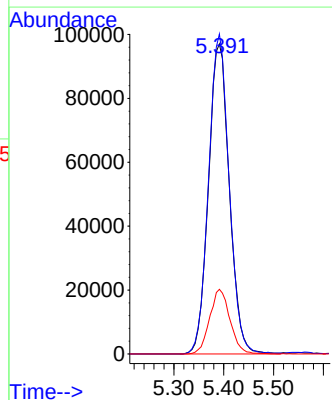
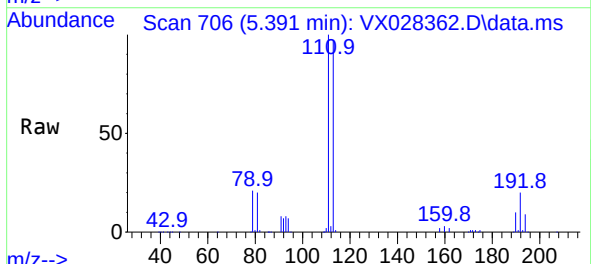




#43
Isopropyl Acetate
Concen: 2.713 ug/l
RT: 6.342 min Scan# 861
Delta R.T. 0.006 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05




Instrument :
MSVOA_X
ClientSampleId :
MH-10D


Tgt Ion: 43 Resp: 30500
Ion Ratio Lower Upper
43 100
61 21.6 18.5 27.7
87 15.9 13.0 19.6

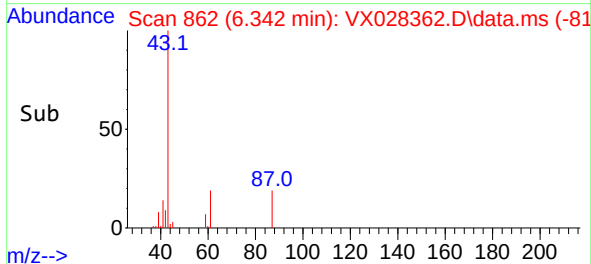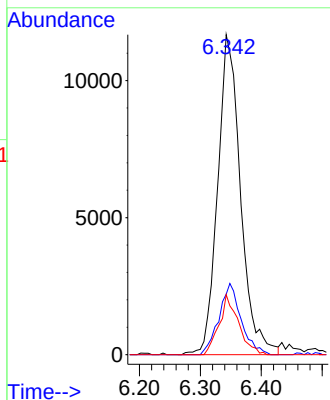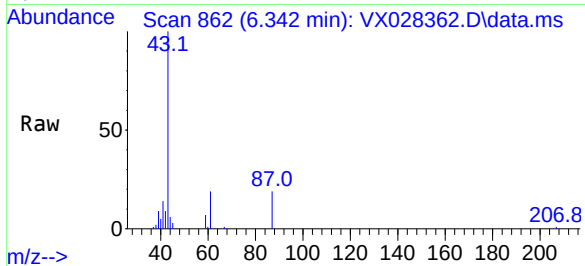

#50
Toluene-d8
Concen: 52.594 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05

Tgt Ion: 98 Resp: 1054405
Ion Ratio Lower Upper
98 100
100 66.4 52.6 78.8


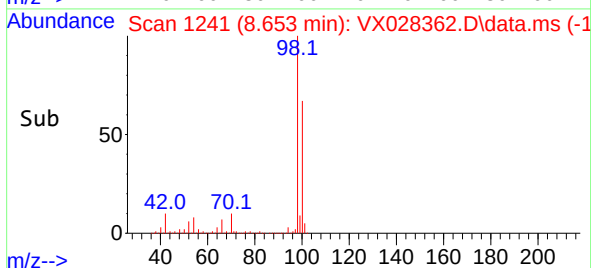
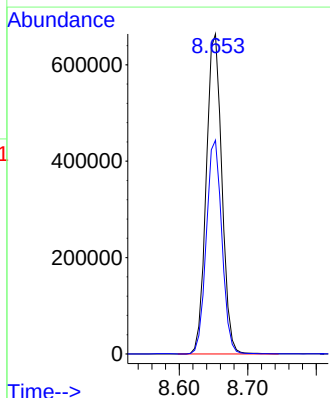
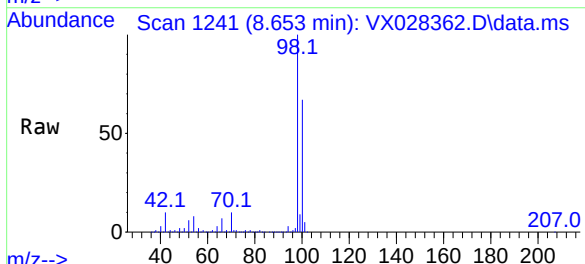


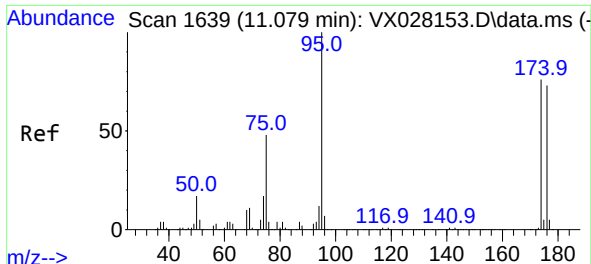

#62
4-Bromofluorobenzene
Concen: 51.275 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05




Instrument :
MSVOA_X
ClientSampleId :
MH-10D

Tgt Ion: 95 Resp: 393047
Ion Ratio Lower Upper
95 100
174 87.9 0.0 163.0
176 85.4 0.0 155.0

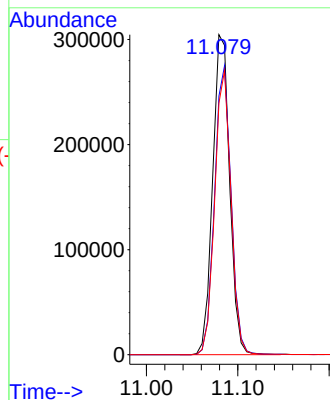


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05

Tgt Ion: 117 Resp: 741696
Ion Ratio Lower Upper
117 100
82 51.1 41.8 62.8
119 31.8 24.8 37.2

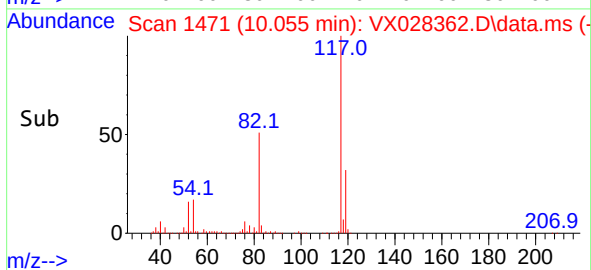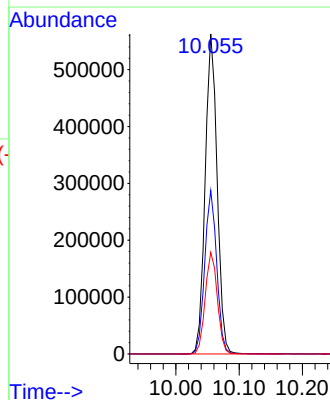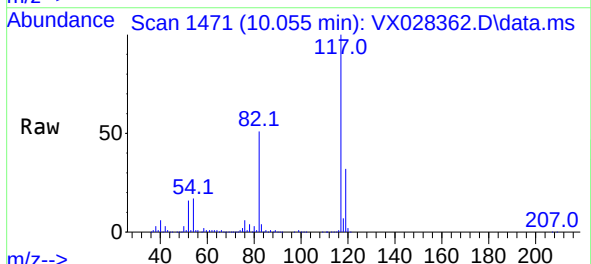

Abundance Scan 1794 (12.024 min): VX028153.D\data.ms (-


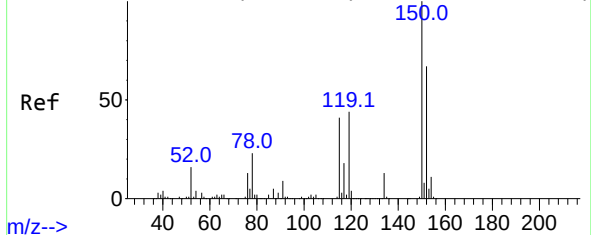


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028362.D
Acq: 26 Apr 2022 20:05

Instrument :
MSVOA_X
ClientSampleId :
MH-10D

Tgt Ion:152 Resp: 357682
Ion Ratio Lower Upper
152 100
115 57.7 37.5 112.7
150 156.6 0.0 338.2

Abundance Scan 1794 (12.024 min): VX028362.D\data.ms

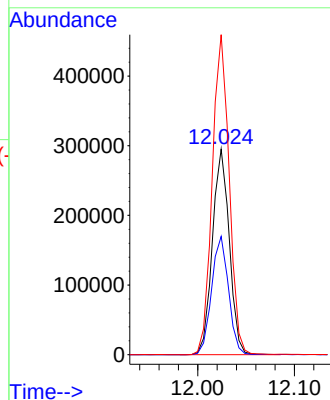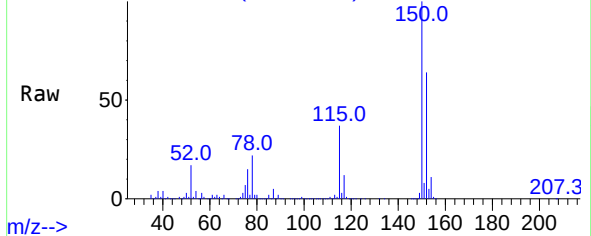

Abundance Scan 1794 (12.024 min): VX028362.D\data.ms (-

