

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035301.D
 Acq On : 26 Apr 2023 10:19
 Operator : JC/MD
 Sample : VX0426WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK629

Quant Time: Apr 27 04:41:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	429856	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	370908	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	182629	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	86960	31.374	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	62.740%		
7) Chloroethane-d5	1.673	69	70260	35.081	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	70.160%		
11) 1,1-Dichloroethene-d2	2.307	65	50354	37.968	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	75.940%		
21) 2-Butanone-d5	4.465	46	165030	89.347	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.350%		
24) Chloroform-d	5.056	84	215834	41.350	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.700%		
26) 1,2-Dichloroethane-d4	5.952	65	144882	43.223	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.440%		
32) Benzene-d6	5.971	84	452421	42.462	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.920%		
36) 1,2-Dichloropropane-d6	7.306	67	141163	43.373	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.740%		
41) Toluene-d8	8.647	98	406430	41.738	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.480%		
43) trans-1,3-Dichloroprop...	8.952	79	55759	39.202	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.400%		
47) 2-Hexanone-d5	9.385	63	119628	91.530	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	91.530%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	182117	45.690	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.380%		
66) 1,2-Dichlorobenzene-d4	12.317	152	158941	44.910	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.820%		
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.313	96	1433	0.558	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035301.D
Acq On : 26 Apr 2023 10:19
Operator : JC/MD
Sample : VX0426WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK629

Quant Time: Apr 27 04:41:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 25 03:03:54 2023
Response via : Initial Calibration

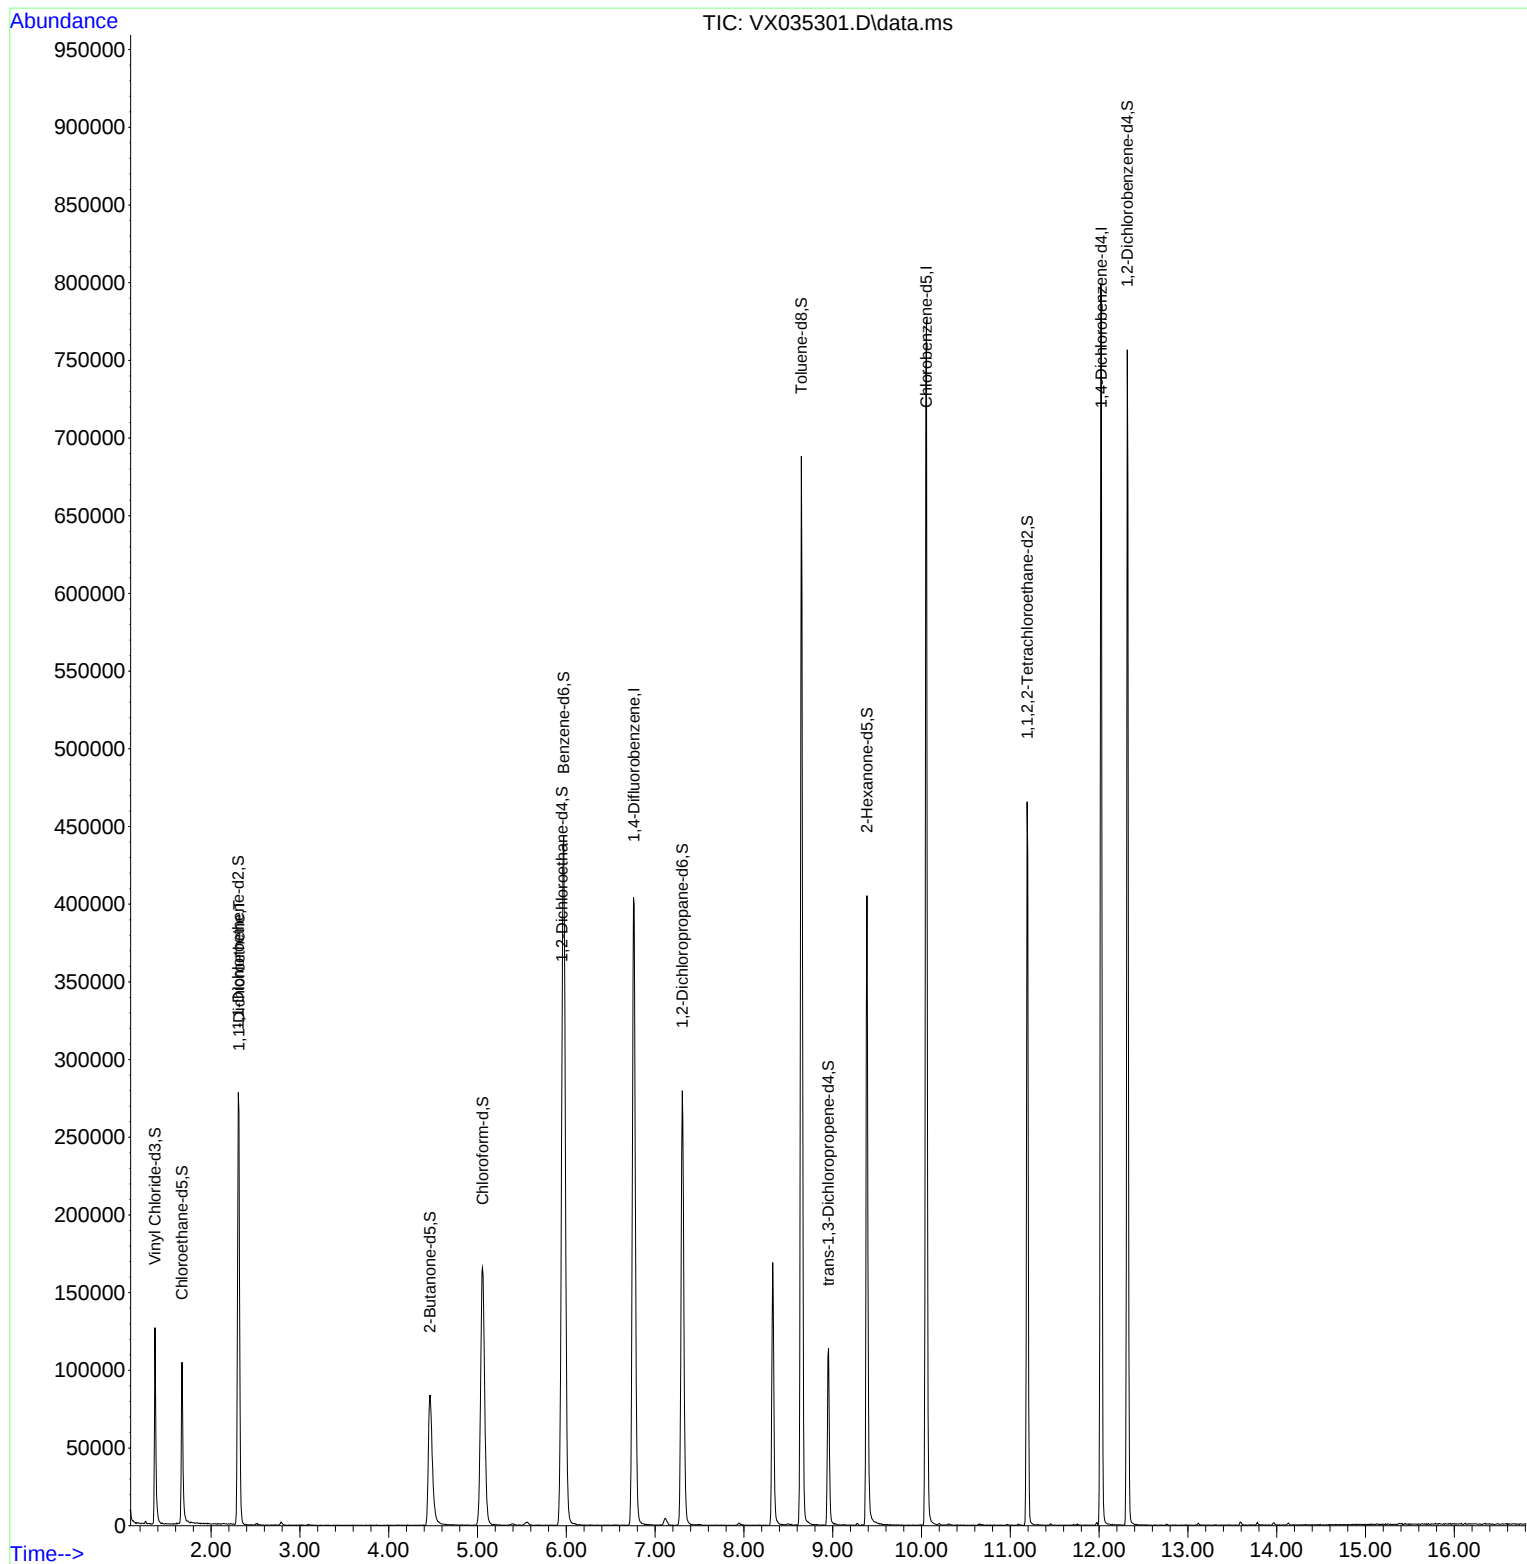

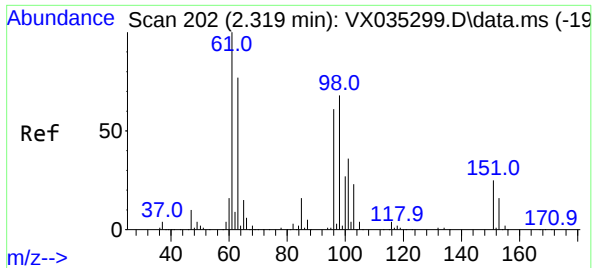

#12
 1,1-Dichloroethene
 Concen: 0.558 ug/L
 RT: 2.313 min Scan# 20
 Delta R.T. -0.006 min
 Lab File: VX035301.D
 Acq: 26 Apr 2023 10:19

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK629

Tgt Ion: 96 Resp: 1433
 Ion Ratio Lower Upper
 96 100
 61 1230.6 119.0 221.0#
 63 10317.3 91.0 169.0#

