




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035303.D
 Acq On : 26 Apr 2023 11:22
 Operator : JC/MD
 Sample : 02479-02ME
 Misc : 4.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW943ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:41:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

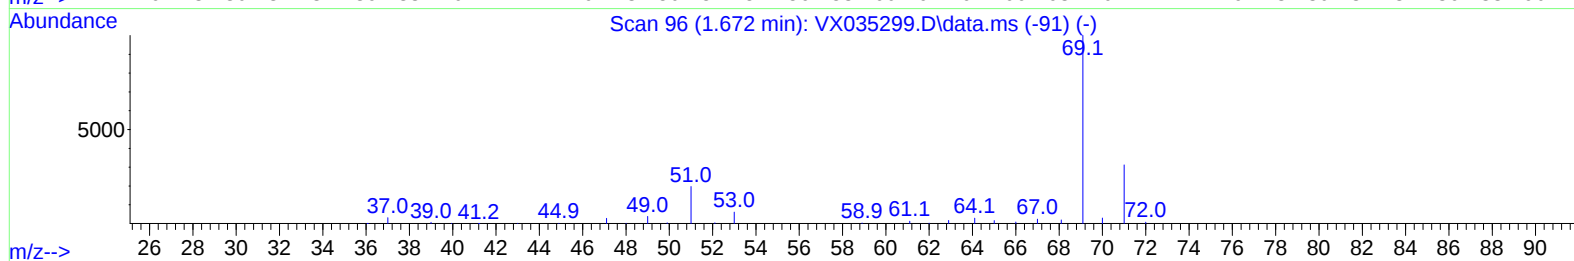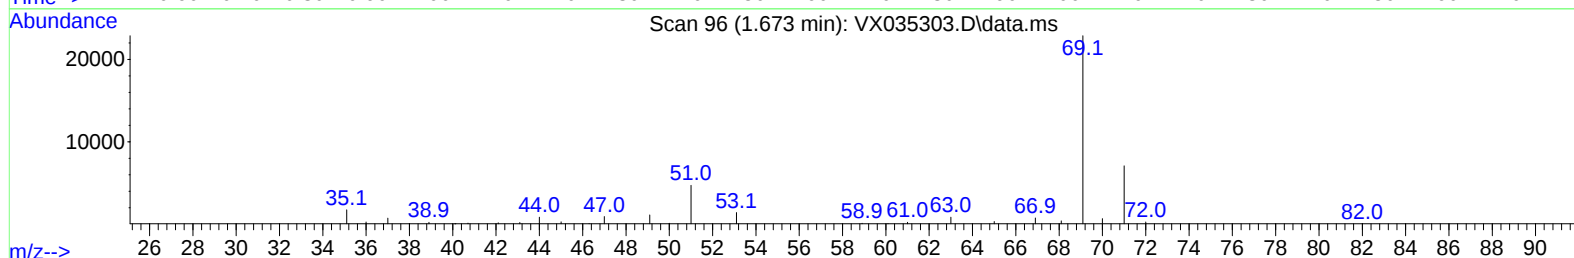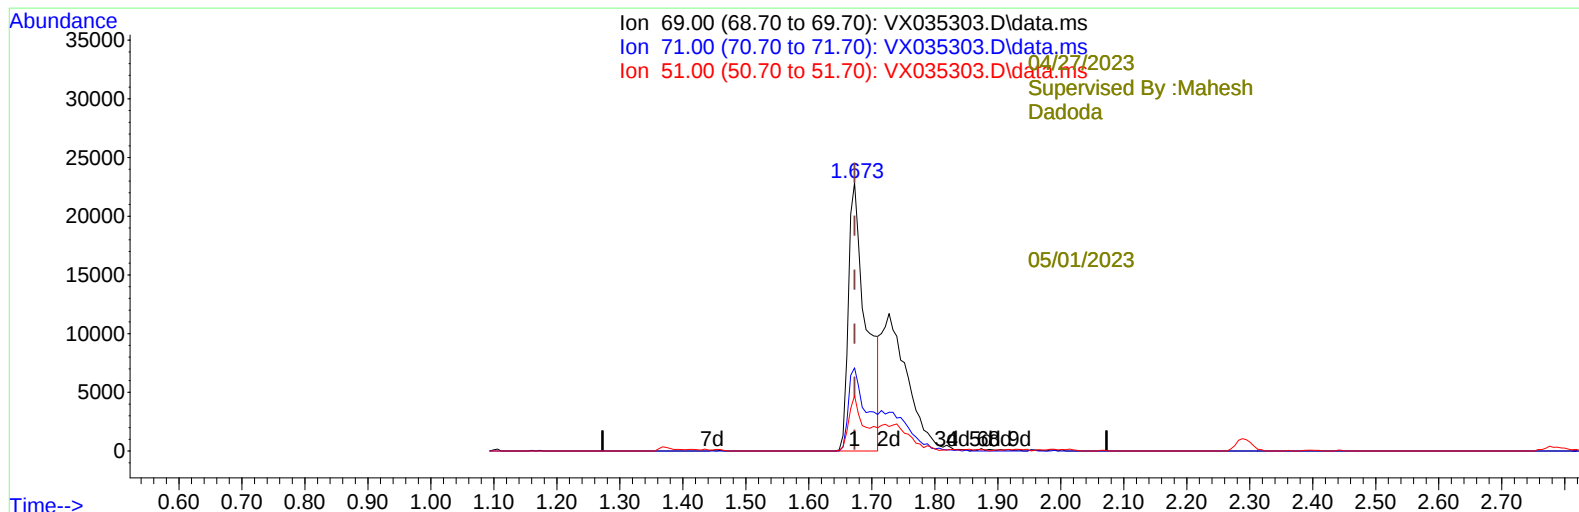

TIC: VX035303.D\data.ms

(7) Chloroethane-d5 (S)

1.673min (+ 0.000) 13.88 ug/L

response 44830

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	23.62
51.00	25.70	16.09#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035303.D
 Acq On : 26 Apr 2023 11:22
 Operator : JC/MD
 Sample : 02479-02ME
 Misc : 4.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW943ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:41:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

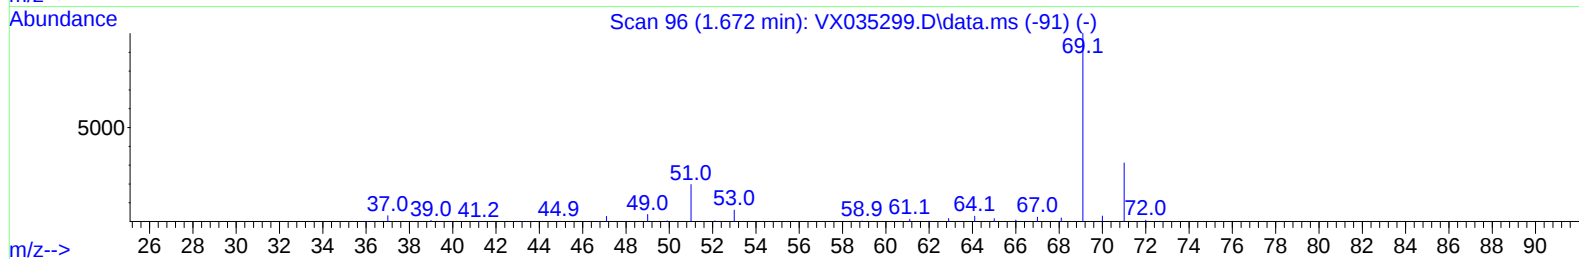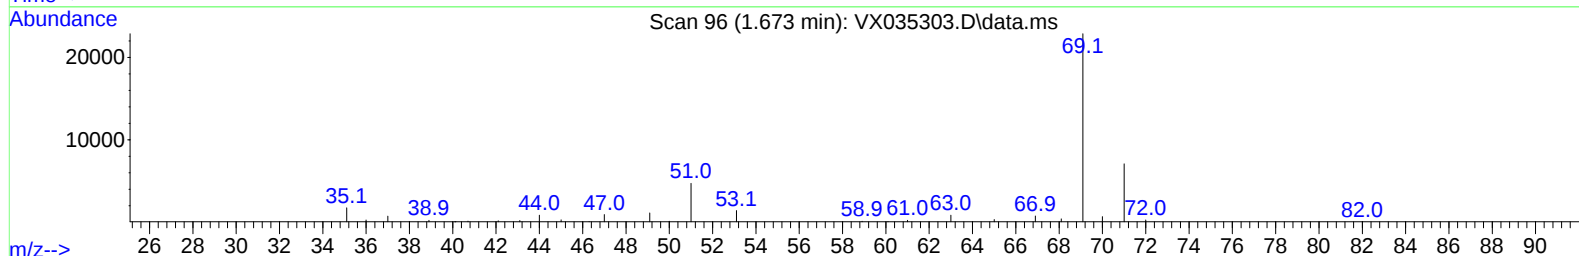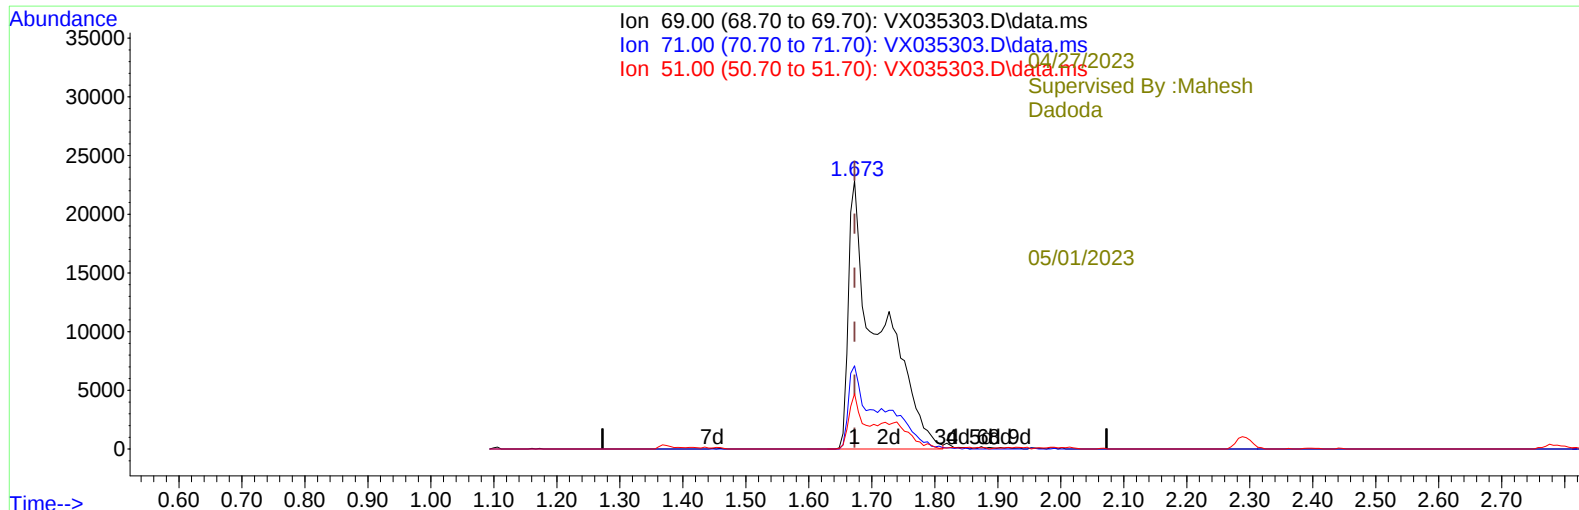

TIC: VX035303.D\data.ms

(7) Chloroethane-d5 (S)

1.673min (+ 0.000) 24.18 ug/L m

response 78107

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	13.56#
51.00	25.70	9.23#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035303.D
 Acq On : 26 Apr 2023 11:22
 Operator : JC/MD
 Sample : 02479-02ME
 Misc : 4.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW943ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:41:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

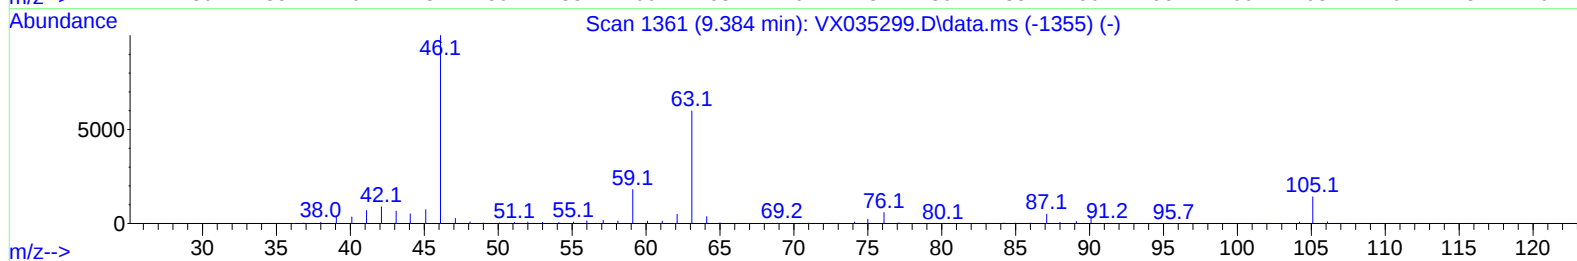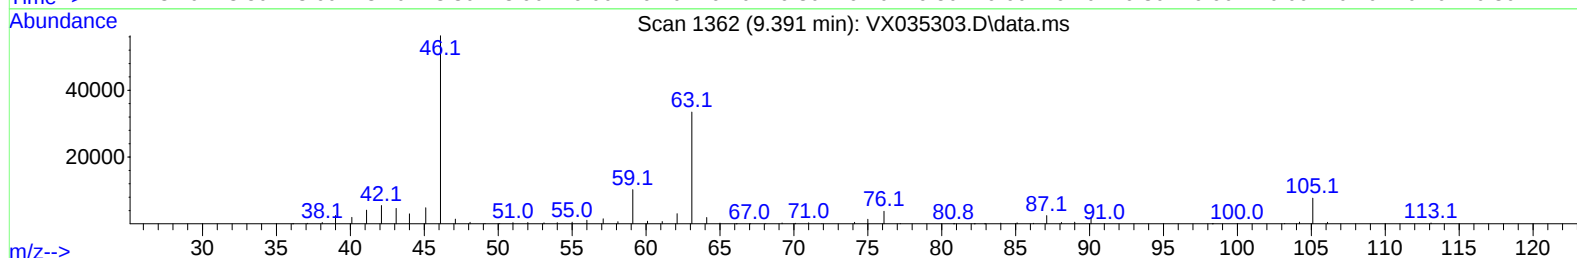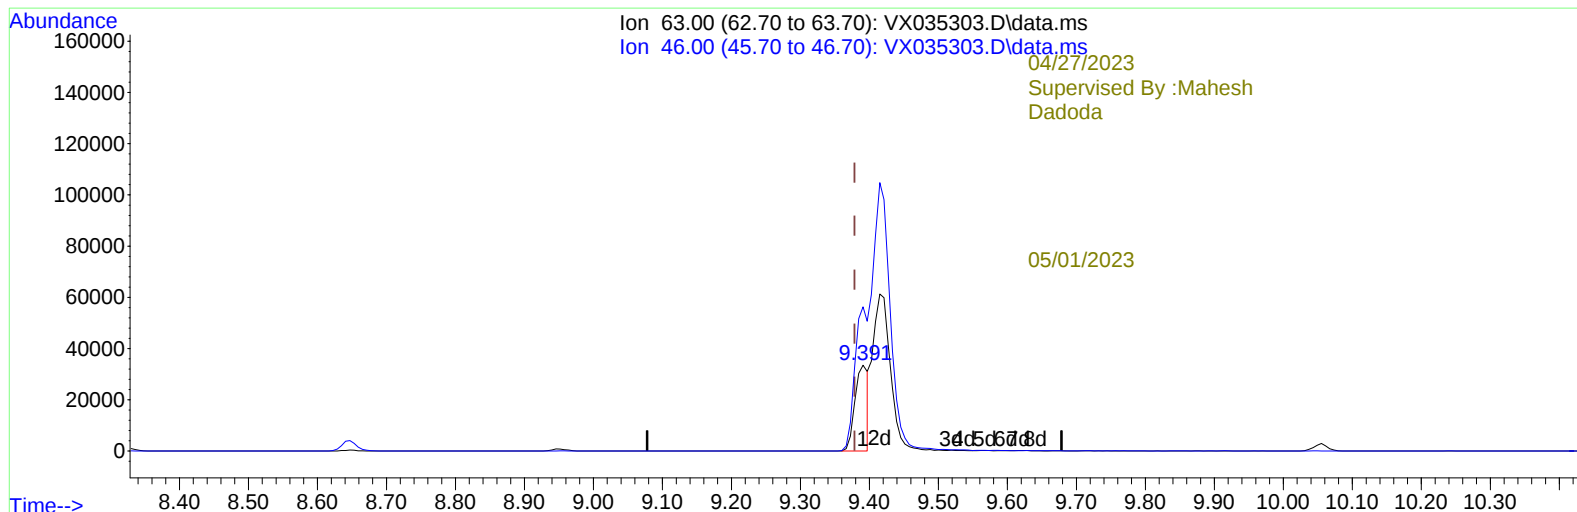

TIC: VX035303.D\data.ms

(47) 2-Hexanone-d5 (S)

9.391min (+ 0.012) 21.02 ug/L

response 44063

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	171.60	169.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035303.D
Acq On : 26 Apr 2023 11:22
Operator : JC/MD
Sample : 02479-02ME
Misc : 4.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW943ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:41:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 25 03:03:54 2023
Response via : Initial Calibration

Reviewed By :John
Carlone

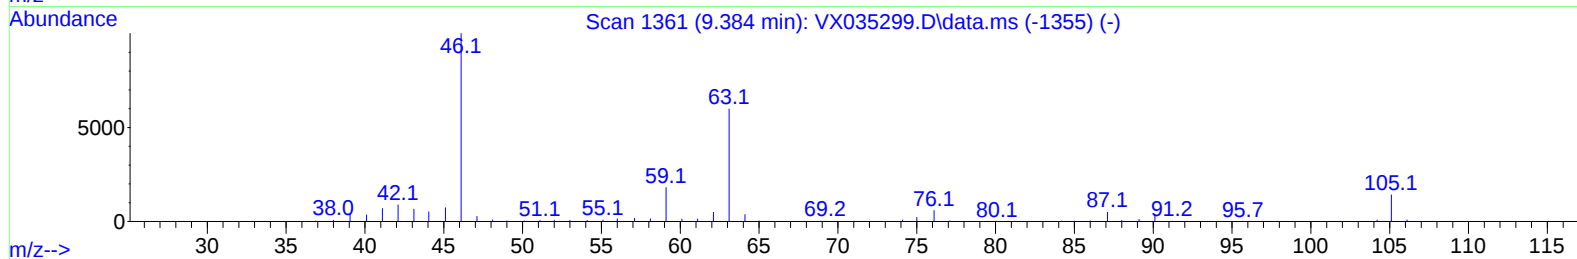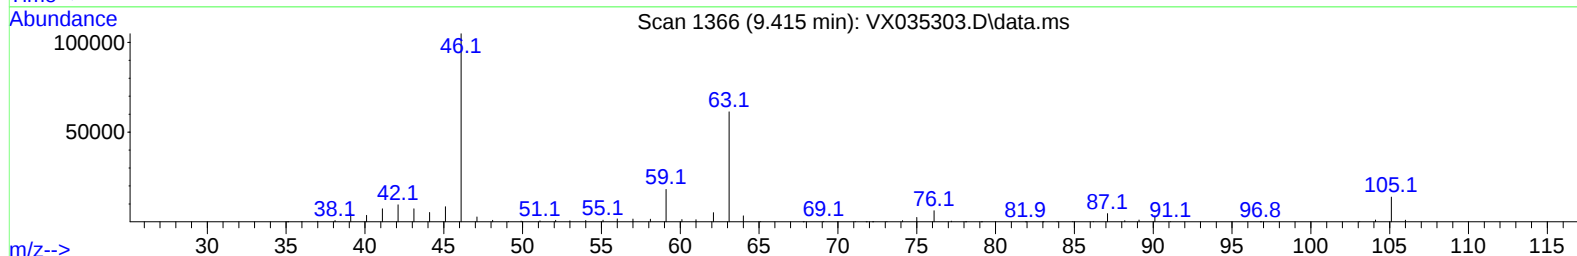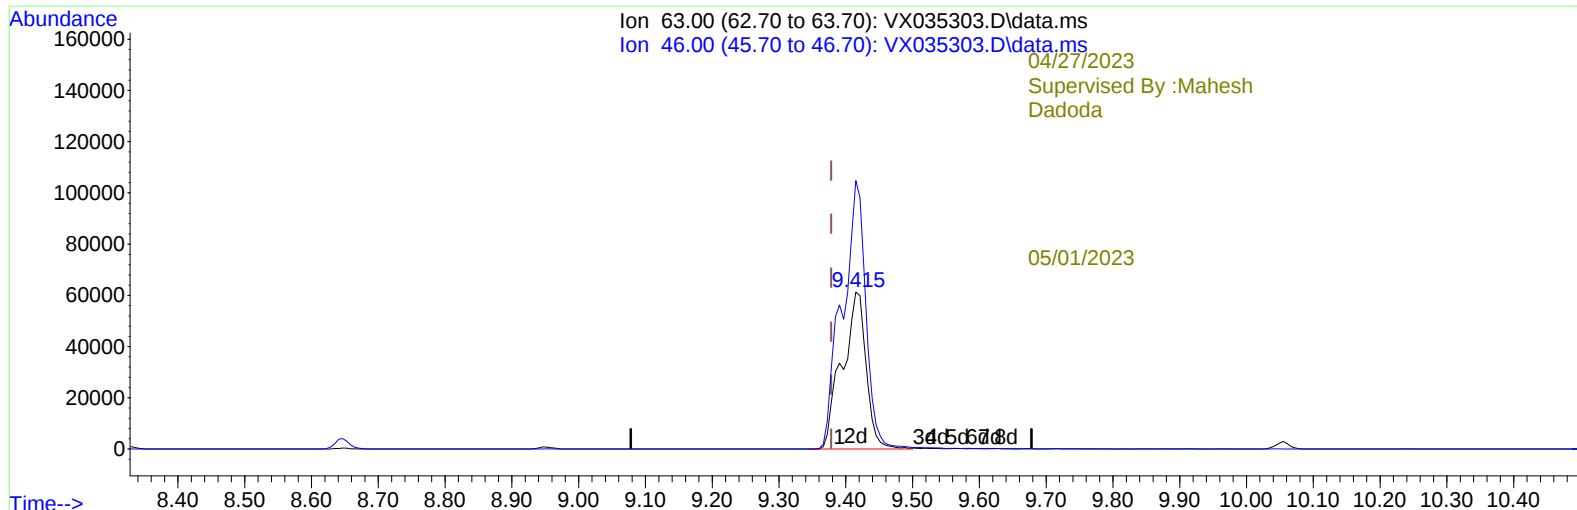

TIC: VX035303.D\data.ms

(47) 2-Hexanone-d5 (S)

9.415min (+ 0.037) 73.12 ug/L m

response 153282

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	171.60	48.79#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035303.D
 Acq On : 26 Apr 2023 11:22
 Operator : JC/MD
 Sample : 02479-02ME
 Misc : 4.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW943ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:41:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Reviewed By :John
 Carlone

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)	
							04/27/2023
							Supervised By :Mahesh
							adoda
Internal Standards							
1) 1,4-Difluorobenzene	6.757	114	693273	50.000	ug/L	0.00	
28) Chlorobenzene-d5	10.055	117	594880	50.000	ug/L	0.00	
58) 1,4-Dichlorobenzene-d4	12.024	152	294533	50.000	ug/L	0.00	
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.368	65	114872	25.697	ug/L	0.00	05/01/2023
Spiked Amount	50.000	Range 60 - 135	Recovery	=	51.400%	#	
7) Chloroethane-d5	1.673	69	78107m	24.181	ug/L	0.00	
Spiked Amount	50.000	Range 70 - 130	Recovery	=	48.360%	#	
11) 1,1-Dichloroethene-d2	2.288	65	66318	31.005	ug/L	-0.02	
Spiked Amount	50.000	Range 60 - 125	Recovery	=	62.020%		
21) 2-Butanone-d5	4.471	46	204829	68.759	ug/L	0.01	
Spiked Amount	100.000	Range 40 - 130	Recovery	=	68.760%		
24) Chloroform-d	5.056	84	287606	34.164	ug/L	0.00	
Spiked Amount	50.000	Range 70 - 125	Recovery	=	68.320%	#	
26) 1,2-Dichloroethane-d4	5.952	65	202500	37.458	ug/L	0.00	
Spiked Amount	50.000	Range 70 - 125	Recovery	=	74.920%		
32) Benzene-d6	5.964	84	638231	37.348	ug/L	0.00	
Spiked Amount	50.000	Range 70 - 125	Recovery	=	74.700%		
36) 1,2-Dichloropropane-d6	7.306	67	198524	38.032	ug/L	0.00	
Spiked Amount	50.000	Range 70 - 120	Recovery	=	76.060%		
41) Toluene-d8	8.647	98	579302	37.092	ug/L	0.00	
Spiked Amount	50.000	Range 80 - 120	Recovery	=	74.180%	#	
43) trans-1,3-Dichloroprop...	8.952	79	76219	33.412	ug/L	0.00	
Spiked Amount	50.000	Range 60 - 125	Recovery	=	66.820%		
47) 2-Hexanone-d5	9.415	63	153282m	73.124	ug/L	0.04	
Spiked Amount	100.000	Range 45 - 130	Recovery	=	73.120%		
56) 1,1,2,2-Tetrachloroeth...	11.201	84	239038	37.392	ug/L	0.01	
Spiked Amount	50.000	Range 65 - 120	Recovery	=	74.780%		
66) 1,2-Dichlorobenzene-d4	12.323	152	224164	39.274	ug/L	0.00	
Spiked Amount	50.000	Range 80 - 120	Recovery	=	78.540%	#	
Target Compounds							Qvalue
25) Chloroform	5.087	83	13804	1.656	ug/L	96	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035303.D
Acq On : 26 Apr 2023 11:22
Operator : JC/MD
Sample : 02479-02ME
Misc : 4.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW943ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:41:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 25 03:03:54 2023
Response via : Initial Calibration

Reviewed By :John
Carlone

