




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035319.D
 Acq On : 26 Apr 2023 17:30
 Operator : JC/MD
 Sample : 02479-12ME
 Misc : 5.08g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW953ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:43:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

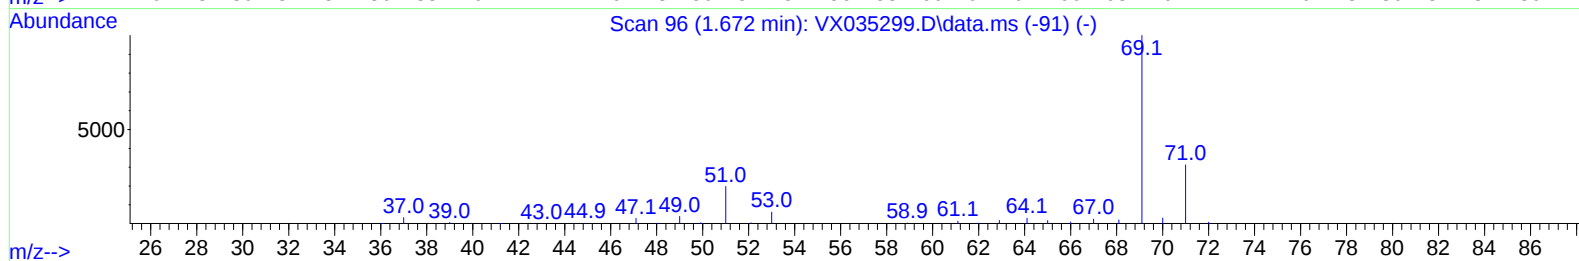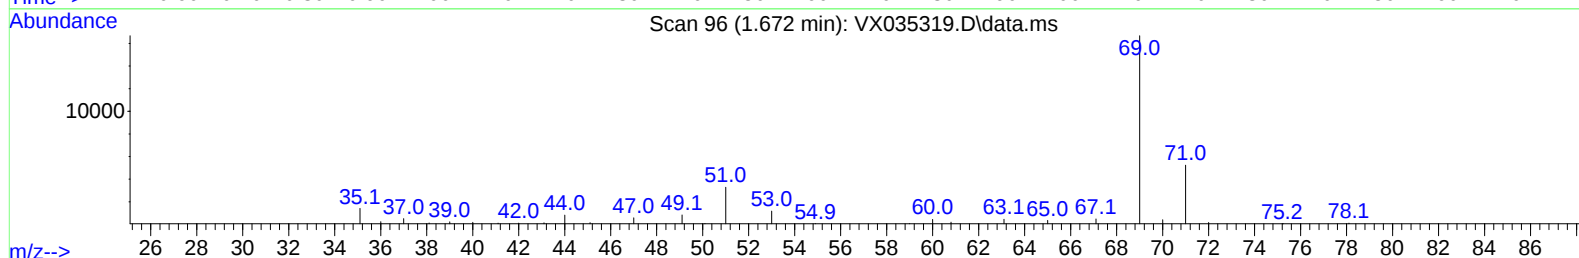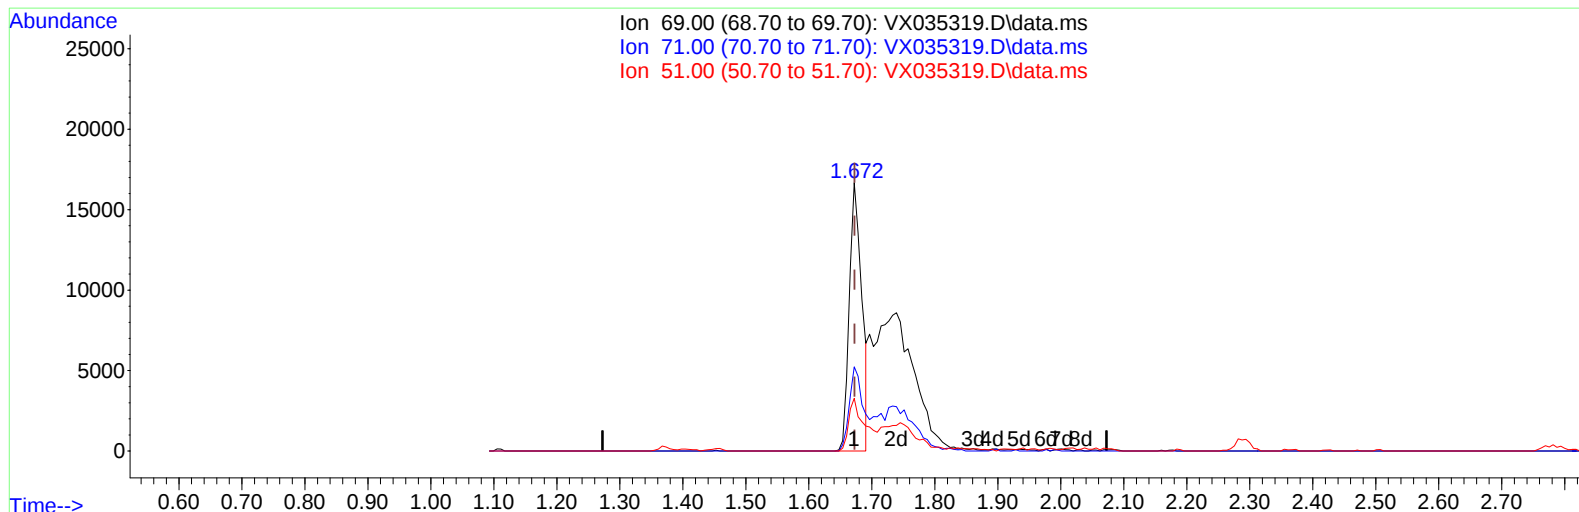

TIC: VX035319.D\data.ms

(7) Chloroethane-d5 (S)

1.672min (-0.000) 11.32 ug/L

response 23045

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	35.42
51.00	25.70	26.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035319.D
 Acq On : 26 Apr 2023 17:30
 Operator : JC/MD
 Sample : 02479-12ME
 Misc : 5.08g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW953ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:43:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

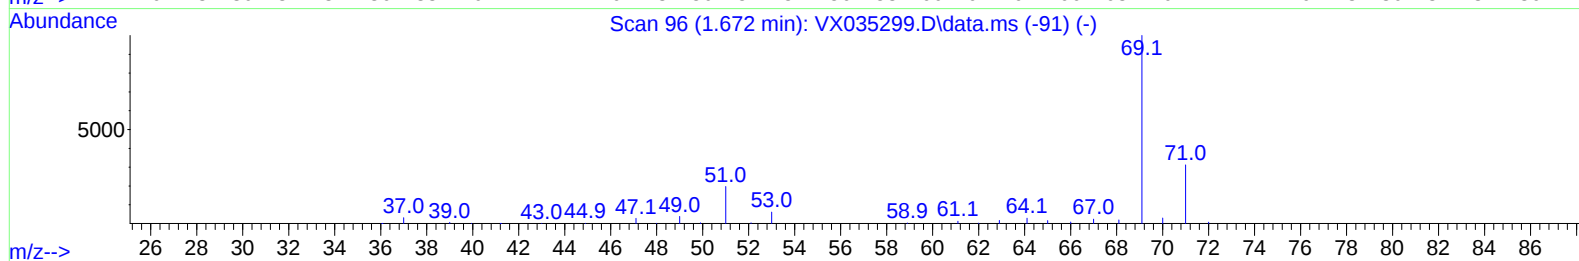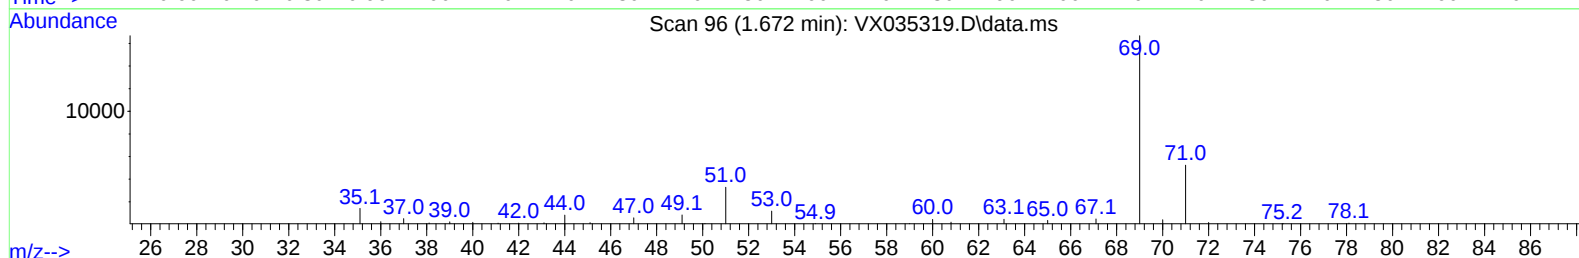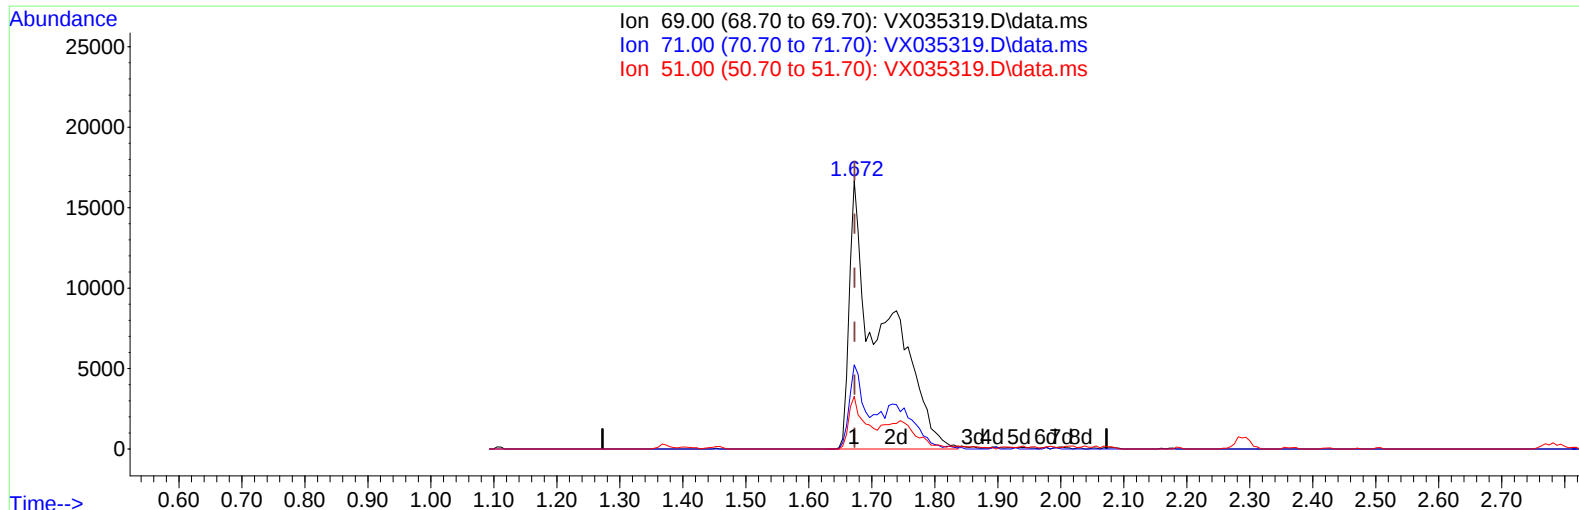

TIC: VX035319.D\data.ms

(7) Chloroethane-d5 (S)

1.672min (-0.000) 30.34 ug/L m

response 61767

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	13.21#
51.00	25.70	9.74#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035319.D
 Acq On : 26 Apr 2023 17:30
 Operator : JC/MD
 Sample : 02479-12ME
 Misc : 5.08g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW953ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:43:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

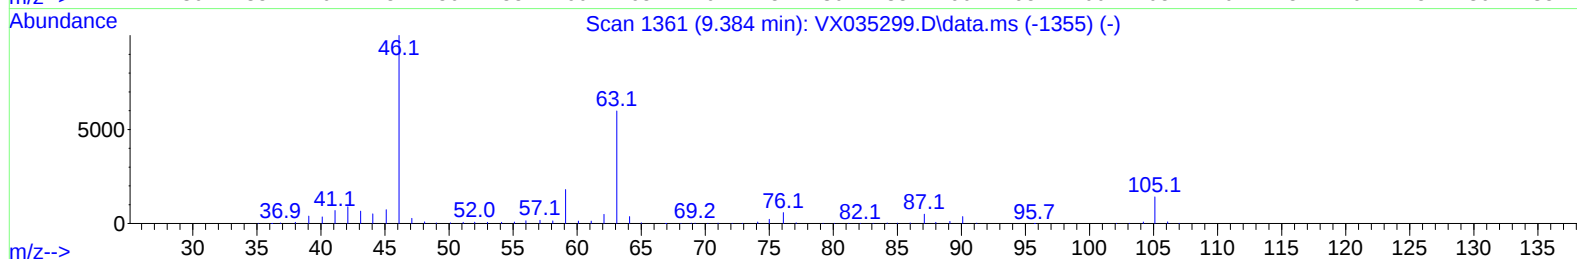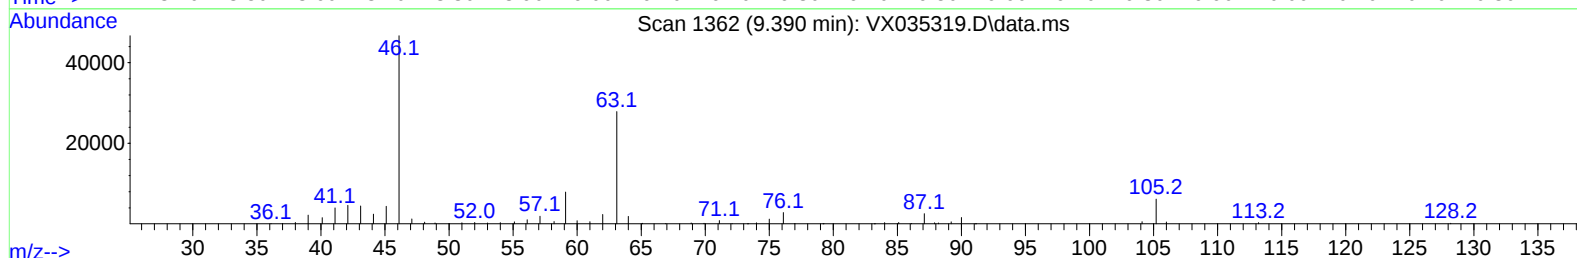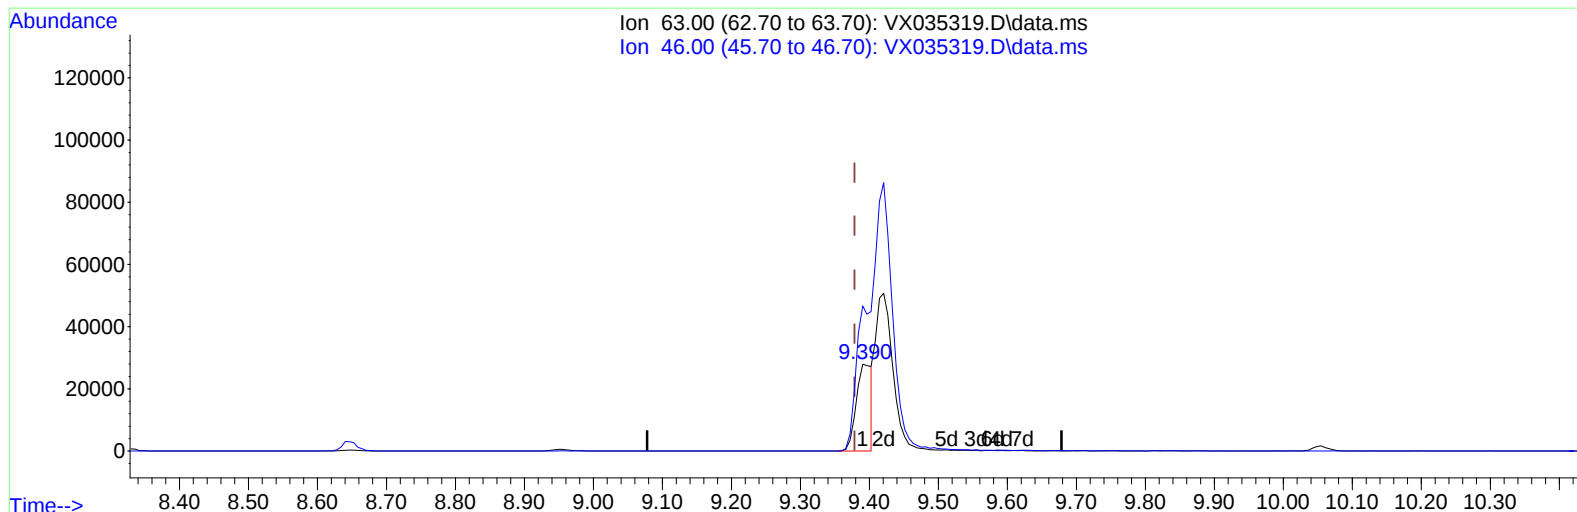

TIC: VX035319.D\data.ms

(47) 2-Hexanone-d5 (S)

9.390min (+ 0.012) 32.62 ug/L

response 43436

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	171.60	129.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035319.D
 Acq On : 26 Apr 2023 17:30
 Operator : JC/MD
 Sample : 02479-12ME
 Misc : 5.08g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW953ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:43:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

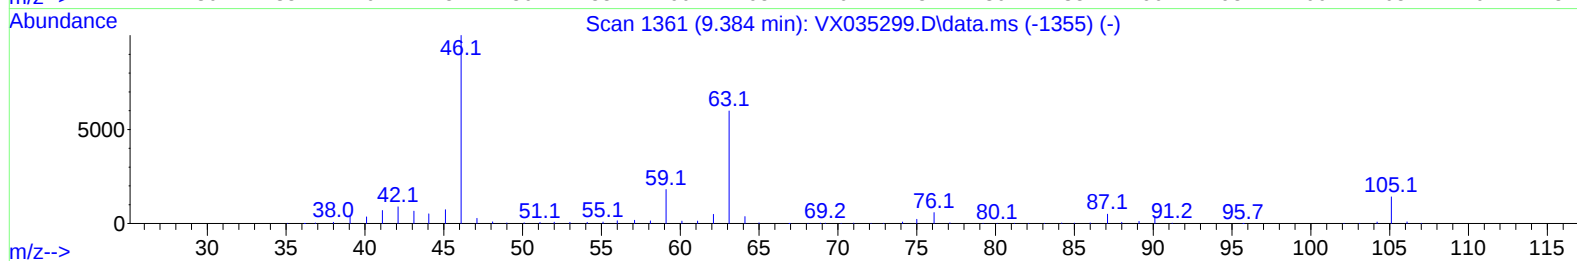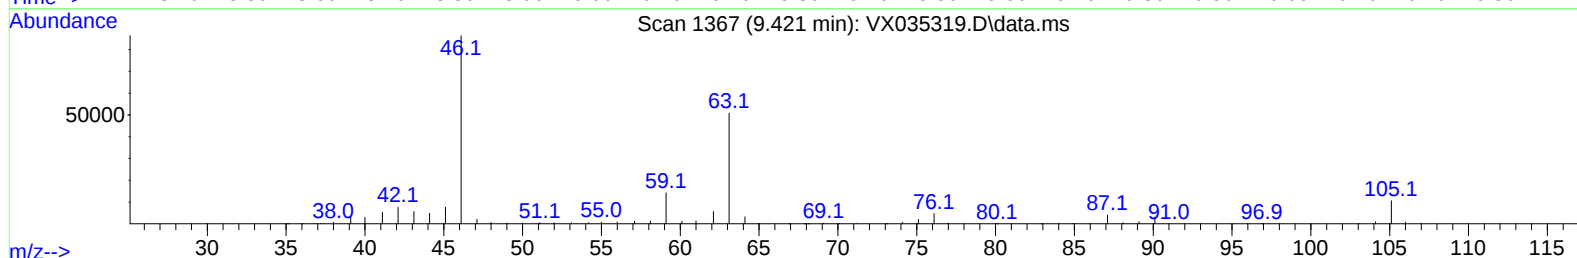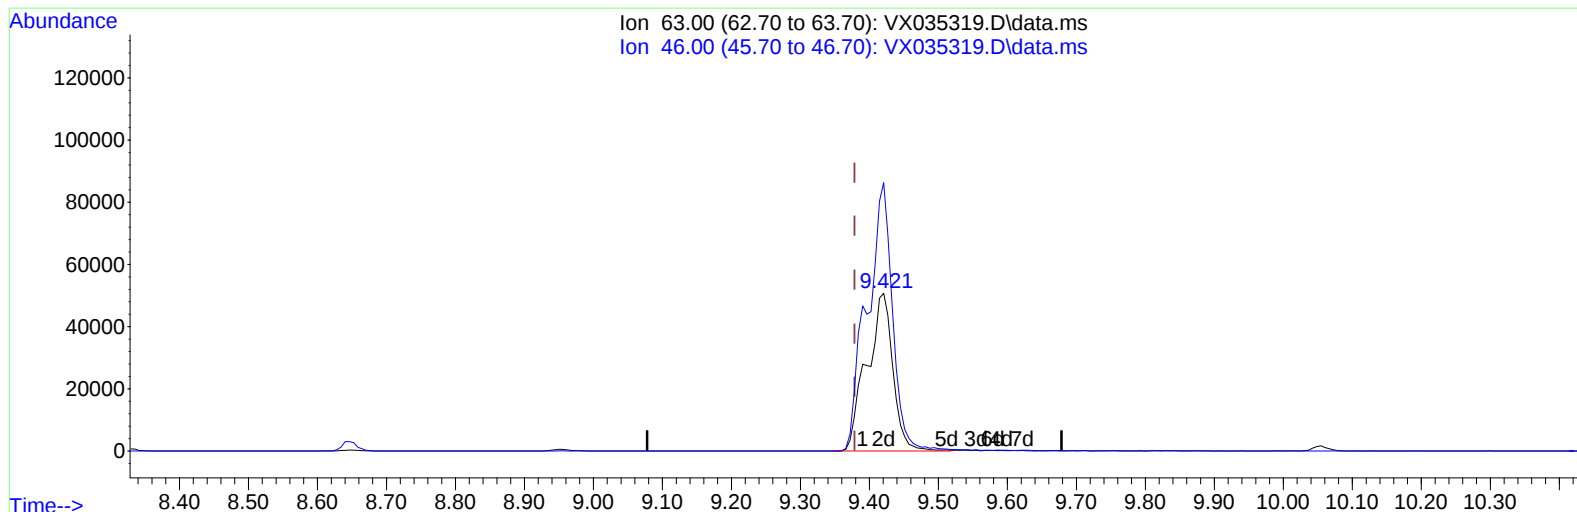

TIC: VX035319.D\data.ms

(47) 2-Hexanone-d5 (S)

9.421min (+ 0.042) 99.99 ug/L m

response 133160

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	171.60	42.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035319.D
 Acq On : 26 Apr 2023 17:30
 Operator : JC/MD
 Sample : 02479-12ME
 Misc : 5.08g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW953ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:43:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.756	114	436882	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	377926	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	185083	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	85455	30.335	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	60.680%		
7) Chloroethane-d5	1.672	69	61767m	30.344	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	60.680%#		
11) 1,1-Dichloroethene-d2	2.288	65	47796	35.460	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.920%		
21) 2-Butanone-d5	4.482	46	177748	94.685	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	94.690%		
24) Chloroform-d	5.056	84	221230	41.702	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.400%		
26) 1,2-Dichloroethane-d4	5.952	65	155961	45.780	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.560%		
32) Benzene-d6	5.964	84	484954	44.670	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.340%		
36) 1,2-Dichloropropane-d6	7.305	67	153601	46.318	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.640%		
41) Toluene-d8	8.646	98	438769	44.222	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.440%		
43) trans-1,3-Dichloroprop...	8.951	79	55848	38.536	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.080%		
47) 2-Hexanone-d5	9.421	63	133160m	99.992	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.990%		
56) 1,1,2,2-Tetrachloroeth...	11.201	84	194712	47.943	ug/L	0.01
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.880%		
66) 1,2-Dichlorobenzene-d4	12.323	152	179456	50.034	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.060%		
Target Compounds						Qvalue
46) Tetrachloroethene	9.274	164	3167	1.396	ug/L	81
57) 1,1,2,2-Tetrachloroethane	11.219	83	3520	0.835	ug/L #	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035319.D
Acq On : 26 Apr 2023 17:30
Operator : JC/MD
Sample : 02479-12ME
Misc : 5.08g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW953ME

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:43:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 25 03:03:54 2023
Response via : Initial Calibration

Reviewed By :John Carlone 04/27/2023
Supervised By :Mahesh Dadoda 05/01/2023

