




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
Data File : VX035324.D  
Acq On : 26 Apr 2023 19:26  
Operator : JC/MD  
Sample : 02419-12MSD  
Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXMLM041823WMA.M  
Quant Title : VOC Analysis  
QLast Update : Tue Apr 25 03:03:54 2023  
Response via : Initial Calibration

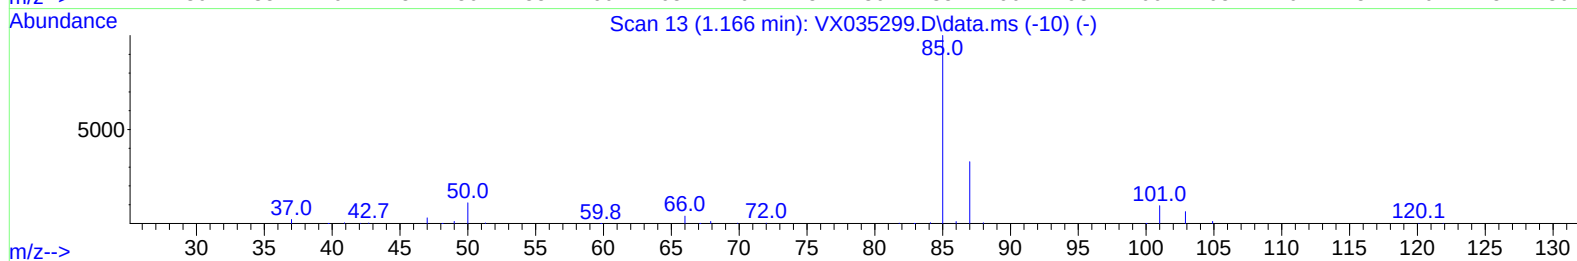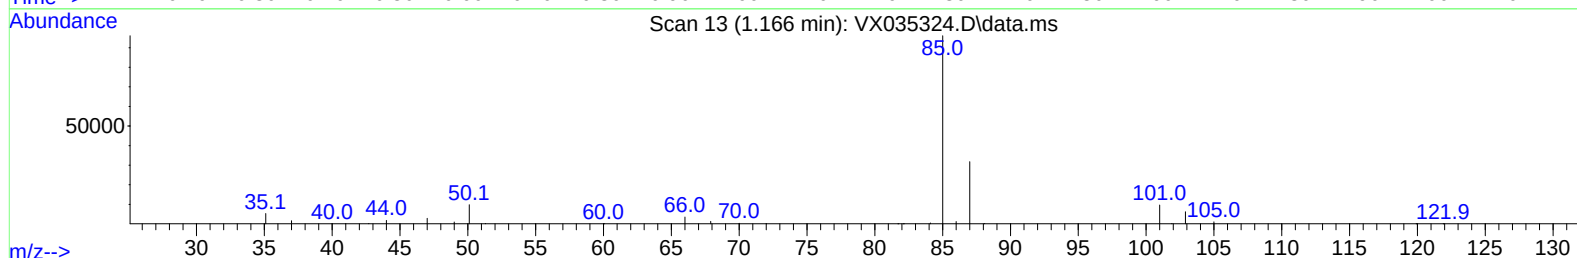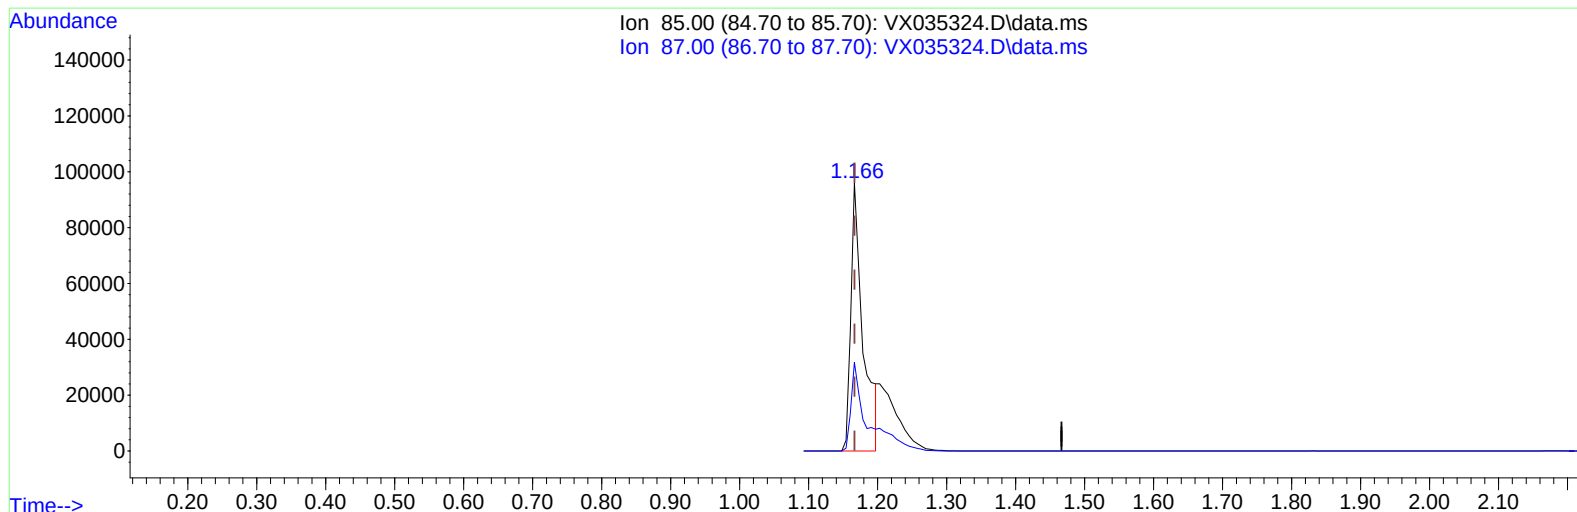

TIC: VX035324.D\data.ms

## (2) Dichlorodifluoromethane (T)

1.166min (-0.000) 33.21 ug/L

response 116384

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 85.00 | 100.00 | 100.00 |
| 87.00 | 32.80  | 27.06  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |






Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
Data File : VX035324.D  
Acq On : 26 Apr 2023 19:26  
Operator : JC/MD  
Sample : 02419-12MSD  
Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXMLM041823WMA.M  
Quant Title : VOC Analysis  
QLast Update : Tue Apr 25 03:03:54 2023  
Response via : Initial Calibration

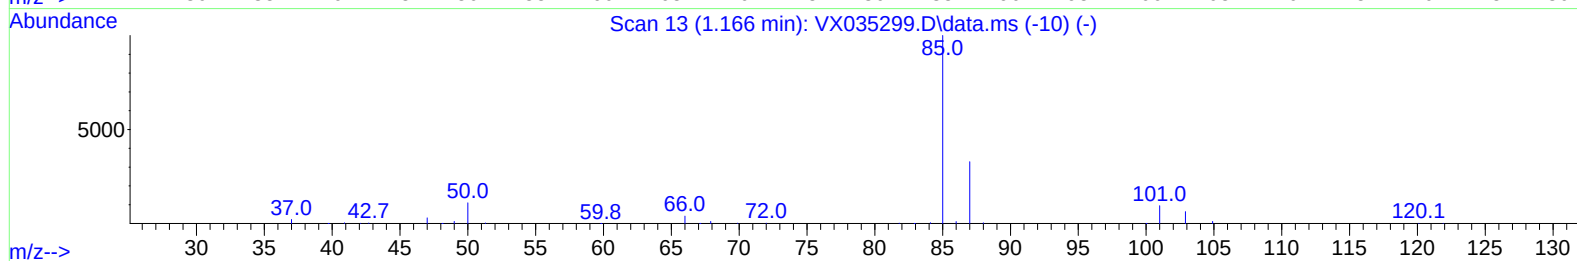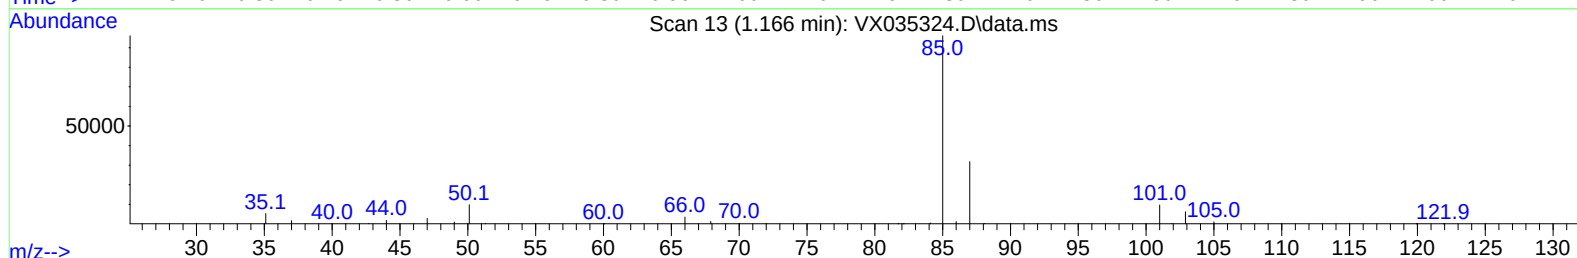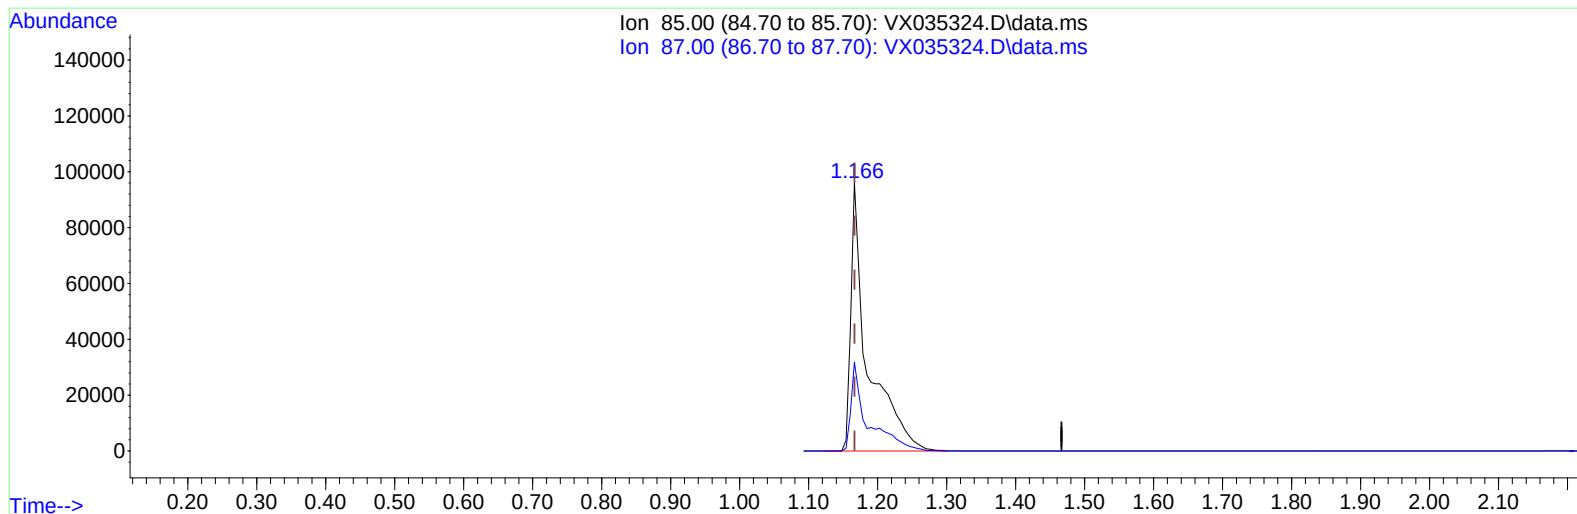

TIC: VX035324.D\data.ms

## (2) Dichlorodifluoromethane (T)

1.166min (-0.000) 46.77 ug/L m

response 163897

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 85.00 | 100.00 | 100.00 |
| 87.00 | 32.80  | 19.22# |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

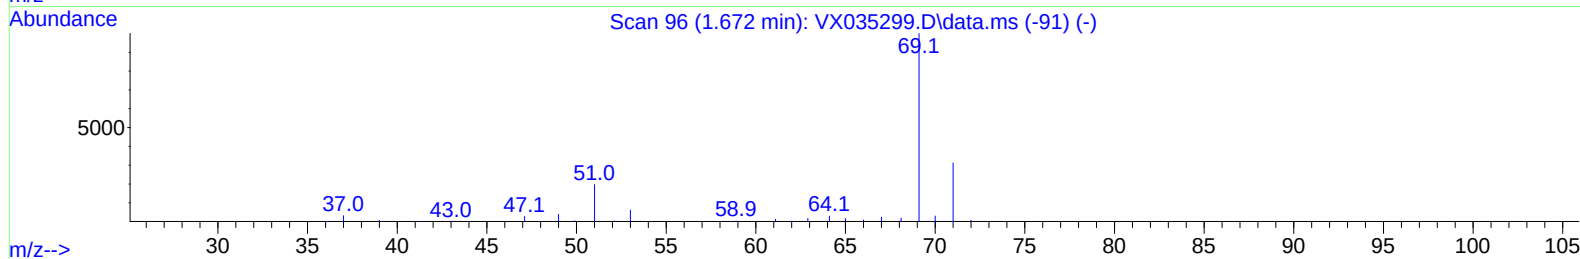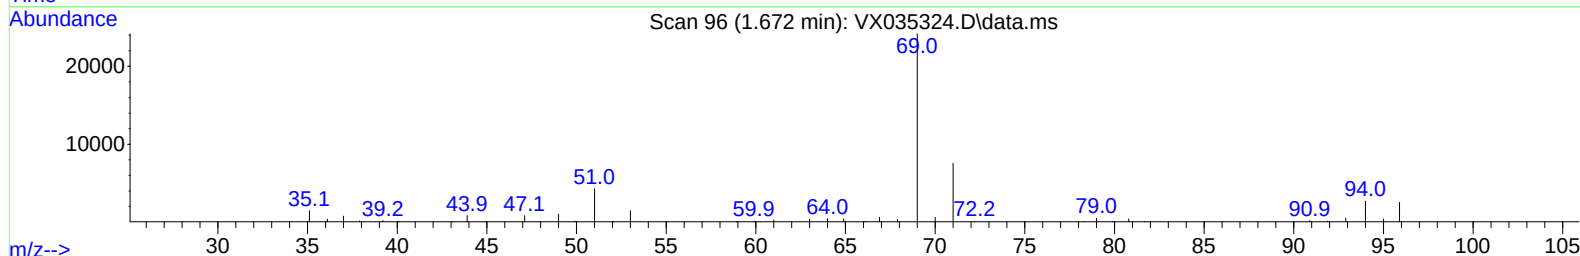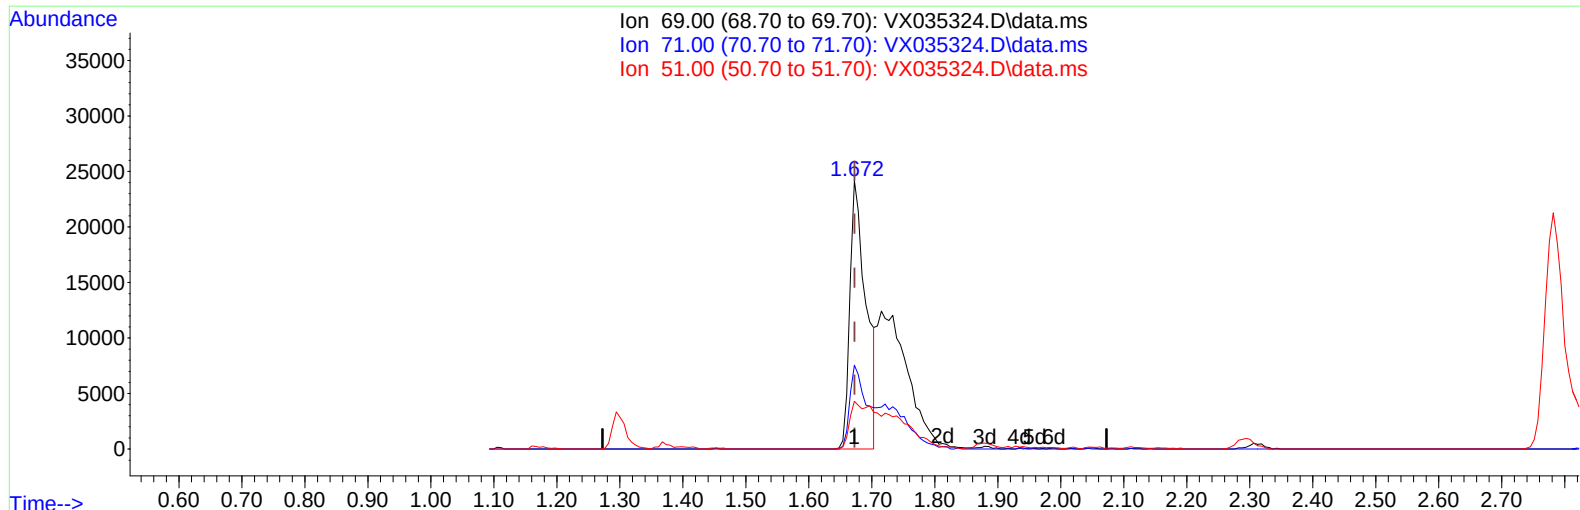

TIC: VX035324.D\data.ms

(7) Chloroethane-d5 (S)

1.672min (-0.000) 19.85 ug/L

response 43245

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 69.00 | 100.00 | 100.00 |
| 71.00 | 31.70  | 32.06  |
| 51.00 | 25.70  | 13.68# |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

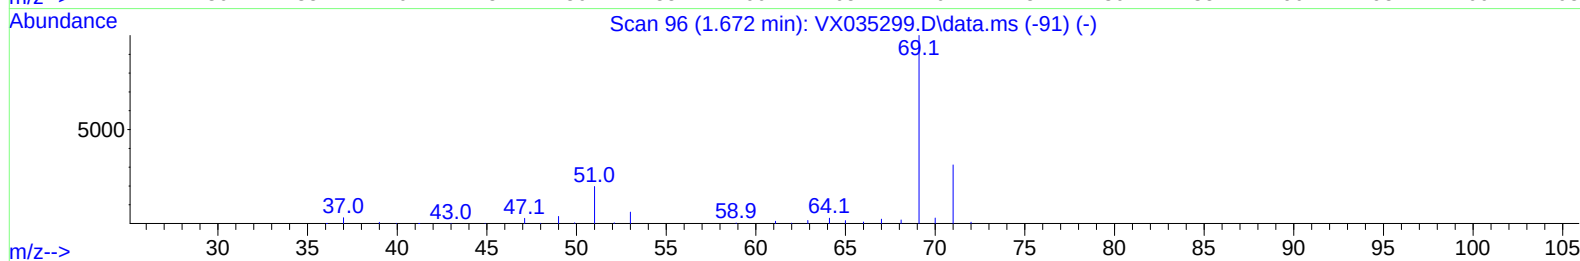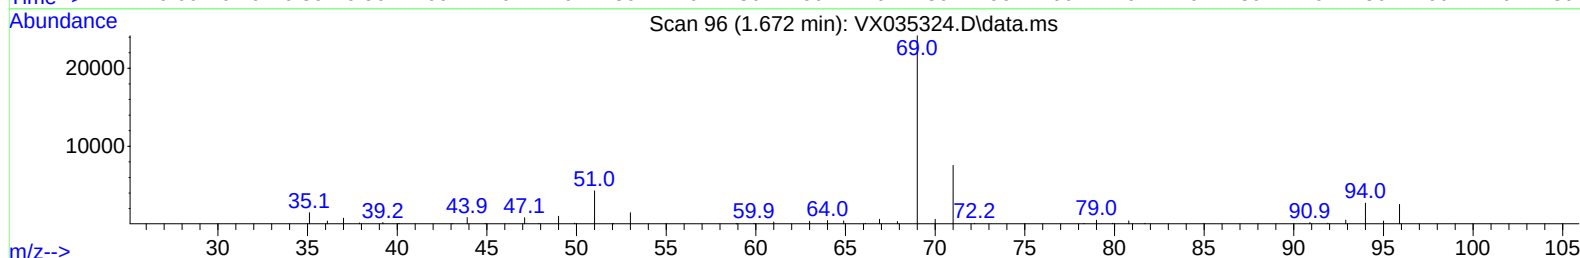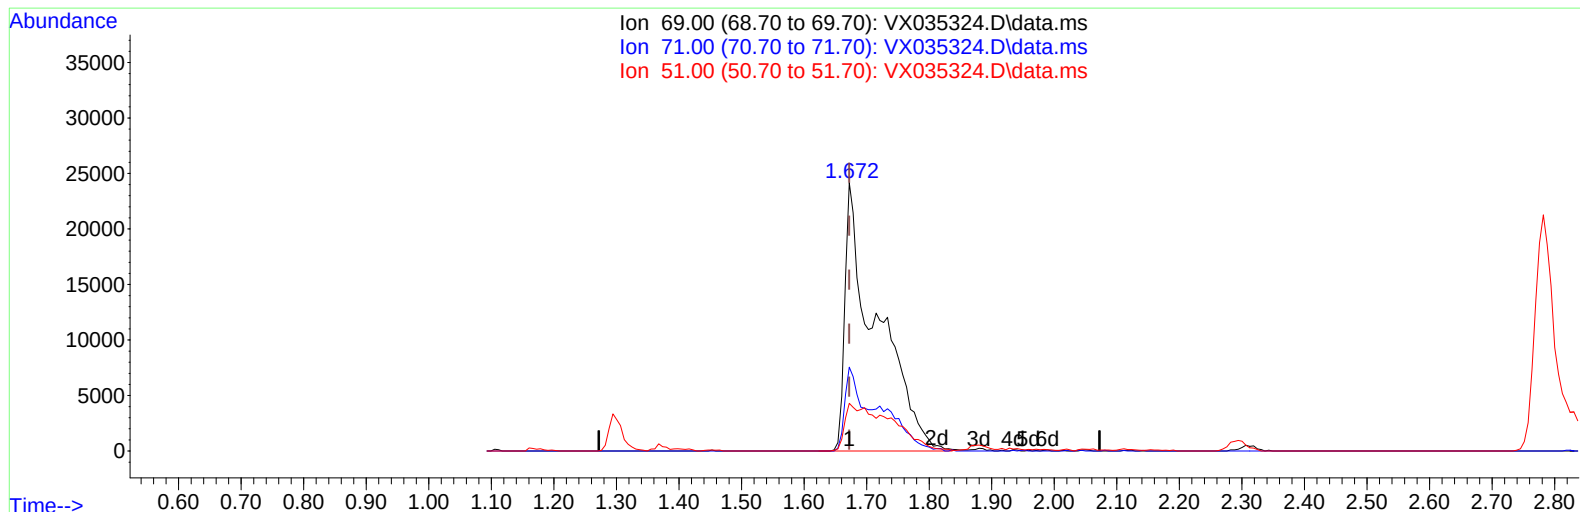

TIC: VX035324.D\data.ms

## (7) Chloroethane-d5 (S)

1.672min (-0.000) 39.19 ug/L m

response 85387

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 69.00 | 100.00 | 100.00 |
| 71.00 | 31.70  | 16.24# |
| 51.00 | 25.70  | 6.93#  |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

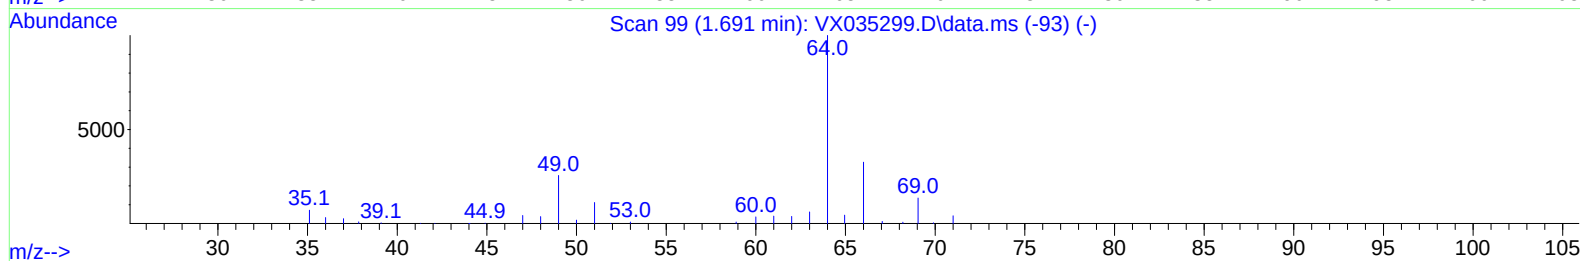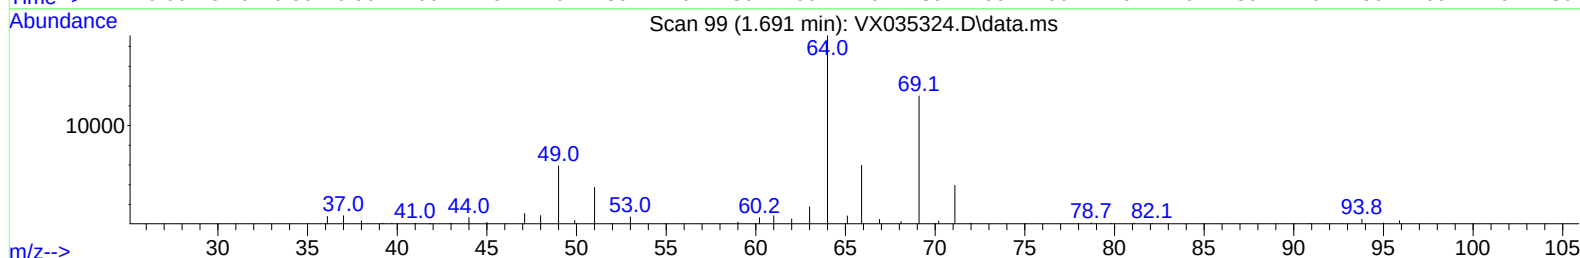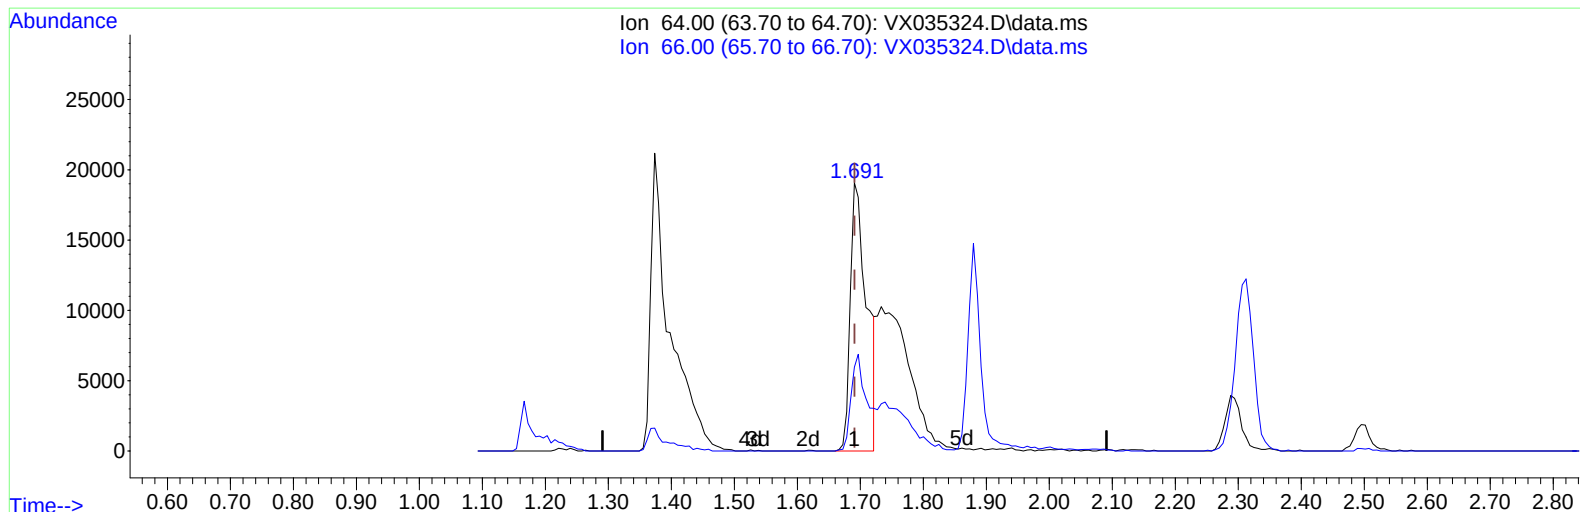

TIC: VX035324.D\data.ms

## (8) Chloroethane (T)

1.691min (-0.000) 18.79 ug/L

response 34690

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 64.00 | 100.00 | 100.00 |
| 66.00 | 31.30  | 31.28  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXMLM041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

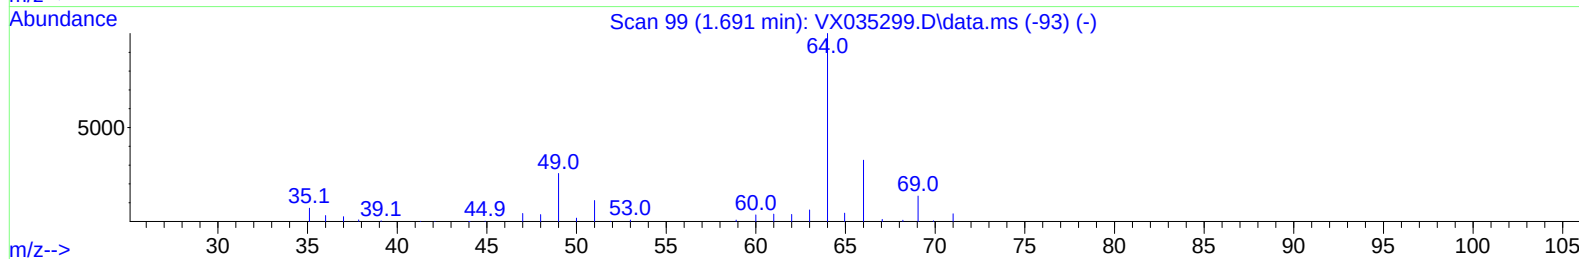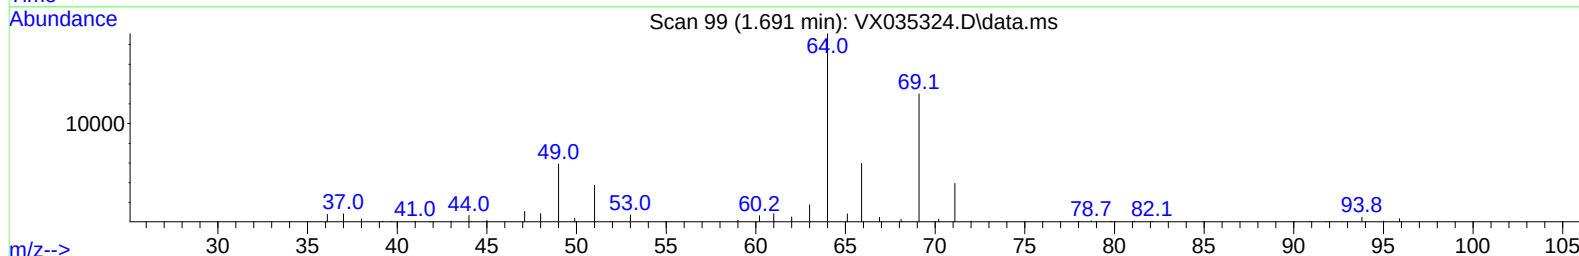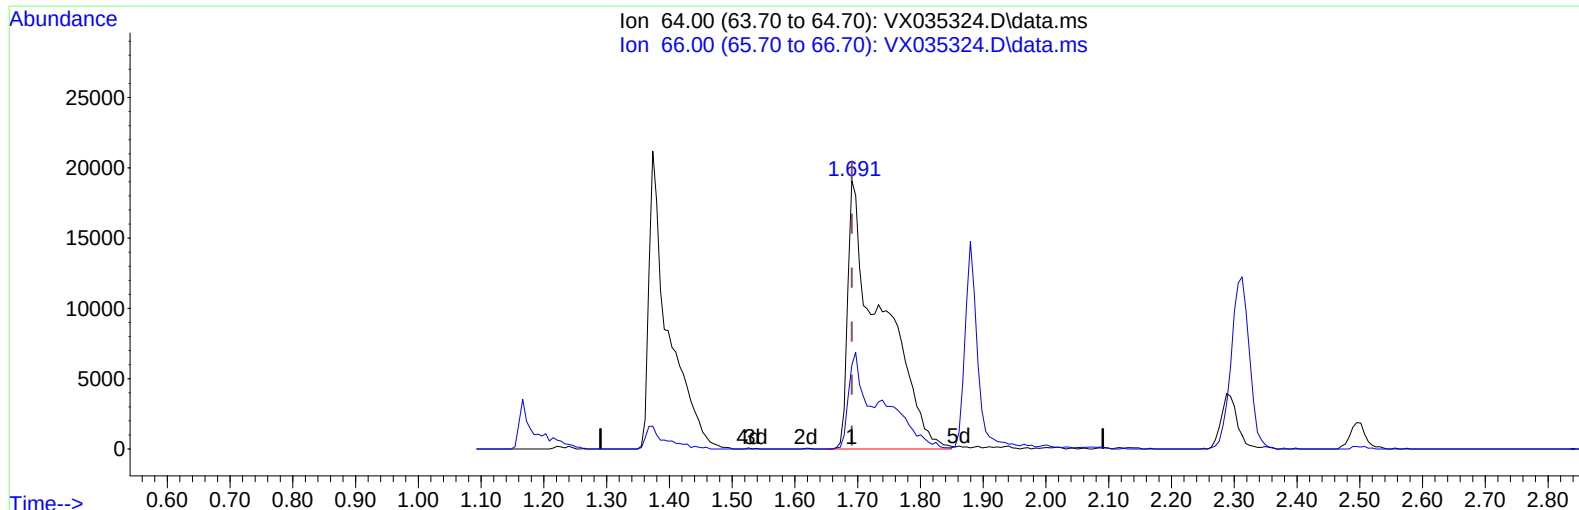

TIC: VX035324.D\data.ms

## (8) Chloroethane (T)

1.691min (-0.000) 38.90 ug/L m

response 71808

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 64.00 | 100.00 | 100.00 |
| 66.00 | 31.30  | 31.28  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
Data File : VX035324.D  
Acq On : 26 Apr 2023 19:26  
Operator : JC/MD  
Sample : 02419-12MSD  
Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML041823WMA.M  
Quant Title : VOC Analysis  
QLast Update : Tue Apr 25 03:03:54 2023  
Response via : Initial Calibration

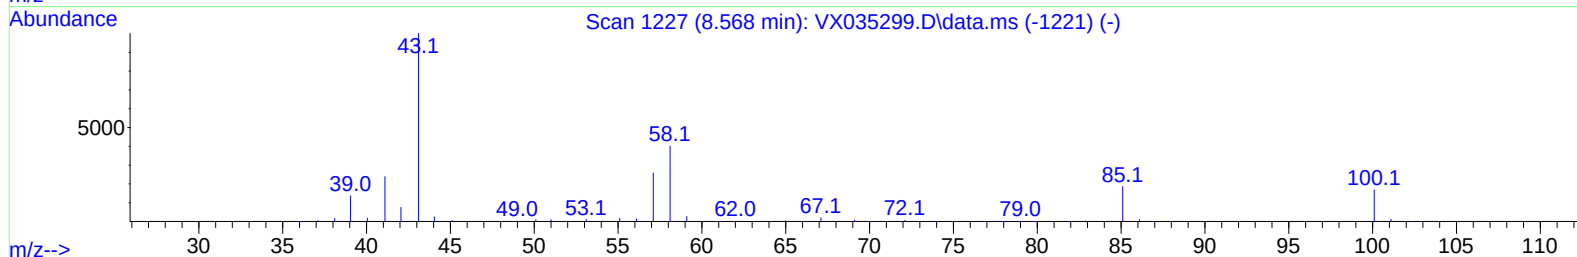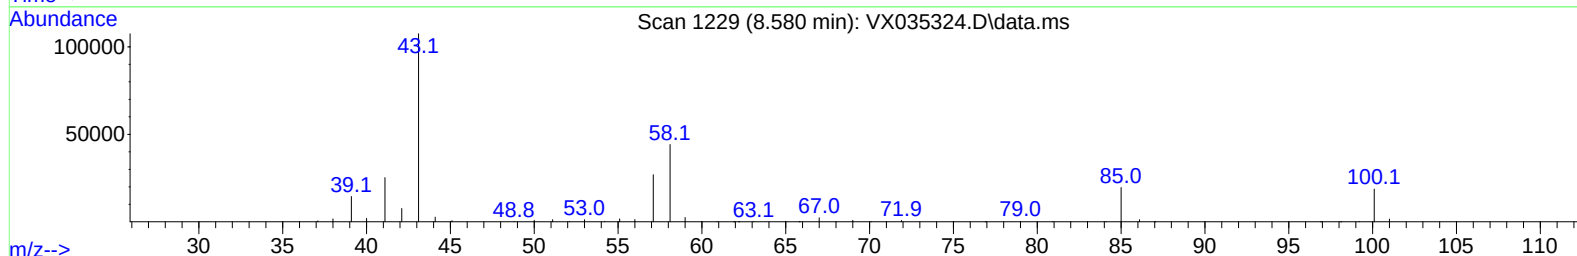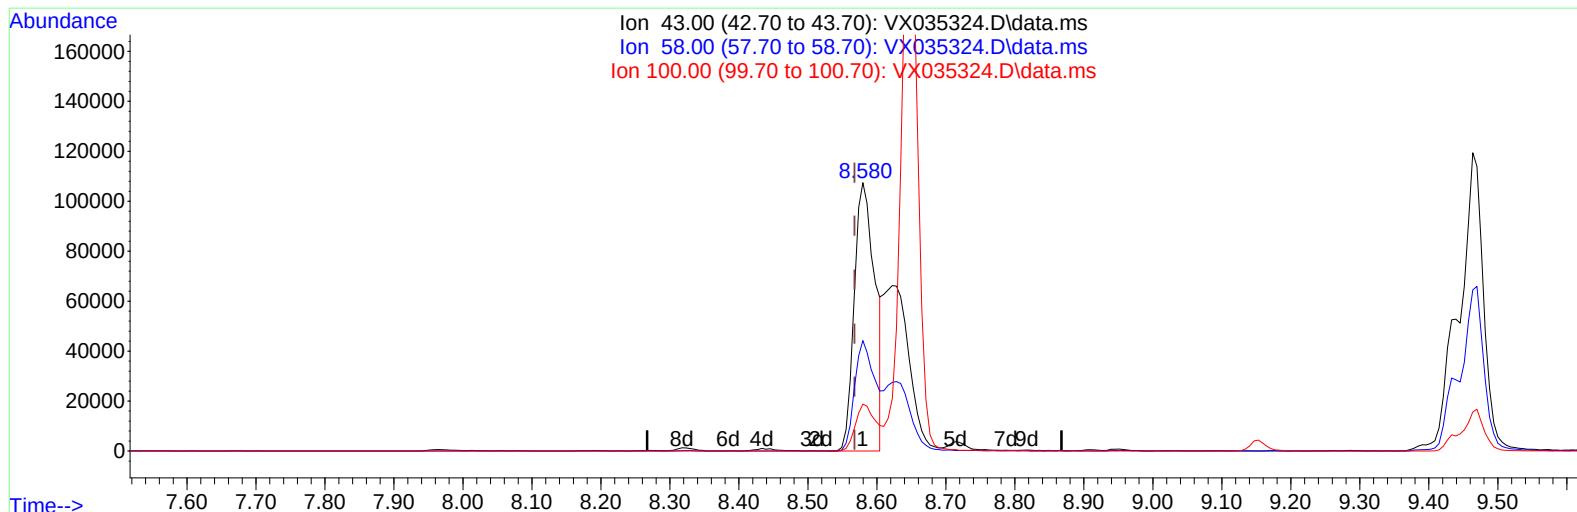

TIC: VX035324.D\data.ms

## (40) 4-Methyl-2-pentanone (T)

8.580min (+ 0.012) 52.23 ug/L

response 224308

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 43.00  | 100.00 | 100.00 |
| 58.00  | 39.40  | 40.18  |
| 100.00 | 16.00  | 18.46  |
| 0.00   | 0.00   | 0.00   |






Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

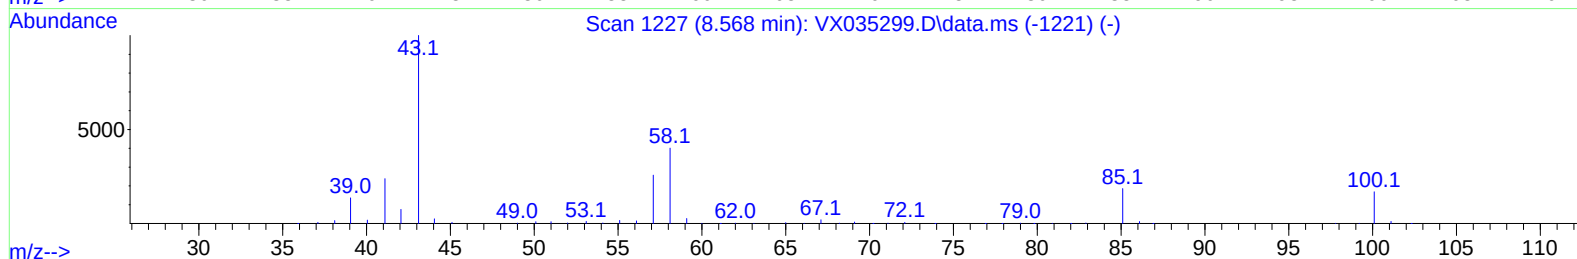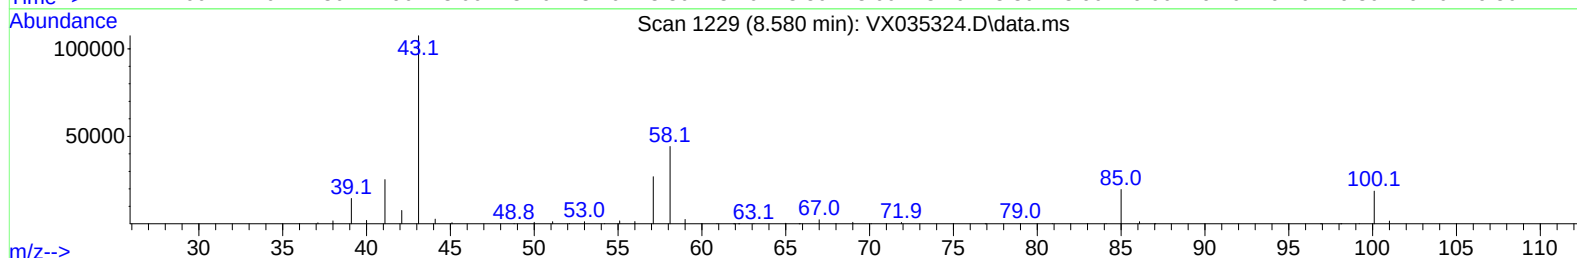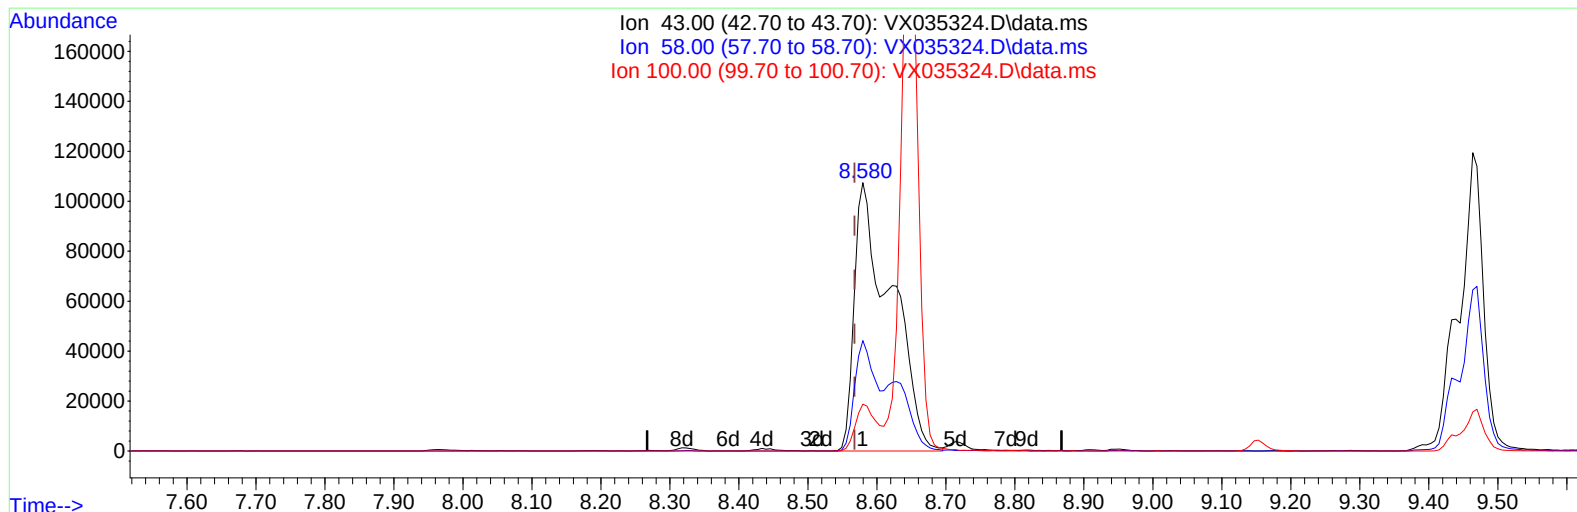

TIC: VX035324.D\data.ms

**(40) 4-Methyl-2-pentanone (T)**

8.580min (+ 0.012) 92.18 ug/L m

response 395833

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 43.00  | 100.00 | 100.00 |
| 58.00  | 39.40  | 22.77# |
| 100.00 | 16.00  | 10.46# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

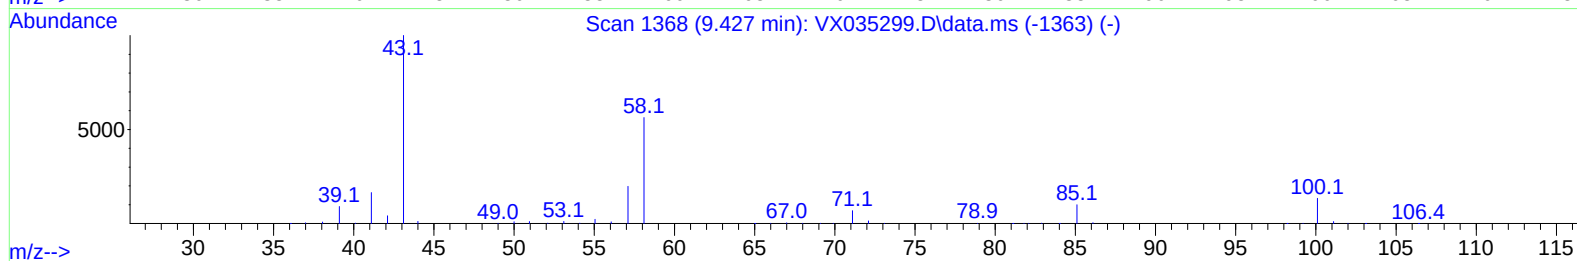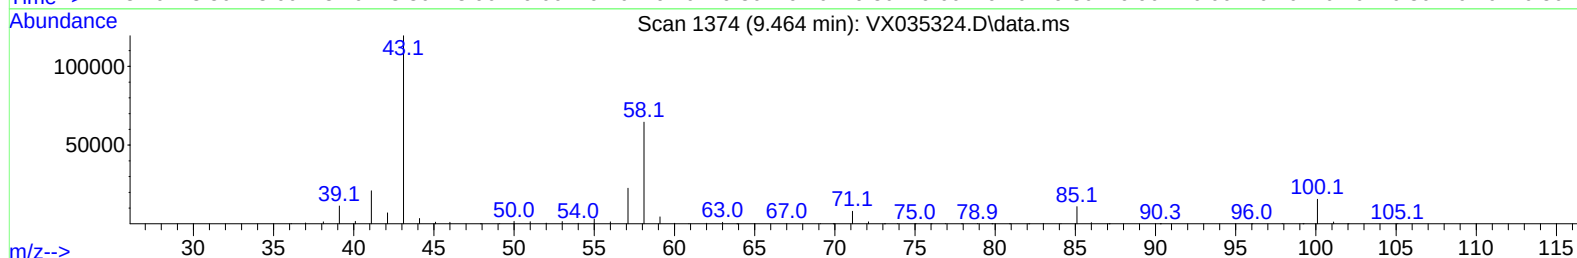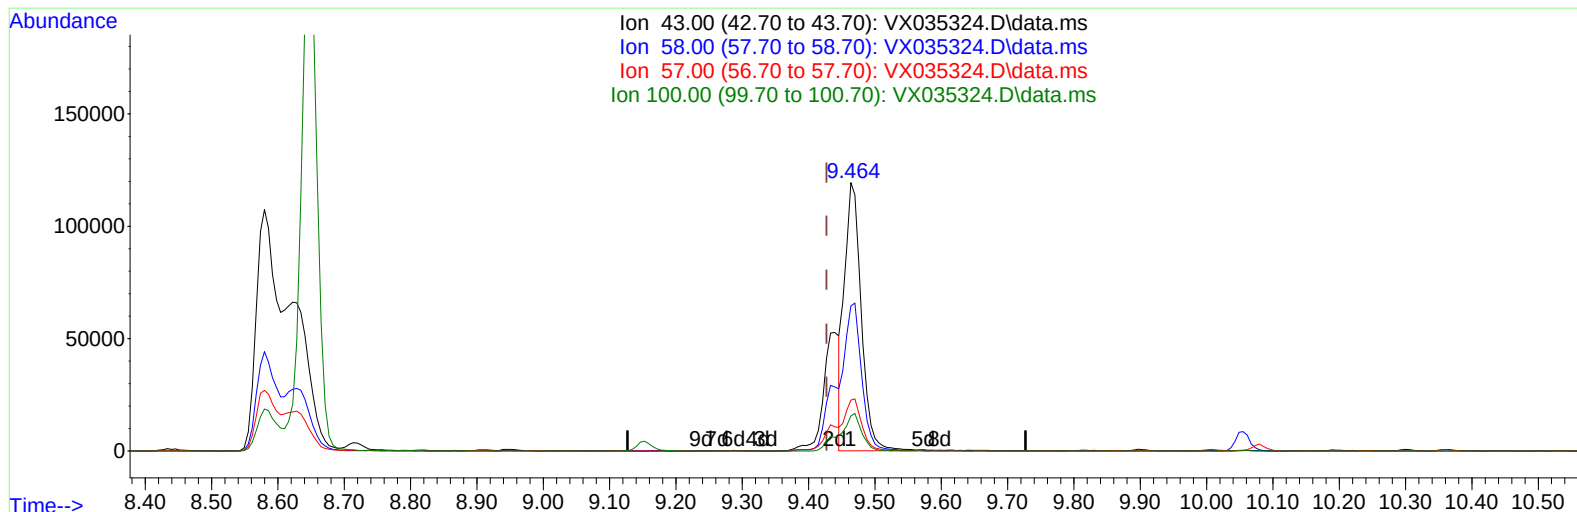

TIC: VX035324.D\data.ms

## (48) 2-Hexanone (T)

9.464min (+ 0.037) 64.41 ug/L

response 210001

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 43.00  | 100.00 | 100.00 |
| 58.00  | 54.00  | 56.51  |
| 57.00  | 19.20  | 20.01  |
| 100.00 | 12.50  | 14.71  |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

Manual IntegrationsAPPROVED

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

| Compound                      | R.T.           | QIon | Response   | Conc     | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|--------|----------|
| -----                         |                |      |            |          |        |          |
| Internal Standards            |                |      |            |          |        |          |
| 1) 1,4-Difluorobenzene        | 6.757          | 114  | 467580     | 50.000   | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 10.055         | 117  | 408572     | 50.000   | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 208092     | 50.000   | ug/L   | 0.00     |
| System Monitoring Compounds   |                |      |            |          |        |          |
| 4) Vinyl Chloride-d3          | 1.368          | 65   | 124144     | 41.176   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 135 |      | Recovery = | 82.360%  |        |          |
| 7) Chloroethane-d5            | 1.672          | 69   | 85387m     | 39.194   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 130 |      | Recovery = | 78.380%  |        |          |
| 11) 1,1-Dichloroethene-d2     | 2.288          | 65   | 64808      | 44.924   | ug/L   | -0.02    |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 89.840%  |        |          |
| 21) 2-Butanone-d5             | 4.489          | 46   | 167085     | 83.162   | ug/L   | 0.03     |
| Spiked Amount 100.000         | Range 40 - 130 |      | Recovery = | 83.160%  |        |          |
| 24) Chloroform-d              | 5.056          | 84   | 274877     | 48.413   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 96.820%  |        |          |
| 26) 1,2-Dichloroethane-d4     | 5.952          | 65   | 174185     | 47.773   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 95.540%  |        |          |
| 32) Benzene-d6                | 5.970          | 84   | 576014     | 49.078   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = | 98.160%  |        |          |
| 36) 1,2-Dichloropropane-d6    | 7.305          | 67   | 173776     | 48.471   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 120 |      | Recovery = | 96.940%  |        |          |
| 41) Toluene-d8                | 8.647          | 98   | 530565     | 49.463   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 98.920%  |        |          |
| 43) trans-1,3-Dichloroprop... | 8.952          | 79   | 79009      | 50.428   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = | 100.860% |        |          |
| 47) 2-Hexanone-d5             | 9.421          | 63   | 124238     | 86.295   | ug/L   | 0.04     |
| Spiked Amount 100.000         | Range 45 - 130 |      | Recovery = | 86.290%  |        |          |
| 56) 1,1,2,2-Tetrachloroeth... | 11.201         | 84   | 204822     | 46.650   | ug/L   | 0.01     |
| Spiked Amount 50.000          | Range 65 - 120 |      | Recovery = | 93.300%  |        |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.323         | 152  | 197383     | 48.947   | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = | 97.900%  |        |          |
| Target Compounds              |                |      |            |          |        |          |
|                               |                |      |            |          | Qvalue |          |
| 2) Dichlorodifluoromethane    | 1.166          | 85   | 163897m    | 46.770   | ug/L   |          |
| 3) Chloromethane              | 1.294          | 50   | 133143     | 41.749   | ug/L   | 98       |
| 5) Vinyl chloride             | 1.374          | 62   | 134685     | 40.696   | ug/L   | 100      |
| 6) Bromomethane               | 1.617          | 94   | 80043      | 40.722   | ug/L   | 99       |
| 8) Chloroethane               | 1.691          | 64   | 71808m     | 38.904   | ug/L   |          |
| 9) Trichlorofluoromethane     | 1.880          | 101  | 166457     | 37.142   | ug/L   | 99       |
| 10) 1,1,2-Trichloro-1,2,2-... | 2.312          | 101  | 154198     | 50.363   | ug/L   | 98       |
| 12) 1,1-Dichloroethene        | 2.300          | 96   | 131374     | 47.029   | ug/L   | 98       |
| 13) Acetone                   | 2.416          | 43   | 120007     | 80.533   | ug/L   | 100      |
| 14) Carbon disulfide          | 2.495          | 76   | 274859     | 39.824   | ug/L   | 100      |
| 15) Methyl Acetate            | 2.715          | 43   | 153035     | 47.941   | ug/L   | 97       |
| 16) Methylene chloride        | 2.782          | 84   | 153779     | 49.440   | ug/L   | 94       |
| 17) trans-1,2-Dichloroethene  | 3.081          | 96   | 139708     | 48.568   | ug/L   | 98       |
| 18) Methyl tert-butyl Ether   | 3.117          | 73   | 510445     | 51.311   | ug/L   | 99       |
| 19) 1,1-Dichloroethane        | 3.605          | 63   | 269755     | 48.648   | ug/L   | 99       |
| 20) cis-1,2-Dichloroethene    | 4.483          | 96   | 167248     | 49.730   | ug/L   | 98       |
| 22) 2-Butanone                | 4.586          | 43   | 195496     | 85.471   | ug/L   | 99       |
| 23) Bromochloromethane        | 4.897          | 128  | 82629      | 49.606   | ug/L   | 95       |
| 25) Chloroform                | 5.092          | 83   | 286116     | 50.892   | ug/L   | 98       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXMLM041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| 27) 1,2-Dichloroethane        | 6.086  | 62   | 222433   | 49.397 | ug/L  | 99       |
| 29) Cyclohexane               | 5.458  | 56   | 255945   | 51.846 | ug/L  | 98       |
| 30) 1,1,1-Trichloroethane     | 5.379  | 97   | 238637   | 49.800 | ug/L  | 97       |
| 31) Carbon tetrachloride      | 5.672  | 117  | 201035   | 49.476 | ug/L  | 98       |
| 33) Benzene                   | 6.031  | 78   | 612835   | 49.530 | ug/L  | 100      |
| 34) Trichloroethene           | 7.123  | 95   | 163715   | 49.741 | ug/L  | 98       |
| 35) Methylcyclohexane         | 7.379  | 83   | 268411   | 60.554 | ug/L  | 98       |
| 37) 1,2-Dichloropropane       | 7.427  | 63   | 162417   | 49.858 | ug/L  | 99       |
| 38) Bromodichloromethane      | 7.824  | 83   | 187430   | 48.696 | ug/L  | 97       |
| 39) cis-1,3-Dichloropropene   | 8.366  | 75   | 251444   | 51.622 | ug/L  | 99       |
| 40) 4-Methyl-2-pentanone      | 8.580  | 43   | 395833m  | 92.177 | ug/L  |          |
| 42) Toluene                   | 8.720  | 91   | 661246   | 51.510 | ug/L  | 98       |
| 44) trans-1,3-Dichloropropene | 8.976  | 75   | 229581   | 52.310 | ug/L  | 100      |
| 45) 1,1,2-Trichloroethane     | 9.153  | 97   | 160111   | 51.796 | ug/L  | 97       |
| 46) Tetrachloroethene         | 9.275  | 164  | 134958   | 55.046 | ug/L  | 98       |
| 48) 2-Hexanone                | 9.464  | 43   | 299208m  | 91.770 | ug/L  |          |
| 49) Dibromochloromethane      | 9.525  | 129  | 147617   | 50.249 | ug/L  | 100      |
| 50) 1,2-Dibromoethane         | 9.610  | 107  | 167690   | 52.135 | ug/L  | 99       |
| 51) Chlorobenzene             | 10.079 | 112  | 432791   | 51.173 | ug/L  | 98       |
| 52) Ethylbenzene              | 10.195 | 91   | 746872   | 52.631 | ug/L  | 100      |
| 53) m,p-Xylene                | 10.305 | 106  | 289292   | 53.237 | ug/L  | 95       |
| 54) o-Xylene                  | 10.640 | 106  | 280840   | 52.567 | ug/L  | 94       |
| 55) Styrene                   | 10.659 | 104  | 470833   | 52.016 | ug/L  | 97       |
| 57) 1,1,2,2-Tetrachloroethane | 11.219 | 83   | 222167   | 48.767 | ug/L  | 99       |
| 59) Bromoform                 | 10.811 | 173  | 97660    | 45.591 | ug/L  | 100      |
| 60) Isopropylbenzene          | 10.963 | 105  | 759088   | 53.647 | ug/L  | 99       |
| 61) 1,2,3-Trichloropropane    | 11.250 | 75   | 175162   | 45.592 | ug/L  | 99       |
| 62) 1,3,5-Trimethylbenzene    | 11.451 | 105  | 640580   | 55.358 | ug/L  | 100      |
| 63) 1,2,4-Trimethylbenzene    | 11.756 | 105  | 636494   | 55.318 | ug/L  | 100      |
| 64) 1,3-Dichlorobenzene       | 11.975 | 146  | 338201   | 52.407 | ug/L  | 98       |
| 65) 1,4-Dichlorobenzene       | 12.042 | 146  | 340493   | 51.563 | ug/L  | 97       |
| 67) 1,2-Dichlorobenzene       | 12.341 | 146  | 330356   | 50.487 | ug/L  | 99       |
| 68) 1,2-Dibromo-3-chloropr... | 12.945 | 75   | 40396    | 42.612 | ug/L  | 98       |
| 69) 1,3,5-Trichlorobenzene    | 13.115 | 180  | 246319   | 61.741 | ug/L  | 100      |
| 70) 1,2,4-trichlorobenzene    | 13.591 | 180  | 232044   | 62.116 | ug/L  | 100      |
| 71) Naphthalene               | 13.774 | 128  | 726013   | 54.560 | ug/L  | 100      |
| 72) 1,2,3-Trichlorobenzene    | 13.963 | 180  | 223175   | 60.516 | ug/L  | 98       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042623\  
 Data File : VX035324.D  
 Acq On : 26 Apr 2023 19:26  
 Operator : JC/MD  
 Sample : 02419-12MSD  
 Misc : 4.88g/5mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 27 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EW925MSD

## Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/27/2023  
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 27 04:44:11 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML041823WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Apr 25 03:03:54 2023  
 Response via : Initial Calibration

