

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035318.D
 Acq On : 26 Apr 2023 17:07
 Operator : JC/MD
 Sample : 02479-15ME
 Misc : 4.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW974ME

Quant Time: Apr 27 04:43:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 25 03:03:54 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 04/27/2023
 Supervised By : Mahesh Dadoda 05/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	439231	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	378426	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	190042	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	83297m	29.411	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	58.820%#		
7) Chloroethane-d5	1.672	69	58816m	28.740	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	57.480%#		
11) 1,1-Dichloroethene-d2	2.288	65	46628	34.408	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.820%		
21) 2-Butanone-d5	4.483	46	175185	92.821	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.820%		
24) Chloroform-d	5.056	84	216444	40.582	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.160%		
26) 1,2-Dichloroethane-d4	5.952	65	153629	44.855	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.700%		
32) Benzene-d6	5.970	84	481356	44.280	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.560%		
36) 1,2-Dichloropropane-d6	7.305	67	151872	45.736	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.480%		
41) Toluene-d8	8.647	98	437034	43.989	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.980%		
43) trans-1,3-Dichloroprop...	8.951	79	54243	37.379	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.760%		
47) 2-Hexanone-d5	9.415	63	124672m	93.494	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.490%		
56) 1,1,2,2-Tetrachloroeth...	11.201	84	186214	45.790	ug/L	0.01
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.580%		
66) 1,2-Dichlorobenzene-d4	12.323	152	173892	47.217	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.440%		
Target Compounds						Qvalue
15) Methyl Acetate	2.715	43	4260	1.421	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035318.D
Acq On : 26 Apr 2023 17:07
Operator : JC/MD
Sample : 02479-15ME
Misc : 4.63g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
EW974ME

Quant Time: Apr 27 04:43:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 25 03:03:54 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 04/27/2023
Supervised By : Mahesh Dadoda 05/01/2023

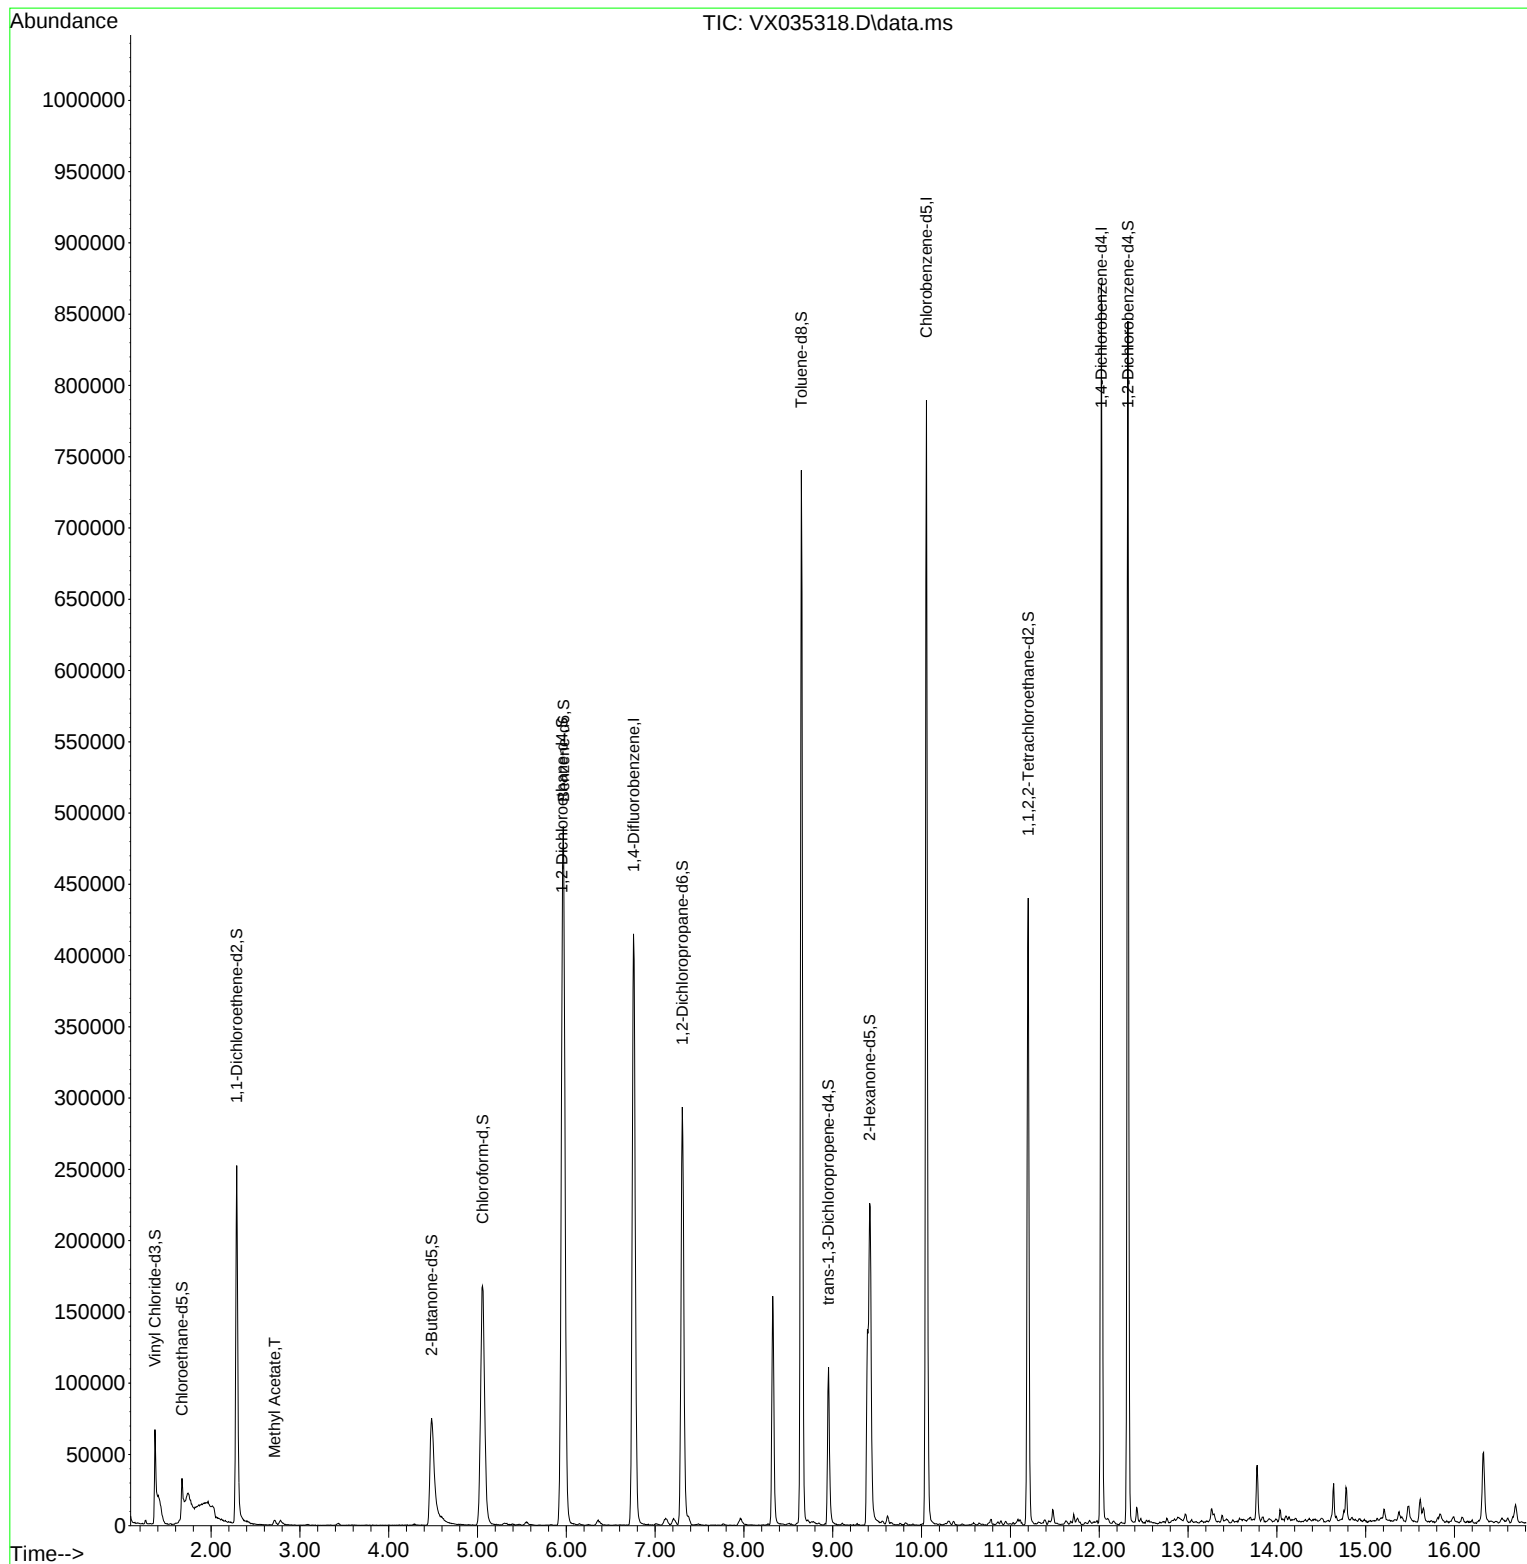

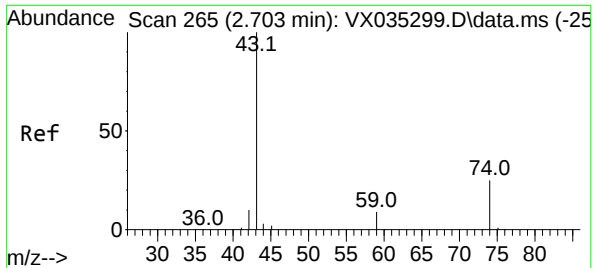

#15
Methyl Acetate
Concen: 1.421 ug/L
RT: 2.715 min Scan# 20
Delta R.T. 0.012 min
Lab File: VX035318.D
Acq: 26 Apr 2023 17:07

Instrument :
MSVOA_X
ClientSampleId :
EW974ME

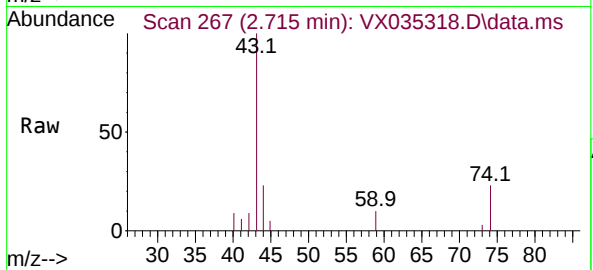

Tgt Ion: 43 Resp: 4260
Ion Ratio Lower Upper
43 100
74 20.4 18.2 27.4

Manual Integrations
APPROVED

Reviewed By :John Carlone 04/27/2023
Supervised By :Mahesh Dadoda 05/01/2023

