

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035300.D
 Acq On : 26 Apr 2023 09:56
 Operator : JC/MD
 Sample : VX0426MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

Signal : TIC: VX035300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	32	rVB3	1516	1410	0.11%	0.013%
2	1.368	42	46	58	rVB	123130	139685	10.63%	1.327%
3	1.672	91	96	107	rBV	99509	135051	10.28%	1.283%
4	2.306	194	200	211	rBV	279551	437987	33.33%	4.162%
5	2.514	230	234	241	rVB2	2193	4162	0.32%	0.040%
6	2.562	241	242	245	rBV2	230	199	0.02%	0.002%
7	2.678	257	261	262	rBV2	436	569	0.04%	0.005%
8	2.751	271	273	274	rBV	262	245	0.02%	0.002%
9	2.788	274	279	285	rVB3	2770	4752	0.36%	0.045%
10	2.867	289	292	295	rBV2	226	319	0.02%	0.003%
11	3.093	325	329	335	rBV5	1175	2554	0.19%	0.024%
12	3.203	346	347	350	rVB2	291	243	0.02%	0.002%
13	3.239	350	353	354	rBV	252	266	0.02%	0.003%
14	3.257	354	356	358	rVB2	211	183	0.01%	0.002%
15	3.355	369	372	374	rVB3	234	290	0.02%	0.003%
16	3.538	400	402	405	rBV2	162	139	0.01%	0.001%
17	3.611	412	414	415	rVB2	398	277	0.02%	0.003%
18	3.635	415	418	421	rVB2	204	233	0.02%	0.002%
19	3.721	429	432	433	rBV	192	223	0.02%	0.002%
20	3.831	446	450	454	rBV2	188	315	0.02%	0.003%
21	3.995	475	477	479	rBV2	205	148	0.01%	0.001%
22	4.026	479	482	485	rVB2	257	235	0.02%	0.002%
23	4.056	485	487	489	rVB	272	193	0.01%	0.002%
24	4.129	497	499	501	rBV	136	150	0.01%	0.001%
25	4.294	522	526	527	rBV2	168	149	0.01%	0.001%
26	4.343	531	534	537	rBV2	267	297	0.02%	0.003%
27	4.465	544	554	577	rBV	79358	255143	19.42%	2.424%
28	4.696	590	592	593	rVB2	419	219	0.02%	0.002%
29	4.891	622	624	625	rBV	195	174	0.01%	0.002%
30	5.056	638	651	674	rVB	170184	520300	39.60%	4.944%
31	5.214	674	677	680	rBV3	489	722	0.05%	0.007%
32	5.367	697	702	704	rBV2	684	1145	0.09%	0.011%
33	5.470	717	719	721	rVB	405	295	0.02%	0.003%
34	5.495	721	723	725	rBV2	151	193	0.01%	0.002%
35	5.556	725	733	743	rVB4	2138	5758	0.44%	0.055%
36	5.964	787	800	817	rBV2	440109	1314005	100.00%	12.485%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035300.D
 Acq On : 26 Apr 2023 09:56
 Operator : JC/MD
 Sample : VX0426MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
 Title : VOC Analysis

37	6.263	847	849	852	rVB3	254	334	0.03%	0.003%
38	6.293	852	854	856	rVB2	223	138	0.01%	0.001%
39	6.440	876	878	881	rBV2	182	233	0.02%	0.002%
40	6.757	920	930	946	rBV	436758	1033767	78.67%	9.822%
41	7.110	979	988	1002	rVB6	4489	11645	0.89%	0.111%
42	7.306	1011	1020	1034	rBV	276312	601181	45.75%	5.712%
43	7.488	1045	1050	1055	rVB4	732	1014	0.08%	0.010%
44	7.824	1102	1105	1106	rBV	174	207	0.02%	0.002%
45	7.940	1120	1124	1127	rBV4	1042	1710	0.13%	0.016%
46	8.074	1145	1146	1149	rVB2	171	150	0.01%	0.001%
47	8.104	1149	1151	1154	rBV2	186	151	0.01%	0.001%
48	8.324	1181	1187	1203	rBV	172955	282419	21.49%	2.683%
49	8.494	1211	1215	1216	rBV3	786	1041	0.08%	0.010%
50	8.580	1226	1229	1233	rBV2	307	493	0.04%	0.005%
51	8.647	1233	1240	1251	rBV	677470	1069981	81.43%	10.166%
52	8.952	1284	1290	1306	rBV	113767	179277	13.64%	1.703%
53	9.275	1339	1343	1348	rVB2	1417	1875	0.14%	0.018%
54	9.311	1348	1349	1354	rVB2	216	224	0.02%	0.002%
55	9.384	1356	1361	1379	rBV	381487	552069	42.01%	5.246%
56	9.866	1438	1440	1442	rBV	222	189	0.01%	0.002%
57	9.933	1447	1451	1453	rVB2	254	285	0.02%	0.003%
58	9.957	1453	1455	1457	rBV2	121	155	0.01%	0.001%
59	10.055	1465	1471	1491	rVV	826821	1165705	88.71%	11.076%
60	10.195	1491	1494	1499	rVV4	1374	2159	0.16%	0.021%
61	10.238	1499	1501	1504	rVB2	425	439	0.03%	0.004%
62	10.305	1509	1512	1518	rVB3	1254	1929	0.15%	0.018%
63	10.403	1527	1528	1530	rBV2	257	200	0.02%	0.002%
64	10.524	1547	1548	1551	rBV	168	146	0.01%	0.001%
65	10.604	1559	1561	1562	rBV	179	144	0.01%	0.001%
66	10.652	1563	1569	1576	rVV5	1755	3947	0.30%	0.038%
67	10.860	1602	1603	1607	rVB	229	197	0.01%	0.002%
68	10.902	1607	1610	1613	rBV2	244	301	0.02%	0.003%
69	10.963	1616	1620	1624	rBV	2000	2358	0.18%	0.022%
70	11.085	1636	1640	1646	rBV4	934	1630	0.12%	0.015%
71	11.189	1652	1657	1668	rBV	485351	604702	46.02%	5.746%
72	11.366	1685	1686	1690	rVB2	238	195	0.01%	0.002%
73	11.451	1697	1700	1707	rVB3	1638	2677	0.20%	0.025%
74	11.549	1715	1716	1717	rBV	264	144	0.01%	0.001%
75	11.756	1746	1750	1756	rVB	1823	2641	0.20%	0.025%
76	11.969	1781	1785	1788	rBV2	3596	4310	0.33%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
 Data File : VX035300.D
 Acq On : 26 Apr 2023 09:56
 Operator : JC/MD
 Sample : VX0426MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK628

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1808	rVV	881255	1153102	87.75%	10.956%
78	12.317	1837	1842	1856	rBV	743703	969701	73.80%	9.214%
79	12.457	1863	1865	1867	rBV	328	366	0.03%	0.003%
80	12.658	1896	1898	1900	rBV2	280	243	0.02%	0.002%
81	12.762	1912	1915	1918	rBV	852	810	0.06%	0.008%
82	13.115	1966	1973	1979	rBV2	4772	6184	0.47%	0.059%
83	13.457	2027	2029	2031	rBV	151	143	0.01%	0.001%
84	13.500	2034	2036	2038	rBV	192	167	0.01%	0.002%
85	13.591	2047	2051	2062	rVB3	6489	8920	0.68%	0.085%
86	13.670	2062	2064	2068	rVB	393	300	0.02%	0.003%
87	13.737	2073	2075	2076	rVB	316	170	0.01%	0.002%
88	13.780	2077	2082	2090	rVV2	7402	10124	0.77%	0.096%
89	13.865	2094	2096	2099	rVB	319	358	0.03%	0.003%
90	13.963	2107	2112	2117	rBV3	6142	8198	0.62%	0.078%
91	14.103	2134	2135	2136	rBV	472	257	0.02%	0.002%
92	14.127	2136	2139	2144	rVB3	1039	1617	0.12%	0.015%
93	14.207	2150	2152	2154	rVB	439	241	0.02%	0.002%
94	14.268	2160	2162	2167	rVB2	359	448	0.03%	0.004%
95	14.310	2167	2169	2170	rBV2	279	223	0.02%	0.002%
96	14.353	2174	2176	2179	rBV3	226	200	0.02%	0.002%
97	14.957	2274	2275	2278	rBV2	508	615	0.05%	0.006%
98	15.194	2312	2314	2317	rVB2	549	459	0.03%	0.004%
99	15.706	2396	2398	2402	rBV4	669	729	0.06%	0.007%
100	16.036	2450	2452	2454	rBV2	688	421	0.03%	0.004%




Sum of corrected areas: 10524586

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035300.D
Acq On : 26 Apr 2023 09:56
Operator : JC/MD
Sample : VX0426MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

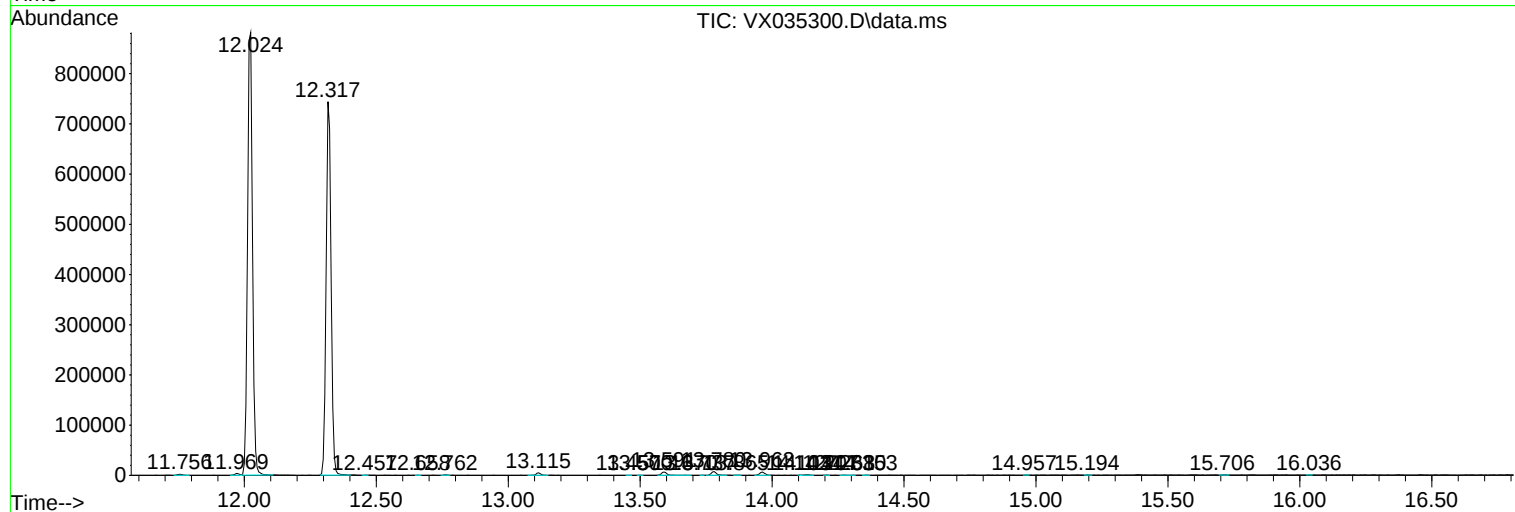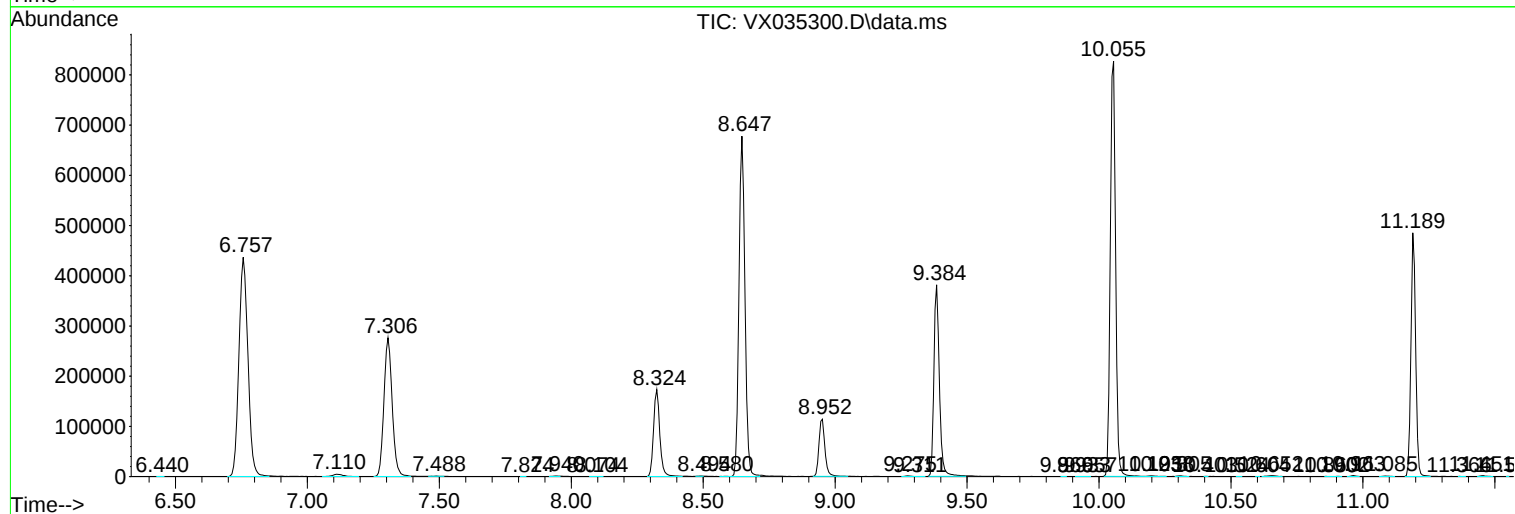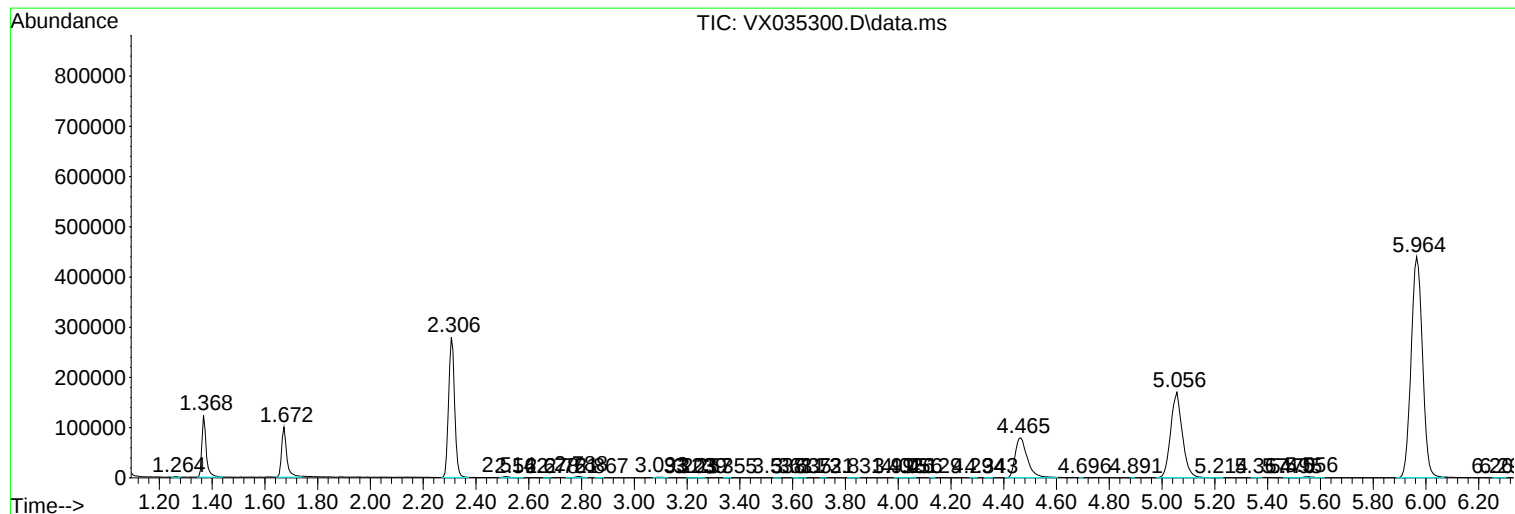

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035300.D
Acq On : 26 Apr 2023 09:56
Operator : JC/MD
Sample : VX0426MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035300.D
Acq On : 26 Apr 2023 09:56
Operator : JC/MD
Sample : VX0426MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK628

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041823WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------