
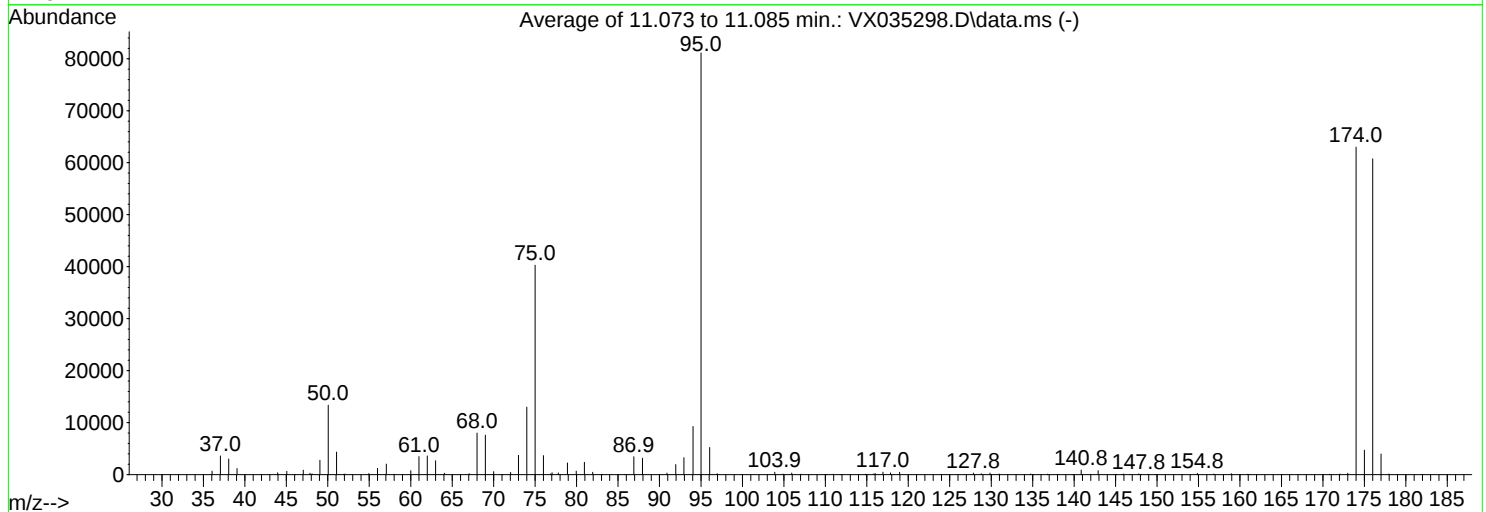


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042623\
Data File : VX035298.D
Acq On : 26 Apr 2023 08:29
Operator : JC/MD
Sample : BFB627
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB627

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041823WMA.M
Title : VOC Analysis
Last Update : Tue Apr 25 03:03:54 2023

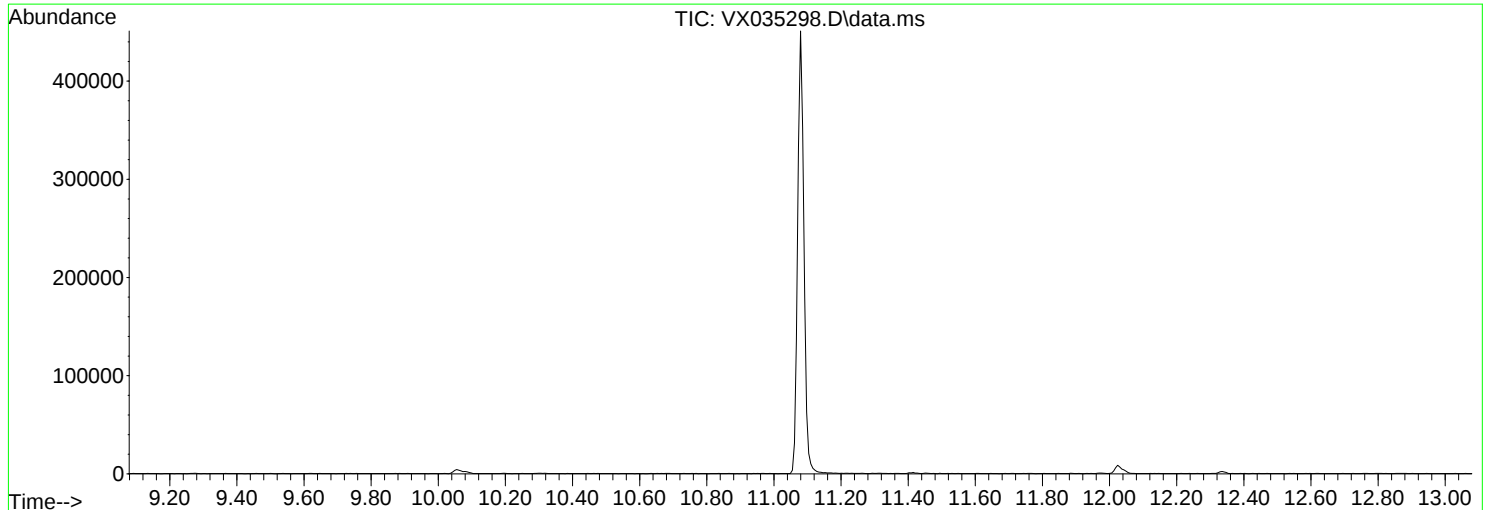

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	13363	PASS
75	95	30	80	49.7	40293	PASS
95	95	100	100	100.0	81133	PASS
96	95	5	9	6.4	5232	PASS
173	174	0.00	2	0.4	269	PASS
174	95	50	120	77.7	63000	PASS
175	174	5	9	7.5	4723	PASS
176	174	95	101	96.4	60744	PASS
177	176	5	9	6.6	3979	PASS

m/z	Abundance
39.90	219.0
43.80	114.0

Instrument :
MSVOA_X
ClientSampleId :
BFB627

m/z	Abundance
36.00	676.0
37.10	3770.0
38.10	3191.0
39.10	1069.0
40.00	236.0
44.00	531.0
45.00	705.0
47.10	914.0
47.80	502.0
49.00	2645.0
50.00	13299.0
51.00	4325.0
51.90	185.0
55.10	160.0
56.00	1100.0
57.00	1984.0
60.00	698.0
61.00	3200.0
62.00	3547.0
63.00	2324.0
64.00	254.0
65.00	88.0
67.00	146.0
68.00	7637.0
69.00	7501.0
70.00	589.0
72.10	339.0
73.00	3545.0
74.00	11635.0
75.00	37480.0
76.00	3420.0
76.90	480.0
77.80	339.0
78.90	2081.0
79.90	674.0
81.00	2079.0
81.90	456.0
86.20	74.0
86.90	3217.0
88.00	3044.0
91.00	344.0
92.00	1635.0
92.90	3286.0
94.00	8892.0
95.00	75280.0
96.00	5059.0
96.90	104.0
103.80	322.0
104.90	116.0
106.00	264.0
107.00	96.0
111.00	79.0
114.90	106.0
115.80	411.0
116.90	330.0
117.80	361.0
118.90	499.0
127.90	313.0
128.80	138.0
130.00	227.0
131.00	70.0
134.80	72.0
136.80	137.0
139.80	66.0
140.90	685.0
142.00	93.0
142.90	698.0
144.90	67.0
145.00	68.0
145.80	125.0
148.10	157.0
149.00	70.0
153.00	74.0
154.80	183.0
156.80	80.0
159.00	221.0
161.00	132.0
170.80	73.0
174.00	47920.0
175.00	3862.0
176.00	46640.0
177.00	3484.0
178.00	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB627

m/z	Abundance
36.00	876.0
37.10	3925.0
38.00	3856.0
39.00	1386.0
40.00	113.0
44.00	589.0
45.10	790.0
46.10	65.0
47.00	1001.0
48.10	492.0
49.00	3008.0
50.10	15313.0
51.10	5159.0
52.10	163.0
54.90	232.0
56.00	1628.0
57.00	2433.0
58.00	145.0
60.10	970.0
61.00	4167.0
62.00	4133.0
63.00	3344.0
64.10	351.0
65.00	91.0
67.00	212.0
68.00	9667.0
69.00	8942.0
70.00	645.0
71.10	60.0
72.10	583.0
73.00	4268.0
74.00	16165.0
75.00	48616.0
76.00	4538.0
77.10	656.0
77.90	414.0
78.90	2607.0
79.90	844.0
80.90	2707.0
81.90	558.0
83.10	90.0
85.80	91.0
86.90	4646.0
88.00	3497.0
90.90	340.0
92.00	2477.0
93.00	3984.0
94.00	10357.0
95.00	94528.0
96.00	6079.0
97.00	262.0
103.90	622.0
104.90	173.0
105.90	367.0
107.10	107.0
111.00	118.0
111.90	68.0
114.90	92.0
116.00	375.0
116.90	661.0
117.90	380.0
119.00	603.0
127.90	315.0
128.80	174.0
129.80	290.0
130.90	196.0
134.70	169.0
135.10	132.0
136.80	151.0
140.80	1011.0
141.90	139.0
142.80	880.0
144.70	65.0
145.10	91.0
146.00	209.0
146.80	126.0
147.80	286.0
148.80	83.0
149.90	71.0
154.90	387.0
156.90	169.0
159.00	206.0
160.90	128.0
170.80	122.0
172.10	167.0
173.00	807.0
174.00	75440.0
175.00	5712.0
176.00	73272.0
177.00	4451.0
178.00	177.0

Instrument :
MSVOA_X
ClientSampleId :
BFB627

m/z	Abundance
36.10	519.0
37.00	3142.0
38.00	2025.0
39.00	1065.0
39.90	147.0
44.10	361.0
45.00	488.0
47.00	710.0
47.90	368.0
49.10	2640.0
50.00	11476.0
51.00	3579.0
52.00	204.0
54.90	249.0
56.10	900.0
57.10	1643.0
58.00	180.0
59.90	640.0
61.00	3064.0
62.00	3117.0
63.00	2327.0
64.10	228.0
67.10	165.0
68.00	6680.0
69.00	6344.0
70.00	553.0
71.90	408.0
73.00	3348.0
74.00	11190.0
75.00	34784.0
76.00	3009.0
77.00	427.0
77.70	290.0
78.90	2040.0
80.00	516.0
80.90	2307.0
82.00	410.0
85.70	112.0
87.00	2450.0
87.90	2933.0
90.80	235.0
91.90	1707.0
93.00	2558.0
94.10	8571.0
95.00	73592.0
96.10	4557.0
97.00	163.0
104.00	402.0
104.90	92.0
105.90	341.0
107.10	113.0
110.20	59.0
110.80	71.0
111.80	74.0
113.00	67.0
114.70	87.0
116.00	412.0
117.00	459.0
117.90	319.0
119.00	287.0
127.80	312.0
128.80	212.0
129.80	370.0
130.90	84.0
134.70	133.0
137.00	141.0
140.80	963.0
141.90	82.0
143.00	779.0
145.10	71.0
145.90	154.0
147.80	224.0
149.80	71.0
153.10	63.0
154.90	213.0
156.90	126.0
158.80	121.0
161.20	101.0
172.00	175.0
174.00	65640.0
175.00	4596.0
176.00	62320.0
177.00	4003.0
177.80	117.0

Instrument :
MSVOA_X
ClientSampleId :
BFB627