

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042624\
 Data File : VX041251.D
 Acq On : 26 Apr 2024 12:15
 Operator : JC/MD
 Sample : PB160528TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 27 02:15:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042224W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 23 05:30:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	202095	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	262778	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	227872	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	115229	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	98822	51.368	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.740%			
35) Dibromofluoromethane	5.385	113	92845	58.084	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 116.160%			
50) Toluene-d8	8.647	98	273829	50.775	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 101.560%			
62) 4-Bromofluorobenzene	11.079	95	103141	51.815	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 103.640%			
Target Compounds						
						Qvalue
3) Chloromethane	1.295	50	405	0.234	ug/l	99
5) Bromomethane	1.599	94	725	0.744	ug/l	88
10) Methyl Iodide	2.447	142	642	0.337	ug/l	# 75
11) Tert butyl alcohol	3.020	59	528	1.532	ug/l	# 78
13) Acrolein	2.233	56	114	0.295	ug/l	# 37
15) Acrylonitrile	3.087	53	266	0.302	ug/l	# 72
16) Acetone	2.392	43	39769	56.792	ug/l	94
17) Carbon Disulfide	2.508	76	973	0.316	ug/l	# 84
18) Methyl Acetate	2.709	43	2280	1.101	ug/l	# 90
20) Methylene Chloride	2.782	84	6239	3.648	ug/l	# 91
25) 2-Butanone	4.587	43	3291	2.752	ug/l	96
29) Tetrahydrofuran	5.044	42	894	1.097	ug/l	# 57
31) Cyclohexane	5.544	56	3249	1.255	ug/l	# 1
36) 1,1-Dichloropropene	5.544	75	12480	6.102	ug/l	# 50
37) Ethyl Acetate	4.739	43	2874	1.281	ug/l	# 91
38) Carbon Tetrachloride	5.544	117	17488	7.656	ug/l	# 15
41) Methacrylonitrile	5.038	41	454	0.389	ug/l	# 35
43) Isopropyl Acetate	6.342	43	98256	27.182	ug/l	99
48) Methyl methacrylate	7.799	41	84562	49.460	ug/l	# 49
49) 1,4-Dioxane	7.684	88	29	0.788	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.549	43	73473	32.473	ug/l	# 50
53) t-1,3-Dichloropropene	8.952	75	689	0.337	ug/l	# 43
54) cis-1,3-Dichloropropene	8.549	75	33631	14.489	ug/l	# 62
57) 1,3-Dichloropropane	9.482	76	4509	1.754	ug/l	# 42
59) 2-Hexanone	9.482	43	61899	35.676	ug/l	# 52
68) m/p-Xylenes	10.305	106	636	0.211	ug/l	99
74) N-amyl acetate	10.640	43	19954	7.082	ug/l	# 53
76) 1,2,3-Trichloropropane	11.079	75	52160	28.095	ug/l	# 39
81) trans-1,4-Dichloro-2-b...	11.079	75	52160	79.265	ug/l	# 5
95) Naphthalene	13.780	128	2299	0.307	ug/l	# 95
96) 1,2,3-Trichlorobenzene	13.963	180	656	0.239	ug/l	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 202095
Ion Ratio Lower Upper
168 100
99 48.3 56.6 85.0#

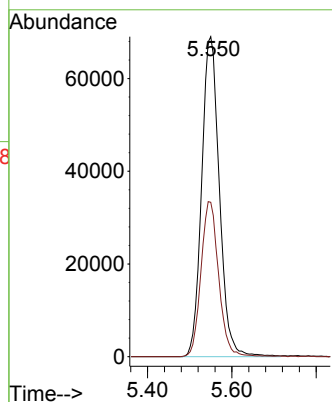

#3
Chloromethane
Concen: 0.234 ug/l
RT: 1.295 min Scan# 34
Delta R.T. -0.006 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Tgt Ion: 50 Resp: 405
Ion Ratio Lower Upper
50 100
52 32.2 25.5 38.3



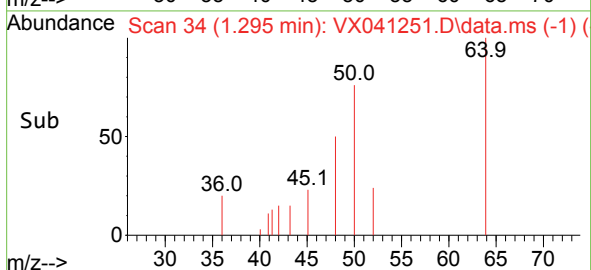



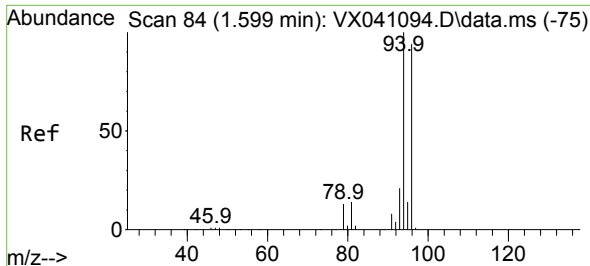

#5
Bromomethane
Concen: 0.744 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 94 Resp: 725
Ion Ratio Lower Upper
94 100
96 81.8 74.6 111.8

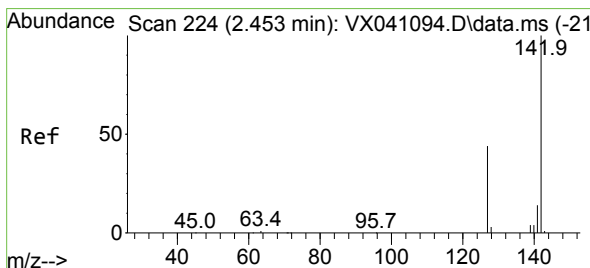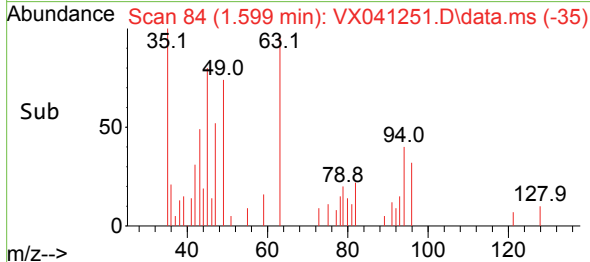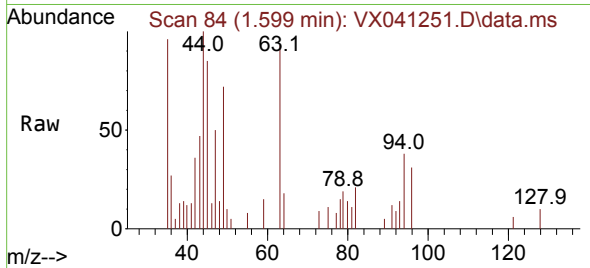

#10
Methyl Iodide
Concen: 0.337 ug/l
RT: 2.447 min Scan# 223
Delta R.T. 0.006 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Tgt Ion: 142 Resp: 642
Ion Ratio Lower Upper
142 100
127 32.6 41.6 62.4#
141 7.5 11.6 17.4#


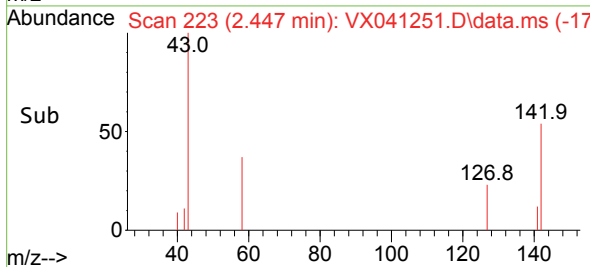

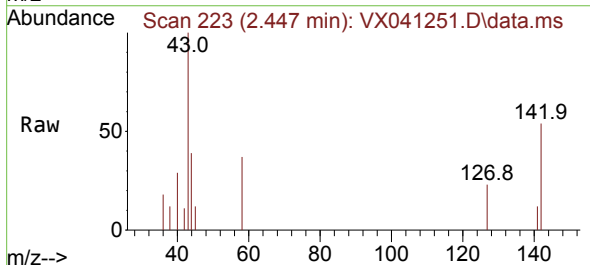




#11
Tert butyl alcohol
Concen: 1.532 ug/l
RT: 3.020 min Scan# 317
Delta R.T. -0.043 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 528
Ion Ratio Lower Upper
59 100
57 0.0 6.0 9.0#

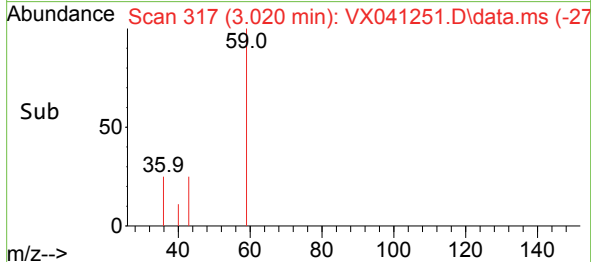

#13
Acrolein
Concen: 0.295 ug/l
RT: 2.233 min Scan# 188
Delta R.T. -0.006 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15


Tgt Ion: 56 Resp: 114
Ion Ratio Lower Upper
56 100
55 19.3 57.1 85.7#

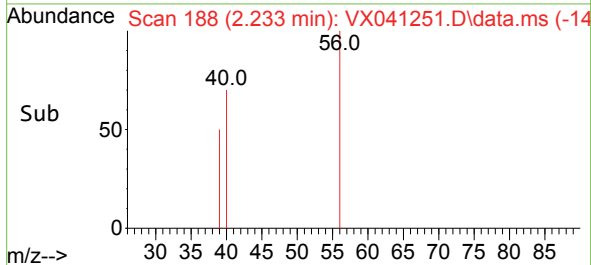






#15
Acrylonitrile
Concen: 0.302 ug/l
RT: 3.087 min Scan# 31
Delta R.T. 0.012 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 266
Ion Ratio Lower Upper
53 100
52 93.6 66.0 99.0
51 0.0 29.8 44.6#



#16
Acetone
Concen: 56.792 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Tgt Ion: 43 Resp: 39769
Ion Ratio Lower Upper
43 100
58 30.7 21.9 32.9

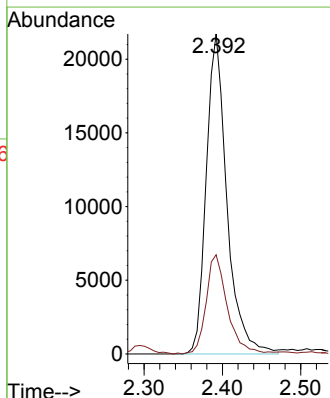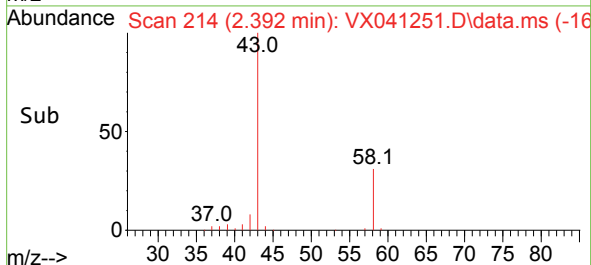



#17

Carbon Disulfide

Concen: 0.316 ug/l

RT: 2.508 min Scan# 21

Delta R.T. 0.006 min


Lab File: VX041251.D

Acq: 26 Apr 2024 12:15

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 76 Resp: 973

Ion Ratio Lower Upper

76 100

78 14.5 7.0 10.6#

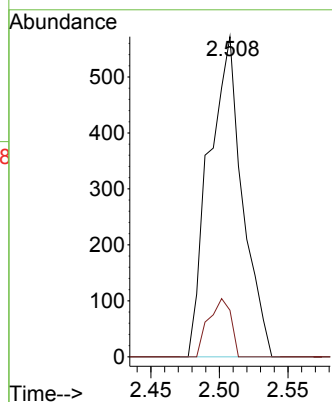

#18

Methyl Acetate

Concen: 1.101 ug/l

RT: 2.709 min Scan# 266

Delta R.T. 0.000 min

Lab File: VX041251.D




Acq: 26 Apr 2024 12:15


Tgt Ion: 43 Resp: 2280

Ion Ratio Lower Upper

43 100


74 17.4 17.8 26.8#

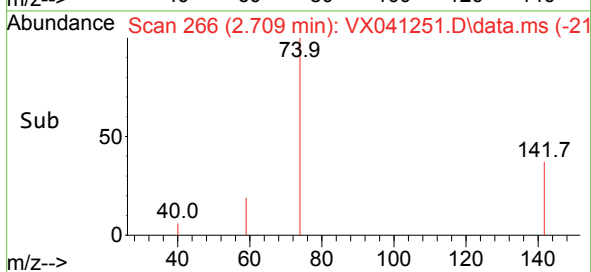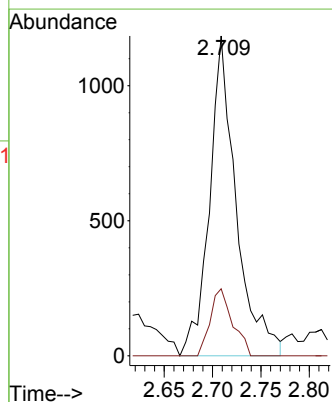






#20
Methylene Chloride
Concen: 3.648 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 84 Resp: 6239




Ion	Ratio	Lower	Upper
84	100		
49	117.3	103.6	155.4
51	31.3	33.8	50.6#
86	61.2	49.4	74.0




#25
2-Butanone
Concen: 2.752 ug/l
RT: 4.587 min Scan# 574
Delta R.T. 0.018 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Tgt Ion: 43 Resp: 3291

Ion	Ratio	Lower	Upper
43	100		
72	22.1	19.4	29.2

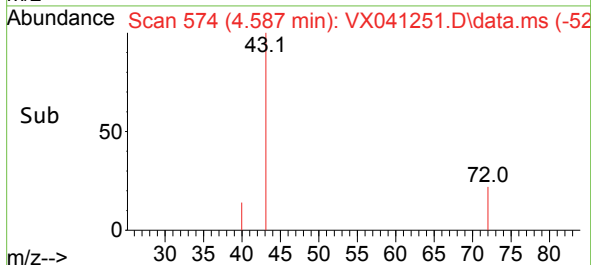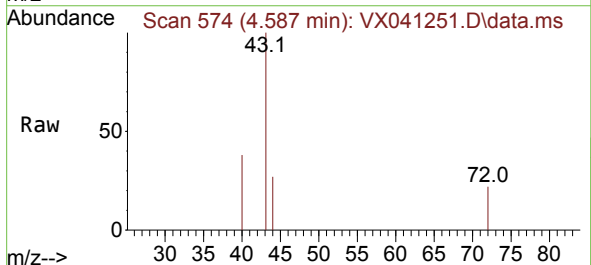



#29

Tetrahydrofuran

Concen: 1.097 ug/l

RT: 5.044 min Scan# 642

Delta R.T. 0.030 min

Lab File: VX041251.D





Acq: 26 Apr 2024 12:15

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:	42	Resp:	894
Ion	Ratio	Lower	Upper
42	100		
72	23.3	34.2	51.4#
71	5.9	32.2	48.2#



#31

Cyclohexane

Concen: 1.255 ug/l




RT: 5.544 min Scan# 731


Delta R.T. 0.079 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15

Tgt Ion:	56	Resp:	3249
Ion	Ratio	Lower	Upper
56	100		
69	181.7	23.4	35.2#
84	136.2	65.9	98.9#





#33

1,2-Dichloroethane-d4

Concen: 51.368 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 98822

Ion Ratio Lower Upper

65 100

67 50.6 0.0 100.2

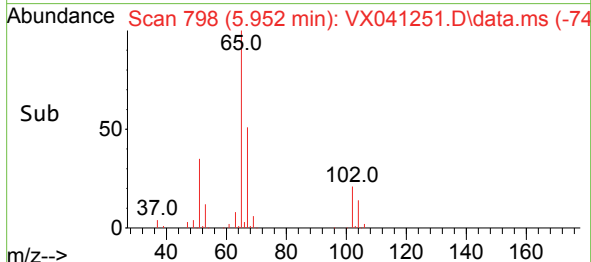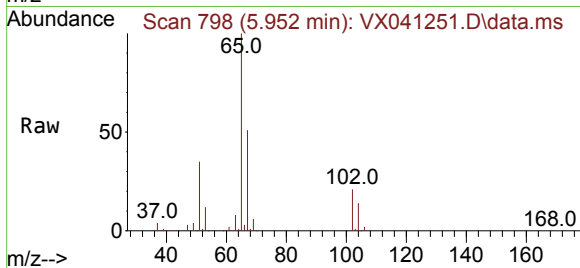

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.006 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15




Tgt Ion: 114 Resp: 262778


Ion Ratio Lower Upper

114 100

63 18.3 0.0 45.0


88 14.9 0.0 36.6

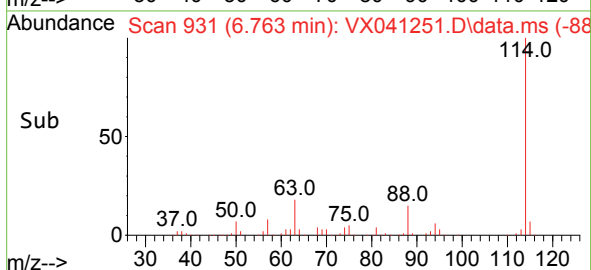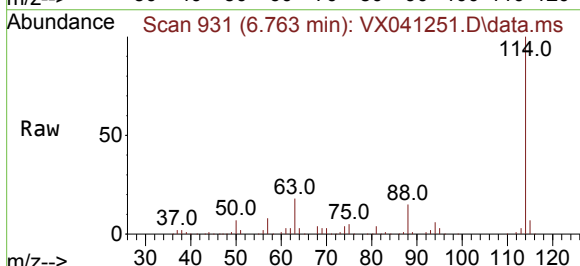



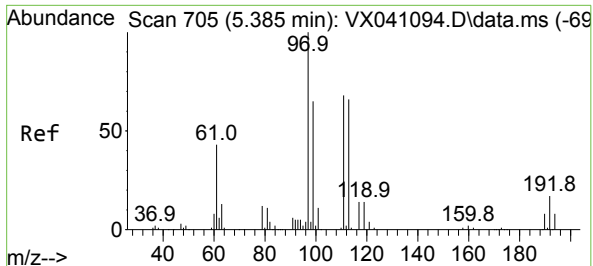


#35
Dibromofluoromethane
Concen: 58.084 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Instrument :
MSVOA_X
ClientSampleId :



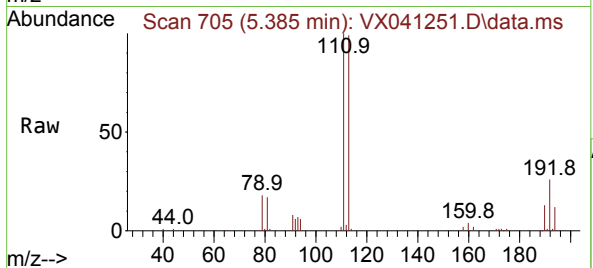



Tgt Ion:113 Resp: 92845
Ion Ratio Lower Upper
113 100
111 101.9 82.9 124.3
192 25.6 13.3 19.9#

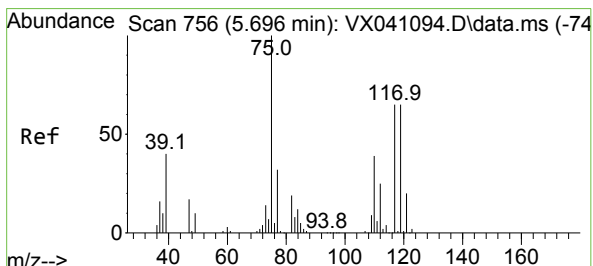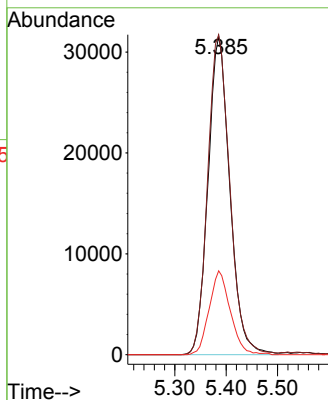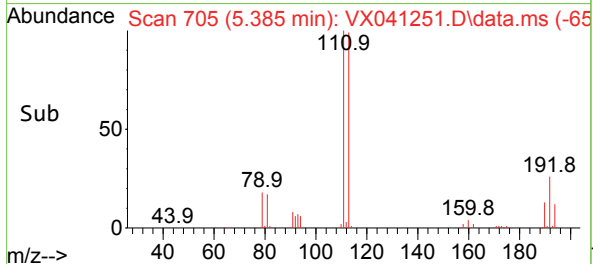

#36
1,1-Dichloropropene
Concen: 6.102 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.146 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Tgt Ion: 75 Resp: 12480
Ion Ratio Lower Upper
75 100
110 8.7 17.0 50.9#
77 0.0 24.7 37.1#


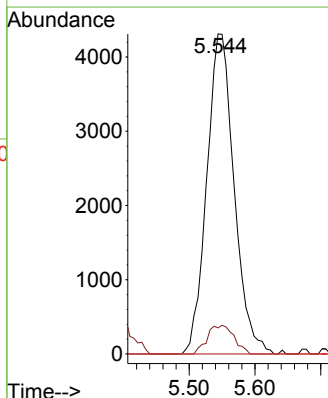
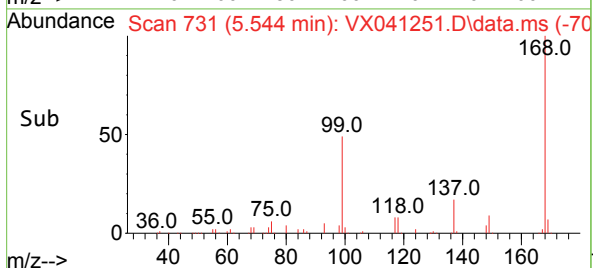
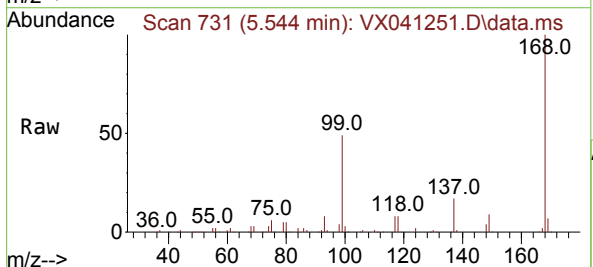




#37
Ethyl Acetate
Concen: 1.281 ug/l
RT: 4.739 min Scan# 599
Delta R.T. 0.018 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2874
Ion Ratio Lower Upper
43 100
61 9.7 10.6 16.0#
70 6.9 8.3 12.5#

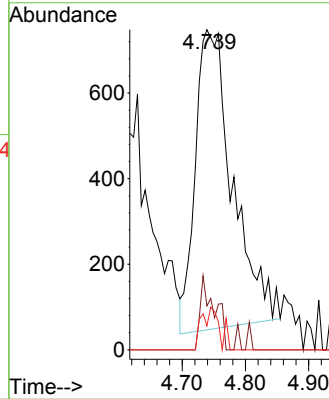

#38
Carbon Tetrachloride
Concen: 7.656 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.128 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15


Tgt Ion: 117 Resp: 17488
Ion Ratio Lower Upper
117 100
119 4.5 78.2 117.2#
121 0.0 24.4 36.6#

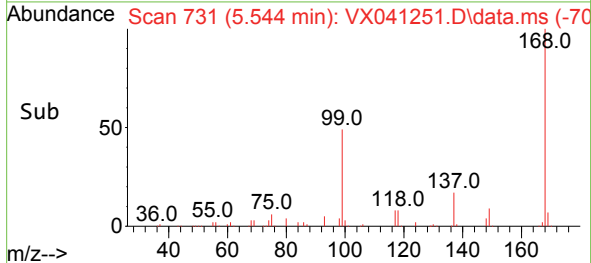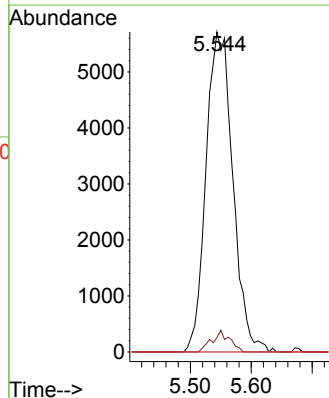






#41
Methacrylonitrile
Concen: 0.389 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.110 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:	41	Resp:	454
Ion	Ratio	Lower	Upper
41	100		
39	20.7	45.2	67.8#
67	0.0	52.6	78.8#
52	0.0	22.7	34.1#



#43
Isopropyl Acetate
Concen: 27.182 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.006 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Tgt Ion:	43	Resp:	98256
Ion	Ratio	Lower	Upper
43	100		
61	18.7	15.2	22.8
87	13.3	9.8	14.6





#48

Methyl methacrylate

Concen: 49.460 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.104 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 41 Resp: 84562

Ion Ratio Lower Upper

41 100

69 0.2 59.2 88.8#

39 55.7 47.7 71.5



#49

1,4-Dioxane

Concen: 0.788 ug/l

RT: 7.684 min Scan# 1082

Delta R.T. 0.006 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15




Tgt Ion: 88 Resp: 29


Ion Ratio Lower Upper

88 100

43 0.0 0.0 0.0

58 1541.4 60.1 90.1#



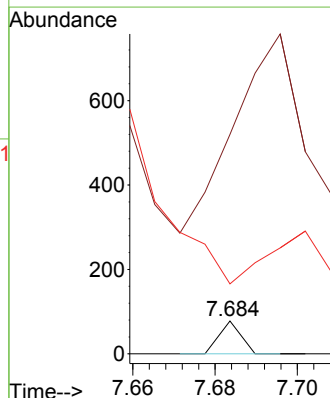





#50
Toluene-d8
Concen: 50.775 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 273829
Ion Ratio Lower Upper
98 100
100 66.0 53.1 79.7

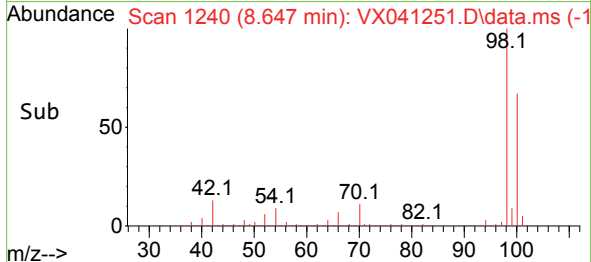

#51
4-Methyl-2-Pentanone
Concen: 32.473 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.030 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

Tgt Ion: 43 Resp: 73473
Ion Ratio Lower Upper
43 100
58 8.1 30.4 45.6#


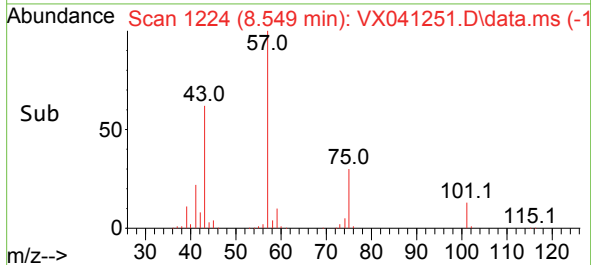






#53
 t-1,3-Dichloropropene
 Concen: 0.337 ug/l
 RT: 8.952 min Scan# 11
 Delta R.T. -0.024 min
 Lab File: VX041251.D
 Acq: 26 Apr 2024 12:15




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 689
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.7 38.5#

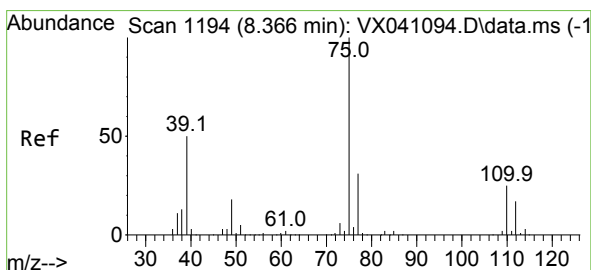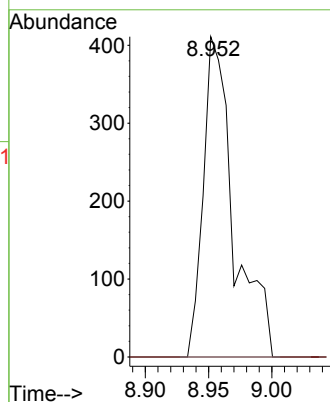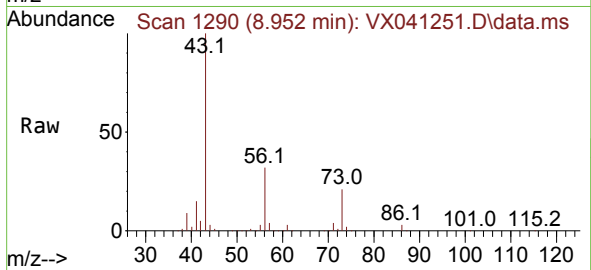

#54
 cis-1,3-Dichloropropene
 Concen: 14.489 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.183 min
 Lab File: VX041251.D
 Acq: 26 Apr 2024 12:15

Tgt Ion: 75 Resp: 33631
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.3 37.9#
 39 37.3 46.7 70.1#

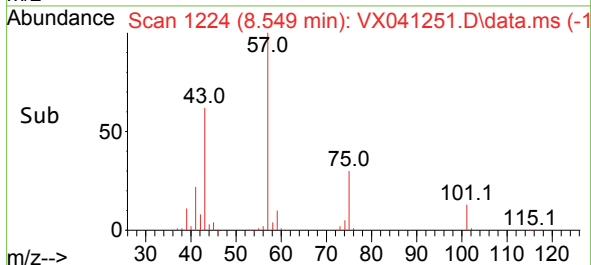



#57

1,3-Dichloropropane

Concen: 1.754 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.171 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 4509

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#



#59

2-Hexanone

Concen: 35.676 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.049 min

Lab File: VX041251.D




Acq: 26 Apr 2024 12:15


Tgt Ion: 43 Resp: 61899

Ion Ratio Lower Upper

43 100


58 18.6 26.2 78.5#

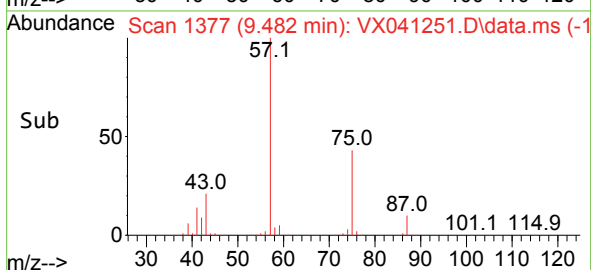






#62
4-Bromofluorobenzene
Concen: 51.815 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 95 Resp: 103141
Ion Ratio Lower Upper
95 100
174 99.8 0.0 135.6
176 95.3 0.0 131.0

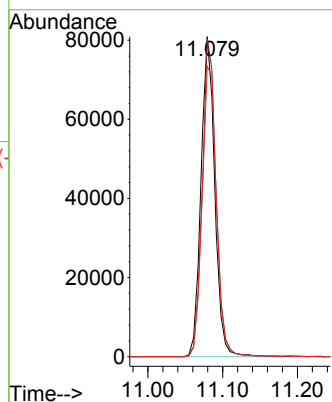


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15



Tgt Ion: 117 Resp: 227872
Ion Ratio Lower Upper
117 100
82 51.2 46.2 69.4
119 33.4 25.5 38.3

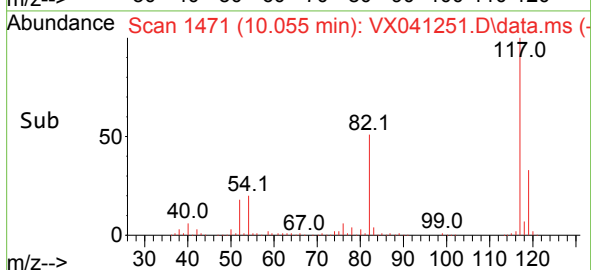

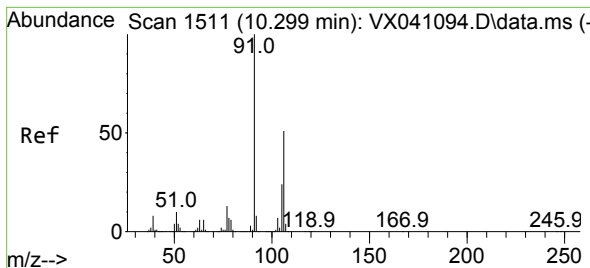

#68

m/p-Xylenes

Concen: 0.211 ug/l

RT: 10.305 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 636

Ion Ratio Lower Upper

106 100

91 205.5 165.5 248.3

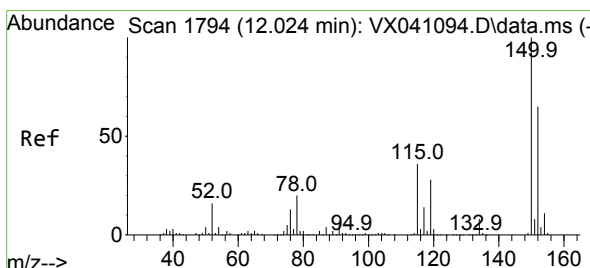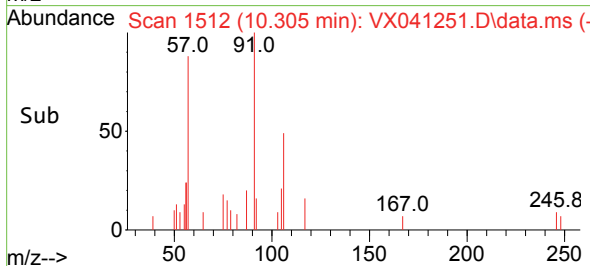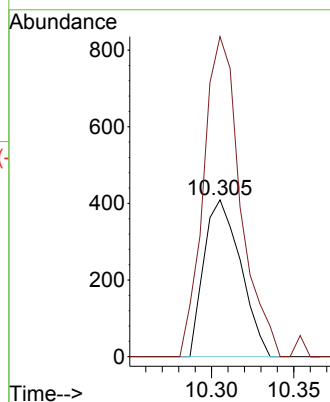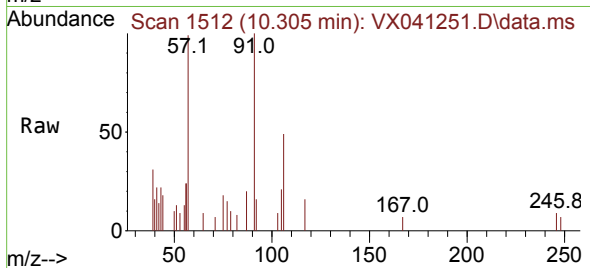

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. -0.006 min

Lab File: VX041251.D

Acq: 26 Apr 2024 12:15




Tgt Ion:152 Resp: 115229


Ion Ratio Lower Upper

152 100

115 53.3 43.3 129.9

150 154.0 0.0 345.0

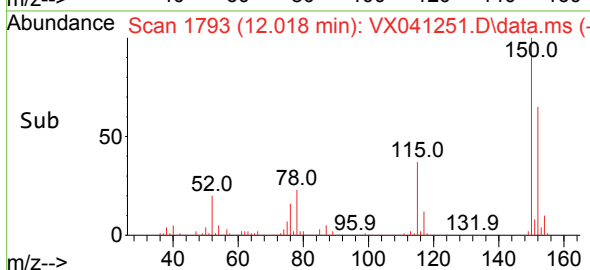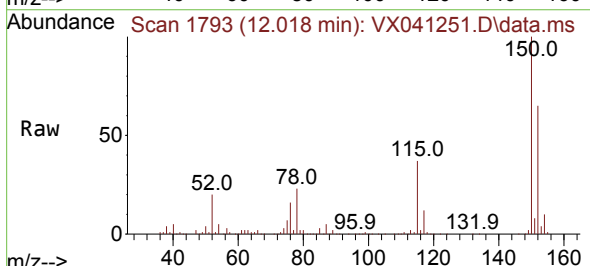



#74

N-amy1 acetate

Concen: 7.082 ug/l

RT: 10.640 min Scan# 1

Delta R.T. -0.201 min


Lab File: VX041251.D

Acq: 26 Apr 2024 12:15

Instrument :

MSVOA_X

ClientSampleId :

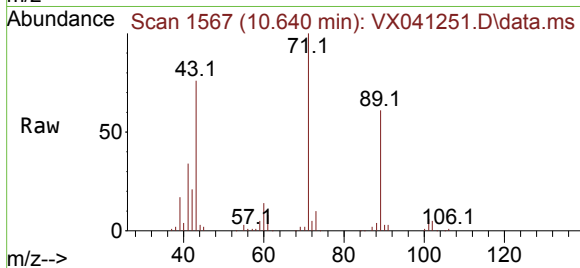

Tgt Ion: 43 Resp: 19954




Ion Ratio Lower Upper

43 100

70 2.2 32.9 49.3#

55 4.2 19.3 28.9#

61 10.1 18.8 28.2#



#76

1,2,3-Trichloropropane

Concen: 28.095 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX041251.D




Acq: 26 Apr 2024 12:15


Tgt Ion: 75 Resp: 52160

Ion Ratio Lower Upper

75 100


77 1.1 19.1 57.5#

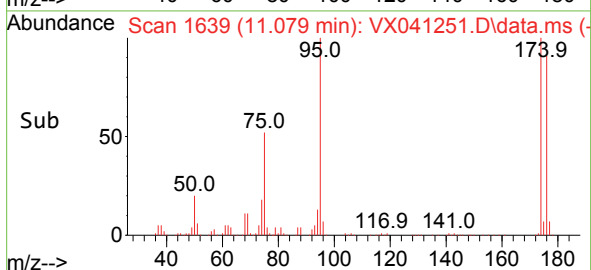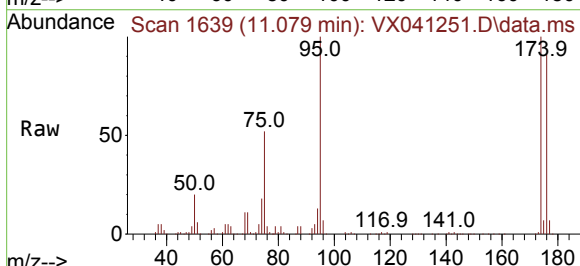






#81
trans-1,4-Dichloro-2-butene
Concen: 79.265 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15


Instrument :
MSVOA_X
ClientSampleId :

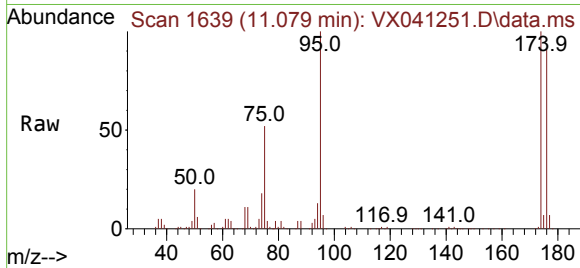



Tgt Ion: 75 Resp: 52160
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#




#95
Naphthalene
Concen: 0.307 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX041251.D
Acq: 26 Apr 2024 12:15

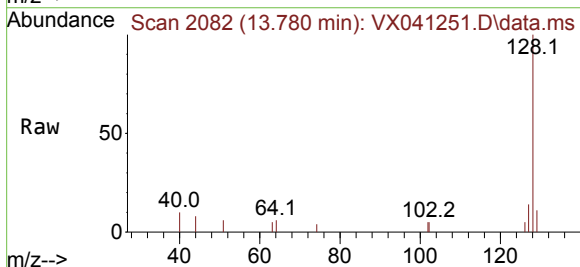


Tgt Ion: 128 Resp: 2299
Ion Ratio Lower Upper
128 100
127 9.9 10.3 15.5#
129 11.4 8.8 13.2

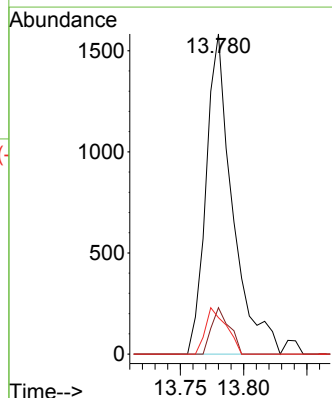

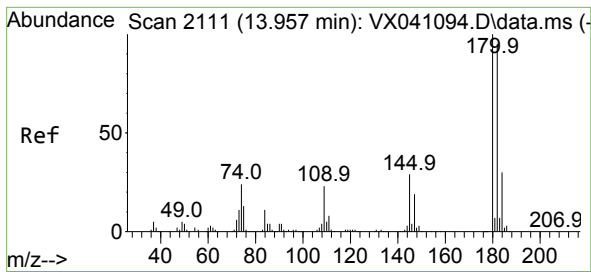

#96
 1,2,3-Trichlorobenzene
 Concen: 0.239 ug/l
 RT: 13.963 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX041251.D
 Acq: 26 Apr 2024 12:15

Instrument :
 MSVOA_X
 ClientSampleId :

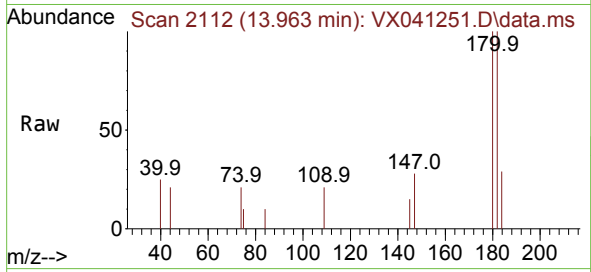

Tgt Ion:180 Resp: 656
 Ion Ratio Lower Upper
 180 100
 182 86.0 46.9 140.6
 145 20.7 17.8 53.5

