

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042722\
 Data File : VX028385.D
 Acq On : 27 Apr 2022 17:52
 Operator : JC/MD
 Sample : N2577-07ME
 Misc : 7.33g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GT-04-(25-30)ME

Quant Time: Apr 28 04:25:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	492778	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	801667	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	722627	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	355669	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	268118	41.729	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	83.460%		
35) Dibromofluoromethane	5.391	113	242300	43.098	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	86.200%		
50) Toluene-d8	8.653	98	916027	42.422	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	84.840%		
62) 4-Bromofluorobenzene	11.086	95	323109	39.135	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	78.260%		
Target Compounds						
16) Acetone	2.368	43	245	Below Cal	Qvalue #	39


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042722\
Data File : VX028385.D
Acq On : 27 Apr 2022 17:52
Operator : JC/MD
Sample : N2577-07ME
Misc : 7.33g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GT-04-(25-30)ME

Quant Time: Apr 28 04:25:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




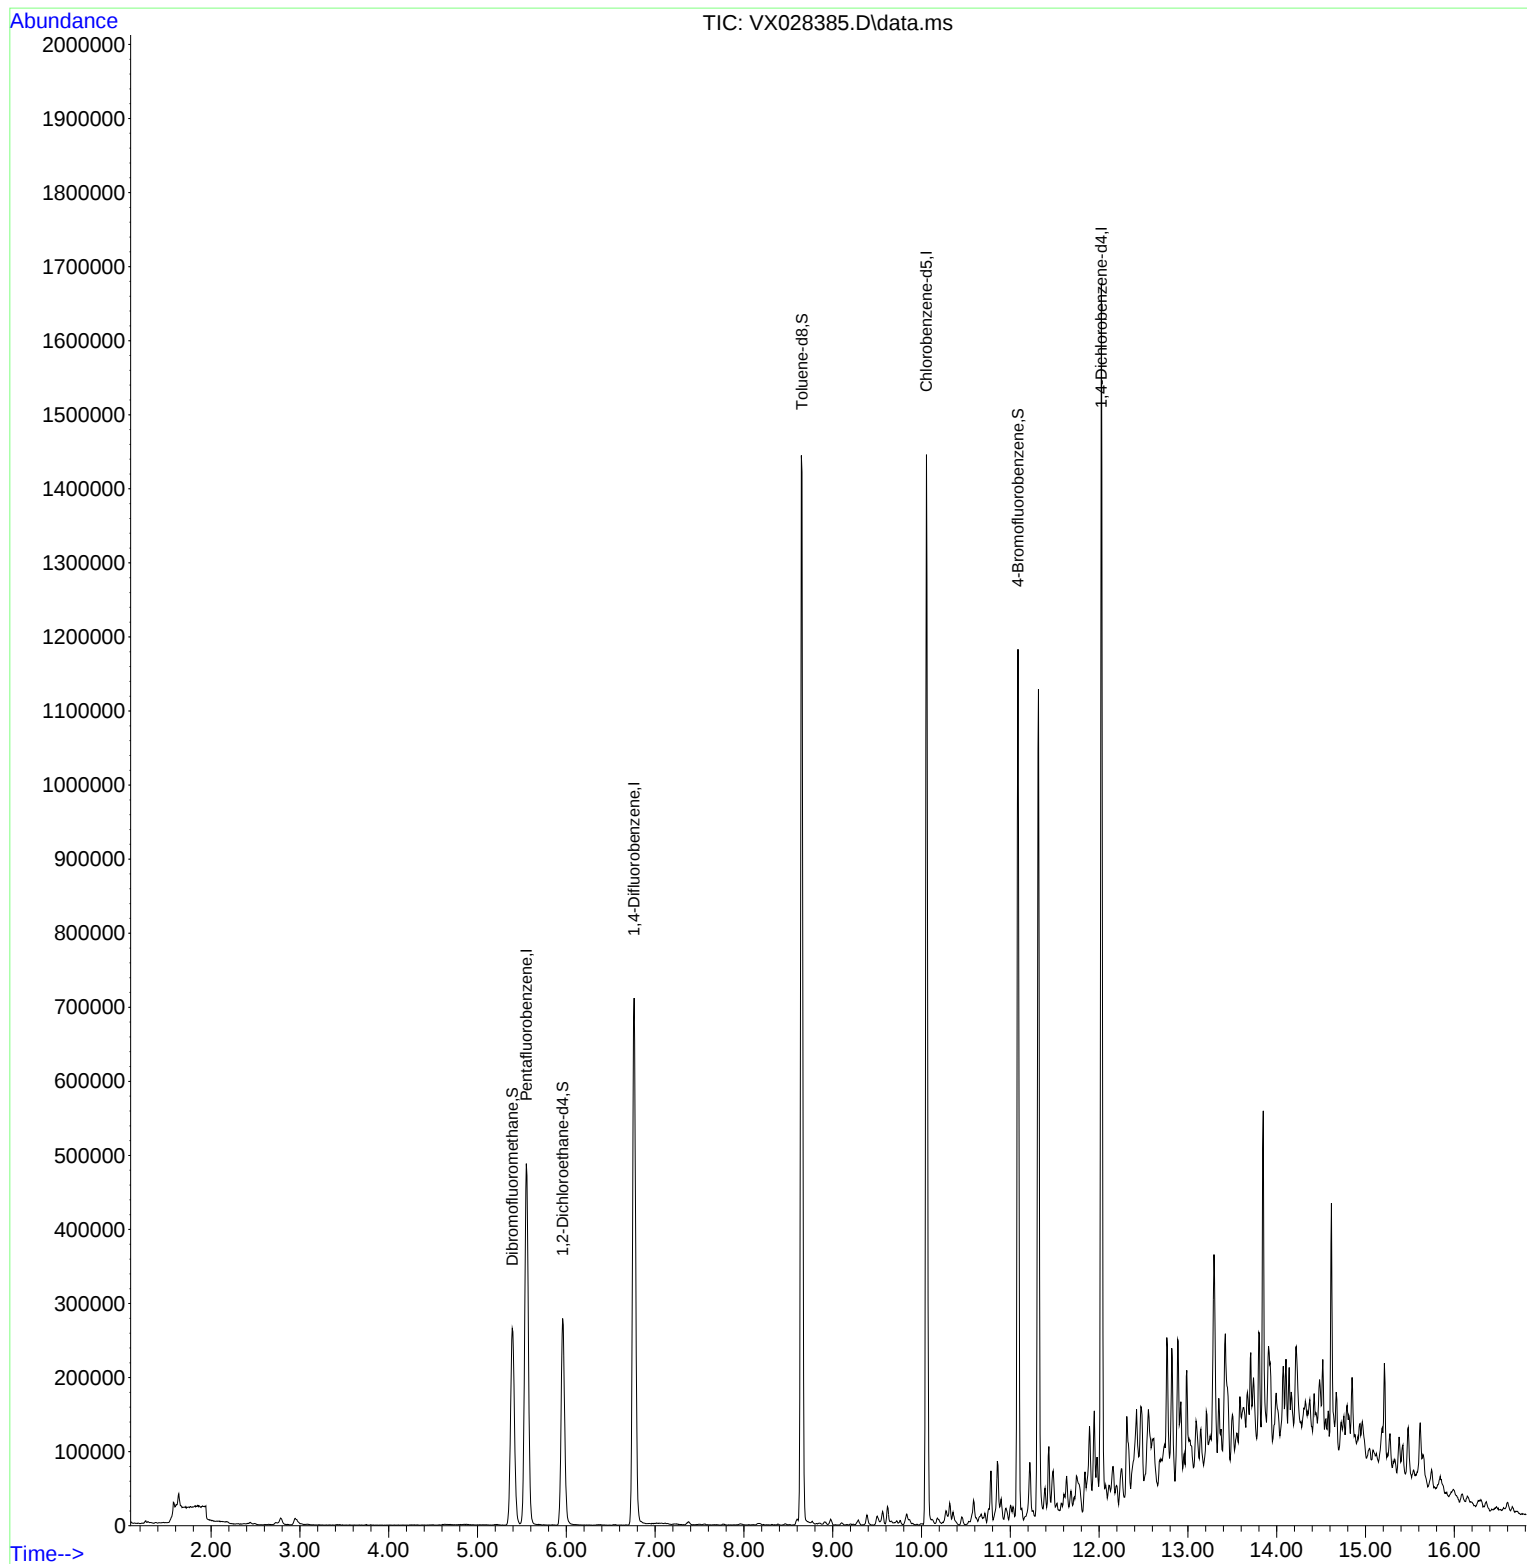


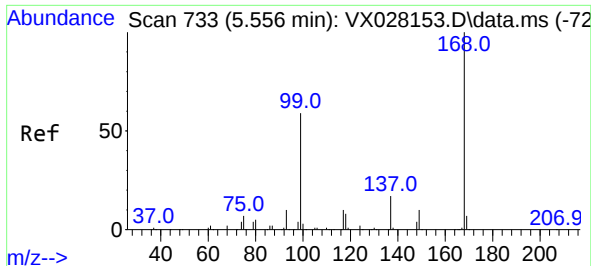

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52




Instrument :
MSVOA_X
ClientSampleId :
GT-04-(25-30)ME


Tgt Ion:168 Resp: 492778
Ion Ratio Lower Upper
168 100
99 53.0 41.7 62.5

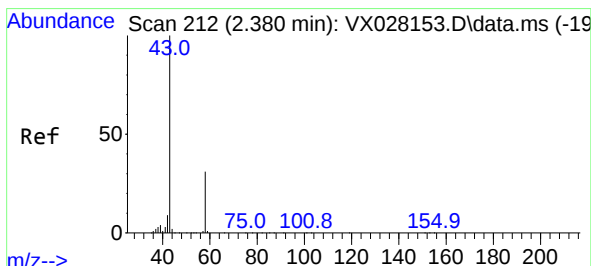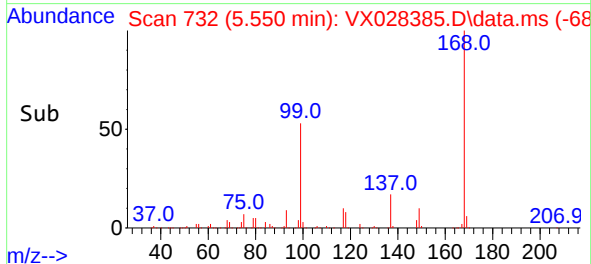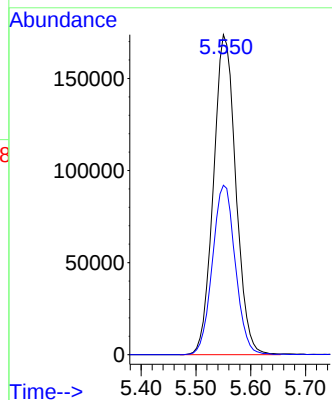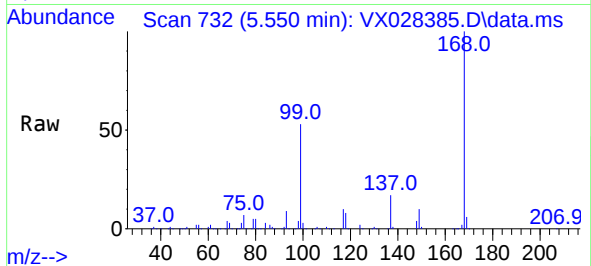

#16
Acetone
Concen: Below Cal
RT: 2.368 min Scan# 210
Delta R.T. -0.012 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52

Tgt Ion: 43 Resp: 245
Ion Ratio Lower Upper
43 100
58 0.0 28.8 43.2#


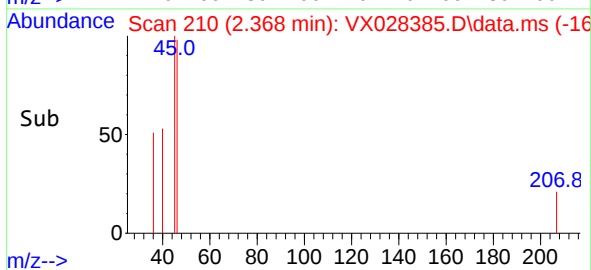
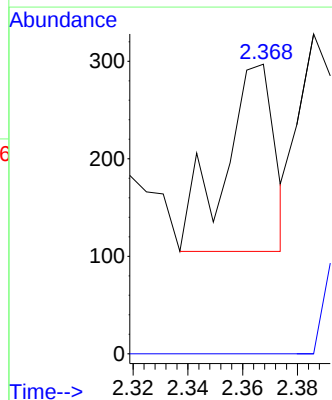
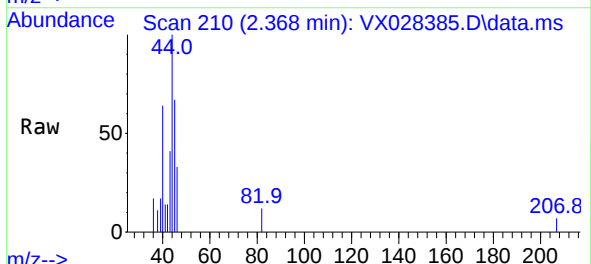


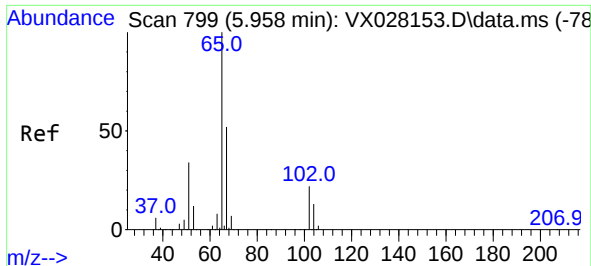

#33
1,2-Dichloroethane-d4
Concen: 41.729 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52




Instrument :
MSVOA_X
ClientSampleId :
GT-04-(25-30)ME


Tgt Ion: 65 Resp: 268118
Ion Ratio Lower Upper
65 100
67 52.4 0.0 107.4

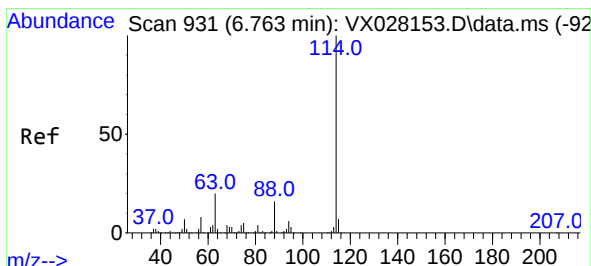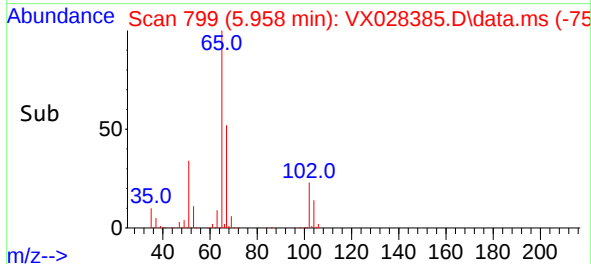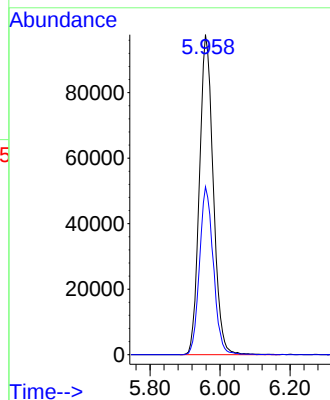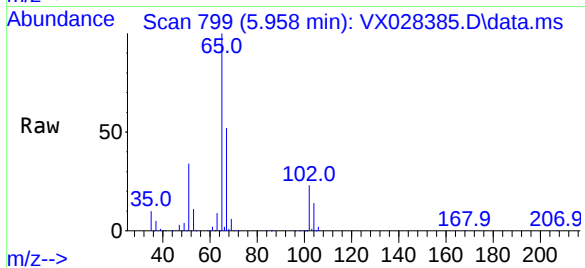

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52


Tgt Ion: 114 Resp: 801667
Ion Ratio Lower Upper
114 100
63 17.4 0.0 36.8
88 14.5 0.0 32.4

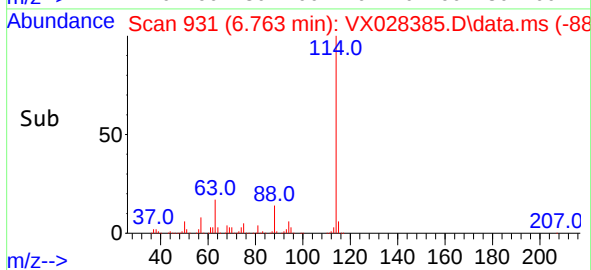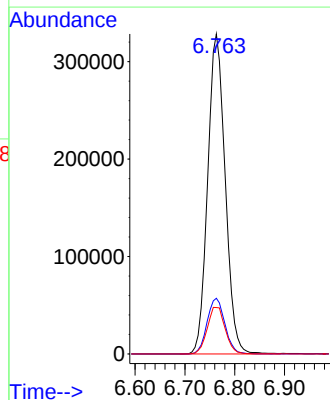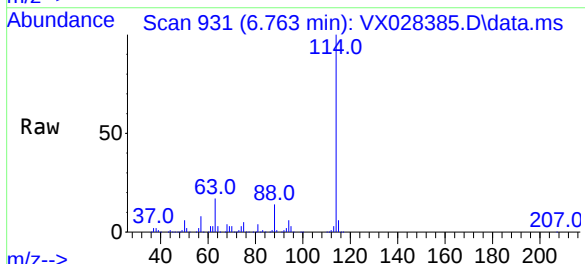



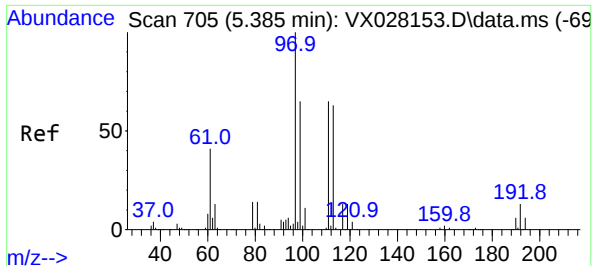


#35
Dibromofluoromethane
Concen: 43.098 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52

Instrument :
MSVOA_X
ClientSampleId :
GT-04-(25-30)ME



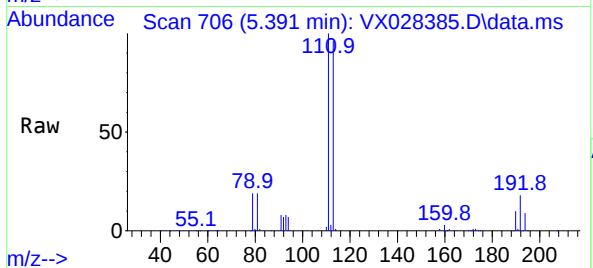



Tgt Ion:113 Resp: 242300
Ion Ratio Lower Upper
113 100
111 103.5 82.8 124.2
192 20.7 16.9 25.3

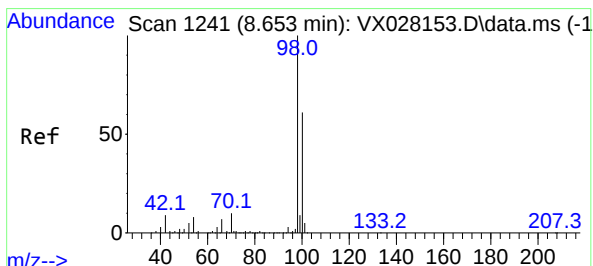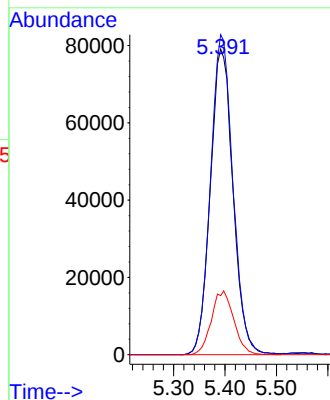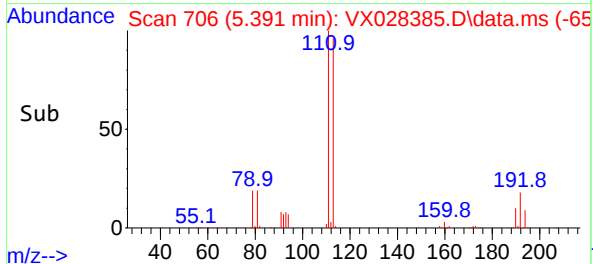

#50
Toluene-d8
Concen: 42.422 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52

Tgt Ion: 98 Resp: 916027
Ion Ratio Lower Upper
98 100
100 66.5 52.6 78.8


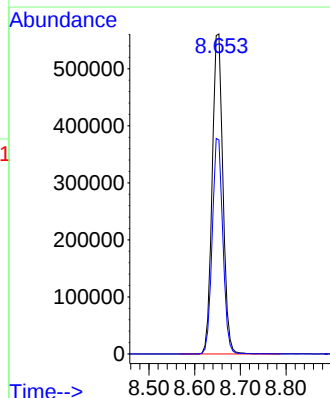
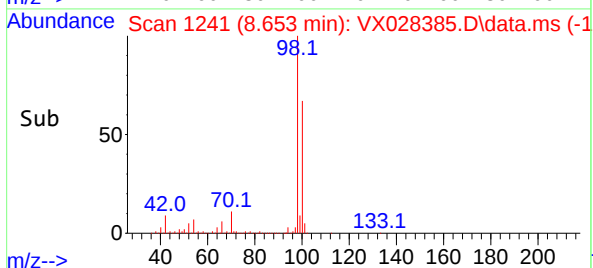
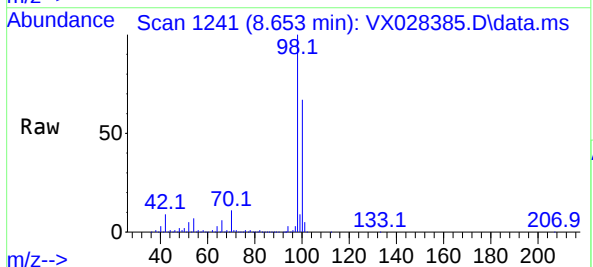


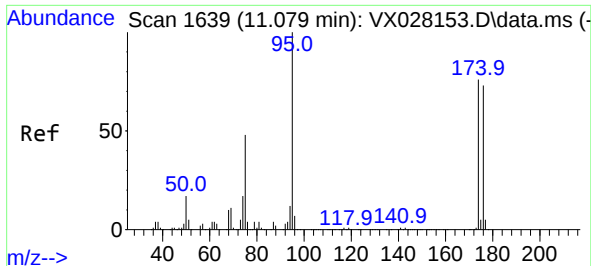

#62
4-Bromofluorobenzene
Concen: 39.135 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52




Instrument :
MSVOA_X
ClientSampleId :
GT-04-(25-30)ME


Tgt Ion: 95 Resp: 323109
Ion Ratio Lower Upper
95 100
174 86.0 0.0 163.0
176 83.6 0.0 155.0

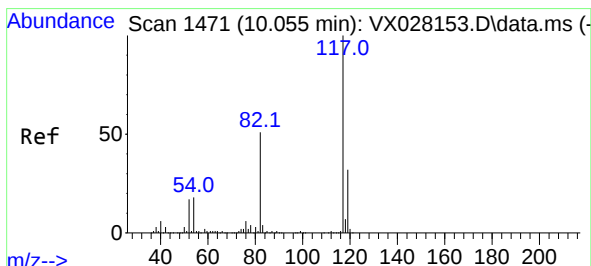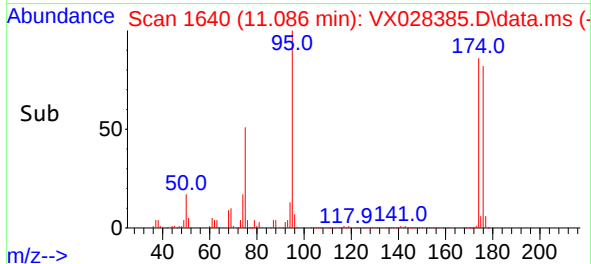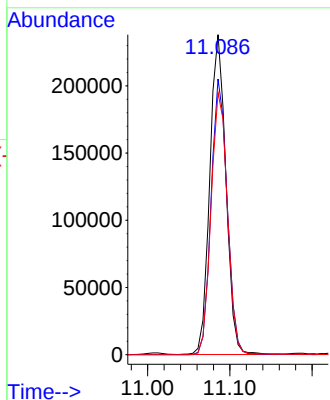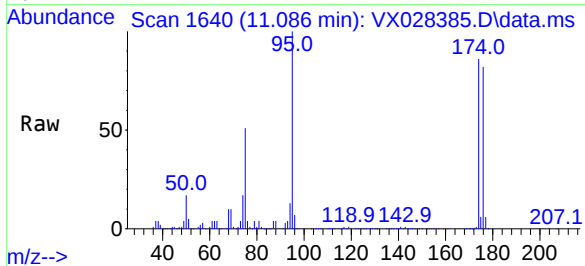

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028385.D
Acq: 27 Apr 2022 17:52

Tgt Ion: 117 Resp: 722627
Ion Ratio Lower Upper
117 100
82 51.7 41.8 62.8
119 31.6 24.8 37.2

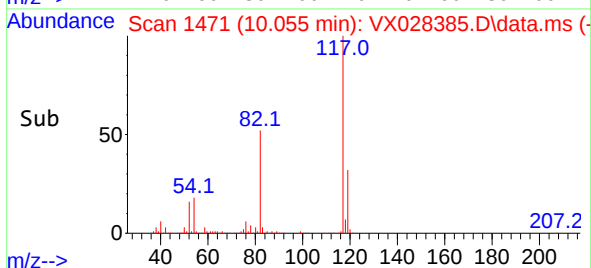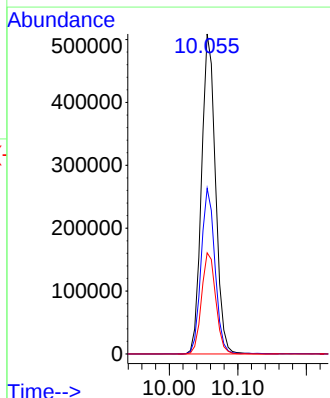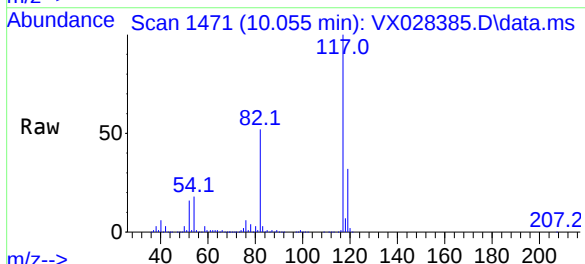

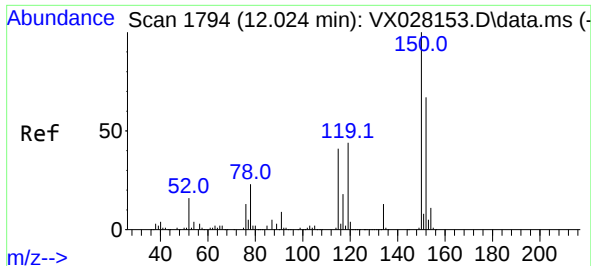

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX028385.D


Acq: 27 Apr 2022 17:52

Instrument :

MSVOA_X

ClientSampleId :

GT-04-(25-30)ME

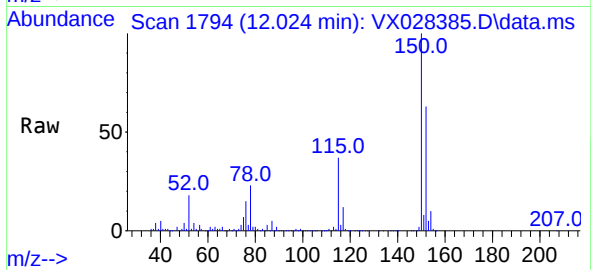

Tgt Ion:152 Resp: 355669

Ion Ratio Lower Upper

152 100

115 57.3 37.5 112.7

150 157.9 0.0 338.2

